

## Prep Standard - Chemical Standard Summary

**Order ID :** P3426

**Test :** SVOCMS Group6

**Prepbatch ID :** PB162423,

**Sequence ID/Qc Batch ID:** BF080724,BF080824,BF080924,BF081024,

**Standard ID :**

EP2499,EP2514,EP2518,SP6524,SP6525,SP6549,SP6550,SP6551,SP6552,SP6553,SP6554,SP6555,SP6556,SP6557,SP6558,SP6559,SP6573,

**Chemical ID :**

10ul/1000ul

sample,E3551,E3657,E3744,E3746,E3753,E3768,E3771,M5037,S10102,S10247,S10398,S10591,S10972,S10973,S10974,S10975,S10976,S10977,S10996,S10997,S10998,S10999,S11000,S11001,S11002,S11003,S11012,S11092,S11096,S11102,S11136,S11148,S11434,S11546,S11548,S11554,S11557,S11560,S11563,S11564,S11565,S11566,S11762,S11763,S11764,S11765,S11766,S11898,S11899,S11900,S11901,S11902,S11903,S11904,S11905,S11906,S12033,S12038,S12038 10ul/1000ul sample,S12039,S12076,S12088,S12089,S12090,S12091,S12092,S12093,S12094,S12095,S12096,S12097,S12112,S12117,S9675,W2606,W3112,

## Extractions STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>    | <u>NO.</u>             | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u>           |
|------------------|----------------|------------------------|------------------|------------------------|--------------------|----------------|------------------|--------------------------------|
| 314              | 1.1 H2SO4 SOLN | <a href="#">EP2499</a> | 06/17/2024       | 10/24/2024             | Rajesh Parikh      | None           | None             | RUPESHKUMAR SHAH<br>06/17/2024 |

**FROM** 1000.00000ml of M5037 + 1000.00000ml of W2606 = Final Quantity: 2000.000 ml

| <u>Recipe ID</u> | <u>NAME</u>                | <u>NO.</u>             | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u>           |
|------------------|----------------------------|------------------------|------------------|------------------------|--------------------|----------------|------------------|--------------------------------|
| 1874             | 10 N SODIUM HYDROXIDE SOLN | <a href="#">EP2514</a> | 07/17/2024       | 01/17/2025             | Rajesh Parikh      | None           | None             | RUPESHKUMAR SHAH<br>07/17/2024 |

**FROM** 1000.00000ml of W3112 + 400.00000gram of E3657 = Final Quantity: 1000.000 ml



| <u>Recipe ID</u>   | <u>NAME</u>          | <u>NO.</u>             | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u>                      | <u>PipetteID</u> | <u>Supervised By</u>            |
|--|----------------------|------------------------|------------------|------------------------|--------------------|-------------------------------------|------------------|---------------------------------|
| 3923   | Baked Sodium Sulfate | <a href="#">EP2518</a> | 07/26/2024       | 01/03/2025             | RUPESHKUMAR SHAH   | Extraction_SC<br>ALE_2<br>(EX-SC-2) | None             | Rajesh Parikh<br><br>07/26/2024 |
| <b>FROM</b> 1.00000gram of E3551 = Final Quantity: 4000.000 gram |                      |                        |                  |                        |                    |                                     |                  |                                 |

[illegible]

[illegible]

| <u>Recipe ID</u> | <u>NAME</u>  | <u>NO.</u>             | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u>         |
|------------------|--|------------------------|------------------|------------------------|--------------------|----------------|------------------|------------------------------|
| 3764             | 8270/625 Stock solution 100 ng   | <a href="#">SP6549</a> | 07/09/2024       | 08/26/2024             | Jagrut Upadhyay    | None           | None             | mohammad ahmed<br>07/09/2024 |
| <u>FROM</u>      | 0.26700ml of S10102 + 0.40000ml of S11434 + 0.50000ml of S12112 + 1.00000ml of S11092 + 1.00000ml of S11096 + 1.00000ml of S11102 + 1.00000ml of S11148 + 1.00000ml of S12076 + 3.83300ml of E3746 = Final Quantity: 10.000 ml |                        |                  |                        |                    |                |                  |                              |



## SVOC STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>           | <u>NO.</u>             | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-----------------------|------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 413              | 80 ng BNA ICC, 80 PPM | <a href="#">SP6550</a> | 07/09/2024       | 08/26/2024             | Jagrut Upadhyay    | None           | None             | mohammad ahmed       |
|                  |                       |                        |                  |                        |                    |                |                  | 07/09/2024           |

**FROM** 0.01000ml of S12033 + 0.20000ml of E3746 + 0.80000ml of SP6549 = Final Quantity: 1.010 ml

| <u>Recipe ID</u> | <u>NAME</u>           | <u>NO.</u>             | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-----------------------|------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 412              | 60 ng BNA ICC, 60 PPM | <a href="#">SP6551</a> | 07/09/2024       | 08/26/2024             | Jagrut Upadhyay    | None           | None             | mohammad ahmed       |
|                  |                       |                        |                  |                        |                    |                |                  | 07/09/2024           |

**FROM** 0.01000ml of S12033 + 0.40000ml of E3746 + 0.60000ml of SP6549 = Final Quantity: 1.010 ml

## SVOC STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>           | <u>NO.</u>             | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-----------------------|------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 411              | 50 ng BNA ICC, 50 PPM | <a href="#">SP6552</a> | 07/09/2024       | 08/26/2024             | Jagrut Upadhyay    | None           | None             | mohammad ahmed       |
|                  |                       |                        |                  |                        |                    |                |                  | 07/09/2024           |

**FROM** 0.01000ml of S12033 + 0.50000ml of E3746 + 0.50000ml of SP6549 = Final Quantity: 1.010 ml

| <u>Recipe ID</u> | <u>NAME</u>           | <u>NO.</u>             | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-----------------------|------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 410              | 40 ng BNA ICC, 40 PPM | <a href="#">SP6553</a> | 07/09/2024       | 08/26/2024             | Jagrut Upadhyay    | None           | None             | mohammad ahmed       |
|                  |                       |                        |                  |                        |                    |                |                  | 07/09/2024           |

**FROM** 0.01000ml of S12033 + 0.60000ml of E3746 + 0.40000ml of SP6549 = Final Quantity: 1.010 ml

## SVOC STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>           | <u>NO.</u>             | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-----------------------|------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 3678             | 20 ng BNA ICC, 20 PPM | <a href="#">SP6554</a> | 07/09/2024       | 08/26/2024             | Jagrut Upadhyay    | None           | None             | mohammad ahmed       |
|                  |                       |                        |                  |                        |                    |                |                  | 07/09/2024           |

**FROM** 0.01000ml of S12033 + 0.80000ml of E3746 + 0.20000ml of SP6549 = Final Quantity: 1.010 ml

| <u>Recipe ID</u> | <u>NAME</u>           | <u>NO.</u>             | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-----------------------|------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 408              | 10 ng BNA ICC, 10 PPM | <a href="#">SP6555</a> | 07/09/2024       | 08/26/2024             | Jagrut Upadhyay    | None           | None             | mohammad ahmed       |
|                  |                       |                        |                  |                        |                    |                |                  | 07/09/2024           |

**FROM** 0.01000ml of S12033 + 0.90000ml of E3746 + 0.10000ml of SP6549 = Final Quantity: 1.010 ml

## SVOC STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>         | <u>NO.</u>             | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|---------------------|------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 407              | 5 ng BNA ICC, 5 PPM | <a href="#">SP6556</a> | 07/09/2024       | 08/26/2024             | Jagrut Upadhyay    | None           | None             | mohammad ahmed       |
| 07/09/2024       |                     |                        |                  |                        |                    |                |                  |                      |

**FROM** 0.01000ml of S12033 + 0.95000ml of E3746 + 0.05000ml of SP6549 = Final Quantity: 1.010 ml

| <u>Recipe ID</u> | <u>NAME</u>             | <u>NO.</u>             | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------------|------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 175              | 2.5 ng BNA ICC, 2.5 PPM | <a href="#">SP6557</a> | 07/09/2024       | 08/26/2024             | Jagrut Upadhyay    | None           | None             | mohammad ahmed       |
| 07/09/2024       |                         |                        |                  |                        |                    |                |                  |                      |

**FROM** 0.01000ml of S12033 + 0.50000ml of E3746 + 0.50000ml of SP6556 = Final Quantity: 1.010 ml

[illegible]

| <u>Recipe ID</u> | <u>NAME</u>   | <u>NO.</u>             | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u>         |
|------------------|---|------------------------|------------------|------------------------|--------------------|----------------|------------------|------------------------------|
| 416              | 40 ng BNA ICV, 40 PPM   | <a href="#">SP6559</a> | 07/09/2024       | 11/30/2024             | Jagrut Upadhyay    | None           | None             | mohammad ahmed<br>07/11/2024 |
| <u>FROM</u>      | 0.01000ml of S12033 + 0.60000ml of E3768 + 0.40000ml of SP6558 = Final Quantity: 1.010 ml |                        |                  |                        |                    |                |                  |                              |

## SVOC STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>   | <u>NO.</u>             | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|---|------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 3895             | 50 ug/ml DFTPP 8270E  | <a href="#">SP6573</a> | 07/15/2024       | 01/08/2025             | Rahul Chavli       | None           | None             | Yogesh Patel         |
| 07/17/2024       |   |                        |                  |                        |                    |                |                  |                      |
| <u>FROM</u>      | 1.00000ml of S10247 + 19.00000ml of E3768 = Final Quantity: 20.000 ml |                        |                  |                        |                    |                |                  |                      |

## CHEMICAL RECEIPT LOG BOOK

| Supplier                    | ItemCode / ItemName                                    | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|-----------------------------|--|--------|-----------------|-------------------------|-----------------------------|----------------|
| PCI Scientific Supply, Inc. | PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1 | 313201 | 01/03/2025      | 01/03/2024 / Rajesh     | 07/20/2023 / Rajesh         | E3551          |

| Supplier                    | ItemCode / ItemName                                  | Lot #      | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|-----------------------------|--|------------|-----------------|-------------------------|-----------------------------|----------------|
| PCI Scientific Supply, Inc. | PC19510-5 / Sodium Hydroxide Pellets 2.5 Kg, Pk of 4 | 23B1556310 | 12/31/2025      | 12/04/2023 / Rajesh     | 12/01/2023 / Rajesh         | E3657          |

| Supplier         | ItemCode / ItemName                        | Lot #       | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|--|-------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9254-03 / Acetone, Ultra Resi (cs/4x4L) | 23H14626005 | 11/29/2024      | 05/29/2024 / Rajesh     | 05/23/2024 / Rajesh         | E3744          |

| Supplier         | ItemCode / ItemName   | Lot #      | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|---|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L) | 24C0162011 | 11/25/2024      | 05/25/2024 / Rajesh     | 05/08/2024 / Rajesh         | E3746          |

| Supplier         | ItemCode / ItemName                        | Lot #      | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|--|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9254-03 / Acetone, Ultra Resi (cs/4x4L) | 23H1462005 | 12/01/2024      | 06/01/2024 / Rajesh     | 05/31/2024 / Rajesh         | E3753          |

| Supplier         | ItemCode / ItemName   | Lot #      | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|---|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L) | 24E2462004 | 01/08/2025      | 07/08/2024 / Rajesh     | 06/21/2024 / Rajesh         | E3768          |

## CHEMICAL RECEIPT LOG BOOK

| Supplier         | ItemCode / ItemName   | Lot #      | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|---|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L) | 24F1062004 | 01/19/2025      | 07/19/2024 / Rajesh     | 07/16/2024 / Rajesh         | E3771          |

| Supplier         | ItemCode / ItemName                                     | Lot #      | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|---|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L) | 0000250349 | 12/15/2024      | 01/06/2022 / mohan      | 09/18/2021 / mohan          | M5037          |

| Supplier          | ItemCode / ItemName                                       | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|-------------------|---|--------|-----------------|-------------------------|-----------------------------|----------------|
| CPI International | Z-112090-04 / CLP Acid Surrogate Solution, 7500 mg/L, 1ml | 440246 | 09/29/2024      | 03/29/2024 / Jagrut     | 12/09/2021 / Christian      | S10102         |

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31615 / SV Mixture, GC/MS Tuning Mixture, CH <sub>2</sub> Cl <sub>2</sub> , 1mL, | A0182667 | 01/15/2025      | 07/15/2024 / Rahul      | 03/18/2022 / Christian      | S10247         |

| Supplier | ItemCode / ItemName                                     | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555871 / Custom Standard, 4-nitrophenol Std [CS 5238-4] | A0185300 | 10/26/2024      | 04/26/2024 / Rahul      | 05/18/2022 / Christian      | S10398         |

| Supplier | ItemCode / ItemName                                 | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555868 / Custom Standard, Benzidine Std [CS 5328-1] | A0186373 | 08/29/2024      | 02/29/2024 / Jagrut     | 07/05/2022 / Christian      | S10591         |



## CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31087 / Acid Surrogate<br>10,000ug/ml,methanol,5ml/<br>ampul | A0188108 | 08/31/2030      | 05/31/2024 /<br>Jagrut  | 12/28/2022 /<br>Christian   | S10972         |

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31087 / Acid Surrogate<br>10,000ug/ml,methanol,5ml/<br>ampul | A0188108 | 11/30/2024      | 05/31/2024 /<br>Jagrut  | 12/28/2022 /<br>Christian   | S10973         |

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31087 / Acid Surrogate<br>10,000ug/ml,methanol,5ml/<br>ampul | A0188108 | 11/30/2024      | 05/31/2024 /<br>Jagrut  | 12/28/2022 /<br>Christian   | S10974         |

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31087 / Acid Surrogate<br>10,000ug/ml,methanol,5ml/<br>ampul | A0188108 | 11/30/2024      | 05/31/2024 /<br>Jagrut  | 12/28/2022 /<br>Christian   | S10975         |

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31087 / Acid Surrogate<br>10,000ug/ml,methanol,5ml/<br>ampul | A0188108 | 11/30/2024      | 05/31/2024 /<br>Jagrut  | 12/28/2022 /<br>Christian   | S10976         |

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31087 / Acid Surrogate<br>10,000ug/ml,methanol,5ml/<br>ampul | A0188108 | 11/30/2024      | 05/31/2024 /<br>Jagrut  | 12/28/2022 /<br>Christian   | S10977         |

## CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31086 / Base Neutral Surrogate<br>5000ug/ml,CH <sub>2</sub> Cl <sub>2</sub> ,5ml | A0189418 | 08/31/2028      | 05/31/2024 / Jagrut     | 12/28/2022 / Christian      | S10996         |

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31086 / Base Neutral Surrogate<br>5000ug/ml,CH <sub>2</sub> Cl <sub>2</sub> ,5ml | A0189418 | 11/30/2024      | 05/31/2024 / Jagrut     | 12/28/2022 / Christian      | S10997         |

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31086 / Base Neutral Surrogate<br>5000ug/ml,CH <sub>2</sub> Cl <sub>2</sub> ,5ml | A0189418 | 11/30/2024      | 05/31/2024 / Jagrut     | 12/28/2022 / Christian      | S10998         |

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31086 / Base Neutral Surrogate<br>5000ug/ml,CH <sub>2</sub> Cl <sub>2</sub> ,5ml | A0189418 | 11/30/2024      | 05/31/2024 / Jagrut     | 12/28/2022 / Christian      | S10999         |

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31086 / Base Neutral Surrogate<br>5000ug/ml,CH <sub>2</sub> Cl <sub>2</sub> ,5ml | A0189418 | 11/30/2024      | 05/31/2024 / Jagrut     | 12/28/2022 / Christian      | S11000         |

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31086 / Base Neutral Surrogate<br>5000ug/ml,CH <sub>2</sub> Cl <sub>2</sub> ,5ml | A0189418 | 11/30/2024      | 05/31/2024 / Jagrut     | 12/28/2022 / Christian      | S11001         |

## CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31086 / Base Neutral Surrogate<br>5000ug/ml,CH <sub>2</sub> Cl <sub>2</sub> ,5ml | A0189418 | 11/30/2024      | 05/31/2024 / Jagrut     | 12/28/2022 / Christian      | S11002         |

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31086 / Base Neutral Surrogate<br>5000ug/ml,CH <sub>2</sub> Cl <sub>2</sub> ,5ml | A0189418 | 11/30/2024      | 05/31/2024 / Jagrut     | 12/28/2022 / Christian      | S11003         |

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555872 / Custom Standard,<br>pentachlorophenol Std [CS 5328-5] | A0193449 | 10/26/2024      | 04/26/2024 / Rahul      | 01/13/2023 / Christian      | S11012         |

| Supplier          | ItemCode / ItemName   | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|-------------------|---|--------|-----------------|-------------------------|-----------------------------|----------------|
| CPI International | Z-110817-01 / Custom 8270 Mix, 4-55, 1000 mg/L, 1 ml, (Maximum Expiration: 90 Days) | 414125 | 01/09/2025      | 07/09/2024 / Jagrut     | 02/07/2023 / Christian      | S11092         |

| Supplier          | ItemCode / ItemName  | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|-------------------|--|--------|-----------------|-------------------------|-----------------------------|----------------|
| CPI International | z-110381-01 / 8270 Calibration Solution, 76-1, 500 & 1,000 mg/L, 1ml | 495831 | 01/09/2025      | 07/09/2024 / Jagrut     | 02/07/2023 / Christian      | S11096         |

| Supplier          | ItemCode / ItemName   | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|-------------------|---|--------|-----------------|-------------------------|-----------------------------|----------------|
| CPI International | Z-010442-07 / Benzaldehyde Solution, 1000 mg/L, 1.3 ml, (Maximum Expiration: 90 Days) | 495833 | 01/09/2025      | 07/09/2024 / Jagrut     | 02/07/2023 / Christian      | S11102         |

## CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName   | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555870 / Custom Standard, 2,4-dinitrophenol Std [CS 5328-3] | A0194698 | 08/29/2024      | 02/29/2024 / Jagrut     | 02/20/2023 / Christian      | S11136         |

| Supplier          | ItemCode / ItemName   | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|-------------------|---|--------|-----------------|-------------------------|-----------------------------|----------------|
| CPI International | Z-010074-07 / 3,3'-Dichlorobenzidine Solution, 1,000 mg/L, 1 ml, (Maximum Expiration: 180 days) | 406703 | 01/09/2025      | 07/09/2024 / Jagrut     | 03/06/2023 / Christian      | S11148         |

| Supplier          | ItemCode / ItemName   | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|-------------------|---|--------|-----------------|-------------------------|-----------------------------|----------------|
| CPI International | Z-110094-02 / CLP Base/Neutral Surrogate Solution, 5000 mg/L, 1ml | 503442 | 08/26/2024      | 07/09/2024 / Jagrut     | 07/26/2023 / yogesh         | S11434         |

| Supplier | ItemCode / ItemName   | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555223 / Custom 8270 Plus Std #1 [2nd lot at \$100 per ampul if requested - contact ARM with Request] | A0201940 | 10/26/2024      | 04/26/2024 / Rahul      | 09/18/2023 / Kiran          | S11546         |

[CS 4978-1]

| Supplier | ItemCode / ItemName   | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555223 / Custom 8270 Plus Std #1 [2nd lot at \$100 per ampul if requested - contact ARM with Request] | A0201940 | 12/05/2024      | 06/05/2024 / Rahul      | 09/18/2023 / Kiran          | S11548         |

[CS 4978-1]

| Supplier | ItemCode / ItemName   | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555223 / Custom 8270 Plus Std #1 [2nd lot at \$100 per ampul if requested - contact ARM with Request] | A0201940 | 12/05/2024      | 06/05/2024 / Rahul      | 09/18/2023 / Kiran          | S11554         |

[CS 4978-1]

## CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555223 / Custom 8270<br>Plus Std #1 [2nd lot at \$100<br>per ampul if requested -<br>contact ARM with Request] | A0201940 | 11/16/2024      | 05/16/2024 /<br>Jagrut  | 09/18/2023 /<br>Kiran       | S11557         |

[CS 4978-1]

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555223 / Custom 8270<br>Plus Std #1 [2nd lot at \$100<br>per ampul if requested -<br>contact ARM with Request] | A0201940 | 12/05/2024      | 06/05/2024 /<br>Rahul   | 09/18/2023 /<br>Kiran       | S11560         |

[CS 4978-1]

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555223 / Custom 8270<br>Plus Std #1 [2nd lot at \$100<br>per ampul if requested -<br>contact ARM with Request] | A0201940 | 12/05/2024      | 06/05/2024 /<br>Rahul   | 09/18/2023 /<br>Kiran       | S11563         |

[CS 4978-1]

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555223 / Custom 8270<br>Plus Std #1 [2nd lot at \$100<br>per ampul if requested -<br>contact ARM with Request] | A0201940 | 12/05/2024      | 06/05/2024 /<br>Rahul   | 09/18/2023 /<br>Kiran       | S11564         |

[CS 4978-1]

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555223 / Custom 8270<br>Plus Std #1 [2nd lot at \$100<br>per ampul if requested -<br>contact ARM with Request] | A0201940 | 12/05/2024      | 06/05/2024 /<br>Rahul   | 09/18/2023 /<br>Kiran       | S11565         |

[CS 4978-1]

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555223 / Custom 8270<br>Plus Std #1 [2nd lot at \$100<br>per ampul if requested -<br>contact ARM with Request] | A0201940 | 12/05/2024      | 06/05/2024 /<br>Rahul   | 09/18/2023 /<br>Kiran       | S11566         |

[CS 4978-1]

## CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName   | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31853 / 1,4-Dioxane, 2000 ug/ml , Solvent: Methylene Chloride | A0196453 | 11/13/2024      | 05/13/2024 / Jagrut     | 11/21/2023 / Rahul          | S11762         |

| Supplier | ItemCode / ItemName   | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31853 / 1,4-Dioxane, 2000 ug/ml , Solvent: Methylene Chloride | A0196453 | 12/05/2024      | 06/05/2024 / Rahul      | 11/21/2023 / Rahul          | S11763         |

| Supplier | ItemCode / ItemName   | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31853 / 1,4-Dioxane, 2000 ug/ml , Solvent: Methylene Chloride | A0196453 | 12/05/2024      | 06/05/2024 / Rahul      | 11/21/2023 / Rahul          | S11764         |

| Supplier | ItemCode / ItemName   | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31853 / 1,4-Dioxane, 2000 ug/ml , Solvent: Methylene Chloride | A0196453 | 12/05/2024      | 06/05/2024 / Rahul      | 11/21/2023 / Rahul          | S11765         |

| Supplier | ItemCode / ItemName   | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31853 / 1,4-Dioxane, 2000 ug/ml , Solvent: Methylene Chloride | A0196453 | 12/14/2024      | 06/14/2024 / Rahul      | 11/21/2023 / Rahul          | S11766         |

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31850 / 8270 SV Mix, 8270 Mega Mix 1mL, 1000ug/mL, CH <sub>2</sub> Cl <sub>2</sub> [New Solvent 100% CH <sub>2</sub> Cl <sub>2</sub> ] | A0197982 | 11/30/2024      | 06/05/2024 / Rahul      | 11/21/2023 / rahul          | S11898         |

## CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31850 / 8270 SV Mix,<br>8270 Mega Mix 1mL,<br>1000ug/mL, CH <sub>2</sub> Cl <sub>2</sub> [New Solvent 100% CH <sub>2</sub> Cl <sub>2</sub> ] | A0197982 | 11/30/2024      | 06/05/2024 /<br>Rahul   | 11/21/2023 /<br>rahul       | S11899         |

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31850 / 8270 SV Mix,<br>8270 Mega Mix 1mL,<br>1000ug/mL, CH <sub>2</sub> Cl <sub>2</sub> [New Solvent 100% CH <sub>2</sub> Cl <sub>2</sub> ] | A0197982 | 11/30/2024      | 06/05/2024 /<br>Rahul   | 11/21/2023 /<br>rahul       | S11900         |

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31850 / 8270 SV Mix,<br>8270 Mega Mix 1mL,<br>1000ug/mL, CH <sub>2</sub> Cl <sub>2</sub> [New Solvent 100% CH <sub>2</sub> Cl <sub>2</sub> ] | A0197982 | 10/26/2024      | 04/26/2024 /<br>Rahul   | 11/21/2023 /<br>rahul       | S11901         |

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31850 / 8270 SV Mix,<br>8270 Mega Mix 1mL,<br>1000ug/mL, CH <sub>2</sub> Cl <sub>2</sub> [New Solvent 100% CH <sub>2</sub> Cl <sub>2</sub> ] | A0197982 | 11/16/2024      | 05/16/2024 /<br>Jagrut  | 11/21/2023 /<br>rahul       | S11902         |

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31850 / 8270 SV Mix,<br>8270 Mega Mix 1mL,<br>1000ug/mL, CH <sub>2</sub> Cl <sub>2</sub> [New Solvent 100% CH <sub>2</sub> Cl <sub>2</sub> ] | A0197982 | 11/30/2024      | 06/05/2024 /<br>Rahul   | 11/21/2023 /<br>rahul       | S11903         |

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31850 / 8270 SV Mix,<br>8270 Mega Mix 1mL,<br>1000ug/mL, CH <sub>2</sub> Cl <sub>2</sub> [New Solvent 100% CH <sub>2</sub> Cl <sub>2</sub> ] | A0197982 | 11/30/2024      | 06/05/2024 /<br>Rahul   | 11/21/2023 /<br>rahul       | S11904         |

## CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31850 / 8270 SV Mix, 8270 Mega Mix 1mL, 1000ug/mL, CH <sub>2</sub> Cl <sub>2</sub> [New Solvent 100% CH <sub>2</sub> Cl <sub>2</sub> ] | A0197982 | 11/30/2024      | 06/05/2024 / Rahul      | 11/21/2023 / rahul          | S11905         |

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31850 / 8270 SV Mix, 8270 Mega Mix 1mL, 1000ug/mL, CH <sub>2</sub> Cl <sub>2</sub> [New Solvent 100% CH <sub>2</sub> Cl <sub>2</sub> ] | A0197982 | 11/30/2024      | 06/05/2024 / Rahul      | 11/21/2023 / rahul          | S11906         |

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31206 / SV Mix, CLP method, Internal Std, 2000ug/mL, CH <sub>2</sub> Cl <sub>2</sub> , 1mL | A0201320 | 01/01/2025      | 07/01/2024 / Rahul      | 12/21/2023 / Rahul          | S12033         |

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31206 / SV Mix, CLP method, Internal Std, 2000ug/mL, CH <sub>2</sub> Cl <sub>2</sub> , 1mL | A0201320 | 02/05/2025      | 08/05/2024 / Rahul      | 12/21/2023 / Rahul          | S12038         |

| Supplier | ItemCode / ItemName  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31206 / SV Mix, CLP method, Internal Std, 2000ug/mL, CH <sub>2</sub> Cl <sub>2</sub> , 1mL | A0201320 | 02/07/2025      | 08/07/2024 / anahy      | 12/21/2023 / Rahul          | S12039         |

| Supplier          | ItemCode / ItemName  | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|-------------------|--|--------|-----------------|-------------------------|-----------------------------|----------------|
| CPI International | Z-110816-01 / Custom 8270 Mix, 4-79, 1000 mg/L, 1 mL, (Maximum Expiration: 180 Days) | 414127 | 01/09/2025      | 07/09/2024 / Jagrut     | 01/31/2024 / Rahul          | S12076         |



## CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName   | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555224 / Custom 8270<br>Plus Std #2 [2nd lot at \$85<br>per ampul if requested -<br>contact ARM with Request] | A0207706 | 10/26/2024      | 04/26/2024 /<br>Rahul   | 02/05/2024 /<br>Rahul       | S12088         |

[CS 4978-2]

| Supplier | ItemCode / ItemName   | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555224 / Custom 8270<br>Plus Std #2 [2nd lot at \$85<br>per ampul if requested -<br>contact ARM with Request] | A0207706 | 11/16/2024      | 05/16/2024 /<br>Jagrut  | 02/05/2024 /<br>Rahul       | S12089         |

[CS 4978-2]

| Supplier | ItemCode / ItemName   | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555224 / Custom 8270<br>Plus Std #2 [2nd lot at \$85<br>per ampul if requested -<br>contact ARM with Request] | A0207706 | 12/05/2024      | 06/05/2024 /<br>Rahul   | 02/05/2024 /<br>Rahul       | S12090         |

[CS 4978-2]

| Supplier | ItemCode / ItemName   | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555224 / Custom 8270<br>Plus Std #2 [2nd lot at \$85<br>per ampul if requested -<br>contact ARM with Request] | A0207706 | 12/05/2024      | 06/05/2024 /<br>Rahul   | 02/05/2024 /<br>Rahul       | S12091         |

[CS 4978-2]

| Supplier | ItemCode / ItemName   | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555224 / Custom 8270<br>Plus Std #2 [2nd lot at \$85<br>per ampul if requested -<br>contact ARM with Request] | A0207706 | 12/05/2024      | 06/05/2024 /<br>Rahul   | 02/05/2024 /<br>Rahul       | S12092         |

[CS 4978-2]

| Supplier | ItemCode / ItemName   | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555224 / Custom 8270<br>Plus Std #2 [2nd lot at \$85<br>per ampul if requested -<br>contact ARM with Request] | A0207706 | 12/05/2024      | 06/05/2024 /<br>Rahul   | 02/05/2024 /<br>Rahul       | S12093         |

[CS 4978-2]

## CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName   | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555224 / Custom 8270<br>Plus Std #2 [2nd lot at \$85<br>per ampul if requested -<br>contact ARM with Request] | A0207706 | 12/05/2024      | 06/05/2024 /<br>Rahul   | 02/05/2024 /<br>Rahul       | S12094         |

[CS 4978-2]

| Supplier | ItemCode / ItemName   | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555224 / Custom 8270<br>Plus Std #2 [2nd lot at \$85<br>per ampul if requested -<br>contact ARM with Request] | A0207706 | 12/05/2024      | 06/05/2024 /<br>Rahul   | 02/05/2024 /<br>Rahul       | S12095         |

[CS 4978-2]

| Supplier | ItemCode / ItemName   | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555224 / Custom 8270<br>Plus Std #2 [2nd lot at \$85<br>per ampul if requested -<br>contact ARM with Request] | A0207706 | 12/05/2024      | 06/05/2024 /<br>Rahul   | 02/05/2024 /<br>Rahul       | S12096         |

[CS 4978-2]

| Supplier | ItemCode / ItemName   | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555224 / Custom 8270<br>Plus Std #2 [2nd lot at \$85<br>per ampul if requested -<br>contact ARM with Request] | A0207706 | 01/09/2025      | 07/09/2024 /<br>Jagrut  | 02/05/2024 /<br>Rahul       | S12097         |

[CS 4978-2]

| Supplier          | ItemCode / ItemName                                   | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|-------------------|---|--------|-----------------|-------------------------|-----------------------------|----------------|
| CPI International | z-010223-01 / 1,4-Dioxane<br>Solution, 2,000mg/L, 1ml | 454157 | 01/09/2025      | 07/09/2024 /<br>Jagrut  | 03/08/2024 /<br>Rahul       | S12112         |

| Supplier | ItemCode / ItemName   | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31850 / 8270 SV Mix,<br>8270 Mega Mix 1mL,<br>1000ug/mL, CH <sub>2</sub> Cl <sub>2</sub> [New<br>Solvent 100% CH <sub>2</sub> Cl <sub>2</sub> ] | A0203726 | 12/05/2024      | 06/05/2024 /<br>Rahul   | 03/15/2024 /<br>Rahul       | S12117         |

## CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName   | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 555869 / Custom Standard, hexachlorocyclopentadiene Std [CS 5328-2] | A0175226 | 08/31/2024      | 06/05/2024 / Rahul      | 08/12/2021 / Christian      | S9675          |

| Supplier         | ItemCode / ItemName | Lot #               | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|---------------------|---------------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | DIW / DI Water      | Daily Lab-Certified | 10/24/2024      | 10/24/2019 / apatel     | 10/24/2019 / apatel         | W2606          |

| Supplier         | ItemCode / ItemName | Lot #               | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|---------------------|---------------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | DIW / DI Water      | Daily Lab-Certified | 07/03/2029      | 07/03/2024 / lwona      | 07/03/2024 / lwona          | W3112          |



5580 Skylane Blvd  
Santa Rosa, CA 95403

(707)525-5788  
(800)878-7654 Toll Free  
(707)545-7901 Fax

Manufacturer's Quality System  
Audited & Registered  
by TUV USA to ISO 9001:2015

Date Received: \_\_\_\_\_

## Certificate of Analysis

Rev 0

Page 1 of 1

|              |          |          |                    |            |   |
|--------------|----------|----------|--------------------|------------|---|
| Catalog No.: | Lot No.: | Storage: | Solvent:           | Exp. Date: | Description:                                      |
| Z-010074-07  | 406703   | ≤ -10 °C | Methylene Chloride | 3/30/2025  | 3,3'-Dichlorobenzidine Solution, 1,000 mg/L, 1 mL |

| Compound               | CAS No. | Purity (%) | Compound Lot No. | Concentration, mg/L |
|------------------------|---------|------------|------------------|---------------------|
| 3,3'-dichlorobenzidine | 91-94-1 | 99.5       | 74.3.26P         | 989 ± 7.53          |

Received on  
02/07/23  
by  
CG  
S11084  
to  
S11088

\*Not a certified value

Certified By: \_\_\_\_\_

Jacob Mulloy  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values  
listed are determined gravimetrically.



5580 Skylane Blvd  
Santa Rosa, CA 95403

(707)525-5788  
(800)878-7654 Toll Free  
(707)545-7901 Fax

Manufacturer's Quality System  
Audited & Registered  
by TUV USA to ISO 9001:2015

Date Received: \_\_\_\_\_

## Certificate of Analysis

Rev 0

Page 1 of 1

|                     |                 |                 |                    |                   |  |
|---------------------|-----------------|-----------------|--------------------|-------------------|--|
| <b>Catalog No.:</b> | <b>Lot No.:</b> | <b>Storage:</b> | <b>Solvent:</b>    | <b>Exp. Date:</b> | <b>Description:</b>                    |
| Z-110817-01         | 414125          | ≤ -10 °C        | Methylene Chloride | 6/21/2025         | Custom 8270 Mix, 4-55, 1000 mg/L, 1 mL |

| Compound                   | CAS No. | Purity (%) | Compound Lot No. | Concentration, mg/L |
|----------------------------|---------|------------|------------------|---------------------|
| acetophenone               | 98-86-2 | 99.2       | 85.8.1P          | 998 ± 11.5          |
| benzoic acid               | 65-85-0 | 100        | 123.7.1P         | 1010 ± 5.88         |
| biphenyl                   | 92-52-4 | 99.9       | 366.29.1P        | 999 ± 5.82          |
| 1,2,4,5-tetrachlorobenzene | 95-94-3 | 99.7       | 53.7.2P          | 993 ± 5.79          |

Received on  
02/07/23  
by  
CG  
S11089  
to  
S11093

\*Not a certified value

Manufactured by o2si smart solutions, Accredited to ISO 9001:2008 by NSF and ISO/IEC 17025:2005 (Certification No. 3031.01) and ISO Guide 34:2009 (Certification No. 3031.02) by A2LA

Certified By: \_\_\_\_\_

Shane Overcash  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values listed are determined gravimetrically.



5580 Skylane Blvd  
Santa Rosa, CA 95403

(707)525-5788  
(800)878-7654 Toll Free  
(707)545-7901 Fax

Manufacturer's Quality System  
Audited & Registered  
by TUV USA to ISO 9001:2015

Date Received: \_\_\_\_\_

## Certificate of Analysis

Rev 0

Page 1 of 1

**Catalog No.:** Lot No.: **Storage:** **Solvent:** **Exp. Date:** **Description:**  
Z-112090 440246  $\leq -10^{\circ}\text{C}$  Methylene Chloride 2/16/2026 CLP Acid Surrogate Solution, 7,500 mg/L, 1 mL  
-04

| Compound                      | CAS No.    | Purity (%) | Compound Lot No. | Concentration, mg/L |
|-------------------------------|------------|------------|------------------|---------------------|
| 2-chlorophenol-d <sub>4</sub> | 93951-73-6 | 99.3       | 248.12.7P        | 7487 $\pm$ 17.2     |
| 2-fluorophenol                | 367-12-4   | 99.8       | 10.7.3.3P        | 7513 $\pm$ 17.26    |
| phenol-d <sub>6</sub>         | 13127-88-3 | 99.9       | 949.120.8P       | 7481 $\pm$ 17.19    |
| 2,4,6-tribromophenol          | 118-79-6   | 99.8       | 12.1.6P          | 7469 $\pm$ 17.17    |

Received on

02/25/21

by  
CG

S9236  
to

S9240

\*Not a certified value

Manufactured by o2si smart solutions, Accredited to ISO 9001:2008 by NSF and ISO/IEC 17025:2005 (Certification No. 3031.01) and ISO Guide 34:2009 (Certification No. 3031.02) by A2LA

*Erica Castiglione*

Certified By:

Erica Castiglione  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values listed are determined gravimetrically.



5580 Skylane Blvd  
Santa Rosa, CA 95403

(707)525-5788  
(800)878-7654 Toll Free  
(707)545-7901 Fax

Receivalon  
02/07/23 by CG

Sheet S11096  
to  
S11099

Manufacturer's Quality System  
Audited & Registered  
by TUV USA to ISO 9001:2015

Date Received: \_\_\_\_\_

## Certificate of Analysis

Rev 0

Page 1 of 4

| Catalog No.: | Lot No.: | Storage: | Solvent:           | Exp. Date: | Description:   |
|--------------|----------|----------|--------------------|------------|--|
| Z-110381-01  | 495831   | ≤ -10 °C | Methylene Chloride | 10/30/2027 | Method 8270 Calibration Solution, 76-1, 500 & 1,000 mg/L, 1 mL |

| Compound                          | CAS No.  | Purity (%) | Compound Lot No. | Concentration, mg/L |
|-----------------------------------|----------|------------|------------------|---------------------|
| acenaphthene                      | 83-32-9  | 99.9       | 13.1.5P          | 1003 ± 17.27        |
| acenaphthylene                    | 208-96-8 | 97.6       | 14.290.1P        | 999.8 ± 17.22       |
| aniline                           | 62-53-3  | 99.9       | 64.7.1P          | 995 ± 17.13         |
| anthracene                        | 120-12-7 | 99.5       | 15.7.1P          | 1001 ± 17.24        |
| azobenzene                        | 103-33-3 | 98.1       | 252.7.2P         | 999.1 ± 17.21       |
| benzo[a]anthracene                | 56-55-3  | 100        | 16.7.3P          | 1001 ± 17.24        |
| benzo[b]fluoranthene              | 205-99-2 | 99.8       | 17.421.3P        | 1001 ± 19.91        |
| benzo[k]fluoranthene              | 207-08-9 | 98.9       | 18.421.4P        | 1001 ± 17.92        |
| benzo[ghi]perylene                | 191-24-2 | 93         | 19.286.4P        | 999.6 ± 19.88       |
| benzo[a]pyrene                    | 50-32-8  | 97         | 20.286.2P        | 999.1 ± 26.35       |
| benzyl alcohol                    | 100-51-6 | 99.9       | 65.18.1P         | 1001 ± 17.24        |
| bis(2-chloroethoxy)methane        | 111-91-1 | 99.1       | 31.3.15P         | 999.7 ± 17.89       |
| bis(2-chloroethyl)ether           | 111-44-4 | 99.8       | 32.7.1P          | 1001 ± 17.23        |
| bis(2-chloro-1-methylethyl) ether | 108-60-1 | 99.5       | 34.3.13P         | 999.5 ± 17.89       |
| bis(2-ethylhexyl)adipate          | 103-23-1 | 99.5       | 874.7.1P         | 999.5 ± 17.21       |
| bis(2-ethylhexyl)phthalate        | 117-81-7 | 99.4       | 33.29.1P         | 998.8 ± 19.86       |
| 4-bromophenyl phenyl ether        | 101-55-3 | 99.4       | 35.7.1P          | 999.1 ± 17.2        |
| butyl benzyl phthalate            | 85-68-7  | 98.4       | 36.1.6P          | 984.7 ± 19.58       |
| carbazole                         | 86-74-8  | 99.4       | 239.7.2P         | 1000 ± 17.22        |

\*Not a certified value

Manufactured by o2si smart solutions, Accredited to ISO 9001:2008 by NSF and ISO/IEC 17025:2005 (Certification No. 3031.01) and ISO Guide 34:2009 (Certification No. 3031.02) by A2LA

*Brianna Smith*

Certified By: \_\_\_\_\_

Brianna Smith  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values listed are determined gravimetrically.

# Certificate of Analysis

Page 4 of 4

Catalog No.: Z-110381-01

Lot No.: 495831

Expiration Date: 10/30/2027

| <u>Compound</u>        | <u>CAS No.</u> | <u>Purity (%)</u> | <u>Compound Lot No.</u> | <u>Concentration, mg/L</u> |
|------------------------|----------------|-------------------|-------------------------|----------------------------|
| 1,2,4-trichlorobenzene | 120-82-1       | 99.6              | 54.29.1P                | 1000 ± 17.22               |
| 2,4,5-trichlorophenol  | 95-95-4        | 96.5              | 121.7.1.1P              | 1000 ± 17.22               |
| 2,4,6-trichlorophenol  | 88-06-2        | 99.6              | 113.7.1P                | 1002 ± 17.25               |

\*Not a certified value

Manufactured by o2si smart solutions, Accredited to ISO 9001:2008 by NSF and ISO/IEC 17025:2005 (Certification No. 3031.01) and ISO Guide 34:2009 (Certification No. 3031.02) by A2LA

Certified By:



Briana Smith  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values listed are determined gravimetrically.





5580 Skylane Blvd  
Santa Rosa, CA 95403

(707)525-5788  
(800)878-7654 Toll Free  
(707)545-7901 Fax

Manufacturer's Quality System  
Audited & Registered  
by TUV USA to ISO 9001:2015

Date Received: \_\_\_\_\_

## Certificate of Analysis

Rev 0

Page 1 of 1

|                     |                 |                 |                    |                   |  |
|---------------------|-----------------|-----------------|--------------------|-------------------|--|
| <b>Catalog No.:</b> | <b>Lot No.:</b> | <b>Storage:</b> | <b>Solvent:</b>    | <b>Exp. Date:</b> | <b>Description:</b>                      |
| Z-010442-07         | 495833          | ≤ -10 °C        | Methylene Chloride | 1/16/2028         | Benzaldehyde Solution, 1000 mg/L, 1.3 mL |

| <u>Compound</u> | <u>CAS No.</u> | <u>Purity (%)</u> | <u>Compound Lot No.</u> | <u>Concentration, mg/L</u> |
|-----------------|----------------|-------------------|-------------------------|----------------------------|
| benzaldehyde    | 100-52-7       | 98.3              | 442.421.1P              | 996.8 ± 11.49              |

Received on  
02/07/23  
by CG

S11101  
to  
S11103

\*Not a certified value

Certified By: \_\_\_\_\_

*S. Hunter*

Scott Hunter  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values  
listed are determined gravimetrically.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

# CERTIFIED REFERENCE MATERIAL

## Gravimetric Certificate



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Received on  
08/12/21  
by  
CG  
S 9671  
to  
S 9675

**Catalog No. :** 555869 **Lot No.:** A0175226

**Description :** Custom Hexachlorocyclopentadiene Standard

Custom Hexachlorocyclopentadiene Standard 25,000µg/mL, Methanol, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** August 31, 2024 **Storage:** 10°C or colder

**Ship:** Ambient

### CERTIFIED VALUES

| Component # | Compound   | Grav. Conc. (weight/volume) | Expanded Uncertainty (95% C.L.; K=2)   |
|-------------|--|-----------------------------|--|
| 1           | Hexachlorocyclopentadiene<br>CAS # 77-47-4 (Lot 0012019)<br>Purity 99% | 25,032.0 µg/mL              | +/- 231.6508 µg/mL Gravimetric<br>+/- 1,251.3257 µg/mL Unstressed<br>+/- 1,281.8032 µg/mL Stressed |

**Solvent:** Methanol  
CAS # 67-56-1  
Purity 99%

*Lane Kibe*  
Lane Kibe - Mix Technician

Date Mixed: 09-Aug-2021

Balance: B345965662

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

| Label Conditions  | Standard Conditions | Non-Standard Conditions |
|---|---------------------|-------------------------|
| 25°C Nominal (Room Temperature)                           | < 60°C              | ≥ 60°C up to 7 days     |
| 10°C or colder (Refrigerate)                              | < 40°C              | ≥ 40°C up to 7 days     |
| 0°C or colder (Freezer)<br>-20°C or colder (Deep Freezer) | < 25°C              | ≥ 25°C up to 7 days     |

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



# CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## Certificate of Analysis



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Received on  
03/10/22  
by  
CG  
S10242  
to  
S10247

**Catalog No. :** 31615 **Lot No.:** A0182667

**Description :** GC/MS Tuning Mixture  
GC/MS Tuning Mixture 1,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** March 31, 2025 **Storage:** 10°C or colder

**Handling:** Contains carcinogen/reproductive toxin. **Ship:** Ambient

### CERTIFIED VALUES

| Elution Order | Compound   | Grav. Conc. (weight/volume) | Expanded Uncertainty (95% C.L.; K=2)   |
|---------------|--|-----------------------------|--|
| 1             | Pentachlorophenol<br>CAS # 87-86-5 (Lot 211229RSR)<br>Purity 99%                     | 1,003.6 µg/mL               | +/- 5.8897 µg/mL Gravimetric<br>+/- 45.7132 µg/mL Unstressed<br>+/- 66.0037 µg/mL Stressed |
| 2             | DFTPP (Decafluorotriphenylphosphine)<br>CAS # 5074-71-5 (Lot Q117-147)<br>Purity 95% | 1,006.6 µg/mL               | +/- 5.9074 µg/mL Gravimetric<br>+/- 45.8508 µg/mL Unstressed<br>+/- 66.2023 µg/mL Stressed |
| 3             | Benzidine<br>CAS # 92-87-5 (Lot 211228JLM)<br>Purity 99%                             | 1,008.4 µg/mL               | +/- 5.9179 µg/mL Gravimetric<br>+/- 45.9318 µg/mL Unstressed<br>+/- 66.3193 µg/mL Stressed |
| 4             | 4,4'-DDT<br>CAS # 50-29-3 (Lot 210916JLM)<br>Purity 99%                              | 1,007.6 µg/mL               | +/- 5.9132 µg/mL Gravimetric<br>+/- 45.8954 µg/mL Unstressed<br>+/- 66.2667 µg/mL Stressed |

**Solvent:** Methylene chloride  
CAS # 75-09-2  
Purity 99%

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

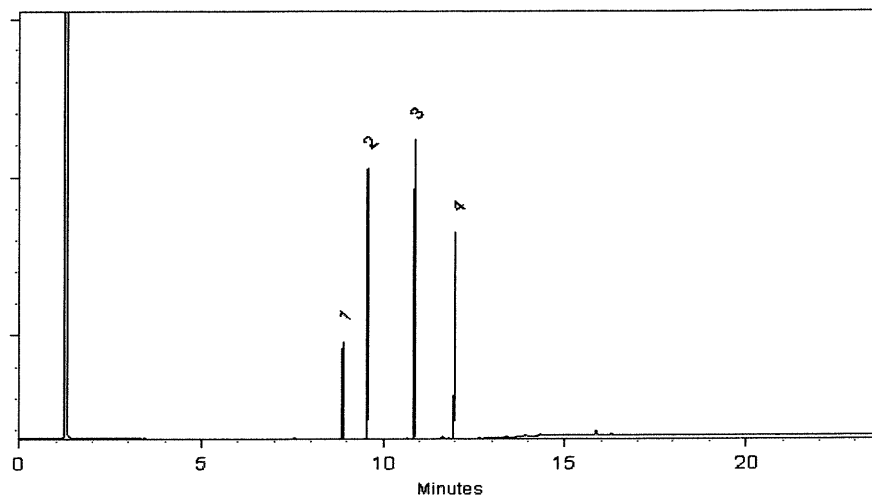

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Morgan Craighead - Mix Technician

Date Mixed: 08-Mar-2022

Balance: B345965662

Marlene Cowan - Operations Tech I

Date Passed: 10-Mar-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



# CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## Gravimetric Certificate



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 555871 Lot No.: A0185300  
Description : Custom 4-Nitrophenol Standard  
Custom 4-Nitrophenol Standard 25,000µg/mL, Methanol, 1mL/ampul  
Container Size : 2 mL Pkg Amt: > 1 mL  
Expiration Date : May 31, 2025 Storage: 10°C or colder  
Ship: Ambient

Received by  
CG ON  
05/18/22  
S10393  
+0  
S10402

### CERTIFIED VALUES

| Component # | Compound  | Grav. Conc. (weight/volume) | Expanded Uncertainty (95% C.L.; K=2)   |
|-------------|---|-----------------------------|--|
| 1           | 4-Nitrophenol<br>CAS # 100-02-7<br>Purity 99%<br>(Lot MKCN1089) | 25,060.0 µg/mL              | +/- 231.9100 µg/mL Gravimetric<br>+/- 753.2622 µg/mL Unstressed<br>+/- 905.6020 µg/mL Stressed |

Solvent: Methanol  
CAS # 67-56-1  
Purity 99%

Katelyn McGinnis - Operations Tech I

Date Mixed: 16-May-2022 Balance: 1128342314

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

| Label Conditions  | Standard Conditions | Non-Standard Conditions |
|---|---------------------|-------------------------|
| 25°C Nominal (Room Temperature)                           | < 60°C              | ≥ 60°C up to 7 days     |
| 10°C or colder (Refrigerate)                              | < 40°C              | ≥ 40°C up to 7 days     |
| 0°C or colder (Freezer)<br>-20°C or colder (Deep Freezer) | < 25°C              | ≥ 25°C up to 7 days     |

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

# CERTIFIED REFERENCE MATERIAL

## Gravimetric Certificate



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Received by  
CG  
on  
07/05/22  
S 10583  
to  
S 10592

**Catalog No. :** 555868 **Lot No.:** A0186373

**Description :** Custom Benzidine Standard  
Custom Benzidine Standard 25,000µg/mL, Methanol, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** June 30, 2025 **Storage:** 10°C or colder

**Handling:** Contains carcinogen/reproductive toxin. **Ship:** Ambient

### CERTIFIED VALUES

| Component # | Compound                      | Grav. Conc. (weight/volume) | Expanded Uncertainty (95% C.L.; K=2) |
|-------------|-------------------------------|-----------------------------|--------------------------------------|
| 1           | Benzidine                     | 25,200.0 µg/mL              | +/- 233.2055 µg/mL Gravimetric       |
|             | CAS # 92-87-5 (Lot 220511RSR) |                             | +/- 351.6606 µg/mL Unstressed        |
|             | Purity 99%                    |                             | +/- 512.6054 µg/mL Stressed          |

**Solvent:** Methanol  
CAS # 67-56-1  
Purity 99%

Tom Suckal - Mix Technician

Date Mixed: 16-Jun-2022 Balance: 1122030677

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

| Label Conditions  | Standard Conditions | Non-Standard Conditions |
|---|---------------------|-------------------------|
| 25°C Nominal (Room Temperature)                           | < 60°C              | ≥ 60°C up to 7 days     |
| 10°C or colder (Refrigerate)                              | < 40°C              | ≥ 40°C up to 7 days     |
| 0°C or colder (Freezer)<br>-20°C or colder (Deep Freezer) | < 25°C              | ≥ 25°C up to 7 days     |

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

# CERTIFIED REFERENCE MATERIAL

## Certificate of Analysis



ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31087 **Lot No.:** A0188108  
**Description :** Acid Surrogate Mix (4/89 SOW)  
Acid Surrogate 10,000µg/mL, Methanol, 5mL/ampul  
**Container Size :** 5 mL **Pkg Amt:** > 5 mL  
**Expiration Date :** August 31, 2030 **Storage:** 10°C or colder  
**Ship:** Ambient

Received by  
CG on  
12/28/22  
S10951  
FO  
S10980

### CERTIFIED VALUES

| Elution Order | Compound   | Grav. Conc. (weight/volume) | Expanded Uncertainty (95% C.L.; K=2)  |
|---------------|--|-----------------------------|---|
| 1             | 2-Fluorophenol<br>CAS # 367-12-4<br>Purity 99%<br>(Lot STBF3761V)      | 10,088.5 µg/mL              | +/- 58.6554 µg/mL Gravimetric<br>+/- 294.4162 µg/mL Unstressed<br>+/- 357.2628 µg/mL Stressed |
| 2             | Phenol-d6<br>CAS # 13127-88-3<br>Purity 99%<br>(Lot PR-31262)          | 10,043.3 µg/mL              | +/- 58.3923 µg/mL Gravimetric<br>+/- 293.0957 µg/mL Unstressed<br>+/- 355.6603 µg/mL Stressed |
| 3             | 2,4,6-Tribromophenol<br>CAS # 118-79-6<br>Purity 99%<br>(Lot MKCJ7664) | 10,010.0 µg/mL              | +/- 58.1990 µg/mL Gravimetric<br>+/- 292.1253 µg/mL Unstressed<br>+/- 354.4829 µg/mL Stressed |

**Solvent:** Methanol  
CAS # 67-56-1  
Purity 99%

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**

FID



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Morgan Craighead - Mix Technician

Date Mixed: 02-Aug-2022

Balance: 1127510105

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 05-Aug-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

# CERTIFIED REFERENCE MATERIAL

## Certificate of Analysis



ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31087 **Lot No.:** A0188108

**Description :** Acid Surrogate Mix (4/89 SOW)

Acid Surrogate 10,000µg/mL, Methanol, 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** August 31, 2030 **Storage:** 10°C or colder

**Ship:** Ambient

Received by  
CG on  
12/28/22  
S10951  
to  
S10980

### CERTIFIED VALUES

| Elution Order | Compound   | Grav. Conc. (weight/volume) | Expanded Uncertainty (95% C.L.; K=2)  |
|---------------|--|-----------------------------|---|
| 1             | 2-Fluorophenol<br>CAS # 367-12-4<br>Purity 99%<br>(Lot STBF3761V)      | 10,088.5 µg/mL              | +/- 58.6554 µg/mL Gravimetric<br>+/- 294.4162 µg/mL Unstressed<br>+/- 357.2628 µg/mL Stressed |
| 2             | Phenol-d6<br>CAS # 13127-88-3<br>Purity 99%<br>(Lot PR-31262)          | 10,043.3 µg/mL              | +/- 58.3923 µg/mL Gravimetric<br>+/- 293.0957 µg/mL Unstressed<br>+/- 355.6603 µg/mL Stressed |
| 3             | 2,4,6-Tribromophenol<br>CAS # 118-79-6<br>Purity 99%<br>(Lot MKCJ7664) | 10,010.0 µg/mL              | +/- 58.1990 µg/mL Gravimetric<br>+/- 292.1253 µg/mL Unstressed<br>+/- 354.4829 µg/mL Stressed |

**Solvent:** Methanol  
CAS # 67-56-1  
Purity 99%

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**

FID



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Morgan Craighead - Mix Technician

Date Mixed: 02-Aug-2022 Balance: 1127510105

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 05-Aug-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

# CERTIFIED REFERENCE MATERIAL

## Certificate of Analysis



ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31087 **Lot No.:** A0188108  
**Description :** Acid Surrogate Mix (4/89 SOW)  
Acid Surrogate 10,000µg/mL, Methanol, 5mL/ampul  
**Container Size :** 5 mL **Pkg Amt:** > 5 mL  
**Expiration Date :** August 31, 2030 **Storage:** 10°C or colder  
**Ship:** Ambient

Received by  
CG on  
12/28/22  
S10951  
to  
S10980

### CERTIFIED VALUES

| Elution Order | Compound   | Grav. Conc. (weight/volume) | Expanded Uncertainty (95% C.L.; K=2)  |
|---------------|--|-----------------------------|---|
| 1             | 2-Fluorophenol<br>CAS # 367-12-4<br>Purity 99%<br>(Lot STBF3761V)      | 10,088.5 µg/mL              | +/- 58.6554 µg/mL Gravimetric<br>+/- 294.4162 µg/mL Unstressed<br>+/- 357.2628 µg/mL Stressed |
| 2             | Phenol-d6<br>CAS # 13127-88-3<br>Purity 99%<br>(Lot PR-31262)          | 10,043.3 µg/mL              | +/- 58.3923 µg/mL Gravimetric<br>+/- 293.0957 µg/mL Unstressed<br>+/- 355.6603 µg/mL Stressed |
| 3             | 2,4,6-Tribromophenol<br>CAS # 118-79-6<br>Purity 99%<br>(Lot MKCJ7664) | 10,010.0 µg/mL              | +/- 58.1990 µg/mL Gravimetric<br>+/- 292.1253 µg/mL Unstressed<br>+/- 354.4829 µg/mL Stressed |

**Solvent:** Methanol  
CAS # 67-56-1  
Purity 99%

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**

FID



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Morgan Craighead - Mix Technician

Date Mixed: 02-Aug-2022 Balance: 1127510105

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 05-Aug-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

# CERTIFIED REFERENCE MATERIAL

## Certificate of Analysis



ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31087 **Lot No.:** A0188108  
**Description :** Acid Surrogate Mix (4/89 SOW)  
Acid Surrogate 10,000µg/mL, Methanol, 5mL/ampul  
**Container Size :** 5 mL **Pkg Amt:** > 5 mL  
**Expiration Date :** August 31, 2030 **Storage:** 10°C or colder  
**Ship:** Ambient

Received by  
CG on  
12/28/22  
S10951  
to  
S10980

### CERTIFIED VALUES

| Elution Order | Compound   | Grav. Conc. (weight/volume) | Expanded Uncertainty (95% C.L.; K=2)  |
|---------------|--|-----------------------------|---|
| 1             | 2-Fluorophenol<br>CAS # 367-12-4<br>Purity 99%<br>(Lot STBF3761V)      | 10,088.5 µg/mL              | +/- 58.6554 µg/mL Gravimetric<br>+/- 294.4162 µg/mL Unstressed<br>+/- 357.2628 µg/mL Stressed |
| 2             | Phenol-d6<br>CAS # 13127-88-3<br>Purity 99%<br>(Lot PR-31262)          | 10,043.3 µg/mL              | +/- 58.3923 µg/mL Gravimetric<br>+/- 293.0957 µg/mL Unstressed<br>+/- 355.6603 µg/mL Stressed |
| 3             | 2,4,6-Tribromophenol<br>CAS # 118-79-6<br>Purity 99%<br>(Lot MKCJ7664) | 10,010.0 µg/mL              | +/- 58.1990 µg/mL Gravimetric<br>+/- 292.1253 µg/mL Unstressed<br>+/- 354.4829 µg/mL Stressed |

**Solvent:** Methanol  
CAS # 67-56-1  
Purity 99%



**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**

FID



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Morgan Craighead - Mix Technician

Date Mixed: 02-Aug-2022

Balance: 1127510105

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 05-Aug-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

# CERTIFIED REFERENCE MATERIAL

## Certificate of Analysis



ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31087 **Lot No.:** A0188108

**Description :** Acid Surrogate Mix (4/89 SOW)

Acid Surrogate 10,000µg/mL, Methanol, 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** August 31, 2030 **Storage:** 10°C or colder

**Ship:** Ambient

Received by  
CG on  
12/28/22  
S10951  
FO  
S10980

### CERTIFIED VALUES

| Elution Order | Compound   | Grav. Conc. (weight/volume) | Expanded Uncertainty (95% C.L.; K=2)  |
|---------------|--|-----------------------------|---|
| 1             | 2-Fluorophenol<br>CAS # 367-12-4<br>Purity 99%<br>(Lot STBF3761V)      | 10,088.5 µg/mL              | +/- 58.6554 µg/mL Gravimetric<br>+/- 294.4162 µg/mL Unstressed<br>+/- 357.2628 µg/mL Stressed |
| 2             | Phenol-d6<br>CAS # 13127-88-3<br>Purity 99%<br>(Lot PR-31262)          | 10,043.3 µg/mL              | +/- 58.3923 µg/mL Gravimetric<br>+/- 293.0957 µg/mL Unstressed<br>+/- 355.6603 µg/mL Stressed |
| 3             | 2,4,6-Tribromophenol<br>CAS # 118-79-6<br>Purity 99%<br>(Lot MKCJ7664) | 10,010.0 µg/mL              | +/- 58.1990 µg/mL Gravimetric<br>+/- 292.1253 µg/mL Unstressed<br>+/- 354.4829 µg/mL Stressed |

**Solvent:** Methanol  
CAS # 67-56-1  
Purity 99%

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**

FID



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Morgan Craighead - Mix Technician

Date Mixed: 02-Aug-2022 Balance: 1127510105

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 05-Aug-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

# CERTIFIED REFERENCE MATERIAL

## Certificate of Analysis



ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31087 **Lot No.:** A0188108  
**Description :** Acid Surrogate Mix (4/89 SOW)  
Acid Surrogate 10,000µg/mL, Methanol, 5mL/ampul  
**Container Size :** 5 mL **Pkg Amt:** > 5 mL  
**Expiration Date :** August 31, 2030 **Storage:** 10°C or colder  
**Ship:** Ambient

Received by  
CG on  
12/28/22  
S10951  
to  
S10980

### CERTIFIED VALUES

| Elution Order | Compound   | Grav. Conc. (weight/volume) | Expanded Uncertainty (95% C.L.; K=2)  |
|---------------|--|-----------------------------|---|
| 1             | 2-Fluorophenol<br>CAS # 367-12-4<br>Purity 99%<br>(Lot STBF3761V)      | 10,088.5 µg/mL              | +/- 58.6554 µg/mL Gravimetric<br>+/- 294.4162 µg/mL Unstressed<br>+/- 357.2628 µg/mL Stressed |
| 2             | Phenol-d6<br>CAS # 13127-88-3<br>Purity 99%<br>(Lot PR-31262)          | 10,043.3 µg/mL              | +/- 58.3923 µg/mL Gravimetric<br>+/- 293.0957 µg/mL Unstressed<br>+/- 355.6603 µg/mL Stressed |
| 3             | 2,4,6-Tribromophenol<br>CAS # 118-79-6<br>Purity 99%<br>(Lot MKCJ7664) | 10,010.0 µg/mL              | +/- 58.1990 µg/mL Gravimetric<br>+/- 292.1253 µg/mL Unstressed<br>+/- 354.4829 µg/mL Stressed |

**Solvent:** Methanol  
CAS # 67-56-1  
Purity 99%

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**

FID



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Morgan Craighead - Mix Technician

Date Mixed: 02-Aug-2022

Balance: 1127510105

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 05-Aug-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Received by  
CG on  
12/28/22  
\$10981  
to  
S11010

**Catalog No. :** 31086 **Lot No.:** A0189418  
**Description :** B/N Surrogate Mix (4/89 SOW)  
Base Neutral Surrogate 5000µg/mL, Methylene Chloride, 5mL/ampul  
**Container Size :** 5 mL **Pkg Amt:** > 5 mL  
**Expiration Date :** August 31, 2028 **Storage:** 10°C or colder  
**Handling:** Sonicate prior to use. **Ship:** Ambient

### CERTIFIED VALUES

| Elution Order | Compound   | Grav. Conc. (weight/volume) | Expanded Uncertainty (95% C.L.; K=2)  |
|---------------|--|-----------------------------|---|
| 1             | Nitrobenzene-d5<br>CAS # 4165-60-0 (Lot PR-29940A)<br>Purity 99% | 5,009.8 µg/mL               | +/- 29.1271 µg/mL Gravimetric<br>+/- 225.6421 µg/mL Unstressed<br>+/- 250.3778 µg/mL Stressed |
| 2             | 2-Fluorobiphenyl<br>CAS # 321-60-8 (Lot 00021384)<br>Purity 99%  | 5,026.6 µg/mL               | +/- 29.2250 µg/mL Gravimetric<br>+/- 226.4003 µg/mL Unstressed<br>+/- 251.2191 µg/mL Stressed |
| 3             | p-Terphenyl-d14<br>CAS # 1718-51-0 (Lot PR-30504)<br>Purity 99%  | 5,027.3 µg/mL               | +/- 29.2289 µg/mL Gravimetric<br>+/- 226.4304 µg/mL Unstressed<br>+/- 251.2524 µg/mL Stressed |

**Solvent:** Methylene chloride  
CAS # 75-09-2  
Purity 99%

#### Tech Tips:

Due to the limited solubility of p-terphenyl-d14 in methanol, we do not recommend that this mixture be diluted in methanol.

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

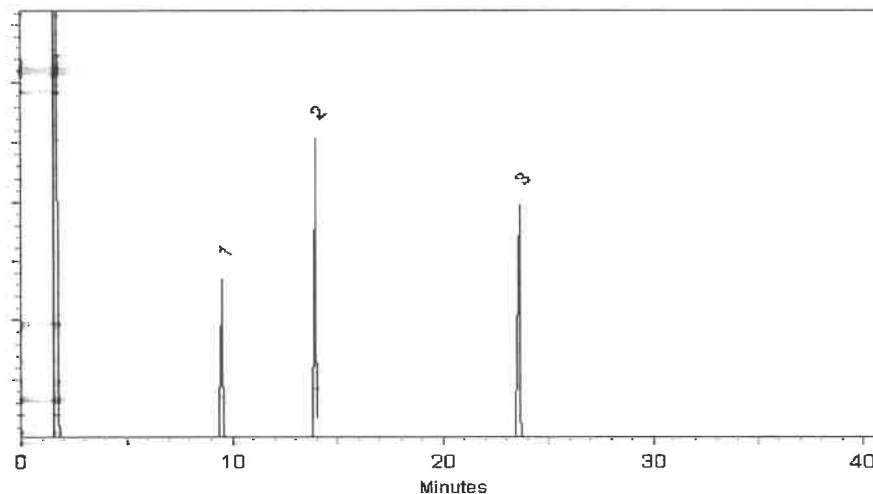

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
John Friedline - Operations Technician I

Date Mixed: 09-Sep-2022

Balance: 1128353505

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 13-Sep-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31086 **Lot No.:** A0189418  
**Description :** B/N Surrogate Mix (4/89 SOW)  
Base Neutral Surrogate 5000µg/mL, Methylene Chloride, 5mL/ampul  
**Container Size :** 5 mL **Pkg Amt:** > 5 mL  
**Expiration Date :** August 31, 2028 **Storage:** 10°C or colder  
**Handling:** Sonicate prior to use. **Ship:** Ambient

Received by  
CG on  
12/28/22  
\$10981  
to  
S11010

### CERTIFIED VALUES

| Elution Order | Compound   | Grav. Conc. (weight/volume) | Expanded Uncertainty (95% C.L.; K=2)  |
|---------------|--|-----------------------------|---|
| 1             | Nitrobenzene-d5<br>CAS # 4165-60-0 (Lot PR-29940A)<br>Purity 99% | 5,009.8 µg/mL               | +/- 29.1271 µg/mL Gravimetric<br>+/- 225.6421 µg/mL Unstressed<br>+/- 250.3778 µg/mL Stressed |
| 2             | 2-Fluorobiphenyl<br>CAS # 321-60-8 (Lot 00021384)<br>Purity 99%  | 5,026.6 µg/mL               | +/- 29.2250 µg/mL Gravimetric<br>+/- 226.4003 µg/mL Unstressed<br>+/- 251.2191 µg/mL Stressed |
| 3             | p-Terphenyl-d14<br>CAS # 1718-51-0 (Lot PR-30504)<br>Purity 99%  | 5,027.3 µg/mL               | +/- 29.2289 µg/mL Gravimetric<br>+/- 226.4304 µg/mL Unstressed<br>+/- 251.2524 µg/mL Stressed |

**Solvent:** Methylene chloride  
CAS # 75-09-2  
Purity 99%

#### Tech Tips:

Due to the limited solubility of p-terphenyl-d14 in methanol, we do not recommend that this mixture be diluted in methanol.



**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

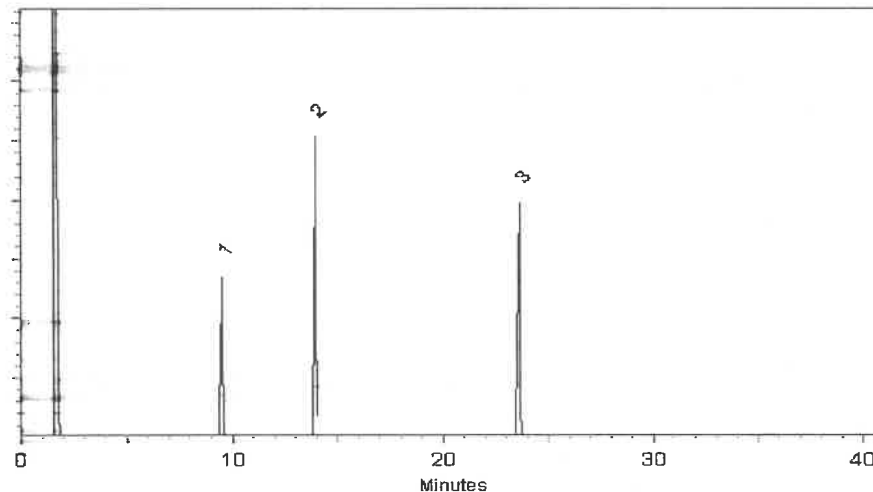

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
John Friedline - Operations Technician I

Date Mixed: 09-Sep-2022

Balance: 1128353505

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 13-Sep-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31086 **Lot No.:** A0189418  
**Description :** B/N Surrogate Mix (4/89 SOW)  
Base Neutral Surrogate 5000µg/mL, Methylene Chloride, 5mL/ampul  
**Container Size :** 5 mL **Pkg Amt:** > 5 mL  
**Expiration Date :** August 31, 2028 **Storage:** 10°C or colder  
**Handling:** Sonicate prior to use. **Ship:** Ambient

Received by  
CG on  
12/28/22  
\$10981  
to  
S11010

### CERTIFIED VALUES

| Elution Order | Compound   | Grav. Conc. (weight/volume) | Expanded Uncertainty (95% C.L.; K=2)  |
|---------------|--|-----------------------------|---|
| 1             | Nitrobenzene-d5<br>CAS # 4165-60-0 (Lot PR-29940A)<br>Purity 99% | 5,009.8 µg/mL               | +/- 29.1271 µg/mL Gravimetric<br>+/- 225.6421 µg/mL Unstressed<br>+/- 250.3778 µg/mL Stressed |
| 2             | 2-Fluorobiphenyl<br>CAS # 321-60-8 (Lot 00021384)<br>Purity 99%  | 5,026.6 µg/mL               | +/- 29.2250 µg/mL Gravimetric<br>+/- 226.4003 µg/mL Unstressed<br>+/- 251.2191 µg/mL Stressed |
| 3             | p-Terphenyl-d14<br>CAS # 1718-51-0 (Lot PR-30504)<br>Purity 99%  | 5,027.3 µg/mL               | +/- 29.2289 µg/mL Gravimetric<br>+/- 226.4304 µg/mL Unstressed<br>+/- 251.2524 µg/mL Stressed |

**Solvent:** Methylene chloride  
CAS # 75-09-2  
Purity 99%

#### Tech Tips:

Due to the limited solubility of p-terphenyl-d14 in methanol, we do not recommend that this mixture be diluted in methanol.

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

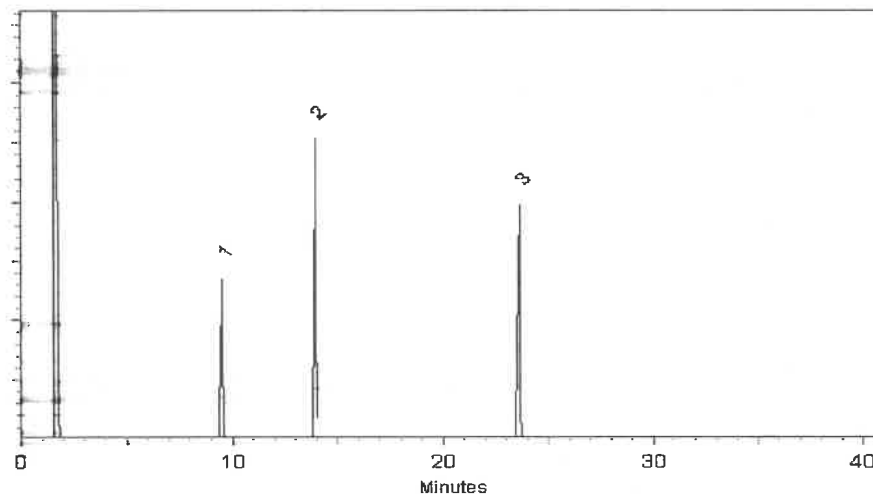

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
John Friedline - Operations Technician I

Date Mixed: 09-Sep-2022

Balance: 1128353505

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 13-Sep-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31086 **Lot No.:** A0189418  
**Description :** B/N Surrogate Mix (4/89 SOW)  
Base Neutral Surrogate 5000µg/mL, Methylene Chloride, 5mL/ampul  
**Container Size :** 5 mL **Pkg Amt:** > 5 mL  
**Expiration Date :** August 31, 2028 **Storage:** 10°C or colder  
**Handling:** Sonicate prior to use. **Ship:** Ambient

Received by  
CG on  
12/28/22  
\$10981  
to  
S11010

### CERTIFIED VALUES

| Elution Order | Compound   | Grav. Conc. (weight/volume) | Expanded Uncertainty (95% C.L.; K=2)  |
|---------------|--|-----------------------------|---|
| 1             | Nitrobenzene-d5<br>CAS # 4165-60-0 (Lot PR-29940A)<br>Purity 99% | 5,009.8 µg/mL               | +/- 29.1271 µg/mL Gravimetric<br>+/- 225.6421 µg/mL Unstressed<br>+/- 250.3778 µg/mL Stressed |
| 2             | 2-Fluorobiphenyl<br>CAS # 321-60-8 (Lot 00021384)<br>Purity 99%  | 5,026.6 µg/mL               | +/- 29.2250 µg/mL Gravimetric<br>+/- 226.4003 µg/mL Unstressed<br>+/- 251.2191 µg/mL Stressed |
| 3             | p-Terphenyl-d14<br>CAS # 1718-51-0 (Lot PR-30504)<br>Purity 99%  | 5,027.3 µg/mL               | +/- 29.2289 µg/mL Gravimetric<br>+/- 226.4304 µg/mL Unstressed<br>+/- 251.2524 µg/mL Stressed |

**Solvent:** Methylene chloride  
CAS # 75-09-2  
Purity 99%

#### Tech Tips:

Due to the limited solubility of p-terphenyl-d14 in methanol, we do not recommend that this mixture be diluted in methanol.

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

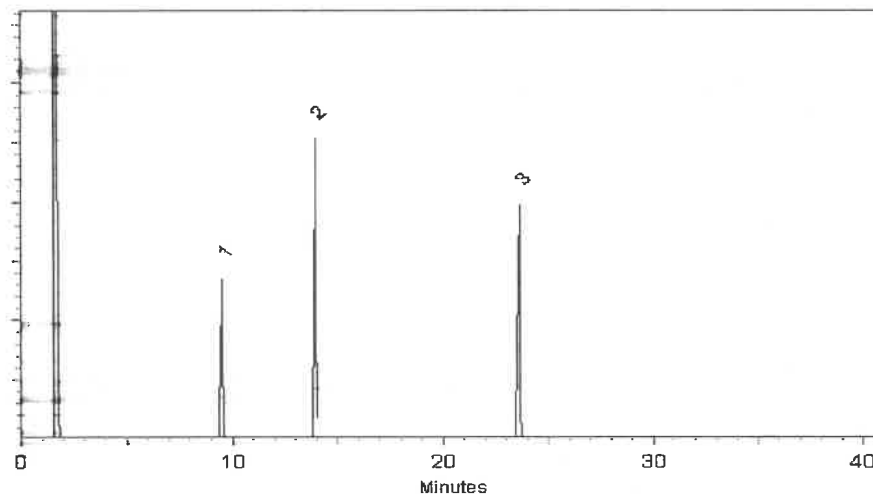

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
John Friedline - Operations Technician I

Date Mixed: 09-Sep-2022

Balance: 1128353505

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 13-Sep-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31086 **Lot No.:** A0189418  
**Description :** B/N Surrogate Mix (4/89 SOW)  
Base Neutral Surrogate 5000µg/mL, Methylene Chloride, 5mL/ampul  
**Container Size :** 5 mL **Pkg Amt:** > 5 mL  
**Expiration Date :** August 31, 2028 **Storage:** 10°C or colder  
**Handling:** Sonicate prior to use. **Ship:** Ambient

Received by  
CG on  
12/28/22  
\$10981  
to  
S11010

### CERTIFIED VALUES

| Elution Order | Compound   | Grav. Conc. (weight/volume) | Expanded Uncertainty (95% C.L.; K=2)  |
|---------------|--|-----------------------------|---|
| 1             | Nitrobenzene-d5<br>CAS # 4165-60-0 (Lot PR-29940A)<br>Purity 99% | 5,009.8 µg/mL               | +/- 29.1271 µg/mL Gravimetric<br>+/- 225.6421 µg/mL Unstressed<br>+/- 250.3778 µg/mL Stressed |
| 2             | 2-Fluorobiphenyl<br>CAS # 321-60-8 (Lot 00021384)<br>Purity 99%  | 5,026.6 µg/mL               | +/- 29.2250 µg/mL Gravimetric<br>+/- 226.4003 µg/mL Unstressed<br>+/- 251.2191 µg/mL Stressed |
| 3             | p-Terphenyl-d14<br>CAS # 1718-51-0 (Lot PR-30504)<br>Purity 99%  | 5,027.3 µg/mL               | +/- 29.2289 µg/mL Gravimetric<br>+/- 226.4304 µg/mL Unstressed<br>+/- 251.2524 µg/mL Stressed |

**Solvent:** Methylene chloride  
CAS # 75-09-2  
Purity 99%

#### Tech Tips:

Due to the limited solubility of p-terphenyl-d14 in methanol, we do not recommend that this mixture be diluted in methanol.

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**

FID



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
John Friedline - Operations Technician I

Date Mixed: 09-Sep-2022

Balance: 1128353505

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 13-Sep-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31086 **Lot No.:** A0189418  
**Description :** B/N Surrogate Mix (4/89 SOW)  
Base Neutral Surrogate 5000µg/mL, Methylene Chloride, 5mL/ampul  
**Container Size :** 5 mL **Pkg Amt:** > 5 mL  
**Expiration Date :** August 31, 2028 **Storage:** 10°C or colder  
**Handling:** Sonicate prior to use. **Ship:** Ambient

Received by  
CG on  
12/28/22  
\$10981  
to  
S11010

### CERTIFIED VALUES

| Elution Order | Compound   | Grav. Conc. (weight/volume) | Expanded Uncertainty (95% C.L.; K=2)  |
|---------------|--|-----------------------------|---|
| 1             | Nitrobenzene-d5<br>CAS # 4165-60-0 (Lot PR-29940A)<br>Purity 99% | 5,009.8 µg/mL               | +/- 29.1271 µg/mL Gravimetric<br>+/- 225.6421 µg/mL Unstressed<br>+/- 250.3778 µg/mL Stressed |
| 2             | 2-Fluorobiphenyl<br>CAS # 321-60-8 (Lot 00021384)<br>Purity 99%  | 5,026.6 µg/mL               | +/- 29.2250 µg/mL Gravimetric<br>+/- 226.4003 µg/mL Unstressed<br>+/- 251.2191 µg/mL Stressed |
| 3             | p-Terphenyl-d14<br>CAS # 1718-51-0 (Lot PR-30504)<br>Purity 99%  | 5,027.3 µg/mL               | +/- 29.2289 µg/mL Gravimetric<br>+/- 226.4304 µg/mL Unstressed<br>+/- 251.2524 µg/mL Stressed |

**Solvent:** Methylene chloride  
CAS # 75-09-2  
Purity 99%

#### Tech Tips:

Due to the limited solubility of p-terphenyl-d14 in methanol, we do not recommend that this mixture be diluted in methanol.



**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

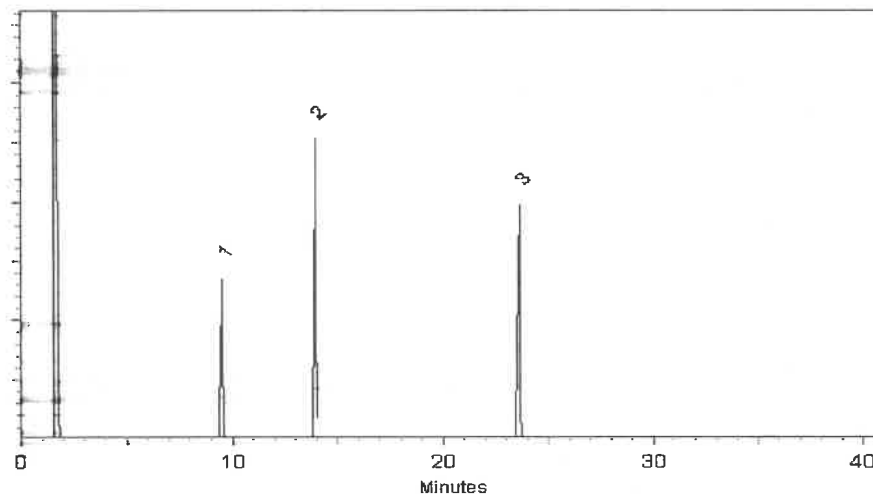

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
John Friedline - Operations Technician I

Date Mixed: 09-Sep-2022

Balance: 1128353505

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 13-Sep-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31086 **Lot No.:** A0189418  
**Description :** B/N Surrogate Mix (4/89 SOW)  
Base Neutral Surrogate 5000µg/mL, Methylene Chloride, 5mL/ampul  
**Container Size :** 5 mL **Pkg Amt:** > 5 mL  
**Expiration Date :** August 31, 2028 **Storage:** 10°C or colder  
**Handling:** Sonicate prior to use. **Ship:** Ambient

Received by  
CG on  
12/28/22  
\$10981  
to  
S11010

### CERTIFIED VALUES

| Elution Order | Compound   | Grav. Conc. (weight/volume) | Expanded Uncertainty (95% C.L.; K=2)  |
|---------------|--|-----------------------------|---|
| 1             | Nitrobenzene-d5<br>CAS # 4165-60-0 (Lot PR-29940A)<br>Purity 99% | 5,009.8 µg/mL               | +/- 29.1271 µg/mL Gravimetric<br>+/- 225.6421 µg/mL Unstressed<br>+/- 250.3778 µg/mL Stressed |
| 2             | 2-Fluorobiphenyl<br>CAS # 321-60-8 (Lot 00021384)<br>Purity 99%  | 5,026.6 µg/mL               | +/- 29.2250 µg/mL Gravimetric<br>+/- 226.4003 µg/mL Unstressed<br>+/- 251.2191 µg/mL Stressed |
| 3             | p-Terphenyl-d14<br>CAS # 1718-51-0 (Lot PR-30504)<br>Purity 99%  | 5,027.3 µg/mL               | +/- 29.2289 µg/mL Gravimetric<br>+/- 226.4304 µg/mL Unstressed<br>+/- 251.2524 µg/mL Stressed |

**Solvent:** Methylene chloride  
CAS # 75-09-2  
Purity 99%

#### Tech Tips:

Due to the limited solubility of p-terphenyl-d14 in methanol, we do not recommend that this mixture be diluted in methanol.

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

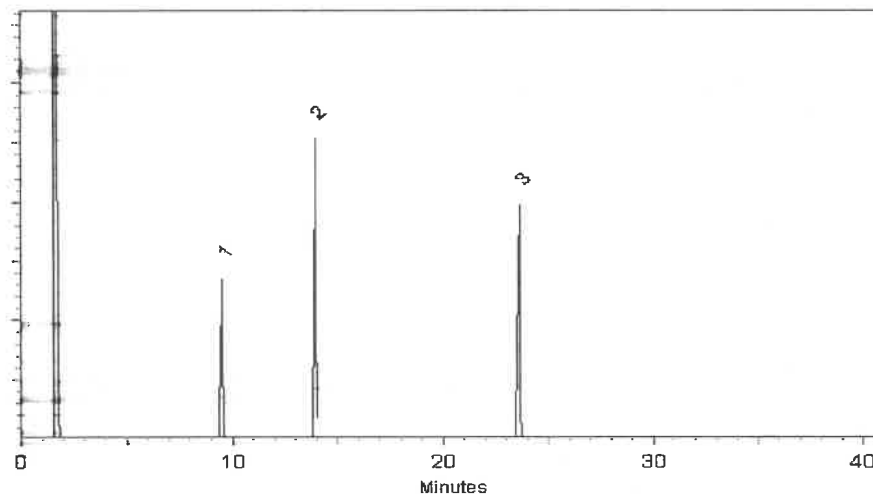

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
John Friedline - Operations Technician I

Date Mixed: 09-Sep-2022

Balance: 1128353505

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 13-Sep-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

# CERTIFIED REFERENCE MATERIAL

## Certificate of Analysis



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Received by  
CG on  
12/28/22  
\$10981  
to  
\$11010

**Catalog No. :** 31086 **Lot No.:** A0189418  
**Description :** B/N Surrogate Mix (4/89 SOW)  
Base Neutral Surrogate 5000µg/mL, Methylene Chloride, 5mL/ampul  
**Container Size :** 5 mL **Pkg Amt:** > 5 mL  
**Expiration Date :** August 31, 2028 **Storage:** 10°C or colder  
**Handling:** Sonicate prior to use. **Ship:** Ambient

### CERTIFIED VALUES

| Elution Order | Compound   | Grav. Conc. (weight/volume) | Expanded Uncertainty (95% C.L.; K=2)  |
|---------------|--|-----------------------------|---|
| 1             | Nitrobenzene-d5<br>CAS # 4165-60-0 (Lot PR-29940A)<br>Purity 99% | 5,009.8 µg/mL               | +/- 29.1271 µg/mL Gravimetric<br>+/- 225.6421 µg/mL Unstressed<br>+/- 250.3778 µg/mL Stressed |
| 2             | 2-Fluorobiphenyl<br>CAS # 321-60-8 (Lot 00021384)<br>Purity 99%  | 5,026.6 µg/mL               | +/- 29.2250 µg/mL Gravimetric<br>+/- 226.4003 µg/mL Unstressed<br>+/- 251.2191 µg/mL Stressed |
| 3             | p-Terphenyl-d14<br>CAS # 1718-51-0 (Lot PR-30504)<br>Purity 99%  | 5,027.3 µg/mL               | +/- 29.2289 µg/mL Gravimetric<br>+/- 226.4304 µg/mL Unstressed<br>+/- 251.2524 µg/mL Stressed |

**Solvent:** Methylene chloride  
CAS # 75-09-2  
Purity 99%

#### Tech Tips:

Due to the limited solubility of p-terphenyl-d14 in methanol, we do not recommend that this mixture be diluted in methanol.

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

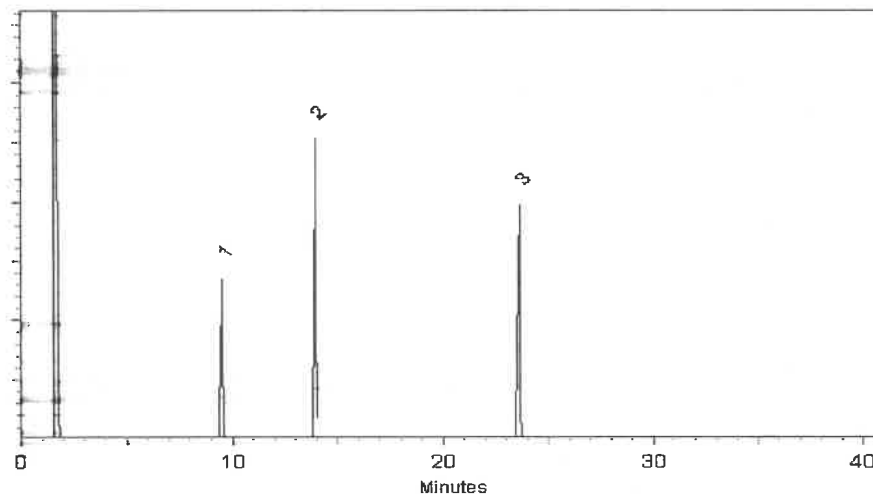

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
John Friedline - Operations Technician I

Date Mixed: 09-Sep-2022

Balance: 1128353505

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 13-Sep-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

gravimetric



## FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 555872 **Lot No.:** A0193449  
**Description :** Custom Pentachlorophenol Standard  
Custom Pentachlorophenol Standard 25,000µg/mL, Methanol,  
1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** January 31, 2026 **Storage:** 10°C or colder  
**Ship:** Ambient

Received on  
01/13/23  
by  
CG  
S11011  
+0  
S11015

## CERTIFIED VALUES

| Component # | Compound          | CAS #   | Lot #    | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|-------------|-------------------|---------|----------|--------|-----------------------------|--|
| 1           | Pentachlorophenol | 87-86-5 | RP221012 | 99%    | 25,050.0 µg/mL              | +/- 778.6378                           |

**Solvent:** Methanol  
**CAS #** 67-56-1  
**Purity** 99%

*Russ Bookhamer*

Russ Bookhamer - Operations Technician I

**Date Mixed:** 11-Jan-2023

**Balance:** B442140311

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 555870 Lot No.: A0194698  
Description : Custom 2,4-Dinitrophenol Standard  
Custom 2,4-Dinitrophenol Standard 25,000µg/mL, Methanol, 1mL/ampul  
Container Size : 2 mL Pkg Amt: > 1 mL  
Expiration Date : February 28, 2026 Storage: 10°C or colder  
Ship: Ambient

CERTIFIED

| Component # | Compound          | CAS #   | Lot #       | Purity | Grav. Conc. (weight/volume) |
|-------------|-------------------|---------|-------------|--------|-----------------------------|
| 1           | 2,4-Dinitrophenol | 51-28-5 | DR221221RSR | 99%    | 25,195.0 µg/mL              |

Solvent: Methanol  
CAS # 67-56-1  
Purity 99%

Russ Bookhamer - Operations Technician I

Date Mixed: 15-Feb-2023

Balance: B442140311

Manufactured under Restek®  
Registered Quality  
Certificate #FM 8



**tified Reference Material Notes**

**es:**

n date valid for unopened ampul stored in compliance with the recommended conditions.  
nty, concentration, and expiration of the CRM are based on the unopened product being stored according to the  
ended condition found in the storage field.

d/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD,  
LC/MS, RI, and/or melting point.

nds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A  
n factor is used to calculate the amount of compound necessary to achieve the desired concentration of the  
mpound in solution.

isomeric compounds is reported as the sum of the isomers.

lues are rounded to the nearest whole number.

**rtainty Value Notes:**

rtainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded  
ty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability  
ty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

erage factor of 2, which gives a level of confidence of approximately 95%.

ged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure  
imum packaged amount can be sufficiently transferred.

**Notes:**

tion is based upon gravimetric preparation using either a balance whose calibration has been verified daily  
Γ traceable weights, and/or dilutions with Class A glassware.

:

the unopened product, when stored in compliance with the recommended conditions, is guaranteed through  
ion displayed on the product label and certificate. Contact Restek for additional opened product stability  
n, with the knowledge/understanding that open product stability is subject to the specific handling and  
ntal conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with  
tards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom  
rm. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861,  
ides complete instructions.

ssolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely



**PRODUCTOS  
QUÍMICOS  
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR  
MONTERREY, N.L. MEXICO  
CP 64070  
TEL +52 81 13 52 57 57  
www.pqm.com.mx

## CERTIFICATE OF ANALYSIS

|                        |                                   |               |                                 |
|------------------------|-----------------------------------|---------------|---------------------------------|
| PRODUCT :              | SODIUM SULFATE CRYSTALS ANHYDROUS |               |                                 |
| QUALITY :              | ACS (CODE RMB3375)                | FORMULA :     | Na <sub>2</sub> SO <sub>4</sub> |
| SPECIFICATION NUMBER : | 6399                              | RELEASE DATE: | ABR/21/2023                     |
| LOT NUMBER :           | 313201                            |               |                                 |

| TEST                                     | SPECIFICATIONS | LOT VALUES  |
|--|----------------|-------------|
| Assay (Na <sub>2</sub> SO <sub>4</sub> ) | Min. 99.0%     | 99.7 %      |
| pH of a 5% solution at 25°C              | 5.2 - 9.2      | 6.1         |
| Insoluble matter                         | Max. 0.01%     | 0.005 %     |
| Loss on ignition                         | Max. 0.5%      | 0.1 %       |
| Chloride (Cl)                            | Max. 0.001%    | <0.001 %    |
| Nitrogen compounds (as N)                | Max. 5 ppm     | <5 ppm      |
| Phosphate (PO <sub>4</sub> )             | Max. 0.001%    | <0.001 %    |
| Heavy metals (as Pb)                     | Max. 5 ppm     | <5 ppm      |
| Iron (Fe)                                | Max. 0.001%    | <0.001 %    |
| Calcium (Ca)                             | Max. 0.01%     | 0.002 %     |
| Magnesium (Mg)                           | Max. 0.005%    | 0.001 %     |
| Potassium (K)                            | Max. 0.008%    | 0.003 %     |
| Extraction-concentration suitability     | Passes test    | Passes test |
| Appearance                               | Passes test    | Passes test |
| Identification                           | Passes test    | Passes test |
| Solubility and foreign matter            | Passes test    | Passes test |
| Retained on US Standard No. 10 sieve     | Max. 1%        | 0.1 %       |
| Retained on US Standard No. 60 sieve     | Min. 94%       | 97.3 %      |
| Through US Standard No. 60 sieve         | Max. 5%        | 2.5 %       |
| Through US Standard No. 100 sieve        | Max. 10%       | 0.1 %       |

### COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/24/23 E 3551

RC-02-01, Ed. 3



# Certificate of Analysis

## Sodium Hydroxide (Pellets)

**Material:** 0583  
**Grade:** ACS GRADE  
**Batch Number:** 23B1556310

**Chemical Formula:** NaOH  
**Molecular Weight:** 40  
**CAS #:** 1310-73-2  
**Appearance:**

**Manufacture Date:** 12/14/2022  
**Expiration Date:** 12/31/2025

**Storage:** Room Temperature

Pellets

| TEST               | SPECIFICATION          | ANALYSIS            | DISPOSITION |
|--------------------|------------------------|---------------------|-------------|
| Calcium            | $\leq 0.005 \%$        | $< 0.005 \%$        | PASS        |
| Chloride           | $\leq 0.005 \%$        | 0.002 %             | PASS        |
| Heavy Metals       | $\leq 0.002 \%$        | $< 0.002 \%$        | PASS        |
| Iron               | $\leq 0.001 \%$        | $< 0.001 \%$        | PASS        |
| Magnesium          | $\leq 0.002 \%$        | $< 0.002 \%$        | PASS        |
| Mercury            | $\leq 0.1 \text{ ppm}$ | $< 0.1 \text{ ppm}$ | PASS        |
| Nickel             | $\leq 0.001 \%$        | $< 0.001 \%$        | PASS        |
| Nitrogen Compounds | $\leq 0.001 \%$        | $< 0.001 \%$        | PASS        |
| Phosphate          | $\leq 0.001 \%$        | $< 0.001 \%$        | PASS        |
| Potassium          | $\leq 0.02 \%$         | $< 0.02 \%$         | PASS        |
| Purity             | $\geq 97.0 \%$         | 99.2 %              | PASS        |
| Sodium Carbonate   | $\leq 1.0 \%$          | 0.5 %               | PASS        |
| Sulfate            | $\leq 0.003 \%$        | $< 0.003 \%$        | PASS        |

Internal ID #: 710

### Signature

We certify that this batch conforms to the specifications listed.

This document has been electronically produced and is valid without a signature.

Leona Edwardson, Quality Control Sr. Manager - Solon  
VWR Chemicals, LLC.  
28600 Fountain Parkway, Solon OH 44139 USA

### Additional Information

Analysis may have been rounded to significant digits in specification limits.

Product meets analytical specifications of the grades listed.



Acetone  
BAKER RESI-ANALYZED® Reagent  
For Organic Residue Analysis



Material No.: 9254-03  
Batch No.: 23H1462005  
Manufactured Date: 2023-07-26  
Expiration Date: 2026-07-25  
Revision No.: 0

## Certificate of Analysis

| Test  | Specification | Result      |
|---|---------------|-------------|
| Assay ((CH <sub>3</sub> ) <sub>2</sub> CO) (by GC, corrected for water) | ≥ 99.4 %      | 99.7 %      |
| Color (APHA)  | ≤ 10          | 5           |
| Residue after Evaporation   | ≤ 1.0 ppm     | 0.3 ppm     |
| Substances Reducing Permanganate  | Passes Test   | Passes Test |
| Titration Acid (μeq/g)  | ≤ 0.3         | 0.1         |
| Titration Base (μeq/g)  | ≤ 0.6         | < 0.1       |
| Water (H <sub>2</sub> O)  | ≤ 0.5 %       | 0.3 %       |
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)    | ≤ 5           | < 1         |
| ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)    | ≤ 10          | 1           |

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

Rec'd by RP on 5/23/24

E 3744

Ken Koehnlein  
Sr. Manager, Quality Assurance

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4  
Batch No.: 24C0162011  
Manufactured Date: 2024-01-04  
Expiration Date: 2025-04-04  
Revision No.: 0

## Certificate of Analysis

| Test   | Specification          | Result   |
|--|------------------------|----------|
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)                       | $\leq 5$               | < 1      |
| ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)                       | $\leq 10$              | 2        |
| Assay ( $\text{CH}_2\text{Cl}_2$ ) (by GC, exclusive of preservative, corrected for water) | $\geq 99.8 \%$         | 100.0 %  |
| Color (APHA)   | $\leq 10$              | 10       |
| Residue after Evaporation  | $\leq 1.0 \text{ ppm}$ | 0.2 ppm  |
| Titration Acid ( $\mu\text{eq/g}$ )  | $\leq 0.3$             | < 0.1    |
| Chloride (Cl)  | $\leq 10 \text{ ppm}$  | < 5 ppm  |
| Water (by KF, coulometric)   | $\leq 0.02 \%$         | < 0.01 % |

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC  
Manufacturer source batch: MG24A04224

E 3746

Ken Koehnlein  
Sr. Manager, Quality Assurance

Acetone  
BAKER RESI-ANALYZED® Reagent  
For Organic Residue Analysis



Material No.: 9254-03  
Batch No.: 23H1462005  
Manufactured Date: 2023-07-26  
Expiration Date: 2026-07-25  
Revision No.: 0

## Certificate of Analysis

| Test  | Specification | Result      |
|---|---------------|-------------|
| Assay ((CH <sub>3</sub> ) <sub>2</sub> CO) (by GC, corrected for water) | ≥ 99.4 %      | 99.7 %      |
| Color (APHA)  | ≤ 10          | 5           |
| Residue after Evaporation   | ≤ 1.0 ppm     | 0.3 ppm     |
| Substances Reducing Permanganate  | Passes Test   | Passes Test |
| Titration Acid (μeq/g)  | ≤ 0.3         | 0.1         |
| Titration Base (μeq/g)  | ≤ 0.6         | < 0.1       |
| Water (H <sub>2</sub> O)  | ≤ 0.5 %       | 0.3 %       |
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)    | ≤ 5           | < 1         |
| ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)    | ≤ 10          | 1           |

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 5/31/24

E3753

Ken Koehnlein  
Sr. Manager, Quality Assurance

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4  
Batch No.: 24E2462004  
Manufactured Date: 2024-04-10  
Expiration Date: 2025-07-10  
Revision No.: 0

## Certificate of Analysis

| Test   | Specification          | Result   |
|--|------------------------|----------|
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)                       | $\leq 5$               | 3        |
| ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)                       | $\leq 10$              | 3        |
| Assay ( $\text{CH}_2\text{Cl}_2$ ) (by GC, exclusive of preservative, corrected for water) | $\geq 99.8 \%$         | 100.0 %  |
| Color (APHA)   | $\leq 10$              | 5        |
| Residue after Evaporation  | $\leq 1.0 \text{ ppm}$ | 0.1 ppm  |
| Titration Acid ( $\mu\text{eq/g}$ )  | $\leq 0.3$             | < 0.1    |
| Chloride (Cl)  | $\leq 10 \text{ ppm}$  | 5 ppm    |
| Water (by KF, coulometric)   | $\leq 0.02 \%$         | < 0.01 % |

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC  
Manufacturer source batch: MG24D10725

E 3768

Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087, U.S.A. Phone 610.386.1700

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4  
Batch No.: 24F1062004  
Manufactured Date: 2024-04-15  
Expiration Date: 2025-07-15  
Revision No.: 0

## Certificate of Analysis

| Test   | Specification  | Result   |
|--|----------------|----------|
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)                             | $\leq 5$       | < 1      |
| ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)                             | $\leq 10$      | 7        |
| Assay (CH <sub>2</sub> Cl <sub>2</sub> ) (by GC, exclusive of preservative, corrected for water) | $\geq 99.8 \%$ | 100.0 %  |
| Color (APHA)   | $\leq 10$      | 5        |
| Residue after Evaporation  | $\leq 1.0$ ppm | 0.1 ppm  |
| Titration Acid ( $\mu$ eq/g)   | $\leq 0.3$     | < 0.1    |
| Chloride (Cl)  | $\leq 10$ ppm  | < 5 ppm  |
| Water (by KF, coulometric)   | $\leq 0.02 \%$ | < 0.01 % |

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC  
Manufacturer source batch: MG24D15750

E 3771

Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1



Sulfuric Acid

BAKER INSTRA-ANALYZED® Reagent

For Trace Metal Analysis

Low Selenium

avantorsm



Material No.: 9673-33

Batch No.: 0000250349

Manufactured Date: 2019/12/17

Retest Date: 2024/12/15

Revision No: 1

## Certificate of Analysis

| Test   | Specification | Result |
|--|---------------|--------|
| ACS - Assay (H <sub>2</sub> SO <sub>4</sub> )                | 95.0 - 98.0 % | 96.5   |
| Appearance   | Passes Test   | PT     |
| ACS - Color (APHA)   | <= 10         | 5      |
| ACS - Residue after Ignition                                 | <= 3 ppm      | 1      |
| ACS - Substances Reducing Permanganate (as SO <sub>2</sub> ) | <= 2 ppm      | < 2    |
| Ammonium (NH <sub>4</sub> )                                  | <= 1 ppm      | < 1    |
| Chloride (Cl)  | <= 0.1 ppm    | < 0.1  |
| Nitrate (NO <sub>3</sub> )                                   | <= 0.2 ppm    | < 0.1  |
| Phosphate (PO <sub>4</sub> )                                 | <= 0.5 ppm    | < 0.1  |
| Trace Impurities - Aluminum (Al)                             | <= 30.0 ppb   | 0.2    |
| Arsenic and Antimony (as As)                                 | <= 4 ppb      | < 2    |
| Trace Impurities - Barium (Ba)                               | <= 10.0 ppb   | < 1.0  |
| Trace Impurities - Beryllium (Be)                            | <= 10.0 ppb   | < 1.0  |
| Trace Impurities - Bismuth (Bi)                              | <= 10.0 ppb   | < 1.0  |
| Trace Impurities - Boron (B)                                 | <= 10.0 ppb   | < 5.0  |
| Trace Impurities - Cadmium (Cd)                              | <= 2.0 ppb    | < 0.3  |
| Trace Impurities - Calcium (Ca)                              | <= 50.0 ppb   | 2.9    |
| Trace Impurities - Chromium (Cr)                             | <= 6.0 ppb    | < 0.4  |
| Trace Impurities - Cobalt (Co)                               | <= 0.5 ppb    | < 0.3  |
| Trace Impurities - Copper (Cu)                               | <= 1.0 ppb    | < 0.1  |
| Trace Impurities - Gallium (Ga)                              | <= 10.0 ppb   | < 1.0  |
| Trace Impurities - Germanium (Ge)                            | <= 10.0 ppb   | < 10.0 |
| Trace Impurities - Gold (Au)                                 | <= 10.0 ppb   | < 0.2  |
| Heavy Metals (as Pb)   | <= 500 ppb    | < 100  |

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC


100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Material No.: 9673-33  
Batch No.: 0000250349

| Test                               | Specification | Result |
|------------------------------------|---------------|--------|
| Trace Impurities - Iron (Fe)       | <= 50.0 ppb   | 4.1    |
| Trace Impurities - Lead (Pb)       | <= 0.5 ppb    | < 0.5  |
| Trace Impurities - Lithium (Li)    | <= 10.0 ppb   | < 1.0  |
| Trace Impurities - Magnesium (Mg)  | <= 7.0 ppb    | 0.4    |
| Trace Impurities - Manganese (Mn)  | <= 1.0 ppb    | < 0.4  |
| Trace Impurities - Mercury (Hg)    | <= 0.5 ppb    | < 0.1  |
| Trace Impurities - Molybdenum (Mo) | <= 10.0 ppb   | < 5.0  |
| Trace Impurities - Nickel (Ni)     | <= 2.0 ppb    | < 0.3  |
| Trace Impurities - Niobium (Nb)    | <= 10.0 ppb   | < 1.0  |
| Trace Impurities - Potassium (K)   | <= 500.0 ppb  | < 2.0  |
| Trace Impurities - Selenium (Se)   | <= 50.0 ppb   | 22.9   |
| Trace Impurities - Silicon (Si)    | <= 100.0 ppb  | < 10.0 |
| Trace Impurities - Silver (Ag)     | <= 1.0 ppb    | < 0.3  |
| Trace Impurities - Sodium (Na)     | <= 500.0 ppb  | 2.7    |
| Trace Impurities - Strontium (Sr)  | <= 5.0 ppb    | < 0.2  |
| Trace Impurities - Tantalum (Ta)   | <= 10.0 ppb   | < 5.0  |
| Trace Impurities - Thallium (Tl)   | <= 20.0 ppb   | < 5.0  |
| Trace Impurities - Tin (Sn)        | <= 5.0 ppb    | < 0.8  |
| Trace Impurities - Titanium (Ti)   | <= 10.0 ppb   | < 1.0  |
| Trace Impurities - Vanadium (V)    | <= 10.0 ppb   | < 1.0  |
| Trace Impurities - Zinc (Zn)       | <= 5.0 ppb    | 0.3    |
| Trace Impurities - Zirconium (Zr)  | <= 10.0 ppb   | < 1.0  |

For Laboratory, Research or Manufacturing Use

Country of Origin: US  
Packaging Site: Phillipsburg Mfg Ctr & DC

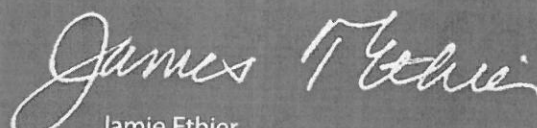  
Jamie Ethier  
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC  
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700



5580 Skyline Blvd  
Santa Rosa, CA 95403

(707)525-5788  
(800)878-7654 Toll Free  
(707)545-7901 Fax

Manufacturer's Quality System  
Audited & Registered  
by TUV USA to ISO 9001:2015

Date Received: \_\_\_\_\_

## Certificate of Analysis

Page 1 of 1

Catalog No.: Lot No.:  
Z-110094-02 503442

Solvent: Storage:  
Methylene Chloride  $\leq -10^{\circ}\text{C}$

Exp. Date: Description:  
8/26/2024 CLP Base/Neutral Surrogate Solution, 5,000 mg/L, 1 ml

| Compound                   | CAS No.   | Purity (%) | Compound Lot No. | Concentration, mg/L |
|----------------------------|-----------|------------|------------------|---------------------|
| 1,2-dichlorobenzene- $d_4$ | 2199-69-1 | 99.7       | 247.29.3P        | 5052 $\pm$ 122.61   |
| 2-fluorobiphenyl           | 321-60-8  | 99.7       | 8.7.1.1P         | 5005 $\pm$ 121.47   |
| nitrobenzene- $d_4$        | 4165-60-0 | 100        | 7.9.2P           | 5040 $\pm$ 122.21   |
| p-terphenyl- $d_{14}$      | 1718-51-0 | 99.6       | 9.12.9P          | 5027 $\pm$ 122      |

\*Not a certified value

Certified By: \_\_\_\_\_

*Joanna Radu*

Joanna Radu  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values  
listed are determined gravimetrically.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 555223 Lot No.: A0201940  
Description: Custom 8270 Plus Standard #1  
Custom 8270 Plus Standard #1 1,000µg/mL, Methylene Chloride, 1mL/ampul  
Container Size: 2 mL  
Expiration Date: September 30, 2025  
Handling: This product is photosensitive.  
Pkg Amt: > 1 mL  
Storage: 10°C or colder  
Ship: Ambient

511539  
↓  
51568  
} 7.P.  
09/19/

| CERTIFIED VALUES            |                        |           |            |        |                             |  |
|-----------------------------|------------------------|-----------|------------|--------|-----------------------------|--|
| Component #                 | Compound               | CAS #     | Lot #      | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
| 1                           | 3,3'-Dichlorobenzidine | 91-94-1   | S230321RSR | 99%    | 1,001.0 µg/mL               | +/- 22.9799                            |
| 2                           | Atrazine               | 1912-24-9 | 5FYWL      | 99%    | 1,010.0 µg/mL               | +/- 23.1865                            |
| 3                           | Benzidine              | 92-87-5   | S221205RSR | 99%    | 1,008.0 µg/mL               | +/- 23.1406                            |
| 4                           | epsilon-Caprolactam    | 105-60-2  | I16X016    | 99%    | 1,008.0 µg/mL               | +/- 23.1406                            |
| Solvent: Methylene chloride |                        |           |            |        |                             |  |
| CAS # 75-09-2               |                        |           |            |        |                             |  |
| Purity 99%                  |                        |           |            |        |                             |  |

REVIEWED

By Jennifer Pollino at 7:10 am, Sep 13, 2023

Sam Moodler - Operations Tech I

Date Mixed: 13-Sep-2023

Balance: B345965662

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 555223 Lot No.: A0201940  
Description: Custom 8270 Plus Standard #1  
Custom 8270 Plus Standard #1 1,000µg/mL, Methylene Chloride, 1mL/ampul  
Container Size: 2 mL Pkg Amt: > 1 mL  
Expiration Date: September 30, 2025 Storage: 10°C or colder  
Handling: This product is photosensitive. Ship: Ambient

511539  
↓  
51568  
} 7.P.  
09/19/

| CERTIFIED VALUES            |                        |           |            |        |                             |  |
|-----------------------------|------------------------|-----------|------------|--------|-----------------------------|--|
| Component #                 | Compound               | CAS #     | Lot #      | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
| 1                           | 3,3'-Dichlorobenzidine | 91-94-1   | S230321RSR | 99%    | 1,001.0 µg/mL               | +/- 22.9799                            |
| 2                           | Atrazine               | 1912-24-9 | 5FYWL      | 99%    | 1,010.0 µg/mL               | +/- 23.1865                            |
| 3                           | Benzidine              | 92-87-5   | S221205RSR | 99%    | 1,008.0 µg/mL               | +/- 23.1406                            |
| 4                           | epsilon-Caprolactam    | 105-60-2  | I16X016    | 99%    | 1,008.0 µg/mL               | +/- 23.1406                            |
| Solvent: Methylene chloride |                        |           |            |        |                             |  |
| CAS # 75-09-2               |                        |           |            |        |                             |  |
| Purity 99%                  |                        |           |            |        |                             |  |

REVIEWED

By Jennifer Pollino at 7:10 am, Sep 13, 2023

Sam Moodler - Operations Tech I

Date Mixed: 13-Sep-2023

Balance: B345965662

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 555223 Lot No.: A0201940  
Description: Custom 8270 Plus Standard #1  
Custom 8270 Plus Standard #1 1,000µg/mL, Methylene Chloride, 1mL/ampul  
Container Size: 2 mL  
Expiration Date: September 30, 2025  
Handling: This product is photosensitive.  
Pkg Amt: > 1 mL  
Storage: 10°C or colder  
Ship: Ambient

511539  
↓  
51568  
} 7.P.  
09/19/

| CERTIFIED VALUES            |                        |           |            |        |                             |  |
|-----------------------------|------------------------|-----------|------------|--------|-----------------------------|--|
| Component #                 | Compound               | CAS #     | Lot #      | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
| 1                           | 3,3'-Dichlorobenzidine | 91-94-1   | S230321RSR | 99%    | 1,001.0 µg/mL               | +/- 22.9799                            |
| 2                           | Atrazine               | 1912-24-9 | 5FYWL      | 99%    | 1,010.0 µg/mL               | +/- 23.1865                            |
| 3                           | Benzidine              | 92-87-5   | S221205RSR | 99%    | 1,008.0 µg/mL               | +/- 23.1406                            |
| 4                           | epsilon-Caprolactam    | 105-60-2  | I16X016    | 99%    | 1,008.0 µg/mL               | +/- 23.1406                            |
| Solvent: Methylene chloride |                        |           |            |        |                             |  |
| CAS # 75-09-2               |                        |           |            |        |                             |  |
| Purity 99%                  |                        |           |            |        |                             |  |

REVIEWED

By Jennifer Pollino at 7:10 am, Sep 13, 2023

Sam Moodler - Operations Tech I

Date Mixed: 13-Sep-2023

Balance: B345965662

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 555223 Lot No.: A0201940  
Description: Custom 8270 Plus Standard #1  
Custom 8270 Plus Standard #1 1,000µg/mL, Methylene Chloride, 1mL/ampul  
Container Size: 2 mL  
Expiration Date: September 30, 2025  
Handling: This product is photosensitive.  
Pkg Amt: > 1 mL  
Storage: 10°C or colder  
Ship: Ambient

511539  
↓  
51568  
} 7.P.  
09/19/

| CERTIFIED VALUES            |                        |           |            |        |                             |  |
|-----------------------------|------------------------|-----------|------------|--------|-----------------------------|--|
| Component #                 | Compound               | CAS #     | Lot #      | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
| 1                           | 3,3'-Dichlorobenzidine | 91-94-1   | S230321RSR | 99%    | 1,001.0 µg/mL               | +/- 22.9799                            |
| 2                           | Atrazine               | 1912-24-9 | 5FYWL      | 99%    | 1,010.0 µg/mL               | +/- 23.1865                            |
| 3                           | Benzidine              | 92-87-5   | S221205RSR | 99%    | 1,008.0 µg/mL               | +/- 23.1406                            |
| 4                           | epsilon-Caprolactam    | 105-60-2  | I16X016    | 99%    | 1,008.0 µg/mL               | +/- 23.1406                            |
| Solvent: Methylene chloride |                        |           |            |        |                             |  |
| CAS # 75-09-2               |                        |           |            |        |                             |  |
| Purity 99%                  |                        |           |            |        |                             |  |

REVIEWED

By Jennifer Pollino at 7:10 am, Sep 13, 2023

Sam Moodler - Operations Tech I

Date Mixed: 13-Sep-2023

Balance: B345965662

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 555223 Lot No.: A0201940  
Description: Custom 8270 Plus Standard #1  
Custom 8270 Plus Standard #1 1,000µg/mL, Methylene Chloride, 1mL/ampul  
Container Size: 2 mL  
Expiration Date: September 30, 2025  
Handling: This product is photosensitive.  
Pkg Amt: > 1 mL  
Storage: 10°C or colder  
Ship: Ambient

511539  
↓  
51568  
} 7.P.  
09/19/

| CERTIFIED VALUES            |                        |           |            |        |                             |  |
|-----------------------------|------------------------|-----------|------------|--------|-----------------------------|--|
| Component #                 | Compound               | CAS #     | Lot #      | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
| 1                           | 3,3'-Dichlorobenzidine | 91-94-1   | S230321RSR | 99%    | 1,001.0 µg/mL               | +/- 22.9799                            |
| 2                           | Atrazine               | 1912-24-9 | 5FYWL      | 99%    | 1,010.0 µg/mL               | +/- 23.1865                            |
| 3                           | Benzidine              | 92-87-5   | S221205RSR | 99%    | 1,008.0 µg/mL               | +/- 23.1406                            |
| 4                           | epsilon-Caprolactam    | 105-60-2  | I16X016    | 99%    | 1,008.0 µg/mL               | +/- 23.1406                            |
| Solvent: Methylene chloride |                        |           |            |        |                             |  |
| CAS # 75-09-2               |                        |           |            |        |                             |  |
| Purity 99%                  |                        |           |            |        |                             |  |

REVIEWED

By Jennifer Pollino at 7:10 am, Sep 13, 2023

Sam Moodler - Operations Tech I

Date Mixed: 13-Sep-2023

Balance: B345965662

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 555223 Lot No.: A0201940  
Description: Custom 8270 Plus Standard #1  
Custom 8270 Plus Standard #1 1,000µg/mL, Methylene Chloride, 1mL/ampul  
Container Size: 2 mL  
Expiration Date: September 30, 2025  
Handling: This product is photosensitive.  
Pkg Amt: > 1 mL  
Storage: 10°C or colder  
Ship: Ambient

511539  
↓  
51568  
} 7.P.  
09/19/

| CERTIFIED VALUES            |                        |           |            |        |                             |  |
|-----------------------------|------------------------|-----------|------------|--------|-----------------------------|--|
| Component #                 | Compound               | CAS #     | Lot #      | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
| 1                           | 3,3'-Dichlorobenzidine | 91-94-1   | S230321RSR | 99%    | 1,001.0 µg/mL               | +/- 22.9799                            |
| 2                           | Atrazine               | 1912-24-9 | 5FYWL      | 99%    | 1,010.0 µg/mL               | +/- 23.1865                            |
| 3                           | Benzidine              | 92-87-5   | S221205RSR | 99%    | 1,008.0 µg/mL               | +/- 23.1406                            |
| 4                           | epsilon-Caprolactam    | 105-60-2  | I16X016    | 99%    | 1,008.0 µg/mL               | +/- 23.1406                            |
| Solvent: Methylene chloride |                        |           |            |        |                             |  |
| CAS # 75-09-2               |                        |           |            |        |                             |  |
| Purity 99%                  |                        |           |            |        |                             |  |

REVIEWED

By Jennifer Pollino at 7:10 am, Sep 13, 2023

Sam Moodler - Operations Tech I

Date Mixed: 13-Sep-2023

Balance: B345965662

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 555223 Lot No.: A0201940  
Description: Custom 8270 Plus Standard #1  
Custom 8270 Plus Standard #1 1,000µg/mL, Methylene Chloride, 1mL/ampul  
Container Size: 2 mL  
Expiration Date: September 30, 2025  
Handling: This product is photosensitive.  
Pkg Amt: > 1 mL  
Storage: 10°C or colder  
Ship: Ambient

511539  
↓  
51568  
} 7.P.  
09/19/

| CERTIFIED VALUES            |                        |           |            |        |                             |  |
|-----------------------------|------------------------|-----------|------------|--------|-----------------------------|--|
| Component #                 | Compound               | CAS #     | Lot #      | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
| 1                           | 3,3'-Dichlorobenzidine | 91-94-1   | S230321RSR | 99%    | 1,001.0 µg/mL               | +/- 22.9799                            |
| 2                           | Atrazine               | 1912-24-9 | 5FYWL      | 99%    | 1,010.0 µg/mL               | +/- 23.1865                            |
| 3                           | Benzidine              | 92-87-5   | S221205RSR | 99%    | 1,008.0 µg/mL               | +/- 23.1406                            |
| 4                           | epsilon-Caprolactam    | 105-60-2  | I16X016    | 99%    | 1,008.0 µg/mL               | +/- 23.1406                            |
| Solvent: Methylene chloride |                        |           |            |        |                             |  |
| CAS # 75-09-2               |                        |           |            |        |                             |  |
| Purity 99%                  |                        |           |            |        |                             |  |

REVIEWED

By Jennifer Pollino at 7:10 am, Sep 13, 2023

Sam Moodler - Operations Tech I

Date Mixed: 13-Sep-2023

Balance: B345965662

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 555223 Lot No.: A0201940  
Description: Custom 8270 Plus Standard #1  
Custom 8270 Plus Standard #1 1,000µg/mL, Methylene Chloride, 1mL/ampul  
Container Size: 2 mL  
Expiration Date: September 30, 2025  
Handling: This product is photosensitive.  
Pkg Amt: > 1 mL  
Storage: 10°C or colder  
Ship: Ambient

511539  
↓  
51568  
} 7.P.  
09/19/

| CERTIFIED VALUES            |                        |           |            |        |                             |  |
|-----------------------------|------------------------|-----------|------------|--------|-----------------------------|--|
| Component #                 | Compound               | CAS #     | Lot #      | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
| 1                           | 3,3'-Dichlorobenzidine | 91-94-1   | S230321RSR | 99%    | 1,001.0 µg/mL               | +/- 22.9799                            |
| 2                           | Atrazine               | 1912-24-9 | 5FYWL      | 99%    | 1,010.0 µg/mL               | +/- 23.1865                            |
| 3                           | Benzidine              | 92-87-5   | S221205RSR | 99%    | 1,008.0 µg/mL               | +/- 23.1406                            |
| 4                           | epsilon-Caprolactam    | 105-60-2  | I16X016    | 99%    | 1,008.0 µg/mL               | +/- 23.1406                            |
| Solvent: Methylene chloride |                        |           |            |        |                             |  |
| CAS # 75-09-2               |                        |           |            |        |                             |  |
| Purity 99%                  |                        |           |            |        |                             |  |

REVIEWED

By Jennifer Pollino at 7:10 am, Sep 13, 2023

Sam Moodler - Operations Tech I

Date Mixed: 13-Sep-2023

Balance: B345965662

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 555223 Lot No.: A0201940  
Description: Custom 8270 Plus Standard #1  
Custom 8270 Plus Standard #1 1,000µg/mL, Methylene Chloride, 1mL/ampul  
Container Size: 2 mL  
Expiration Date: September 30, 2025  
Handling: This product is photosensitive.  
Pkg Amt: > 1 mL  
Storage: 10°C or colder  
Ship: Ambient

511539  
↓  
51568  
} 7.P.  
09/19/

| CERTIFIED VALUES            |                        |           |            |        |                             |  |
|-----------------------------|------------------------|-----------|------------|--------|-----------------------------|--|
| Component #                 | Compound               | CAS #     | Lot #      | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
| 1                           | 3,3'-Dichlorobenzidine | 91-94-1   | S230321RSR | 99%    | 1,001.0 µg/mL               | +/- 22.9799                            |
| 2                           | Atrazine               | 1912-24-9 | 5FYWL      | 99%    | 1,010.0 µg/mL               | +/- 23.1865                            |
| 3                           | Benzidine              | 92-87-5   | S221205RSR | 99%    | 1,008.0 µg/mL               | +/- 23.1406                            |
| 4                           | epsilon-Caprolactam    | 105-60-2  | I16X016    | 99%    | 1,008.0 µg/mL               | +/- 23.1406                            |
| Solvent: Methylene chloride |                        |           |            |        |                             |  |
| CAS # 75-09-2               |                        |           |            |        |                             |  |
| Purity 99%                  |                        |           |            |        |                             |  |

REVIEWED

By Jennifer Pollino at 7:10 am, Sep 13, 2023

Sam Moodler - Operations Tech I

Date Mixed: 13-Sep-2023

Balance: B345965662

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

**Catalog No. :** 31853 **Lot No.:** A0196453  
**Description :** 1,4-dioxane  
1,4-Dioxane 2,000µg/mL, Methylene Chloride, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** March 31, 2028 **Storage:** 0°C or colder  
**Ship:** Ambient

S11749  
↓  
S11794 } RC / 11/30/23

### CERTIFIED VALUES

| Elution Order | Compound    | CAS #    | Lot #    | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|-------------|----------|----------|--------|-----------------------------|--|
| 1             | 1,4-Dioxane | 123-91-1 | SHBN3770 | 99%    | 2,013.0 µg/mL               | +/- 25.0521                            |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant flow 1.8 mL/min.

**Temp. Program:**

80°C (hold 0.1 min.) to 330°C  
@ 9.6°C/min. (hold 2.86 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

340°C

**Det. Type:**

FID

**Split Vent:**

100 mL/min.

**Inj. Vol**

1µl



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Sam Moodler*  
Sam Moodler - Operations Tech I

Date Mixed: 30-Mar-2023

Balance Serial # B707717271

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 31-Mar-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

**Catalog No. :** 31853 **Lot No.:** A0196453  
**Description :** 1,4-dioxane  
1,4-Dioxane 2,000µg/mL, Methylene Chloride, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** March 31, 2028 **Storage:** 0°C or colder  
**Ship:** Ambient

S11749  
↓  
S11794 } RC / 11/30/23

### CERTIFIED VALUES

| Elution Order | Compound    | CAS #    | Lot #    | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|-------------|----------|----------|--------|-----------------------------|--|
| 1             | 1,4-Dioxane | 123-91-1 | SHBN3770 | 99%    | 2,013.0 µg/mL               | +/- 25.0521                            |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant flow 1.8 mL/min.

**Temp. Program:**

80°C (hold 0.1 min.) to 330°C  
@ 9.6°C/min. (hold 2.86 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

340°C

**Det. Type:**

FID

**Split Vent:**

100 ml/min.

**Inj. Vol**

1µl



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Sam Moodler*  
Sam Moodler - Operations Tech I

Date Mixed: 30-Mar-2023

Balance Serial # B707717271

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 31-Mar-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31853 **Lot No.:** A0196453  
**Description :** 1,4-dioxane  
1,4-Dioxane 2,000µg/mL, Methylene Chloride, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** March 31, 2028 **Storage:** 0°C or colder  
**Ship:** Ambient

S11749  
↓  
S11794 } RC / 11/30/23

### CERTIFIED VALUES

| Elution Order | Compound    | CAS #    | Lot #    | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|-------------|----------|----------|--------|-----------------------------|--|
| 1             | 1,4-Dioxane | 123-91-1 | SHBN3770 | 99%    | 2,013.0 µg/mL               | +/- 25.0521                            |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant flow 1.8 mL/min.

**Temp. Program:**

80°C (hold 0.1 min.) to 330°C  
@ 9.6°C/min. (hold 2.86 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

340°C

**Det. Type:**

FID

**Split Vent:**

100 mL/min.

**Inj. Vol**

1µl



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Sam Moodler*  
Sam Moodler - Operations Tech I

Date Mixed: 30-Mar-2023

Balance Serial # B707717271

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 31-Mar-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31853 **Lot No.:** A0196453  
**Description :** 1,4-dioxane  
1,4-Dioxane 2,000µg/mL, Methylene Chloride, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** March 31, 2028 **Storage:** 0°C or colder  
**Ship:** Ambient

S11749  
↓  
S11794 } RC / 11/30/23

### CERTIFIED VALUES

| Elution Order | Compound    | CAS #    | Lot #    | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|-------------|----------|----------|--------|-----------------------------|--|
| 1             | 1,4-Dioxane | 123-91-1 | SHBN3770 | 99%    | 2,013.0 µg/mL               | +/- 25.0521                            |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant flow 1.8 mL/min.

**Temp. Program:**

80°C (hold 0.1 min.) to 330°C  
@ 9.6°C/min. (hold 2.86 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

340°C

**Det. Type:**

FID

**Split Vent:**

100 ml/min.

**Inj. Vol**

1µl



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Sam Moodler*  
Sam Moodler - Operations Tech I

Date Mixed: 30-Mar-2023 Balance Serial # B707717271

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 31-Mar-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

**Catalog No. :** 31853 **Lot No.:** A0196453  
**Description :** 1,4-dioxane  
1,4-Dioxane 2,000µg/mL, Methylene Chloride, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** March 31, 2028 **Storage:** 0°C or colder  
**Ship:** Ambient

S11749  
↓  
S11794 } RC / 11/30/23

### CERTIFIED VALUES

| Elution Order | Compound    | CAS #    | Lot #    | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|-------------|----------|----------|--------|-----------------------------|--|
| 1             | 1,4-Dioxane | 123-91-1 | SHBN3770 | 99%    | 2,013.0 µg/mL               | +/- 25.0521                            |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant flow 1.8 mL/min.

**Temp. Program:**

80°C (hold 0.1 min.) to 330°C  
@ 9.6°C/min. (hold 2.86 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

340°C

**Det. Type:**

FID

**Split Vent:**

100 ml/min.

**Inj. Vol**

1µl



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Sam Moodler*  
Sam Moodler - Operations Tech I

Date Mixed: 30-Mar-2023      Balance Serial # B707717271

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 31-Mar-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



## FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

**Catalog No. :** 31850 **Lot No.:** A0197982

**Description :** 8270 MegaMix®  
8270 MegaMix® 500-1,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** November 30, 2024 **Storage:** 0°C or colder

**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

511877  
↓  
511906

RC/  
11/30/23

## CERTIFIED VALUES

| Elution Order | Compound                     | CAS #    | Lot #     | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------------|----------|-----------|--------|-----------------------------|--|
| 1             | Pyridine                     | 110-86-1 | SHBN7324  | 99%    | 1,006.9 µg/mL               | +/- 36.6352                            |
| 2             | N-Nitrosodimethylamine       | 62-75-9  | 230209JLM | 99%    | 1,007.4 µg/mL               | +/- 36.6514                            |
| 3             | Phenol                       | 108-95-2 | MKCK1120  | 99%    | 1,005.3 µg/mL               | +/- 36.5746                            |
| 4             | Aniline                      | 62-53-3  | X22F726   | 99%    | 1,004.6 µg/mL               | +/- 36.5503                            |
| 5             | Bis(2-chloroethyl)ether      | 111-44-4 | SHBL6942  | 99%    | 1,005.1 µg/mL               | +/- 36.5665                            |
| 6             | 2-Chlorophenol               | 95-57-8  | STBJ3909  | 99%    | 1,007.1 µg/mL               | +/- 36.6392                            |
| 7             | 1,3-Dichlorobenzene          | 541-73-1 | BCBZ7498  | 99%    | 1,006.7 µg/mL               | +/- 36.6251                            |
| 8             | 1,4-Dichlorobenzene          | 106-46-7 | MKBS7929V | 99%    | 1,005.6 µg/mL               | +/- 36.5867                            |
| 9             | Benzyl alcohol               | 100-51-6 | SHBK5943  | 99%    | 1,005.4 µg/mL               | +/- 36.5786                            |
| 10            | 1,2-Dichlorobenzene          | 95-50-1  | SHBN3835  | 99%    | 1,003.9 µg/mL               | +/- 36.5240                            |
| 11            | 2-Methylphenol (o-cresol)    | 95-48-7  | SHBN7598  | 99%    | 1,002.3 µg/mL               | +/- 36.4654                            |
| 12            | 2,2'-oxybis(1-chloropropane) | 108-60-1 | 230329JLM | 99%    | 1,004.3 µg/mL               | +/- 36.5402                            |
| 13            | 3-Methylphenol (m-cresol)    | 108-39-4 | STBJ0710  | 99%    | 502.1 µg/mL                 | +/- 18.2671                            |
| 14            | 4-Methylphenol (p-cresol)    | 106-44-5 | SHBN3411  | 99%    | 501.9 µg/mL                 | +/- 18.2631                            |
| 15            | N-Nitroso-di-n-propylamine   | 621-64-7 | N63MG     | 99%    | 1,004.0 µg/mL               | +/- 36.5281                            |
| 16            | Hexachloroethane             | 67-72-1  | QTORH     | 99%    | 1,006.1 µg/mL               | +/- 36.6029                            |
| 17            | Nitrobenzene                 | 98-95-3  | 10224044  | 99%    | 1,003.1 µg/mL               | +/- 36.4957                            |

|    |   |           |             |     |         |       |     |         |
|----|---|-----------|-------------|-----|---------|-------|-----|---------|
| 18 | Isophorone                                    | 78-59-1   | MKCC9506    | 99% | 1,003.8 | µg/mL | +/- | 36.5220 |
| 19 | 2-Nitrophenol                                 | 88-75-5   | RP230509C   | 99% | 1,005.8 | µg/mL | +/- | 36.5948 |
| 20 | 2,4-Dimethylphenol                            | 105-67-9  | XW5GK       | 99% | 1,004.2 | µg/mL | +/- | 36.5341 |
| 21 | Bis(2-chloroethoxy)methane                    | 111-91-1  | 13670200    | 99% | 1,006.3 | µg/mL | +/- | 36.6130 |
| 22 | 2,4-Dichlorophenol                            | 120-83-2  | BCBZ6787    | 99% | 1,004.0 | µg/mL | +/- | 36.5281 |
| 23 | 1,2,4-Trichlorobenzene                        | 120-82-1  | SHBM0526    | 99% | 1,007.1 | µg/mL | +/- | 36.6413 |
| 24 | Naphthalene                                   | 91-20-3   | MKCH0219    | 99% | 1,006.7 | µg/mL | +/- | 36.6271 |
| 25 | 4-Chloroaniline                               | 106-47-8  | WXBC4601V   | 99% | 1,005.4 | µg/mL | +/- | 36.5806 |
| 26 | Hexachlorobutadiene                           | 87-68-3   | X05J        | 99% | 1,006.4 | µg/mL | +/- | 36.6170 |
| 27 | 4-Chloro-3-methylphenol                       | 59-50-7   | BCCD4461    | 99% | 1,004.7 | µg/mL | +/- | 36.5543 |
| 28 | 2-Methylnaphthalene                           | 91-57-6   | STBK0259    | 96% | 1,002.3 | µg/mL | +/- | 36.4679 |
| 29 | 1-Methylnaphthalene                           | 90-12-0   | 5234.00-3   | 99% | 1,000.0 | µg/mL | +/- | 36.3825 |
| 30 | Hexachlorocyclopentadiene                     | 77-47-4   | 0012019     | 99% | 1,006.1 | µg/mL | +/- | 36.6049 |
| 31 | 2,4,6-Trichlorophenol                         | 88-06-2   | STBJ5914    | 99% | 1,004.9 | µg/mL | +/- | 36.5604 |
| 32 | 2,4,5-Trichlorophenol                         | 95-95-4   | FHN01       | 98% | 1,006.5 | µg/mL | +/- | 36.6176 |
| 33 | 2-Chloronaphthalene                           | 91-58-7   | RPN70       | 99% | 1,004.4 | µg/mL | +/- | 36.5422 |
| 34 | 2-Nitroaniline                                | 88-74-4   | RP230509A   | 99% | 1,002.3 | µg/mL | +/- | 36.4654 |
| 35 | 1,4-Dinitrobenzene                            | 100-25-4  | RP230512A   | 99% | 1,001.5 | µg/mL | +/- | 36.4371 |
| 36 | Acenaphthylene                                | 208-96-8  | L10L        | 95% | 1,003.4 | µg/mL | +/- | 36.5066 |
| 37 | 1,3-Dinitrobenzene                            | 99-65-0   | 1-DXX-24-1  | 99% | 1,004.8 | µg/mL | +/- | 36.5564 |
| 38 | Dimethylphthalate                             | 131-11-3  | 10117699    | 99% | 1,004.7 | µg/mL | +/- | 36.5543 |
| 39 | 2,6-Dinitrotoluene                            | 606-20-2  | BCCG1833    | 99% | 1,006.8 | µg/mL | +/- | 36.6312 |
| 40 | 1,2-Dinitrobenzene                            | 528-29-0  | RP230428    | 99% | 1,006.4 | µg/mL | +/- | 36.6170 |
| 41 | Acenaphthene                                  | 83-32-9   | MKCR7169    | 99% | 1,000.0 | µg/mL | +/- | 36.3825 |
| 42 | 3-Nitroaniline                                | 99-09-2   | MKCH5457    | 99% | 1,004.8 | µg/mL | +/- | 36.5584 |
| 43 | 2,4-Dinitrophenol                             | 51-28-5   | DR230417RSR | 99% | 1,005.8 | µg/mL | +/- | 36.5948 |
| 44 | Dibenzofuran                                  | 132-64-9  | MKCN1772    | 99% | 1,004.3 | µg/mL | +/- | 36.5402 |
| 45 | 2,4-Dinitrotoluene                            | 121-14-2  | MKAA0690V   | 99% | 1,005.8 | µg/mL | +/- | 36.5928 |
| 46 | 4-Nitrophenol                                 | 100-02-7  | RP230511A   | 99% | 1,005.8 | µg/mL | +/- | 36.5948 |
| 47 | 2,3,4,6-Tetrachlorophenol                     | 58-90-2   | PR-30126    | 99% | 1,005.9 | µg/mL | +/- | 36.5988 |
| 48 | 2,3,5,6-Tetrachlorophenol                     | 935-95-5  | RP230513    | 99% | 1,004.9 | µg/mL | +/- | 36.5624 |
| 49 | Fluorene                                      | 86-73-7   | 10236068    | 99% | 1,005.4 | µg/mL | +/- | 36.5806 |
| 50 | 4-Chlorophenyl phenyl ether                   | 7005-72-3 | MKCQ0984    | 99% | 1,004.3 | µg/mL | +/- | 36.5382 |
| 51 | Diethylphthalate                              | 84-66-2   | BCCD3396    | 99% | 1,007.1 | µg/mL | +/- | 36.6392 |
| 52 | 4-Nitroaniline                                | 100-01-6  | RP220906    | 99% | 1,005.3 | µg/mL | +/- | 36.5766 |
| 53 | 4,6-Dinitro-2-methylphenol (Dinitro-o-cresol) | 534-52-1  | 230505JLM   | 99% | 1,003.8 | µg/mL | +/- | 36.5200 |

|    |                            |          |              |     |         |       |             |
|----|----------------------------|----------|--------------|-----|---------|-------|-------------|
| 54 | Diphenylamine              | 122-39-4 | MKCH1042     | 99% | 1,002.5 | µg/mL | +/- 36.4735 |
| 55 | Azobenzene                 | 103-33-3 | BCCG7339     | 98% | 1,003.5 | µg/mL | +/- 36.5106 |
| 56 | 4-Bromophenyl phenyl ether | 101-55-3 | STBH6361     | 99% | 1,005.6 | µg/mL | +/- 36.5847 |
| 57 | Hexachlorobenzene          | 118-74-1 | 14257500     | 99% | 1,005.9 | µg/mL | +/- 36.5988 |
| 58 | Pentachlorophenol          | 87-86-5  | RP230504     | 99% | 1,004.2 | µg/mL | +/- 36.5362 |
| 59 | Phenanthrene               | 85-01-8  | MKCQ8876     | 99% | 1,004.1 | µg/mL | +/- 36.5321 |
| 60 | Anthracene                 | 120-12-7 | MKCR0570     | 99% | 1,008.3 | µg/mL | +/- 36.6857 |
| 61 | Carbazole                  | 86-74-8  | 14351100     | 99% | 1,005.1 | µg/mL | +/- 36.5665 |
| 62 | Di-n-butylphthalate        | 84-74-2  | MKCN4337     | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 63 | Fluoranthene               | 206-44-0 | MKCQ4728     | 99% | 1,003.7 | µg/mL | +/- 36.5159 |
| 64 | Pyrene                     | 129-00-0 | BCCG7845     | 99% | 1,004.3 | µg/mL | +/- 36.5382 |
| 65 | Benzyl butyl phthalate     | 85-68-7  | X12I018      | 99% | 1,003.4 | µg/mL | +/- 36.5058 |
| 66 | Bis(2-ethylhexyl)adipate   | 103-23-1 | MKCM1988     | 99% | 1,003.4 | µg/mL | +/- 36.5079 |
| 67 | Benz(a)anthracene          | 56-55-3  | 0012022BAA   | 97% | 1,004.9 | µg/mL | +/- 36.5624 |
| 68 | Chrysene                   | 218-01-9 | RP230512B    | 99% | 1,006.2 | µg/mL | +/- 36.6089 |
| 69 | Bis(2-ethylhexyl)phthalate | 117-81-7 | MKCQ3468     | 99% | 1,003.8 | µg/mL | +/- 36.5220 |
| 70 | Di-n-octyl phthalate       | 117-84-0 | 13994100     | 99% | 1,004.2 | µg/mL | +/- 36.5341 |
| 71 | Benzo(b)fluoranthene       | 205-99-2 | 012013B      | 99% | 1,008.4 | µg/mL | +/- 36.6877 |
| 72 | Benzo(k)fluoranthene       | 207-08-9 | 012022K      | 99% | 1,004.1 | µg/mL | +/- 36.5301 |
| 73 | Benzo(a)pyrene             | 50-32-8  | J6IUE        | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 74 | Indeno(1,2,3-cd)pyrene     | 193-39-5 | 12-JKL-118-9 | 97% | 1,002.0 | µg/mL | +/- 36.4557 |
| 75 | Dibenz(a,h)anthracene      | 53-70-3  | ER032211-01  | 99% | 1,006.1 | µg/mL | +/- 36.6029 |
| 76 | Benzo(g,h,i)perylene       | 191-24-2 | RP230511B    | 98% | 1,006.8 | µg/mL | +/- 36.6295 |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant flow 1.8 mL/min.

**Temp. Program:**

80°C (hold 0.1 min.) to 330°C  
@ 9.6°C/min. (hold 2.86 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

340°C

**Det. Type:**


FID

**Split Vent:**

100 ml/min.

**Inj. Vol**

1µl

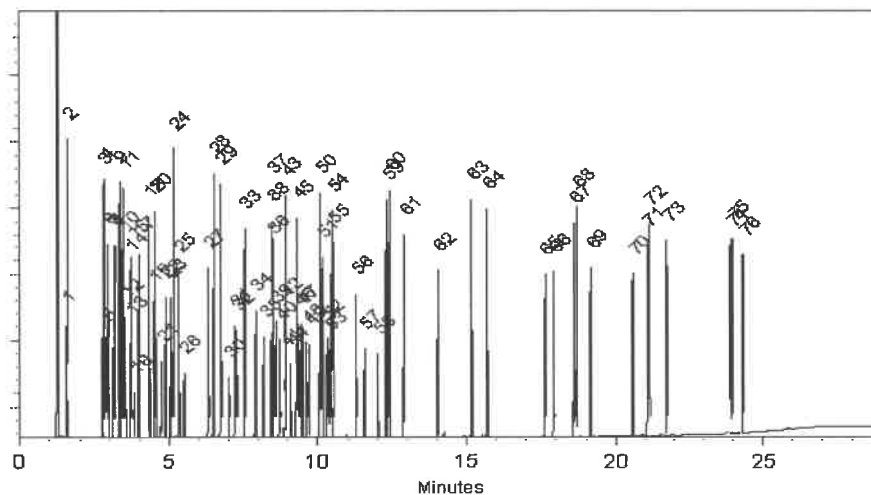

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Tom Suckar - Mix Technician

Date Mixed: 11-May-2023

Balance Serial # 1128353505

  
Christie Mills - Operations Tech II - ARM QC

Date Passed: 18-May-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

## Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 31850 Lot No.: A0197982  
Description: 8270 MegaMix®  
8270 MegaMix® 500-1,000µg/mL, Methylene Chloride, 1mL/ampul  
Container Size: 2 mL Pkg Amt: > 1 mL  
Expiration Date: November 30, 2024 Storage: 0°C or colder  
Handling: Sonication required. Mix is photosensitive. Ship: Ambient

511877  
↓  
511906  
RC/  
11/30/23

### CERTIFIED VALUES

| Elution Order | Compound                     | CAS #    | Lot #     | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------------|----------|-----------|--------|-----------------------------|--|
| 1             | Pyridine                     | 110-86-1 | SHBN7324  | 99%    | 1,006.9 µg/mL               | +/- 36.6352                            |
| 2             | N-Nitrosodimethylamine       | 62-75-9  | 230209JLM | 99%    | 1,007.4 µg/mL               | +/- 36.6514                            |
| 3             | Phenol                       | 108-95-2 | MKCK1120  | 99%    | 1,005.3 µg/mL               | +/- 36.5746                            |
| 4             | Aniline                      | 62-53-3  | X22F726   | 99%    | 1,004.6 µg/mL               | +/- 36.5503                            |
| 5             | Bis(2-chloroethyl)ether      | 111-44-4 | SHBL6942  | 99%    | 1,005.1 µg/mL               | +/- 36.5665                            |
| 6             | 2-Chlorophenol               | 95-57-8  | STBJ3909  | 99%    | 1,007.1 µg/mL               | +/- 36.6392                            |
| 7             | 1,3-Dichlorobenzene          | 541-73-1 | BCBZ7498  | 99%    | 1,006.7 µg/mL               | +/- 36.6251                            |
| 8             | 1,4-Dichlorobenzene          | 106-46-7 | MKBS7929V | 99%    | 1,005.6 µg/mL               | +/- 36.5867                            |
| 9             | Benzyl alcohol               | 100-51-6 | SHBK5943  | 99%    | 1,005.4 µg/mL               | +/- 36.5786                            |
| 10            | 1,2-Dichlorobenzene          | 95-50-1  | SHBN3835  | 99%    | 1,003.9 µg/mL               | +/- 36.5240                            |
| 11            | 2-Methylphenol (o-cresol)    | 95-48-7  | SHBN7598  | 99%    | 1,002.3 µg/mL               | +/- 36.4654                            |
| 12            | 2,2'-oxybis(1-chloropropane) | 108-60-1 | 230329JLM | 99%    | 1,004.3 µg/mL               | +/- 36.5402                            |
| 13            | 3-Methylphenol (m-cresol)    | 108-39-4 | STBJ0710  | 99%    | 502.1 µg/mL                 | +/- 18.2671                            |
| 14            | 4-Methylphenol (p-cresol)    | 106-44-5 | SHBN3411  | 99%    | 501.9 µg/mL                 | +/- 18.2631                            |
| 15            | N-Nitroso-di-n-propylamine   | 621-64-7 | N63MG     | 99%    | 1,004.0 µg/mL               | +/- 36.5281                            |
| 16            | Hexachloroethane             | 67-72-1  | QTORH     | 99%    | 1,006.1 µg/mL               | +/- 36.6029                            |
| 17            | Nitrobenzene                 | 98-95-3  | 10224044  | 99%    | 1,003.1 µg/mL               | +/- 36.4957                            |

|    |   |           |             |     |         |       |             |
|----|---|-----------|-------------|-----|---------|-------|-------------|
| 18 | Isophorone                                    | 78-59-1   | MKCC9506    | 99% | 1,003.8 | µg/mL | +/- 36.5220 |
| 19 | 2-Nitrophenol                                 | 88-75-5   | RP230509C   | 99% | 1,005.8 | µg/mL | +/- 36.5948 |
| 20 | 2,4-Dimethylphenol                            | 105-67-9  | XW5GK       | 99% | 1,004.2 | µg/mL | +/- 36.5341 |
| 21 | Bis(2-chloroethoxy)methane                    | 111-91-1  | 13670200    | 99% | 1,006.3 | µg/mL | +/- 36.6130 |
| 22 | 2,4-Dichlorophenol                            | 120-83-2  | BCBZ6787    | 99% | 1,004.0 | µg/mL | +/- 36.5281 |
| 23 | 1,2,4-Trichlorobenzene                        | 120-82-1  | SHBM0526    | 99% | 1,007.1 | µg/mL | +/- 36.6413 |
| 24 | Naphthalene                                   | 91-20-3   | MKCH0219    | 99% | 1,006.7 | µg/mL | +/- 36.6271 |
| 25 | 4-Chloroaniline                               | 106-47-8  | WXBC4601V   | 99% | 1,005.4 | µg/mL | +/- 36.5806 |
| 26 | Hexachlorobutadiene                           | 87-68-3   | X05J        | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 27 | 4-Chloro-3-methylphenol                       | 59-50-7   | BCCD4461    | 99% | 1,004.7 | µg/mL | +/- 36.5543 |
| 28 | 2-Methylnaphthalene                           | 91-57-6   | STBK0259    | 96% | 1,002.3 | µg/mL | +/- 36.4679 |
| 29 | 1-Methylnaphthalene                           | 90-12-0   | 5234.00-3   | 99% | 1,000.0 | µg/mL | +/- 36.3825 |
| 30 | Hexachlorocyclopentadiene                     | 77-47-4   | 0012019     | 99% | 1,006.1 | µg/mL | +/- 36.6049 |
| 31 | 2,4,6-Trichlorophenol                         | 88-06-2   | STBJ5914    | 99% | 1,004.9 | µg/mL | +/- 36.5604 |
| 32 | 2,4,5-Trichlorophenol                         | 95-95-4   | FHN01       | 98% | 1,006.5 | µg/mL | +/- 36.6176 |
| 33 | 2-Chloronaphthalene                           | 91-58-7   | RPN70       | 99% | 1,004.4 | µg/mL | +/- 36.5422 |
| 34 | 2-Nitroaniline                                | 88-74-4   | RP230509A   | 99% | 1,002.3 | µg/mL | +/- 36.4654 |
| 35 | 1,4-Dinitrobenzene                            | 100-25-4  | RP230512A   | 99% | 1,001.5 | µg/mL | +/- 36.4371 |
| 36 | Acenaphthylene                                | 208-96-8  | L10L        | 95% | 1,003.4 | µg/mL | +/- 36.5066 |
| 37 | 1,3-Dinitrobenzene                            | 99-65-0   | 1-DXX-24-1  | 99% | 1,004.8 | µg/mL | +/- 36.5564 |
| 38 | Dimethylphthalate                             | 131-11-3  | 10117699    | 99% | 1,004.7 | µg/mL | +/- 36.5543 |
| 39 | 2,6-Dinitrotoluene                            | 606-20-2  | BCCG1833    | 99% | 1,006.8 | µg/mL | +/- 36.6312 |
| 40 | 1,2-Dinitrobenzene                            | 528-29-0  | RP230428    | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 41 | Acenaphthene                                  | 83-32-9   | MKCR7169    | 99% | 1,000.0 | µg/mL | +/- 36.3825 |
| 42 | 3-Nitroaniline                                | 99-09-2   | MKCH5457    | 99% | 1,004.8 | µg/mL | +/- 36.5584 |
| 43 | 2,4-Dinitrophenol                             | 51-28-5   | DR230417RSR | 99% | 1,005.8 | µg/mL | +/- 36.5948 |
| 44 | Dibenzofuran                                  | 132-64-9  | MKCN1772    | 99% | 1,004.3 | µg/mL | +/- 36.5402 |
| 45 | 2,4-Dinitrotoluene                            | 121-14-2  | MKAA0690V   | 99% | 1,005.8 | µg/mL | +/- 36.5928 |
| 46 | 4-Nitrophenol                                 | 100-02-7  | RP230511A   | 99% | 1,005.8 | µg/mL | +/- 36.5948 |
| 47 | 2,3,4,6-Tetrachlorophenol                     | 58-90-2   | PR-30126    | 99% | 1,005.9 | µg/mL | +/- 36.5988 |
| 48 | 2,3,5,6-Tetrachlorophenol                     | 935-95-5  | RP230513    | 99% | 1,004.9 | µg/mL | +/- 36.5624 |
| 49 | Fluorene                                      | 86-73-7   | 10236068    | 99% | 1,005.4 | µg/mL | +/- 36.5806 |
| 50 | 4-Chlorophenyl phenyl ether                   | 7005-72-3 | MKCQ0984    | 99% | 1,004.3 | µg/mL | +/- 36.5382 |
| 51 | Diethylphthalate                              | 84-66-2   | BCCD3396    | 99% | 1,007.1 | µg/mL | +/- 36.6392 |
| 52 | 4-Nitroaniline                                | 100-01-6  | RP220906    | 99% | 1,005.3 | µg/mL | +/- 36.5766 |
| 53 | 4,6-Dinitro-2-methylphenol (Dinitro-o-cresol) | 534-52-1  | 230505JLM   | 99% | 1,003.8 | µg/mL | +/- 36.5200 |



|    |                            |          |              |     |         |       |             |
|----|----------------------------|----------|--------------|-----|---------|-------|-------------|
| 54 | Diphenylamine              | 122-39-4 | MKCH1042     | 99% | 1,002.5 | µg/mL | +/- 36.4735 |
| 55 | Azobenzene                 | 103-33-3 | BCCG7339     | 98% | 1,003.5 | µg/mL | +/- 36.5106 |
| 56 | 4-Bromophenyl phenyl ether | 101-55-3 | STBH6361     | 99% | 1,005.6 | µg/mL | +/- 36.5847 |
| 57 | Hexachlorobenzene          | 118-74-1 | 14257500     | 99% | 1,005.9 | µg/mL | +/- 36.5988 |
| 58 | Pentachlorophenol          | 87-86-5  | RP230504     | 99% | 1,004.2 | µg/mL | +/- 36.5362 |
| 59 | Phenanthrene               | 85-01-8  | MKCQ8876     | 99% | 1,004.1 | µg/mL | +/- 36.5321 |
| 60 | Anthracene                 | 120-12-7 | MKCR0570     | 99% | 1,008.3 | µg/mL | +/- 36.6857 |
| 61 | Carbazole                  | 86-74-8  | 14351100     | 99% | 1,005.1 | µg/mL | +/- 36.5665 |
| 62 | Di-n-butylphthalate        | 84-74-2  | MKCN4337     | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 63 | Fluoranthene               | 206-44-0 | MKCQ4728     | 99% | 1,003.7 | µg/mL | +/- 36.5159 |
| 64 | Pyrene                     | 129-00-0 | BCCG7845     | 99% | 1,004.3 | µg/mL | +/- 36.5382 |
| 65 | Benzyl butyl phthalate     | 85-68-7  | X12I018      | 99% | 1,003.4 | µg/mL | +/- 36.5058 |
| 66 | Bis(2-ethylhexyl)adipate   | 103-23-1 | MKCM1988     | 99% | 1,003.4 | µg/mL | +/- 36.5079 |
| 67 | Benz(a)anthracene          | 56-55-3  | 0012022BAA   | 97% | 1,004.9 | µg/mL | +/- 36.5624 |
| 68 | Chrysene                   | 218-01-9 | RP230512B    | 99% | 1,006.2 | µg/mL | +/- 36.6089 |
| 69 | Bis(2-ethylhexyl)phthalate | 117-81-7 | MKCQ3468     | 99% | 1,003.8 | µg/mL | +/- 36.5220 |
| 70 | Di-n-octyl phthalate       | 117-84-0 | 13994100     | 99% | 1,004.2 | µg/mL | +/- 36.5341 |
| 71 | Benzo(b)fluoranthene       | 205-99-2 | 012013B      | 99% | 1,008.4 | µg/mL | +/- 36.6877 |
| 72 | Benzo(k)fluoranthene       | 207-08-9 | 012022K      | 99% | 1,004.1 | µg/mL | +/- 36.5301 |
| 73 | Benzo(a)pyrene             | 50-32-8  | J6IUE        | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 74 | Indeno(1,2,3-cd)pyrene     | 193-39-5 | 12-JKL-118-9 | 97% | 1,002.0 | µg/mL | +/- 36.4557 |
| 75 | Dibenz(a,h)anthracene      | 53-70-3  | ER032211-01  | 99% | 1,006.1 | µg/mL | +/- 36.6029 |
| 76 | Benzo(g,h,i)perylene       | 191-24-2 | RP230511B    | 98% | 1,006.8 | µg/mL | +/- 36.6295 |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant flow 1.8 mL/min.

**Temp. Program:**

80°C (hold 0.1 min.) to 330°C  
@ 9.6°C/min. (hold 2.86 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

340°C

**Det. Type:**


FID

**Split Vent:**

100 ml/min.

**Inj. Vol**

1µl

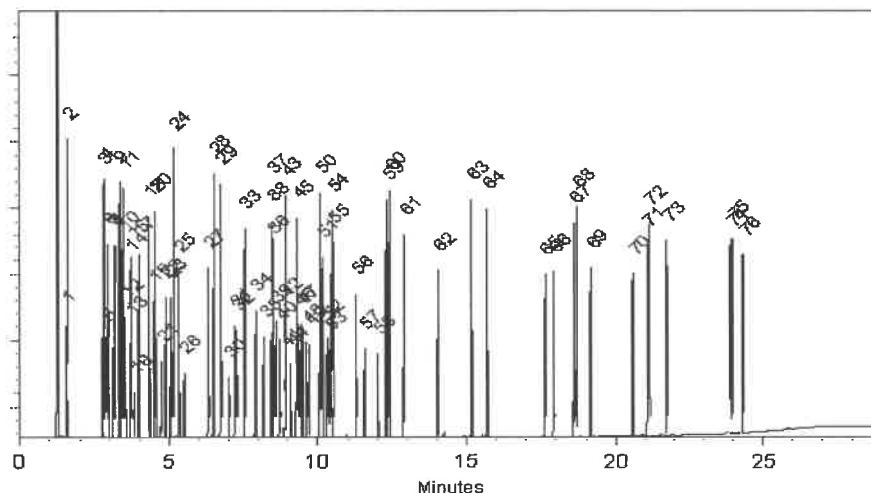

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Tom Suckar - Mix Technician

Date Mixed: 11-May-2023

Balance Serial # 1128353505

  
Christie Mills - Operations Tech II - ARM QC

Date Passed: 18-May-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

## Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31850 **Lot No.:** A0197982  
**Description :** 8270 MegaMix®  
8270 MegaMix® 500-1,000µg/mL, Methylene Chloride, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** November 30, 2024 **Storage:** 0°C or colder  
**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

511877  
↓  
511906  
RC/  
11/30/23

### CERTIFIED VALUES

| Elution Order | Compound                     | CAS #    | Lot #     | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------------|----------|-----------|--------|-----------------------------|--|
| 1             | Pyridine                     | 110-86-1 | SHBN7324  | 99%    | 1,006.9 µg/mL               | +/- 36.6352                            |
| 2             | N-Nitrosodimethylamine       | 62-75-9  | 230209JLM | 99%    | 1,007.4 µg/mL               | +/- 36.6514                            |
| 3             | Phenol                       | 108-95-2 | MKCK1120  | 99%    | 1,005.3 µg/mL               | +/- 36.5746                            |
| 4             | Aniline                      | 62-53-3  | X22F726   | 99%    | 1,004.6 µg/mL               | +/- 36.5503                            |
| 5             | Bis(2-chloroethyl)ether      | 111-44-4 | SHBL6942  | 99%    | 1,005.1 µg/mL               | +/- 36.5665                            |
| 6             | 2-Chlorophenol               | 95-57-8  | STBJ3909  | 99%    | 1,007.1 µg/mL               | +/- 36.6392                            |
| 7             | 1,3-Dichlorobenzene          | 541-73-1 | BCBZ7498  | 99%    | 1,006.7 µg/mL               | +/- 36.6251                            |
| 8             | 1,4-Dichlorobenzene          | 106-46-7 | MKBS7929V | 99%    | 1,005.6 µg/mL               | +/- 36.5867                            |
| 9             | Benzyl alcohol               | 100-51-6 | SHBK5943  | 99%    | 1,005.4 µg/mL               | +/- 36.5786                            |
| 10            | 1,2-Dichlorobenzene          | 95-50-1  | SHBN3835  | 99%    | 1,003.9 µg/mL               | +/- 36.5240                            |
| 11            | 2-Methylphenol (o-cresol)    | 95-48-7  | SHBN7598  | 99%    | 1,002.3 µg/mL               | +/- 36.4654                            |
| 12            | 2,2'-oxybis(1-chloropropane) | 108-60-1 | 230329JLM | 99%    | 1,004.3 µg/mL               | +/- 36.5402                            |
| 13            | 3-Methylphenol (m-cresol)    | 108-39-4 | STBJ0710  | 99%    | 502.1 µg/mL                 | +/- 18.2671                            |
| 14            | 4-Methylphenol (p-cresol)    | 106-44-5 | SHBN3411  | 99%    | 501.9 µg/mL                 | +/- 18.2631                            |
| 15            | N-Nitroso-di-n-propylamine   | 621-64-7 | N63MG     | 99%    | 1,004.0 µg/mL               | +/- 36.5281                            |
| 16            | Hexachloroethane             | 67-72-1  | QTORH     | 99%    | 1,006.1 µg/mL               | +/- 36.6029                            |
| 17            | Nitrobenzene                 | 98-95-3  | 10224044  | 99%    | 1,003.1 µg/mL               | +/- 36.4957                            |

|    |   |           |             |     |         |       |             |
|----|---|-----------|-------------|-----|---------|-------|-------------|
| 18 | Isophorone                                    | 78-59-1   | MKCC9506    | 99% | 1,003.8 | µg/mL | +/- 36.5220 |
| 19 | 2-Nitrophenol                                 | 88-75-5   | RP230509C   | 99% | 1,005.8 | µg/mL | +/- 36.5948 |
| 20 | 2,4-Dimethylphenol                            | 105-67-9  | XW5GK       | 99% | 1,004.2 | µg/mL | +/- 36.5341 |
| 21 | Bis(2-chloroethoxy)methane                    | 111-91-1  | 13670200    | 99% | 1,006.3 | µg/mL | +/- 36.6130 |
| 22 | 2,4-Dichlorophenol                            | 120-83-2  | BCBZ6787    | 99% | 1,004.0 | µg/mL | +/- 36.5281 |
| 23 | 1,2,4-Trichlorobenzene                        | 120-82-1  | SHBM0526    | 99% | 1,007.1 | µg/mL | +/- 36.6413 |
| 24 | Naphthalene                                   | 91-20-3   | MKCH0219    | 99% | 1,006.7 | µg/mL | +/- 36.6271 |
| 25 | 4-Chloroaniline                               | 106-47-8  | WXBC4601V   | 99% | 1,005.4 | µg/mL | +/- 36.5806 |
| 26 | Hexachlorobutadiene                           | 87-68-3   | X05J        | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 27 | 4-Chloro-3-methylphenol                       | 59-50-7   | BCCD4461    | 99% | 1,004.7 | µg/mL | +/- 36.5543 |
| 28 | 2-Methylnaphthalene                           | 91-57-6   | STBK0259    | 96% | 1,002.3 | µg/mL | +/- 36.4679 |
| 29 | 1-Methylnaphthalene                           | 90-12-0   | 5234.00-3   | 99% | 1,000.0 | µg/mL | +/- 36.3825 |
| 30 | Hexachlorocyclopentadiene                     | 77-47-4   | 0012019     | 99% | 1,006.1 | µg/mL | +/- 36.6049 |
| 31 | 2,4,6-Trichlorophenol                         | 88-06-2   | STBJ5914    | 99% | 1,004.9 | µg/mL | +/- 36.5604 |
| 32 | 2,4,5-Trichlorophenol                         | 95-95-4   | FHN01       | 98% | 1,006.5 | µg/mL | +/- 36.6176 |
| 33 | 2-Chloronaphthalene                           | 91-58-7   | RPN70       | 99% | 1,004.4 | µg/mL | +/- 36.5422 |
| 34 | 2-Nitroaniline                                | 88-74-4   | RP230509A   | 99% | 1,002.3 | µg/mL | +/- 36.4654 |
| 35 | 1,4-Dinitrobenzene                            | 100-25-4  | RP230512A   | 99% | 1,001.5 | µg/mL | +/- 36.4371 |
| 36 | Acenaphthylene                                | 208-96-8  | L10L        | 95% | 1,003.4 | µg/mL | +/- 36.5066 |
| 37 | 1,3-Dinitrobenzene                            | 99-65-0   | 1-DXX-24-1  | 99% | 1,004.8 | µg/mL | +/- 36.5564 |
| 38 | Dimethylphthalate                             | 131-11-3  | 10117699    | 99% | 1,004.7 | µg/mL | +/- 36.5543 |
| 39 | 2,6-Dinitrotoluene                            | 606-20-2  | BCCG1833    | 99% | 1,006.8 | µg/mL | +/- 36.6312 |
| 40 | 1,2-Dinitrobenzene                            | 528-29-0  | RP230428    | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 41 | Acenaphthene                                  | 83-32-9   | MKCR7169    | 99% | 1,000.0 | µg/mL | +/- 36.3825 |
| 42 | 3-Nitroaniline                                | 99-09-2   | MKCH5457    | 99% | 1,004.8 | µg/mL | +/- 36.5584 |
| 43 | 2,4-Dinitrophenol                             | 51-28-5   | DR230417RSR | 99% | 1,005.8 | µg/mL | +/- 36.5948 |
| 44 | Dibenzofuran                                  | 132-64-9  | MKCN1772    | 99% | 1,004.3 | µg/mL | +/- 36.5402 |
| 45 | 2,4-Dinitrotoluene                            | 121-14-2  | MKAA0690V   | 99% | 1,005.8 | µg/mL | +/- 36.5928 |
| 46 | 4-Nitrophenol                                 | 100-02-7  | RP230511A   | 99% | 1,005.8 | µg/mL | +/- 36.5948 |
| 47 | 2,3,4,6-Tetrachlorophenol                     | 58-90-2   | PR-30126    | 99% | 1,005.9 | µg/mL | +/- 36.5988 |
| 48 | 2,3,5,6-Tetrachlorophenol                     | 935-95-5  | RP230513    | 99% | 1,004.9 | µg/mL | +/- 36.5624 |
| 49 | Fluorene                                      | 86-73-7   | 10236068    | 99% | 1,005.4 | µg/mL | +/- 36.5806 |
| 50 | 4-Chlorophenyl phenyl ether                   | 7005-72-3 | MKCQ0984    | 99% | 1,004.3 | µg/mL | +/- 36.5382 |
| 51 | Diethylphthalate                              | 84-66-2   | BCCD3396    | 99% | 1,007.1 | µg/mL | +/- 36.6392 |
| 52 | 4-Nitroaniline                                | 100-01-6  | RP220906    | 99% | 1,005.3 | µg/mL | +/- 36.5766 |
| 53 | 4,6-Dinitro-2-methylphenol (Dinitro-o-cresol) | 534-52-1  | 230505JLM   | 99% | 1,003.8 | µg/mL | +/- 36.5200 |

|    |                            |          |              |     |         |       |             |
|----|----------------------------|----------|--------------|-----|---------|-------|-------------|
| 54 | Diphenylamine              | 122-39-4 | MKCH1042     | 99% | 1,002.5 | µg/mL | +/- 36.4735 |
| 55 | Azobenzene                 | 103-33-3 | BCCG7339     | 98% | 1,003.5 | µg/mL | +/- 36.5106 |
| 56 | 4-Bromophenyl phenyl ether | 101-55-3 | STBH6361     | 99% | 1,005.6 | µg/mL | +/- 36.5847 |
| 57 | Hexachlorobenzene          | 118-74-1 | 14257500     | 99% | 1,005.9 | µg/mL | +/- 36.5988 |
| 58 | Pentachlorophenol          | 87-86-5  | RP230504     | 99% | 1,004.2 | µg/mL | +/- 36.5362 |
| 59 | Phenanthrene               | 85-01-8  | MKCQ8876     | 99% | 1,004.1 | µg/mL | +/- 36.5321 |
| 60 | Anthracene                 | 120-12-7 | MKCR0570     | 99% | 1,008.3 | µg/mL | +/- 36.6857 |
| 61 | Carbazole                  | 86-74-8  | 14351100     | 99% | 1,005.1 | µg/mL | +/- 36.5665 |
| 62 | Di-n-butylphthalate        | 84-74-2  | MKCN4337     | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 63 | Fluoranthene               | 206-44-0 | MKCQ4728     | 99% | 1,003.7 | µg/mL | +/- 36.5159 |
| 64 | Pyrene                     | 129-00-0 | BCCG7845     | 99% | 1,004.3 | µg/mL | +/- 36.5382 |
| 65 | Benzyl butyl phthalate     | 85-68-7  | X12I018      | 99% | 1,003.4 | µg/mL | +/- 36.5058 |
| 66 | Bis(2-ethylhexyl)adipate   | 103-23-1 | MKCM1988     | 99% | 1,003.4 | µg/mL | +/- 36.5079 |
| 67 | Benz(a)anthracene          | 56-55-3  | 0012022BAA   | 97% | 1,004.9 | µg/mL | +/- 36.5624 |
| 68 | Chrysene                   | 218-01-9 | RP230512B    | 99% | 1,006.2 | µg/mL | +/- 36.6089 |
| 69 | Bis(2-ethylhexyl)phthalate | 117-81-7 | MKCQ3468     | 99% | 1,003.8 | µg/mL | +/- 36.5220 |
| 70 | Di-n-octyl phthalate       | 117-84-0 | 13994100     | 99% | 1,004.2 | µg/mL | +/- 36.5341 |
| 71 | Benzo(b)fluoranthene       | 205-99-2 | 012013B      | 99% | 1,008.4 | µg/mL | +/- 36.6877 |
| 72 | Benzo(k)fluoranthene       | 207-08-9 | 012022K      | 99% | 1,004.1 | µg/mL | +/- 36.5301 |
| 73 | Benzo(a)pyrene             | 50-32-8  | J6IUE        | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 74 | Indeno(1,2,3-cd)pyrene     | 193-39-5 | 12-JKL-118-9 | 97% | 1,002.0 | µg/mL | +/- 36.4557 |
| 75 | Dibenz(a,h)anthracene      | 53-70-3  | ER032211-01  | 99% | 1,006.1 | µg/mL | +/- 36.6029 |
| 76 | Benzo(g,h,i)perylene       | 191-24-2 | RP230511B    | 98% | 1,006.8 | µg/mL | +/- 36.6295 |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant flow 1.8 mL/min.

**Temp. Program:**

80°C (hold 0.1 min.) to 330°C  
@ 9.6°C/min. (hold 2.86 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

340°C

**Det. Type:**


FID

**Split Vent:**

100 ml/min.

**Inj. Vol**

1µl

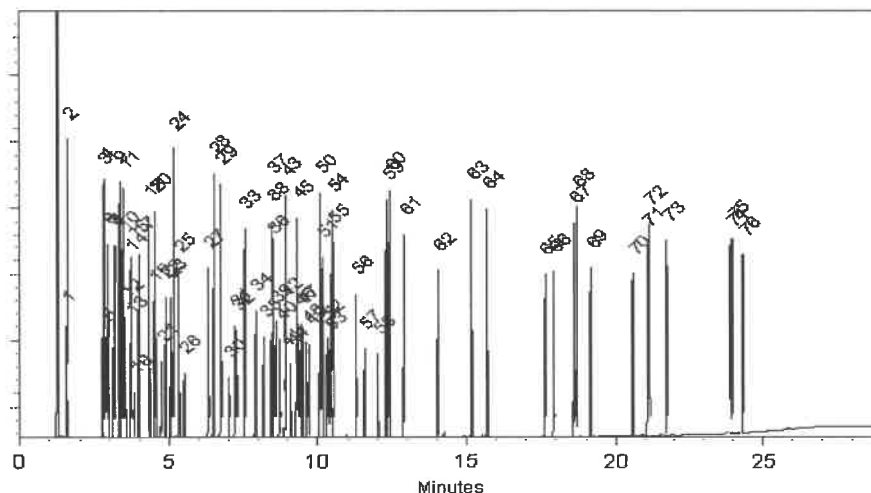

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Tom Suckar - Mix Technician

Date Mixed: 11-May-2023

Balance Serial # 1128353505

  
Christie Mills - Operations Tech II - ARM QC

Date Passed: 18-May-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



## FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

**Catalog No. :** 31850 **Lot No.:** A0197982

**Description :** 8270 MegaMix®  
8270 MegaMix® 500-1,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** November 30, 2024 **Storage:** 0°C or colder

**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

511877  
↓  
511906

RC/  
11/30/23

## CERTIFIED VALUES

| Elution Order | Compound                     | CAS #    | Lot #     | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------------|----------|-----------|--------|-----------------------------|--|
| 1             | Pyridine                     | 110-86-1 | SHBN7324  | 99%    | 1,006.9 µg/mL               | +/- 36.6352                            |
| 2             | N-Nitrosodimethylamine       | 62-75-9  | 230209JLM | 99%    | 1,007.4 µg/mL               | +/- 36.6514                            |
| 3             | Phenol                       | 108-95-2 | MKCK1120  | 99%    | 1,005.3 µg/mL               | +/- 36.5746                            |
| 4             | Aniline                      | 62-53-3  | X22F726   | 99%    | 1,004.6 µg/mL               | +/- 36.5503                            |
| 5             | Bis(2-chloroethyl)ether      | 111-44-4 | SHBL6942  | 99%    | 1,005.1 µg/mL               | +/- 36.5665                            |
| 6             | 2-Chlorophenol               | 95-57-8  | STBJ3909  | 99%    | 1,007.1 µg/mL               | +/- 36.6392                            |
| 7             | 1,3-Dichlorobenzene          | 541-73-1 | BCBZ7498  | 99%    | 1,006.7 µg/mL               | +/- 36.6251                            |
| 8             | 1,4-Dichlorobenzene          | 106-46-7 | MKBS7929V | 99%    | 1,005.6 µg/mL               | +/- 36.5867                            |
| 9             | Benzyl alcohol               | 100-51-6 | SHBK5943  | 99%    | 1,005.4 µg/mL               | +/- 36.5786                            |
| 10            | 1,2-Dichlorobenzene          | 95-50-1  | SHBN3835  | 99%    | 1,003.9 µg/mL               | +/- 36.5240                            |
| 11            | 2-Methylphenol (o-cresol)    | 95-48-7  | SHBN7598  | 99%    | 1,002.3 µg/mL               | +/- 36.4654                            |
| 12            | 2,2'-oxybis(1-chloropropane) | 108-60-1 | 230329JLM | 99%    | 1,004.3 µg/mL               | +/- 36.5402                            |
| 13            | 3-Methylphenol (m-cresol)    | 108-39-4 | STBJ0710  | 99%    | 502.1 µg/mL                 | +/- 18.2671                            |
| 14            | 4-Methylphenol (p-cresol)    | 106-44-5 | SHBN3411  | 99%    | 501.9 µg/mL                 | +/- 18.2631                            |
| 15            | N-Nitroso-di-n-propylamine   | 621-64-7 | N63MG     | 99%    | 1,004.0 µg/mL               | +/- 36.5281                            |
| 16            | Hexachloroethane             | 67-72-1  | QTORH     | 99%    | 1,006.1 µg/mL               | +/- 36.6029                            |
| 17            | Nitrobenzene                 | 98-95-3  | 10224044  | 99%    | 1,003.1 µg/mL               | +/- 36.4957                            |

|    |   |           |             |     |         |       |     |         |
|----|---|-----------|-------------|-----|---------|-------|-----|---------|
| 18 | Isophorone                                    | 78-59-1   | MKCC9506    | 99% | 1,003.8 | µg/mL | +/- | 36.5220 |
| 19 | 2-Nitrophenol                                 | 88-75-5   | RP230509C   | 99% | 1,005.8 | µg/mL | +/- | 36.5948 |
| 20 | 2,4-Dimethylphenol                            | 105-67-9  | XW5GK       | 99% | 1,004.2 | µg/mL | +/- | 36.5341 |
| 21 | Bis(2-chloroethoxy)methane                    | 111-91-1  | 13670200    | 99% | 1,006.3 | µg/mL | +/- | 36.6130 |
| 22 | 2,4-Dichlorophenol                            | 120-83-2  | BCBZ6787    | 99% | 1,004.0 | µg/mL | +/- | 36.5281 |
| 23 | 1,2,4-Trichlorobenzene                        | 120-82-1  | SHBM0526    | 99% | 1,007.1 | µg/mL | +/- | 36.6413 |
| 24 | Naphthalene                                   | 91-20-3   | MKCH0219    | 99% | 1,006.7 | µg/mL | +/- | 36.6271 |
| 25 | 4-Chloroaniline                               | 106-47-8  | WXBC4601V   | 99% | 1,005.4 | µg/mL | +/- | 36.5806 |
| 26 | Hexachlorobutadiene                           | 87-68-3   | X05J        | 99% | 1,006.4 | µg/mL | +/- | 36.6170 |
| 27 | 4-Chloro-3-methylphenol                       | 59-50-7   | BCCD4461    | 99% | 1,004.7 | µg/mL | +/- | 36.5543 |
| 28 | 2-Methylnaphthalene                           | 91-57-6   | STBK0259    | 96% | 1,002.3 | µg/mL | +/- | 36.4679 |
| 29 | 1-Methylnaphthalene                           | 90-12-0   | 5234.00-3   | 99% | 1,000.0 | µg/mL | +/- | 36.3825 |
| 30 | Hexachlorocyclopentadiene                     | 77-47-4   | 0012019     | 99% | 1,006.1 | µg/mL | +/- | 36.6049 |
| 31 | 2,4,6-Trichlorophenol                         | 88-06-2   | STBJ5914    | 99% | 1,004.9 | µg/mL | +/- | 36.5604 |
| 32 | 2,4,5-Trichlorophenol                         | 95-95-4   | FHN01       | 98% | 1,006.5 | µg/mL | +/- | 36.6176 |
| 33 | 2-Chloronaphthalene                           | 91-58-7   | RPN70       | 99% | 1,004.4 | µg/mL | +/- | 36.5422 |
| 34 | 2-Nitroaniline                                | 88-74-4   | RP230509A   | 99% | 1,002.3 | µg/mL | +/- | 36.4654 |
| 35 | 1,4-Dinitrobenzene                            | 100-25-4  | RP230512A   | 99% | 1,001.5 | µg/mL | +/- | 36.4371 |
| 36 | Acenaphthylene                                | 208-96-8  | L10L        | 95% | 1,003.4 | µg/mL | +/- | 36.5066 |
| 37 | 1,3-Dinitrobenzene                            | 99-65-0   | 1-DXX-24-1  | 99% | 1,004.8 | µg/mL | +/- | 36.5564 |
| 38 | Dimethylphthalate                             | 131-11-3  | 10117699    | 99% | 1,004.7 | µg/mL | +/- | 36.5543 |
| 39 | 2,6-Dinitrotoluene                            | 606-20-2  | BCCG1833    | 99% | 1,006.8 | µg/mL | +/- | 36.6312 |
| 40 | 1,2-Dinitrobenzene                            | 528-29-0  | RP230428    | 99% | 1,006.4 | µg/mL | +/- | 36.6170 |
| 41 | Acenaphthene                                  | 83-32-9   | MKCR7169    | 99% | 1,000.0 | µg/mL | +/- | 36.3825 |
| 42 | 3-Nitroaniline                                | 99-09-2   | MKCH5457    | 99% | 1,004.8 | µg/mL | +/- | 36.5584 |
| 43 | 2,4-Dinitrophenol                             | 51-28-5   | DR230417RSR | 99% | 1,005.8 | µg/mL | +/- | 36.5948 |
| 44 | Dibenzofuran                                  | 132-64-9  | MKCN1772    | 99% | 1,004.3 | µg/mL | +/- | 36.5402 |
| 45 | 2,4-Dinitrotoluene                            | 121-14-2  | MKAA0690V   | 99% | 1,005.8 | µg/mL | +/- | 36.5928 |
| 46 | 4-Nitrophenol                                 | 100-02-7  | RP230511A   | 99% | 1,005.8 | µg/mL | +/- | 36.5948 |
| 47 | 2,3,4,6-Tetrachlorophenol                     | 58-90-2   | PR-30126    | 99% | 1,005.9 | µg/mL | +/- | 36.5988 |
| 48 | 2,3,5,6-Tetrachlorophenol                     | 935-95-5  | RP230513    | 99% | 1,004.9 | µg/mL | +/- | 36.5624 |
| 49 | Fluorene                                      | 86-73-7   | 10236068    | 99% | 1,005.4 | µg/mL | +/- | 36.5806 |
| 50 | 4-Chlorophenyl phenyl ether                   | 7005-72-3 | MKCQ0984    | 99% | 1,004.3 | µg/mL | +/- | 36.5382 |
| 51 | Diethylphthalate                              | 84-66-2   | BCCD3396    | 99% | 1,007.1 | µg/mL | +/- | 36.6392 |
| 52 | 4-Nitroaniline                                | 100-01-6  | RP220906    | 99% | 1,005.3 | µg/mL | +/- | 36.5766 |
| 53 | 4,6-Dinitro-2-methylphenol (Dinitro-o-cresol) | 534-52-1  | 230505JLM   | 99% | 1,003.8 | µg/mL | +/- | 36.5200 |



|    |                            |          |              |     |         |       |             |
|----|----------------------------|----------|--------------|-----|---------|-------|-------------|
| 54 | Diphenylamine              | 122-39-4 | MKCH1042     | 99% | 1,002.5 | µg/mL | +/- 36.4735 |
| 55 | Azobenzene                 | 103-33-3 | BCCG7339     | 98% | 1,003.5 | µg/mL | +/- 36.5106 |
| 56 | 4-Bromophenyl phenyl ether | 101-55-3 | STBH6361     | 99% | 1,005.6 | µg/mL | +/- 36.5847 |
| 57 | Hexachlorobenzene          | 118-74-1 | 14257500     | 99% | 1,005.9 | µg/mL | +/- 36.5988 |
| 58 | Pentachlorophenol          | 87-86-5  | RP230504     | 99% | 1,004.2 | µg/mL | +/- 36.5362 |
| 59 | Phenanthrene               | 85-01-8  | MKCQ8876     | 99% | 1,004.1 | µg/mL | +/- 36.5321 |
| 60 | Anthracene                 | 120-12-7 | MKCR0570     | 99% | 1,008.3 | µg/mL | +/- 36.6857 |
| 61 | Carbazole                  | 86-74-8  | 14351100     | 99% | 1,005.1 | µg/mL | +/- 36.5665 |
| 62 | Di-n-butylphthalate        | 84-74-2  | MKCN4337     | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 63 | Fluoranthene               | 206-44-0 | MKCQ4728     | 99% | 1,003.7 | µg/mL | +/- 36.5159 |
| 64 | Pyrene                     | 129-00-0 | BCCG7845     | 99% | 1,004.3 | µg/mL | +/- 36.5382 |
| 65 | Benzyl butyl phthalate     | 85-68-7  | X12I018      | 99% | 1,003.4 | µg/mL | +/- 36.5058 |
| 66 | Bis(2-ethylhexyl)adipate   | 103-23-1 | MKCM1988     | 99% | 1,003.4 | µg/mL | +/- 36.5079 |
| 67 | Benz(a)anthracene          | 56-55-3  | 0012022BAA   | 97% | 1,004.9 | µg/mL | +/- 36.5624 |
| 68 | Chrysene                   | 218-01-9 | RP230512B    | 99% | 1,006.2 | µg/mL | +/- 36.6089 |
| 69 | Bis(2-ethylhexyl)phthalate | 117-81-7 | MKCQ3468     | 99% | 1,003.8 | µg/mL | +/- 36.5220 |
| 70 | Di-n-octyl phthalate       | 117-84-0 | 13994100     | 99% | 1,004.2 | µg/mL | +/- 36.5341 |
| 71 | Benzo(b)fluoranthene       | 205-99-2 | 012013B      | 99% | 1,008.4 | µg/mL | +/- 36.6877 |
| 72 | Benzo(k)fluoranthene       | 207-08-9 | 012022K      | 99% | 1,004.1 | µg/mL | +/- 36.5301 |
| 73 | Benzo(a)pyrene             | 50-32-8  | J6IUE        | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 74 | Indeno(1,2,3-cd)pyrene     | 193-39-5 | 12-JKL-118-9 | 97% | 1,002.0 | µg/mL | +/- 36.4557 |
| 75 | Dibenz(a,h)anthracene      | 53-70-3  | ER032211-01  | 99% | 1,006.1 | µg/mL | +/- 36.6029 |
| 76 | Benzo(g,h,i)perylene       | 191-24-2 | RP230511B    | 98% | 1,006.8 | µg/mL | +/- 36.6295 |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant flow 1.8 mL/min.

**Temp. Program:**

80°C (hold 0.1 min.) to 330°C  
@ 9.6°C/min. (hold 2.86 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

340°C

**Det. Type:**


FID

**Split Vent:**

100 ml/min.

**Inj. Vol**

1µl

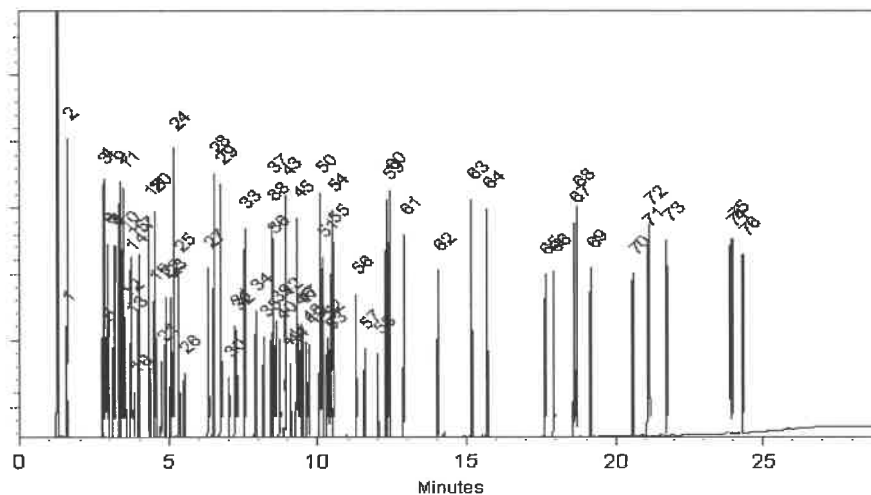

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Tom Suckar - Mix Technician

Date Mixed: 11-May-2023

Balance Serial # 1128353505

  
Christie Mills - Operations Tech II - ARM QC

Date Passed: 18-May-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



## FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

**Catalog No. :** 31850 **Lot No.:** A0197982

**Description :** 8270 MegaMix®  
8270 MegaMix® 500-1,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** November 30, 2024 **Storage:** 0°C or colder

**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

511877  
↓  
511906

RC/  
11/30/23

## CERTIFIED VALUES

| Elution Order | Compound                     | CAS #    | Lot #     | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------------|----------|-----------|--------|-----------------------------|--|
| 1             | Pyridine                     | 110-86-1 | SHBN7324  | 99%    | 1,006.9 µg/mL               | +/- 36.6352                            |
| 2             | N-Nitrosodimethylamine       | 62-75-9  | 230209JLM | 99%    | 1,007.4 µg/mL               | +/- 36.6514                            |
| 3             | Phenol                       | 108-95-2 | MKCK1120  | 99%    | 1,005.3 µg/mL               | +/- 36.5746                            |
| 4             | Aniline                      | 62-53-3  | X22F726   | 99%    | 1,004.6 µg/mL               | +/- 36.5503                            |
| 5             | Bis(2-chloroethyl)ether      | 111-44-4 | SHBL6942  | 99%    | 1,005.1 µg/mL               | +/- 36.5665                            |
| 6             | 2-Chlorophenol               | 95-57-8  | STBJ3909  | 99%    | 1,007.1 µg/mL               | +/- 36.6392                            |
| 7             | 1,3-Dichlorobenzene          | 541-73-1 | BCBZ7498  | 99%    | 1,006.7 µg/mL               | +/- 36.6251                            |
| 8             | 1,4-Dichlorobenzene          | 106-46-7 | MKBS7929V | 99%    | 1,005.6 µg/mL               | +/- 36.5867                            |
| 9             | Benzyl alcohol               | 100-51-6 | SHBK5943  | 99%    | 1,005.4 µg/mL               | +/- 36.5786                            |
| 10            | 1,2-Dichlorobenzene          | 95-50-1  | SHBN3835  | 99%    | 1,003.9 µg/mL               | +/- 36.5240                            |
| 11            | 2-Methylphenol (o-cresol)    | 95-48-7  | SHBN7598  | 99%    | 1,002.3 µg/mL               | +/- 36.4654                            |
| 12            | 2,2'-oxybis(1-chloropropane) | 108-60-1 | 230329JLM | 99%    | 1,004.3 µg/mL               | +/- 36.5402                            |
| 13            | 3-Methylphenol (m-cresol)    | 108-39-4 | STBJ0710  | 99%    | 502.1 µg/mL                 | +/- 18.2671                            |
| 14            | 4-Methylphenol (p-cresol)    | 106-44-5 | SHBN3411  | 99%    | 501.9 µg/mL                 | +/- 18.2631                            |
| 15            | N-Nitroso-di-n-propylamine   | 621-64-7 | N63MG     | 99%    | 1,004.0 µg/mL               | +/- 36.5281                            |
| 16            | Hexachloroethane             | 67-72-1  | QTORH     | 99%    | 1,006.1 µg/mL               | +/- 36.6029                            |
| 17            | Nitrobenzene                 | 98-95-3  | 10224044  | 99%    | 1,003.1 µg/mL               | +/- 36.4957                            |

|    |   |           |             |     |         |       |     |         |
|----|---|-----------|-------------|-----|---------|-------|-----|---------|
| 18 | Isophorone                                    | 78-59-1   | MKCC9506    | 99% | 1,003.8 | µg/mL | +/- | 36.5220 |
| 19 | 2-Nitrophenol                                 | 88-75-5   | RP230509C   | 99% | 1,005.8 | µg/mL | +/- | 36.5948 |
| 20 | 2,4-Dimethylphenol                            | 105-67-9  | XW5GK       | 99% | 1,004.2 | µg/mL | +/- | 36.5341 |
| 21 | Bis(2-chloroethoxy)methane                    | 111-91-1  | 13670200    | 99% | 1,006.3 | µg/mL | +/- | 36.6130 |
| 22 | 2,4-Dichlorophenol                            | 120-83-2  | BCBZ6787    | 99% | 1,004.0 | µg/mL | +/- | 36.5281 |
| 23 | 1,2,4-Trichlorobenzene                        | 120-82-1  | SHBM0526    | 99% | 1,007.1 | µg/mL | +/- | 36.6413 |
| 24 | Naphthalene                                   | 91-20-3   | MKCH0219    | 99% | 1,006.7 | µg/mL | +/- | 36.6271 |
| 25 | 4-Chloroaniline                               | 106-47-8  | WXBC4601V   | 99% | 1,005.4 | µg/mL | +/- | 36.5806 |
| 26 | Hexachlorobutadiene                           | 87-68-3   | X05J        | 99% | 1,006.4 | µg/mL | +/- | 36.6170 |
| 27 | 4-Chloro-3-methylphenol                       | 59-50-7   | BCCD4461    | 99% | 1,004.7 | µg/mL | +/- | 36.5543 |
| 28 | 2-Methylnaphthalene                           | 91-57-6   | STBK0259    | 96% | 1,002.3 | µg/mL | +/- | 36.4679 |
| 29 | 1-Methylnaphthalene                           | 90-12-0   | 5234.00-3   | 99% | 1,000.0 | µg/mL | +/- | 36.3825 |
| 30 | Hexachlorocyclopentadiene                     | 77-47-4   | 0012019     | 99% | 1,006.1 | µg/mL | +/- | 36.6049 |
| 31 | 2,4,6-Trichlorophenol                         | 88-06-2   | STBJ5914    | 99% | 1,004.9 | µg/mL | +/- | 36.5604 |
| 32 | 2,4,5-Trichlorophenol                         | 95-95-4   | FHN01       | 98% | 1,006.5 | µg/mL | +/- | 36.6176 |
| 33 | 2-Chloronaphthalene                           | 91-58-7   | RPN70       | 99% | 1,004.4 | µg/mL | +/- | 36.5422 |
| 34 | 2-Nitroaniline                                | 88-74-4   | RP230509A   | 99% | 1,002.3 | µg/mL | +/- | 36.4654 |
| 35 | 1,4-Dinitrobenzene                            | 100-25-4  | RP230512A   | 99% | 1,001.5 | µg/mL | +/- | 36.4371 |
| 36 | Acenaphthylene                                | 208-96-8  | L10L        | 95% | 1,003.4 | µg/mL | +/- | 36.5066 |
| 37 | 1,3-Dinitrobenzene                            | 99-65-0   | 1-DXX-24-1  | 99% | 1,004.8 | µg/mL | +/- | 36.5564 |
| 38 | Dimethylphthalate                             | 131-11-3  | 10117699    | 99% | 1,004.7 | µg/mL | +/- | 36.5543 |
| 39 | 2,6-Dinitrotoluene                            | 606-20-2  | BCCG1833    | 99% | 1,006.8 | µg/mL | +/- | 36.6312 |
| 40 | 1,2-Dinitrobenzene                            | 528-29-0  | RP230428    | 99% | 1,006.4 | µg/mL | +/- | 36.6170 |
| 41 | Acenaphthene                                  | 83-32-9   | MKCR7169    | 99% | 1,000.0 | µg/mL | +/- | 36.3825 |
| 42 | 3-Nitroaniline                                | 99-09-2   | MKCH5457    | 99% | 1,004.8 | µg/mL | +/- | 36.5584 |
| 43 | 2,4-Dinitrophenol                             | 51-28-5   | DR230417RSR | 99% | 1,005.8 | µg/mL | +/- | 36.5948 |
| 44 | Dibenzofuran                                  | 132-64-9  | MKCN1772    | 99% | 1,004.3 | µg/mL | +/- | 36.5402 |
| 45 | 2,4-Dinitrotoluene                            | 121-14-2  | MKAA0690V   | 99% | 1,005.8 | µg/mL | +/- | 36.5928 |
| 46 | 4-Nitrophenol                                 | 100-02-7  | RP230511A   | 99% | 1,005.8 | µg/mL | +/- | 36.5948 |
| 47 | 2,3,4,6-Tetrachlorophenol                     | 58-90-2   | PR-30126    | 99% | 1,005.9 | µg/mL | +/- | 36.5988 |
| 48 | 2,3,5,6-Tetrachlorophenol                     | 935-95-5  | RP230513    | 99% | 1,004.9 | µg/mL | +/- | 36.5624 |
| 49 | Fluorene                                      | 86-73-7   | 10236068    | 99% | 1,005.4 | µg/mL | +/- | 36.5806 |
| 50 | 4-Chlorophenyl phenyl ether                   | 7005-72-3 | MKCQ0984    | 99% | 1,004.3 | µg/mL | +/- | 36.5382 |
| 51 | Diethylphthalate                              | 84-66-2   | BCCD3396    | 99% | 1,007.1 | µg/mL | +/- | 36.6392 |
| 52 | 4-Nitroaniline                                | 100-01-6  | RP220906    | 99% | 1,005.3 | µg/mL | +/- | 36.5766 |
| 53 | 4,6-Dinitro-2-methylphenol (Dinitro-o-cresol) | 534-52-1  | 230505JLM   | 99% | 1,003.8 | µg/mL | +/- | 36.5200 |

|    |                            |          |              |     |         |       |             |
|----|----------------------------|----------|--------------|-----|---------|-------|-------------|
| 54 | Diphenylamine              | 122-39-4 | MKCH1042     | 99% | 1,002.5 | µg/mL | +/- 36.4735 |
| 55 | Azobenzene                 | 103-33-3 | BCCG7339     | 98% | 1,003.5 | µg/mL | +/- 36.5106 |
| 56 | 4-Bromophenyl phenyl ether | 101-55-3 | STBH6361     | 99% | 1,005.6 | µg/mL | +/- 36.5847 |
| 57 | Hexachlorobenzene          | 118-74-1 | 14257500     | 99% | 1,005.9 | µg/mL | +/- 36.5988 |
| 58 | Pentachlorophenol          | 87-86-5  | RP230504     | 99% | 1,004.2 | µg/mL | +/- 36.5362 |
| 59 | Phenanthrene               | 85-01-8  | MKCQ8876     | 99% | 1,004.1 | µg/mL | +/- 36.5321 |
| 60 | Anthracene                 | 120-12-7 | MKCR0570     | 99% | 1,008.3 | µg/mL | +/- 36.6857 |
| 61 | Carbazole                  | 86-74-8  | 14351100     | 99% | 1,005.1 | µg/mL | +/- 36.5665 |
| 62 | Di-n-butylphthalate        | 84-74-2  | MKCN4337     | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 63 | Fluoranthene               | 206-44-0 | MKCQ4728     | 99% | 1,003.7 | µg/mL | +/- 36.5159 |
| 64 | Pyrene                     | 129-00-0 | BCCG7845     | 99% | 1,004.3 | µg/mL | +/- 36.5382 |
| 65 | Benzyl butyl phthalate     | 85-68-7  | X12I018      | 99% | 1,003.4 | µg/mL | +/- 36.5058 |
| 66 | Bis(2-ethylhexyl)adipate   | 103-23-1 | MKCM1988     | 99% | 1,003.4 | µg/mL | +/- 36.5079 |
| 67 | Benz(a)anthracene          | 56-55-3  | 0012022BAA   | 97% | 1,004.9 | µg/mL | +/- 36.5624 |
| 68 | Chrysene                   | 218-01-9 | RP230512B    | 99% | 1,006.2 | µg/mL | +/- 36.6089 |
| 69 | Bis(2-ethylhexyl)phthalate | 117-81-7 | MKCQ3468     | 99% | 1,003.8 | µg/mL | +/- 36.5220 |
| 70 | Di-n-octyl phthalate       | 117-84-0 | 13994100     | 99% | 1,004.2 | µg/mL | +/- 36.5341 |
| 71 | Benzo(b)fluoranthene       | 205-99-2 | 012013B      | 99% | 1,008.4 | µg/mL | +/- 36.6877 |
| 72 | Benzo(k)fluoranthene       | 207-08-9 | 012022K      | 99% | 1,004.1 | µg/mL | +/- 36.5301 |
| 73 | Benzo(a)pyrene             | 50-32-8  | J6IUE        | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 74 | Indeno(1,2,3-cd)pyrene     | 193-39-5 | 12-JKL-118-9 | 97% | 1,002.0 | µg/mL | +/- 36.4557 |
| 75 | Dibenz(a,h)anthracene      | 53-70-3  | ER032211-01  | 99% | 1,006.1 | µg/mL | +/- 36.6029 |
| 76 | Benzo(g,h,i)perylene       | 191-24-2 | RP230511B    | 98% | 1,006.8 | µg/mL | +/- 36.6295 |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant flow 1.8 mL/min.

**Temp. Program:**

80°C (hold 0.1 min.) to 330°C  
@ 9.6°C/min. (hold 2.86 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

340°C

**Det. Type:**


FID

**Split Vent:**

100 ml/min.

**Inj. Vol**

1µl

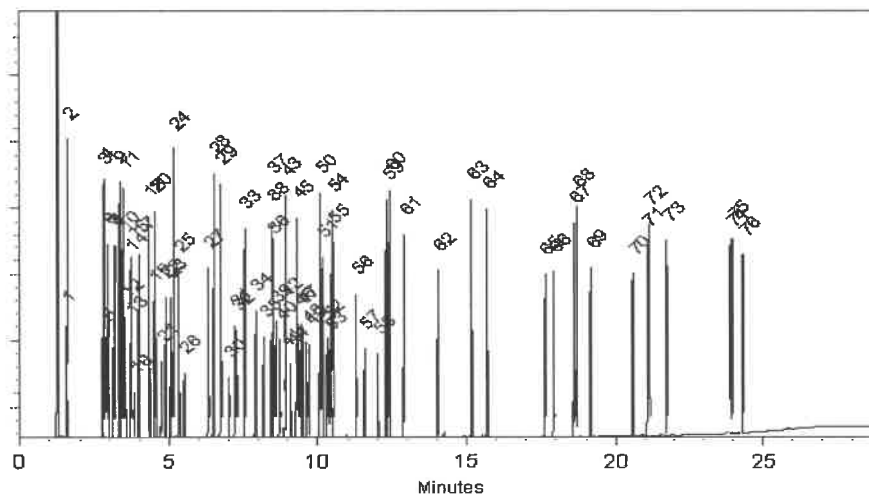

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Tom Suckar - Mix Technician

Date Mixed: 11-May-2023

Balance Serial # 1128353505

  
Christie Mills - Operations Tech II - ARM QC

Date Passed: 18-May-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



## FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

**Catalog No. :** 31850 **Lot No.:** A0197982

**Description :** 8270 MegaMix®  
8270 MegaMix® 500-1,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** November 30, 2024 **Storage:** 0°C or colder

**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

511877  
↓  
511906

RC/  
11/30/23

## CERTIFIED VALUES

| Elution Order | Compound                     | CAS #    | Lot #     | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------------|----------|-----------|--------|-----------------------------|--|
| 1             | Pyridine                     | 110-86-1 | SHBN7324  | 99%    | 1,006.9 µg/mL               | +/- 36.6352                            |
| 2             | N-Nitrosodimethylamine       | 62-75-9  | 230209JLM | 99%    | 1,007.4 µg/mL               | +/- 36.6514                            |
| 3             | Phenol                       | 108-95-2 | MKCK1120  | 99%    | 1,005.3 µg/mL               | +/- 36.5746                            |
| 4             | Aniline                      | 62-53-3  | X22F726   | 99%    | 1,004.6 µg/mL               | +/- 36.5503                            |
| 5             | Bis(2-chloroethyl)ether      | 111-44-4 | SHBL6942  | 99%    | 1,005.1 µg/mL               | +/- 36.5665                            |
| 6             | 2-Chlorophenol               | 95-57-8  | STBJ3909  | 99%    | 1,007.1 µg/mL               | +/- 36.6392                            |
| 7             | 1,3-Dichlorobenzene          | 541-73-1 | BCBZ7498  | 99%    | 1,006.7 µg/mL               | +/- 36.6251                            |
| 8             | 1,4-Dichlorobenzene          | 106-46-7 | MKBS7929V | 99%    | 1,005.6 µg/mL               | +/- 36.5867                            |
| 9             | Benzyl alcohol               | 100-51-6 | SHBK5943  | 99%    | 1,005.4 µg/mL               | +/- 36.5786                            |
| 10            | 1,2-Dichlorobenzene          | 95-50-1  | SHBN3835  | 99%    | 1,003.9 µg/mL               | +/- 36.5240                            |
| 11            | 2-Methylphenol (o-cresol)    | 95-48-7  | SHBN7598  | 99%    | 1,002.3 µg/mL               | +/- 36.4654                            |
| 12            | 2,2'-oxybis(1-chloropropane) | 108-60-1 | 230329JLM | 99%    | 1,004.3 µg/mL               | +/- 36.5402                            |
| 13            | 3-Methylphenol (m-cresol)    | 108-39-4 | STBJ0710  | 99%    | 502.1 µg/mL                 | +/- 18.2671                            |
| 14            | 4-Methylphenol (p-cresol)    | 106-44-5 | SHBN3411  | 99%    | 501.9 µg/mL                 | +/- 18.2631                            |
| 15            | N-Nitroso-di-n-propylamine   | 621-64-7 | N63MG     | 99%    | 1,004.0 µg/mL               | +/- 36.5281                            |
| 16            | Hexachloroethane             | 67-72-1  | QTORH     | 99%    | 1,006.1 µg/mL               | +/- 36.6029                            |
| 17            | Nitrobenzene                 | 98-95-3  | 10224044  | 99%    | 1,003.1 µg/mL               | +/- 36.4957                            |

|    |   |           |             |     |         |       |     |         |
|----|---|-----------|-------------|-----|---------|-------|-----|---------|
| 18 | Isophorone                                    | 78-59-1   | MKCC9506    | 99% | 1,003.8 | µg/mL | +/- | 36.5220 |
| 19 | 2-Nitrophenol                                 | 88-75-5   | RP230509C   | 99% | 1,005.8 | µg/mL | +/- | 36.5948 |
| 20 | 2,4-Dimethylphenol                            | 105-67-9  | XW5GK       | 99% | 1,004.2 | µg/mL | +/- | 36.5341 |
| 21 | Bis(2-chloroethoxy)methane                    | 111-91-1  | 13670200    | 99% | 1,006.3 | µg/mL | +/- | 36.6130 |
| 22 | 2,4-Dichlorophenol                            | 120-83-2  | BCBZ6787    | 99% | 1,004.0 | µg/mL | +/- | 36.5281 |
| 23 | 1,2,4-Trichlorobenzene                        | 120-82-1  | SHBM0526    | 99% | 1,007.1 | µg/mL | +/- | 36.6413 |
| 24 | Naphthalene                                   | 91-20-3   | MKCH0219    | 99% | 1,006.7 | µg/mL | +/- | 36.6271 |
| 25 | 4-Chloroaniline                               | 106-47-8  | WXBC4601V   | 99% | 1,005.4 | µg/mL | +/- | 36.5806 |
| 26 | Hexachlorobutadiene                           | 87-68-3   | X05J        | 99% | 1,006.4 | µg/mL | +/- | 36.6170 |
| 27 | 4-Chloro-3-methylphenol                       | 59-50-7   | BCCD4461    | 99% | 1,004.7 | µg/mL | +/- | 36.5543 |
| 28 | 2-Methylnaphthalene                           | 91-57-6   | STBK0259    | 96% | 1,002.3 | µg/mL | +/- | 36.4679 |
| 29 | 1-Methylnaphthalene                           | 90-12-0   | 5234.00-3   | 99% | 1,000.0 | µg/mL | +/- | 36.3825 |
| 30 | Hexachlorocyclopentadiene                     | 77-47-4   | 0012019     | 99% | 1,006.1 | µg/mL | +/- | 36.6049 |
| 31 | 2,4,6-Trichlorophenol                         | 88-06-2   | STBJ5914    | 99% | 1,004.9 | µg/mL | +/- | 36.5604 |
| 32 | 2,4,5-Trichlorophenol                         | 95-95-4   | FHN01       | 98% | 1,006.5 | µg/mL | +/- | 36.6176 |
| 33 | 2-Chloronaphthalene                           | 91-58-7   | RPN70       | 99% | 1,004.4 | µg/mL | +/- | 36.5422 |
| 34 | 2-Nitroaniline                                | 88-74-4   | RP230509A   | 99% | 1,002.3 | µg/mL | +/- | 36.4654 |
| 35 | 1,4-Dinitrobenzene                            | 100-25-4  | RP230512A   | 99% | 1,001.5 | µg/mL | +/- | 36.4371 |
| 36 | Acenaphthylene                                | 208-96-8  | L10L        | 95% | 1,003.4 | µg/mL | +/- | 36.5066 |
| 37 | 1,3-Dinitrobenzene                            | 99-65-0   | 1-DXX-24-1  | 99% | 1,004.8 | µg/mL | +/- | 36.5564 |
| 38 | Dimethylphthalate                             | 131-11-3  | 10117699    | 99% | 1,004.7 | µg/mL | +/- | 36.5543 |
| 39 | 2,6-Dinitrotoluene                            | 606-20-2  | BCCG1833    | 99% | 1,006.8 | µg/mL | +/- | 36.6312 |
| 40 | 1,2-Dinitrobenzene                            | 528-29-0  | RP230428    | 99% | 1,006.4 | µg/mL | +/- | 36.6170 |
| 41 | Acenaphthene                                  | 83-32-9   | MKCR7169    | 99% | 1,000.0 | µg/mL | +/- | 36.3825 |
| 42 | 3-Nitroaniline                                | 99-09-2   | MKCH5457    | 99% | 1,004.8 | µg/mL | +/- | 36.5584 |
| 43 | 2,4-Dinitrophenol                             | 51-28-5   | DR230417RSR | 99% | 1,005.8 | µg/mL | +/- | 36.5948 |
| 44 | Dibenzofuran                                  | 132-64-9  | MKCN1772    | 99% | 1,004.3 | µg/mL | +/- | 36.5402 |
| 45 | 2,4-Dinitrotoluene                            | 121-14-2  | MKAA0690V   | 99% | 1,005.8 | µg/mL | +/- | 36.5928 |
| 46 | 4-Nitrophenol                                 | 100-02-7  | RP230511A   | 99% | 1,005.8 | µg/mL | +/- | 36.5948 |
| 47 | 2,3,4,6-Tetrachlorophenol                     | 58-90-2   | PR-30126    | 99% | 1,005.9 | µg/mL | +/- | 36.5988 |
| 48 | 2,3,5,6-Tetrachlorophenol                     | 935-95-5  | RP230513    | 99% | 1,004.9 | µg/mL | +/- | 36.5624 |
| 49 | Fluorene                                      | 86-73-7   | 10236068    | 99% | 1,005.4 | µg/mL | +/- | 36.5806 |
| 50 | 4-Chlorophenyl phenyl ether                   | 7005-72-3 | MKCQ0984    | 99% | 1,004.3 | µg/mL | +/- | 36.5382 |
| 51 | Diethylphthalate                              | 84-66-2   | BCCD3396    | 99% | 1,007.1 | µg/mL | +/- | 36.6392 |
| 52 | 4-Nitroaniline                                | 100-01-6  | RP220906    | 99% | 1,005.3 | µg/mL | +/- | 36.5766 |
| 53 | 4,6-Dinitro-2-methylphenol (Dinitro-o-cresol) | 534-52-1  | 230505JLM   | 99% | 1,003.8 | µg/mL | +/- | 36.5200 |



|    |                            |          |              |     |         |       |             |
|----|----------------------------|----------|--------------|-----|---------|-------|-------------|
| 54 | Diphenylamine              | 122-39-4 | MKCH1042     | 99% | 1,002.5 | µg/mL | +/- 36.4735 |
| 55 | Azobenzene                 | 103-33-3 | BCCG7339     | 98% | 1,003.5 | µg/mL | +/- 36.5106 |
| 56 | 4-Bromophenyl phenyl ether | 101-55-3 | STBH6361     | 99% | 1,005.6 | µg/mL | +/- 36.5847 |
| 57 | Hexachlorobenzene          | 118-74-1 | 14257500     | 99% | 1,005.9 | µg/mL | +/- 36.5988 |
| 58 | Pentachlorophenol          | 87-86-5  | RP230504     | 99% | 1,004.2 | µg/mL | +/- 36.5362 |
| 59 | Phenanthrene               | 85-01-8  | MKCQ8876     | 99% | 1,004.1 | µg/mL | +/- 36.5321 |
| 60 | Anthracene                 | 120-12-7 | MKCR0570     | 99% | 1,008.3 | µg/mL | +/- 36.6857 |
| 61 | Carbazole                  | 86-74-8  | 14351100     | 99% | 1,005.1 | µg/mL | +/- 36.5665 |
| 62 | Di-n-butylphthalate        | 84-74-2  | MKCN4337     | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 63 | Fluoranthene               | 206-44-0 | MKCQ4728     | 99% | 1,003.7 | µg/mL | +/- 36.5159 |
| 64 | Pyrene                     | 129-00-0 | BCCG7845     | 99% | 1,004.3 | µg/mL | +/- 36.5382 |
| 65 | Benzyl butyl phthalate     | 85-68-7  | X12I018      | 99% | 1,003.4 | µg/mL | +/- 36.5058 |
| 66 | Bis(2-ethylhexyl)adipate   | 103-23-1 | MKCM1988     | 99% | 1,003.4 | µg/mL | +/- 36.5079 |
| 67 | Benz(a)anthracene          | 56-55-3  | 0012022BAA   | 97% | 1,004.9 | µg/mL | +/- 36.5624 |
| 68 | Chrysene                   | 218-01-9 | RP230512B    | 99% | 1,006.2 | µg/mL | +/- 36.6089 |
| 69 | Bis(2-ethylhexyl)phthalate | 117-81-7 | MKCQ3468     | 99% | 1,003.8 | µg/mL | +/- 36.5220 |
| 70 | Di-n-octyl phthalate       | 117-84-0 | 13994100     | 99% | 1,004.2 | µg/mL | +/- 36.5341 |
| 71 | Benzo(b)fluoranthene       | 205-99-2 | 012013B      | 99% | 1,008.4 | µg/mL | +/- 36.6877 |
| 72 | Benzo(k)fluoranthene       | 207-08-9 | 012022K      | 99% | 1,004.1 | µg/mL | +/- 36.5301 |
| 73 | Benzo(a)pyrene             | 50-32-8  | J6IUE        | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 74 | Indeno(1,2,3-cd)pyrene     | 193-39-5 | 12-JKL-118-9 | 97% | 1,002.0 | µg/mL | +/- 36.4557 |
| 75 | Dibenz(a,h)anthracene      | 53-70-3  | ER032211-01  | 99% | 1,006.1 | µg/mL | +/- 36.6029 |
| 76 | Benzo(g,h,i)perylene       | 191-24-2 | RP230511B    | 98% | 1,006.8 | µg/mL | +/- 36.6295 |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant flow 1.8 mL/min.

**Temp. Program:**

80°C (hold 0.1 min.) to 330°C  
@ 9.6°C/min. (hold 2.86 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

340°C

**Det. Type:**


FID

**Split Vent:**

100 ml/min.

**Inj. Vol**

1µl

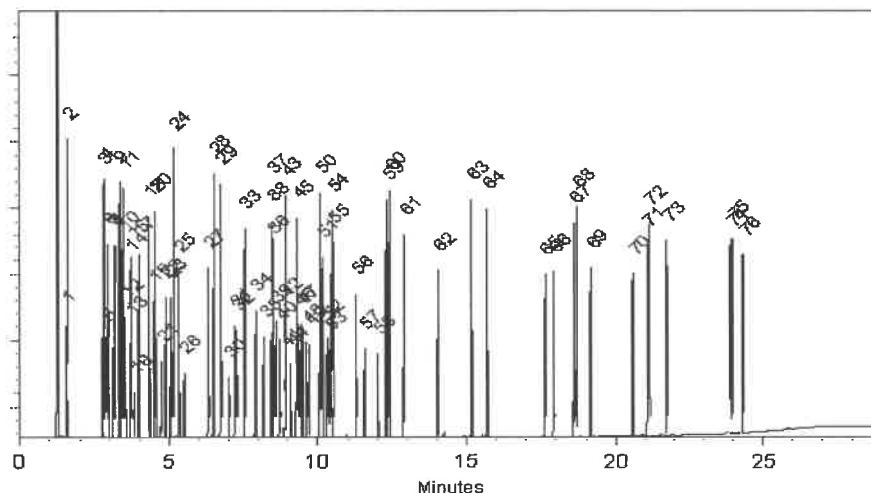

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Tom Suckar - Mix Technician

Date Mixed: 11-May-2023

Balance Serial # 1128353505

  
Christie Mills - Operations Tech II - ARM QC

Date Passed: 18-May-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

## Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 31850 Lot No.: A0197982  
Description: 8270 MegaMix®  
8270 MegaMix® 500-1,000µg/mL, Methylene Chloride, 1mL/ampul  
Container Size: 2 mL Pkg Amt: > 1 mL  
Expiration Date: November 30, 2024 Storage: 0°C or colder  
Handling: Sonication required. Mix is photosensitive. Ship: Ambient

511877  
↓  
511906  
RC/  
11/30/23

### CERTIFIED VALUES

| Elution Order | Compound                     | CAS #    | Lot #     | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------------|----------|-----------|--------|-----------------------------|--|
| 1             | Pyridine                     | 110-86-1 | SHBN7324  | 99%    | 1,006.9 µg/mL               | +/- 36.6352                            |
| 2             | N-Nitrosodimethylamine       | 62-75-9  | 230209JLM | 99%    | 1,007.4 µg/mL               | +/- 36.6514                            |
| 3             | Phenol                       | 108-95-2 | MKCK1120  | 99%    | 1,005.3 µg/mL               | +/- 36.5746                            |
| 4             | Aniline                      | 62-53-3  | X22F726   | 99%    | 1,004.6 µg/mL               | +/- 36.5503                            |
| 5             | Bis(2-chloroethyl)ether      | 111-44-4 | SHBL6942  | 99%    | 1,005.1 µg/mL               | +/- 36.5665                            |
| 6             | 2-Chlorophenol               | 95-57-8  | STBJ3909  | 99%    | 1,007.1 µg/mL               | +/- 36.6392                            |
| 7             | 1,3-Dichlorobenzene          | 541-73-1 | BCBZ7498  | 99%    | 1,006.7 µg/mL               | +/- 36.6251                            |
| 8             | 1,4-Dichlorobenzene          | 106-46-7 | MKBS7929V | 99%    | 1,005.6 µg/mL               | +/- 36.5867                            |
| 9             | Benzyl alcohol               | 100-51-6 | SHBK5943  | 99%    | 1,005.4 µg/mL               | +/- 36.5786                            |
| 10            | 1,2-Dichlorobenzene          | 95-50-1  | SHBN3835  | 99%    | 1,003.9 µg/mL               | +/- 36.5240                            |
| 11            | 2-Methylphenol (o-cresol)    | 95-48-7  | SHBN7598  | 99%    | 1,002.3 µg/mL               | +/- 36.4654                            |
| 12            | 2,2'-oxybis(1-chloropropane) | 108-60-1 | 230329JLM | 99%    | 1,004.3 µg/mL               | +/- 36.5402                            |
| 13            | 3-Methylphenol (m-cresol)    | 108-39-4 | STBJ0710  | 99%    | 502.1 µg/mL                 | +/- 18.2671                            |
| 14            | 4-Methylphenol (p-cresol)    | 106-44-5 | SHBN3411  | 99%    | 501.9 µg/mL                 | +/- 18.2631                            |
| 15            | N-Nitroso-di-n-propylamine   | 621-64-7 | N63MG     | 99%    | 1,004.0 µg/mL               | +/- 36.5281                            |
| 16            | Hexachloroethane             | 67-72-1  | QTORH     | 99%    | 1,006.1 µg/mL               | +/- 36.6029                            |
| 17            | Nitrobenzene                 | 98-95-3  | 10224044  | 99%    | 1,003.1 µg/mL               | +/- 36.4957                            |

|    |   |           |             |     |         |       |             |
|----|---|-----------|-------------|-----|---------|-------|-------------|
| 18 | Isophorone                                    | 78-59-1   | MKCC9506    | 99% | 1,003.8 | µg/mL | +/- 36.5220 |
| 19 | 2-Nitrophenol                                 | 88-75-5   | RP230509C   | 99% | 1,005.8 | µg/mL | +/- 36.5948 |
| 20 | 2,4-Dimethylphenol                            | 105-67-9  | XW5GK       | 99% | 1,004.2 | µg/mL | +/- 36.5341 |
| 21 | Bis(2-chloroethoxy)methane                    | 111-91-1  | 13670200    | 99% | 1,006.3 | µg/mL | +/- 36.6130 |
| 22 | 2,4-Dichlorophenol                            | 120-83-2  | BCBZ6787    | 99% | 1,004.0 | µg/mL | +/- 36.5281 |
| 23 | 1,2,4-Trichlorobenzene                        | 120-82-1  | SHBM0526    | 99% | 1,007.1 | µg/mL | +/- 36.6413 |
| 24 | Naphthalene                                   | 91-20-3   | MKCH0219    | 99% | 1,006.7 | µg/mL | +/- 36.6271 |
| 25 | 4-Chloroaniline                               | 106-47-8  | WXBC4601V   | 99% | 1,005.4 | µg/mL | +/- 36.5806 |
| 26 | Hexachlorobutadiene                           | 87-68-3   | X05J        | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 27 | 4-Chloro-3-methylphenol                       | 59-50-7   | BCCD4461    | 99% | 1,004.7 | µg/mL | +/- 36.5543 |
| 28 | 2-Methylnaphthalene                           | 91-57-6   | STBK0259    | 96% | 1,002.3 | µg/mL | +/- 36.4679 |
| 29 | 1-Methylnaphthalene                           | 90-12-0   | 5234.00-3   | 99% | 1,000.0 | µg/mL | +/- 36.3825 |
| 30 | Hexachlorocyclopentadiene                     | 77-47-4   | 0012019     | 99% | 1,006.1 | µg/mL | +/- 36.6049 |
| 31 | 2,4,6-Trichlorophenol                         | 88-06-2   | STBJ5914    | 99% | 1,004.9 | µg/mL | +/- 36.5604 |
| 32 | 2,4,5-Trichlorophenol                         | 95-95-4   | FHN01       | 98% | 1,006.5 | µg/mL | +/- 36.6176 |
| 33 | 2-Chloronaphthalene                           | 91-58-7   | RPN70       | 99% | 1,004.4 | µg/mL | +/- 36.5422 |
| 34 | 2-Nitroaniline                                | 88-74-4   | RP230509A   | 99% | 1,002.3 | µg/mL | +/- 36.4654 |
| 35 | 1,4-Dinitrobenzene                            | 100-25-4  | RP230512A   | 99% | 1,001.5 | µg/mL | +/- 36.4371 |
| 36 | Acenaphthylene                                | 208-96-8  | L10L        | 95% | 1,003.4 | µg/mL | +/- 36.5066 |
| 37 | 1,3-Dinitrobenzene                            | 99-65-0   | 1-DXX-24-1  | 99% | 1,004.8 | µg/mL | +/- 36.5564 |
| 38 | Dimethylphthalate                             | 131-11-3  | 10117699    | 99% | 1,004.7 | µg/mL | +/- 36.5543 |
| 39 | 2,6-Dinitrotoluene                            | 606-20-2  | BCCG1833    | 99% | 1,006.8 | µg/mL | +/- 36.6312 |
| 40 | 1,2-Dinitrobenzene                            | 528-29-0  | RP230428    | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 41 | Acenaphthene                                  | 83-32-9   | MKCR7169    | 99% | 1,000.0 | µg/mL | +/- 36.3825 |
| 42 | 3-Nitroaniline                                | 99-09-2   | MKCH5457    | 99% | 1,004.8 | µg/mL | +/- 36.5584 |
| 43 | 2,4-Dinitrophenol                             | 51-28-5   | DR230417RSR | 99% | 1,005.8 | µg/mL | +/- 36.5948 |
| 44 | Dibenzofuran                                  | 132-64-9  | MKCN1772    | 99% | 1,004.3 | µg/mL | +/- 36.5402 |
| 45 | 2,4-Dinitrotoluene                            | 121-14-2  | MKAA0690V   | 99% | 1,005.8 | µg/mL | +/- 36.5928 |
| 46 | 4-Nitrophenol                                 | 100-02-7  | RP230511A   | 99% | 1,005.8 | µg/mL | +/- 36.5948 |
| 47 | 2,3,4,6-Tetrachlorophenol                     | 58-90-2   | PR-30126    | 99% | 1,005.9 | µg/mL | +/- 36.5988 |
| 48 | 2,3,5,6-Tetrachlorophenol                     | 935-95-5  | RP230513    | 99% | 1,004.9 | µg/mL | +/- 36.5624 |
| 49 | Fluorene                                      | 86-73-7   | 10236068    | 99% | 1,005.4 | µg/mL | +/- 36.5806 |
| 50 | 4-Chlorophenyl phenyl ether                   | 7005-72-3 | MKCQ0984    | 99% | 1,004.3 | µg/mL | +/- 36.5382 |
| 51 | Diethylphthalate                              | 84-66-2   | BCCD3396    | 99% | 1,007.1 | µg/mL | +/- 36.6392 |
| 52 | 4-Nitroaniline                                | 100-01-6  | RP220906    | 99% | 1,005.3 | µg/mL | +/- 36.5766 |
| 53 | 4,6-Dinitro-2-methylphenol (Dinitro-o-cresol) | 534-52-1  | 230505JLM   | 99% | 1,003.8 | µg/mL | +/- 36.5200 |

|    |                            |          |              |     |         |       |             |
|----|----------------------------|----------|--------------|-----|---------|-------|-------------|
| 54 | Diphenylamine              | 122-39-4 | MKCH1042     | 99% | 1,002.5 | µg/mL | +/- 36.4735 |
| 55 | Azobenzene                 | 103-33-3 | BCCG7339     | 98% | 1,003.5 | µg/mL | +/- 36.5106 |
| 56 | 4-Bromophenyl phenyl ether | 101-55-3 | STBH6361     | 99% | 1,005.6 | µg/mL | +/- 36.5847 |
| 57 | Hexachlorobenzene          | 118-74-1 | 14257500     | 99% | 1,005.9 | µg/mL | +/- 36.5988 |
| 58 | Pentachlorophenol          | 87-86-5  | RP230504     | 99% | 1,004.2 | µg/mL | +/- 36.5362 |
| 59 | Phenanthrene               | 85-01-8  | MKCQ8876     | 99% | 1,004.1 | µg/mL | +/- 36.5321 |
| 60 | Anthracene                 | 120-12-7 | MKCR0570     | 99% | 1,008.3 | µg/mL | +/- 36.6857 |
| 61 | Carbazole                  | 86-74-8  | 14351100     | 99% | 1,005.1 | µg/mL | +/- 36.5665 |
| 62 | Di-n-butylphthalate        | 84-74-2  | MKCN4337     | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 63 | Fluoranthene               | 206-44-0 | MKCQ4728     | 99% | 1,003.7 | µg/mL | +/- 36.5159 |
| 64 | Pyrene                     | 129-00-0 | BCCG7845     | 99% | 1,004.3 | µg/mL | +/- 36.5382 |
| 65 | Benzyl butyl phthalate     | 85-68-7  | X12I018      | 99% | 1,003.4 | µg/mL | +/- 36.5058 |
| 66 | Bis(2-ethylhexyl)adipate   | 103-23-1 | MKCM1988     | 99% | 1,003.4 | µg/mL | +/- 36.5079 |
| 67 | Benz(a)anthracene          | 56-55-3  | 0012022BAA   | 97% | 1,004.9 | µg/mL | +/- 36.5624 |
| 68 | Chrysene                   | 218-01-9 | RP230512B    | 99% | 1,006.2 | µg/mL | +/- 36.6089 |
| 69 | Bis(2-ethylhexyl)phthalate | 117-81-7 | MKCQ3468     | 99% | 1,003.8 | µg/mL | +/- 36.5220 |
| 70 | Di-n-octyl phthalate       | 117-84-0 | 13994100     | 99% | 1,004.2 | µg/mL | +/- 36.5341 |
| 71 | Benzo(b)fluoranthene       | 205-99-2 | 012013B      | 99% | 1,008.4 | µg/mL | +/- 36.6877 |
| 72 | Benzo(k)fluoranthene       | 207-08-9 | 012022K      | 99% | 1,004.1 | µg/mL | +/- 36.5301 |
| 73 | Benzo(a)pyrene             | 50-32-8  | J6IUE        | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 74 | Indeno(1,2,3-cd)pyrene     | 193-39-5 | 12-JKL-118-9 | 97% | 1,002.0 | µg/mL | +/- 36.4557 |
| 75 | Dibenz(a,h)anthracene      | 53-70-3  | ER032211-01  | 99% | 1,006.1 | µg/mL | +/- 36.6029 |
| 76 | Benzo(g,h,i)perylene       | 191-24-2 | RP230511B    | 98% | 1,006.8 | µg/mL | +/- 36.6295 |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant flow 1.8 mL/min.

**Temp. Program:**

80°C (hold 0.1 min.) to 330°C  
@ 9.6°C/min. (hold 2.86 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

340°C

**Det. Type:**


FID

**Split Vent:**

100 ml/min.

**Inj. Vol**

1µl

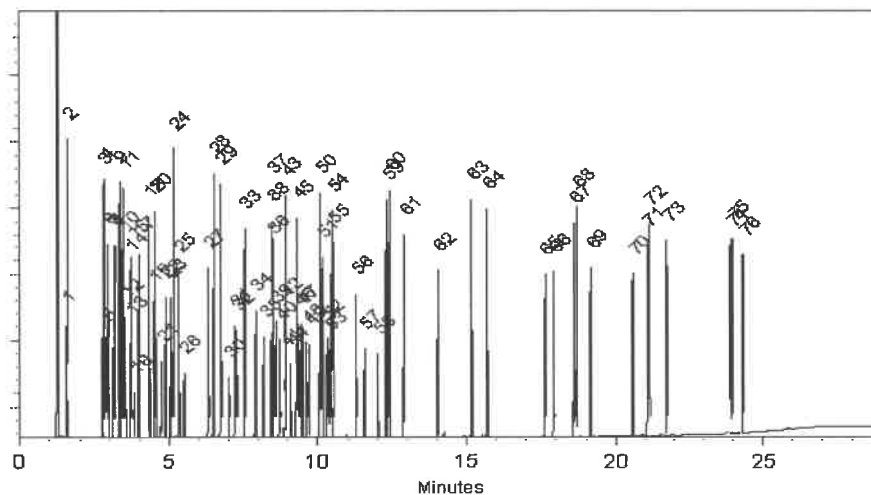

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Tom Suckar - Mix Technician

Date Mixed: 11-May-2023

Balance Serial # 1128353505

  
Christie Mills - Operations Tech II - ARM QC

Date Passed: 18-May-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



## FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 31850 Lot No.: A0197982  
Description: 8270 MegaMix®  
8270 MegaMix® 500-1,000µg/mL, Methylene Chloride, 1mL/ampul  
Container Size: 2 mL Pkg Amt: > 1 mL  
Expiration Date: November 30, 2024 Storage: 0°C or colder  
Handling: Sonication required. Mix is photosensitive. Ship: Ambient

511877  
↓  
511906  
RC/  
11/30/23

## CERTIFIED VALUES

| Elution Order | Compound                     | CAS #    | Lot #     | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------------|----------|-----------|--------|-----------------------------|--|
| 1             | Pyridine                     | 110-86-1 | SHBN7324  | 99%    | 1,006.9 µg/mL               | +/- 36.6352                            |
| 2             | N-Nitrosodimethylamine       | 62-75-9  | 230209JLM | 99%    | 1,007.4 µg/mL               | +/- 36.6514                            |
| 3             | Phenol                       | 108-95-2 | MKCK1120  | 99%    | 1,005.3 µg/mL               | +/- 36.5746                            |
| 4             | Aniline                      | 62-53-3  | X22F726   | 99%    | 1,004.6 µg/mL               | +/- 36.5503                            |
| 5             | Bis(2-chloroethyl)ether      | 111-44-4 | SHBL6942  | 99%    | 1,005.1 µg/mL               | +/- 36.5665                            |
| 6             | 2-Chlorophenol               | 95-57-8  | STBJ3909  | 99%    | 1,007.1 µg/mL               | +/- 36.6392                            |
| 7             | 1,3-Dichlorobenzene          | 541-73-1 | BCBZ7498  | 99%    | 1,006.7 µg/mL               | +/- 36.6251                            |
| 8             | 1,4-Dichlorobenzene          | 106-46-7 | MKBS7929V | 99%    | 1,005.6 µg/mL               | +/- 36.5867                            |
| 9             | Benzyl alcohol               | 100-51-6 | SHBK5943  | 99%    | 1,005.4 µg/mL               | +/- 36.5786                            |
| 10            | 1,2-Dichlorobenzene          | 95-50-1  | SHBN3835  | 99%    | 1,003.9 µg/mL               | +/- 36.5240                            |
| 11            | 2-Methylphenol (o-cresol)    | 95-48-7  | SHBN7598  | 99%    | 1,002.3 µg/mL               | +/- 36.4654                            |
| 12            | 2,2'-oxybis(1-chloropropane) | 108-60-1 | 230329JLM | 99%    | 1,004.3 µg/mL               | +/- 36.5402                            |
| 13            | 3-Methylphenol (m-cresol)    | 108-39-4 | STBJ0710  | 99%    | 502.1 µg/mL                 | +/- 18.2671                            |
| 14            | 4-Methylphenol (p-cresol)    | 106-44-5 | SHBN3411  | 99%    | 501.9 µg/mL                 | +/- 18.2631                            |
| 15            | N-Nitroso-di-n-propylamine   | 621-64-7 | N63MG     | 99%    | 1,004.0 µg/mL               | +/- 36.5281                            |
| 16            | Hexachloroethane             | 67-72-1  | QTORH     | 99%    | 1,006.1 µg/mL               | +/- 36.6029                            |
| 17            | Nitrobenzene                 | 98-95-3  | 10224044  | 99%    | 1,003.1 µg/mL               | +/- 36.4957                            |

|    |   |           |             |     |         |       |     |         |
|----|---|-----------|-------------|-----|---------|-------|-----|---------|
| 18 | Isophorone                                    | 78-59-1   | MKCC9506    | 99% | 1,003.8 | µg/mL | +/- | 36.5220 |
| 19 | 2-Nitrophenol                                 | 88-75-5   | RP230509C   | 99% | 1,005.8 | µg/mL | +/- | 36.5948 |
| 20 | 2,4-Dimethylphenol                            | 105-67-9  | XW5GK       | 99% | 1,004.2 | µg/mL | +/- | 36.5341 |
| 21 | Bis(2-chloroethoxy)methane                    | 111-91-1  | 13670200    | 99% | 1,006.3 | µg/mL | +/- | 36.6130 |
| 22 | 2,4-Dichlorophenol                            | 120-83-2  | BCBZ6787    | 99% | 1,004.0 | µg/mL | +/- | 36.5281 |
| 23 | 1,2,4-Trichlorobenzene                        | 120-82-1  | SHBM0526    | 99% | 1,007.1 | µg/mL | +/- | 36.6413 |
| 24 | Naphthalene                                   | 91-20-3   | MKCH0219    | 99% | 1,006.7 | µg/mL | +/- | 36.6271 |
| 25 | 4-Chloroaniline                               | 106-47-8  | WXBC4601V   | 99% | 1,005.4 | µg/mL | +/- | 36.5806 |
| 26 | Hexachlorobutadiene                           | 87-68-3   | X05J        | 99% | 1,006.4 | µg/mL | +/- | 36.6170 |
| 27 | 4-Chloro-3-methylphenol                       | 59-50-7   | BCCD4461    | 99% | 1,004.7 | µg/mL | +/- | 36.5543 |
| 28 | 2-Methylnaphthalene                           | 91-57-6   | STBK0259    | 96% | 1,002.3 | µg/mL | +/- | 36.4679 |
| 29 | 1-Methylnaphthalene                           | 90-12-0   | 5234.00-3   | 99% | 1,000.0 | µg/mL | +/- | 36.3825 |
| 30 | Hexachlorocyclopentadiene                     | 77-47-4   | 0012019     | 99% | 1,006.1 | µg/mL | +/- | 36.6049 |
| 31 | 2,4,6-Trichlorophenol                         | 88-06-2   | STBJ5914    | 99% | 1,004.9 | µg/mL | +/- | 36.5604 |
| 32 | 2,4,5-Trichlorophenol                         | 95-95-4   | FHN01       | 98% | 1,006.5 | µg/mL | +/- | 36.6176 |
| 33 | 2-Chloronaphthalene                           | 91-58-7   | RPN70       | 99% | 1,004.4 | µg/mL | +/- | 36.5422 |
| 34 | 2-Nitroaniline                                | 88-74-4   | RP230509A   | 99% | 1,002.3 | µg/mL | +/- | 36.4654 |
| 35 | 1,4-Dinitrobenzene                            | 100-25-4  | RP230512A   | 99% | 1,001.5 | µg/mL | +/- | 36.4371 |
| 36 | Acenaphthylene                                | 208-96-8  | L10L        | 95% | 1,003.4 | µg/mL | +/- | 36.5066 |
| 37 | 1,3-Dinitrobenzene                            | 99-65-0   | 1-DXX-24-1  | 99% | 1,004.8 | µg/mL | +/- | 36.5564 |
| 38 | Dimethylphthalate                             | 131-11-3  | 10117699    | 99% | 1,004.7 | µg/mL | +/- | 36.5543 |
| 39 | 2,6-Dinitrotoluene                            | 606-20-2  | BCCG1833    | 99% | 1,006.8 | µg/mL | +/- | 36.6312 |
| 40 | 1,2-Dinitrobenzene                            | 528-29-0  | RP230428    | 99% | 1,006.4 | µg/mL | +/- | 36.6170 |
| 41 | Acenaphthene                                  | 83-32-9   | MKCR7169    | 99% | 1,000.0 | µg/mL | +/- | 36.3825 |
| 42 | 3-Nitroaniline                                | 99-09-2   | MKCH5457    | 99% | 1,004.8 | µg/mL | +/- | 36.5584 |
| 43 | 2,4-Dinitrophenol                             | 51-28-5   | DR230417RSR | 99% | 1,005.8 | µg/mL | +/- | 36.5948 |
| 44 | Dibenzofuran                                  | 132-64-9  | MKCN1772    | 99% | 1,004.3 | µg/mL | +/- | 36.5402 |
| 45 | 2,4-Dinitrotoluene                            | 121-14-2  | MKAA0690V   | 99% | 1,005.8 | µg/mL | +/- | 36.5928 |
| 46 | 4-Nitrophenol                                 | 100-02-7  | RP230511A   | 99% | 1,005.8 | µg/mL | +/- | 36.5948 |
| 47 | 2,3,4,6-Tetrachlorophenol                     | 58-90-2   | PR-30126    | 99% | 1,005.9 | µg/mL | +/- | 36.5988 |
| 48 | 2,3,5,6-Tetrachlorophenol                     | 935-95-5  | RP230513    | 99% | 1,004.9 | µg/mL | +/- | 36.5624 |
| 49 | Fluorene                                      | 86-73-7   | 10236068    | 99% | 1,005.4 | µg/mL | +/- | 36.5806 |
| 50 | 4-Chlorophenyl phenyl ether                   | 7005-72-3 | MKCQ0984    | 99% | 1,004.3 | µg/mL | +/- | 36.5382 |
| 51 | Diethylphthalate                              | 84-66-2   | BCCD3396    | 99% | 1,007.1 | µg/mL | +/- | 36.6392 |
| 52 | 4-Nitroaniline                                | 100-01-6  | RP220906    | 99% | 1,005.3 | µg/mL | +/- | 36.5766 |
| 53 | 4,6-Dinitro-2-methylphenol (Dinitro-o-cresol) | 534-52-1  | 230505JLM   | 99% | 1,003.8 | µg/mL | +/- | 36.5200 |



|    |                            |          |              |     |         |       |             |
|----|----------------------------|----------|--------------|-----|---------|-------|-------------|
| 54 | Diphenylamine              | 122-39-4 | MKCH1042     | 99% | 1,002.5 | µg/mL | +/- 36.4735 |
| 55 | Azobenzene                 | 103-33-3 | BCCG7339     | 98% | 1,003.5 | µg/mL | +/- 36.5106 |
| 56 | 4-Bromophenyl phenyl ether | 101-55-3 | STBH6361     | 99% | 1,005.6 | µg/mL | +/- 36.5847 |
| 57 | Hexachlorobenzene          | 118-74-1 | 14257500     | 99% | 1,005.9 | µg/mL | +/- 36.5988 |
| 58 | Pentachlorophenol          | 87-86-5  | RP230504     | 99% | 1,004.2 | µg/mL | +/- 36.5362 |
| 59 | Phenanthrene               | 85-01-8  | MKCQ8876     | 99% | 1,004.1 | µg/mL | +/- 36.5321 |
| 60 | Anthracene                 | 120-12-7 | MKCR0570     | 99% | 1,008.3 | µg/mL | +/- 36.6857 |
| 61 | Carbazole                  | 86-74-8  | 14351100     | 99% | 1,005.1 | µg/mL | +/- 36.5665 |
| 62 | Di-n-butylphthalate        | 84-74-2  | MKCN4337     | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 63 | Fluoranthene               | 206-44-0 | MKCQ4728     | 99% | 1,003.7 | µg/mL | +/- 36.5159 |
| 64 | Pyrene                     | 129-00-0 | BCCG7845     | 99% | 1,004.3 | µg/mL | +/- 36.5382 |
| 65 | Benzyl butyl phthalate     | 85-68-7  | X12I018      | 99% | 1,003.4 | µg/mL | +/- 36.5058 |
| 66 | Bis(2-ethylhexyl)adipate   | 103-23-1 | MKCM1988     | 99% | 1,003.4 | µg/mL | +/- 36.5079 |
| 67 | Benz(a)anthracene          | 56-55-3  | 0012022BAA   | 97% | 1,004.9 | µg/mL | +/- 36.5624 |
| 68 | Chrysene                   | 218-01-9 | RP230512B    | 99% | 1,006.2 | µg/mL | +/- 36.6089 |
| 69 | Bis(2-ethylhexyl)phthalate | 117-81-7 | MKCQ3468     | 99% | 1,003.8 | µg/mL | +/- 36.5220 |
| 70 | Di-n-octyl phthalate       | 117-84-0 | 13994100     | 99% | 1,004.2 | µg/mL | +/- 36.5341 |
| 71 | Benzo(b)fluoranthene       | 205-99-2 | 012013B      | 99% | 1,008.4 | µg/mL | +/- 36.6877 |
| 72 | Benzo(k)fluoranthene       | 207-08-9 | 012022K      | 99% | 1,004.1 | µg/mL | +/- 36.5301 |
| 73 | Benzo(a)pyrene             | 50-32-8  | J6IUE        | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 74 | Indeno(1,2,3-cd)pyrene     | 193-39-5 | 12-JKL-118-9 | 97% | 1,002.0 | µg/mL | +/- 36.4557 |
| 75 | Dibenz(a,h)anthracene      | 53-70-3  | ER032211-01  | 99% | 1,006.1 | µg/mL | +/- 36.6029 |
| 76 | Benzo(g,h,i)perylene       | 191-24-2 | RP230511B    | 98% | 1,006.8 | µg/mL | +/- 36.6295 |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant flow 1.8 mL/min.

**Temp. Program:**

80°C (hold 0.1 min.) to 330°C  
@ 9.6°C/min. (hold 2.86 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

340°C

**Det. Type:**


FID

**Split Vent:**

100 ml/min.

**Inj. Vol**

1µl

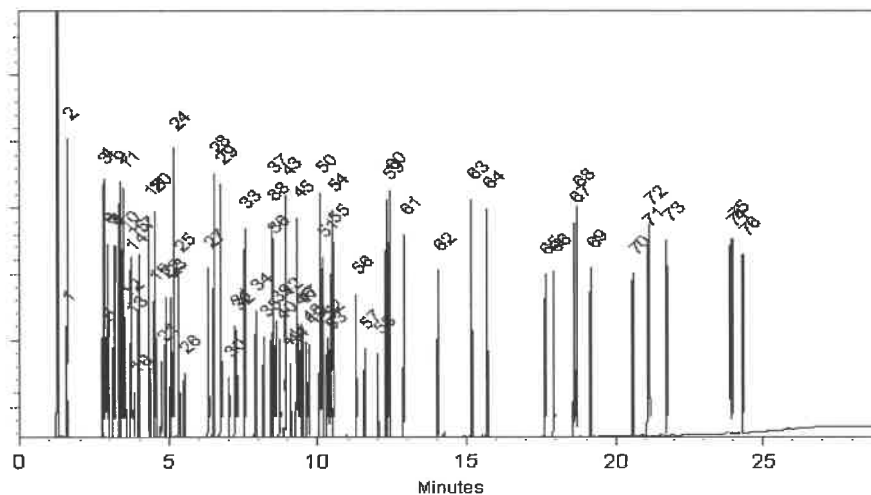

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Tom Suckar - Mix Technician

Date Mixed: 11-May-2023

Balance Serial # 1128353505

  
Christie Mills - Operations Tech II - ARM QC

Date Passed: 18-May-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

## Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 31850 Lot No.: A0197982  
Description: 8270 MegaMix®  
8270 MegaMix® 500-1,000µg/mL, Methylene Chloride, 1mL/ampul  
Container Size: 2 mL Pkg Amt: > 1 mL  
Expiration Date: November 30, 2024 Storage: 0°C or colder  
Handling: Sonication required. Mix is photosensitive. Ship: Ambient

511877  
↓  
511906  
RC/  
11/30/23

### CERTIFIED VALUES

| Elution Order | Compound                     | CAS #    | Lot #     | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------------|----------|-----------|--------|-----------------------------|--|
| 1             | Pyridine                     | 110-86-1 | SHBN7324  | 99%    | 1,006.9 µg/mL               | +/- 36.6352                            |
| 2             | N-Nitrosodimethylamine       | 62-75-9  | 230209JLM | 99%    | 1,007.4 µg/mL               | +/- 36.6514                            |
| 3             | Phenol                       | 108-95-2 | MKCK1120  | 99%    | 1,005.3 µg/mL               | +/- 36.5746                            |
| 4             | Aniline                      | 62-53-3  | X22F726   | 99%    | 1,004.6 µg/mL               | +/- 36.5503                            |
| 5             | Bis(2-chloroethyl)ether      | 111-44-4 | SHBL6942  | 99%    | 1,005.1 µg/mL               | +/- 36.5665                            |
| 6             | 2-Chlorophenol               | 95-57-8  | STBJ3909  | 99%    | 1,007.1 µg/mL               | +/- 36.6392                            |
| 7             | 1,3-Dichlorobenzene          | 541-73-1 | BCBZ7498  | 99%    | 1,006.7 µg/mL               | +/- 36.6251                            |
| 8             | 1,4-Dichlorobenzene          | 106-46-7 | MKBS7929V | 99%    | 1,005.6 µg/mL               | +/- 36.5867                            |
| 9             | Benzyl alcohol               | 100-51-6 | SHBK5943  | 99%    | 1,005.4 µg/mL               | +/- 36.5786                            |
| 10            | 1,2-Dichlorobenzene          | 95-50-1  | SHBN3835  | 99%    | 1,003.9 µg/mL               | +/- 36.5240                            |
| 11            | 2-Methylphenol (o-cresol)    | 95-48-7  | SHBN7598  | 99%    | 1,002.3 µg/mL               | +/- 36.4654                            |
| 12            | 2,2'-oxybis(1-chloropropane) | 108-60-1 | 230329JLM | 99%    | 1,004.3 µg/mL               | +/- 36.5402                            |
| 13            | 3-Methylphenol (m-cresol)    | 108-39-4 | STBJ0710  | 99%    | 502.1 µg/mL                 | +/- 18.2671                            |
| 14            | 4-Methylphenol (p-cresol)    | 106-44-5 | SHBN3411  | 99%    | 501.9 µg/mL                 | +/- 18.2631                            |
| 15            | N-Nitroso-di-n-propylamine   | 621-64-7 | N63MG     | 99%    | 1,004.0 µg/mL               | +/- 36.5281                            |
| 16            | Hexachloroethane             | 67-72-1  | QTORH     | 99%    | 1,006.1 µg/mL               | +/- 36.6029                            |
| 17            | Nitrobenzene                 | 98-95-3  | 10224044  | 99%    | 1,003.1 µg/mL               | +/- 36.4957                            |

|    |   |           |             |     |         |       |             |
|----|---|-----------|-------------|-----|---------|-------|-------------|
| 18 | Isophorone                                    | 78-59-1   | MKCC9506    | 99% | 1,003.8 | µg/mL | +/- 36.5220 |
| 19 | 2-Nitrophenol                                 | 88-75-5   | RP230509C   | 99% | 1,005.8 | µg/mL | +/- 36.5948 |
| 20 | 2,4-Dimethylphenol                            | 105-67-9  | XW5GK       | 99% | 1,004.2 | µg/mL | +/- 36.5341 |
| 21 | Bis(2-chloroethoxy)methane                    | 111-91-1  | 13670200    | 99% | 1,006.3 | µg/mL | +/- 36.6130 |
| 22 | 2,4-Dichlorophenol                            | 120-83-2  | BCBZ6787    | 99% | 1,004.0 | µg/mL | +/- 36.5281 |
| 23 | 1,2,4-Trichlorobenzene                        | 120-82-1  | SHBM0526    | 99% | 1,007.1 | µg/mL | +/- 36.6413 |
| 24 | Naphthalene                                   | 91-20-3   | MKCH0219    | 99% | 1,006.7 | µg/mL | +/- 36.6271 |
| 25 | 4-Chloroaniline                               | 106-47-8  | WXBC4601V   | 99% | 1,005.4 | µg/mL | +/- 36.5806 |
| 26 | Hexachlorobutadiene                           | 87-68-3   | X05J        | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 27 | 4-Chloro-3-methylphenol                       | 59-50-7   | BCCD4461    | 99% | 1,004.7 | µg/mL | +/- 36.5543 |
| 28 | 2-Methylnaphthalene                           | 91-57-6   | STBK0259    | 96% | 1,002.3 | µg/mL | +/- 36.4679 |
| 29 | 1-Methylnaphthalene                           | 90-12-0   | 5234.00-3   | 99% | 1,000.0 | µg/mL | +/- 36.3825 |
| 30 | Hexachlorocyclopentadiene                     | 77-47-4   | 0012019     | 99% | 1,006.1 | µg/mL | +/- 36.6049 |
| 31 | 2,4,6-Trichlorophenol                         | 88-06-2   | STBJ5914    | 99% | 1,004.9 | µg/mL | +/- 36.5604 |
| 32 | 2,4,5-Trichlorophenol                         | 95-95-4   | FHN01       | 98% | 1,006.5 | µg/mL | +/- 36.6176 |
| 33 | 2-Chloronaphthalene                           | 91-58-7   | RPN70       | 99% | 1,004.4 | µg/mL | +/- 36.5422 |
| 34 | 2-Nitroaniline                                | 88-74-4   | RP230509A   | 99% | 1,002.3 | µg/mL | +/- 36.4654 |
| 35 | 1,4-Dinitrobenzene                            | 100-25-4  | RP230512A   | 99% | 1,001.5 | µg/mL | +/- 36.4371 |
| 36 | Acenaphthylene                                | 208-96-8  | L10L        | 95% | 1,003.4 | µg/mL | +/- 36.5066 |
| 37 | 1,3-Dinitrobenzene                            | 99-65-0   | 1-DXX-24-1  | 99% | 1,004.8 | µg/mL | +/- 36.5564 |
| 38 | Dimethylphthalate                             | 131-11-3  | 10117699    | 99% | 1,004.7 | µg/mL | +/- 36.5543 |
| 39 | 2,6-Dinitrotoluene                            | 606-20-2  | BCCG1833    | 99% | 1,006.8 | µg/mL | +/- 36.6312 |
| 40 | 1,2-Dinitrobenzene                            | 528-29-0  | RP230428    | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 41 | Acenaphthene                                  | 83-32-9   | MKCR7169    | 99% | 1,000.0 | µg/mL | +/- 36.3825 |
| 42 | 3-Nitroaniline                                | 99-09-2   | MKCH5457    | 99% | 1,004.8 | µg/mL | +/- 36.5584 |
| 43 | 2,4-Dinitrophenol                             | 51-28-5   | DR230417RSR | 99% | 1,005.8 | µg/mL | +/- 36.5948 |
| 44 | Dibenzofuran                                  | 132-64-9  | MKCN1772    | 99% | 1,004.3 | µg/mL | +/- 36.5402 |
| 45 | 2,4-Dinitrotoluene                            | 121-14-2  | MKAA0690V   | 99% | 1,005.8 | µg/mL | +/- 36.5928 |
| 46 | 4-Nitrophenol                                 | 100-02-7  | RP230511A   | 99% | 1,005.8 | µg/mL | +/- 36.5948 |
| 47 | 2,3,4,6-Tetrachlorophenol                     | 58-90-2   | PR-30126    | 99% | 1,005.9 | µg/mL | +/- 36.5988 |
| 48 | 2,3,5,6-Tetrachlorophenol                     | 935-95-5  | RP230513    | 99% | 1,004.9 | µg/mL | +/- 36.5624 |
| 49 | Fluorene                                      | 86-73-7   | 10236068    | 99% | 1,005.4 | µg/mL | +/- 36.5806 |
| 50 | 4-Chlorophenyl phenyl ether                   | 7005-72-3 | MKCQ0984    | 99% | 1,004.3 | µg/mL | +/- 36.5382 |
| 51 | Diethylphthalate                              | 84-66-2   | BCCD3396    | 99% | 1,007.1 | µg/mL | +/- 36.6392 |
| 52 | 4-Nitroaniline                                | 100-01-6  | RP220906    | 99% | 1,005.3 | µg/mL | +/- 36.5766 |
| 53 | 4,6-Dinitro-2-methylphenol (Dinitro-o-cresol) | 534-52-1  | 230505JLM   | 99% | 1,003.8 | µg/mL | +/- 36.5200 |

|    |                            |          |              |     |         |       |             |
|----|----------------------------|----------|--------------|-----|---------|-------|-------------|
| 54 | Diphenylamine              | 122-39-4 | MKCH1042     | 99% | 1,002.5 | µg/mL | +/- 36.4735 |
| 55 | Azobenzene                 | 103-33-3 | BCCG7339     | 98% | 1,003.5 | µg/mL | +/- 36.5106 |
| 56 | 4-Bromophenyl phenyl ether | 101-55-3 | STBH6361     | 99% | 1,005.6 | µg/mL | +/- 36.5847 |
| 57 | Hexachlorobenzene          | 118-74-1 | 14257500     | 99% | 1,005.9 | µg/mL | +/- 36.5988 |
| 58 | Pentachlorophenol          | 87-86-5  | RP230504     | 99% | 1,004.2 | µg/mL | +/- 36.5362 |
| 59 | Phenanthrene               | 85-01-8  | MKCQ8876     | 99% | 1,004.1 | µg/mL | +/- 36.5321 |
| 60 | Anthracene                 | 120-12-7 | MKCR0570     | 99% | 1,008.3 | µg/mL | +/- 36.6857 |
| 61 | Carbazole                  | 86-74-8  | 14351100     | 99% | 1,005.1 | µg/mL | +/- 36.5665 |
| 62 | Di-n-butylphthalate        | 84-74-2  | MKCN4337     | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 63 | Fluoranthene               | 206-44-0 | MKCQ4728     | 99% | 1,003.7 | µg/mL | +/- 36.5159 |
| 64 | Pyrene                     | 129-00-0 | BCCG7845     | 99% | 1,004.3 | µg/mL | +/- 36.5382 |
| 65 | Benzyl butyl phthalate     | 85-68-7  | X12I018      | 99% | 1,003.4 | µg/mL | +/- 36.5058 |
| 66 | Bis(2-ethylhexyl)adipate   | 103-23-1 | MKCM1988     | 99% | 1,003.4 | µg/mL | +/- 36.5079 |
| 67 | Benz(a)anthracene          | 56-55-3  | 0012022BAA   | 97% | 1,004.9 | µg/mL | +/- 36.5624 |
| 68 | Chrysene                   | 218-01-9 | RP230512B    | 99% | 1,006.2 | µg/mL | +/- 36.6089 |
| 69 | Bis(2-ethylhexyl)phthalate | 117-81-7 | MKCQ3468     | 99% | 1,003.8 | µg/mL | +/- 36.5220 |
| 70 | Di-n-octyl phthalate       | 117-84-0 | 13994100     | 99% | 1,004.2 | µg/mL | +/- 36.5341 |
| 71 | Benzo(b)fluoranthene       | 205-99-2 | 012013B      | 99% | 1,008.4 | µg/mL | +/- 36.6877 |
| 72 | Benzo(k)fluoranthene       | 207-08-9 | 012022K      | 99% | 1,004.1 | µg/mL | +/- 36.5301 |
| 73 | Benzo(a)pyrene             | 50-32-8  | J6IUE        | 99% | 1,006.4 | µg/mL | +/- 36.6170 |
| 74 | Indeno(1,2,3-cd)pyrene     | 193-39-5 | 12-JKL-118-9 | 97% | 1,002.0 | µg/mL | +/- 36.4557 |
| 75 | Dibenz(a,h)anthracene      | 53-70-3  | ER032211-01  | 99% | 1,006.1 | µg/mL | +/- 36.6029 |
| 76 | Benzo(g,h,i)perylene       | 191-24-2 | RP230511B    | 98% | 1,006.8 | µg/mL | +/- 36.6295 |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant flow 1.8 mL/min.

**Temp. Program:**

80°C (hold 0.1 min.) to 330°C  
@ 9.6°C/min. (hold 2.86 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

340°C

**Det. Type:**


FID

**Split Vent:**

100 ml/min.

**Inj. Vol**

1µl

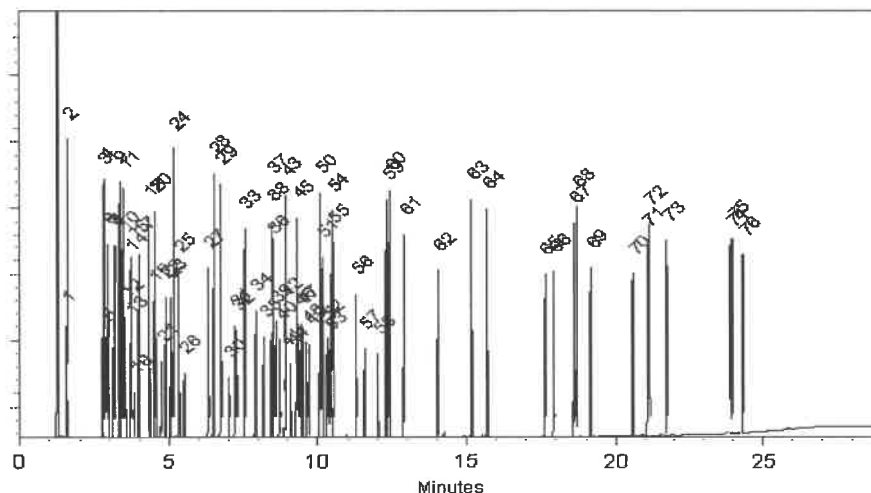

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Tom Suckar - Mix Technician

Date Mixed: 11-May-2023

Balance Serial # 1128353505

  
Christie Mills - Operations Tech II - ARM QC

Date Passed: 18-May-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31206 **Lot No.:** A0201320

**Description :** SV Internal Standard Mix 2mg/ml  
SV Internal Standard Mix 2mg/ml 2000 µg/ml, Methylene Chloride,  
1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** July 31, 2029 **Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

S12013  
↓  
S12042 } RC  
12/26/23

### CERTIFIED VALUES

| Elution Order | Compound               | CAS #      | Lot #    | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------|------------|----------|--------|-----------------------------|--|
| 1             | 1,4-Dichlorobenzene-d4 | 3855-82-1  | PR-30447 | 99%    | 2,017.0 µg/mL               | +/- 90.8469                            |
| 2             | Naphthalene-d8         | 1146-65-2  | M-2180   | 99%    | 2,011.3 µg/mL               | +/- 90.5917                            |
| 3             | Acenaphthene-d10       | 15067-26-2 | PR-33507 | 99%    | 2,008.6 µg/mL               | +/- 90.4685                            |
| 4             | Phenanthrene-d10       | 1517-22-2  | PR-32303 | 99%    | 2,019.4 µg/mL               | +/- 90.9550                            |
| 5             | Chrysene-d12           | 1719-03-5  | PR-32210 | 99%    | 2,013.7 µg/mL               | +/- 90.6968                            |
| 6             | Perylene-d12           | 1520-96-3  | PR-33205 | 99%    | 2,012.7 µg/mL               | +/- 90.6517                            |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

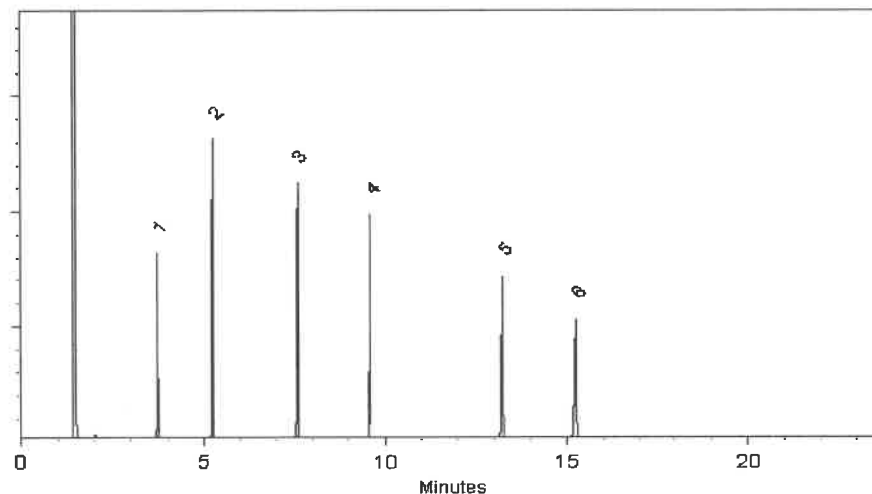

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Peter Robbins - Operations Technician I

Date Mixed: 23-Aug-2023

Balance Serial # B345965662

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 25-Aug-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31206 **Lot No.:** A0201320

**Description :** SV Internal Standard Mix 2mg/ml  
SV Internal Standard Mix 2mg/ml 2000 µg/ml, Methylene Chloride,  
1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** July 31, 2029 **Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

S12013  
↓  
S12042 } RC  
12/26/23

### CERTIFIED VALUES

| Elution Order | Compound               | CAS #      | Lot #    | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------|------------|----------|--------|-----------------------------|--|
| 1             | 1,4-Dichlorobenzene-d4 | 3855-82-1  | PR-30447 | 99%    | 2,017.0 µg/mL               | +/- 90.8469                            |
| 2             | Naphthalene-d8         | 1146-65-2  | M-2180   | 99%    | 2,011.3 µg/mL               | +/- 90.5917                            |
| 3             | Acenaphthene-d10       | 15067-26-2 | PR-33507 | 99%    | 2,008.6 µg/mL               | +/- 90.4685                            |
| 4             | Phenanthrene-d10       | 1517-22-2  | PR-32303 | 99%    | 2,019.4 µg/mL               | +/- 90.9550                            |
| 5             | Chrysene-d12           | 1719-03-5  | PR-32210 | 99%    | 2,013.7 µg/mL               | +/- 90.6968                            |
| 6             | Perylene-d12           | 1520-96-3  | PR-33205 | 99%    | 2,012.7 µg/mL               | +/- 90.6517                            |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

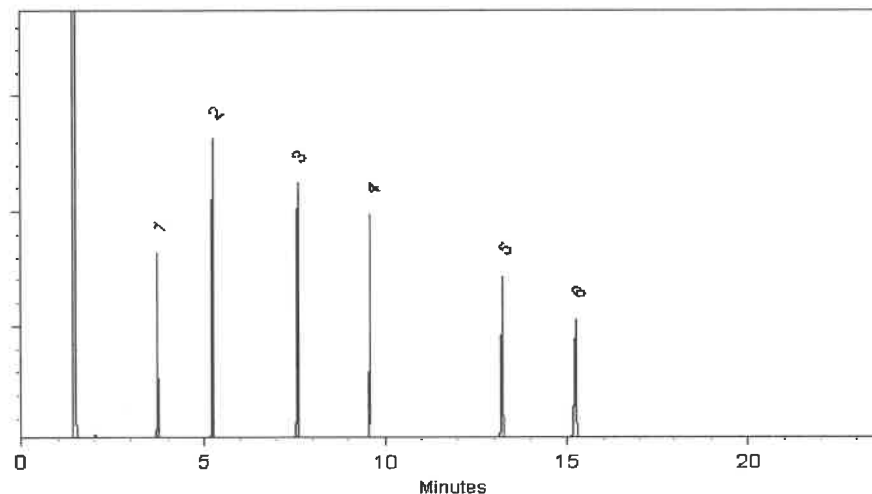

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Peter Robbins - Operations Technician I

Date Mixed: 23-Aug-2023

Balance Serial # B345965662

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 25-Aug-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31206 **Lot No.:** A0201320

**Description :** SV Internal Standard Mix 2mg/ml  
SV Internal Standard Mix 2mg/ml 2000 µg/ml, Methylene Chloride,  
1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** July 31, 2029 **Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

S12013  
↓  
S12042 } RC  
12/26/23

### CERTIFIED VALUES

| Elution Order | Compound               | CAS #      | Lot #    | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------|------------|----------|--------|-----------------------------|--|
| 1             | 1,4-Dichlorobenzene-d4 | 3855-82-1  | PR-30447 | 99%    | 2,017.0 µg/mL               | +/- 90.8469                            |
| 2             | Naphthalene-d8         | 1146-65-2  | M-2180   | 99%    | 2,011.3 µg/mL               | +/- 90.5917                            |
| 3             | Acenaphthene-d10       | 15067-26-2 | PR-33507 | 99%    | 2,008.6 µg/mL               | +/- 90.4685                            |
| 4             | Phenanthrene-d10       | 1517-22-2  | PR-32303 | 99%    | 2,019.4 µg/mL               | +/- 90.9550                            |
| 5             | Chrysene-d12           | 1719-03-5  | PR-32210 | 99%    | 2,013.7 µg/mL               | +/- 90.6968                            |
| 6             | Perylene-d12           | 1520-96-3  | PR-33205 | 99%    | 2,012.7 µg/mL               | +/- 90.6517                            |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

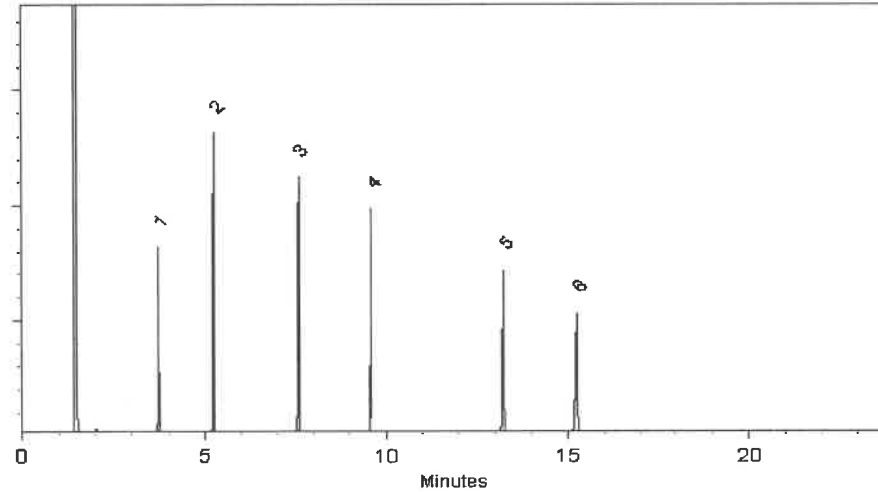

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Peter Robbins - Operations Technician I

Date Mixed: 23-Aug-2023

Balance Serial # B345965662

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 25-Aug-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



5580 Skylane Blvd  
Santa Rosa, CA 95403

(707)525-5788  
(800)878-7654 Toll Free  
(707)545-7901 Fax

Manufacturer's Quality System  
Audited & Registered  
by TUV USA to ISO 9001:2015

Date Received: \_\_\_\_\_

## Certificate of Analysis

Rev 0

Page 1 of 1

|                     |                 |                 |                    |                   |   |
|---------------------|-----------------|-----------------|--------------------|-------------------|---|
| <b>Catalog No.:</b> | <b>Lot No.:</b> | <b>Storage:</b> | <b>Solvent:</b>    | <b>Exp. Date:</b> | <b>Description:</b>                       |
| Z-110816-01         | 414127          | ≤ -10 °C        | Methylene Chloride | 6/21/2025         | Custom 8270 Mix, 4-79,<br>1000 mg/L, 1 mL |

| Compound    | CAS No.   | Purity (%) | Compound Lot No. | Concentration, mg/L |
|-------------|-----------|------------|------------------|---------------------|
| atrazine    | 1912-24-9 | 99.5       | 337.7.3P         | 997 ± 5.81          |
| benzidine   | 92-87-5   | 99.9       | 124.18.6.2P      | 991.8 ± 5.77        |
| caprolactam | 105-60-2  | 99.9       | 271.1.6P         | 999 ± 5.82          |

912075 } RC  
↓  
912079 } 02/01/24

\*Not a certified value

Manufactured by o2si smart solutions, Accredited to ISO 9001:2008 by NSF and ISO/IEC 17025:2005 (Certification No. 3031.01) and ISO Guide 34:2009 (Certification No. 3031.02) by A2LA

Certified By: \_\_\_\_\_

Shane Overcash  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values listed are determined gravimetrically.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 555224 **Lot No.:** A0207706

**Description :** Custom 8270 Plus Standard #2

Custom 8270 Plus Standard #2 1,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** February 28, 2026 **Storage:** 10°C or colder

**Ship:** Ambient

512082 } RC/  
↓  
512111 } 02/22/24

## CERTIFIED VALUES

| Component # | Compound                   | CAS #    | Lot #        | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|-------------|----------------------------|----------|--------------|--------|-----------------------------|--|
| 1           | 1,2,4,5-Tetrachlorobenzene | 95-94-3  | MKCT9480     | 99%    | 1,001.0 µg/mL               | +/- 29.424320                          |
| 2           | Acetophenone               | 98-86-2  | STBH8205     | 99%    | 1,004.0 µg/mL               | +/- 29.512504                          |
| 3           | Benzaldehyde               | 100-52-7 | RD231129RSRA | 99%    | 1,005.0 µg/mL               | +/- 29.541899                          |
| 4           | Benzoic acid               | 65-85-0  | MKCR2694     | 99%    | 1,003.0 µg/mL               | +/- 29.483110                          |
| 5           | Biphenyl                   | 92-52-4  | MKCL6515     | 99%    | 1,006.0 µg/mL               | +/- 29.571294                          |

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

John Friedline - Operations Technician I

Date Mixed: 12-Feb-2024

Balance: B345965662



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 555224 **Lot No.:** A0207706

**Description :** Custom 8270 Plus Standard #2

Custom 8270 Plus Standard #2 1,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** February 28, 2026 **Storage:** 10°C or colder

**Ship:** Ambient

512082 } RC/  
↓  
512111 } 02/22/24

## CERTIFIED VALUES

| Component # | Compound                   | CAS #    | Lot #        | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|-------------|----------------------------|----------|--------------|--------|-----------------------------|--|
| 1           | 1,2,4,5-Tetrachlorobenzene | 95-94-3  | MKCT9480     | 99%    | 1,001.0 µg/mL               | +/- 29.424320                          |
| 2           | Acetophenone               | 98-86-2  | STBH8205     | 99%    | 1,004.0 µg/mL               | +/- 29.512504                          |
| 3           | Benzaldehyde               | 100-52-7 | RD231129RSRA | 99%    | 1,005.0 µg/mL               | +/- 29.541899                          |
| 4           | Benzoic acid               | 65-85-0  | MKCR2694     | 99%    | 1,003.0 µg/mL               | +/- 29.483110                          |
| 5           | Biphenyl                   | 92-52-4  | MKCL6515     | 99%    | 1,006.0 µg/mL               | +/- 29.571294                          |

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

John Friedline - Operations Technician I

Date Mixed: 12-Feb-2024

Balance: B345965662



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 555224 **Lot No.:** A0207706

**Description :** Custom 8270 Plus Standard #2

Custom 8270 Plus Standard #2 1,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** February 28, 2026 **Storage:** 10°C or colder

**Ship:** Ambient

512082 } RC/  
↓  
512111 } 02/22/24

## CERTIFIED VALUES

| Component # | Compound                   | CAS #    | Lot #        | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|-------------|----------------------------|----------|--------------|--------|-----------------------------|--|
| 1           | 1,2,4,5-Tetrachlorobenzene | 95-94-3  | MKCT9480     | 99%    | 1,001.0 µg/mL               | +/- 29.424320                          |
| 2           | Acetophenone               | 98-86-2  | STBH8205     | 99%    | 1,004.0 µg/mL               | +/- 29.512504                          |
| 3           | Benzaldehyde               | 100-52-7 | RD231129RSRA | 99%    | 1,005.0 µg/mL               | +/- 29.541899                          |
| 4           | Benzoic acid               | 65-85-0  | MKCR2694     | 99%    | 1,003.0 µg/mL               | +/- 29.483110                          |
| 5           | Biphenyl                   | 92-52-4  | MKCL6515     | 99%    | 1,006.0 µg/mL               | +/- 29.571294                          |

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

John Friedline - Operations Technician I

Date Mixed: 12-Feb-2024

Balance: B345965662





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 555224 **Lot No.:** A0207706

**Description :** Custom 8270 Plus Standard #2

Custom 8270 Plus Standard #2 1,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** February 28, 2026 **Storage:** 10°C or colder

**Ship:** Ambient

512082 } RC/  
↓  
512111 } 02/22/24

## CERTIFIED VALUES

| Component # | Compound                   | CAS #    | Lot #        | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|-------------|----------------------------|----------|--------------|--------|-----------------------------|--|
| 1           | 1,2,4,5-Tetrachlorobenzene | 95-94-3  | MKCT9480     | 99%    | 1,001.0 µg/mL               | +/- 29.424320                          |
| 2           | Acetophenone               | 98-86-2  | STBH8205     | 99%    | 1,004.0 µg/mL               | +/- 29.512504                          |
| 3           | Benzaldehyde               | 100-52-7 | RD231129RSRA | 99%    | 1,005.0 µg/mL               | +/- 29.541899                          |
| 4           | Benzoic acid               | 65-85-0  | MKCR2694     | 99%    | 1,003.0 µg/mL               | +/- 29.483110                          |
| 5           | Biphenyl                   | 92-52-4  | MKCL6515     | 99%    | 1,006.0 µg/mL               | +/- 29.571294                          |

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

John Friedline - Operations Technician I

Date Mixed: 12-Feb-2024

Balance: B345965662



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

gravimetric



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 555224 **Lot No.:** A0207706

**Description :** Custom 8270 Plus Standard #2

Custom 8270 Plus Standard #2 1,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** February 28, 2026 **Storage:** 10°C or colder

**Ship:** Ambient

512082 } RC/  
↓  
512111 } 02/22/24

### CERTIFIED VALUES

| Component # | Compound                   | CAS #    | Lot #        | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|-------------|----------------------------|----------|--------------|--------|-----------------------------|--|
| 1           | 1,2,4,5-Tetrachlorobenzene | 95-94-3  | MKCT9480     | 99%    | 1,001.0 µg/mL               | +/- 29.424320                          |
| 2           | Acetophenone               | 98-86-2  | STBH8205     | 99%    | 1,004.0 µg/mL               | +/- 29.512504                          |
| 3           | Benzaldehyde               | 100-52-7 | RD231129RSRA | 99%    | 1,005.0 µg/mL               | +/- 29.541899                          |
| 4           | Benzoic acid               | 65-85-0  | MKCR2694     | 99%    | 1,003.0 µg/mL               | +/- 29.483110                          |
| 5           | Biphenyl                   | 92-52-4  | MKCL6515     | 99%    | 1,006.0 µg/mL               | +/- 29.571294                          |

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

John Friedline - Operations Technician I

Date Mixed: 12-Feb-2024

Balance: B345965662



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 555224 **Lot No.:** A0207706

**Description :** Custom 8270 Plus Standard #2

Custom 8270 Plus Standard #2 1,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** February 28, 2026 **Storage:** 10°C or colder

**Ship:** Ambient

512082 } RC/  
↓  
512111 } 02/22/24

## CERTIFIED VALUES

| Component # | Compound                   | CAS #    | Lot #        | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|-------------|----------------------------|----------|--------------|--------|-----------------------------|--|
| 1           | 1,2,4,5-Tetrachlorobenzene | 95-94-3  | MKCT9480     | 99%    | 1,001.0 µg/mL               | +/- 29.424320                          |
| 2           | Acetophenone               | 98-86-2  | STBH8205     | 99%    | 1,004.0 µg/mL               | +/- 29.512504                          |
| 3           | Benzaldehyde               | 100-52-7 | RD231129RSRA | 99%    | 1,005.0 µg/mL               | +/- 29.541899                          |
| 4           | Benzoic acid               | 65-85-0  | MKCR2694     | 99%    | 1,003.0 µg/mL               | +/- 29.483110                          |
| 5           | Biphenyl                   | 92-52-4  | MKCL6515     | 99%    | 1,006.0 µg/mL               | +/- 29.571294                          |

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

John Friedline - Operations Technician I

Date Mixed: 12-Feb-2024

Balance: B345965662



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 555224 **Lot No.:** A0207706

**Description :** Custom 8270 Plus Standard #2

Custom 8270 Plus Standard #2 1,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** February 28, 2026 **Storage:** 10°C or colder

**Ship:** Ambient

512082 } RC/  
↓  
512111 } 02/22/24

## CERTIFIED VALUES

| Component # | Compound                   | CAS #    | Lot #        | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|-------------|----------------------------|----------|--------------|--------|-----------------------------|--|
| 1           | 1,2,4,5-Tetrachlorobenzene | 95-94-3  | MKCT9480     | 99%    | 1,001.0 µg/mL               | +/- 29.424320                          |
| 2           | Acetophenone               | 98-86-2  | STBH8205     | 99%    | 1,004.0 µg/mL               | +/- 29.512504                          |
| 3           | Benzaldehyde               | 100-52-7 | RD231129RSRA | 99%    | 1,005.0 µg/mL               | +/- 29.541899                          |
| 4           | Benzoic acid               | 65-85-0  | MKCR2694     | 99%    | 1,003.0 µg/mL               | +/- 29.483110                          |
| 5           | Biphenyl                   | 92-52-4  | MKCL6515     | 99%    | 1,006.0 µg/mL               | +/- 29.571294                          |

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

John Friedline - Operations Technician I

Date Mixed: 12-Feb-2024

Balance: B345965662



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 555224 **Lot No.:** A0207706

**Description :** Custom 8270 Plus Standard #2

Custom 8270 Plus Standard #2 1,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** February 28, 2026 **Storage:** 10°C or colder

**Ship:** Ambient

512082 } RC/  
↓  
512111 } 02/22/24

## CERTIFIED VALUES

| Component # | Compound                   | CAS #    | Lot #        | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|-------------|----------------------------|----------|--------------|--------|-----------------------------|--|
| 1           | 1,2,4,5-Tetrachlorobenzene | 95-94-3  | MKCT9480     | 99%    | 1,001.0 µg/mL               | +/- 29.424320                          |
| 2           | Acetophenone               | 98-86-2  | STBH8205     | 99%    | 1,004.0 µg/mL               | +/- 29.512504                          |
| 3           | Benzaldehyde               | 100-52-7 | RD231129RSRA | 99%    | 1,005.0 µg/mL               | +/- 29.541899                          |
| 4           | Benzoic acid               | 65-85-0  | MKCR2694     | 99%    | 1,003.0 µg/mL               | +/- 29.483110                          |
| 5           | Biphenyl                   | 92-52-4  | MKCL6515     | 99%    | 1,006.0 µg/mL               | +/- 29.571294                          |

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

John Friedline - Operations Technician I

Date Mixed: 12-Feb-2024

Balance: B345965662



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

gravimetric



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 555224 **Lot No.:** A0207706

**Description :** Custom 8270 Plus Standard #2

Custom 8270 Plus Standard #2 1,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** February 28, 2026 **Storage:** 10°C or colder

**Ship:** Ambient

512082 } RC/  
↓  
512111 } 02/22/24

### CERTIFIED VALUES

| Component # | Compound                   | CAS #    | Lot #        | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|-------------|----------------------------|----------|--------------|--------|-----------------------------|--|
| 1           | 1,2,4,5-Tetrachlorobenzene | 95-94-3  | MKCT9480     | 99%    | 1,001.0 µg/mL               | +/- 29.424320                          |
| 2           | Acetophenone               | 98-86-2  | STBH8205     | 99%    | 1,004.0 µg/mL               | +/- 29.512504                          |
| 3           | Benzaldehyde               | 100-52-7 | RD231129RSRA | 99%    | 1,005.0 µg/mL               | +/- 29.541899                          |
| 4           | Benzoic acid               | 65-85-0  | MKCR2694     | 99%    | 1,003.0 µg/mL               | +/- 29.483110                          |
| 5           | Biphenyl                   | 92-52-4  | MKCL6515     | 99%    | 1,006.0 µg/mL               | +/- 29.571294                          |

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

John Friedline - Operations Technician I

Date Mixed: 12-Feb-2024

Balance: B345965662



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 555224 **Lot No.:** A0207706

**Description :** Custom 8270 Plus Standard #2

Custom 8270 Plus Standard #2 1,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** February 28, 2026 **Storage:** 10°C or colder

**Ship:** Ambient

512082 } RC/  
↓  
512111 } 02/22/24

## CERTIFIED VALUES

| Component # | Compound                   | CAS #    | Lot #        | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|-------------|----------------------------|----------|--------------|--------|-----------------------------|--|
| 1           | 1,2,4,5-Tetrachlorobenzene | 95-94-3  | MKCT9480     | 99%    | 1,001.0 µg/mL               | +/- 29.424320                          |
| 2           | Acetophenone               | 98-86-2  | STBH8205     | 99%    | 1,004.0 µg/mL               | +/- 29.512504                          |
| 3           | Benzaldehyde               | 100-52-7 | RD231129RSRA | 99%    | 1,005.0 µg/mL               | +/- 29.541899                          |
| 4           | Benzoic acid               | 65-85-0  | MKCR2694     | 99%    | 1,003.0 µg/mL               | +/- 29.483110                          |
| 5           | Biphenyl                   | 92-52-4  | MKCL6515     | 99%    | 1,006.0 µg/mL               | +/- 29.571294                          |

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

John Friedline - Operations Technician I

Date Mixed: 12-Feb-2024

Balance: B345965662



5580 Skylane Blvd  
Santa Rosa, CA 95403

(707)525-5788  
(800)878-7654 Toll Free  
(707)545-7901 Fax

Manufacturer's Quality System  
Audited & Registered  
by TUV USA to ISO 9001:2015

Date Received: \_\_\_\_\_

## Certificate of Analysis

Rev 0

Page 1 of 1

| Catalog No.: | Lot No.: | Storage: | Solvent:     | Exp. Date: | Description:                             |                     |
|--------------|----------|----------|--------------|------------|--|---------------------|
| Z-020223-01  | 454157   | ≤ -10 °C | P/T Methanol | 6/10/2026  | 1,4-Dioxane Solution, 2000 mg/L,<br>1 mL |                     |
| Compound     |          |          | CAS No.      | Purity (%) | Compound Lot No.                         | Concentration, mg/L |
| 1,4-dioxane  |          |          | 123-91-1     | 100        | 223.1.3P                                 | 1997 ± 57.08        |

512112 } RC/  
↓  
912116 } 03/08/24

\*Not a certified value

Certified By: \_\_\_\_\_

Melissa Workoff  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values  
listed are determined gravimetrically.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31850 **Lot No.:** A0203726

**Description :** 8270 MegaMix®  
8270 MegaMix® 500-1000 µg/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** April 30, 2025 **Storage:** 0°C or colder

**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

512117 } RC/  
↓ 03/18/24  
512146 }

### CERTIFIED VALUES

| Elution Order | Compound                     | CAS #    | Lot #       | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------------|----------|-------------|--------|-----------------------------|--|
| 1             | Pyridine                     | 110-86-1 | SHBP6240    | 99%    | 1,001.6 µg/mL               | +/- 36.4412                            |
| 2             | N-Nitrosodimethylamine       | 62-75-9  | 230209JLM   | 99%    | 1,005.9 µg/mL               | +/- 36.5968                            |
| 3             | Phenol                       | 108-95-2 | MKCK1120    | 99%    | 1,003.3 µg/mL               | +/- 36.5038                            |
| 4             | Aniline                      | 62-53-3  | X22F726     | 99%    | 1,005.8 µg/mL               | +/- 36.5928                            |
| 5             | Bis(2-chloroethyl)ether      | 111-44-4 | SHBL6942    | 99%    | 1,008.1 µg/mL               | +/- 36.6776                            |
| 6             | 2-Chlorophenol               | 95-57-8  | STBJ3909    | 99%    | 1,001.8 µg/mL               | +/- 36.4492                            |
| 7             | 1,3-Dichlorobenzene          | 541-73-1 | BCCD5315    | 99%    | 1,002.3 µg/mL               | +/- 36.4654                            |
| 8             | 1,4-Dichlorobenzene          | 106-46-7 | MKBS7929V   | 99%    | 1,003.7 µg/mL               | +/- 36.5159                            |
| 9             | Benzyl alcohol               | 100-51-6 | SHBK5469    | 99%    | 1,008.7 µg/mL               | +/- 36.6979                            |
| 10            | 1,2-Dichlorobenzene          | 95-50-1  | SHBN3835    | 99%    | 1,000.3 µg/mL               | +/- 36.3926                            |
| 11            | 2-Methylphenol (o-cresol)    | 95-48-7  | SHBN7598    | 99%    | 1,003.5 µg/mL               | +/- 36.5099                            |
| 12            | 2,2'-oxybis(1-chloropropane) | 108-60-1 | 29-MAR-45-5 | 99%    | 1,007.3 µg/mL               | +/- 36.6493                            |
| 13            | 3-Methylphenol (m-cresol)    | 108-39-4 | STBJ0710    | 99%    | 504.3 µg/mL                 | +/- 18.3500                            |
| 14            | 4-Methylphenol (p-cresol)    | 106-44-5 | SHBN3411    | 99%    | 503.6 µg/mL                 | +/- 18.3237                            |
| 15            | N-Nitroso-di-n-propylamine   | 621-64-7 | N63MG       | 99%    | 1,008.3 µg/mL               | +/- 36.6857                            |
| 16            | Hexachloroethane             | 67-72-1  | QTORH       | 99%    | 1,007.5 µg/mL               | +/- 36.6554                            |
| 17            | Nitrobenzene                 | 98-95-3  | 10224044    | 99%    | 1,008.6 µg/mL               | +/- 36.6938                            |

|    |   |           |             |     |         |       |             |
|----|---|-----------|-------------|-----|---------|-------|-------------|
| 18 | Isophorone                                    | 78-59-1   | MKCC9506    | 99% | 1,005.9 | µg/mL | +/- 36.5988 |
| 19 | 2-Nitrophenol                                 | 88-75-5   | RP230710    | 99% | 1,003.2 | µg/mL | +/- 36.4998 |
| 20 | 2,4-Dimethylphenol                            | 105-67-9  | XW5GK       | 99% | 1,003.8 | µg/mL | +/- 36.5200 |
| 21 | Bis(2-chloroethoxy)methane                    | 111-91-1  | 13670200    | 99% | 1,002.1 | µg/mL | +/- 36.4573 |
| 22 | 2,4-Dichlorophenol                            | 120-83-2  | BCBZ6787    | 99% | 1,003.7 | µg/mL | +/- 36.5180 |
| 23 | 1,2,4-Trichlorobenzene                        | 120-82-1  | SHBP5900    | 99% | 1,007.6 | µg/mL | +/- 36.6574 |
| 24 | Naphthalene                                   | 91-20-3   | STBL1057    | 99% | 1,008.3 | µg/mL | +/- 36.6837 |
| 25 | 4-Chloroaniline                               | 106-47-8  | BCCJ3217    | 99% | 1,001.3 | µg/mL | +/- 36.4290 |
| 26 | Hexachlorobutadiene                           | 87-68-3   | RP230823RSR | 98% | 1,008.3 | µg/mL | +/- 36.6829 |
| 27 | 4-Chloro-3-methylphenol                       | 59-50-7   | BCCD4461    | 99% | 1,003.1 | µg/mL | +/- 36.4937 |
| 28 | 2-Methylnaphthalene                           | 91-57-6   | STBK0259    | 96% | 1,001.9 | µg/mL | +/- 36.4505 |
| 29 | 1-Methylnaphthalene                           | 90-12-0   | 5234.00-8   | 98% | 1,000.0 | µg/mL | +/- 36.3838 |
| 30 | Hexachlorocyclopentadiene                     | 77-47-4   | 099063I14L  | 98% | 1,008.5 | µg/mL | +/- 36.6909 |
| 31 | 2,4,6-Trichlorophenol                         | 88-06-2   | STBJ5914    | 99% | 1,004.4 | µg/mL | +/- 36.5442 |
| 32 | 2,4,5-Trichlorophenol                         | 95-95-4   | FHN01       | 98% | 1,001.9 | µg/mL | +/- 36.4512 |
| 33 | 2-Chloronaphthalene                           | 91-58-7   | RPN7O       | 99% | 1,001.1 | µg/mL | +/- 36.4230 |
| 34 | 2-Nitroaniline                                | 88-74-4   | RP230531    | 99% | 1,002.9 | µg/mL | +/- 36.4876 |
| 35 | 1,4-Dinitrobenzene                            | 100-25-4  | RP230816    | 99% | 1,005.7 | µg/mL | +/- 36.5887 |
| 36 | Acenaphthylene                                | 208-96-8  | p06V        | 98% | 1,009.5 | µg/mL | +/- 36.7265 |
| 37 | 1,3-Dinitrobenzene                            | 99-65-0   | 1-DXX-24-1  | 99% | 1,004.4 | µg/mL | +/- 36.5422 |
| 38 | Dimethylphthalate                             | 131-11-3  | 358221L17K  | 99% | 1,005.9 | µg/mL | +/- 36.5968 |
| 39 | 2,6-Dinitrotoluene                            | 606-20-2  | BCCG1833    | 99% | 1,003.2 | µg/mL | +/- 36.4998 |
| 40 | 1,2-Dinitrobenzene                            | 528-29-0  | RP230428    | 99% | 1,002.2 | µg/mL | +/- 36.4634 |
| 41 | Acenaphthene                                  | 83-32-9   | MKCR7169    | 99% | 1,009.3 | µg/mL | +/- 36.7221 |
| 42 | 3-Nitroaniline                                | 99-09-2   | RP230822RSR | 99% | 1,003.9 | µg/mL | +/- 36.5240 |
| 43 | 2,4-Dinitrophenol                             | 51-28-5   | DR230417RSR | 99% | 1,002.0 | µg/mL | +/- 36.4553 |
| 44 | Dibenzofuran                                  | 132-64-9  | MKCD9952    | 99% | 1,006.7 | µg/mL | +/- 36.6251 |
| 45 | 2,4-Dinitrotoluene                            | 121-14-2  | MKAA0690V   | 99% | 1,003.8 | µg/mL | +/- 36.5220 |
| 46 | 4-Nitrophenol                                 | 100-02-7  | RP230627    | 99% | 1,002.3 | µg/mL | +/- 36.4674 |
| 47 | 2,3,4,6-Tetrachlorophenol                     | 58-90-2   | PR-30126    | 99% | 1,008.7 | µg/mL | +/- 36.6979 |
| 48 | 2,3,5,6-Tetrachlorophenol                     | 935-95-5  | RP230919    | 99% | 1,006.3 | µg/mL | +/- 36.6130 |
| 49 | Fluorene                                      | 86-73-7   | 10241100    | 99% | 1,008.3 | µg/mL | +/- 36.6857 |
| 50 | 4-Chlorophenyl phenyl ether                   | 7005-72-3 | MKCT7248    | 99% | 1,003.8 | µg/mL | +/- 36.5220 |
| 51 | Diethylphthalate                              | 84-66-2   | MKCD2547    | 99% | 1,008.6 | µg/mL | +/- 36.6958 |
| 52 | 4-Nitroaniline                                | 100-01-6  | RP230111    | 99% | 1,001.1 | µg/mL | +/- 36.4230 |
| 53 | 4,6-Dinitro-2-methylphenol (Dinitro-o-cresol) | 534-52-1  | 230718JLM   | 99% | 1,002.0 | µg/mL | +/- 36.4553 |

|    |                            |          |               |     |         |       |             |
|----|----------------------------|----------|---------------|-----|---------|-------|-------------|
| 54 | Diphenylamine              | 122-39-4 | MKCH1042      | 99% | 1,002.3 | µg/mL | +/- 36.4674 |
| 55 | Azobenzene                 | 103-33-3 | BCKK0887      | 99% | 1,005.8 | µg/mL | +/- 36.5928 |
| 56 | 4-Bromophenyl phenyl ether | 101-55-3 | STBH6361      | 99% | 1,003.0 | µg/mL | +/- 36.4917 |
| 57 | Hexachlorobenzene          | 118-74-1 | 14821700      | 99% | 1,007.5 | µg/mL | +/- 36.6554 |
| 58 | Pentachlorophenol          | 87-86-5  | RP230530RSR   | 99% | 1,008.8 | µg/mL | +/- 36.7019 |
| 59 | Phenanthrene               | 85-01-8  | MKCQ8876      | 99% | 1,008.4 | µg/mL | +/- 36.6877 |
| 60 | Anthracene                 | 120-12-7 | MKCR0570      | 99% | 1,009.0 | µg/mL | +/- 36.7100 |
| 61 | Carbazole                  | 86-74-8  | 14351100      | 99% | 1,000.9 | µg/mL | +/- 36.4149 |
| 62 | Di-n-butylphthalate        | 84-74-2  | MKCN4337      | 99% | 1,007.6 | µg/mL | +/- 36.6595 |
| 63 | Fluoranthene               | 206-44-0 | MKCQ4728      | 99% | 1,009.6 | µg/mL | +/- 36.7302 |
| 64 | Pyrene                     | 129-00-0 | BCCG8479      | 98% | 1,007.2 | µg/mL | +/- 36.6453 |
| 65 | Benzyl butyl phthalate     | 85-68-7  | X12I018       | 99% | 1,002.1 | µg/mL | +/- 36.4573 |
| 66 | Bis(2-ethylhexyl)adipate   | 103-23-1 | MKCM1988      | 99% | 1,005.2 | µg/mL | +/- 36.5705 |
| 67 | Benz(a)anthracene          | 56-55-3  | I220012022BAA | 99% | 1,002.2 | µg/mL | +/- 36.4614 |
| 68 | Chrysene                   | 218-01-9 | RP230601      | 99% | 1,008.3 | µg/mL | +/- 36.6837 |
| 69 | Bis(2-ethylhexyl)phthalate | 117-81-7 | MKCQ3468      | 99% | 1,001.8 | µg/mL | +/- 36.4472 |
| 70 | Di-n-octyl phthalate       | 117-84-0 | 14382700      | 99% | 1,006.0 | µg/mL | +/- 36.6008 |
| 71 | Benzo(b)fluoranthene       | 205-99-2 | 012013B       | 99% | 1,002.8 | µg/mL | +/- 36.4836 |
| 72 | Benzo(k)fluoranthene       | 207-08-9 | 012022K       | 99% | 1,003.0 | µg/mL | +/- 36.4917 |
| 73 | Benzo(a)pyrene             | 50-32-8  | P54915-0703   | 99% | 1,002.3 | µg/mL | +/- 36.4674 |
| 74 | Indeno(1,2,3-cd)pyrene     | 193-39-5 | 12-JKL-118-9  | 97% | 1,009.4 | µg/mL | +/- 36.7243 |
| 75 | Dibenz(a,h)anthracene      | 53-70-3  | 2-ASA-59-1    | 99% | 1,007.6 | µg/mL | +/- 36.6595 |
| 76 | Benzo(g,h,i)perylene       | 191-24-2 | RP231003RSR   | 99% | 1,002.9 | µg/mL | +/- 36.4876 |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

