DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071124\
Data File : BN032615.D
Acq On : 10 Jul 2024 15:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN071124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jul 10 23:45:48 2024

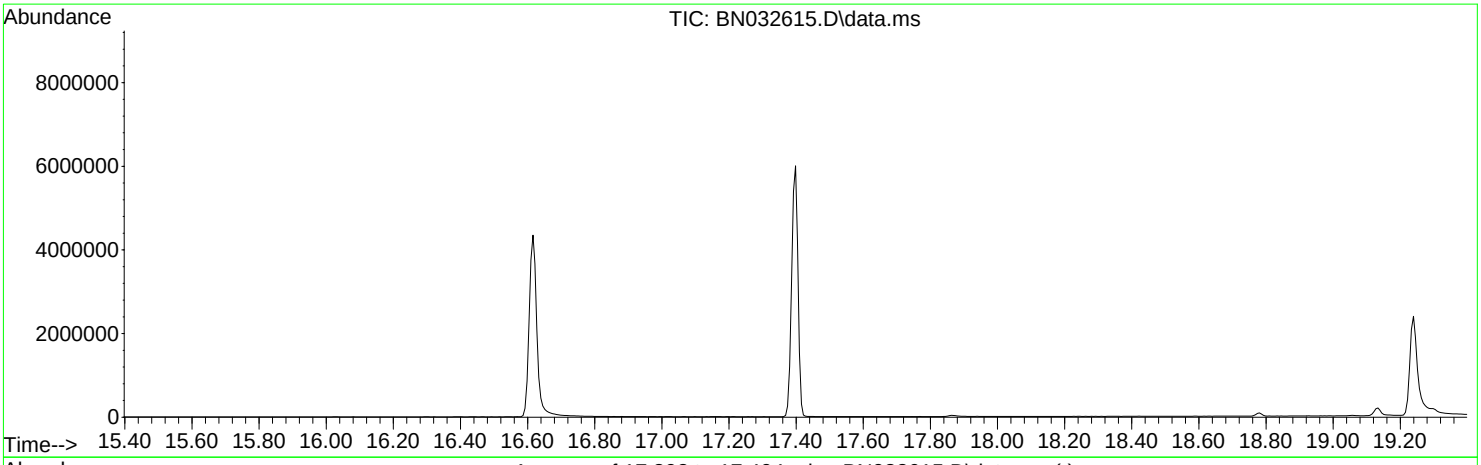

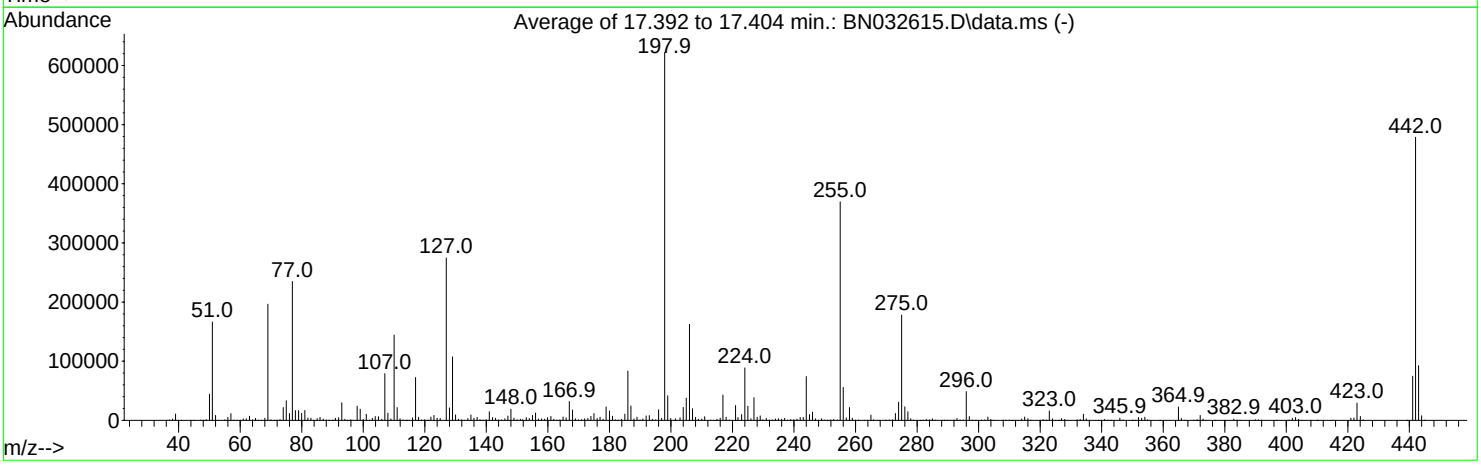

AutoFind: Scans 2449, 2450, 2451; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.7	166320	PASS
68	69	0.00	2	1.8	3465	PASS
69	198	0.00	100	31.6	196373	PASS
70	69	0.00	2	0.5	1066	PASS
127	198	10	80	44.1	274496	PASS
197	198	0.00	2	0.6	3484	PASS
198	198	100	100	100.0	621973	PASS
199	198	5	9	6.7	41595	PASS
275	198	10	60	28.6	178155	PASS
365	198	1	100	3.6	22635	PASS
441	198	0.01	100	12.0	74808	PASS
442	442	50	100	100.0	478507	PASS
443	442	15	24	19.3	92581	PASS

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/11/2024	BNA_N	BN032615.D
Compound Name	**Response**	**Retention Time**
DDT	2244369	20.463
DDD	25705	20.069
DDE	645	19.51
SUM(DDD+DDE)	**SUM(DDT+DDD+DDE)**	**% Breakdown Of DDT**
26350	2270719	1.16

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071124\
Data File : BN032615.D
Acq On : 10 Jul 2024 15:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 11 03:07:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration

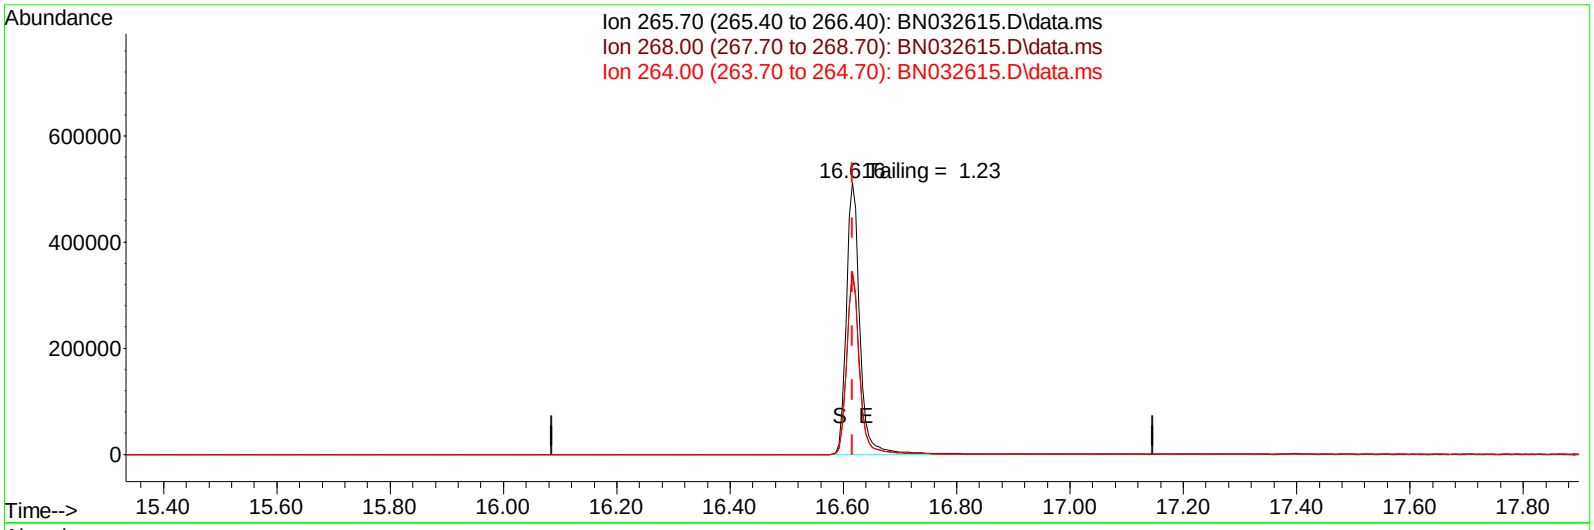

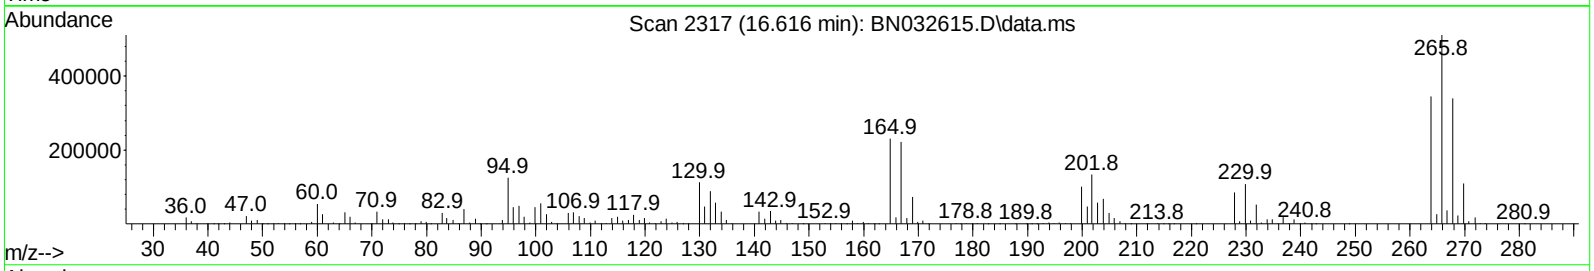

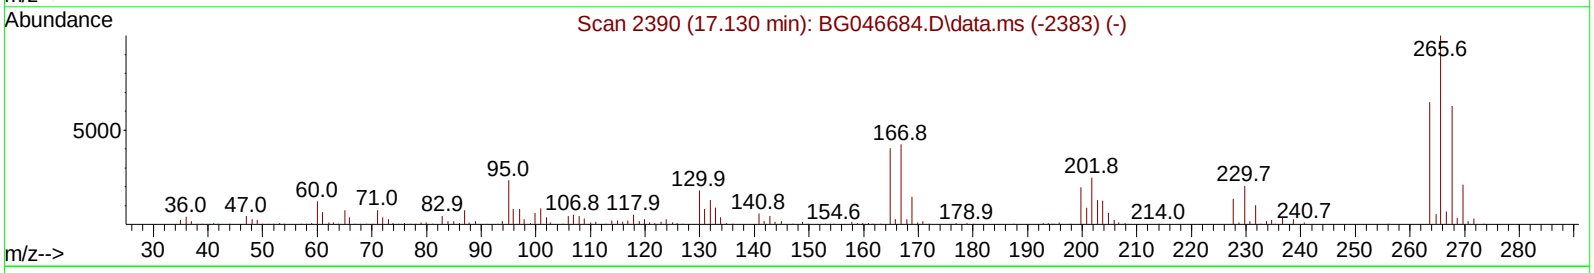

TIC: BN032615.D\data.ms

(70) Pentachlorophenol (C)

16.616min (0.000) 28100.93 ng

response 854109

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.51
264.00	61.60	67.53
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071124\
Data File : BN032615.D
Acq On : 10 Jul 2024 15:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 11 03:07:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration

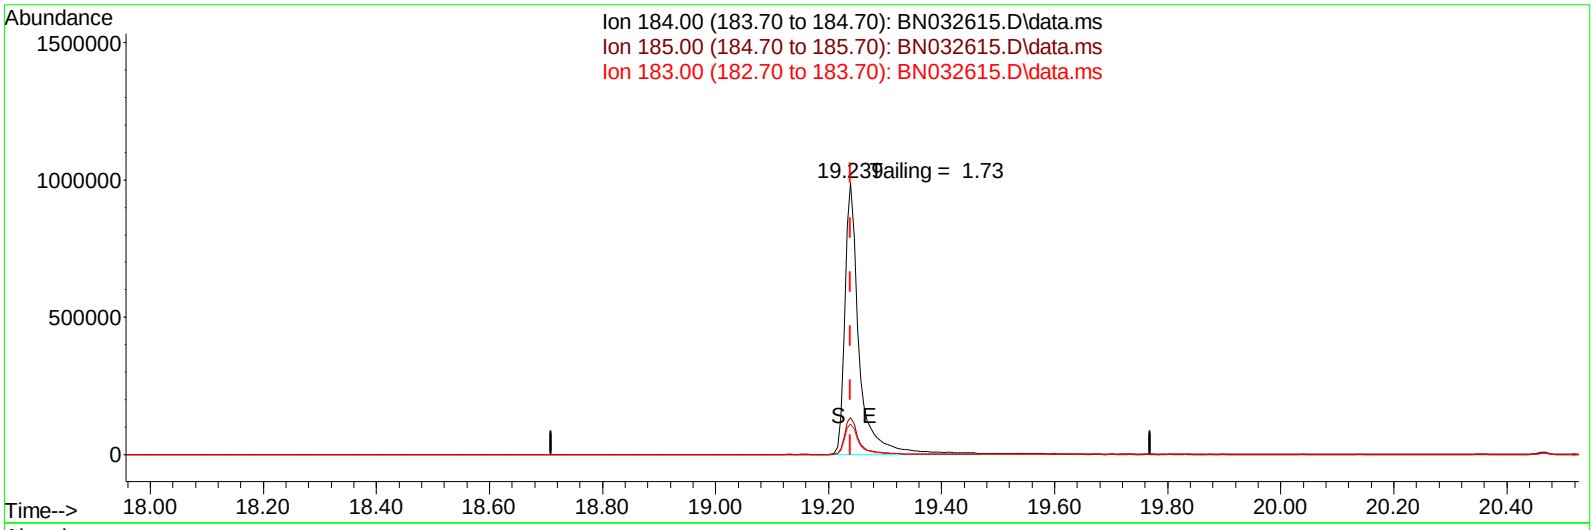

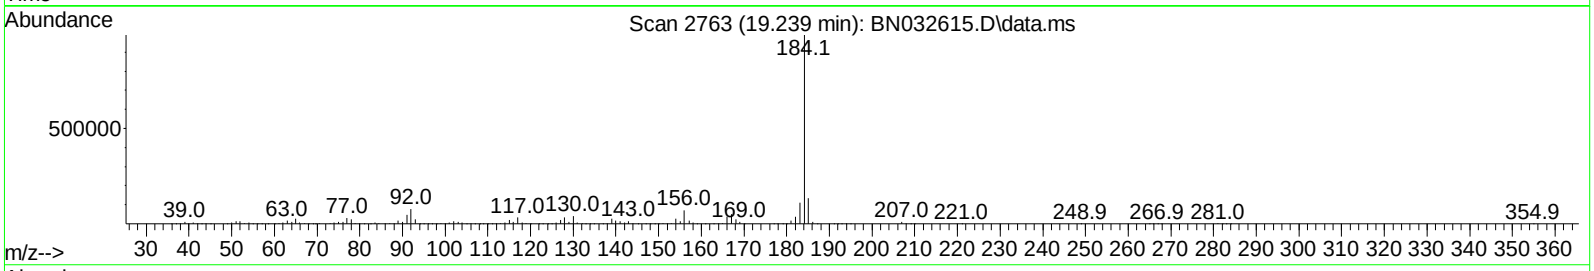

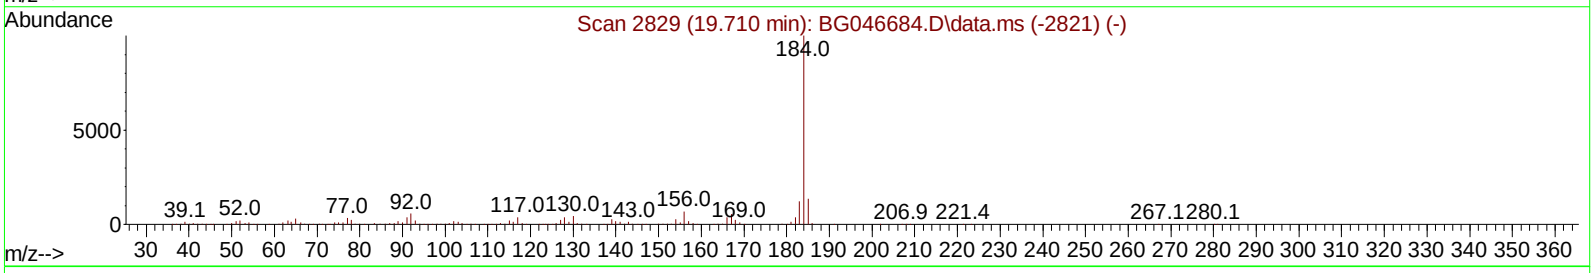

TIC: BN032615.D\data.ms

(77) Benzidine

19.239min (0.000) 190151.31 ng

response 1752584

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.60
183.00	13.20	11.21
0.00	0.00	0.00