
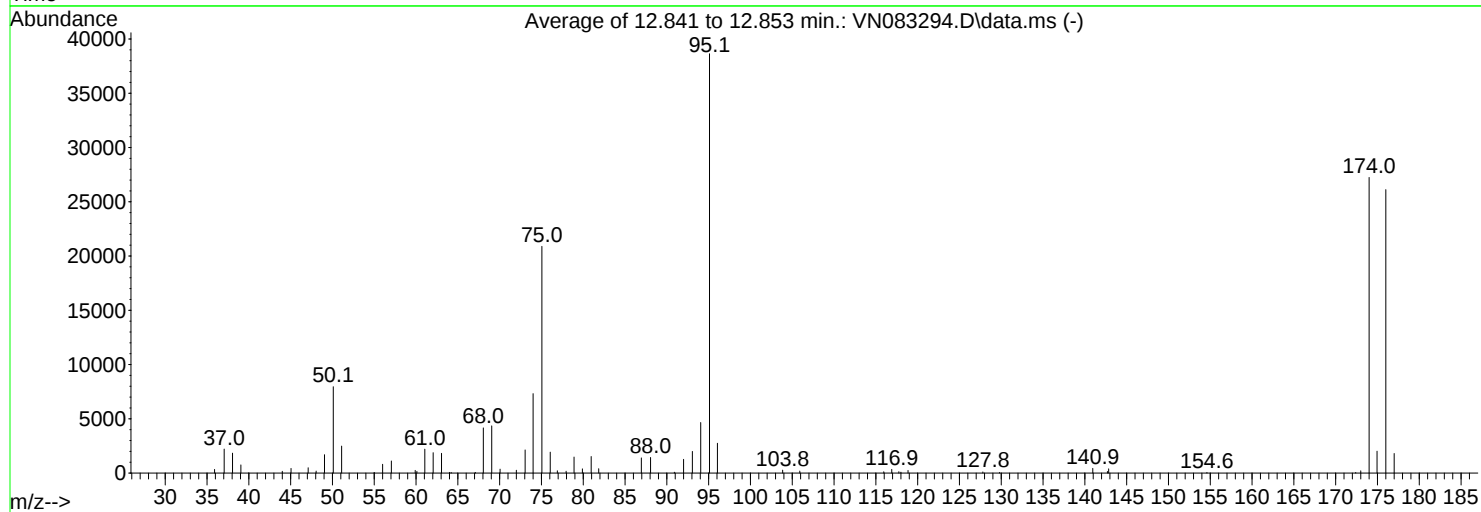


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081424\
Data File : VN083294.D
Acq On : 14 Aug 2024 12:07
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Title : SW846 8260
Last Update : Thu Aug 08 06:30:41 2024

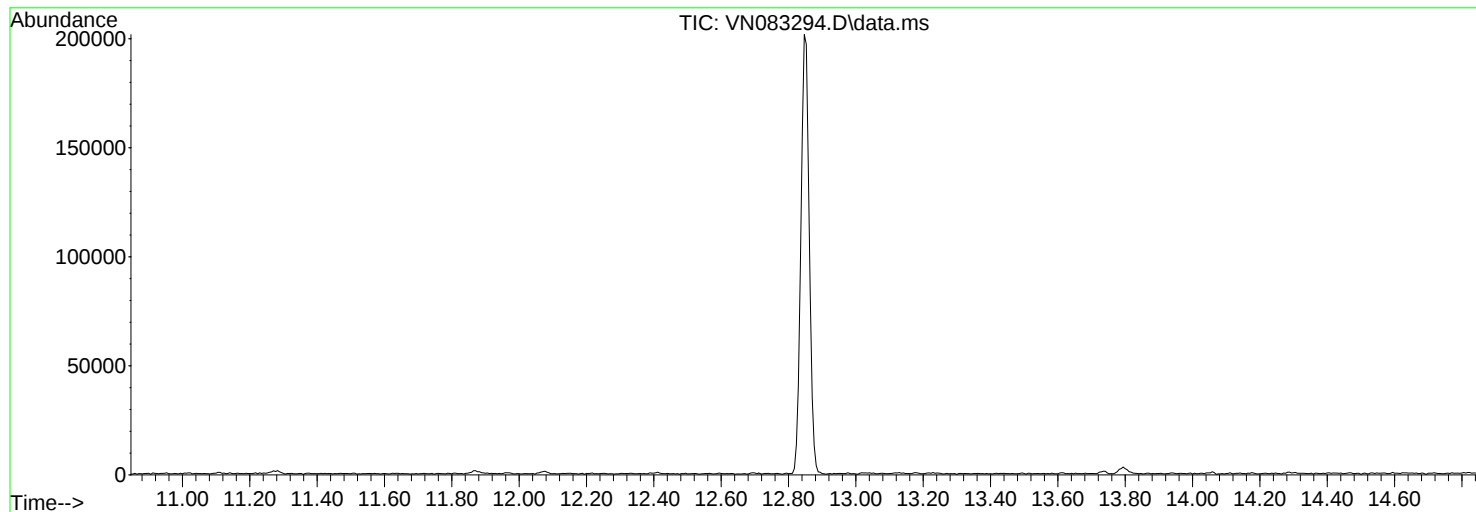

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	7958	PASS
75	95	30	60	54.1	20891	PASS
95	95	100	100	100.0	38643	PASS
96	95	5	9	7.1	2747	PASS
173	174	0.00	2	0.8	207	PASS
174	95	50	100	70.5	27243	PASS
175	174	5	9	7.4	2019	PASS
176	174	95	101	95.9	26120	PASS
177	176	5	9	6.9	1805	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	337	51.10	2486	67.10	57	78.90	1477
37.05	2211	55.00	60	68.05	4163	79.90	389
38.05	1836	56.00	810	69.05	4347	80.95	1527
39.05	750	57.05	1117	70.05	363	81.85	402
40.00	7	59.90	249	72.00	262	86.95	1401
44.00	162	60.10	156	73.05	2130	88.05	1437
45.05	430	61.05	2203	74.00	7320	90.90	79
47.10	492	62.05	1878	75.05	20891	92.00	1264
48.05	185	63.05	1820	76.05	1930	93.05	1994
49.05	1696	64.00	59	76.90	214	94.05	4656
50.10	7958	64.20	56	77.95	173	95.10	38643

Average of 12.841 to 12.853 min.: VN083294.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
96.05	2747	142.70	144				
103.85	269	142.85	389				
105.90	189	154.60	58				
115.95	125	172.40	58				
116.90	340	173.00	207				
117.75	131	174.00	27243				
118.00	87	174.95	2019				
118.85	245	176.00	26120				
127.80	108	177.00	1805				
129.80	58						
140.95	434						

Instrument :

MSVOA_N

ClientSampleId :

BFB