
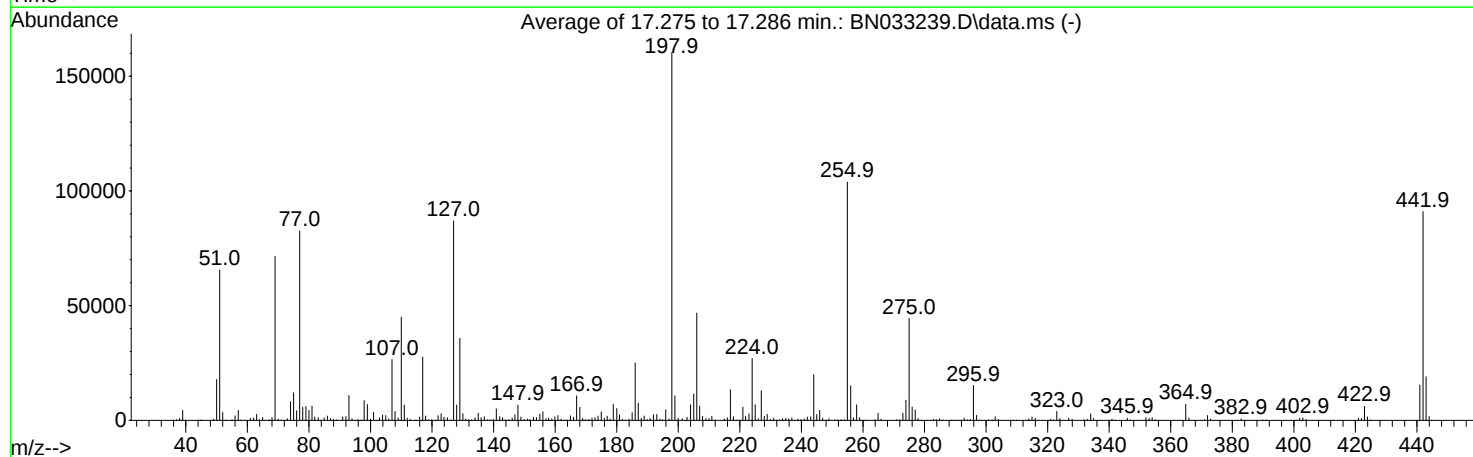


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080524\
Data File : BN033239.D
Acq On : 05 Aug 2024 16:11
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN080524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 05 23:57:48 2024

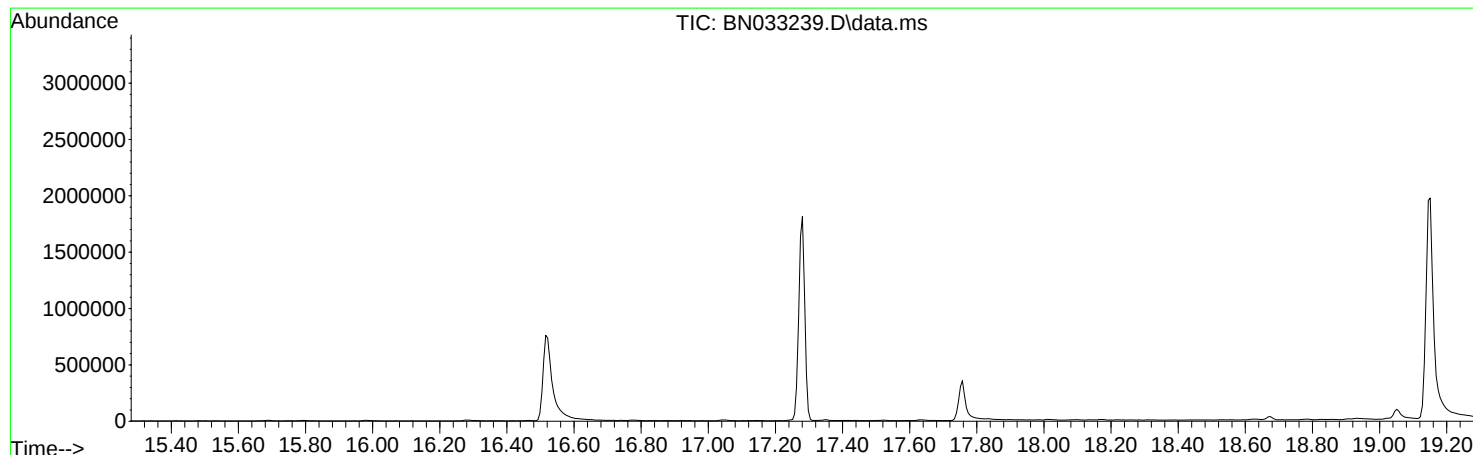




AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.9	65632	PASS
68	69	0.00	2	1.7	1232	PASS
69	198	0.00	100	44.6	71440	PASS
70	69	0.00	2	0.7	498	PASS
127	198	10	80	54.2	86973	PASS
197	198	0.00	2	0.4	626	PASS
198	198	100	100	100.0	160352	PASS
199	198	5	9	6.6	10651	PASS
275	198	10	60	27.7	44424	PASS
365	198	1	100	4.4	7070	PASS
441	198	0.01	100	9.6	15393	PASS
442	442	50	100	100.0	91032	PASS
443	442	15	24	20.9	19047	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080524\
Data File : BN033239.D
Acq On : 05 Aug 2024 16:11
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 06 08:54:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 06 08:54:36 2024
Response via : Initial Calibration

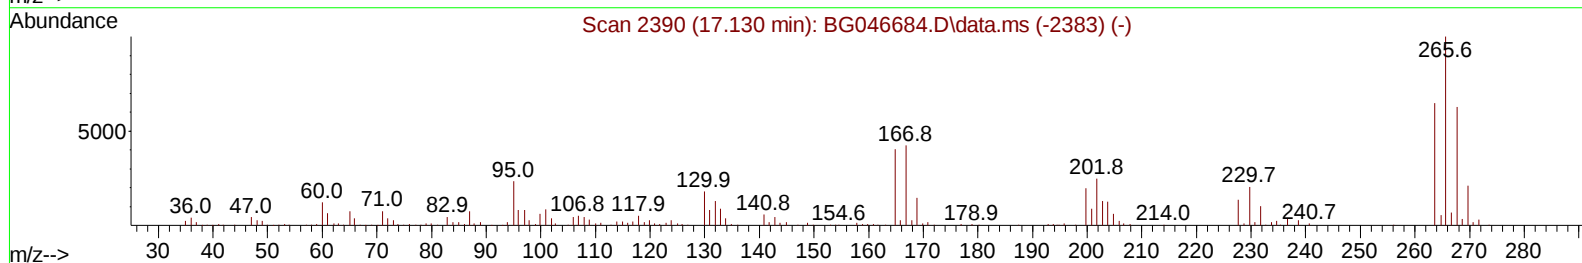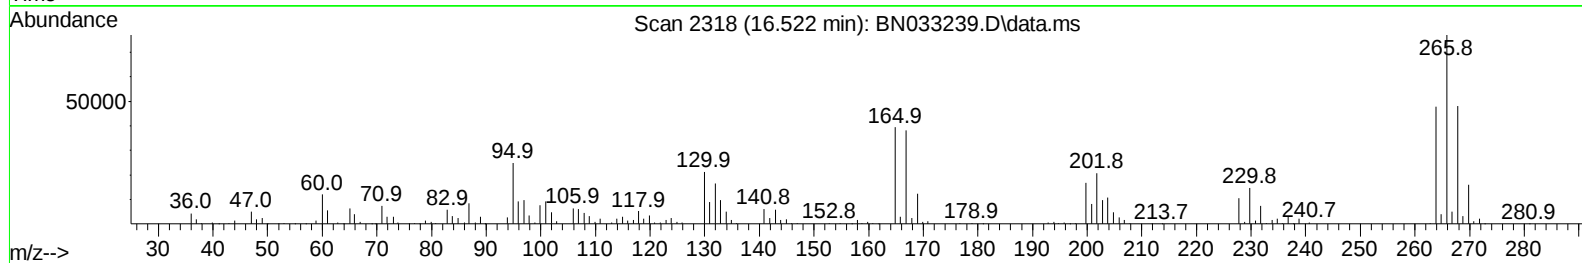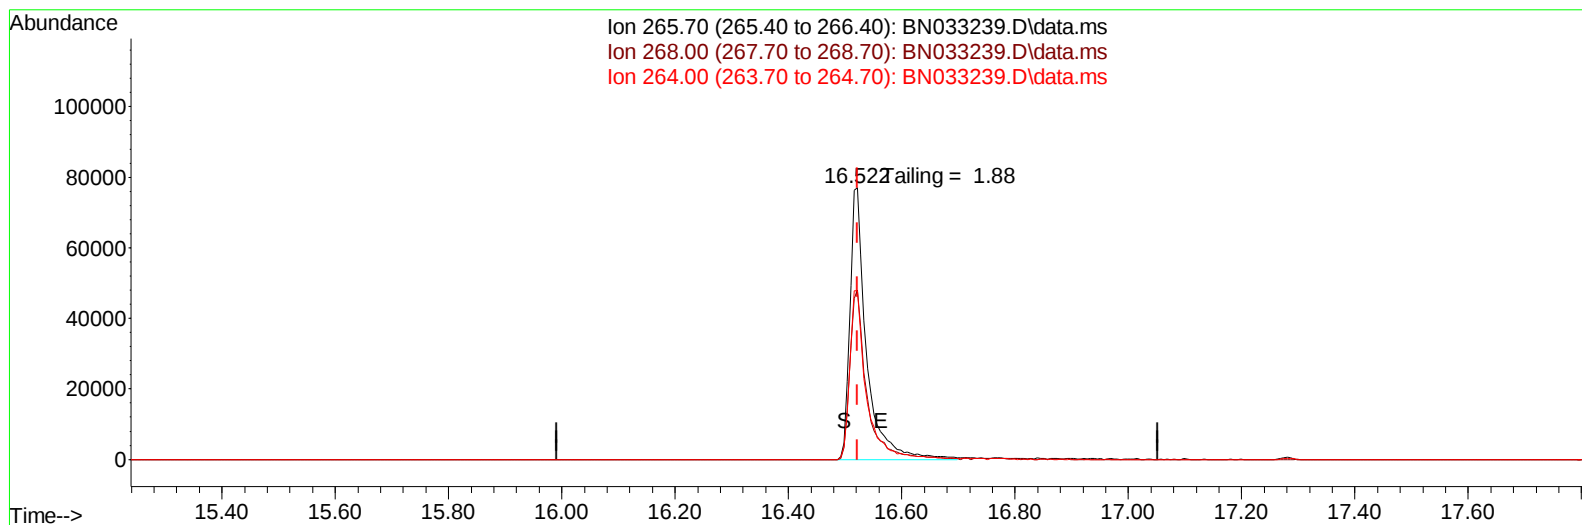

TIC: BN033239.D\data.ms

(70) Pentachlorophenol (C)




16.522min (0.000) 16240.58 ng

response 159315

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.36
264.00	61.60	62.10
0.00	0.00	0.00

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 06 08:54:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 06 08:54:36 2024
Response via : Initial Calibration

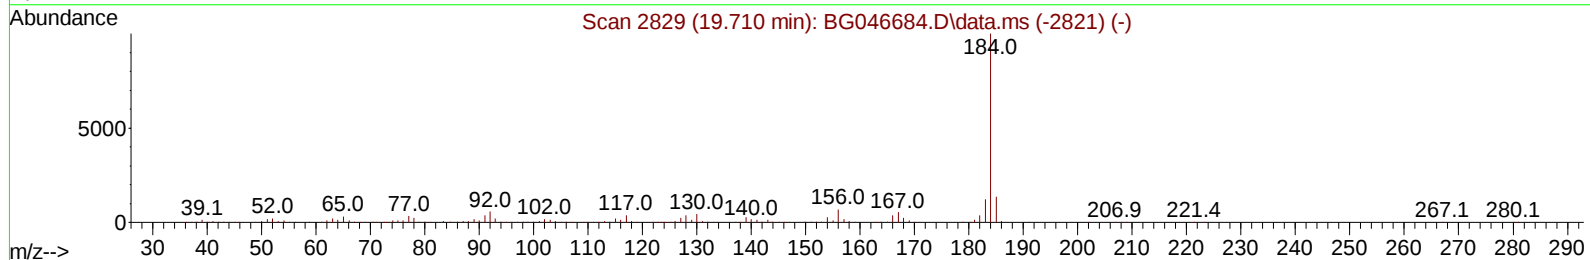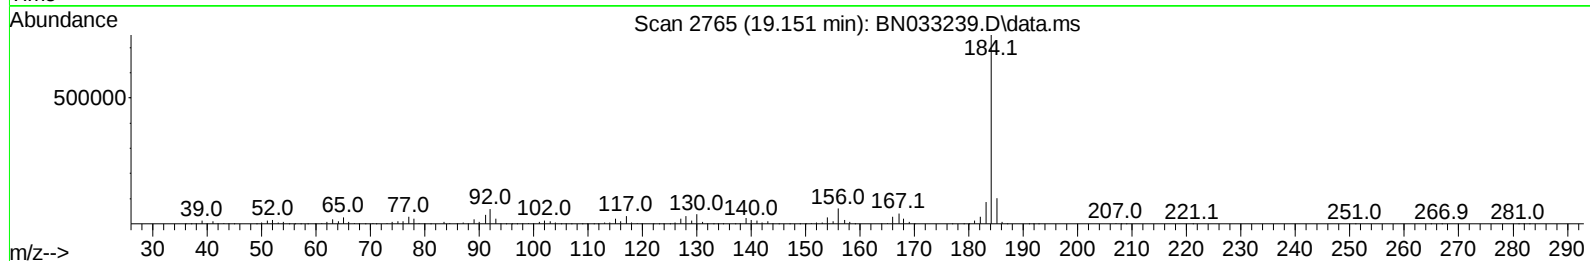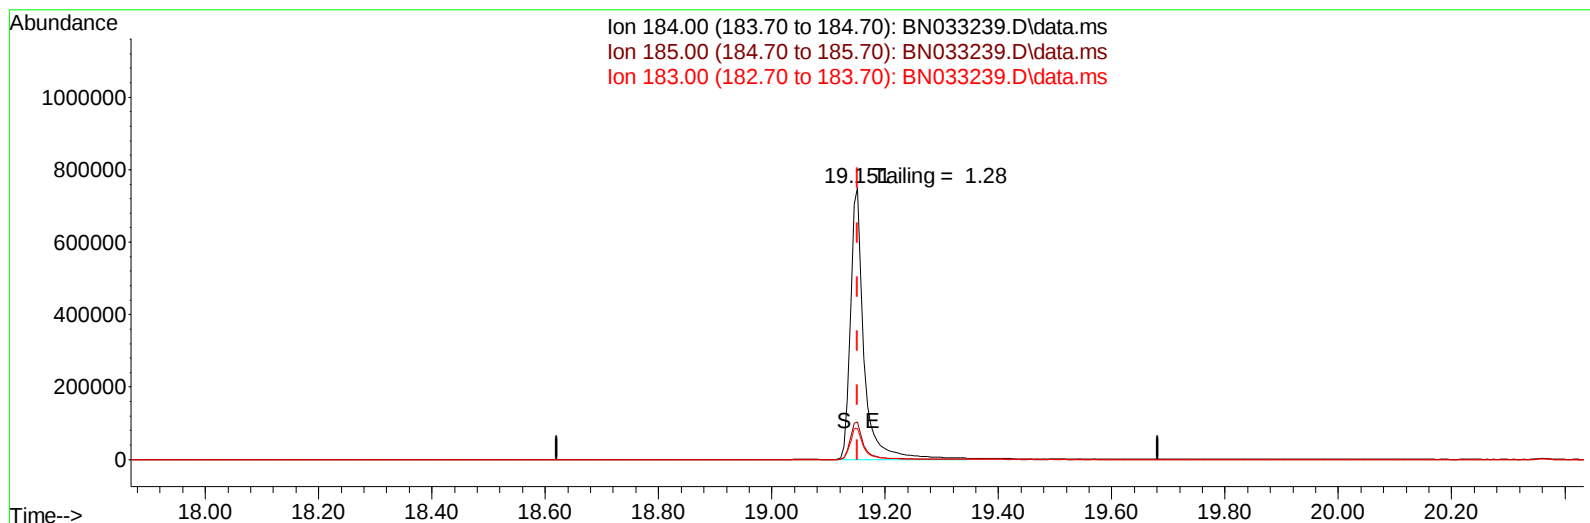

TIC: BN033239.D\data.ms

(77) **Benzidine**

19.151min (0.000) 0.00 ng

response **1263871**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.70
183.00	13.20	11.48
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/5/2024	BNA_N	<u>BN033239.D</u>
Compound Name	Response	Retention Time
DDT	675064	20.363
DDD	9359	19.963
DDE	813	19.416
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10172	685236	1.48

Instrument :
BNA_N
ClientSampleId :
DFTPP