

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080324\
 Data File : BN033234.D
 Acq On : 03 Aug 2024 12:12
 Operator : MA/JU
 Sample : P3440-04
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 922-K1-WS-080124

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/05/2024
 Supervised By :mohammad ahmed 08/07/2024

Quant Time: Aug 05 03:26:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN071124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 02 22:49:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.539	152	2484m	0.400	ng	0.04
7) Naphthalene-d8	10.298	136	8664	0.400	ng	# 0.01
13) Acenaphthene-d10	14.144	164	4994	0.400	ng	0.00
19) Phenanthrene-d10	16.915	188	10648	0.400	ng	0.00
29) Chrysene-d12	21.131	240	7008	0.400	ng	# 0.00
35) Perylene-d12	23.312	264	6904	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.249	112	971m	0.155	ng	0.00
5) Phenol-d6	6.961	99	715m	0.092	ng	0.08
8) Nitrobenzene-d5	8.846	82	1944	0.298	ng	0.03
11) 2-Methylnaphthalene-d10	11.886	152	3609	0.272	ng	-0.01
14) 2,4,6-Tribromophenol	15.686	330	602	0.282	ng	-0.03
15) 2-Fluorobiphenyl	12.775	172	5375	0.289	ng	-0.01
27) Fluoranthene-d10	18.953	212	9419	0.342	ng	0.00
31) Terphenyl-d14	19.547	244	8537	0.594	ng	-0.02
Target Compounds						Qvalue
25) Phenanthrene	16.952	178	958	0.033	ng	99
28) Fluoranthene	18.990	202	1410	0.040	ng	# 82
30) Pyrene	19.357	202	833	0.029	ng	96
34) Bis(2-ethylhexyl)phtha...	21.006	149	3125	0.255	ng	# 78

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080324\
Data File : BN033234.D
Acq On : 03 Aug 2024 12:12
Operator : MA/JU
Sample : P3440-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
922-K1-WS-080124

Quant Time: Aug 05 03:26:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN071124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 02 22:49:47 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/05/2024
Supervised By :mohammad ahmed 08/07/2024

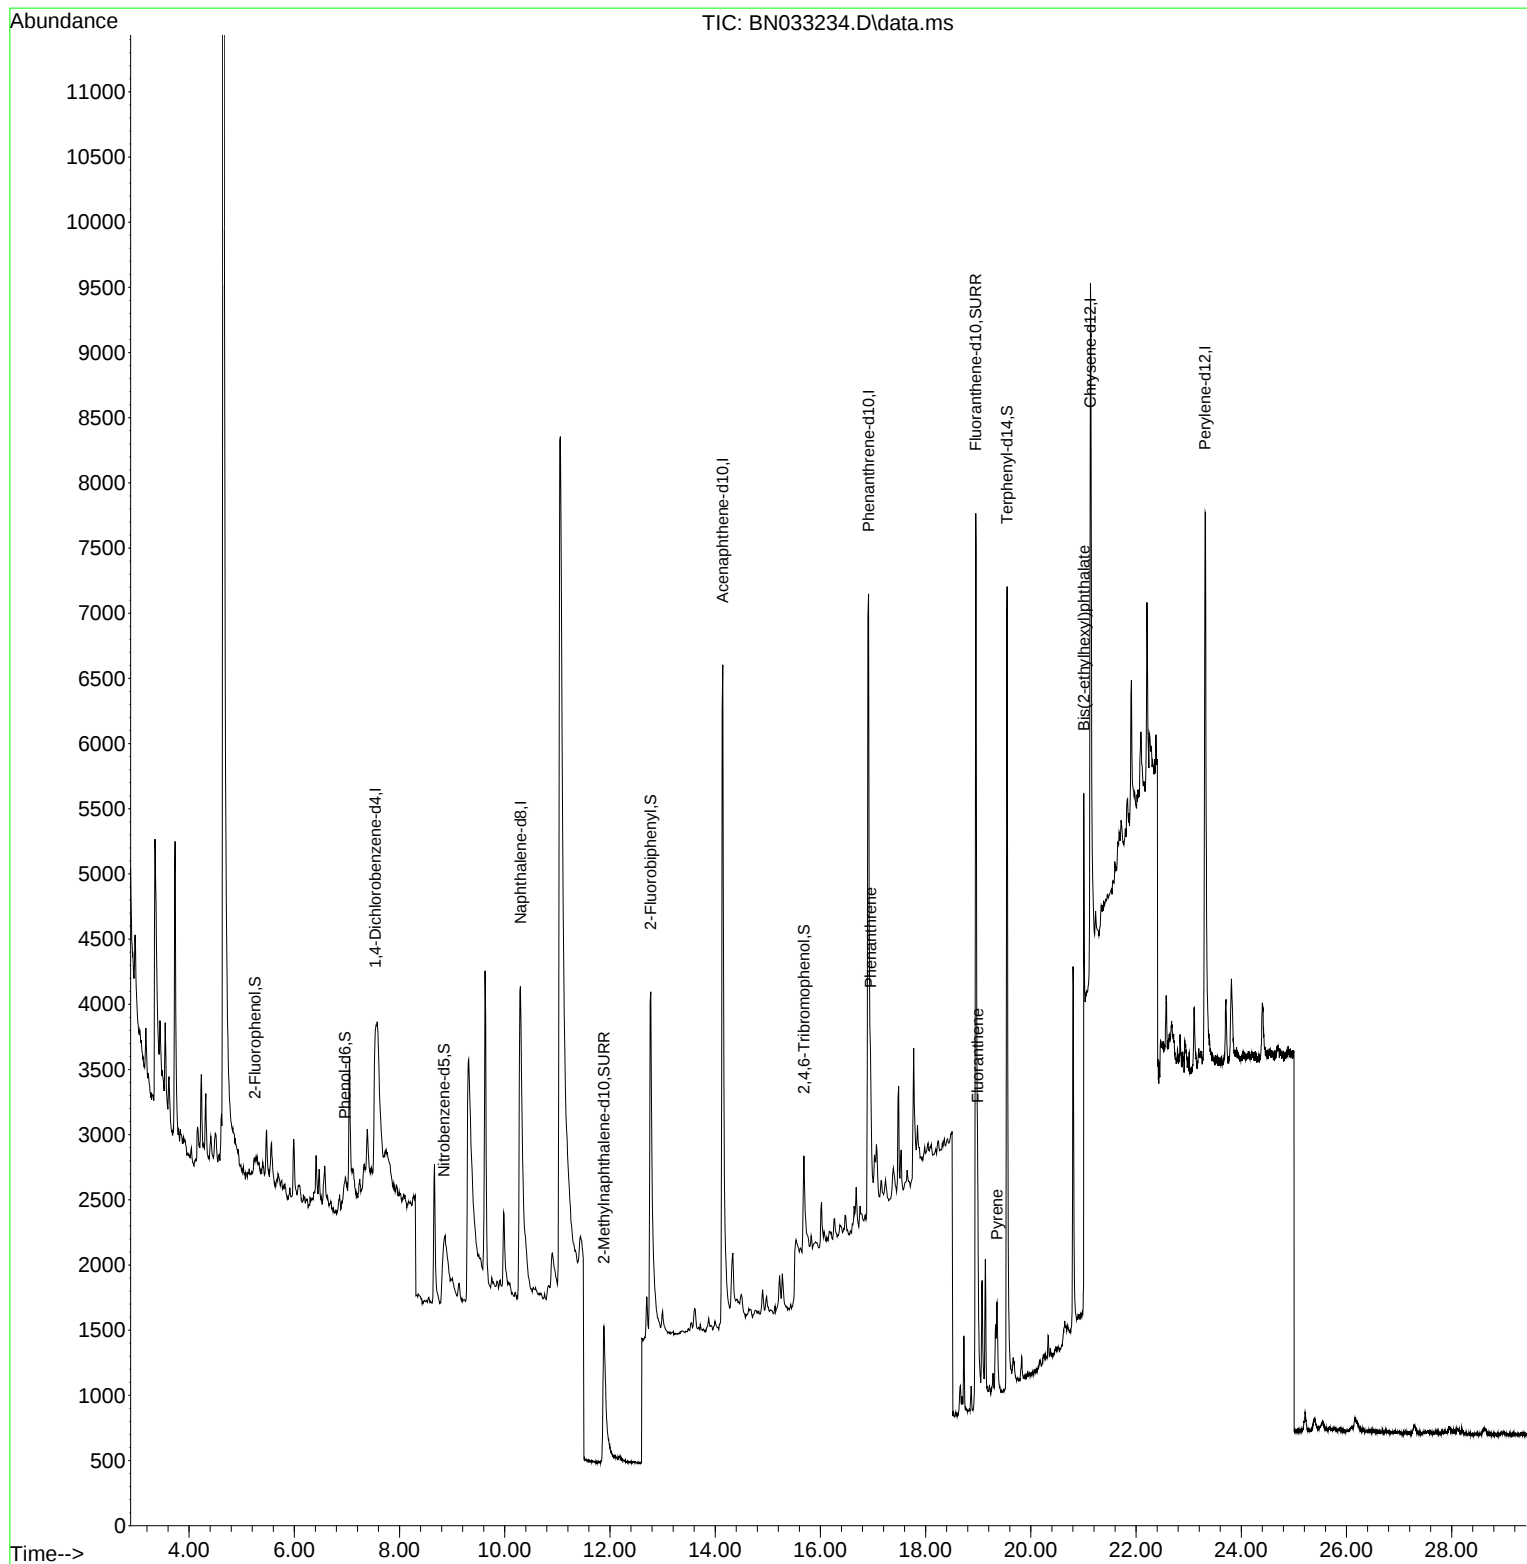



#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng m
 RT: 7.539 min Scan# 645
 Delta R.T. 0.036 min
 Lab File: BN033234.D
 Acq: 03 Aug 2024 12:12




Instrument :
 BNA_N
 ClientSampleId :
 922-K1-WS-080124

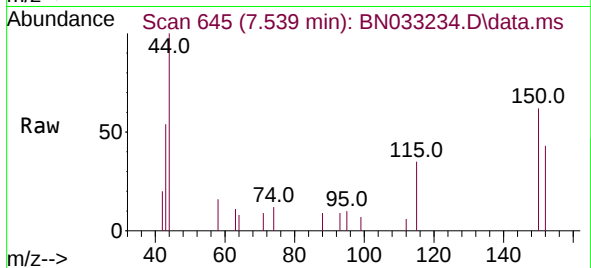

Tgt Ion:152 Resp: 2484
 Ion Ratio Lower Upper
 152 100
 150 143.0 123.8 185.6
 115 81.0 52.8 79.2




Manual Integrations
 APPROVED


Reviewed By :Jagrut Upadhyay 08/05/2024
 Supervised By :mohammad ahmed 08/07/2024

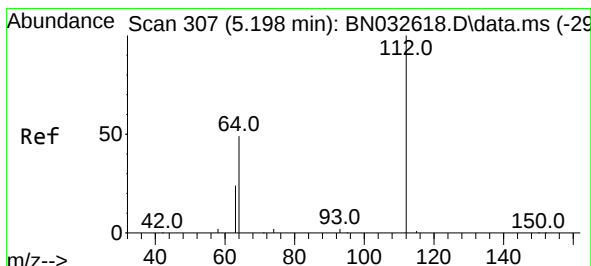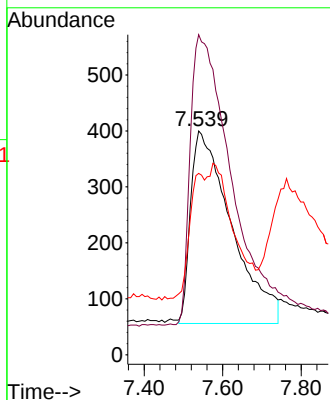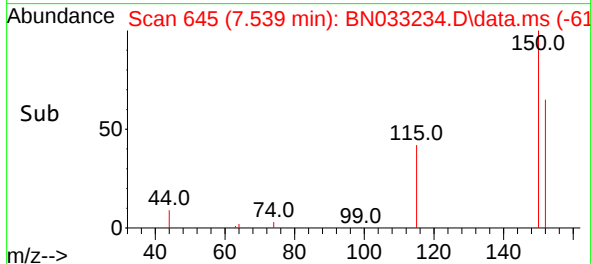

#4
 2-Fluorophenol
 Concen: 0.155 ng m
 RT: 5.249 min Scan# 328
 Delta R.T. 0.007 min
 Lab File: BN033234.D
 Acq: 03 Aug 2024 12:12


Tgt Ion:112 Resp: 971
 Ion Ratio Lower Upper
 112 100
 64 46.9 40.2 60.4
 63 7.7 22.2 33.4

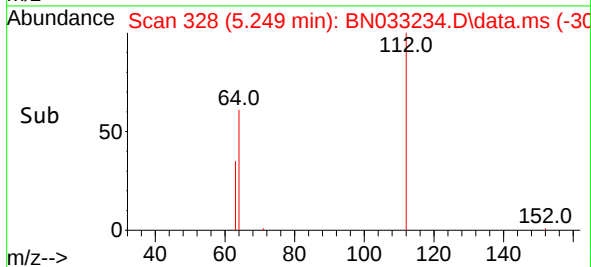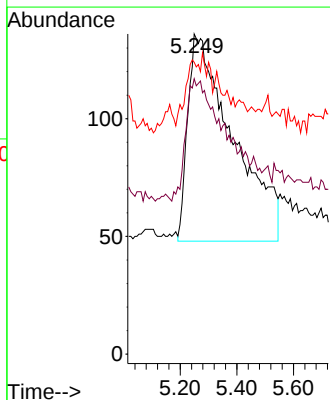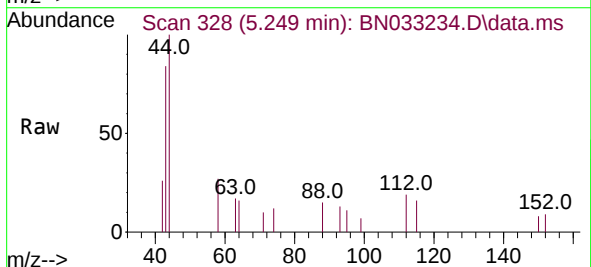

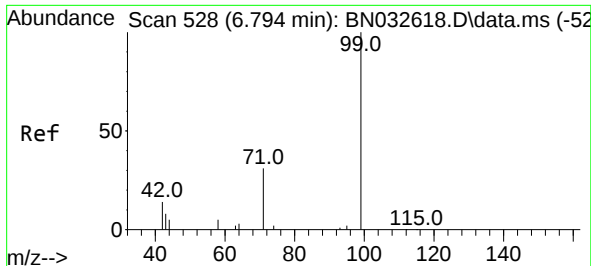

#5
Phenol-d6
Concen: 0.092 ng m
RT: 6.961 min Scan# 509
Delta R.T. 0.080 min
Lab File: BN033234.D
Acq: 03 Aug 2024 12:12




Instrument :
BNA_N
ClientSampleId :
922-K1-WS-080124

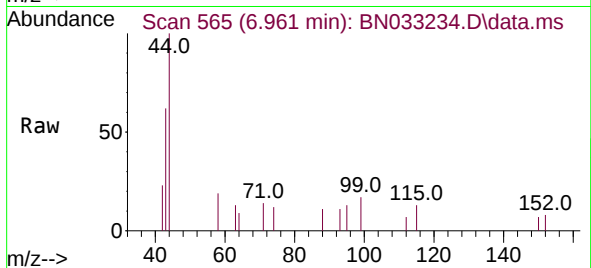


Tgt Ion: 99 Resp: 715
Ion Ratio Lower Upper
99 100
42 4.1 10.5 15.7#
71 29.4 22.3 33.5

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 08/05/2024
Supervised By :mohammad ahmed 08/07/2024

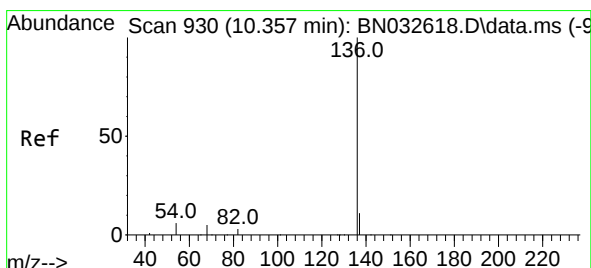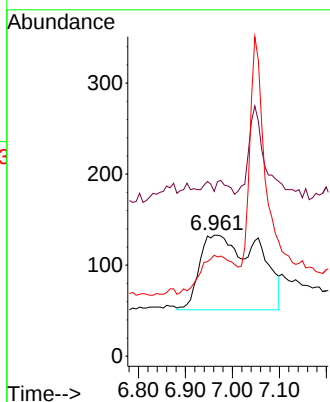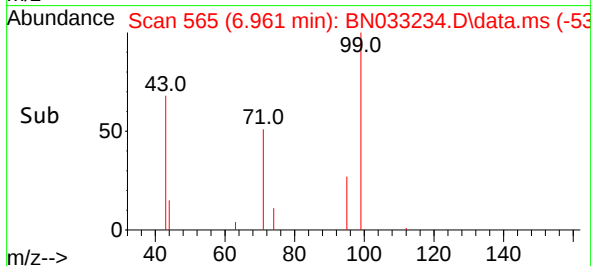


#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.298 min Scan# 938
Delta R.T. 0.011 min
Lab File: BN033234.D
Acq: 03 Aug 2024 12:12

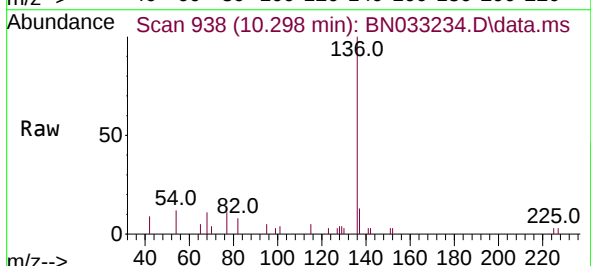

Tgt Ion:136 Resp: 8664
Ion Ratio Lower Upper
136 100
137 13.5 9.9 14.9
54 11.5 6.5 9.7#
68 10.5 5.8 8.8#

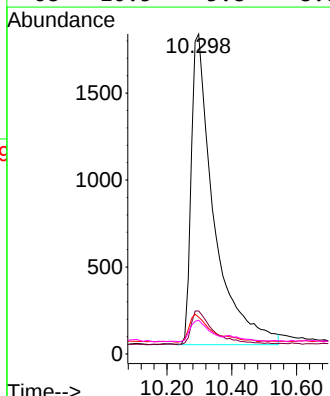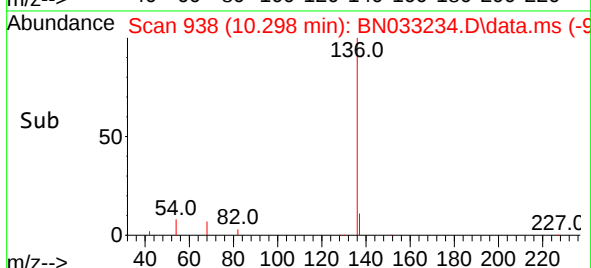

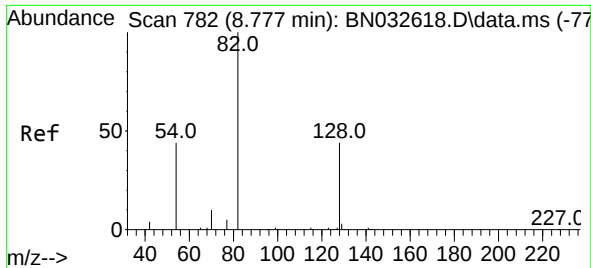





#8
Nitrobenzene-d5
Concen: 0.298 ng
RT: 8.846 min Scan# 80
Delta R.T. 0.032 min
Lab File: BN033234.D
Acq: 03 Aug 2024 12:12

Instrument :
BNA_N
ClientSampleId :
922-K1-WS-080124

Tgt Ion: 82 Resp: 1944
Ion Ratio Lower Upper
82 100
128 52.2 41.7 62.5
54 62.4 39.5 59.3




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/05/2024
Supervised By :mohammad ahmed 08/07/2024

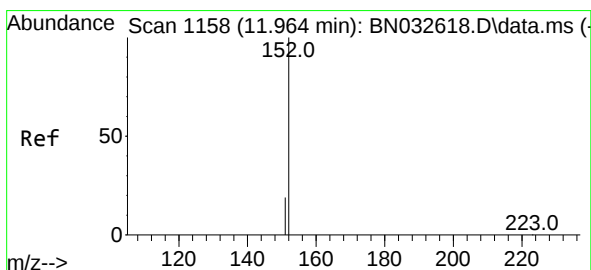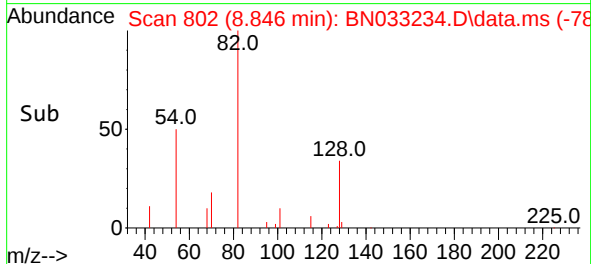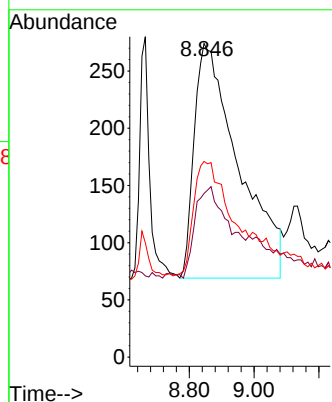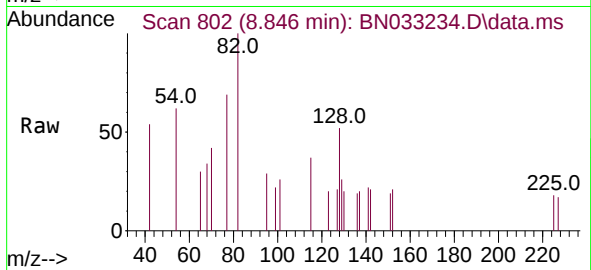

#11
2-Methylnaphthalene-d10
Concen: 0.272 ng
RT: 11.886 min Scan# 1152
Delta R.T. -0.015 min
Lab File: BN033234.D
Acq: 03 Aug 2024 12:12

Tgt Ion:152 Resp: 3609
Ion Ratio Lower Upper
152 100
151 18.3 16.2 24.2

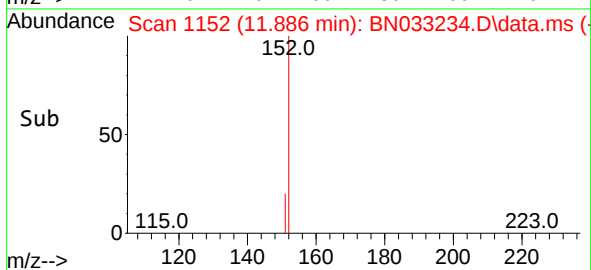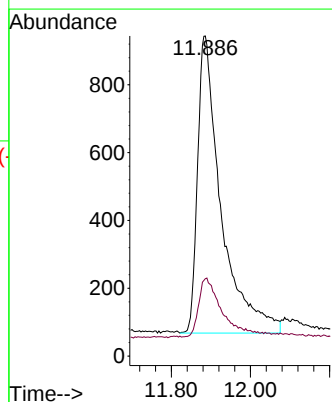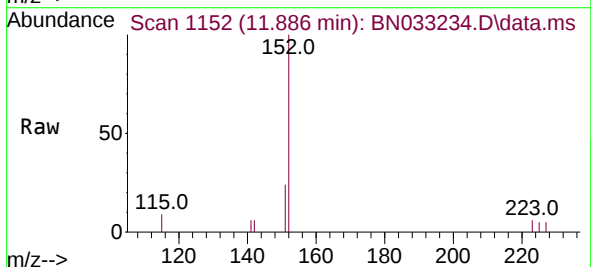

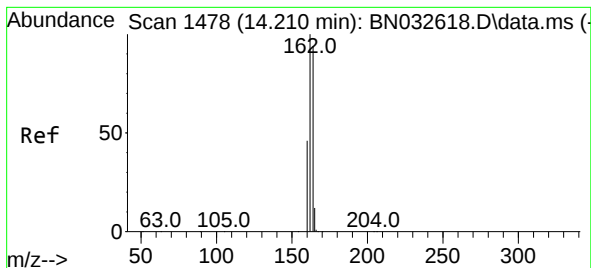

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.144 min Scan# 1478

Delta R.T. 0.007 min

Lab File: BN033234.D


Acq: 03 Aug 2024 12:12

Instrument :

BNA_N

ClientSampleId :

922-K1-WS-080124

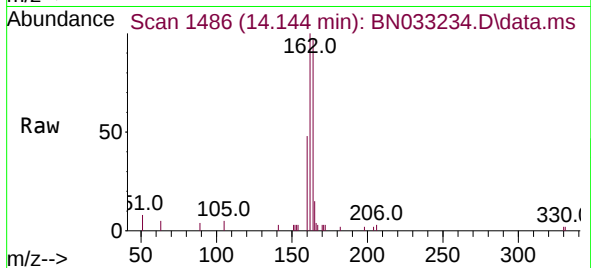

Tgt Ion:164 Resp: 4994

Ion Ratio Lower Upper

164 100

162 103.0 85.0 127.4




160 49.1 39.4 59.2

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 08/05/2024

Supervised By :mohammad ahmed 08/07/2024

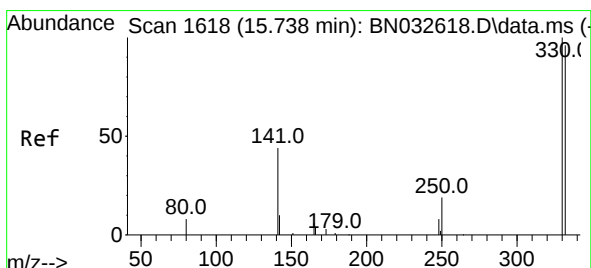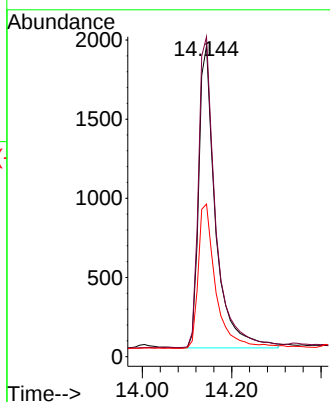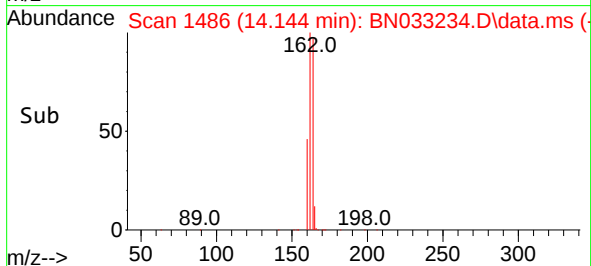

#14

2,4,6-Tribromophenol

Concen: 0.282 ng

RT: 15.686 min Scan# 1628

Delta R.T. -0.030 min

Lab File: BN033234.D

Acq: 03 Aug 2024 12:12




Tgt Ion:330 Resp: 602


Ion Ratio Lower Upper

330 100

332 98.0 77.8 116.8

141 55.5 34.2 51.2#

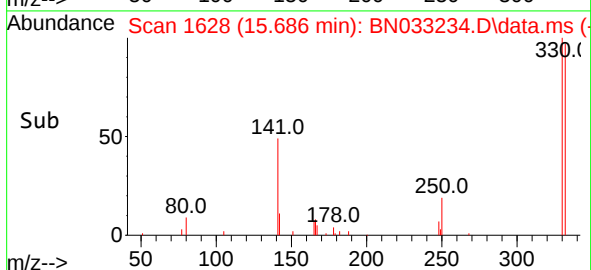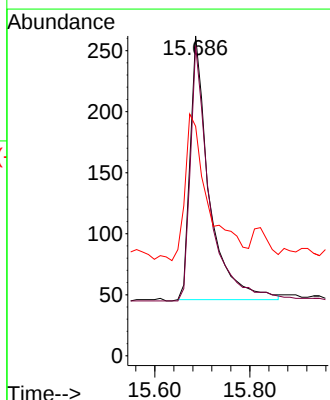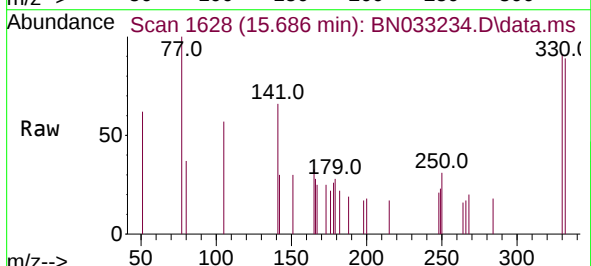

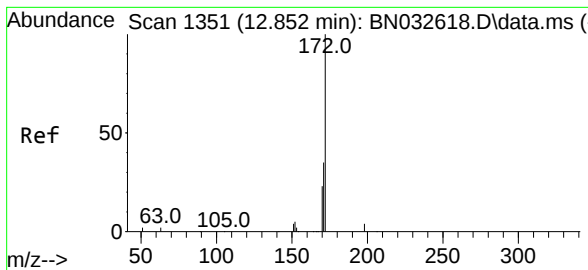

#15
2-Fluorobiphenyl
Concen: 0.289 ng
RT: 12.775 min Scan# 11
Delta R.T. -0.014 min
Lab File: BN033234.D
Acq: 03 Aug 2024 12:12

Instrument :

BNA_N

ClientSampleId :





922-K1-WS-080124

Tgt Ion:172 Resp: 537
Ion Ratio Lower Upper
172 100
171 36.8 28.6 43.0
170 25.9 19.0 28.6

Manual Integrations




APPROVED


Reviewed By :Jagrut Upadhyay 08/05/2024
Supervised By :mohammad ahmed 08/07/2024

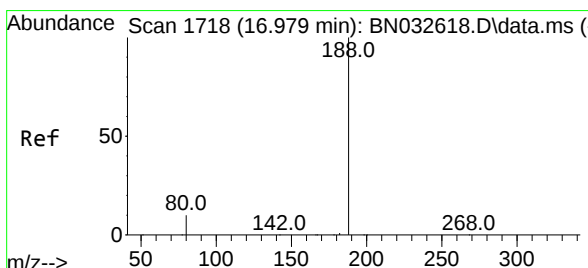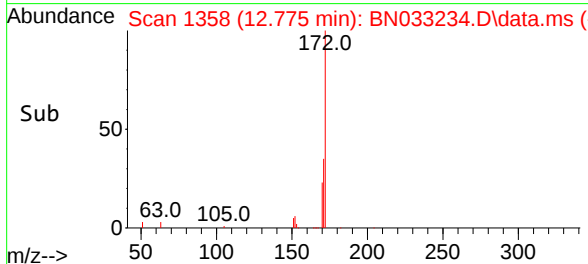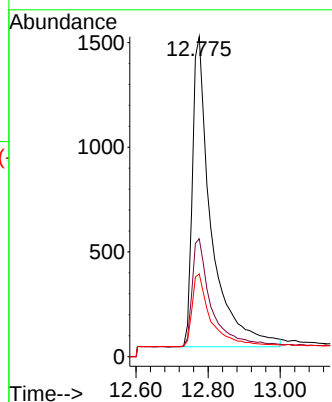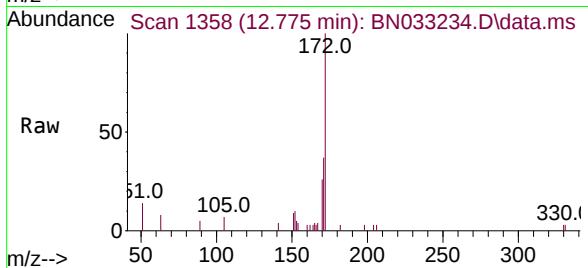

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.915 min Scan# 1727
Delta R.T. -0.005 min
Lab File: BN033234.D
Acq: 03 Aug 2024 12:12


Tgt Ion:188 Resp: 10648
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.4 8.8 13.2

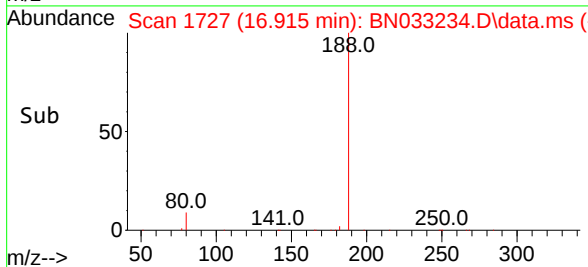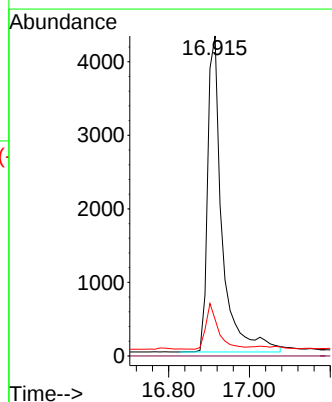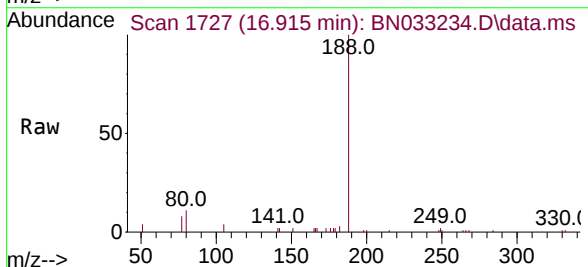

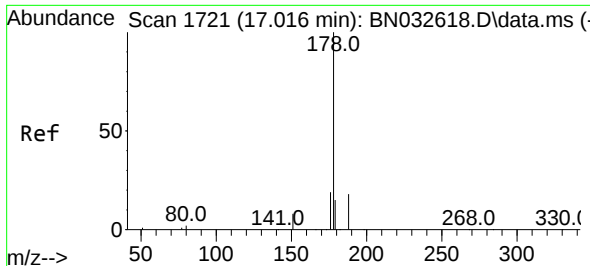

#25
Phenanthrene
Concen: 0.033 ng
RT: 16.952 min Scan# 1721
Delta R.T. -0.018 min
Lab File: BN033234.D
Acq: 03 Aug 2024 12:12




Instrument :
BNA_N
ClientSampleId :
922-K1-WS-080124

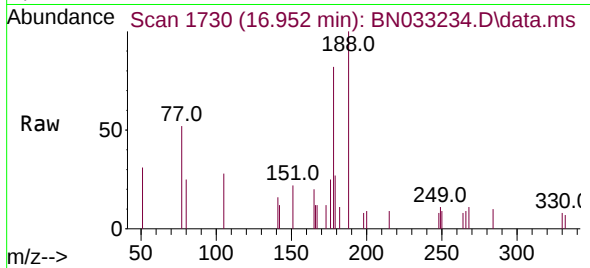

Tgt Ion:178 Resp: 958
Ion Ratio Lower Upper
178 100
176 18.5 15.1 22.7
179 15.0 12.2 18.4




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/05/2024
Supervised By :mohammad ahmed 08/07/2024

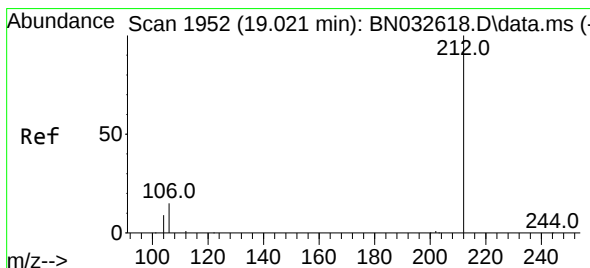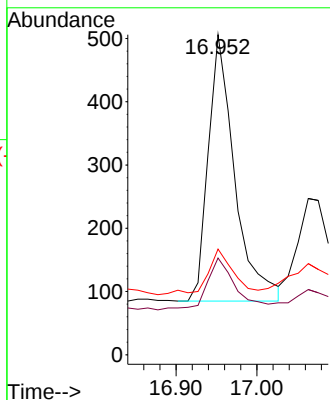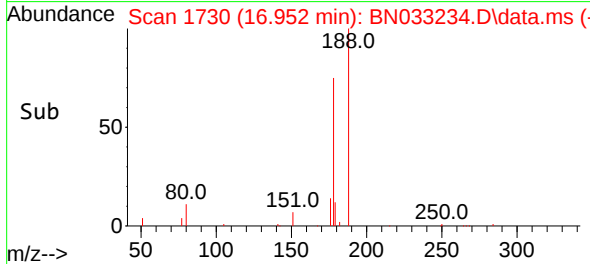

#27
Fluoranthene-d10
Concen: 0.342 ng
RT: 18.953 min Scan# 1950
Delta R.T. -0.007 min
Lab File: BN033234.D
Acq: 03 Aug 2024 12:12


Tgt Ion:212 Resp: 9419
Ion Ratio Lower Upper
212 100
106 15.5 11.9 17.9
104 9.8 6.9 10.3

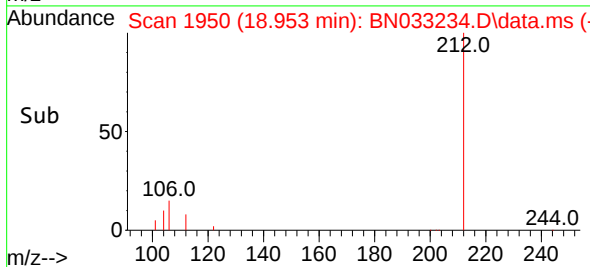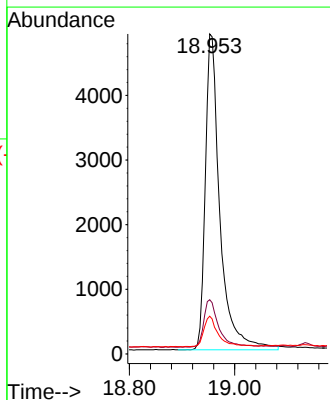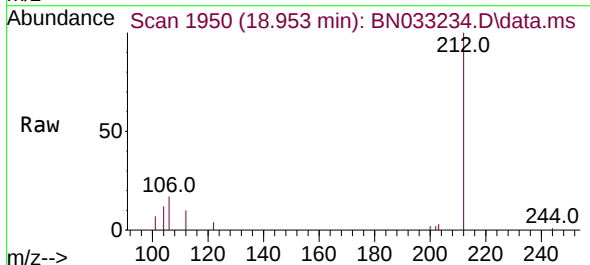

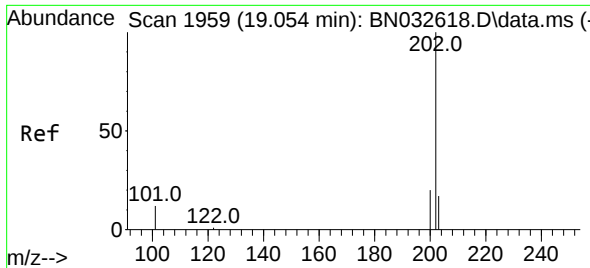

#28
Fluoranthene
Concen: 0.040 ng
RT: 18.990 min Scan# 1959
Delta R.T. -0.002 min
Lab File: BN033234.D
Acq: 03 Aug 2024 12:12




Instrument :
BNA_N
ClientSampleId :
922-K1-WS-080124

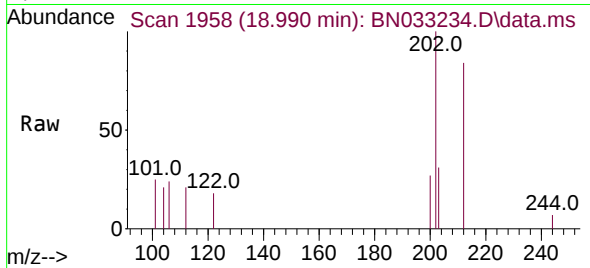

Tgt Ion:202 Resp: 1410
Ion Ratio Lower Upper
202 100
101 0.0 9.6 14.4
203 20.9 13.8 20.6




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/05/2024
Supervised By :mohammad ahmed 08/07/2024

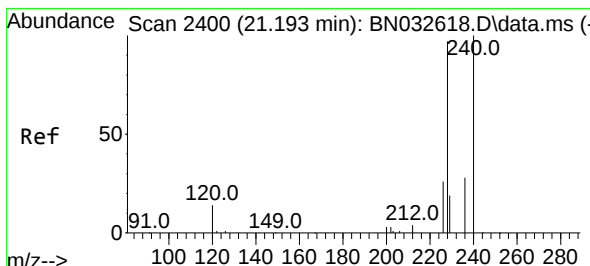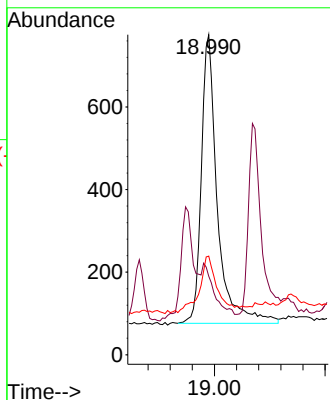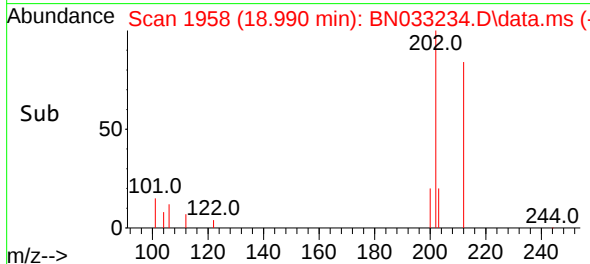

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.131 min Scan# 2406
Delta R.T. -0.002 min
Lab File: BN033234.D
Acq: 03 Aug 2024 12:12

Tgt Ion:240 Resp: 7008
Ion Ratio Lower Upper
240 100
120 22.3 14.8 22.2
236 30.3 23.3 34.9

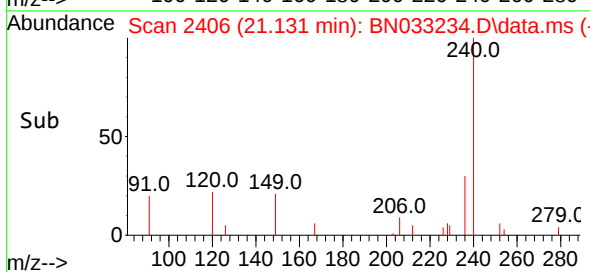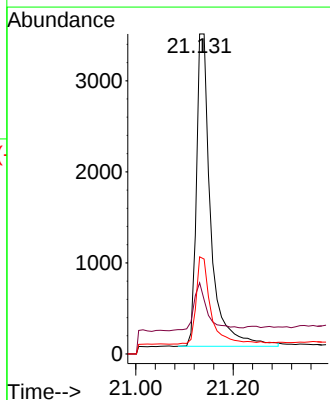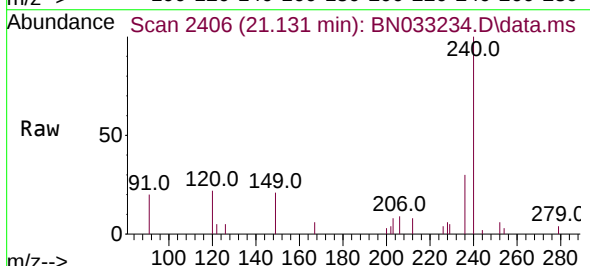

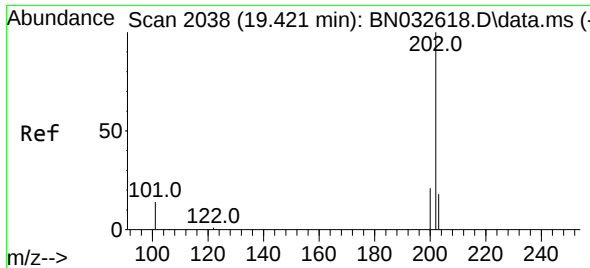





#30
Pyrene
Concen: 0.029 ng
RT: 19.357 min Scan# 2037
Delta R.T. -0.002 min
Lab File: BN033234.D
Acq: 03 Aug 2024 12:12

Instrument :
BNA_N
ClientSampleId :
922-K1-WS-080124

Tgt Ion:202 Resp: 833
Ion Ratio Lower Upper
202 100
200 24.6 16.6 25.0
203 18.5 14.8 22.2




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/05/2024
Supervised By :mohammad ahmed 08/07/2024

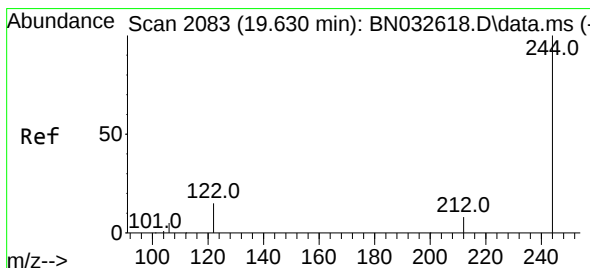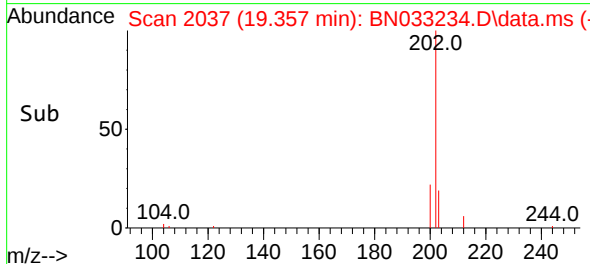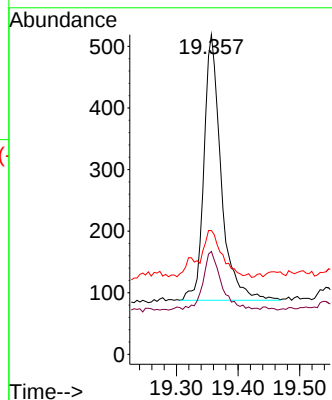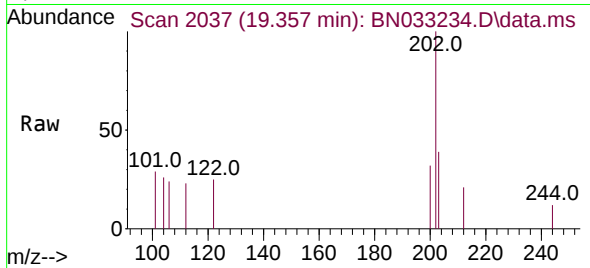

#31
Terphenyl-d14
Concen: 0.594 ng
RT: 19.547 min Scan# 2078
Delta R.T. -0.016 min
Lab File: BN033234.D
Acq: 03 Aug 2024 12:12


Tgt Ion:244 Resp: 8537
Ion Ratio Lower Upper
244 100
212 10.4 7.5 11.3
122 16.7 12.6 19.0

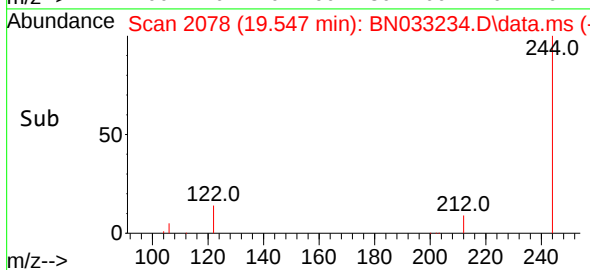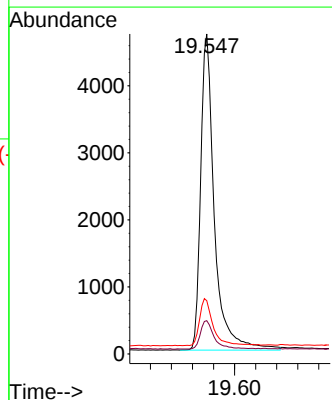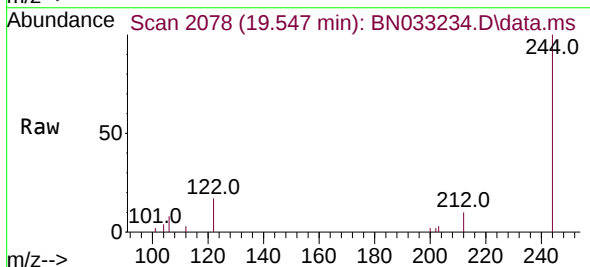

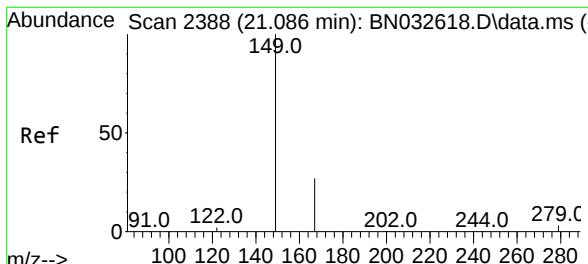

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.255 ng
 RT: 21.006 min Scan# 2100
 Delta R.T. -0.002 min
 Lab File: BN033234.D
 Acq: 03 Aug 2024 12:12

Instrument :
 BNA_N
 ClientSampleId :
 922-K1-WS-080124



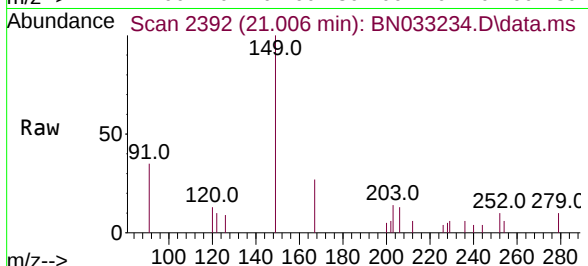


Tgt Ion: 149 Resp: 3125

Ion	Ratio	Lower	Upper
149	100		
167	15.9	21.4	32.2
279	12.8	2.8	4.2

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/05/2024
 Supervised By :mohammad ahmed 08/07/2024

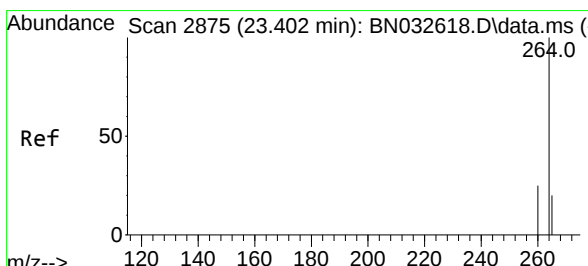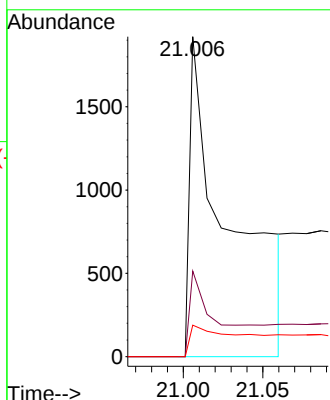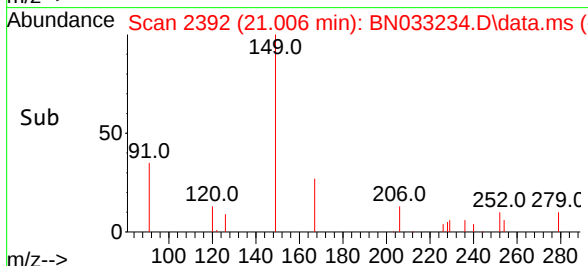

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.312 min Scan# 2857
 Delta R.T. -0.002 min
 Lab File: BN033234.D
 Acq: 03 Aug 2024 12:12

Tgt Ion: 264 Resp: 6904

Ion	Ratio	Lower	Upper
264	100		
260	27.2	20.9	31.3
265	85.2	85.4	128.2

