


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080824\
Data File : BF138855.D
Acq On : 08 Aug 2024 09:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 30 17:50:01 2024

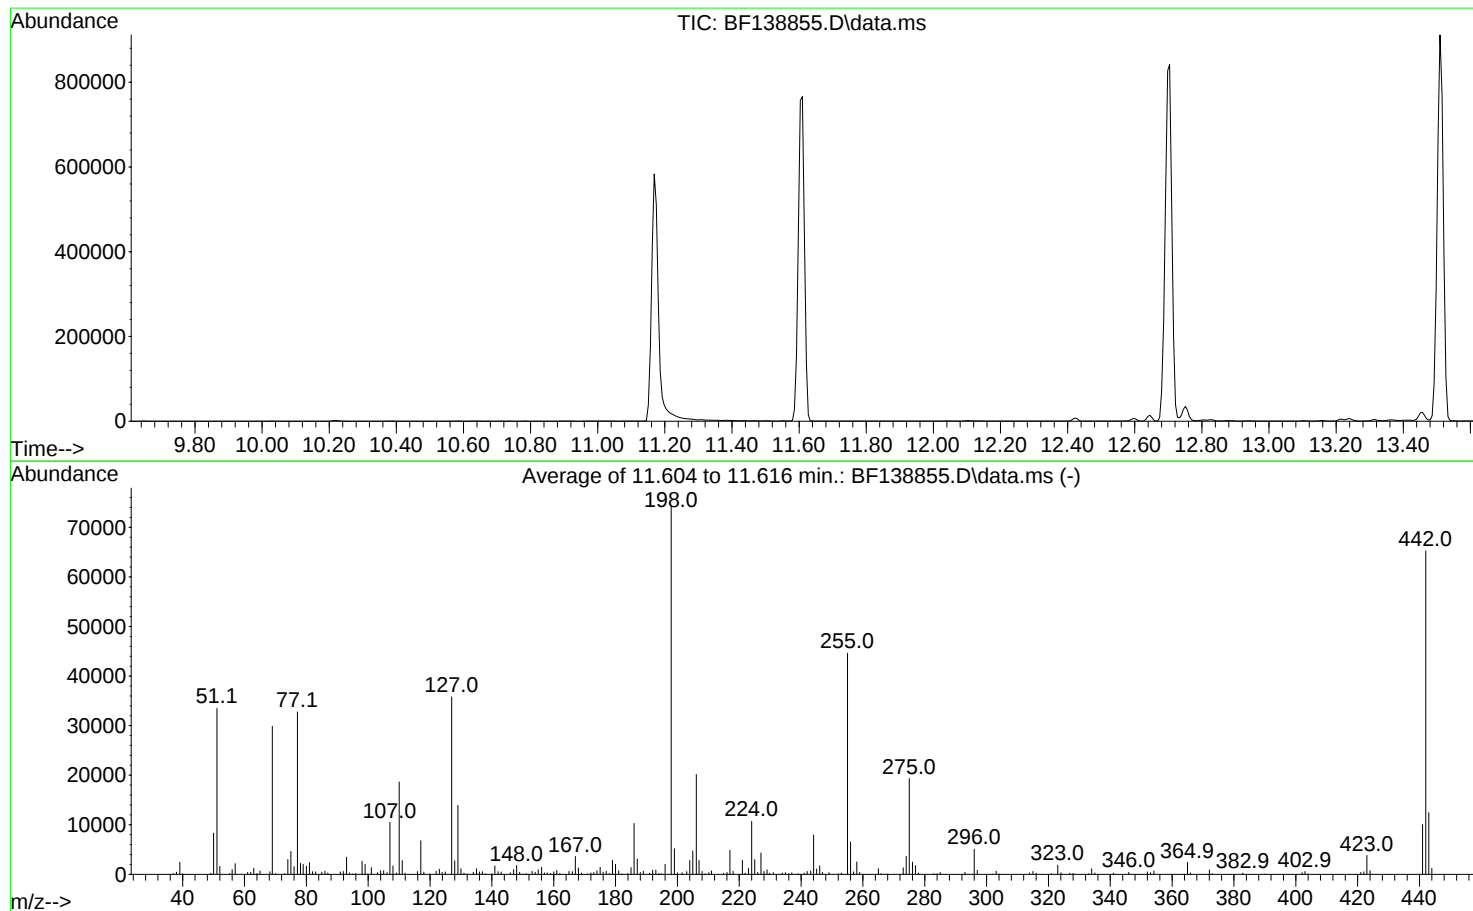

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.1	33485	PASS
68	69	0.00	2	1.8	533	PASS
69	198	0.00	100	40.2	29851	PASS
70	69	0.00	2	0.6	170	PASS
127	198	10	80	48.2	35784	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	74200	PASS
199	198	5	9	7.0	5162	PASS
275	198	10	60	26.1	19335	PASS
365	198	1	100	3.2	2383	PASS
441	198	0.01	100	13.5	10052	PASS
442	442	50	100	100.0	65256	PASS
443	442	15	24	19.1	12449	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/8/2024	BNA_F	<u>BF138855.D</u>
Compound Name	Response	Retention Time
DDT	222446	13.51
DDD	4067	13.239
DDE	545	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4612	227058	2.03

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080824\
Data File : BF138855.D
Acq On : 08 Aug 2024 09:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 08 11:42:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

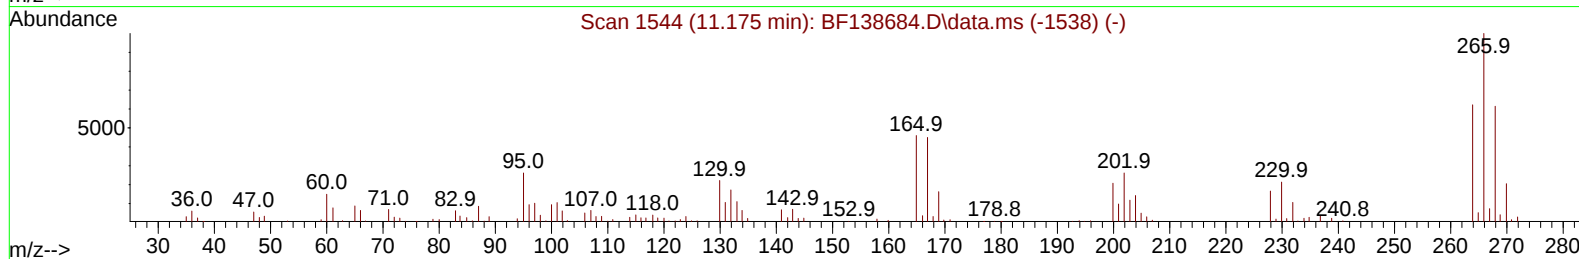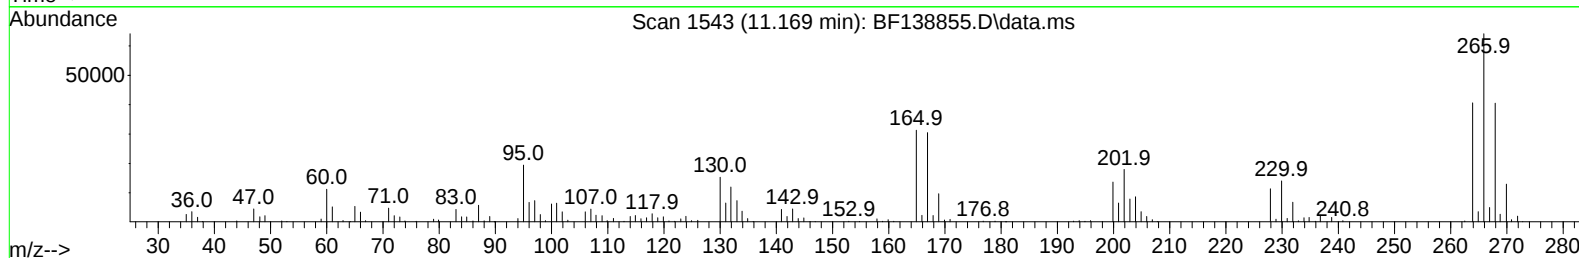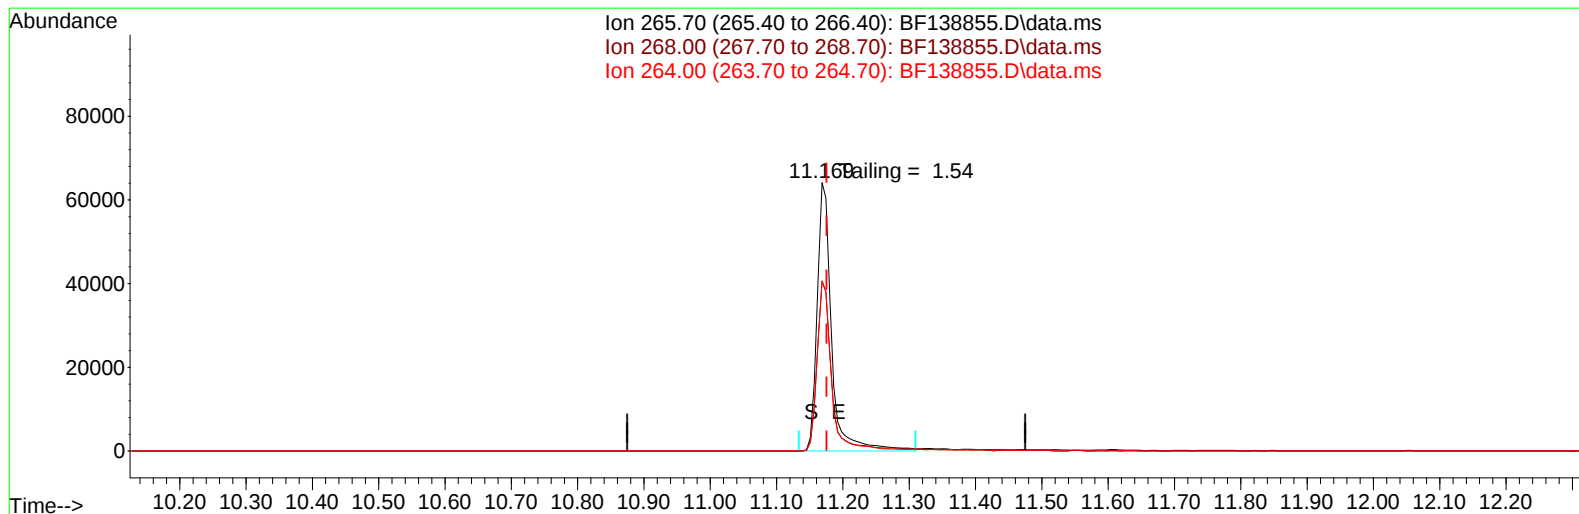

TIC: BF138855.D\data.ms

(70) Pentachlorophenol (C)

11.169min (-0.006) 345616.00 ng




response 97523

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	63.19
264.00	62.20	63.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080824\
Data File : BF138855.D
Acq On : 08 Aug 2024 09:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 08 11:42:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

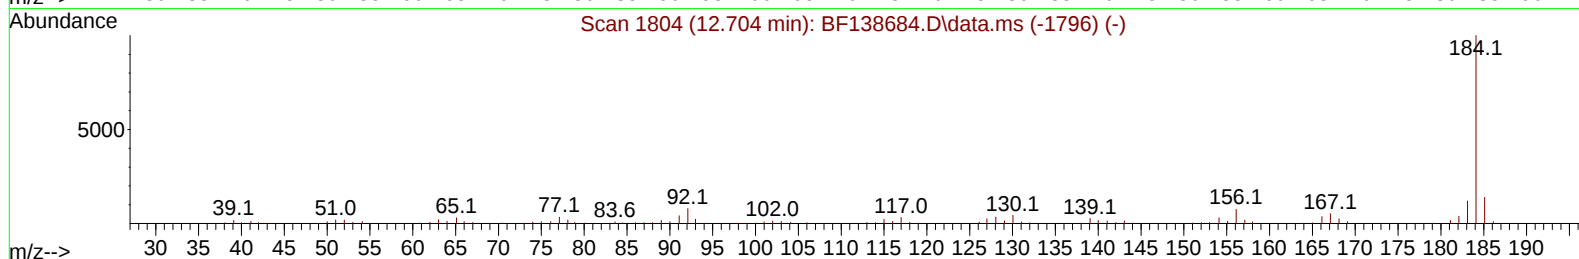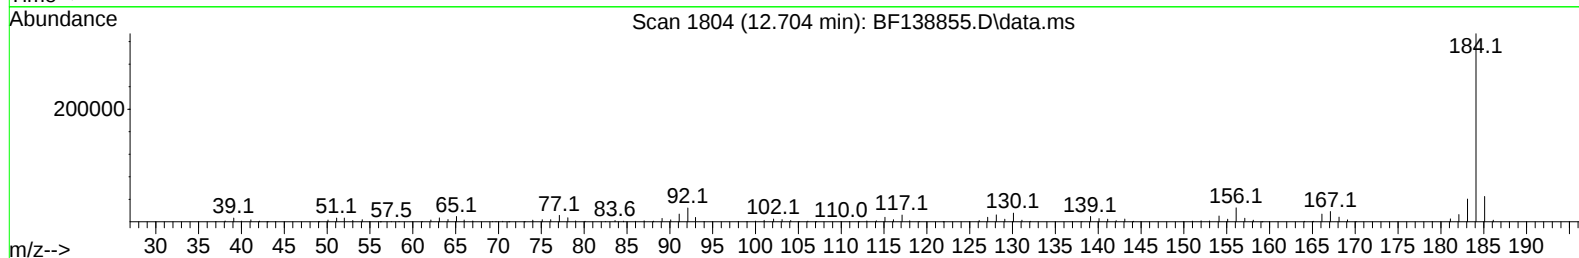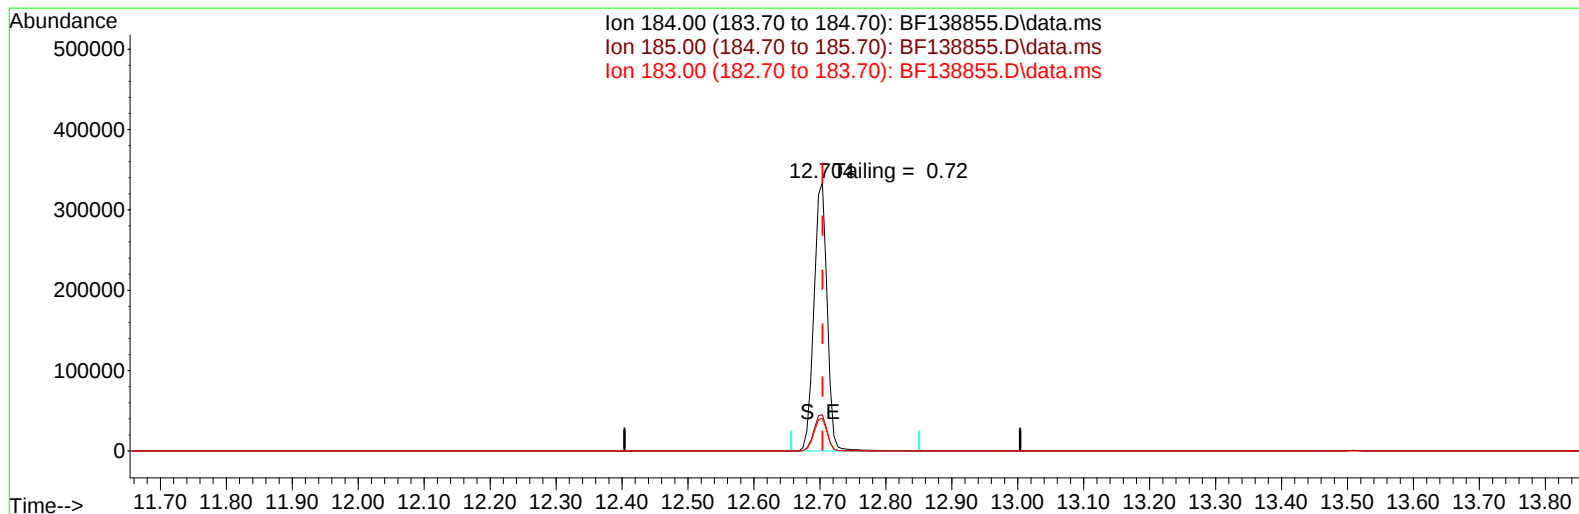

TIC: BF138855.D\data.ms

(77) Benzidine

12.704min (-0.000) 0.00 ng

response 466147

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.51
183.00	12.00	12.16
0.00	0.00	0.00