



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080724\
Data File : VX042876.D
Acq On : 06 Aug 2024 17:07
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080724W.M
Title : SW846 8260
Last Update : Wed Aug 07 02:55:22 2024

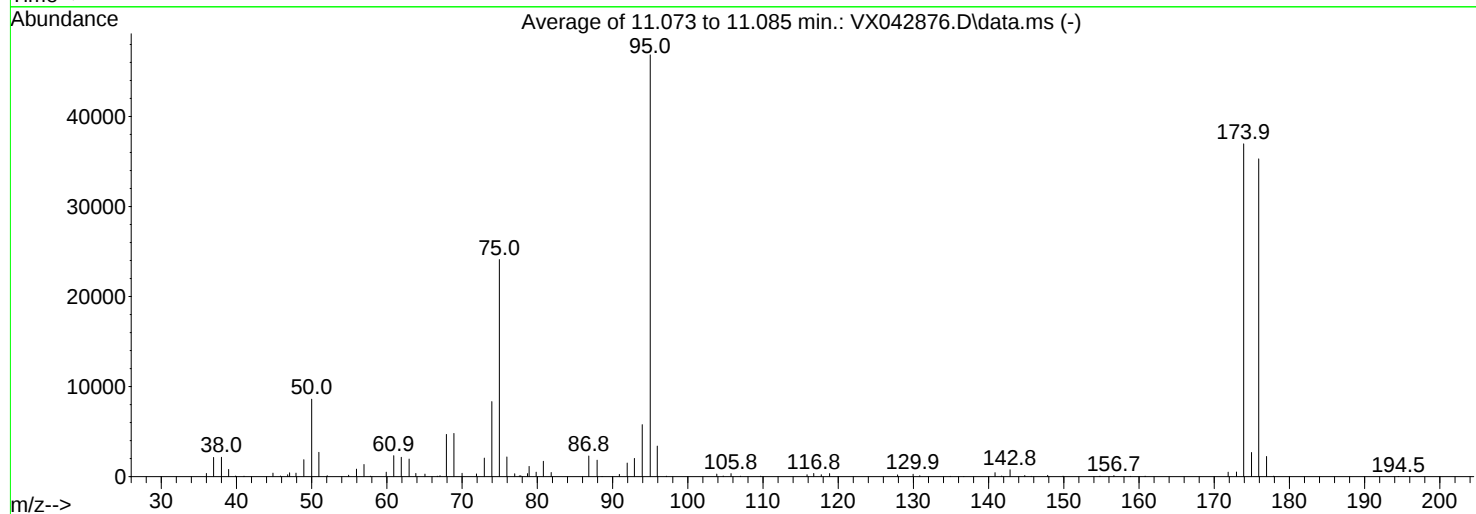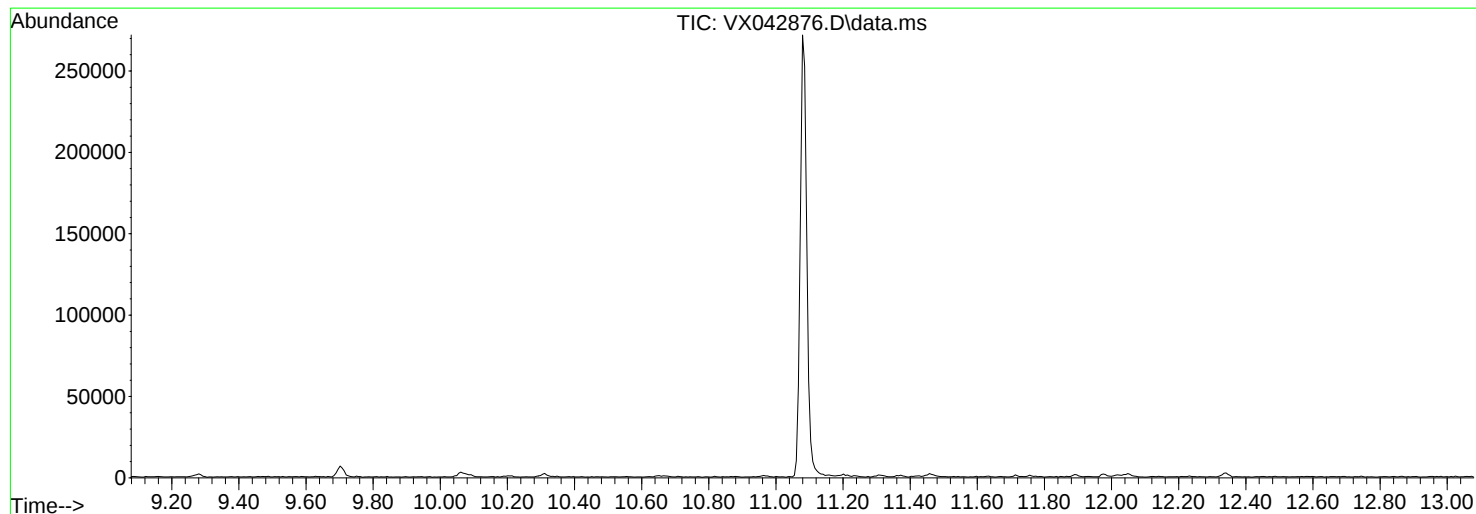

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.4	8600	PASS
75	95	30	60	51.5	24104	PASS
95	95	100	100	100.0	46843	PASS
96	95	5	9	7.2	3395	PASS
173	174	0.00	2	1.4	525	PASS
174	95	50	100	78.9	36968	PASS
175	174	5	9	7.3	2689	PASS
176	174	95	101	95.5	35291	PASS
177	176	5	9	6.4	2247	PASS