
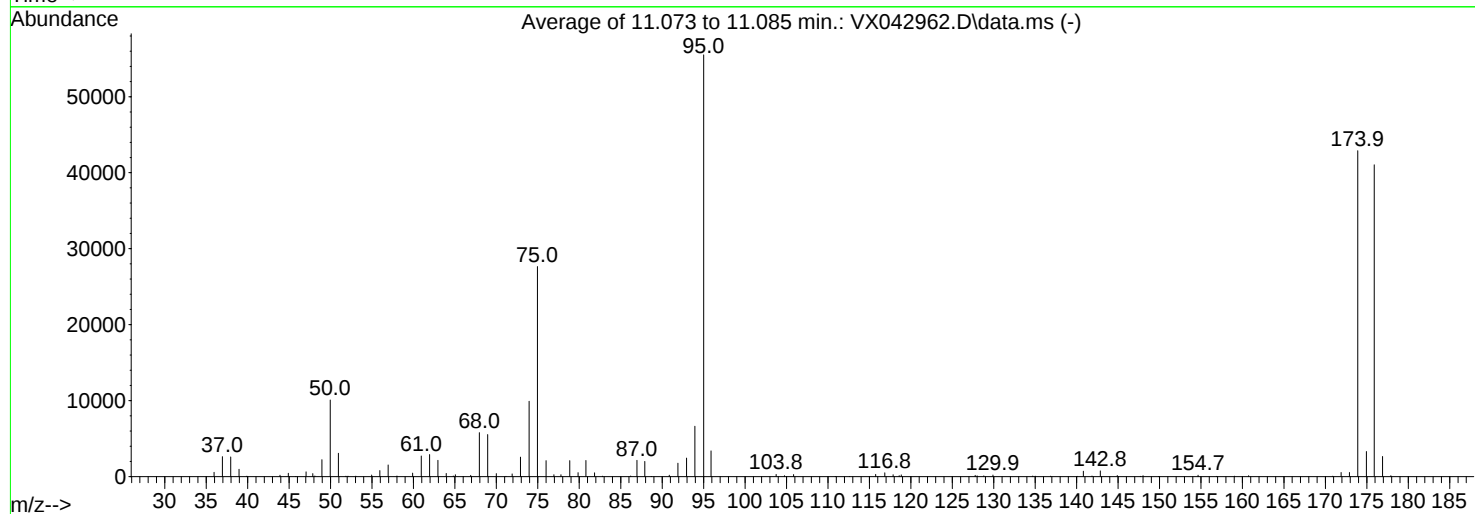


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080824\
Data File : VX042962.D
Acq On : 08 Aug 2024 23:48
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080724W.M
Title : SW846 8260
Last Update : Wed Aug 07 02:55:22 2024

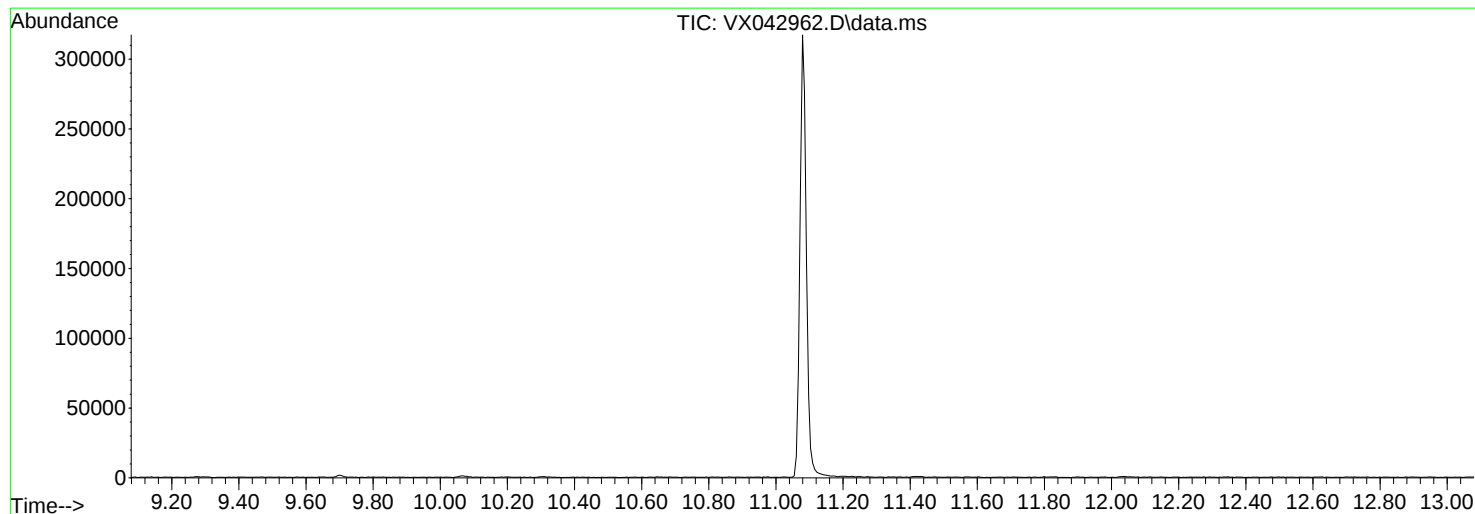

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.2	10082	PASS
75	95	30	60	49.8	27645	PASS
95	95	100	100	100.0	55512	PASS
96	95	5	9	6.1	3397	PASS
173	174	0.00	2	1.3	540	PASS
174	95	50	100	77.3	42891	PASS
175	174	5	9	7.7	3316	PASS
176	174	95	101	95.7	41043	PASS
177	176	5	9	6.5	2657	PASS