


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073024\
Data File : BF138679.D
Acq On : 30 Jul 2024 12:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 30 17:50:01 2024

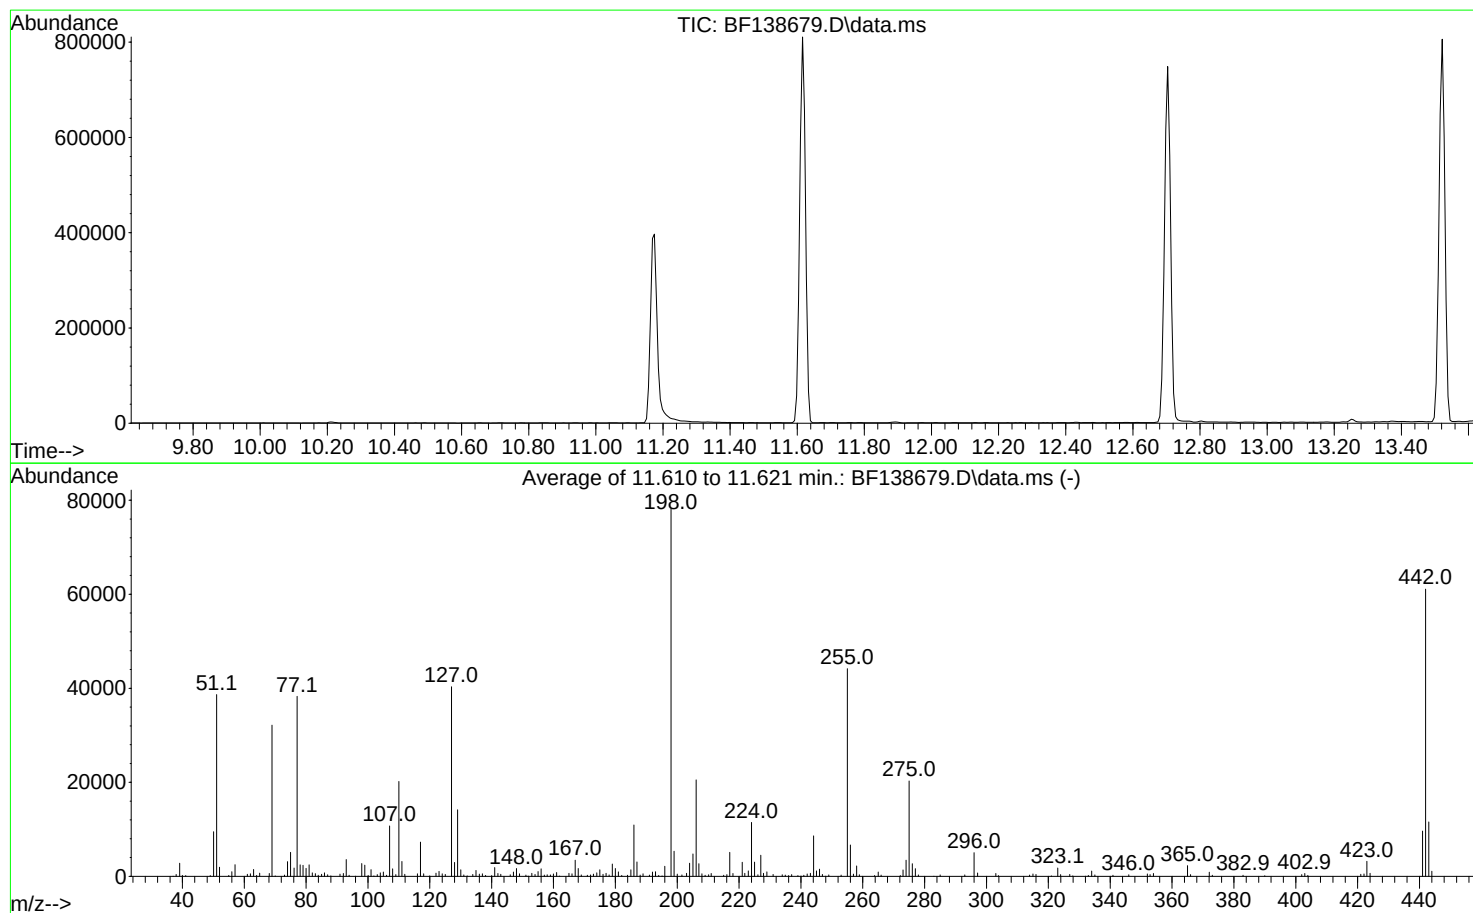




AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1612

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	49.4	38677	PASS
68	69	0.00	2	1.9	605	PASS
69	198	0.00	100	41.1	32171	PASS
70	69	0.00	2	0.4	120	PASS
127	198	10	80	51.5	40312	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	78240	PASS
199	198	5	9	6.8	5335	PASS
275	198	10	60	25.9	20277	PASS
365	198	1	100	2.9	2288	PASS
441	198	0.01	100	12.3	9630	PASS
442	442	50	100	100.0	61072	PASS
443	442	15	24	18.9	11558	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073024\
Data File : BF138679.D
Acq On : 30 Jul 2024 12:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 30 18:29:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

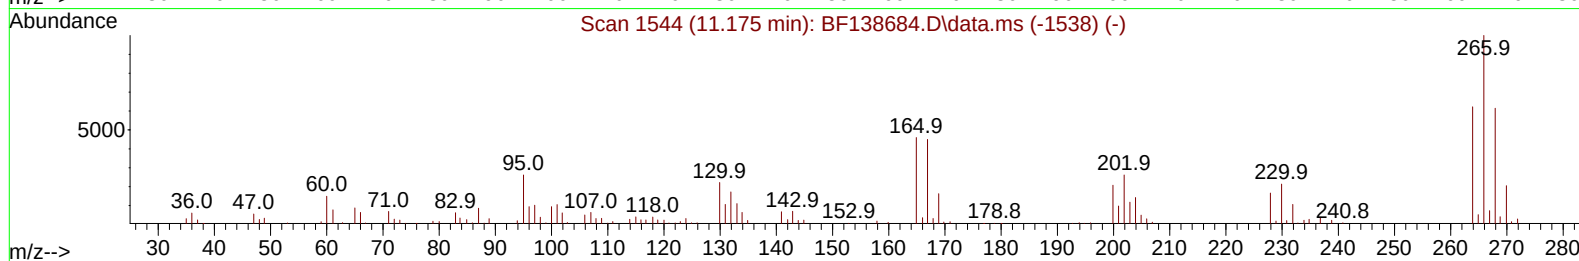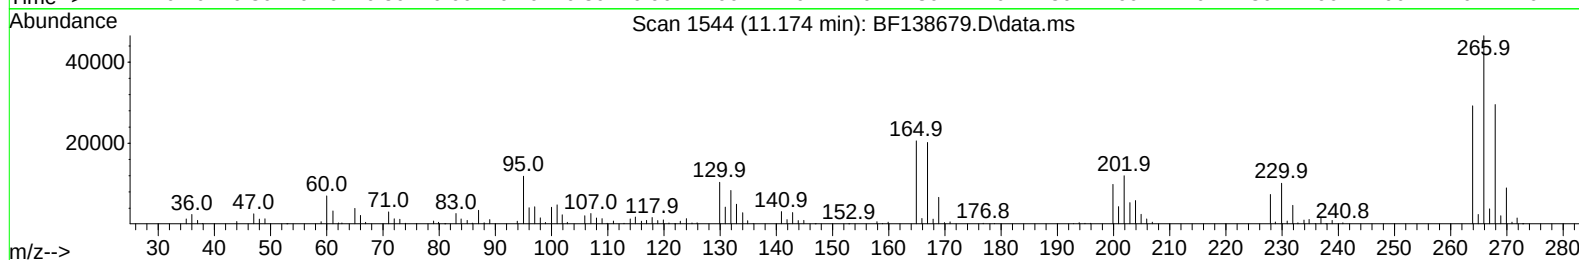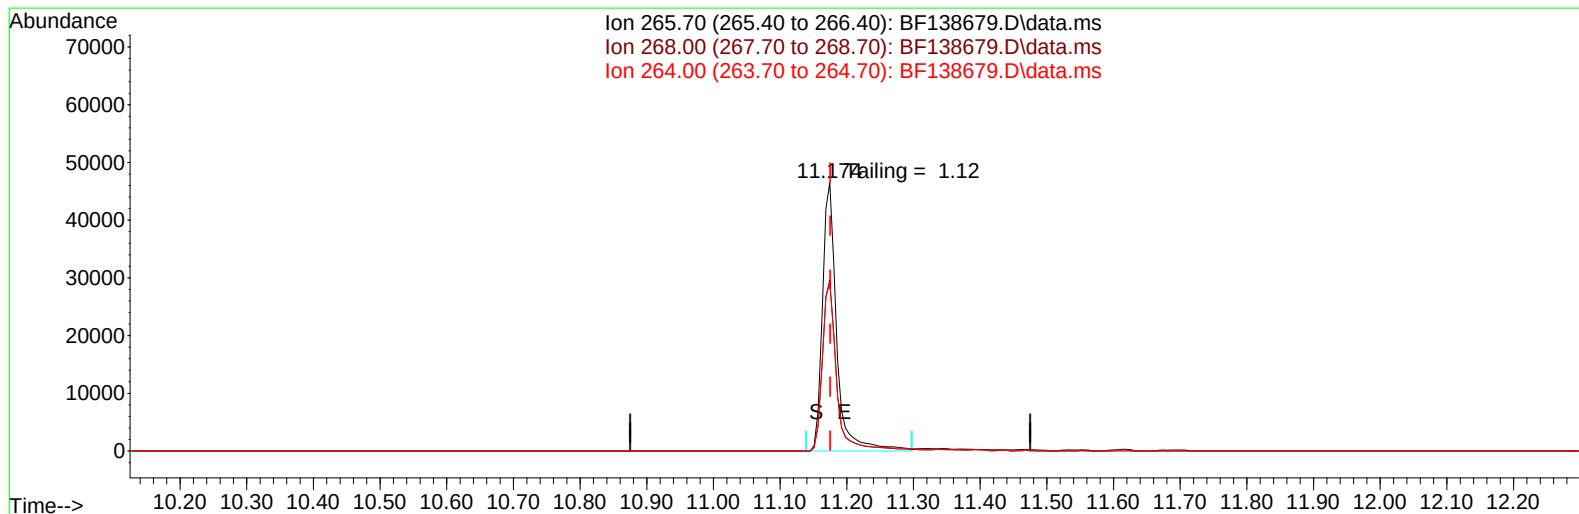

TIC: BF138679.D\data.ms

(70) Pentachlorophenol (C)

11.174min (-0.001) 37845.67 ng




response 69604

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	63.56
264.00	62.20	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073024\
Data File : BF138679.D
Acq On : 30 Jul 2024 12:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 30 18:29:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

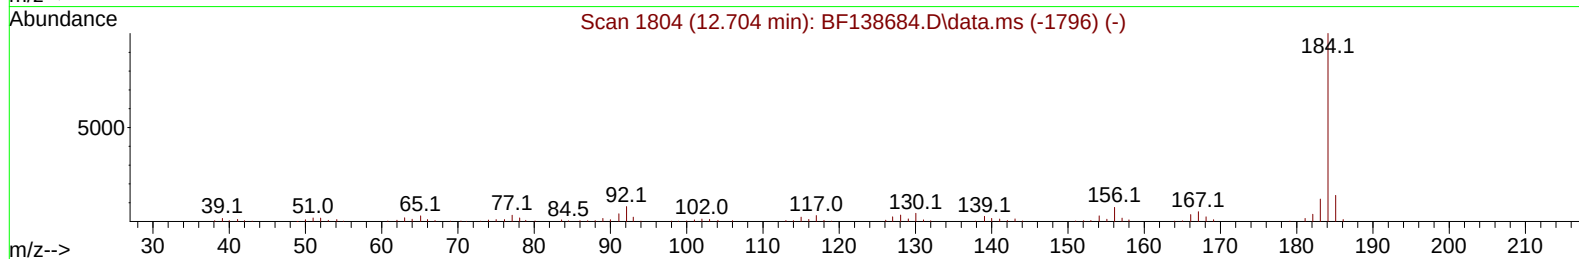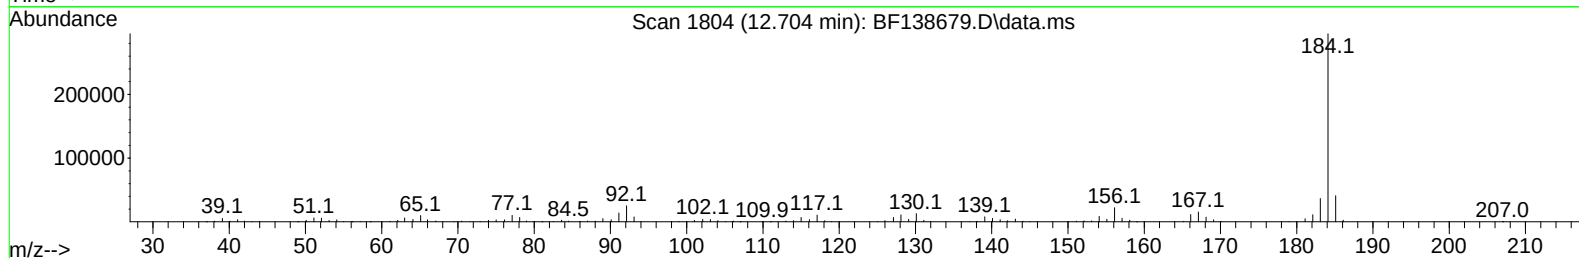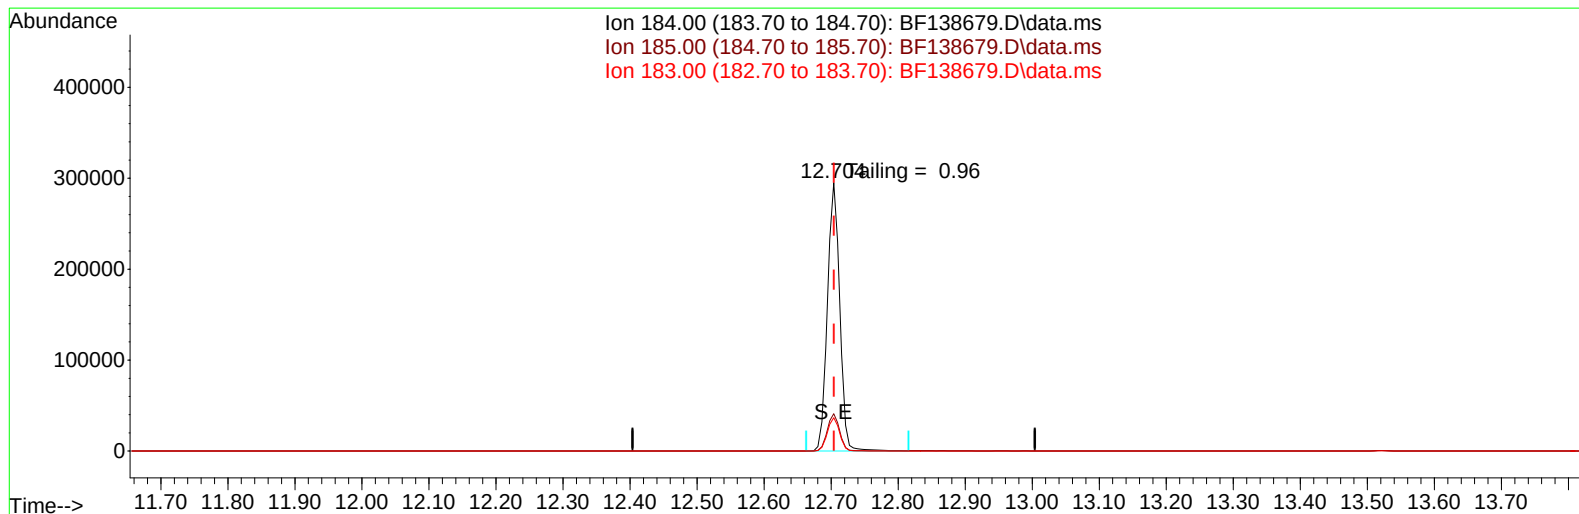

TIC: BF138679.D\data.ms

(77) Benzidine

12.704min (-0.000) 0.00 ng

response 376863

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.91
183.00	12.00	12.39
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/30/2024	BNA_F	<u>BF138679.D</u>
Compound Name	Response	Retention Time
DDT	187682	13.521
DDD	3715	13.251
DDE	369	12.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4084	191766	2.13

Instrument :
BNA_F
ClientSampleId :
DFTPP