
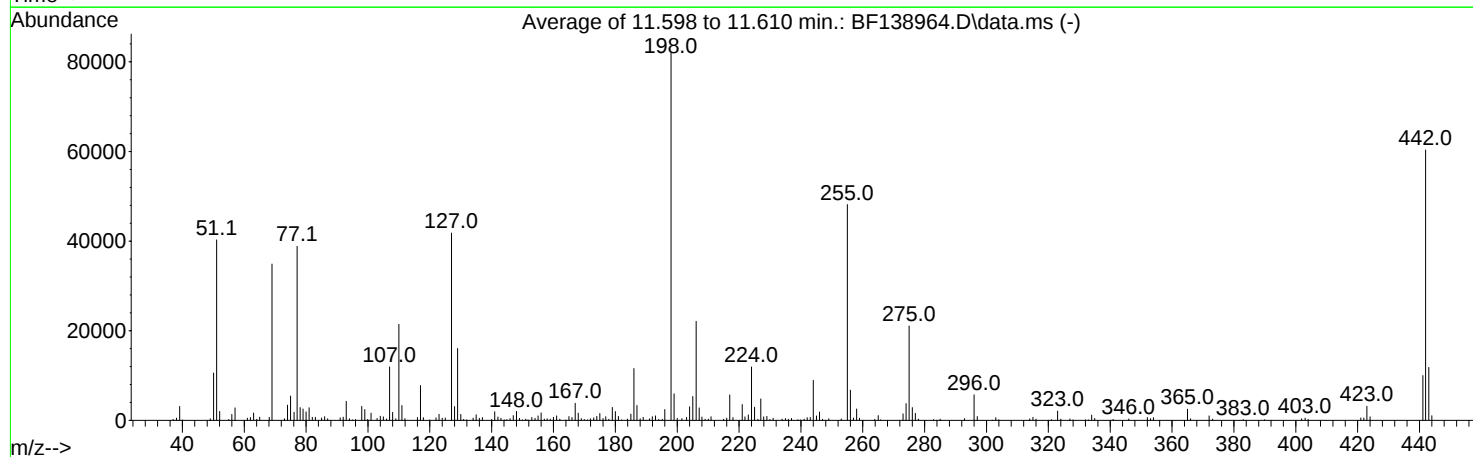


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081324\
Data File : BF138964.D
Acq On : 13 Aug 2024 09:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 30 17:50:01 2024

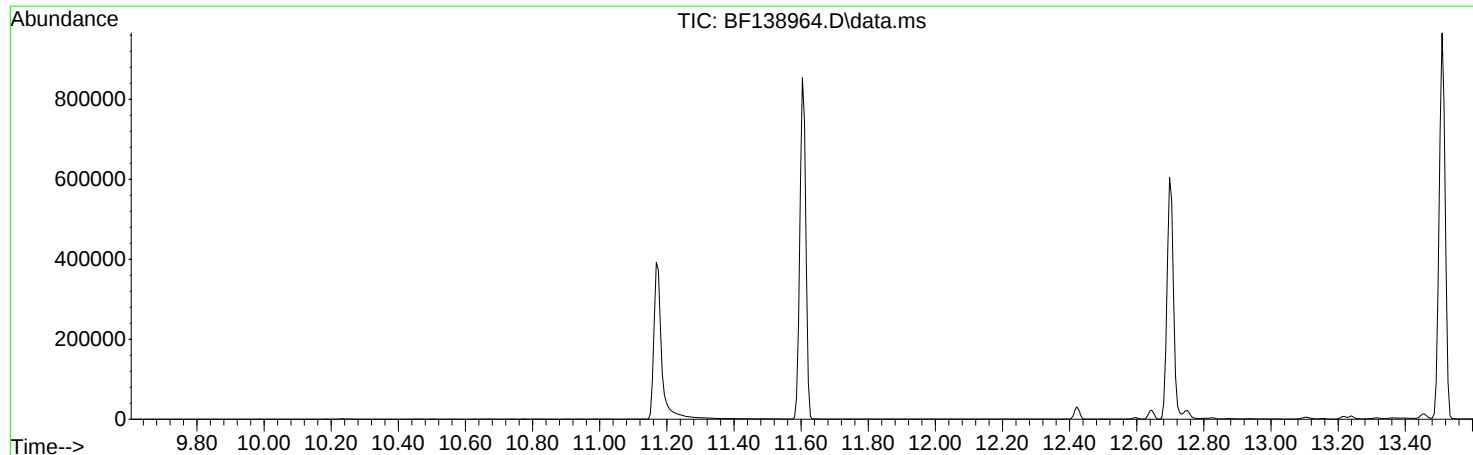

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.1	40267	PASS
68	69	0.00	2	1.9	671	PASS
69	198	0.00	100	42.5	34893	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.9	41821	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	82088	PASS
199	198	5	9	7.2	5919	PASS
275	198	10	60	25.7	21071	PASS
365	198	1	100	3.0	2494	PASS
441	198	0.01	100	12.2	10001	PASS
442	442	50	100	100.0	60347	PASS
443	442	15	24	19.6	11807	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/13/2024	BNA_F	<u>BF138964.D</u>
Compound Name	Response	Retention Time
DDT	230604	13.51
DDD	4887	13.216
DDE	722	12.874
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5609	236213	2.37

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081324\
Data File : BF138964.D
Acq On : 13 Aug 2024 09:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 13 11:45:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

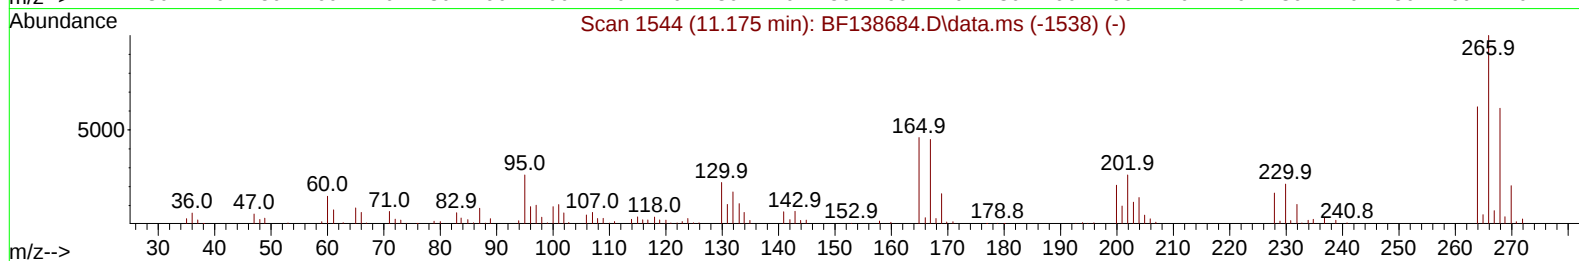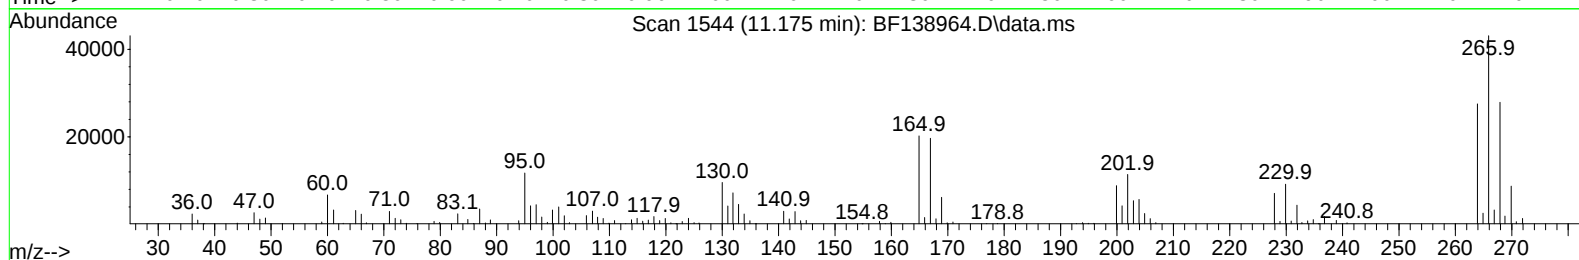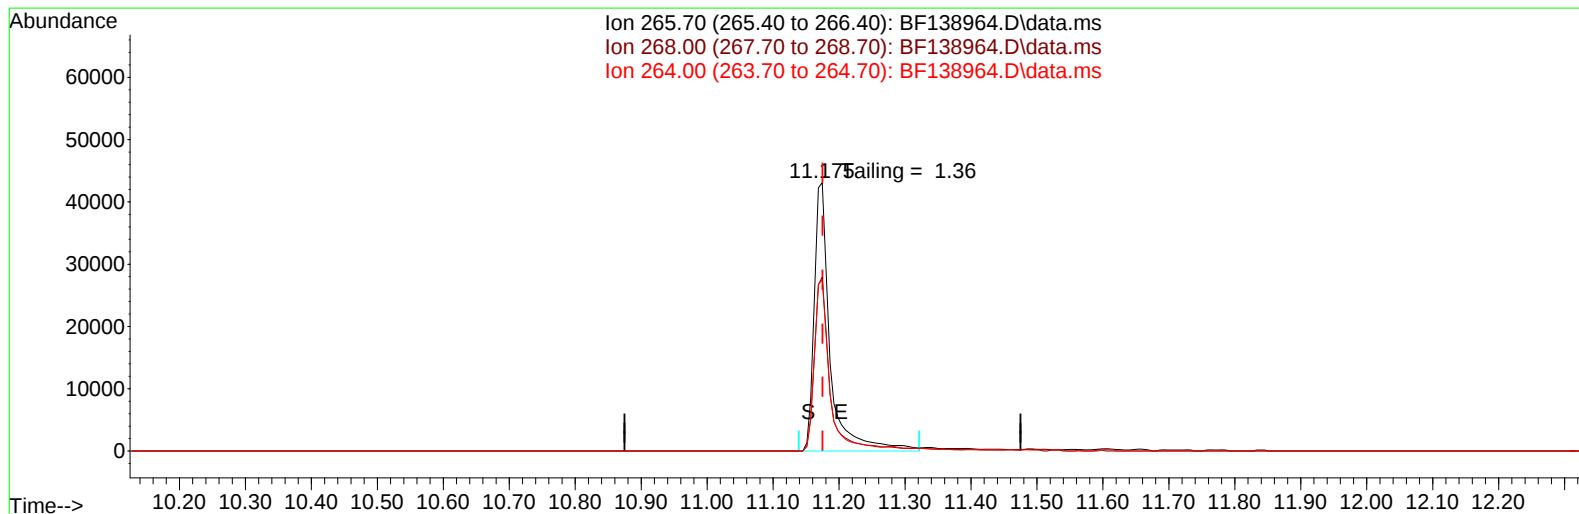

TIC: BF138964.D\data.ms

(70) Pentachlorophenol (C)

11.175min (-0.000) 33750.77 ng




response 73297

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	64.77
264.00	62.20	63.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081324\
Data File : BF138964.D
Acq On : 13 Aug 2024 09:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 13 11:45:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

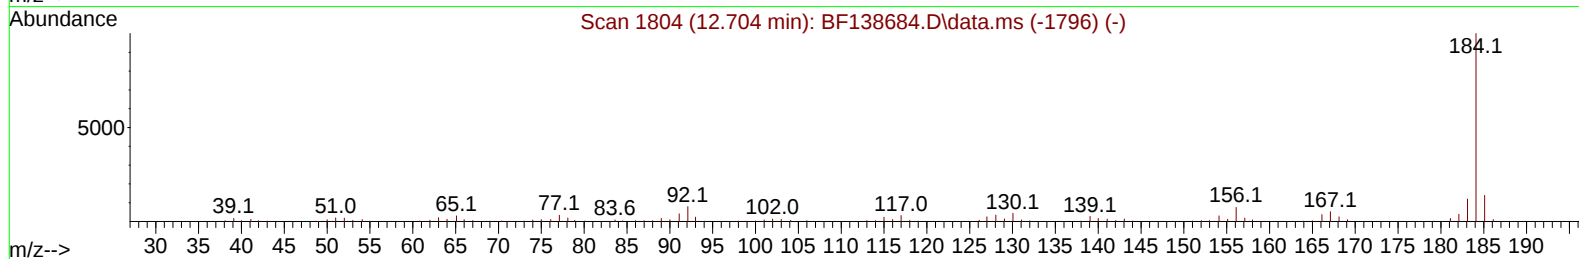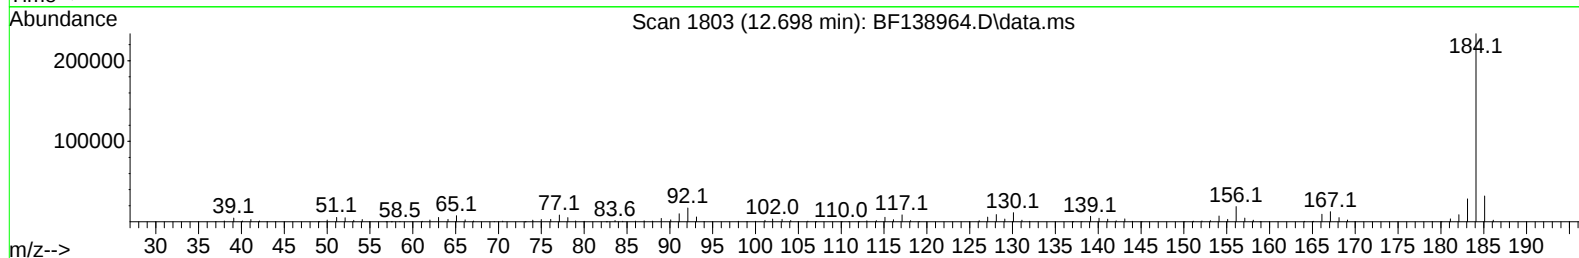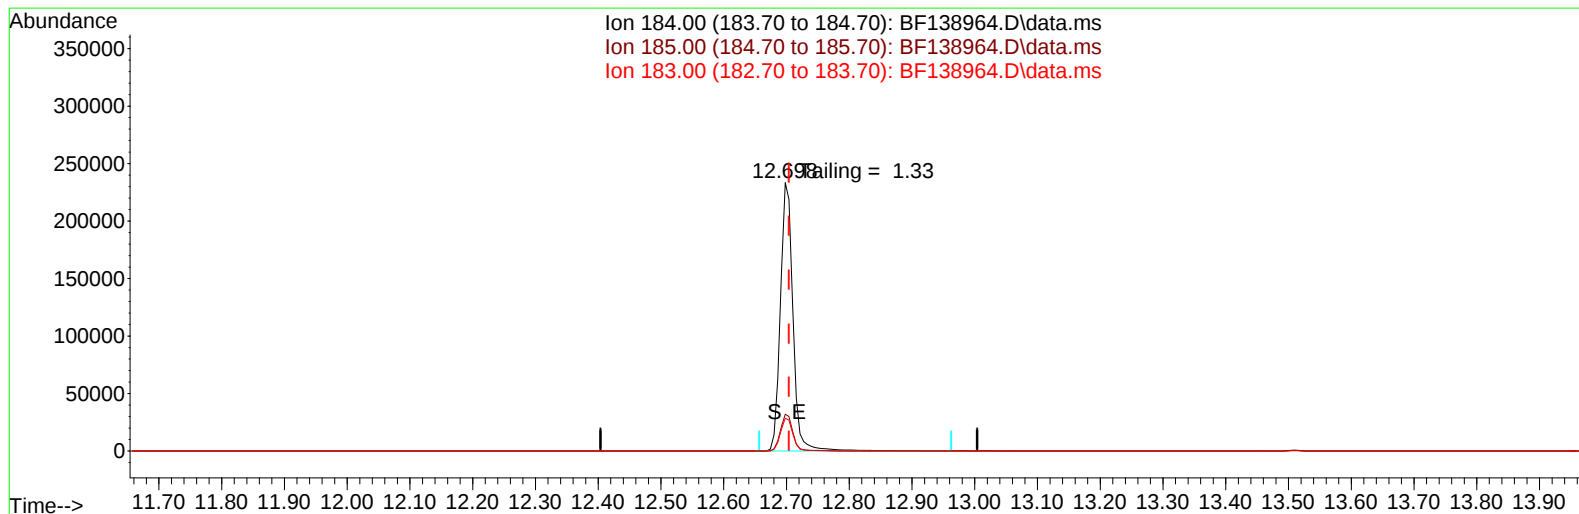

TIC: BF138964.D\data.ms

(77) Benzidine

12.698min (-0.006) 0.00 ng

response 324330

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.74
183.00	12.00	12.25
0.00	0.00	0.00