


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081424\
Data File : BF138987.D
Acq On : 14 Aug 2024 11:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 30 17:50:01 2024

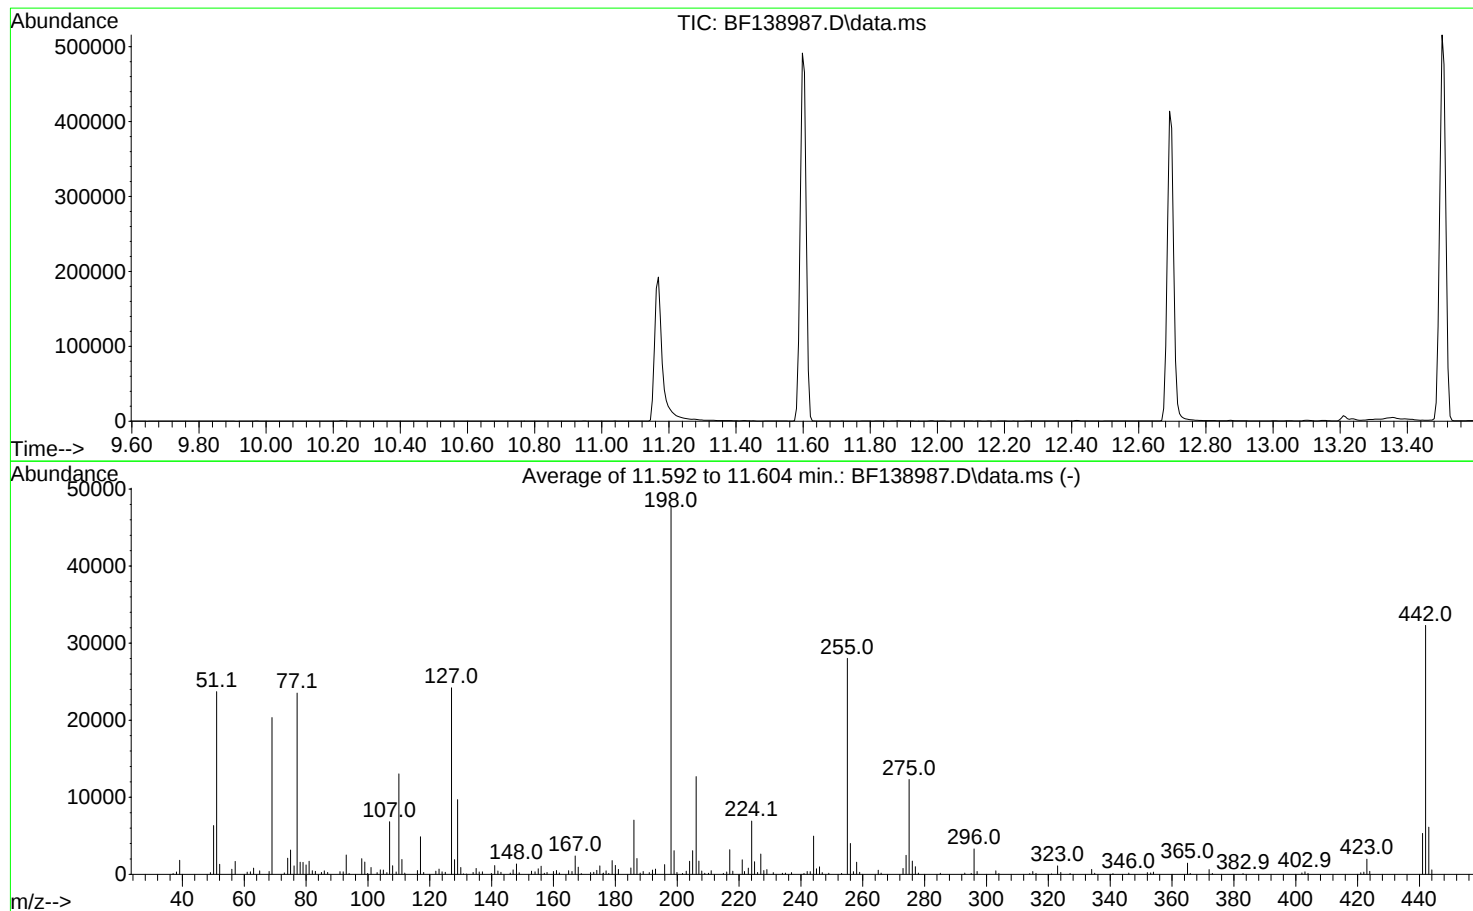

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.7	23707	PASS
68	69	0.00	2	1.8	376	PASS
69	198	0.00	100	42.6	20352	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.7	24208	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	47733	PASS
199	198	5	9	6.4	3077	PASS
275	198	10	60	25.8	12322	PASS
365	198	1	100	3.0	1447	PASS
441	198	0.01	100	11.1	5317	PASS
442	442	50	100	100.0	32304	PASS
443	442	15	24	18.9	6121	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/14/2024	BNA_F	<u>BF138987.D</u>
Compound Name	Response	Retention Time
DDT	122337	13.504
DDD	3496	13.21
DDE	243	12.874
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3739	126076	2.97

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081424\
Data File : BF138987.D
Acq On : 14 Aug 2024 11:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 14 12:15:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

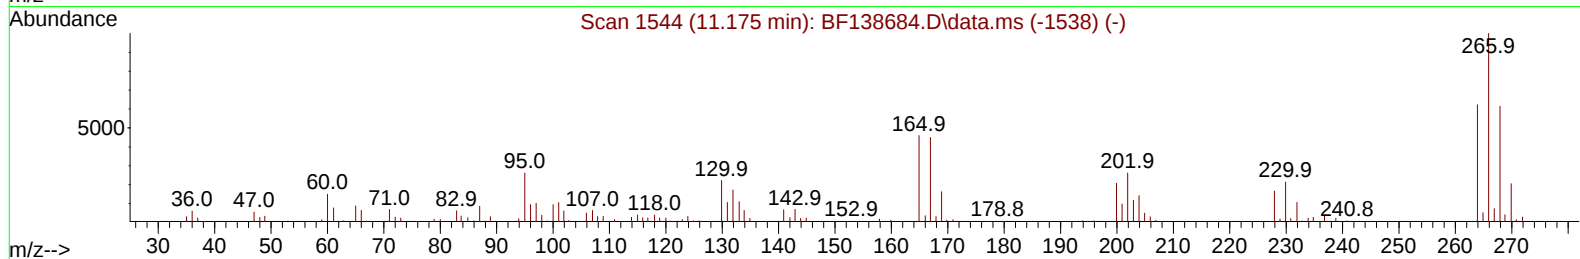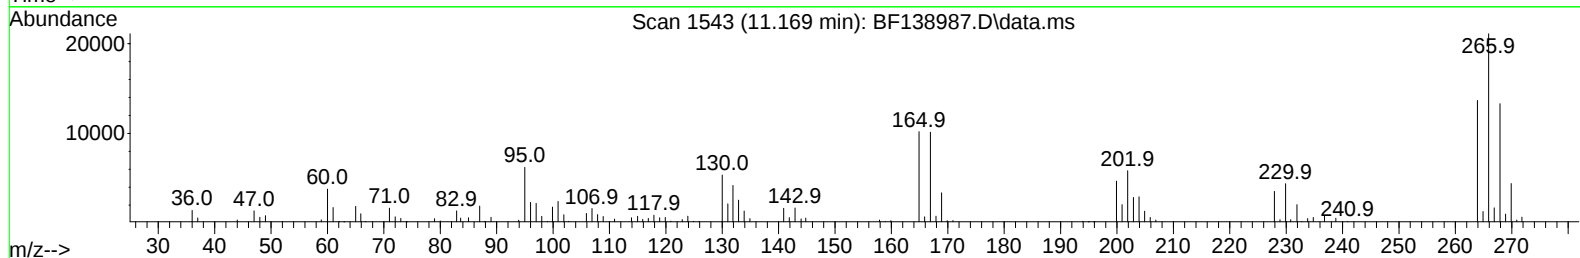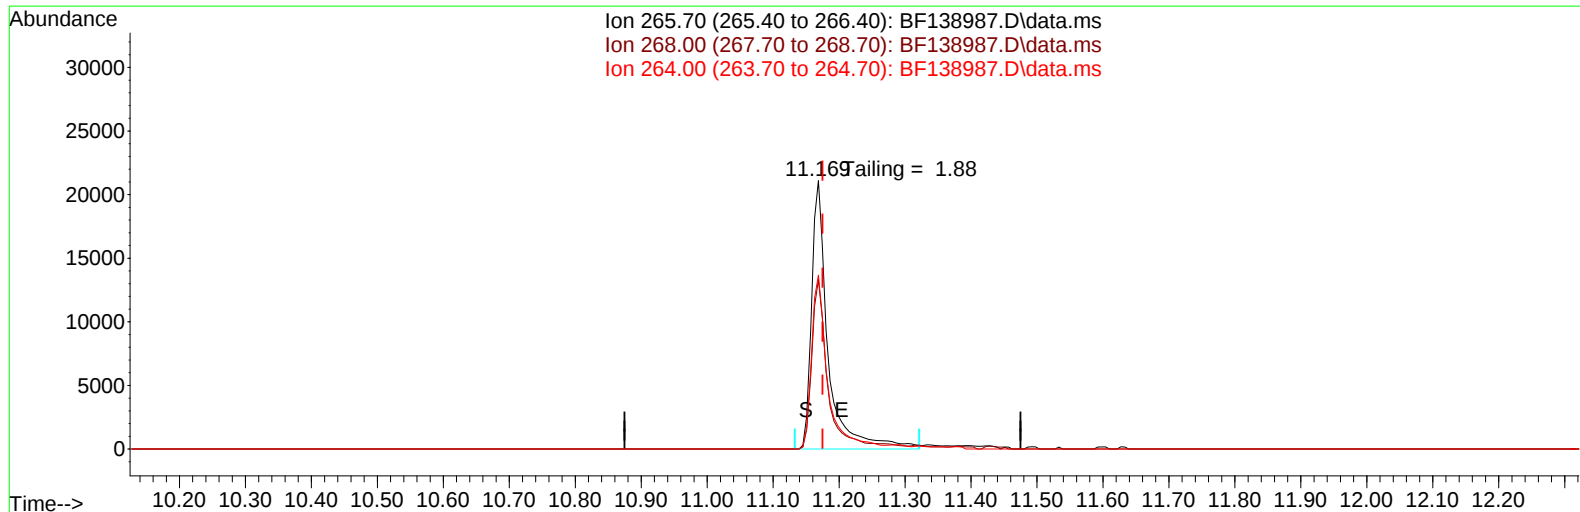

TIC: BF138987.D\data.ms

(70) Pentachlorophenol (C)

11.169min (-0.006) 42832.92 ng




response 37122

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	63.09
264.00	62.20	64.73
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081424\  
Data File : BF138987.D  
Acq On    : 14 Aug 2024  11:33  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 14 12:15:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

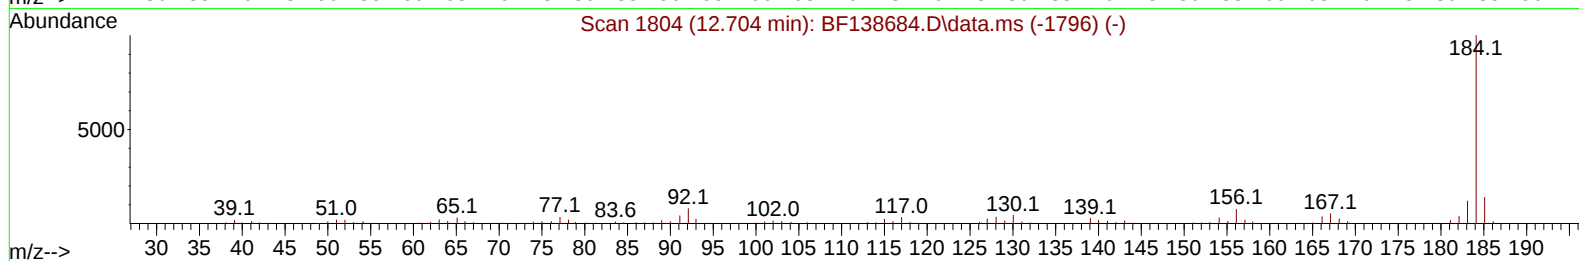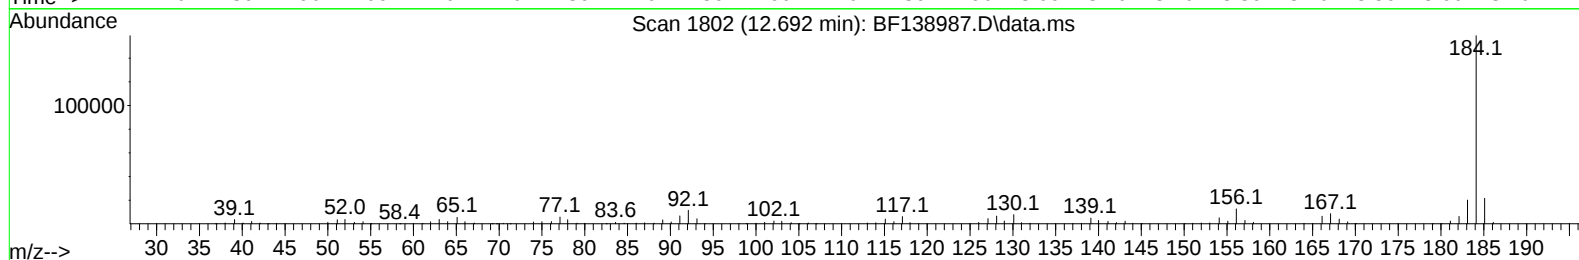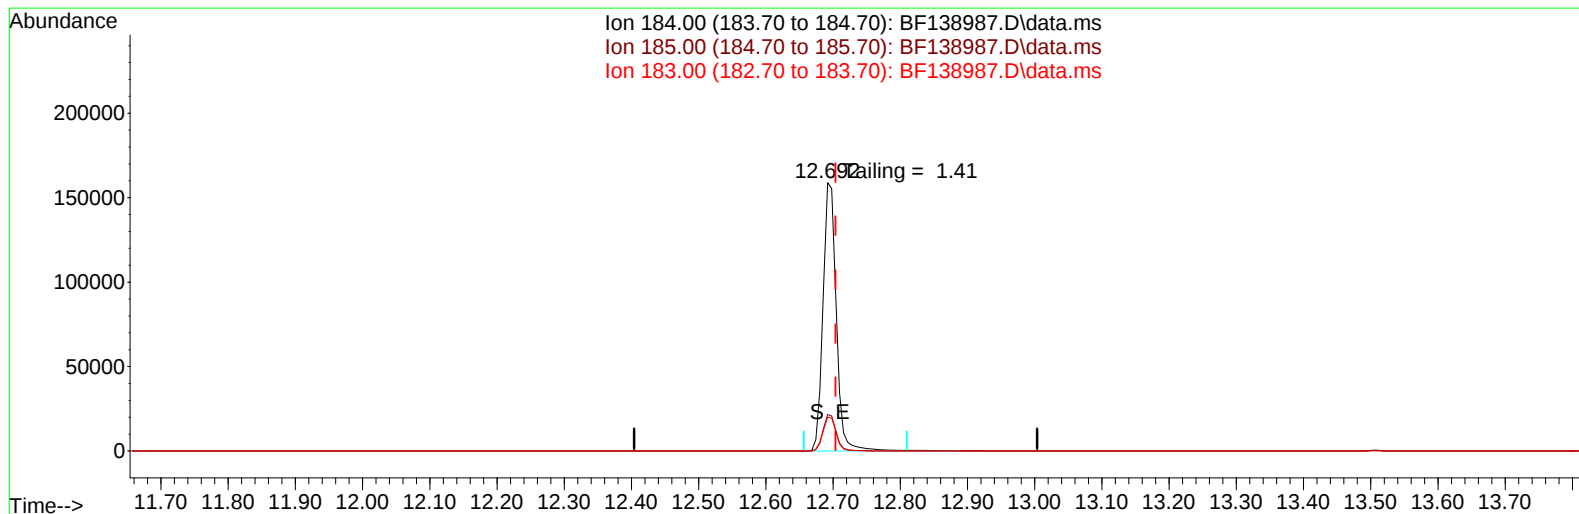

TIC: BF138987.D\data.ms

(77) Benzidine

12.692min (-0.012) 0.00 ng

response **218193**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.59
183.00	12.00	12.68
0.00	0.00	0.00