


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081924\
Data File : BF139064.D
Acq On : 19 Aug 2024 08:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 30 17:50:01 2024

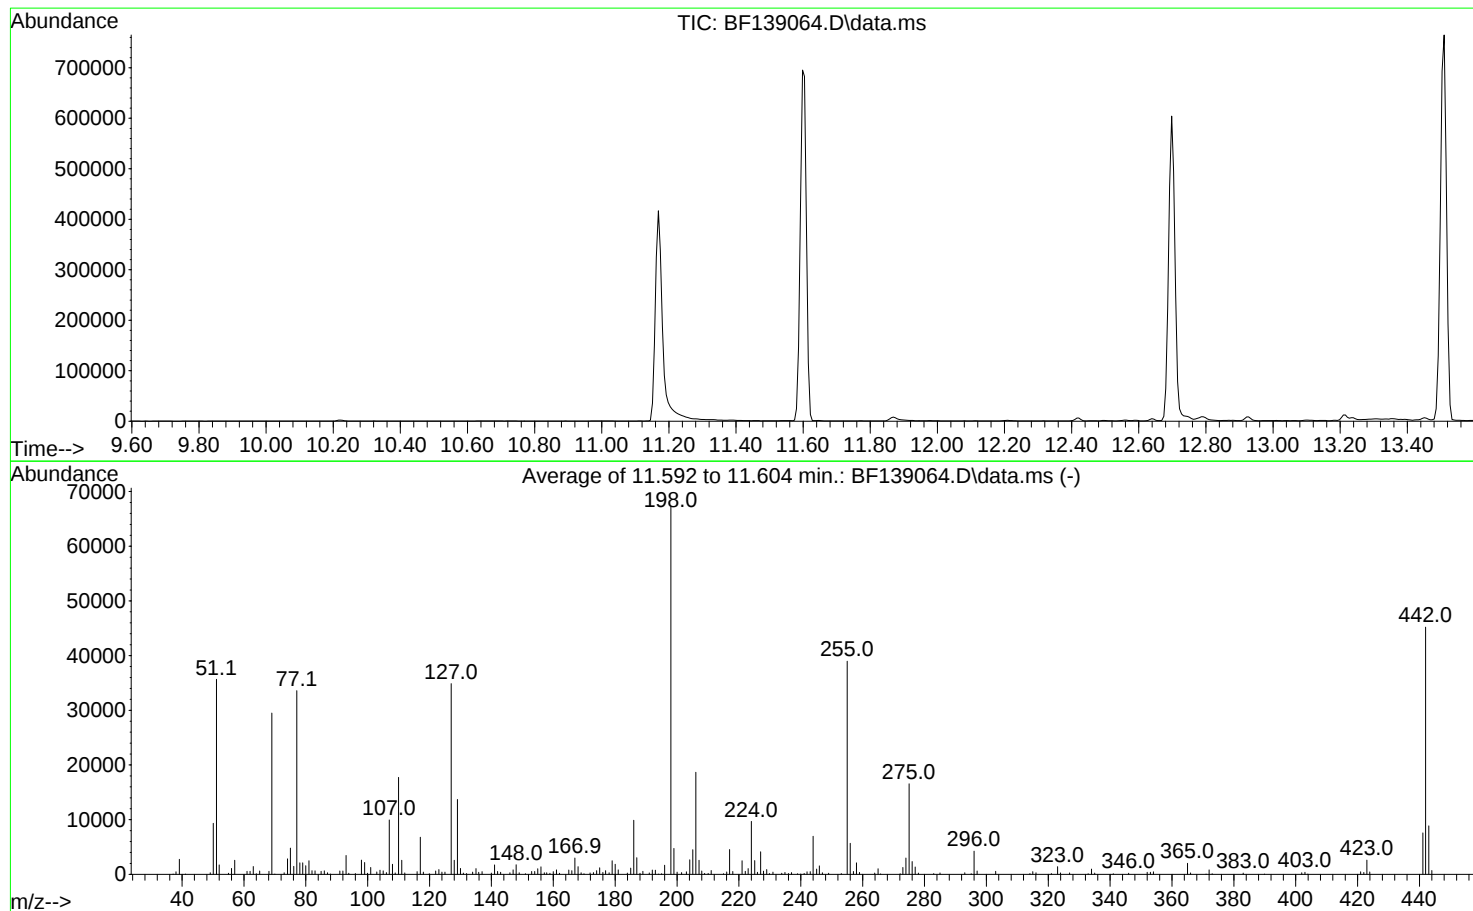

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.0	35667	PASS
68	69	0.00	2	1.9	546	PASS
69	198	0.00	100	43.8	29493	PASS
70	69	0.00	2	0.2	62	PASS
127	198	10	80	51.9	34880	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67267	PASS
199	198	5	9	7.0	4735	PASS
275	198	10	60	24.6	16565	PASS
365	198	1	100	3.0	2022	PASS
441	198	0.01	100	11.3	7575	PASS
442	442	50	100	100.0	45200	PASS
443	442	15	24	19.6	8868	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/19/2024	BNA_F	<u>BF139064.D</u>
Compound Name	Response	Retention Time
DDT	181200	13.51
DDD	5469	13.216
DDE	771	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6240	187440	3.33

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081924\
Data File : BF139064.D
Acq On : 19 Aug 2024 08:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 19 11:09:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

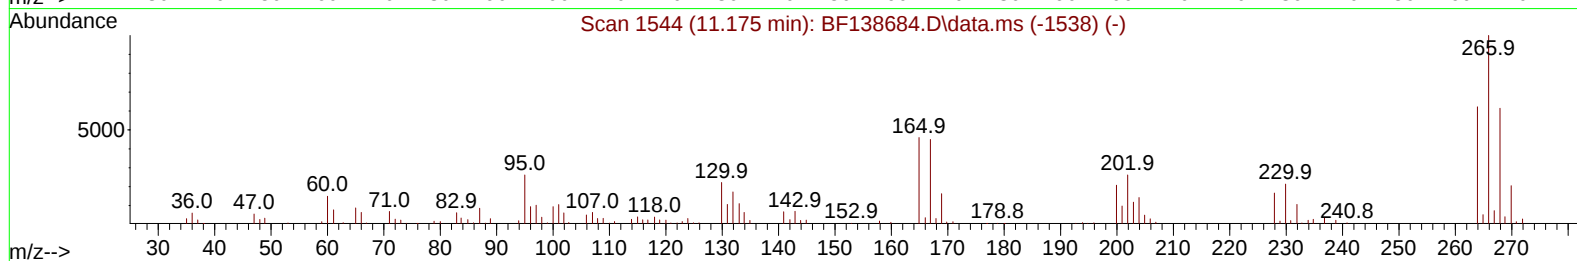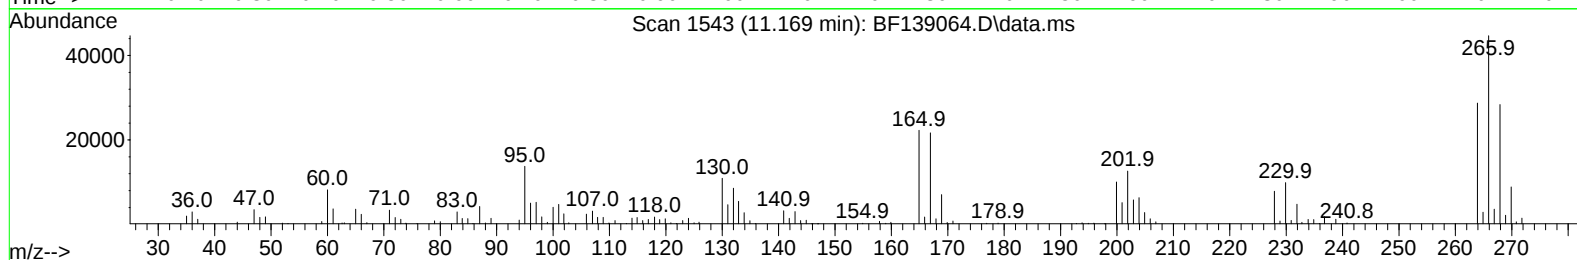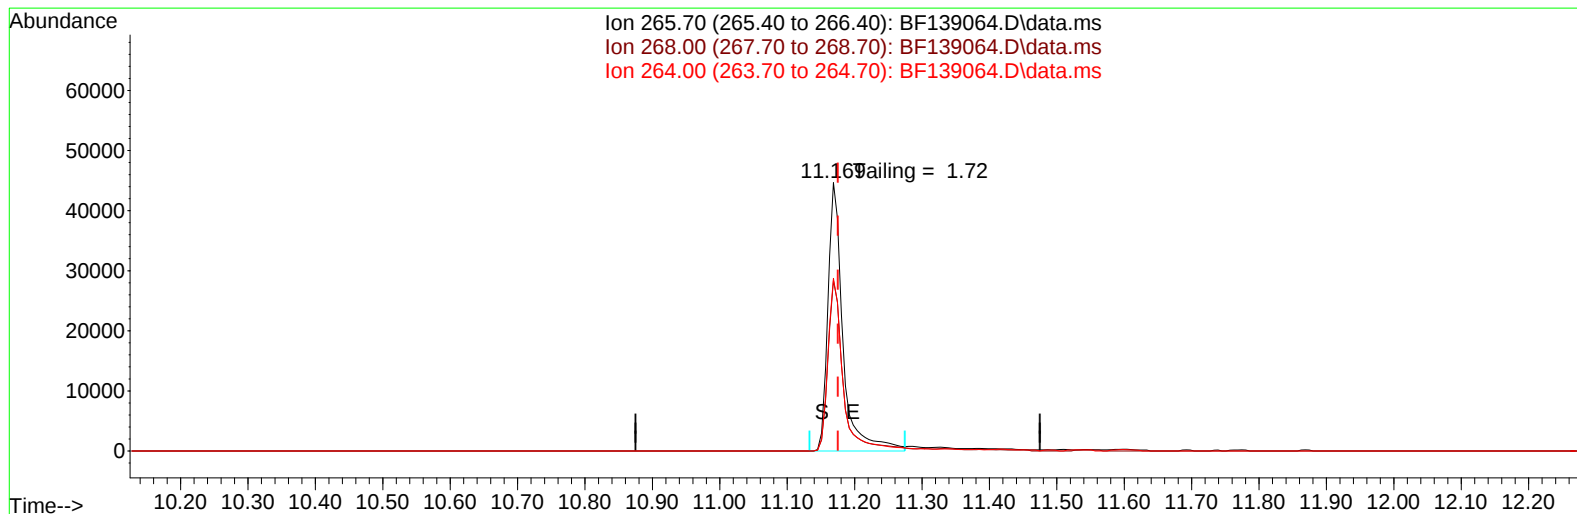

TIC: BF139064.D\data.ms

(70) Pentachlorophenol (C)

11.169min (-0.006) 65165.03 ng




response 69939

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	63.57
264.00	62.20	64.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081924\
Data File : BF139064.D
Acq On : 19 Aug 2024 08:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 19 11:09:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

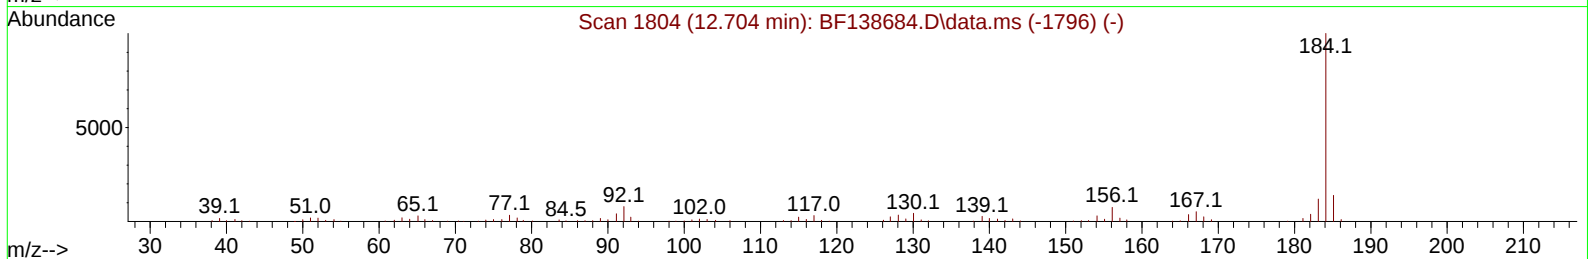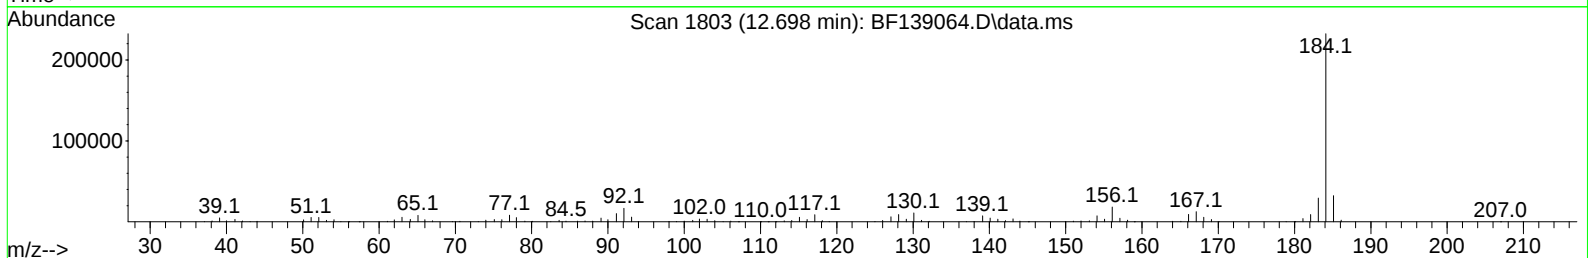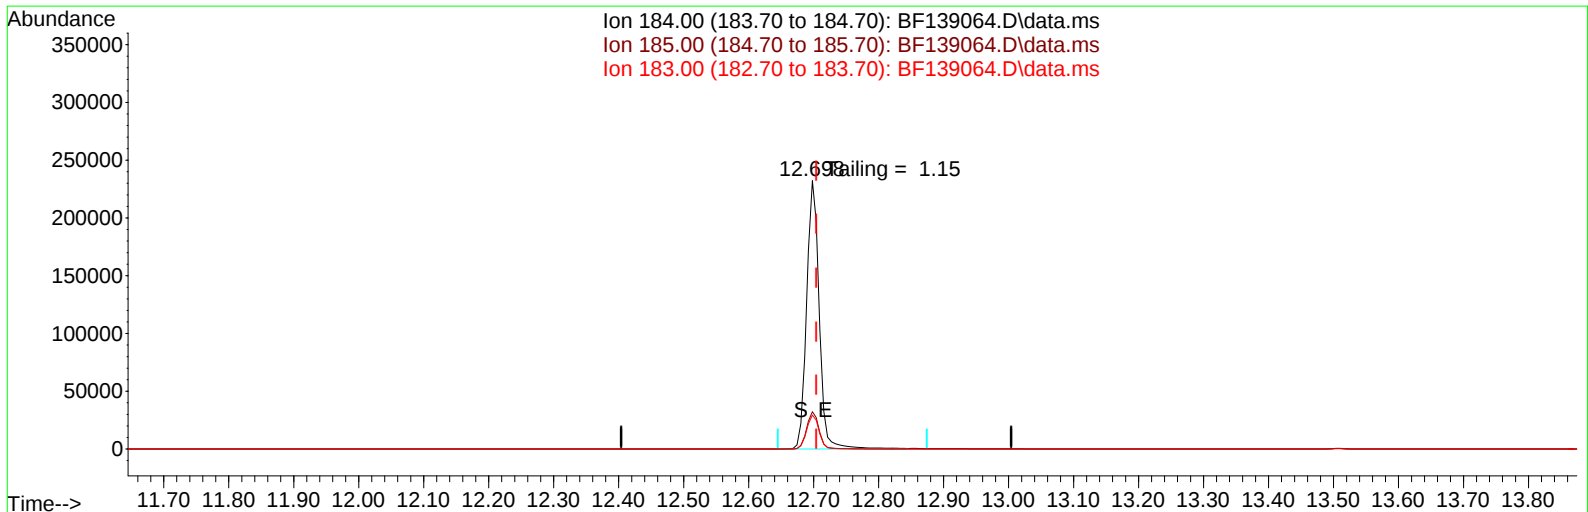

TIC: BF139064.D\data.ms

(77) Benzidine

12.698min (-0.006) 0.00 ng m

response 313382

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.94
183.00	12.00	12.66
0.00	0.00	0.00