


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081524\
Data File : BP021514.D
Acq On : 15 Aug 2024 14:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 14 00:00:30 2024

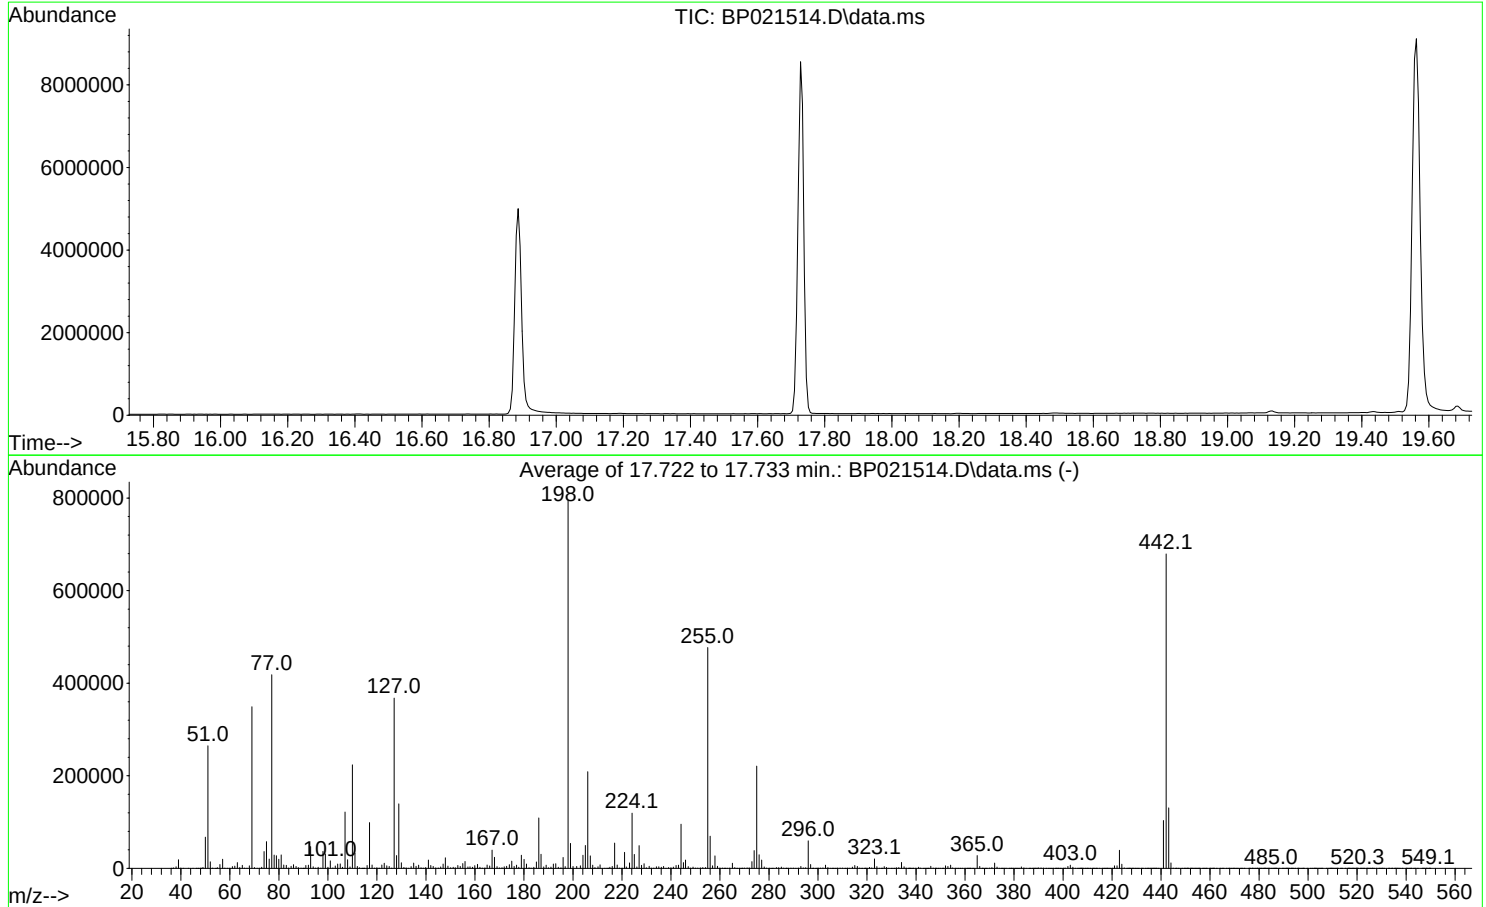




AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	264729	PASS
68	69	0.00	2	1.6	5584	PASS
69	198	0.00	100	43.9	349232	PASS
70	69	0.00	2	0.5	1759	PASS
127	198	10	80	46.3	367723	PASS
197	198	0.00	2	0.5	3836	PASS
198	198	100	100	100.0	794679	PASS
199	198	5	9	6.8	53996	PASS
275	198	10	60	27.8	220736	PASS
365	198	1	100	3.5	27727	PASS
441	198	0.01	100	13.0	103203	PASS
442	442	100	100	100.0	679166	PASS
443	442	15	24	19.2	130616	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081524\
Data File : BP021514.D
Acq On : 15 Aug 2024 14:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 16 02:36:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 00:00:30 2024
Response via : Initial Calibration

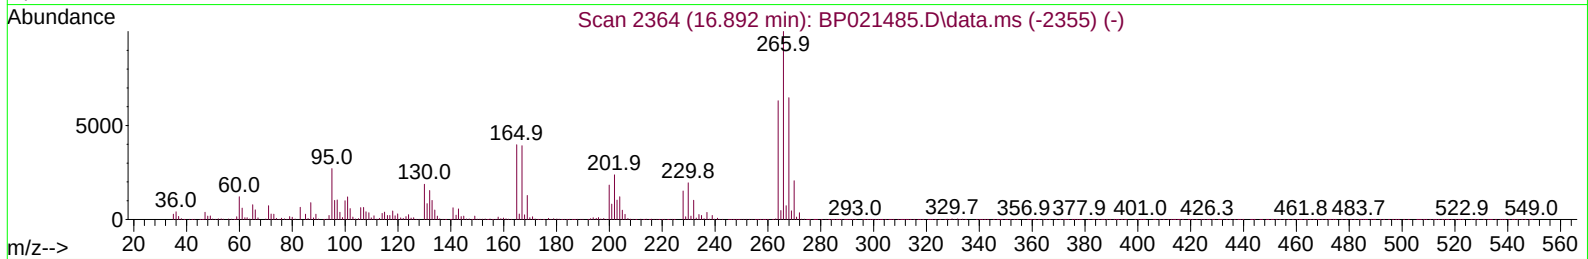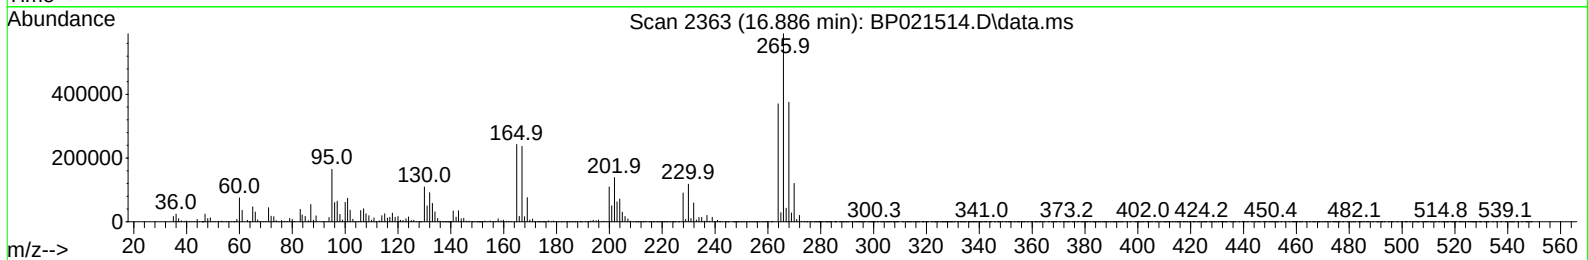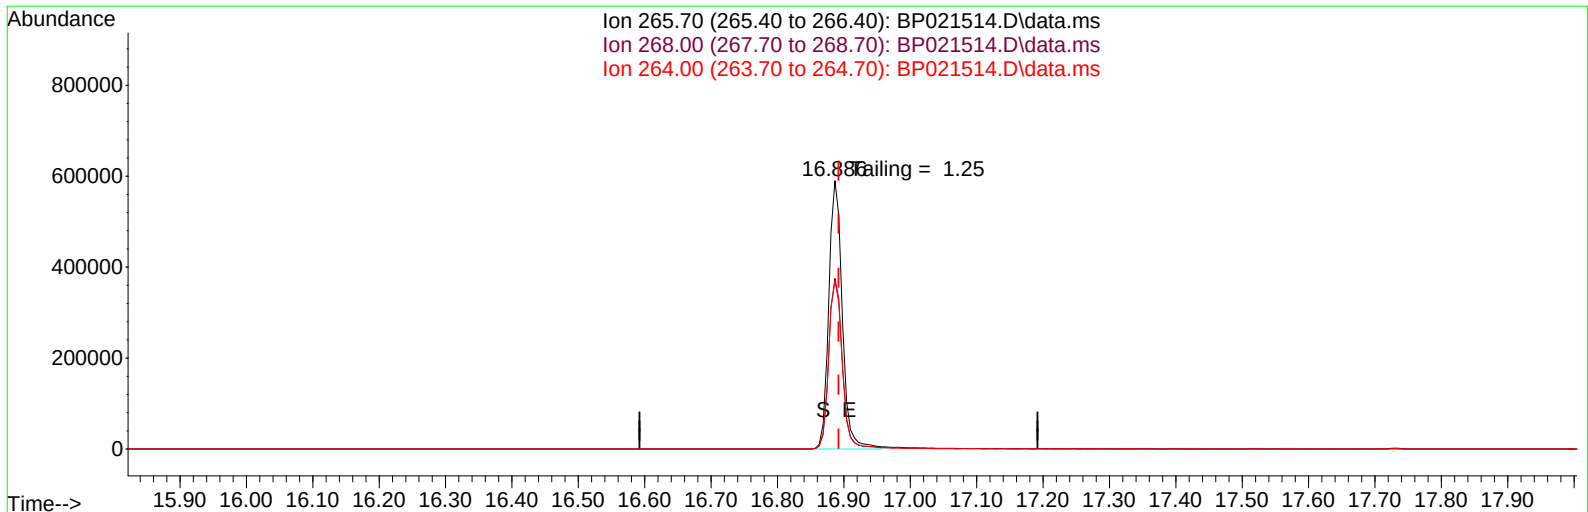

TIC: BP021514.D\data.ms

(70) Pentachlorophenol (C)

16.886min (-0.006) 525145.52 ng




response 842453

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	63.58
264.00	63.10	62.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081524\
 Data File : BP021514.D
 Acq On : 15 Aug 2024 14:54
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 16 02:36:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 00:00:30 2024
 Response via : Initial Calibration

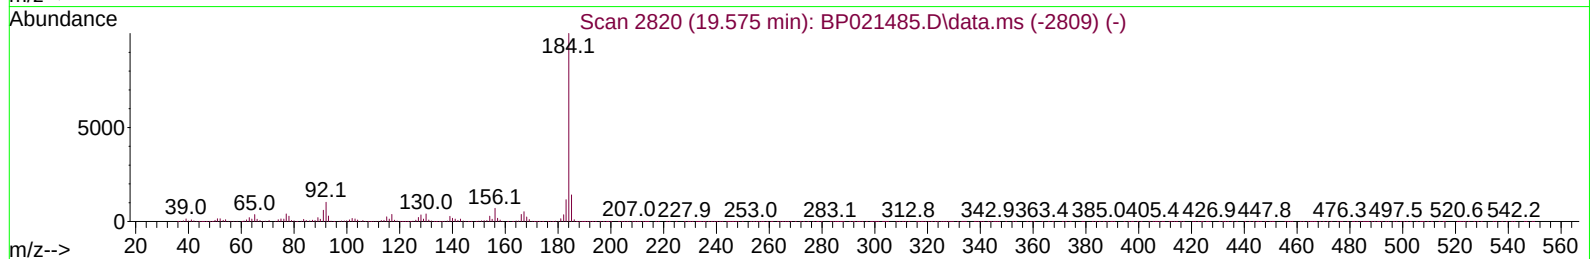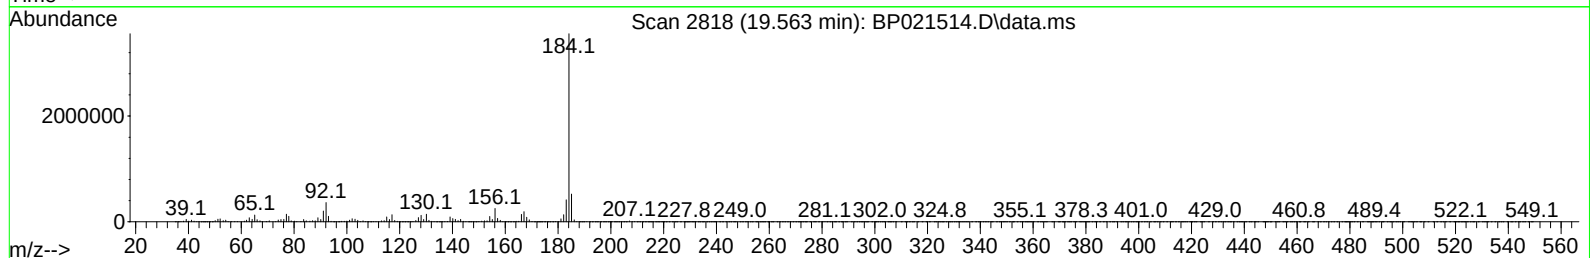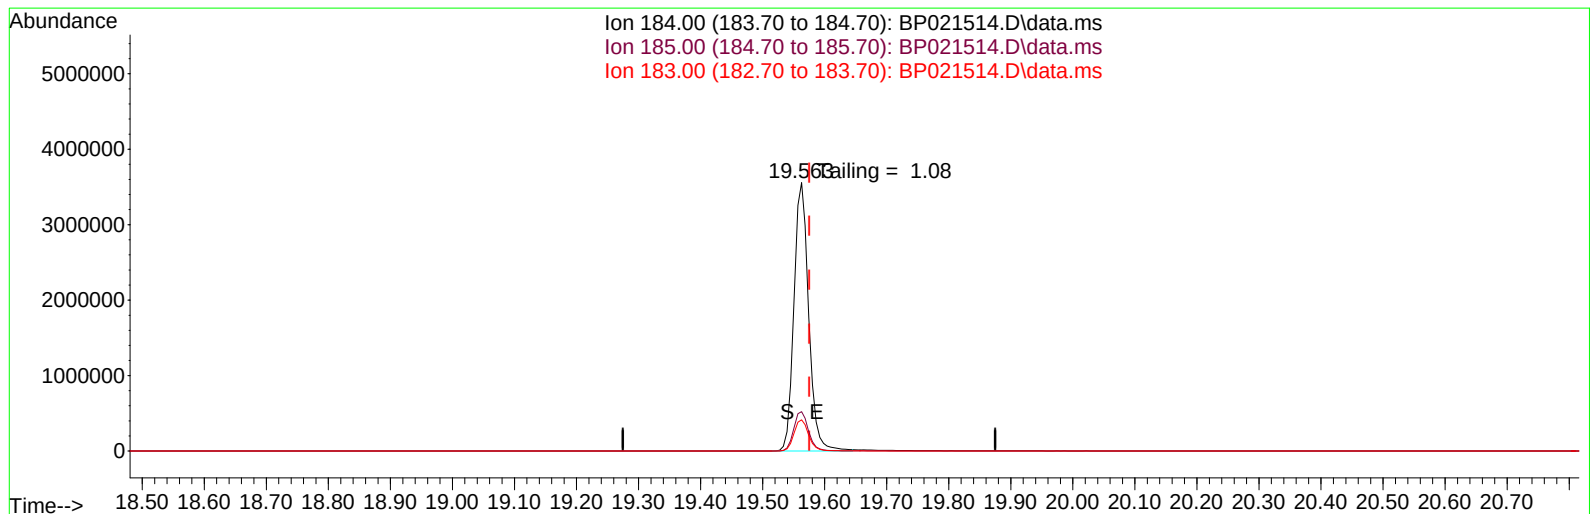

TIC: BP021514.D\data.ms

(77) Benzidine

19.563min (-0.012) -20.00 ng

response 5959833

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.70
183.00	11.60	11.67
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/15/2024	BNA_P	<u>BP021514.D</u>
Compound Name	Response	Retention Time
DDT	2415160	20.869
DDD	25818	20.457
DDE	904	19.874
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26722	2441882	1.09

Instrument :
BNA_P
ClientSampleId :
DFTPP