


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081724\
Data File : BN033446.D
Acq On : 17 Aug 2024 01:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 16 04:44:11 2024

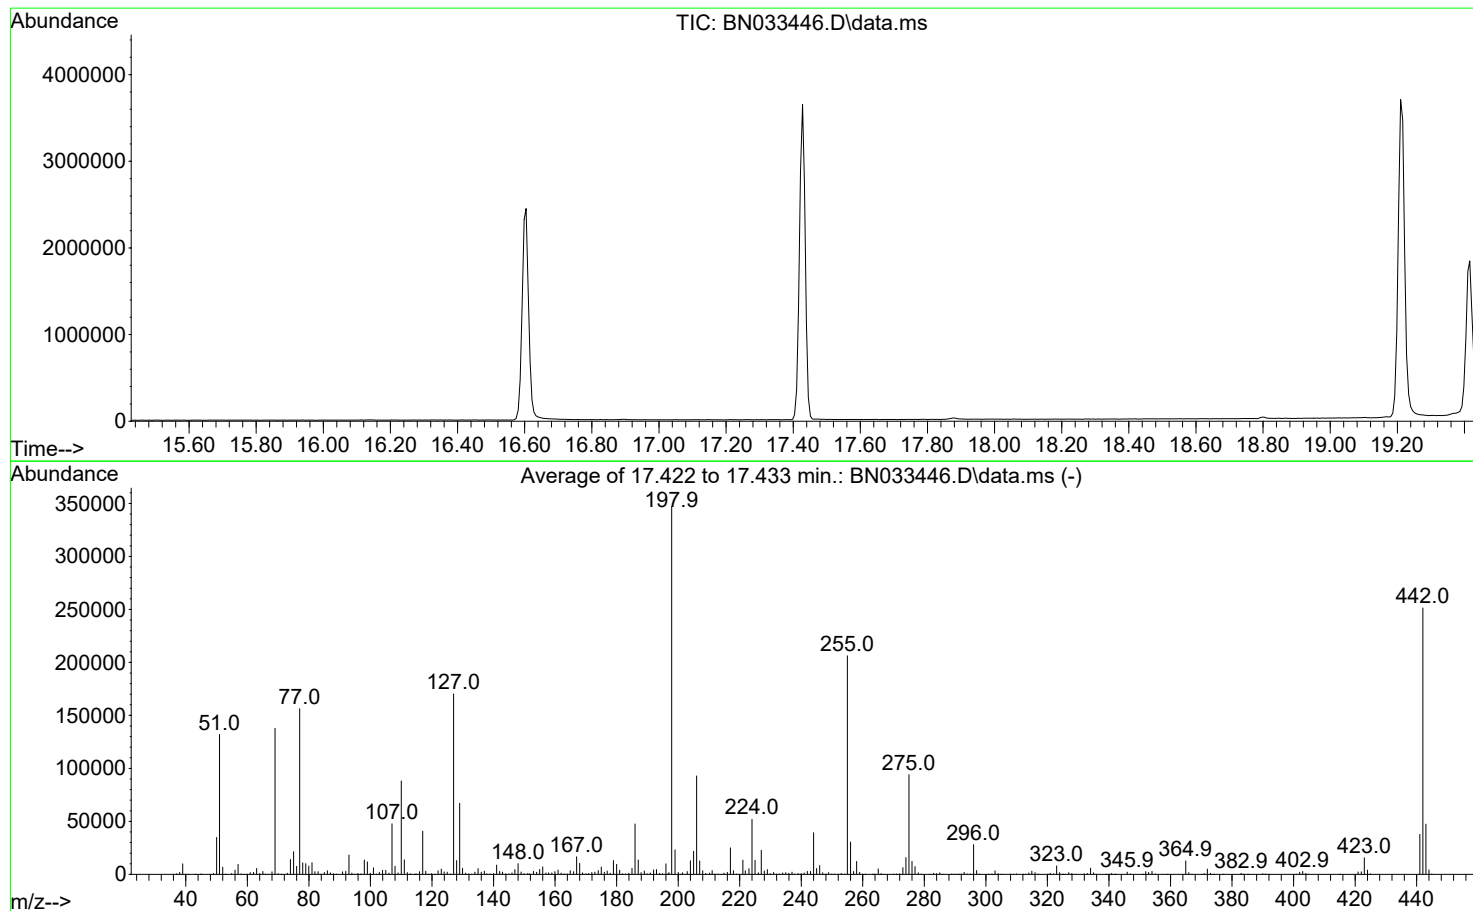

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2447

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	38.1	132082	PASS
68	69	0.00	2	1.8	2448	PASS
69	198	0.00	100	39.7	137843	PASS
70	69	0.00	2	0.5	685	PASS
127	198	10	80	49.1	170261	PASS
197	198	0.00	2	0.5	1737	PASS
198	198	100	100	100.0	347093	PASS
199	198	5	9	6.7	23160	PASS
275	198	10	60	27.1	94128	PASS
365	198	1	100	3.7	12764	PASS
441	198	0.01	100	10.9	37808	PASS
442	442	50	100	100.0	251392	PASS
443	442	15	24	18.9	47464	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/17/2024	BNA_N	<u>BN033446.D</u>
Compound Name	Response	Retention Time
DDT	944309	20.463
DDD	72572	20.022
DDE	2201	19.51
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
74773	1019082	7.34

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081724\
Data File : BN033446.D
Acq On : 17 Aug 2024 01:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 17 03:20:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 17 03:18:59 2024
Response via : Initial Calibration

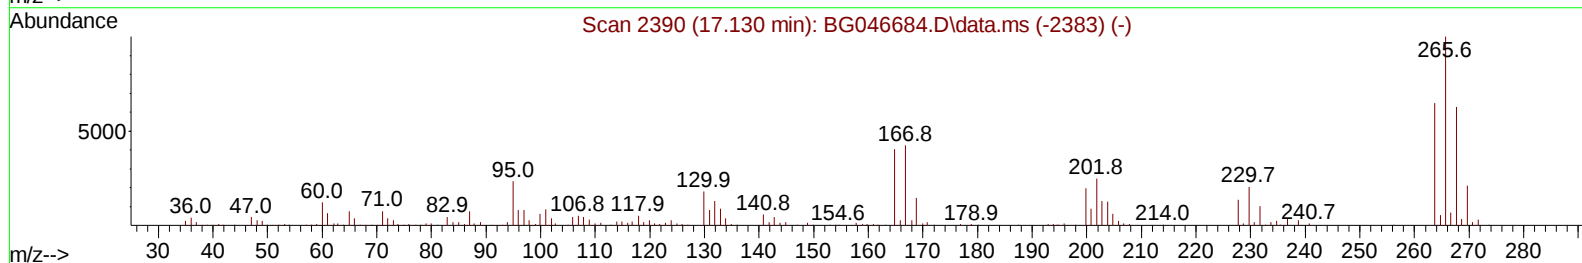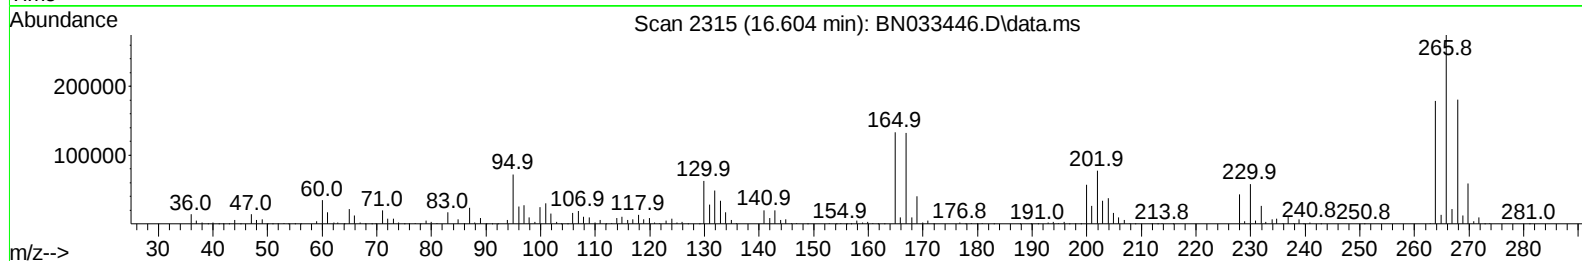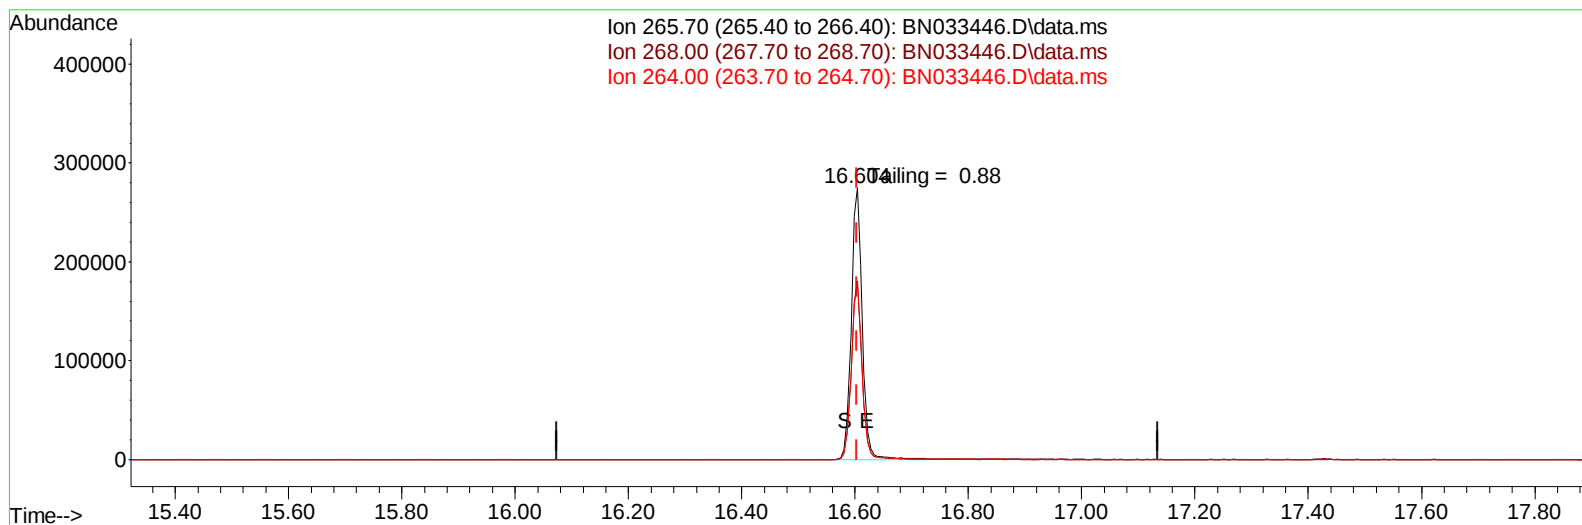

TIC: BN033446.D\data.ms

(70) Pentachlorophenol (C)

16.604min (+ 0.000) 19890.98 ng




response 372297

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.72
264.00	61.60	65.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081724\
Data File : BN033446.D
Acq On : 17 Aug 2024 01:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 17 03:20:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 17 03:18:59 2024
Response via : Initial Calibration

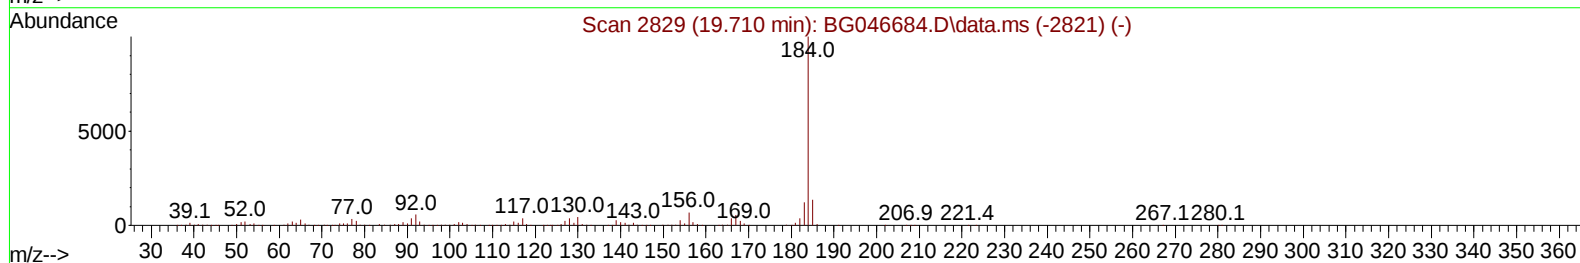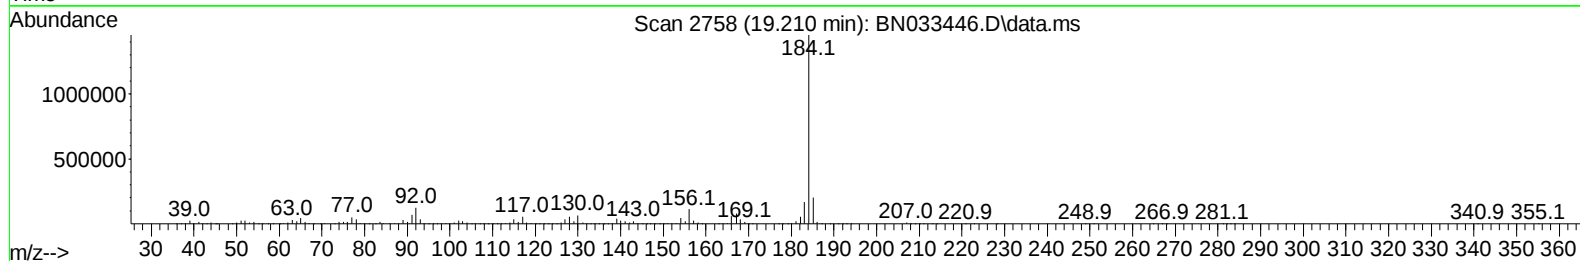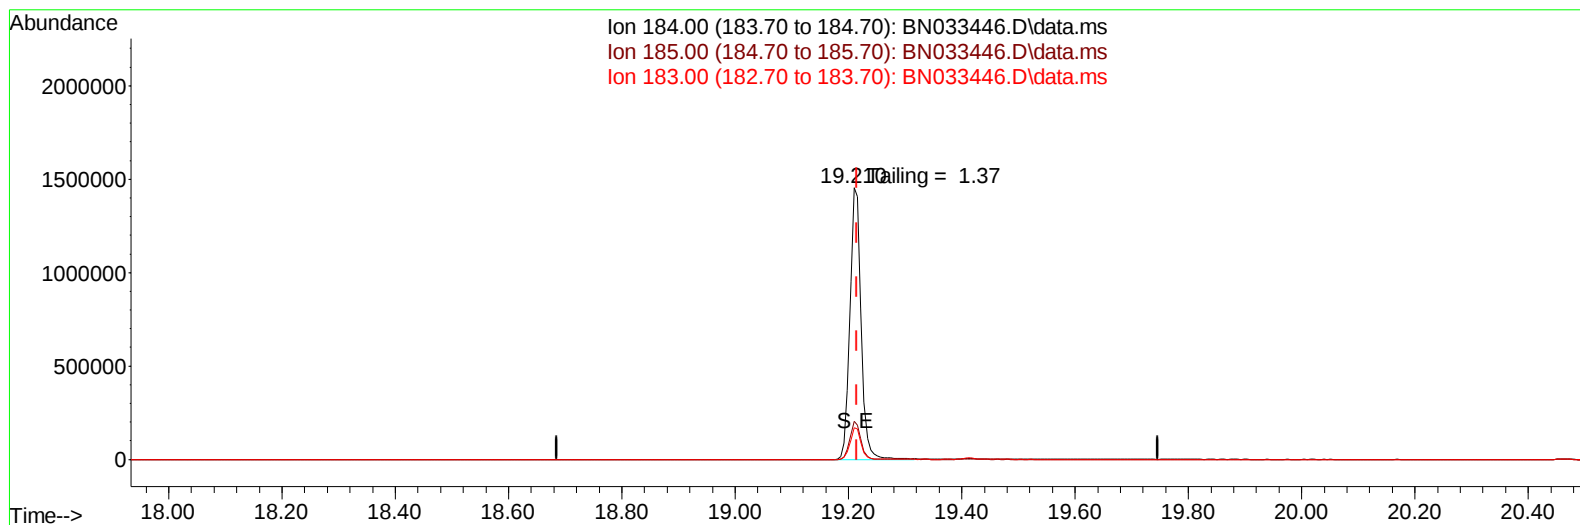

TIC: BN033446.D\data.ms

(77) Benzidine

19.210min (-0.006) 0.00 ng

response 2014139

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.98
183.00	13.20	11.59
0.00	0.00	0.00