
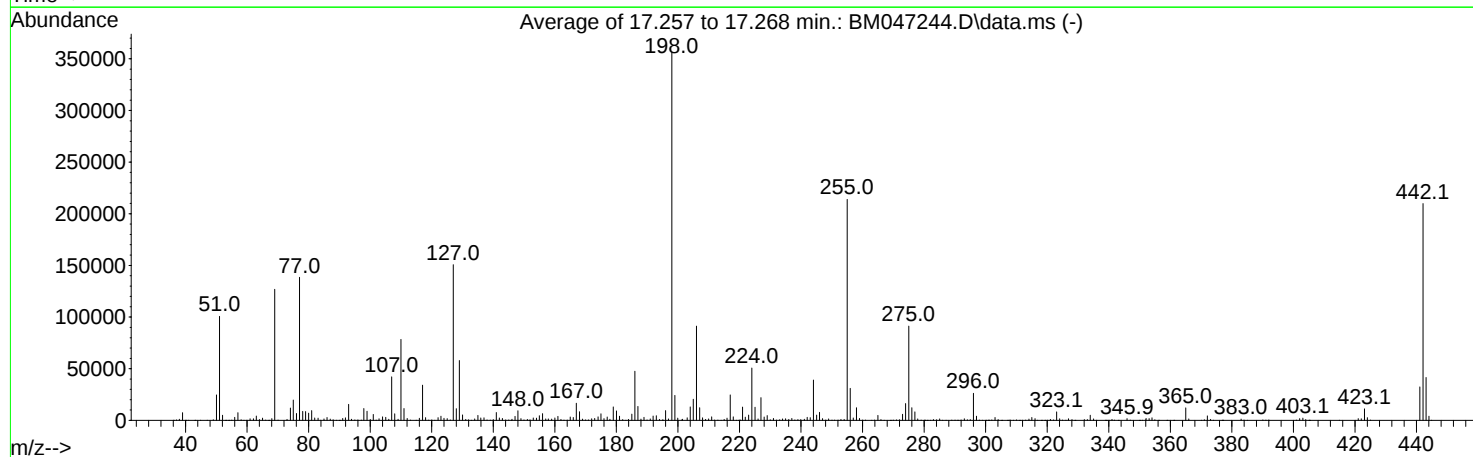


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081924\
Data File : BM047244.D
Acq On : 19 Aug 2024 09:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun Aug 11 23:47:58 2024

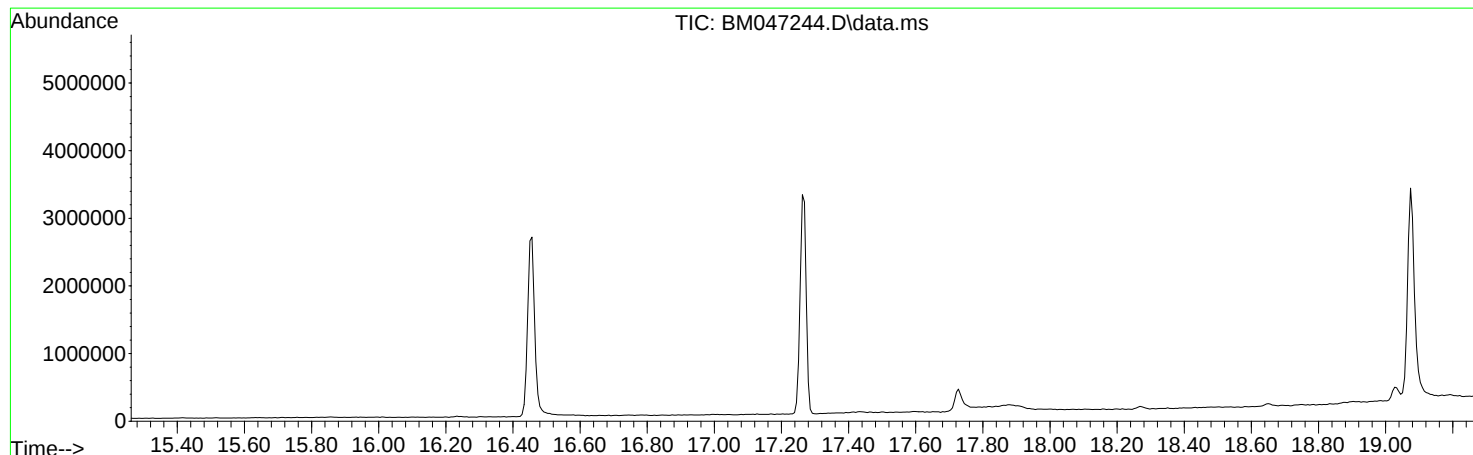

AutoFind: Scans 2443, 2444, 2445; Background Corrected with Scan 2436

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.3	100766	PASS
68	69	0.00	2	1.4	1739	PASS
69	198	0.00	100	35.6	126854	PASS
70	69	0.00	2	0.3	398	PASS
127	198	10	80	42.3	150684	PASS
197	198	0.00	2	0.4	1439	PASS
198	198	100	100	100.0	356095	PASS
199	198	5	9	6.8	24112	PASS
275	198	10	60	25.6	91270	PASS
365	198	1	100	3.4	12027	PASS
441	198	0.01	100	9.1	32381	PASS
442	442	50	100	100.0	209880	PASS
443	442	15	24	19.8	41587	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/19/2024	BNA_M	<u>BM047244.D</u>
Compound Name	Response	Retention Time
DDT	1140644	20.321
DDD	107172	19.88
DDE	3211	19.368
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
110383	1251027	8.82

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081924\
Data File : BM047244.D
Acq On : 19 Aug 2024 09:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 19 11:15:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

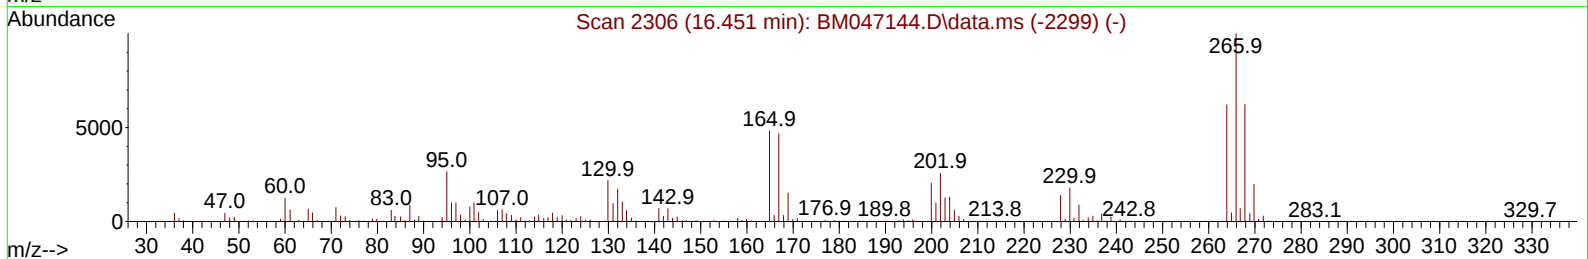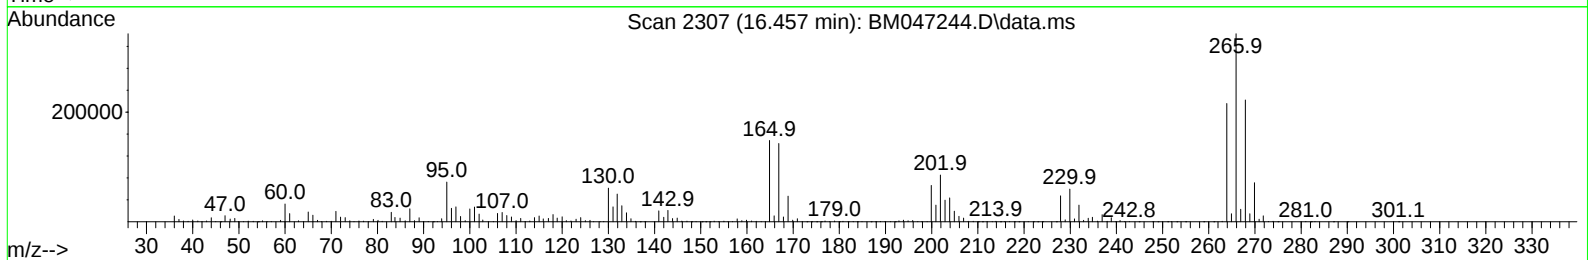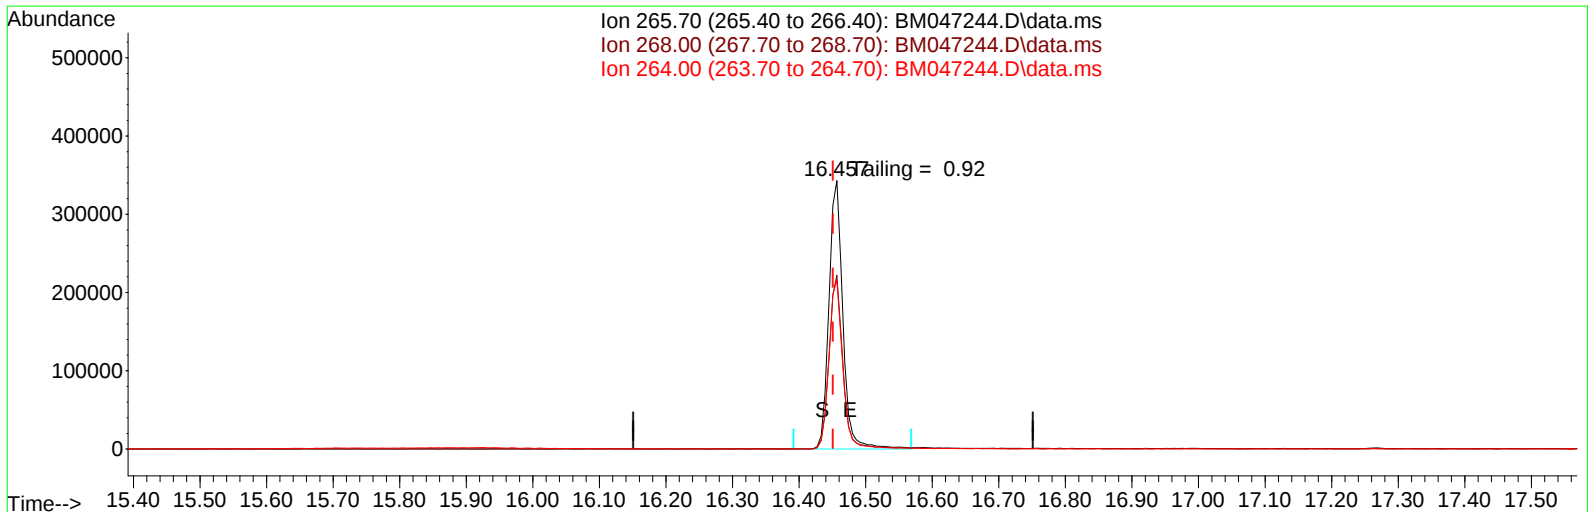

TIC: BM047244.D\data.ms

(70) Pentachlorophenol (C)

16.457min (+ 0.006) 216859.29 ng




response 499995

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.77
264.00	62.00	62.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081924\
Data File : BM047244.D
Acq On : 19 Aug 2024 09:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 19 11:15:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

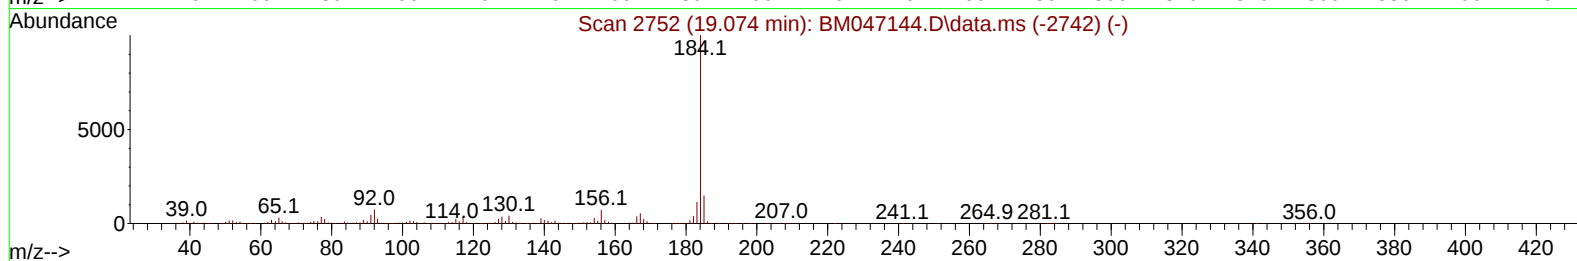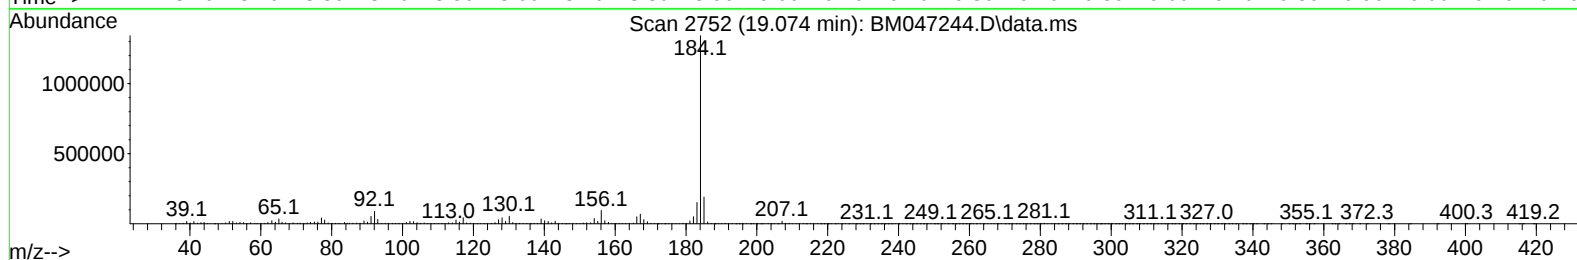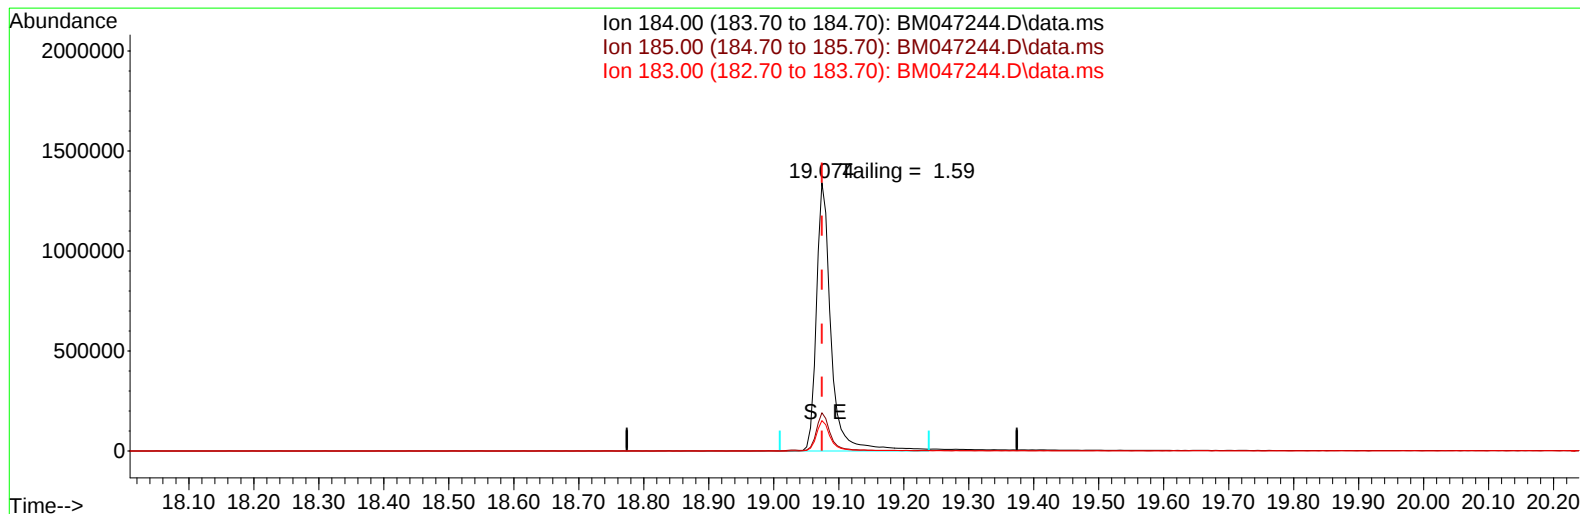

TIC: BM047244.D\data.ms

(77) Benzidine

19.074min (-0.000) 40695.55 ng m

response 2114570

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.26
183.00	11.30	11.34
0.00	0.00	0.00