
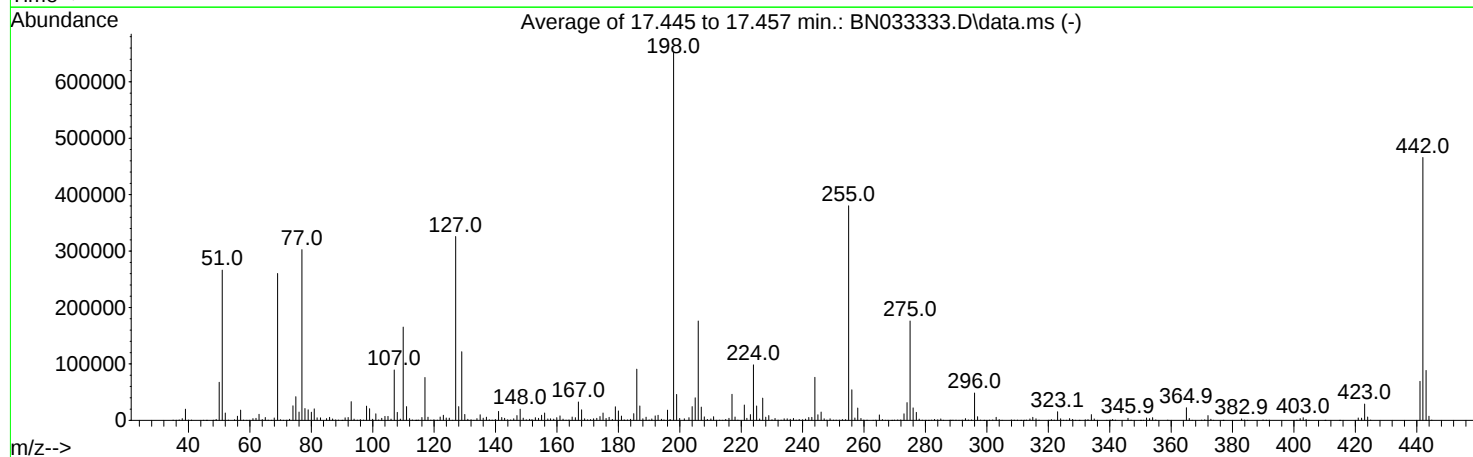


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081024\
Data File : BN033333.D
Acq On : 10 Aug 2024 12:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 12 01:09:50 2024

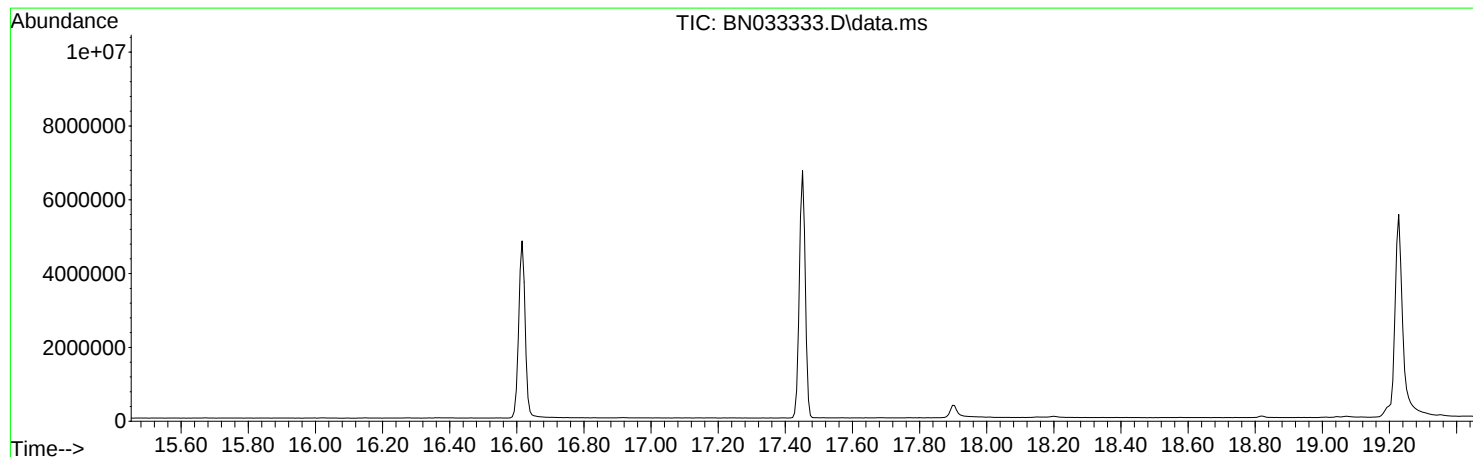

AutoFind: Scans 2441, 2442, 2443; Background Corrected with Scan 2434

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.8	266166	PASS
68	69	0.00	2	1.6	4158	PASS
69	198	0.00	100	39.9	260350	PASS
70	69	0.00	2	0.5	1290	PASS
127	198	10	80	50.0	325931	PASS
197	198	0.00	2	0.2	1035	PASS
198	198	100	100	100.0	651947	PASS
199	198	5	9	7.1	46043	PASS
275	198	10	60	27.0	175979	PASS
365	198	1	100	3.4	22312	PASS
441	198	0.01	100	10.6	69197	PASS
442	442	50	100	100.0	465856	PASS
443	442	15	24	19.0	88587	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/10/2024	BNA_N	<u>BN033333.D</u>
Compound Name	Response	Retention Time
DDT	2334042	20.48
DDD	52614	20.039
DDE	483	19.533
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
53097	2387139	2.22

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081024\
Data File : BN033333.D
Acq On : 10 Aug 2024 12:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 12 01:45:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 12 01:45:39 2024
Response via : Initial Calibration

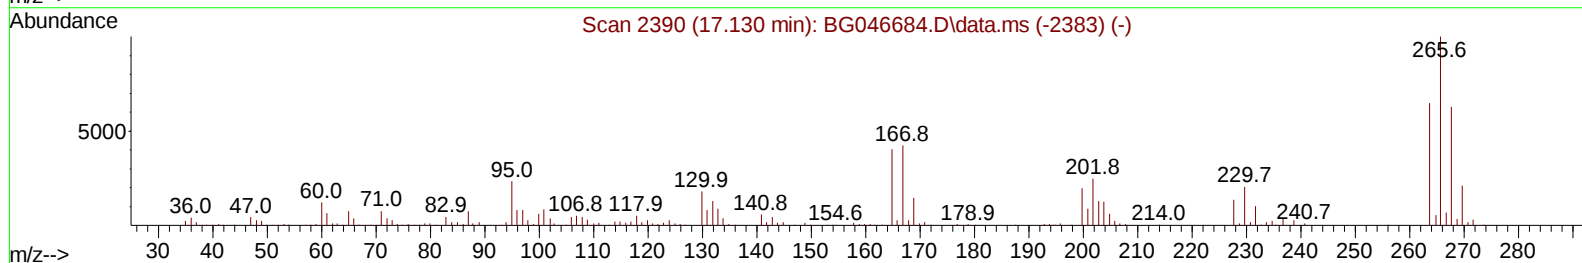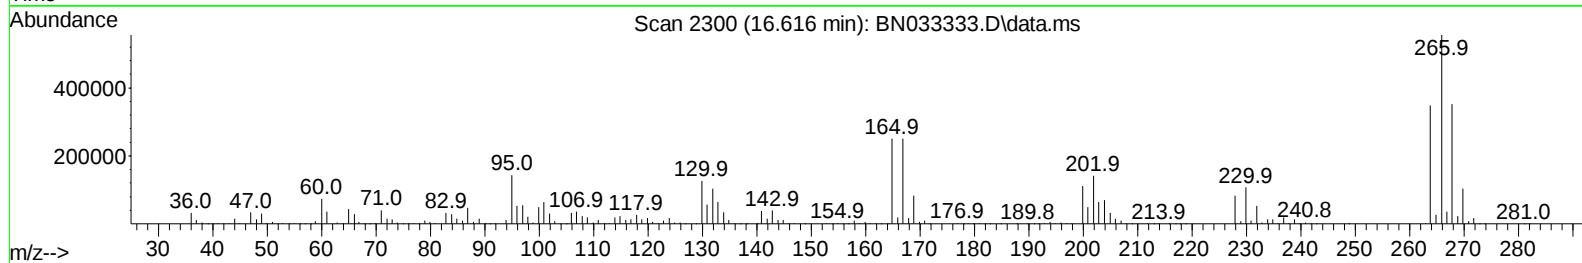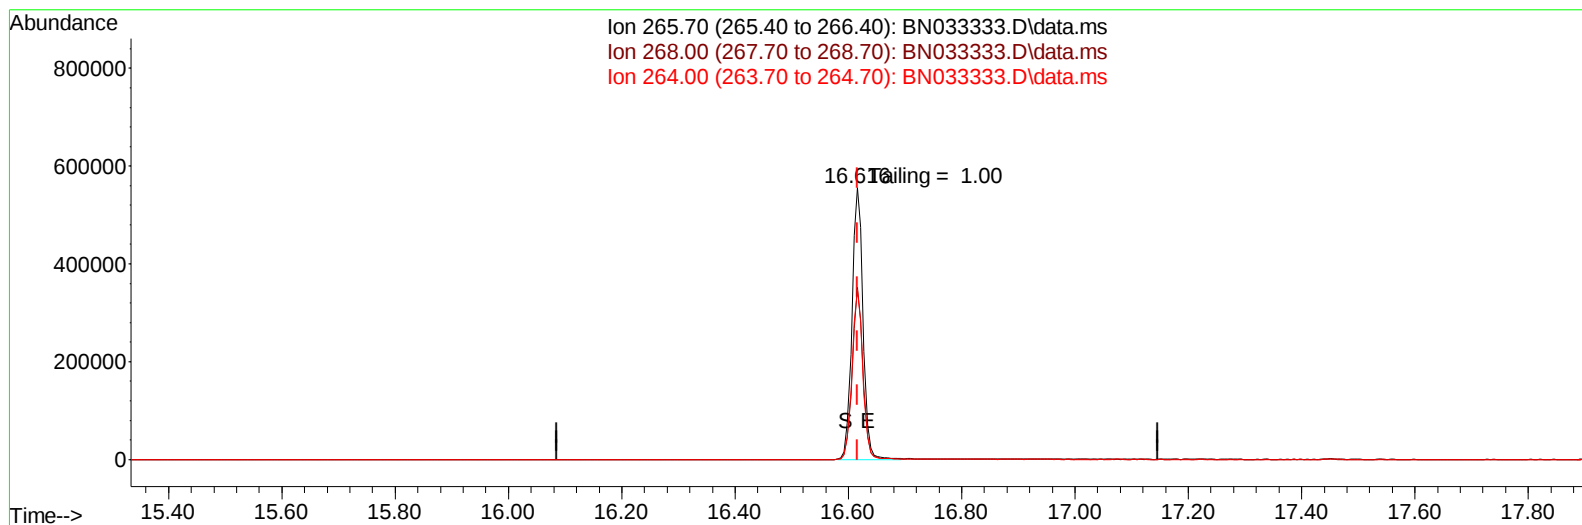

TIC: BN033333.D\data.ms

(70) Pentachlorophenol (C)

16.616min (0.000) 24511.53 ng




response 755976

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.43
264.00	61.60	62.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081024\
Data File : BN033333.D
Acq On : 10 Aug 2024 12:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 12 01:45:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 12 01:45:39 2024
Response via : Initial Calibration

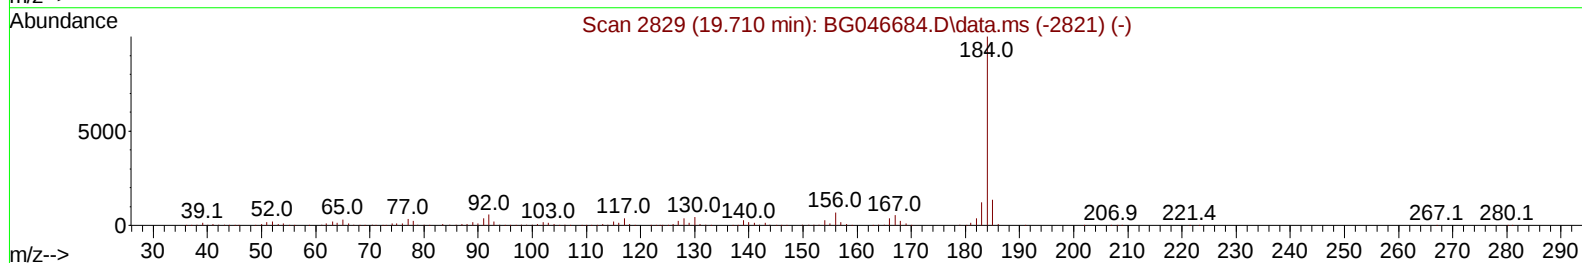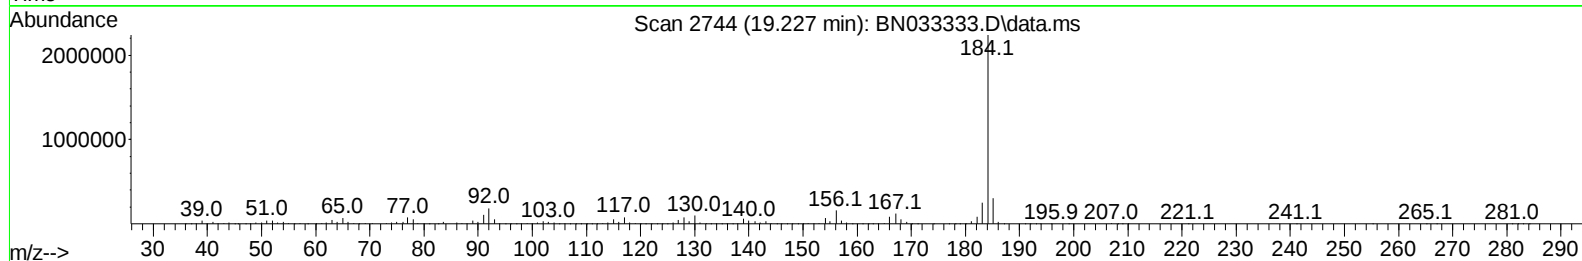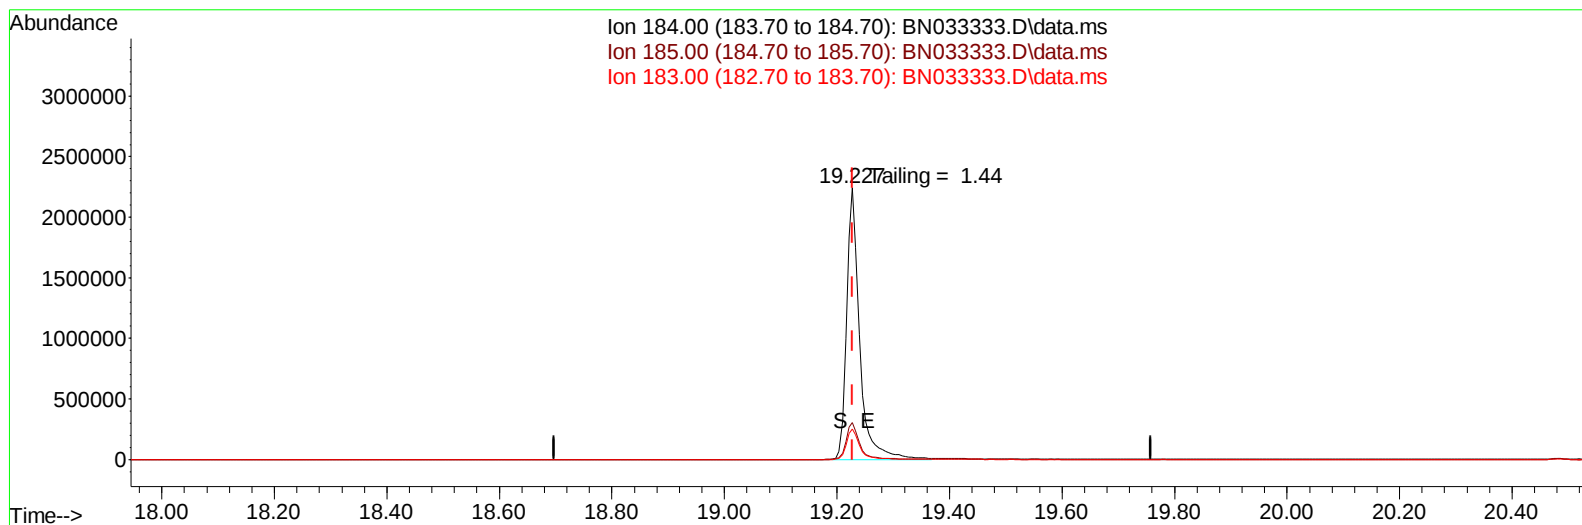

TIC: BN033333.D\data.ms

(77) Benzidine

19.227min (0.000) 0.00 ng

response 3645162

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.61
183.00	13.20	11.18
0.00	0.00	0.00