
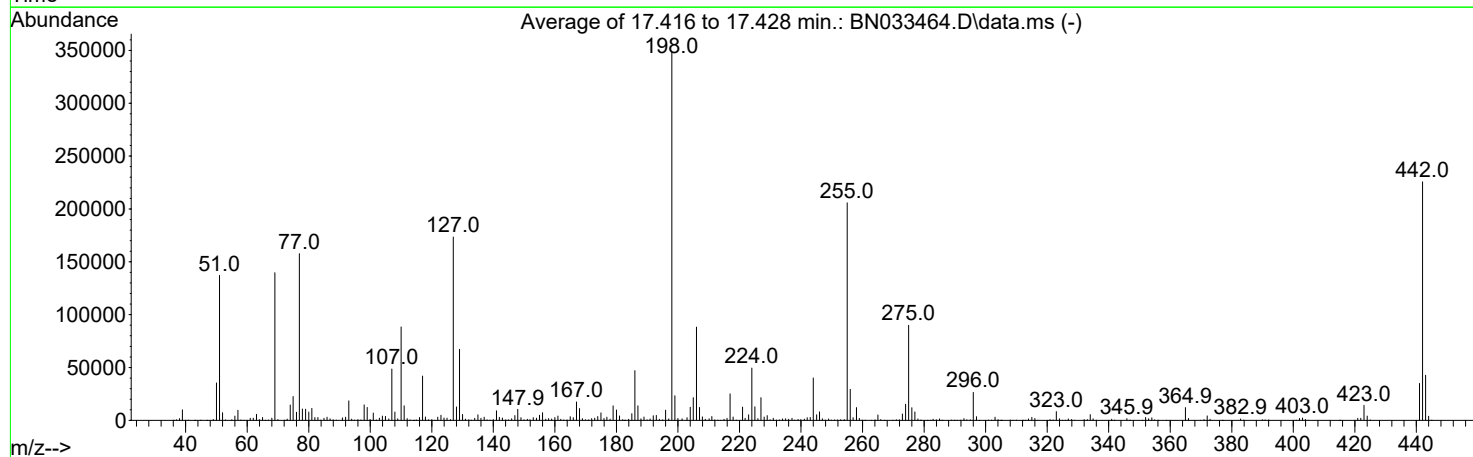


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081824\
Data File : BN033464.D
Acq On : 17 Aug 2024 12:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 16 04:44:11 2024

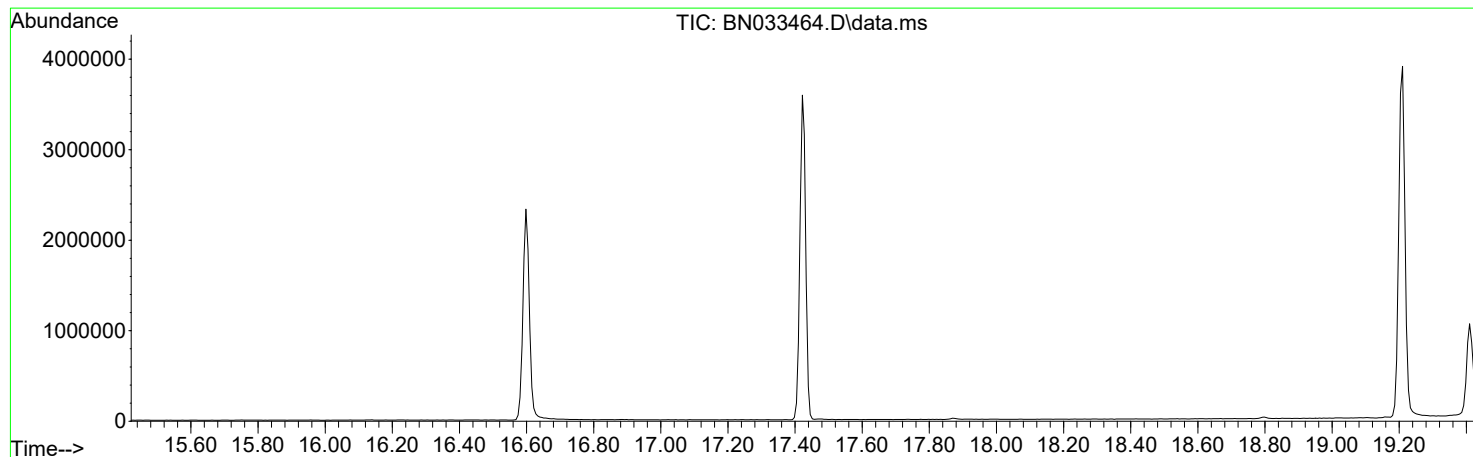

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2446

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	39.4	137124	PASS
68	69	0.00	2	1.6	2183	PASS
69	198	0.00	100	40.1	139656	PASS
70	69	0.00	2	0.5	758	PASS
127	198	10	80	49.8	173461	PASS
197	198	0.00	2	0.4	1307	PASS
198	198	100	100	100.0	347989	PASS
199	198	5	9	6.7	23261	PASS
275	198	10	60	25.9	89979	PASS
365	198	1	100	3.5	12146	PASS
441	198	0.01	100	10.1	35043	PASS
442	442	50	100	100.0	225757	PASS
443	442	15	24	18.9	42704	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/18/2024	BNA_N	<u>BN033464.D</u>
Compound Name	Response	Retention Time
DDT	861928	20.457
DDD	113828	20.016
DDE	25105	19.51
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
138933	1000861	13.88

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081824\
Data File : BN033464.D
Acq On : 17 Aug 2024 12:05
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTTP

Quant Time: Aug 18 00:33:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 18 00:33:21 2024
Response via : Initial Calibration

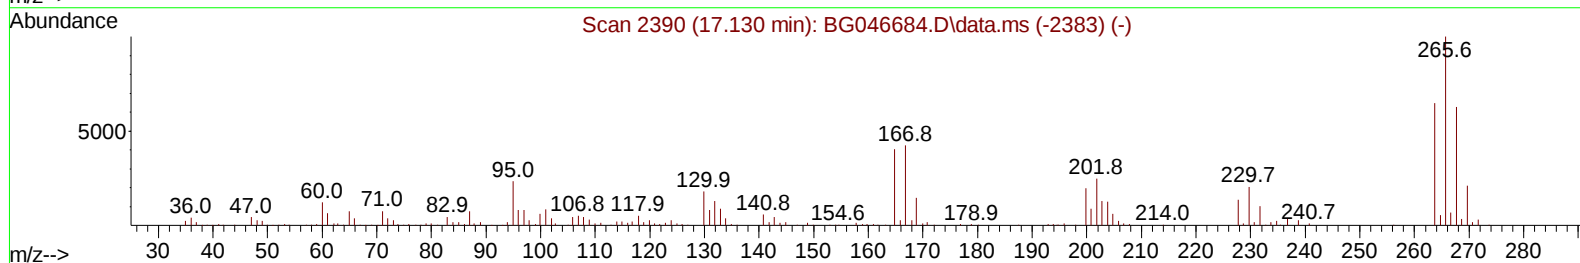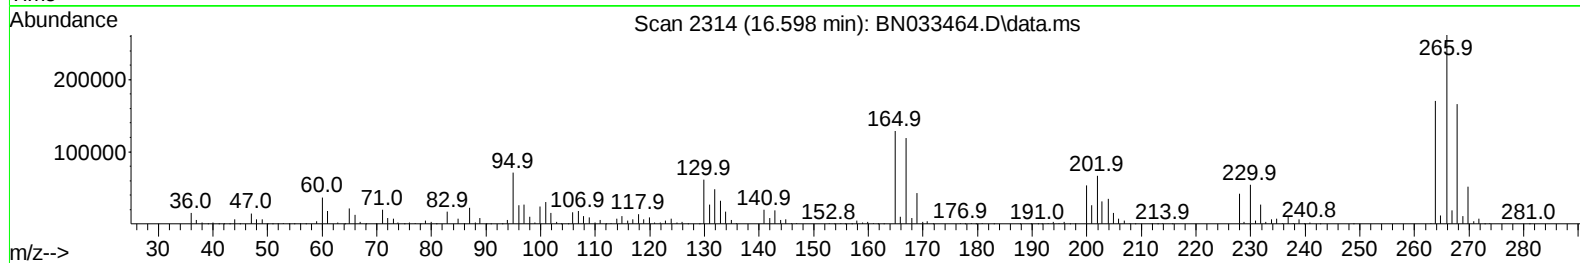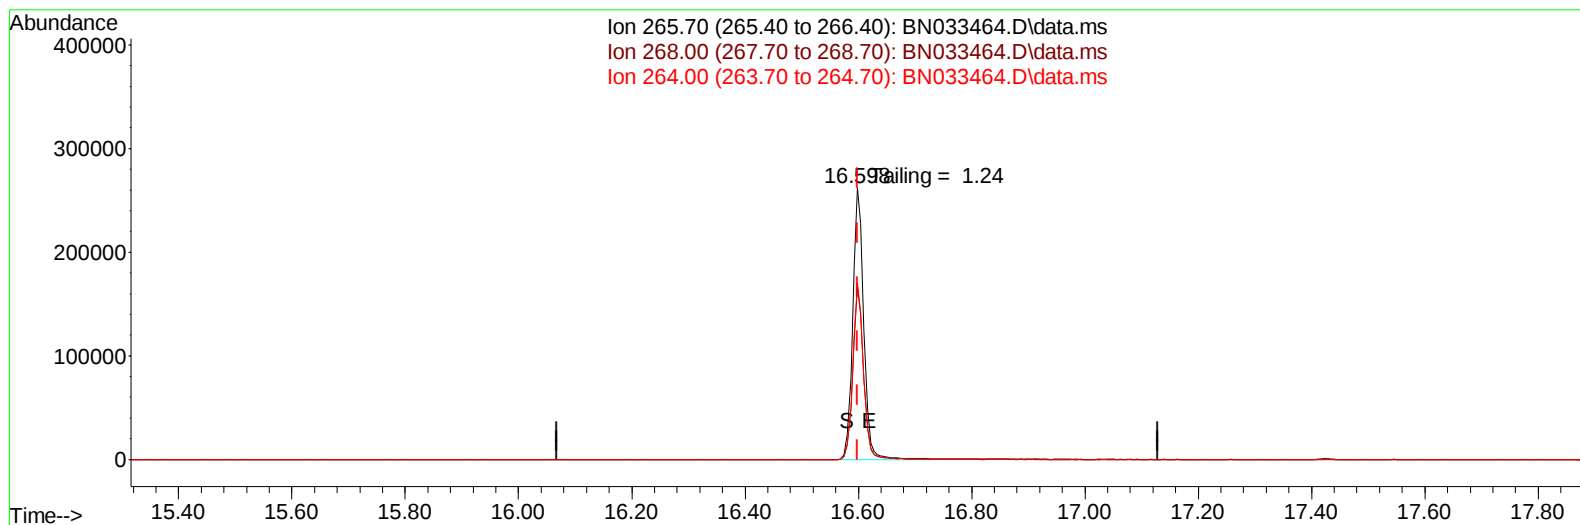

TIC: BN033464.D\data.ms

(70) Pentachlorophenol (C)

16.598min (0.000) 21414.02 ng




response 356438

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.53
264.00	61.60	64.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081824\
Data File : BN033464.D
Acq On : 17 Aug 2024 12:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 18 00:33:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 18 00:33:21 2024
Response via : Initial Calibration

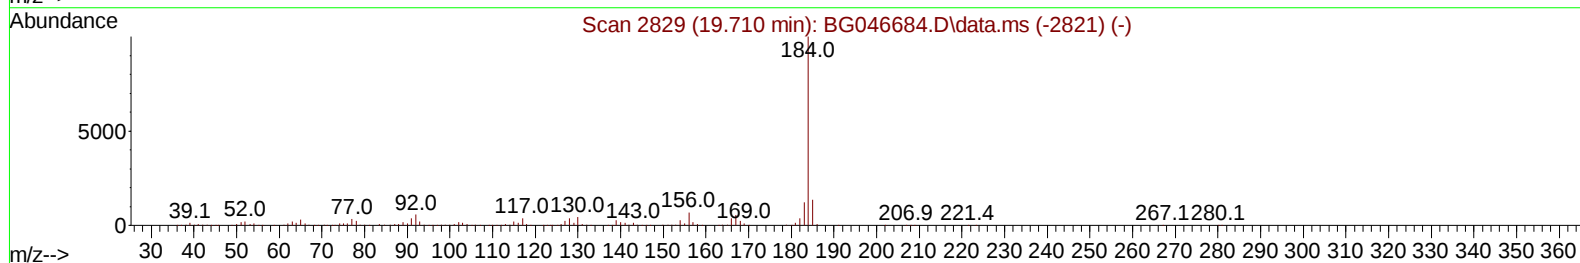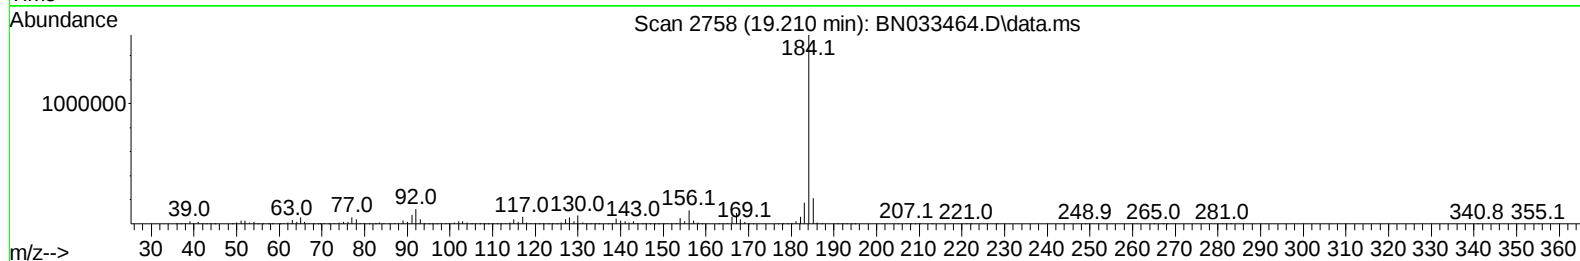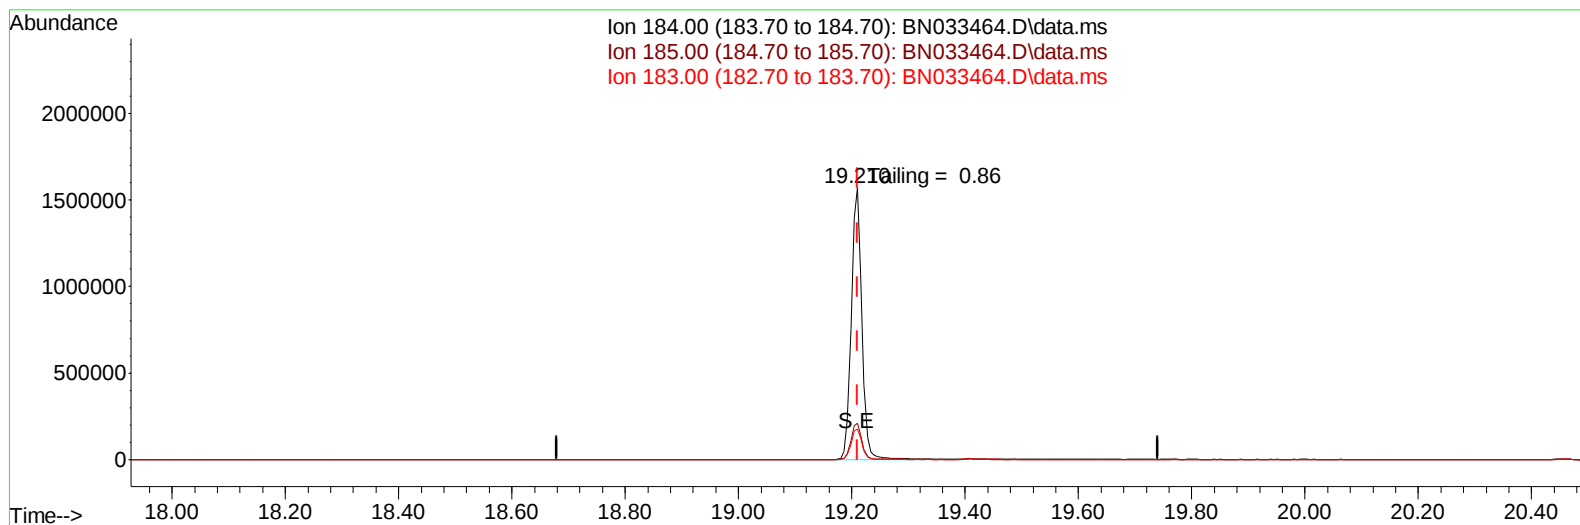

TIC: BN033464.D\data.ms

(77) Benzidine

19.210min (0.000) 0.00 ng

response 2051415

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.42
183.00	13.20	11.26
0.00	0.00	0.00