
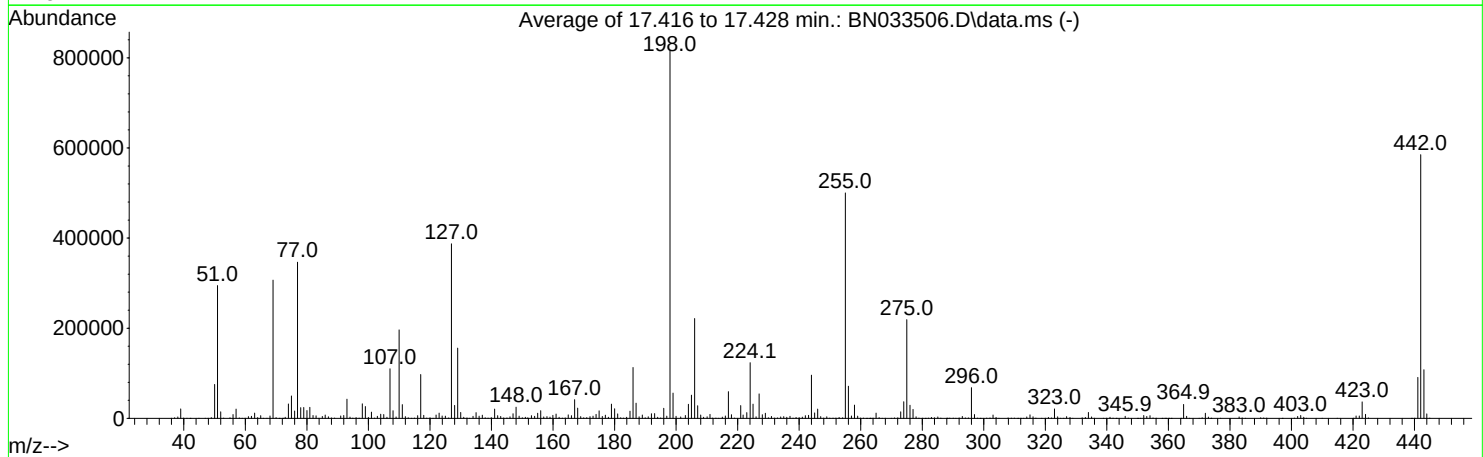


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082024\
Data File : BN033506.D
Acq On : 20 Aug 2024 15:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 19 23:32:18 2024

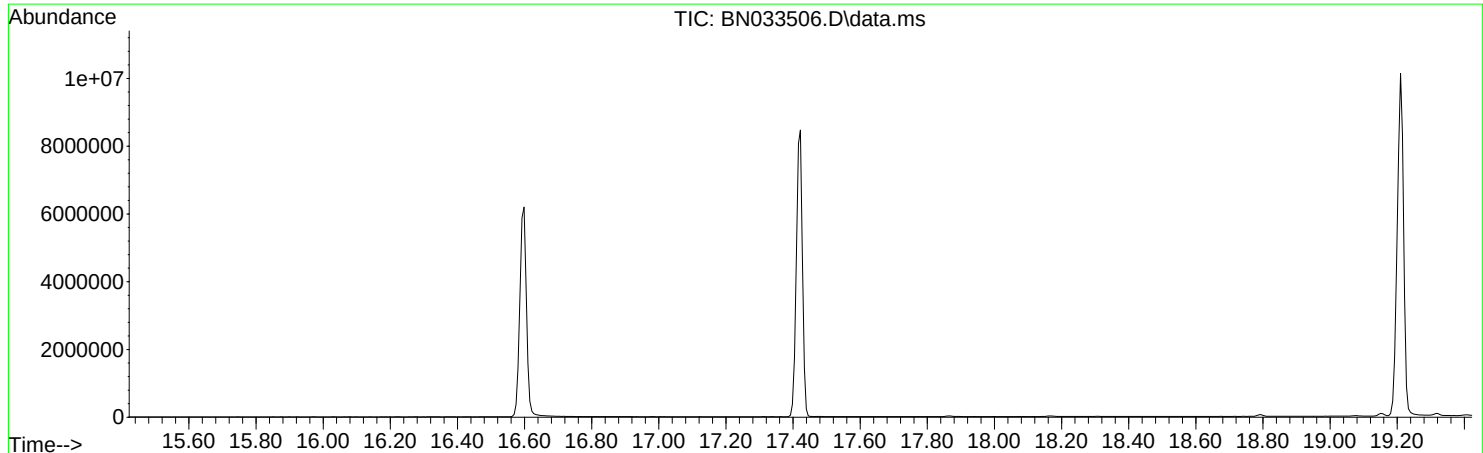




AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	294566	PASS
68	69	0.00	2	1.8	5531	PASS
69	198	0.00	100	37.6	306667	PASS
70	69	0.00	2	0.5	1683	PASS
127	198	10	80	47.5	387349	PASS
197	198	0.00	2	0.6	5093	PASS
198	198	100	100	100.0	816235	PASS
199	198	5	9	6.9	56176	PASS
275	198	10	60	26.9	219243	PASS
365	198	1	100	3.8	30933	PASS
441	198	0.01	100	11.1	90933	PASS
442	442	50	100	100.0	585109	PASS
443	442	15	24	18.4	107917	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082024\
Data File : BN033506.D
Acq On : 20 Aug 2024 15:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 21 05:32:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 05:32:13 2024
Response via : Initial Calibration

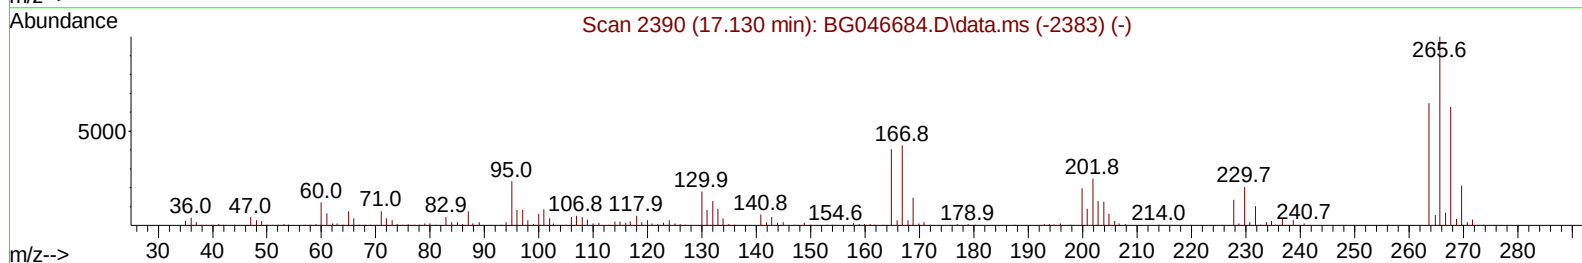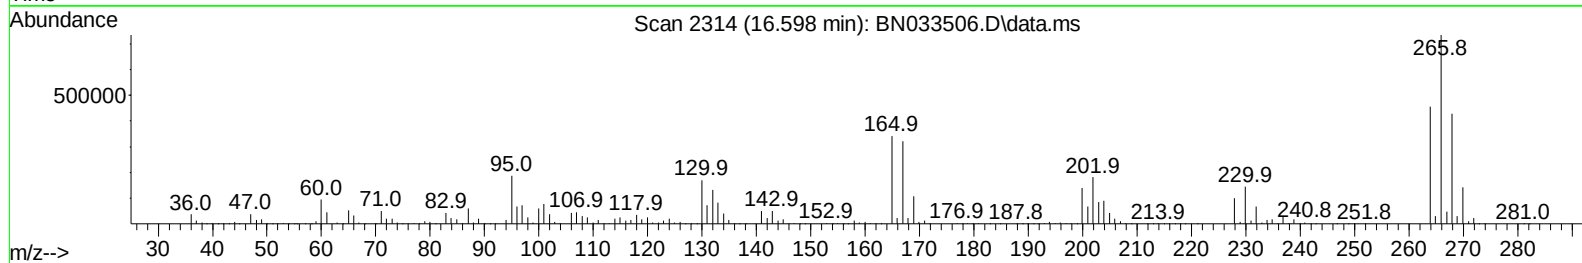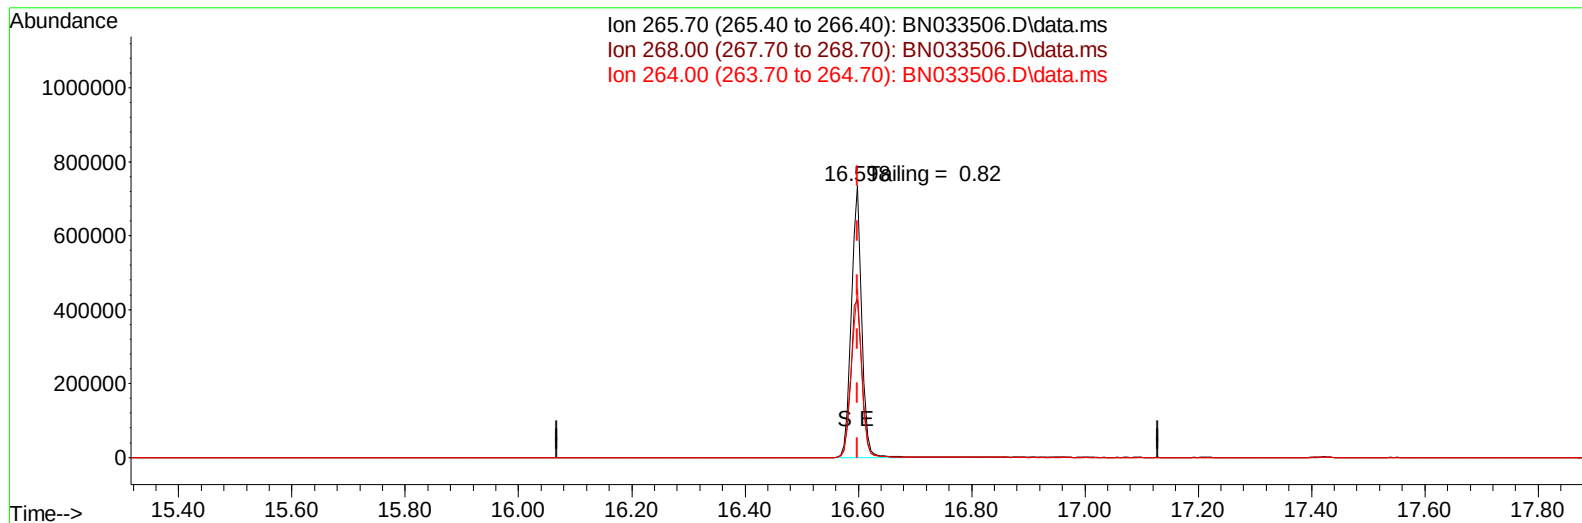

TIC: BN033506.D\data.ms

(70) Pentachlorophenol (C)

16.598min (0.000) 21421.68 ng




response 945798

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.18
264.00	61.60	62.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082024\
Data File : BN033506.D
Acq On : 20 Aug 2024 15:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 21 21:50:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 05:32:13 2024
Response via : Initial Calibration

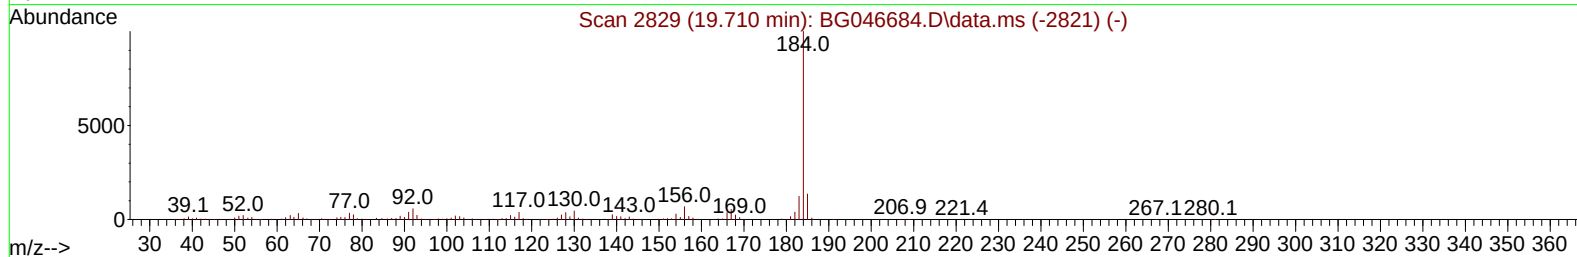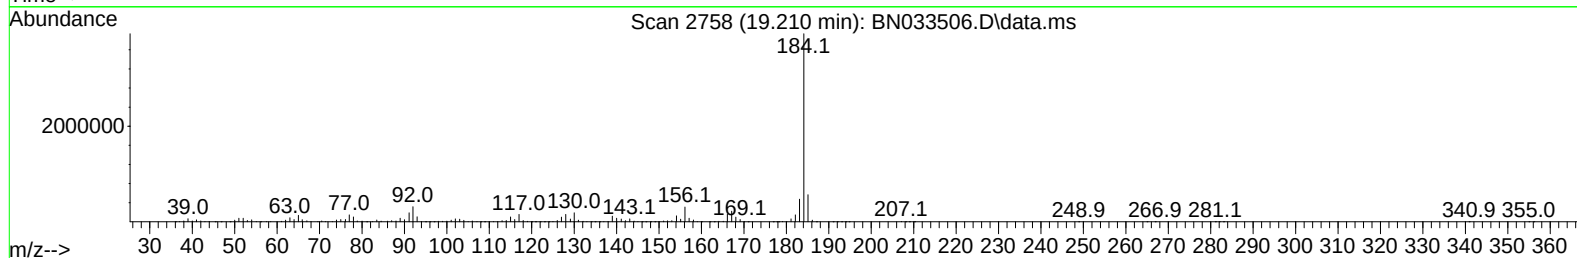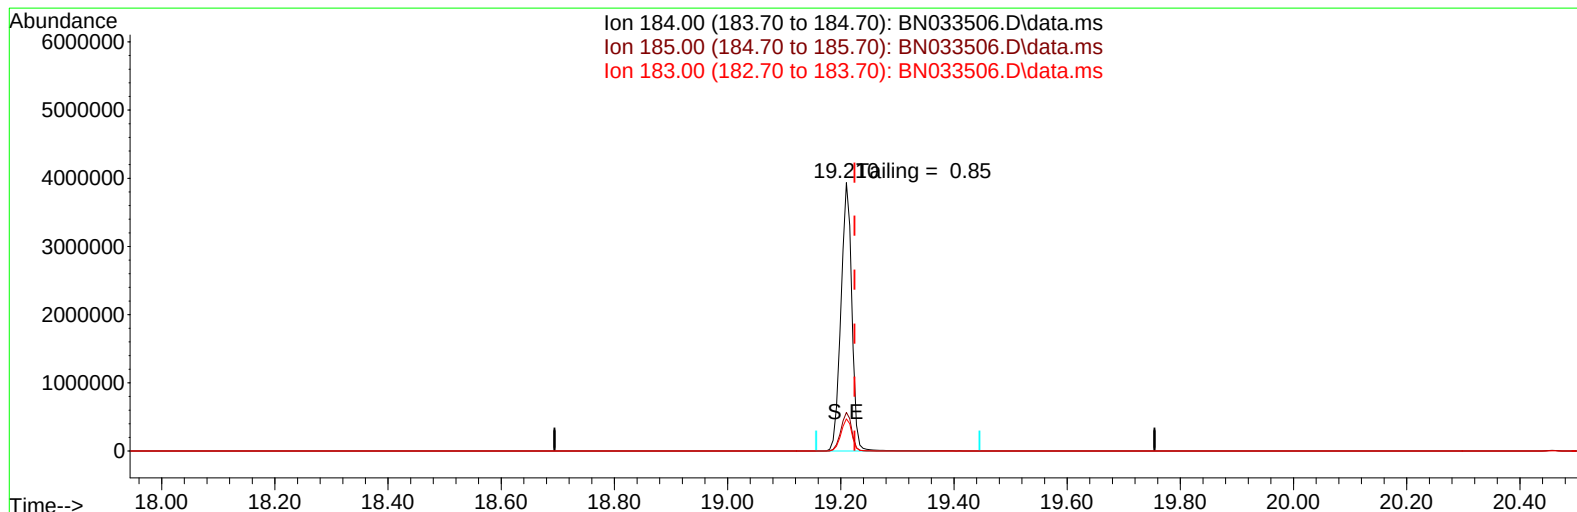

TIC: BN033506.D\data.ms

(77) Benzidine

19.210min (-0.014) 0.00 ng

response 5262962

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.38
183.00	13.20	12.01
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/20/2024	BNA_N	<u>BN033506.D</u>
Compound Name	Response	Retention Time
DDT	2476476	20.457
DDD	70091	20.016
DDE	1205	19.504
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
71296	2547772	2.80

Instrument :
BNA_N
ClientSampleId :
DFTPP