


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM082024\  
Data File : BM047272.D  
Acq On : 20 Aug 2024 15:35  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM081024.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Sun Aug 11 23:47:58 2024

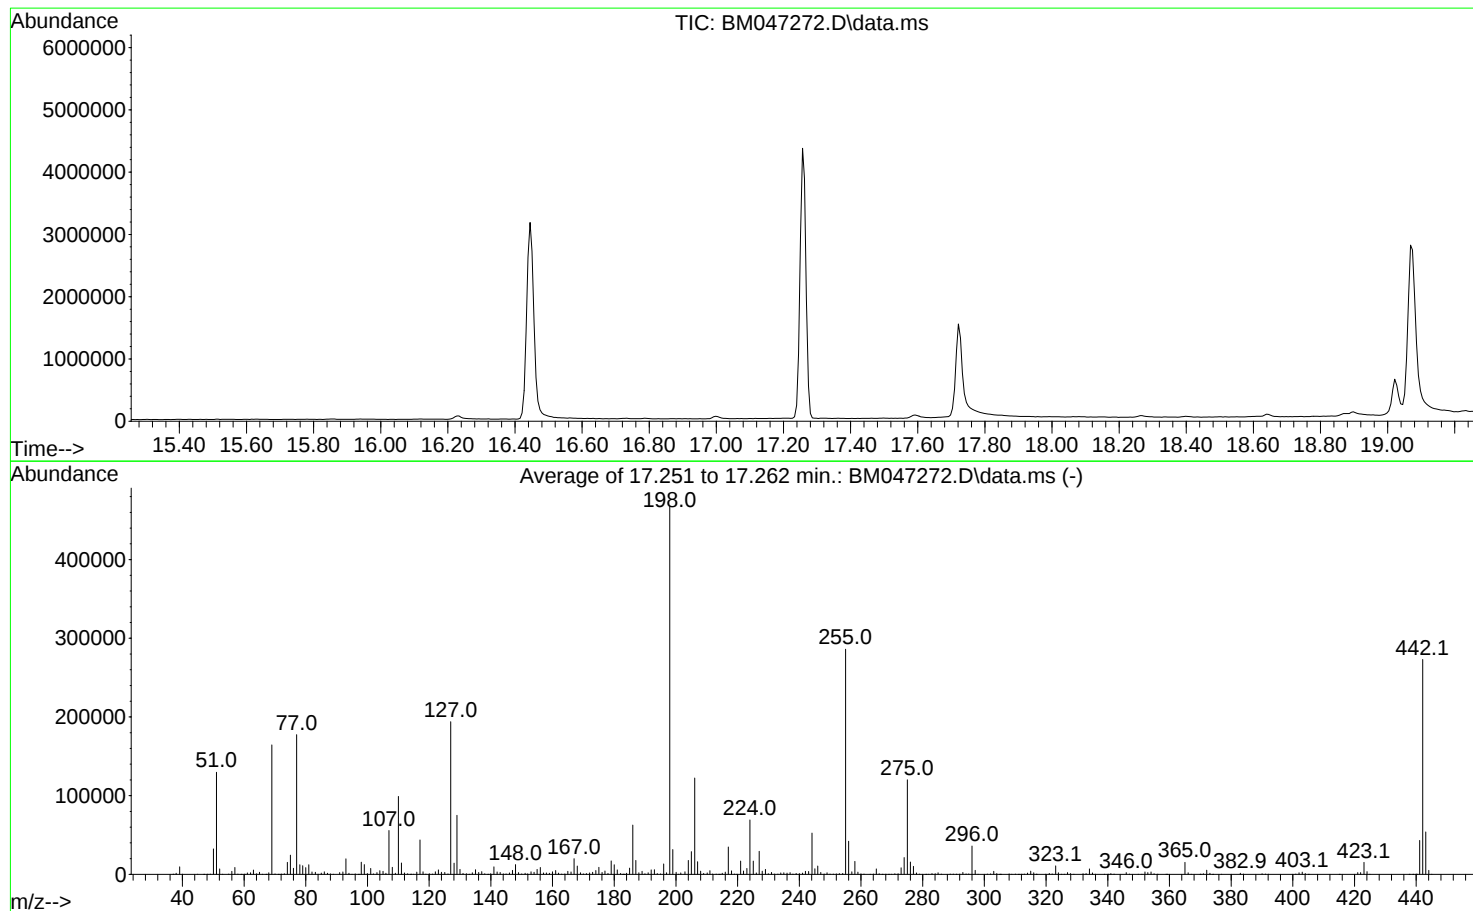

AutoFind: Scans 2442, 2443, 2444; Background Corrected with Scan 2435

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 27.7         | 129703     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.3          | 2093       | PASS                |
| 69             | 198             | 0.00            | 100             | 35.2         | 164504     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 648        | PASS                |
| 127            | 198             | 10              | 80              | 41.5         | 193906     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.4          | 2004       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 467435     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 31467      | PASS                |
| 275            | 198             | 10              | 60              | 25.7         | 120144     | PASS                |
| 365            | 198             | 1               | 100             | 3.3          | 15332      | PASS                |
| 441            | 198             | 0.01            | 100             | 9.2          | 43072      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 273109     | PASS                |
| 443            | 442             | 15              | 24              | 19.8         | 53989      | PASS                |

### DDT Breakdown



| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 8/20/2024     | BNA_M            | <u>BM047272.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1424618          | 20.315             |
| DDD           | 68922            | 19.874             |
| DDE           | 3372             | 19.356             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 72294         | 1496912          | 4.83               |
|               |                  |                    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM082024\  
Data File : BM047272.D  
Acq On : 20 Aug 2024 15:35  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Aug 20 16:33:10 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM081024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sun Aug 11 23:47:58 2024  
Response via : Initial Calibration

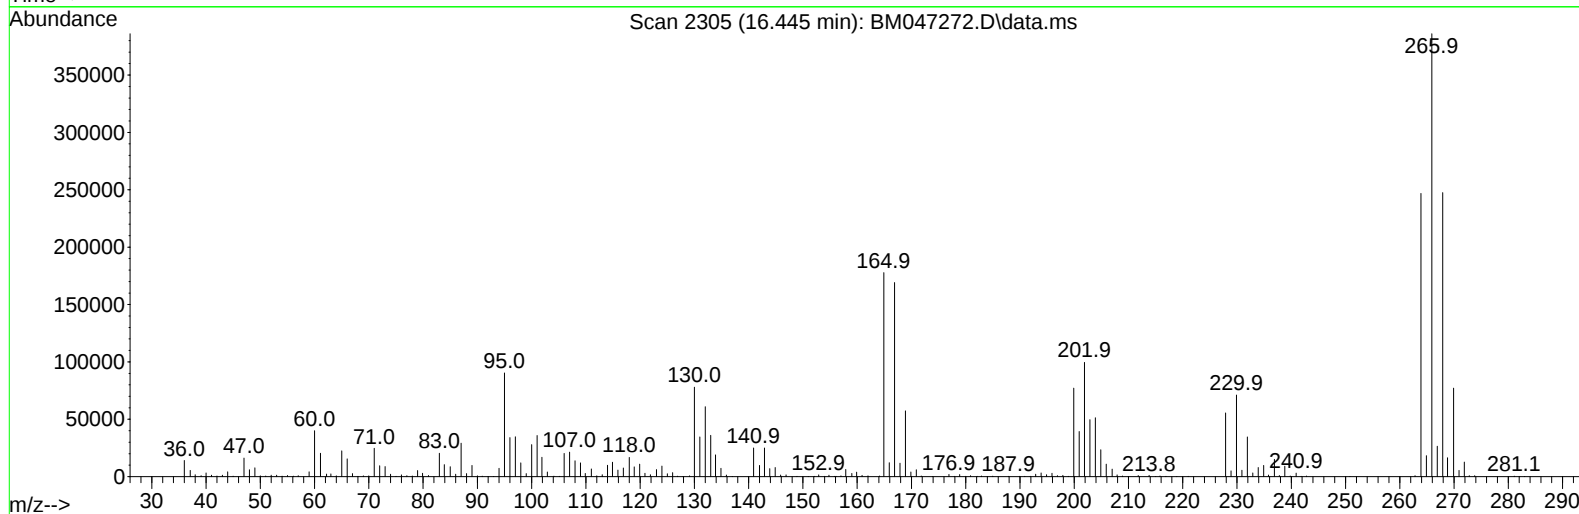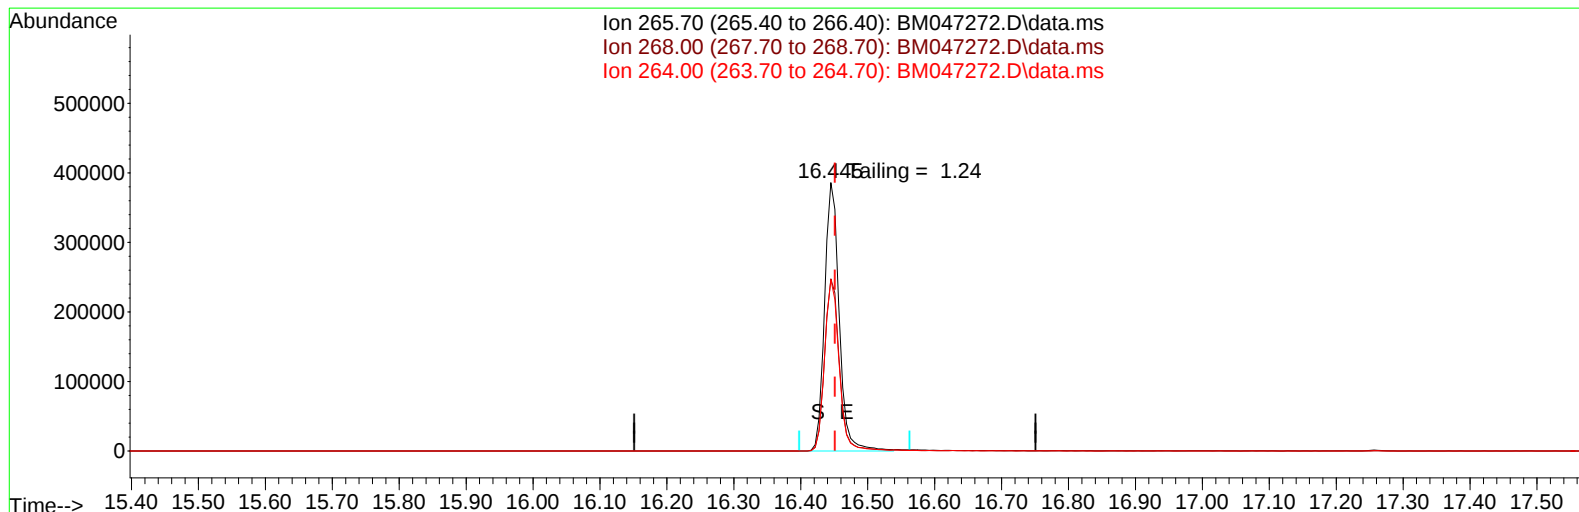

TIC: BM047272.D\data.ms

**(70) Pentachlorophenol (C)**

16.445min (-0.006) 238508.50 ng



response 588500

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 64.14  |
| 264.00 | 62.00  | 63.94  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM082024\  
Data File : BM047272.D  
Acq On : 20 Aug 2024 15:35  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Aug 20 16:33:10 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM081024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sun Aug 11 23:47:58 2024  
Response via : Initial Calibration

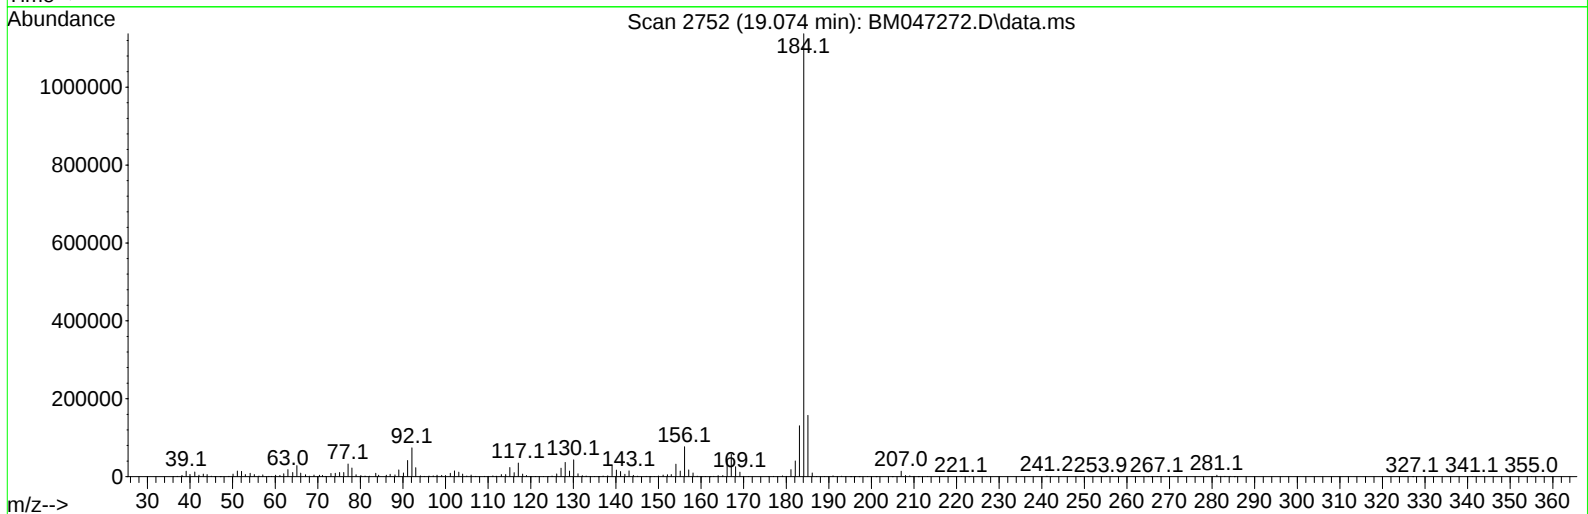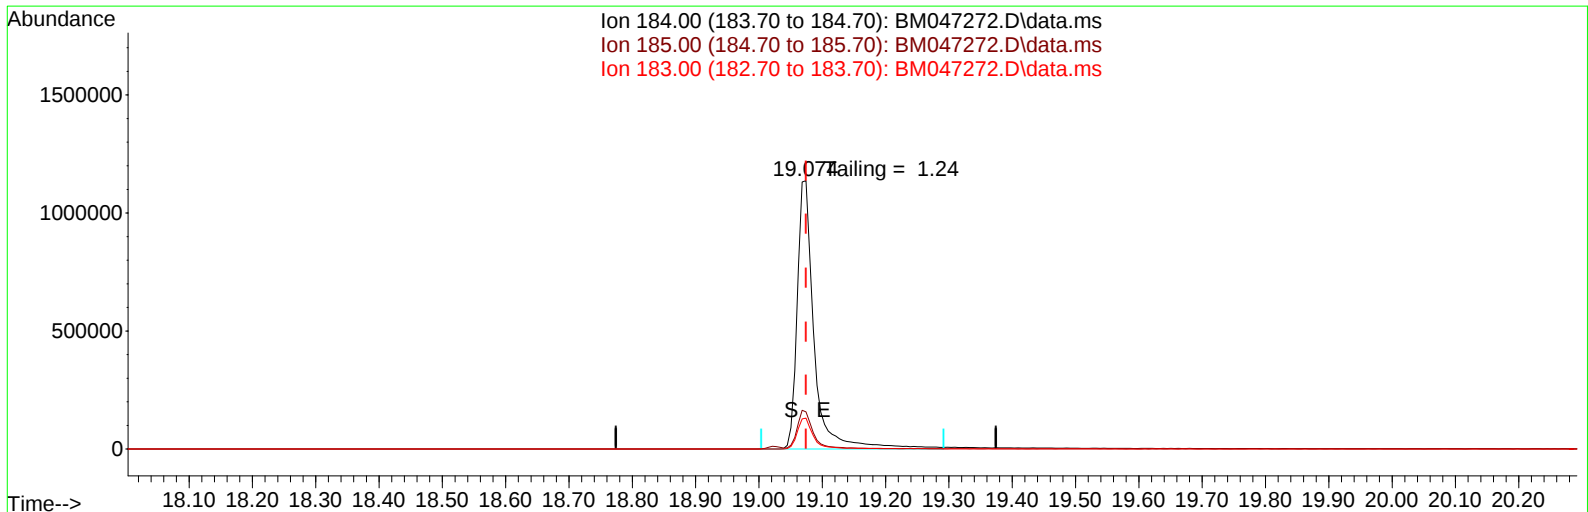

TIC: BM047272.D\data.ms

**(77) Benzidine**

**19.074min (-0.000) 24392.62 ng**

**response 2127873**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.70  | 13.84  |
| 183.00 | 11.30  | 11.50  |
| 0.00   | 0.00   | 0.00   |