
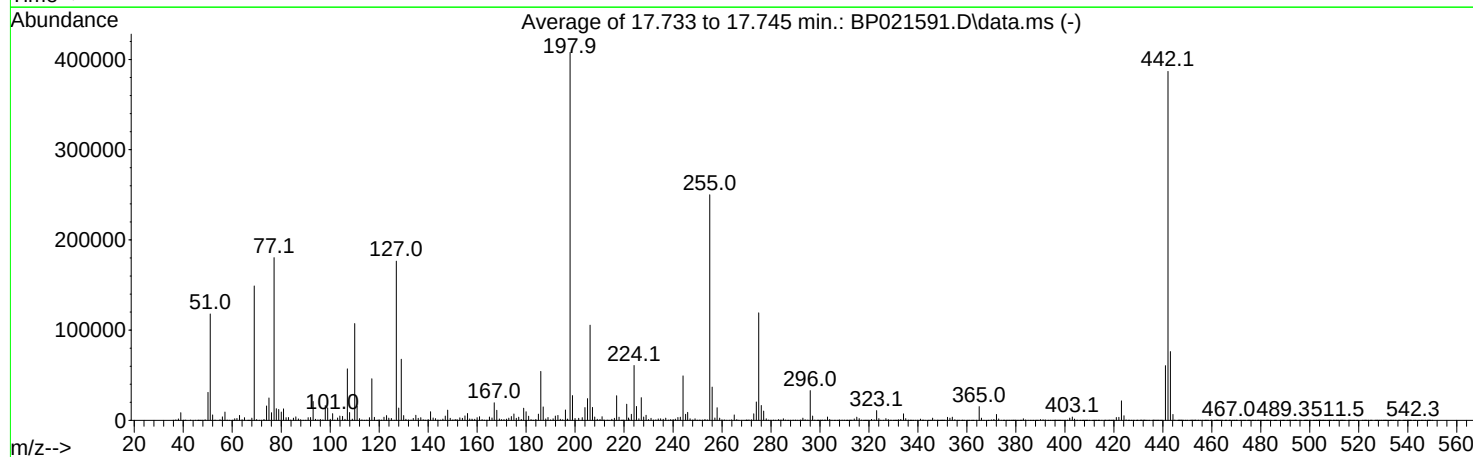


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082124\
Data File : BP021591.D
Acq On : 21 Aug 2024 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 14 00:00:30 2024

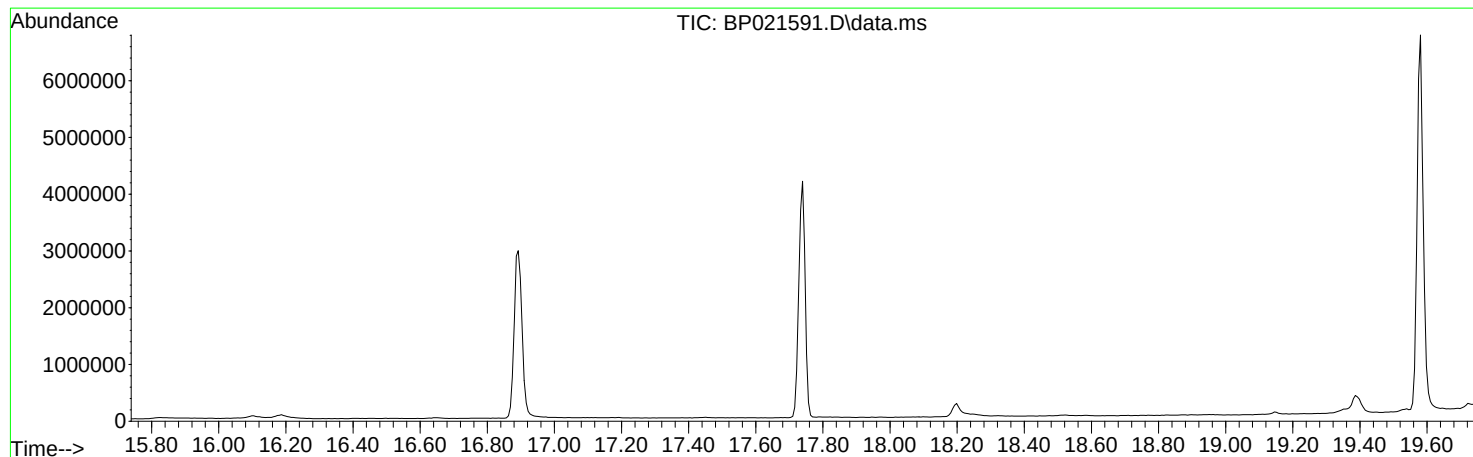

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.9	117899	PASS
68	69	0.00	2	1.7	2470	PASS
69	198	0.00	100	36.5	148969	PASS
70	69	0.00	2	0.6	879	PASS
127	198	10	80	43.3	176509	PASS
197	198	0.00	2	0.3	1413	PASS
198	198	100	100	100.0	407755	PASS
199	198	5	9	6.7	27510	PASS
275	198	10	60	29.2	119232	PASS
365	198	1	100	3.7	15281	PASS
441	198	0.01	100	14.9	60589	PASS
442	442	100	100	100.0	386880	PASS
443	442	15	24	19.7	76245	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/21/2024	BNA_P	<u>BP021591.D</u>
Compound Name	Response	Retention Time
DDT	1571840	20.886
DDD	77683	20.416
DDE	1329	19.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
79012	1650852	4.79

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082124\
Data File : BP021591.D
Acq On : 21 Aug 2024 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 21 18:32:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 00:00:30 2024
Response via : Initial Calibration

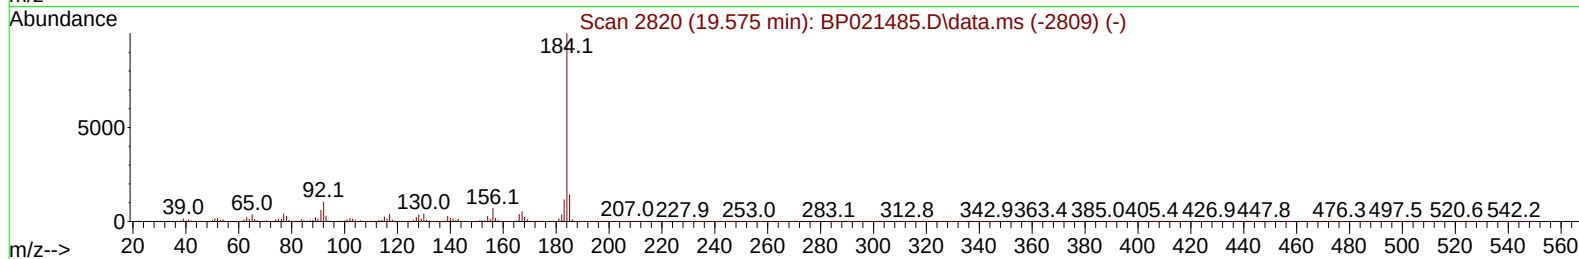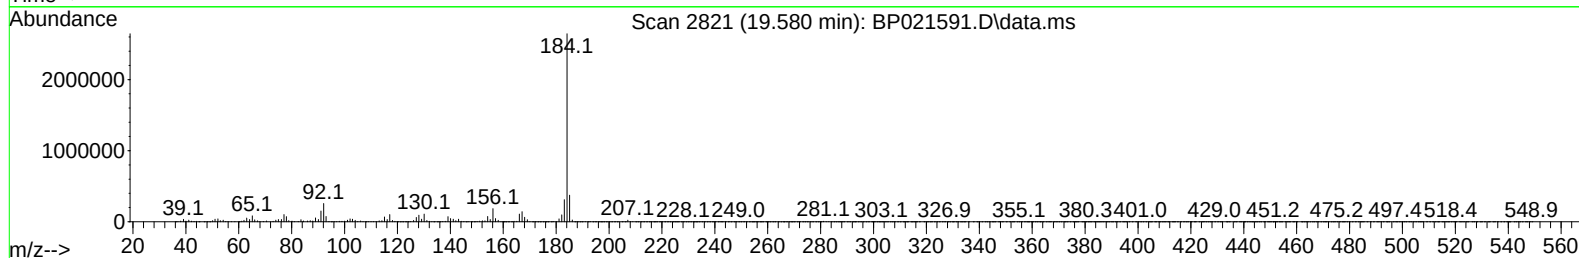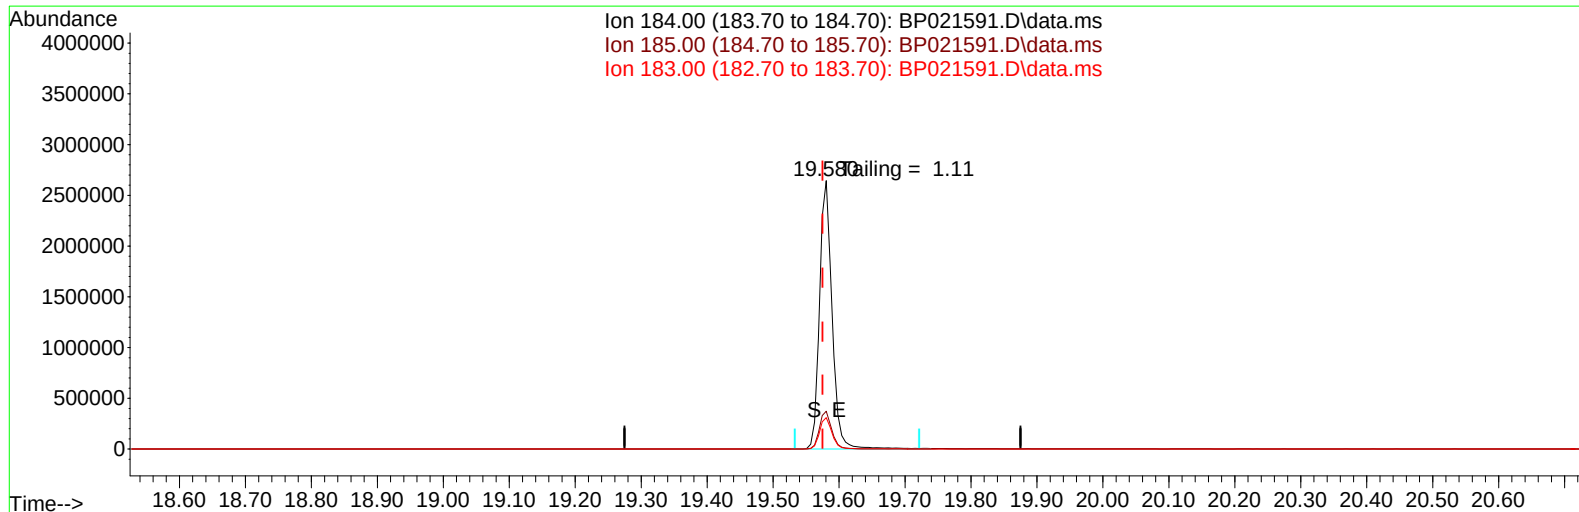

TIC: BP021591.D\data.ms

(77) Benzidine

19.580min (+ 0.005) -20.00 ng

response 3491621

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.10
183.00	11.60	11.72
0.00	0.00	0.00