
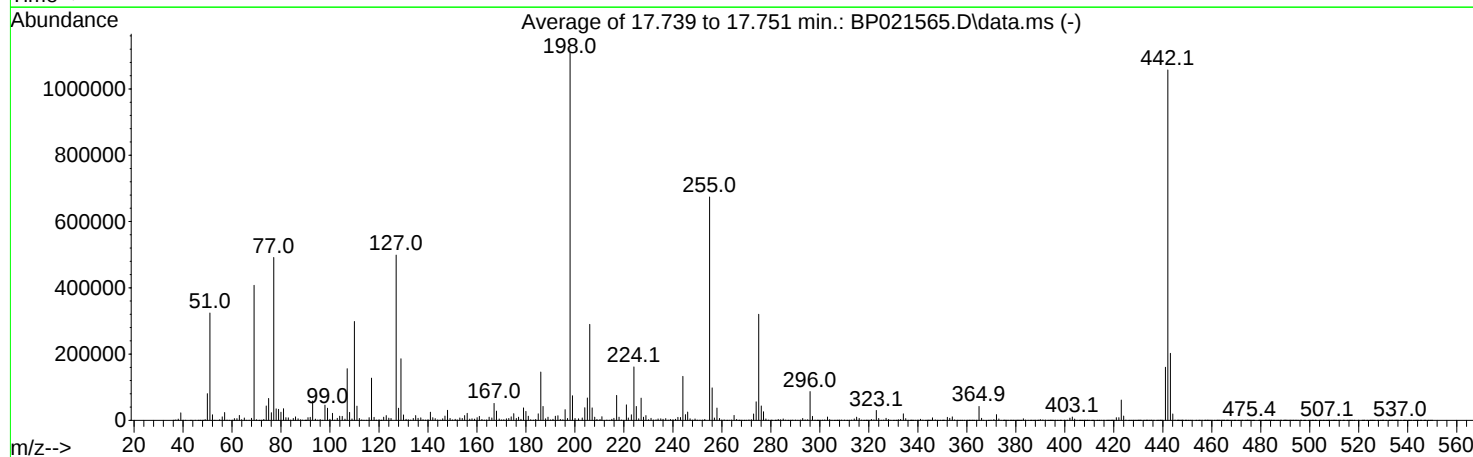


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082024\
Data File : BP021565.D
Acq On : 20 Aug 2024 09:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 14 00:00:30 2024

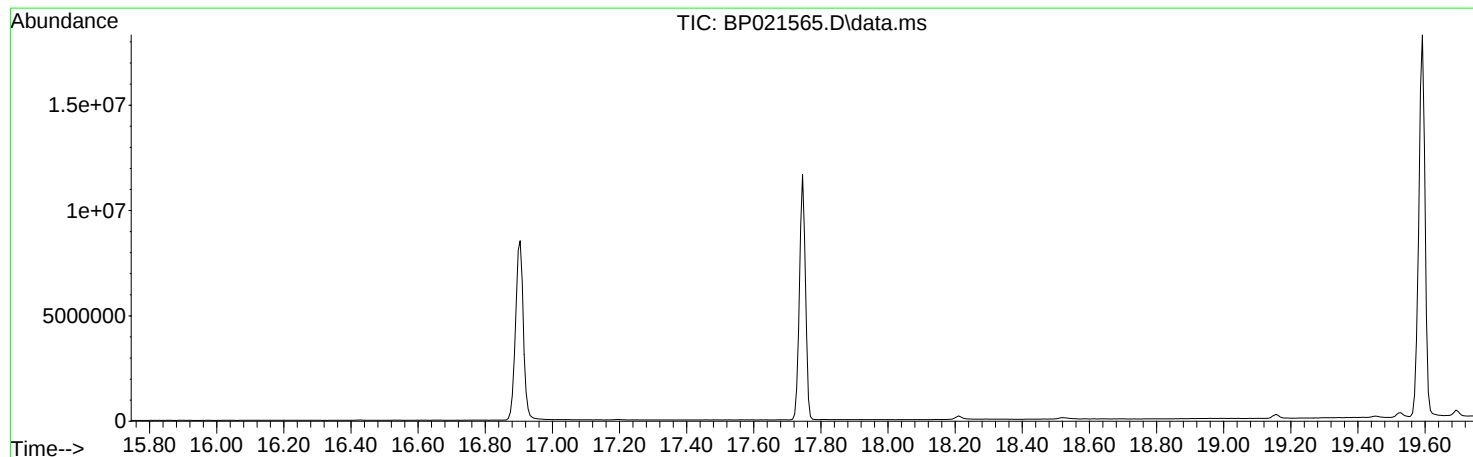

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.2	324123	PASS
68	69	0.00	2	1.6	6547	PASS
69	198	0.00	100	36.7	407478	PASS
70	69	0.00	2	0.5	2016	PASS
127	198	10	80	44.9	498814	PASS
197	198	0.00	2	0.5	5669	PASS
198	198	100	100	100.0	1109972	PASS
199	198	5	9	6.7	74231	PASS
275	198	10	60	28.9	320288	PASS
365	198	1	100	3.8	42187	PASS
441	198	0.01	100	14.4	160344	PASS
442	442	100	100	100.0	1057190	PASS
443	442	15	24	19.1	202151	PASS

DDT Breakdown



Date	Instrument Name	DFTPP Data File
8/20/2024	BNA_P	<u>BP021565.D</u>
Compound Name	Response	Retention Time
DDT	4160702	20.892
DDD	231762	20.422
DDE	2972	19.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
234734	4395436	5.34

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082024\
Data File : BP021565.D
Acq On : 20 Aug 2024 09:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 20 11:19:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 00:00:30 2024
Response via : Initial Calibration

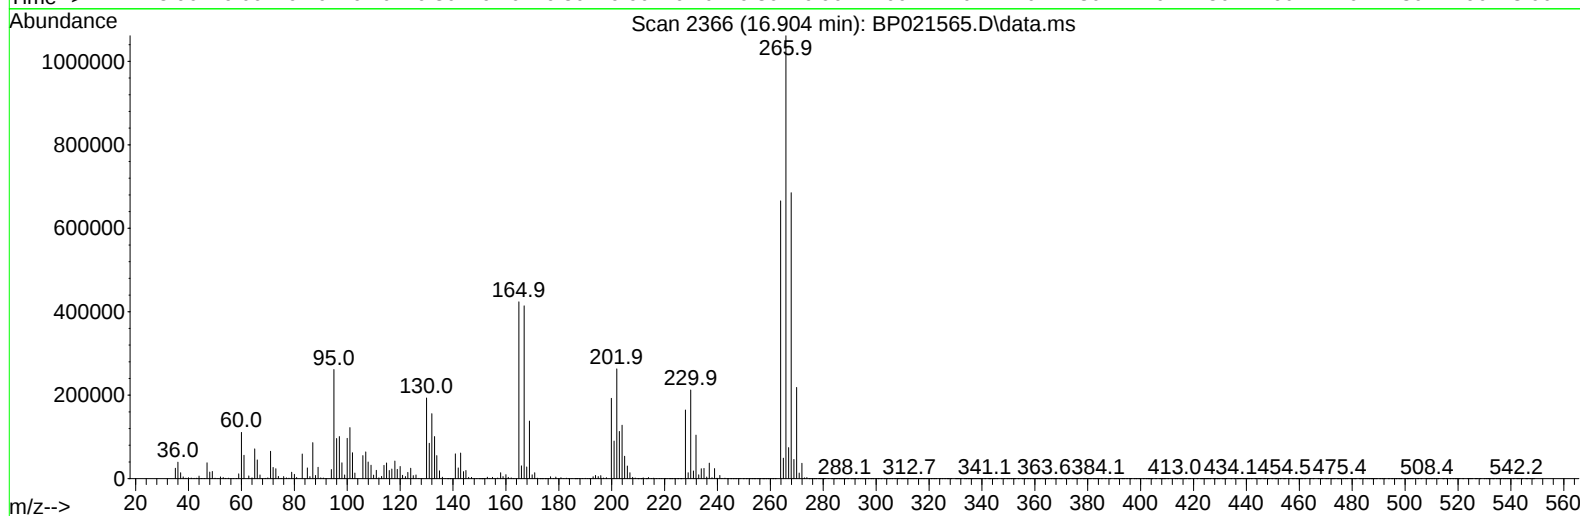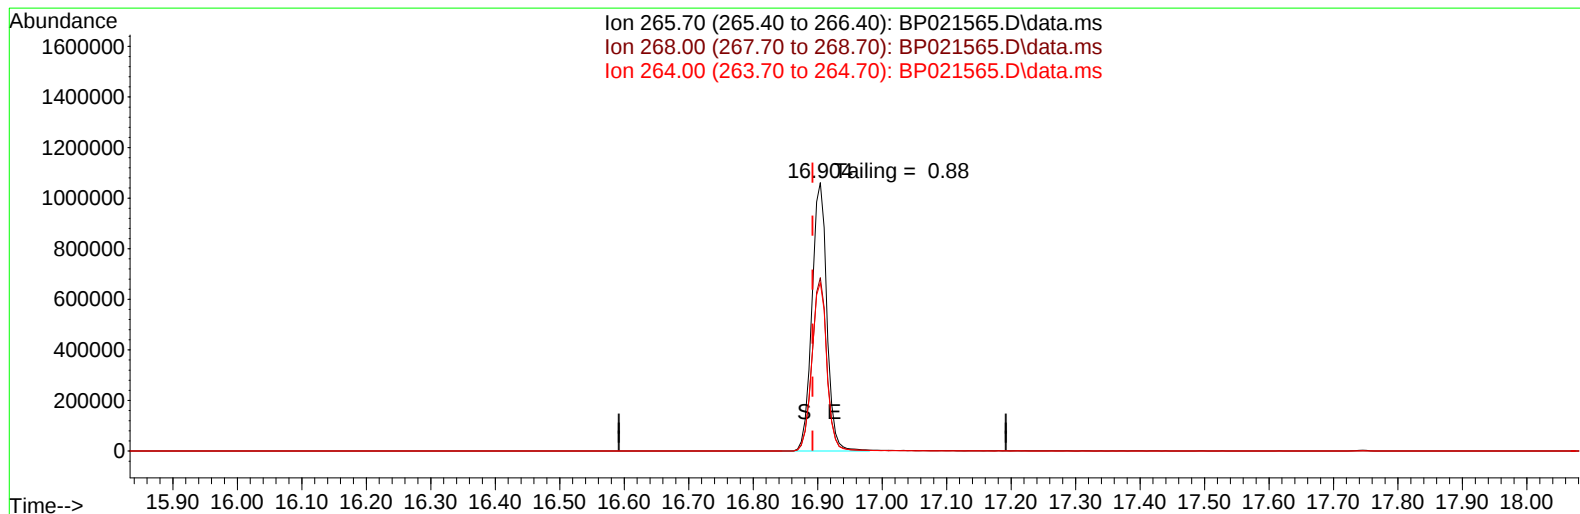

TIC: BP021565.D\data.ms

(70) Pentachlorophenol (C)

16.904min (+ 0.012) 916265.56 ng



response 1726349

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	64.57
264.00	63.10	62.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082024\
Data File : BP021565.D
Acq On : 20 Aug 2024 09:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 20 11:19:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 00:00:30 2024
Response via : Initial Calibration

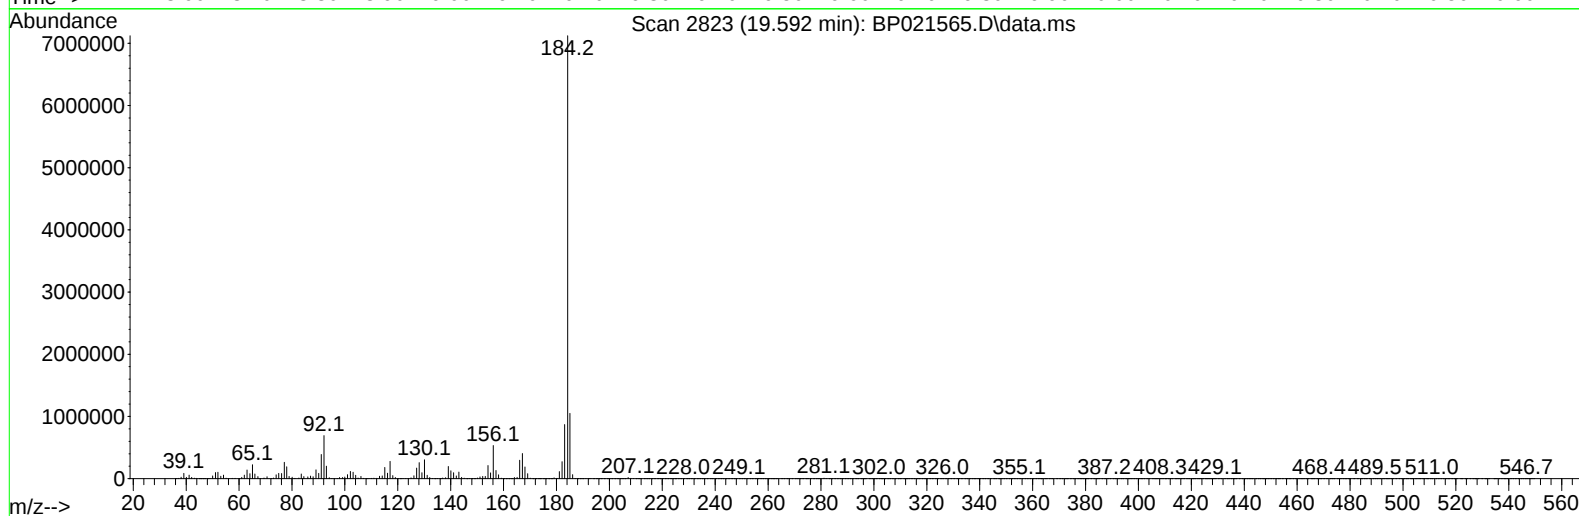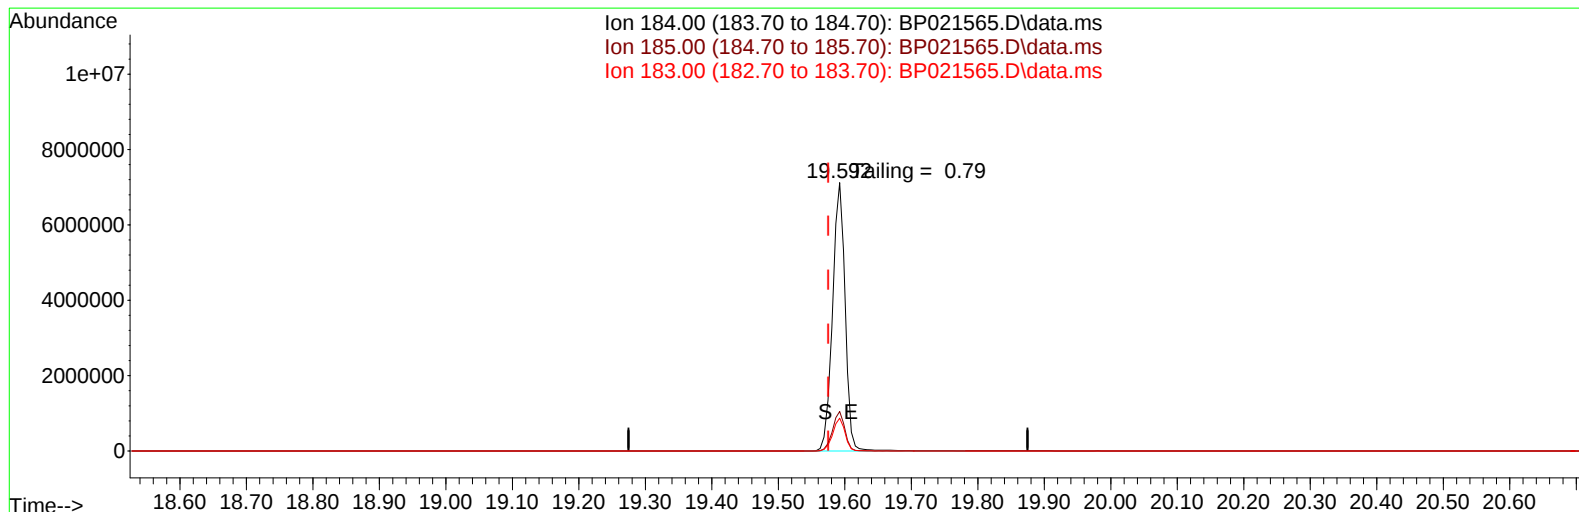

TIC: BP021565.D\data.ms

(77) Benzidine**19.592min (+ 0.017) -20.00 ng****response 9393500**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.73
183.00	11.60	12.22
0.00	0.00	0.00