


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082024\
Data File : BP021574.D
Acq On : 20 Aug 2024 15:57
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 14 00:00:30 2024

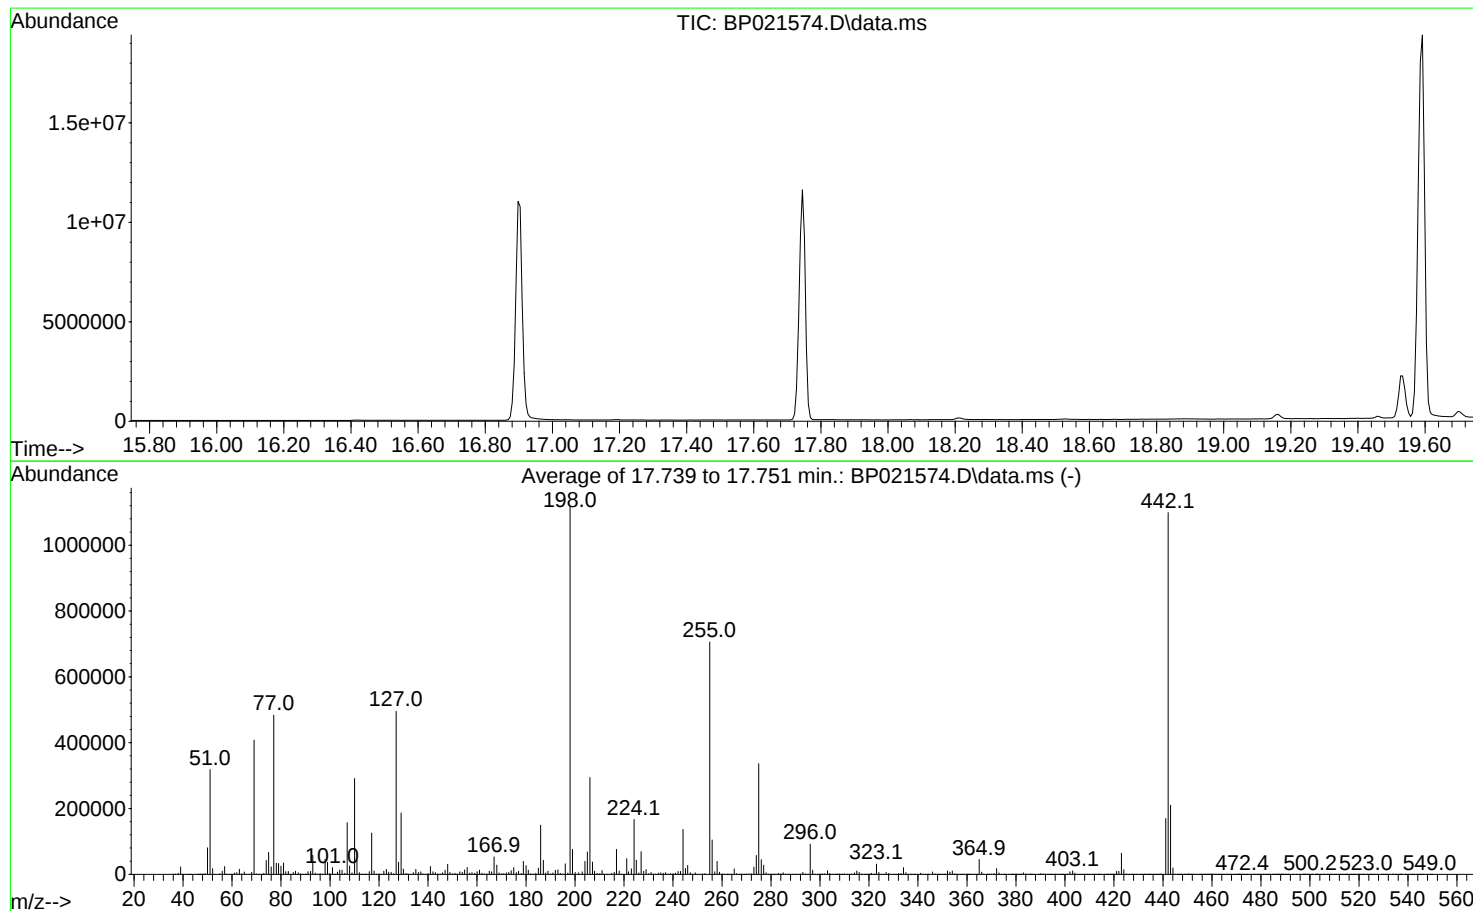

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2496

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.5	318494	PASS
68	69	0.00	2	1.6	6404	PASS
69	198	0.00	100	36.5	407976	PASS
70	69	0.00	2	0.4	1654	PASS
127	198	10	80	44.3	495609	PASS
197	198	0.00	2	0.3	3742	PASS
198	198	100	100	100.0	1117661	PASS
199	198	5	9	6.8	76061	PASS
275	198	10	60	30.1	336655	PASS
365	198	1	100	4.0	45002	PASS
441	198	0.01	100	15.2	169704	PASS
442	442	100	100	100.0	1099215	PASS
443	442	15	24	19.1	210240	PASS

DDT Breakdown



Date	Instrument Name	DFTPP Data File
8/20/2024	BNA_P	<u>BP021574.D</u>
Compound Name	Response	Retention Time
DDT	4861860	20.892
DDD	175942	20.427
DDE	3862	19.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
179804	5041664	3.57

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082024\
Data File : BP021574.D
Acq On : 20 Aug 2024 15:57
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 20 16:56:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 00:00:30 2024
Response via : Initial Calibration

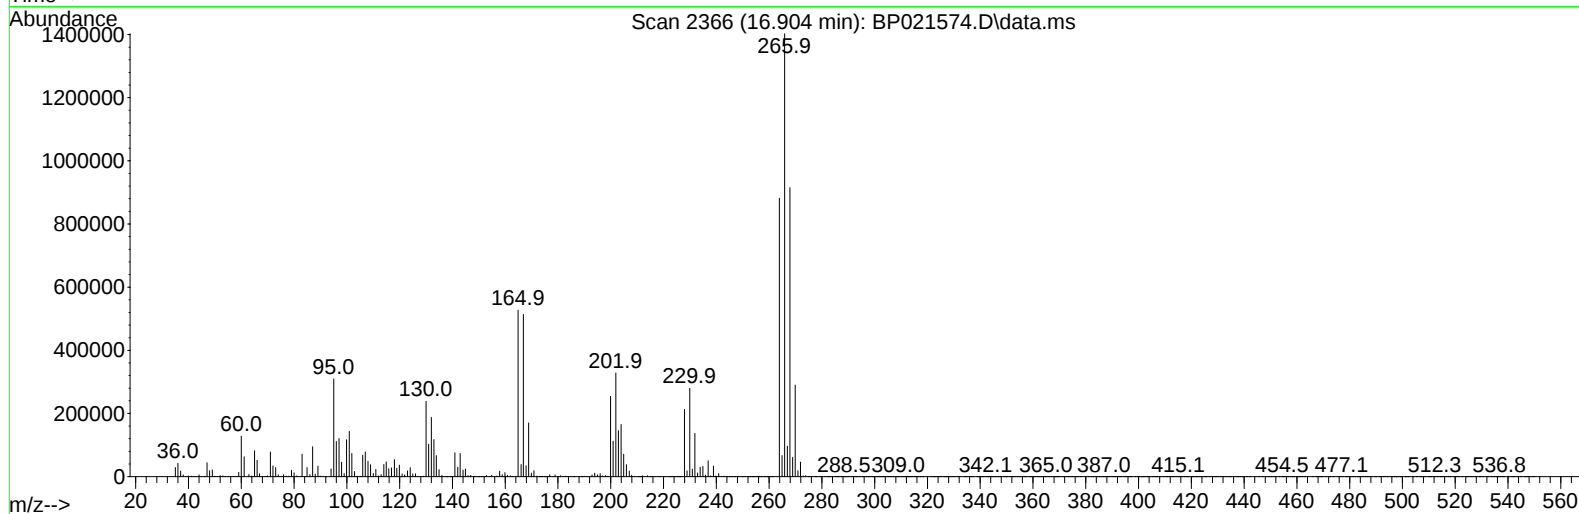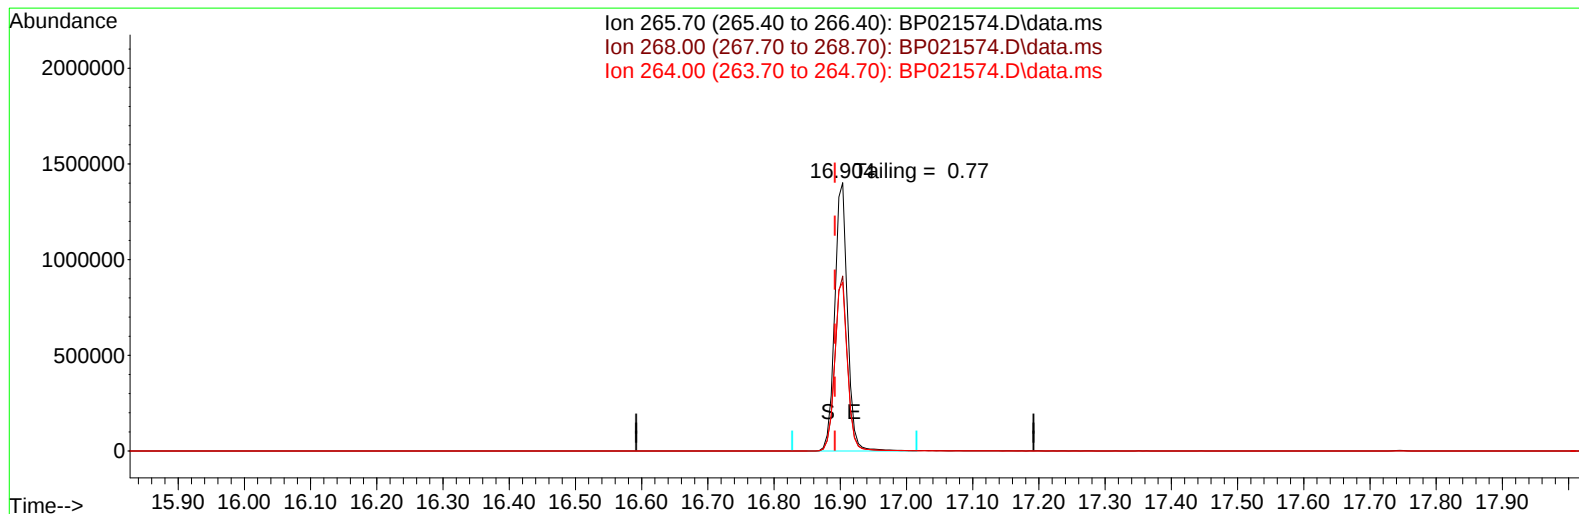

TIC: BP021574.D\data.ms

(70) Pentachlorophenol (C)

16.904min (+ 0.012) 1466831.19 ng



response 1882505

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	65.26
264.00	63.10	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082024\
Data File : BP021574.D
Acq On : 20 Aug 2024 15:57
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 20 16:56:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 00:00:30 2024
Response via : Initial Calibration

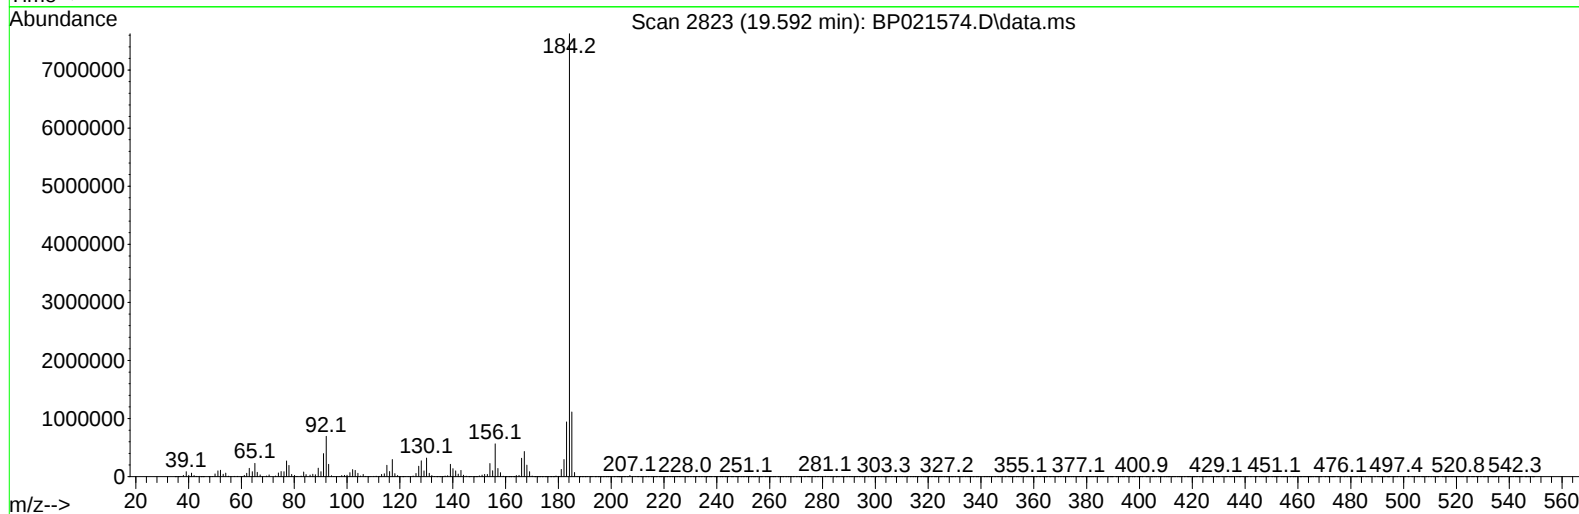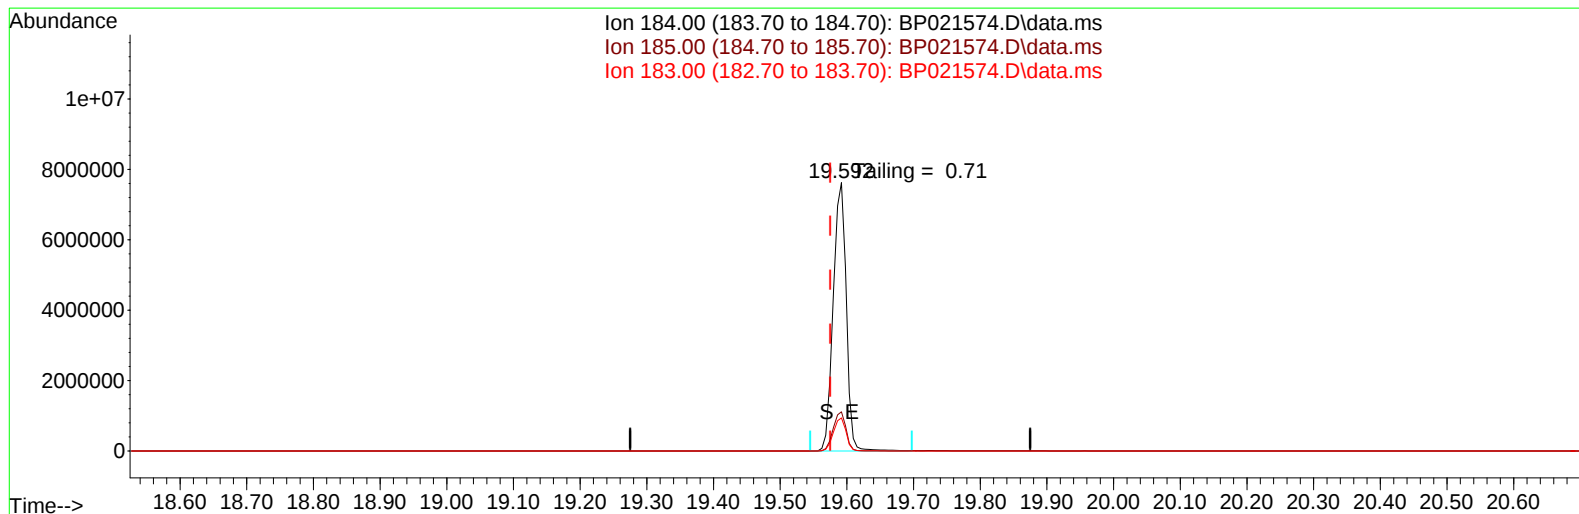

TIC: BP021574.D\data.ms

(77) Benzidine**19.592min (+ 0.017) -20.00 ng****response 10375641**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.60
183.00	11.60	12.36
0.00	0.00	0.00