


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081924\
Data File : BN033478.D
Acq On : 19 Aug 2024 15:37
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 19 23:32:18 2024

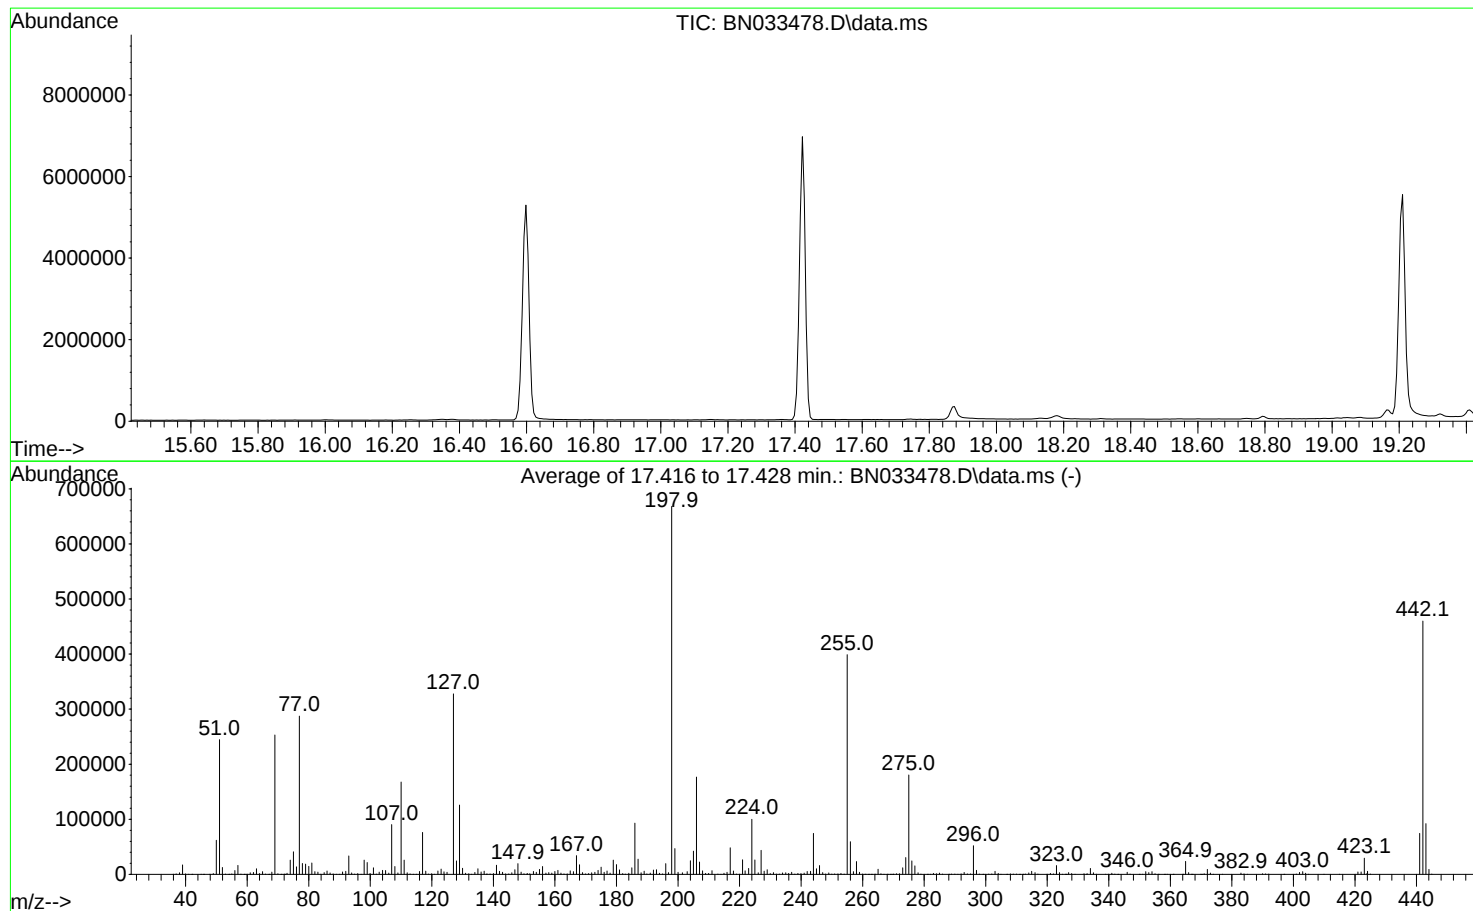




AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	244669	PASS
68	69	0.00	2	1.6	3975	PASS
69	198	0.00	100	37.9	253111	PASS
70	69	0.00	2	0.4	1124	PASS
127	198	10	80	49.1	327765	PASS
197	198	0.00	2	0.5	3324	PASS
198	198	100	100	100.0	667925	PASS
199	198	5	9	7.0	46784	PASS
275	198	10	60	27.0	180331	PASS
365	198	1	100	3.5	23424	PASS
441	198	0.01	100	11.2	74525	PASS
442	442	50	100	100.0	459861	PASS
443	442	15	24	20.0	92101	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081924\
Data File : BN033478.D
Acq On : 19 Aug 2024 15:37
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 20 04:50:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 20 04:49:48 2024
Response via : Initial Calibration

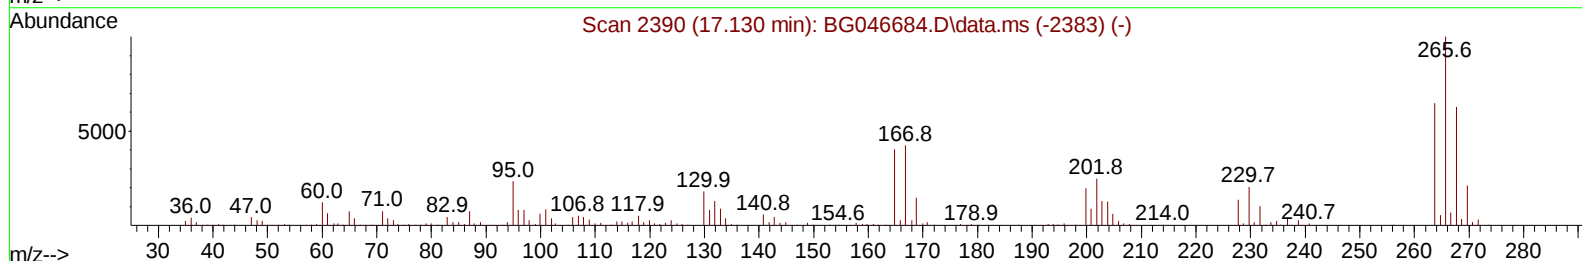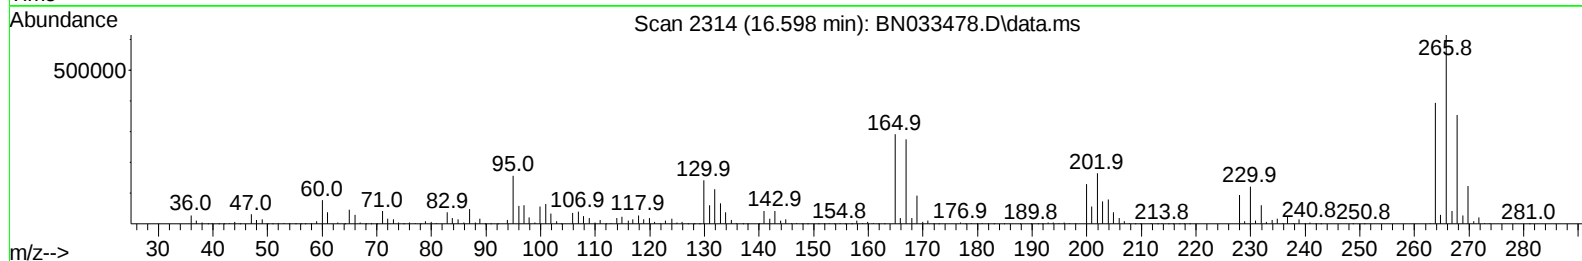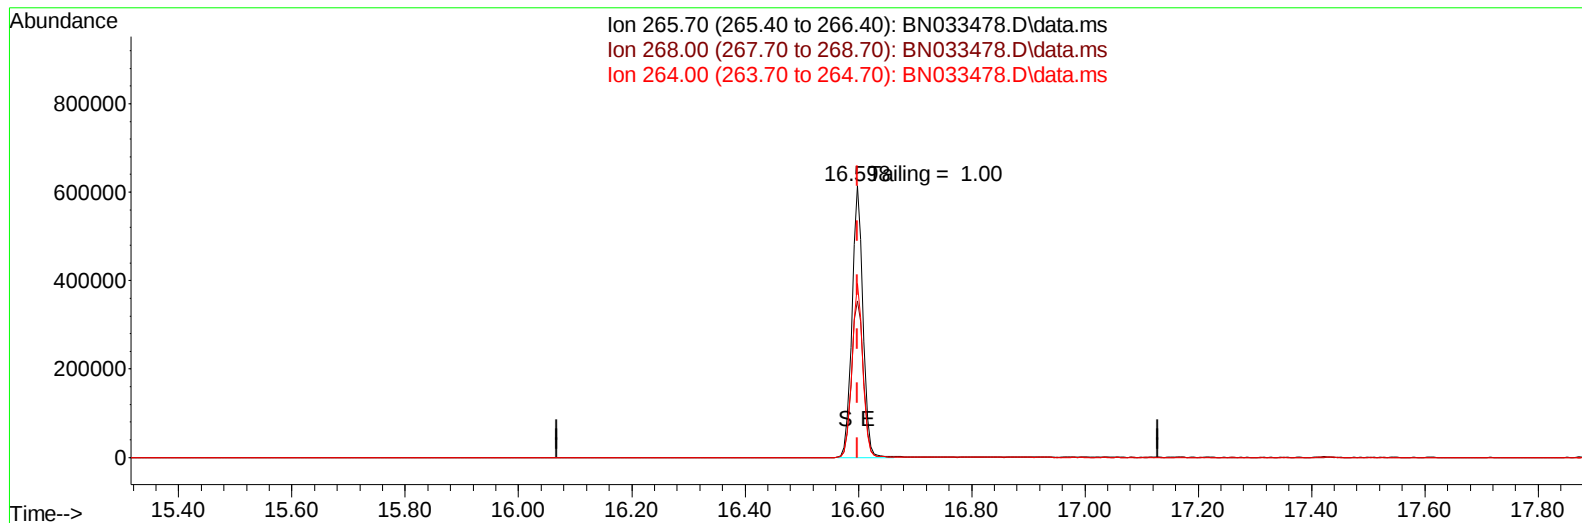

TIC: BN033478.D\data.ms

(70) Pentachlorophenol (C)

16.598min (-0.000) 25243.84 ng




response 836211

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.76
264.00	61.60	64.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081924\
Data File : BN033478.D
Acq On : 19 Aug 2024 15:37
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 20 04:50:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 20 04:49:48 2024
Response via : Initial Calibration

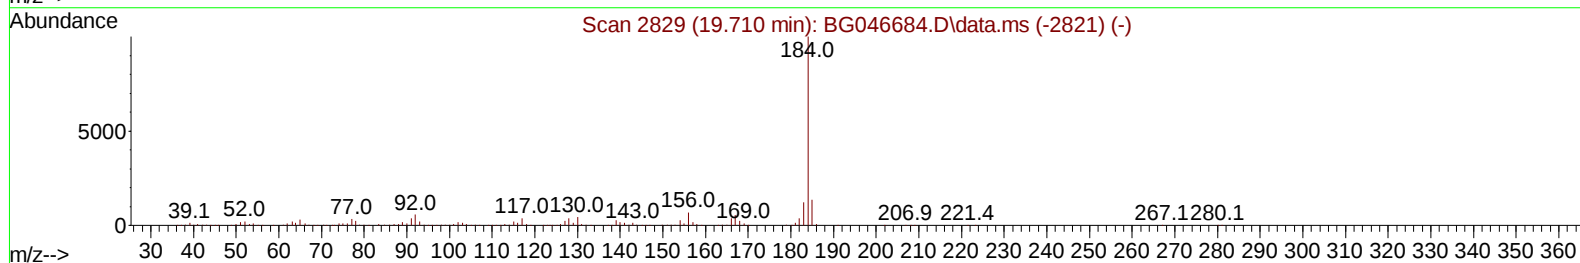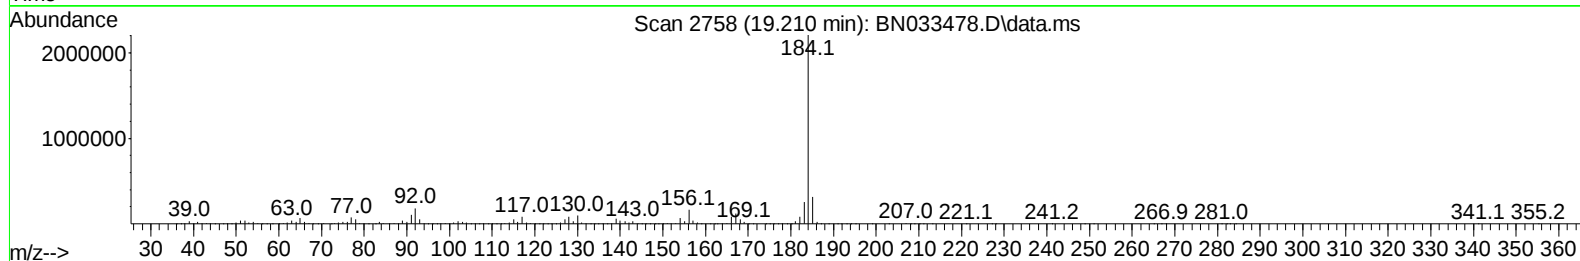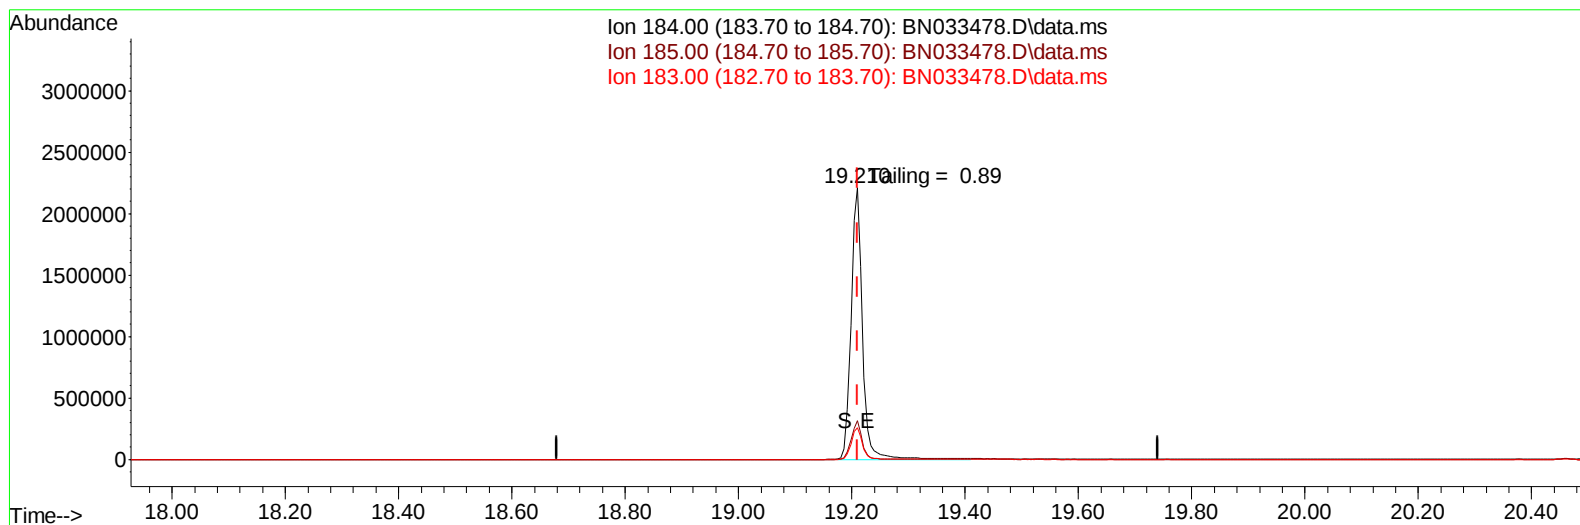

TIC: BN033478.D\data.ms

(77) Benzidine

19.210min (-0.000) 1831888.84 ng

response 3105776

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.31
183.00	13.20	11.63
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/19/2024	BNA_N	<u>BN033478.D</u>
Compound Name	Response	Retention Time
DDT	2164760	20.463
DDD	37665	20.016
DDE	773	19.51
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
38438	2203198	1.74

Instrument :
BNA_N
ClientSampleId :
DFTPP