
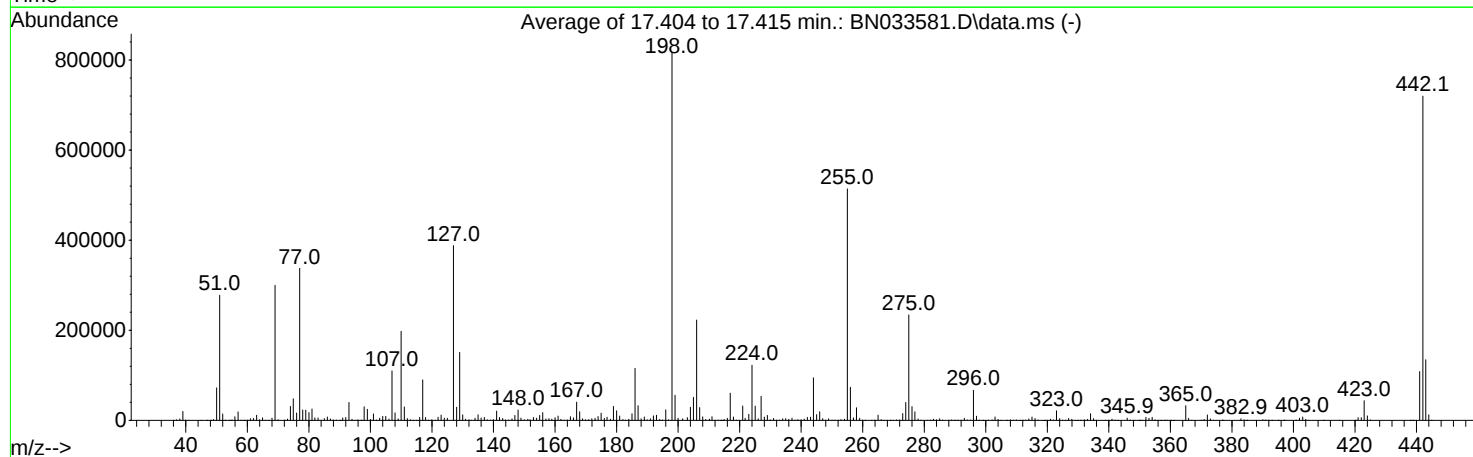


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082324\
Data File : BN033581.D
Acq On : 23 Aug 2024 09:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 23 00:22:18 2024

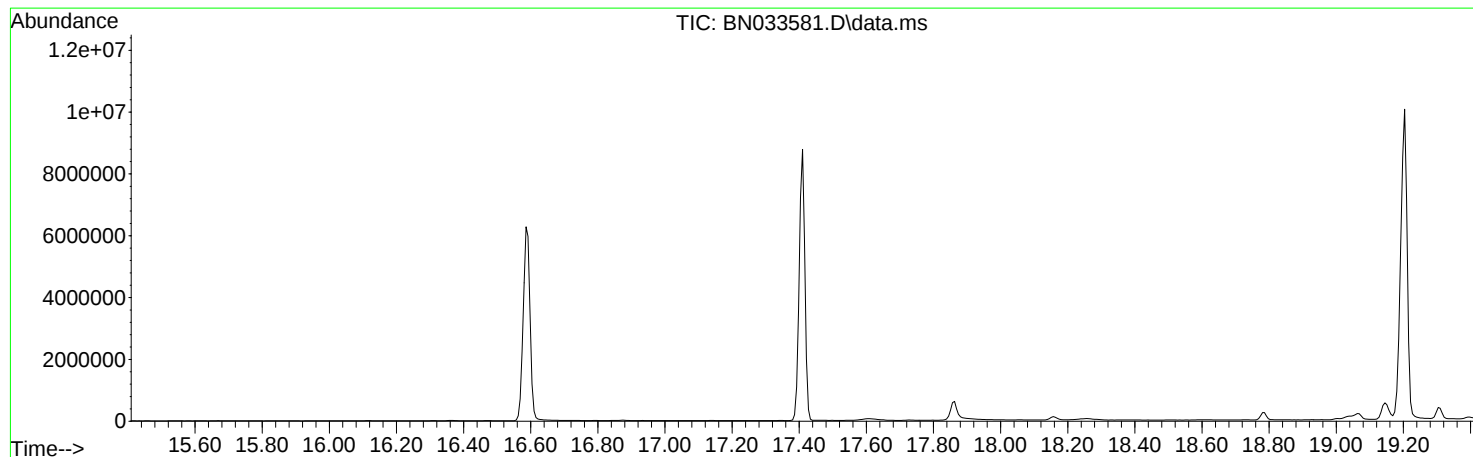

AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2443

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	277730	PASS
68	69	0.00	2	1.6	4842	PASS
69	198	0.00	100	36.7	299688	PASS
70	69	0.00	2	0.4	1334	PASS
127	198	10	80	47.5	387861	PASS
197	198	0.00	2	0.2	1293	PASS
198	198	100	100	100.0	816640	PASS
199	198	5	9	6.8	55896	PASS
275	198	10	60	28.7	234197	PASS
365	198	1	100	4.0	32875	PASS
441	198	0.01	100	13.3	108448	PASS
442	442	50	100	100.0	719509	PASS
443	442	15	24	18.7	134733	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/23/2024	BNA_N	<u>BN033581.D</u>
Compound Name	Response	Retention Time
DDT	2823987	20.451
DDD	38911	20.057
DDE	349	19.492
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
39260	2863247	1.37

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082324\
Data File : BN033581.D
Acq On : 23 Aug 2024 09:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 24 06:44:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 24 06:44:36 2024
Response via : Initial Calibration

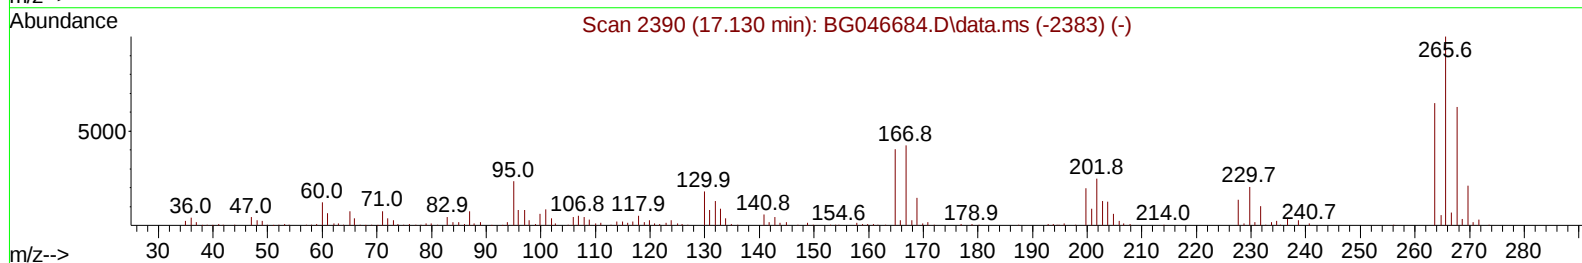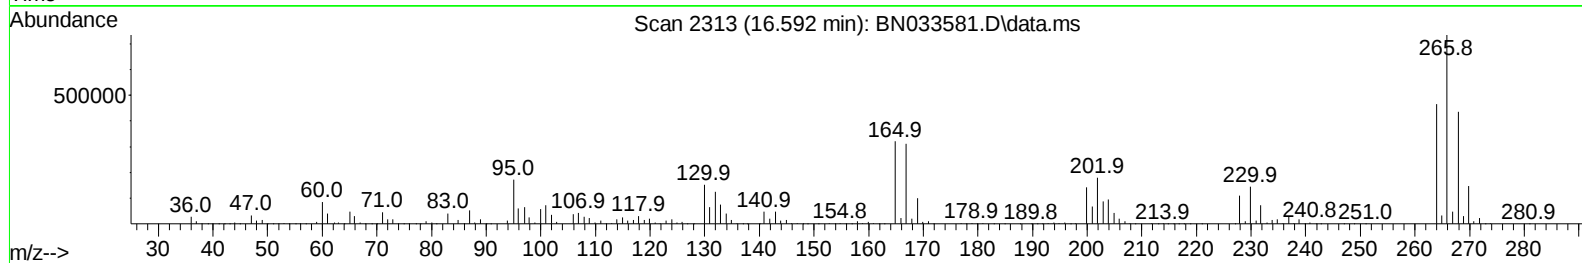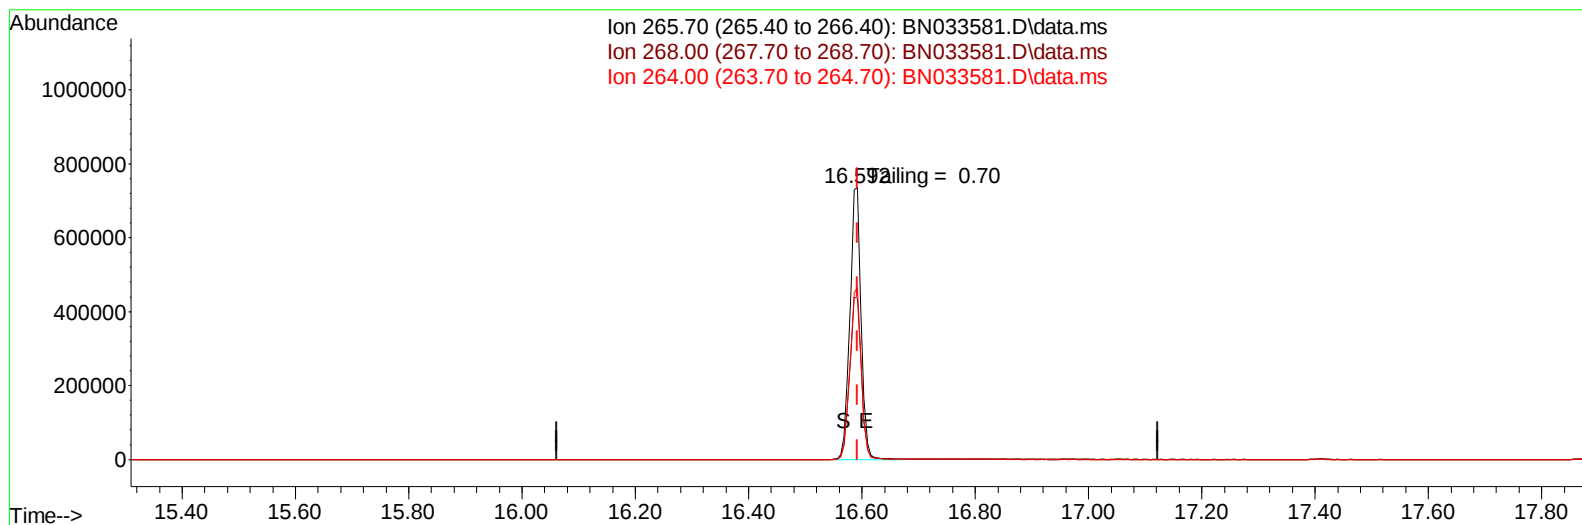

TIC: BN033581.D\data.ms

(70) Pentachlorophenol (C)

16.592min (0.000) 248809.79 ng




response 1021208

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.36
264.00	61.60	63.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082324\
Data File : BN033581.D
Acq On : 23 Aug 2024 09:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 24 06:44:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 24 06:44:36 2024
Response via : Initial Calibration

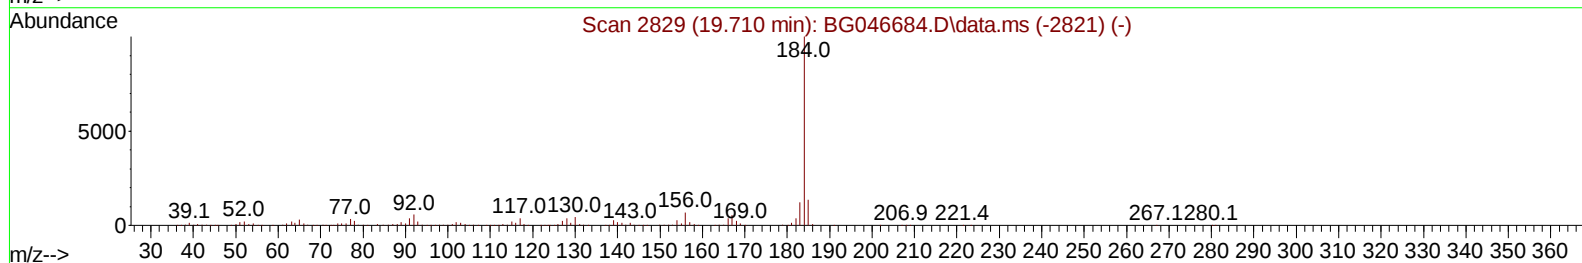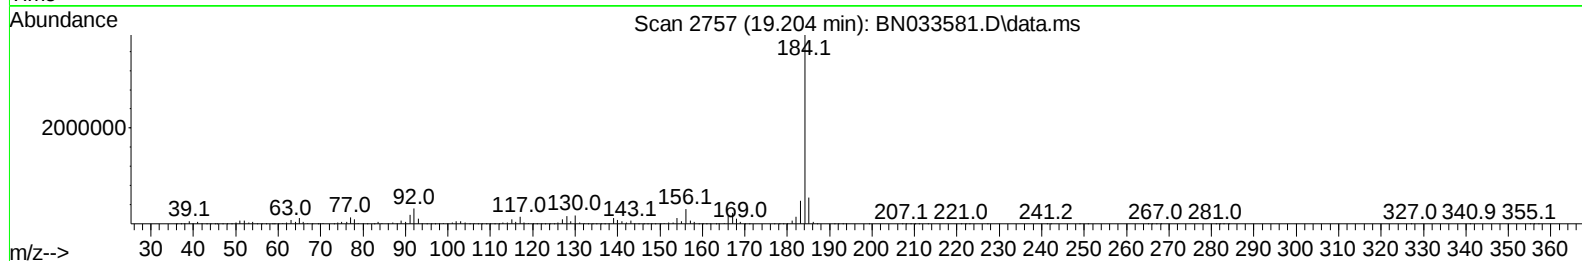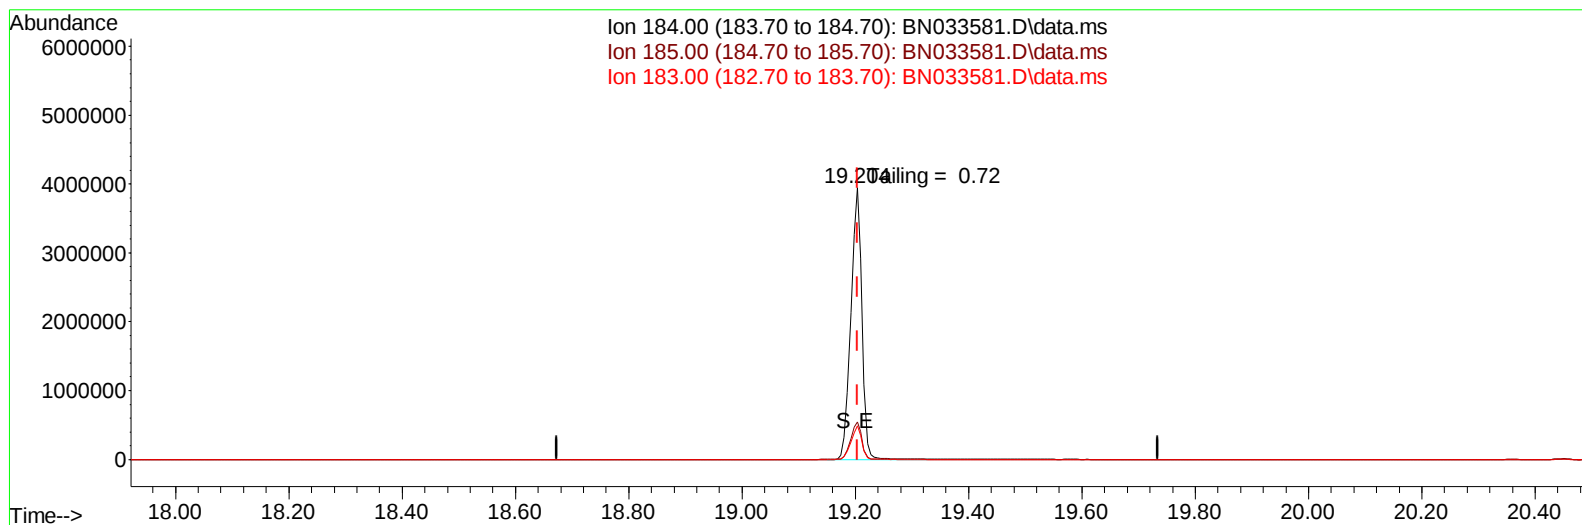

TIC: BN033581.D\data.ms

(77) Benzidine

19.204min (0.000) 4281.63 ng

response 5372497

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.90
183.00	13.20	12.29
0.00	0.00	0.00