


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082224\
Data File : BM047307.D
Acq On : 22 Aug 2024 08:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun Aug 11 23:47:58 2024

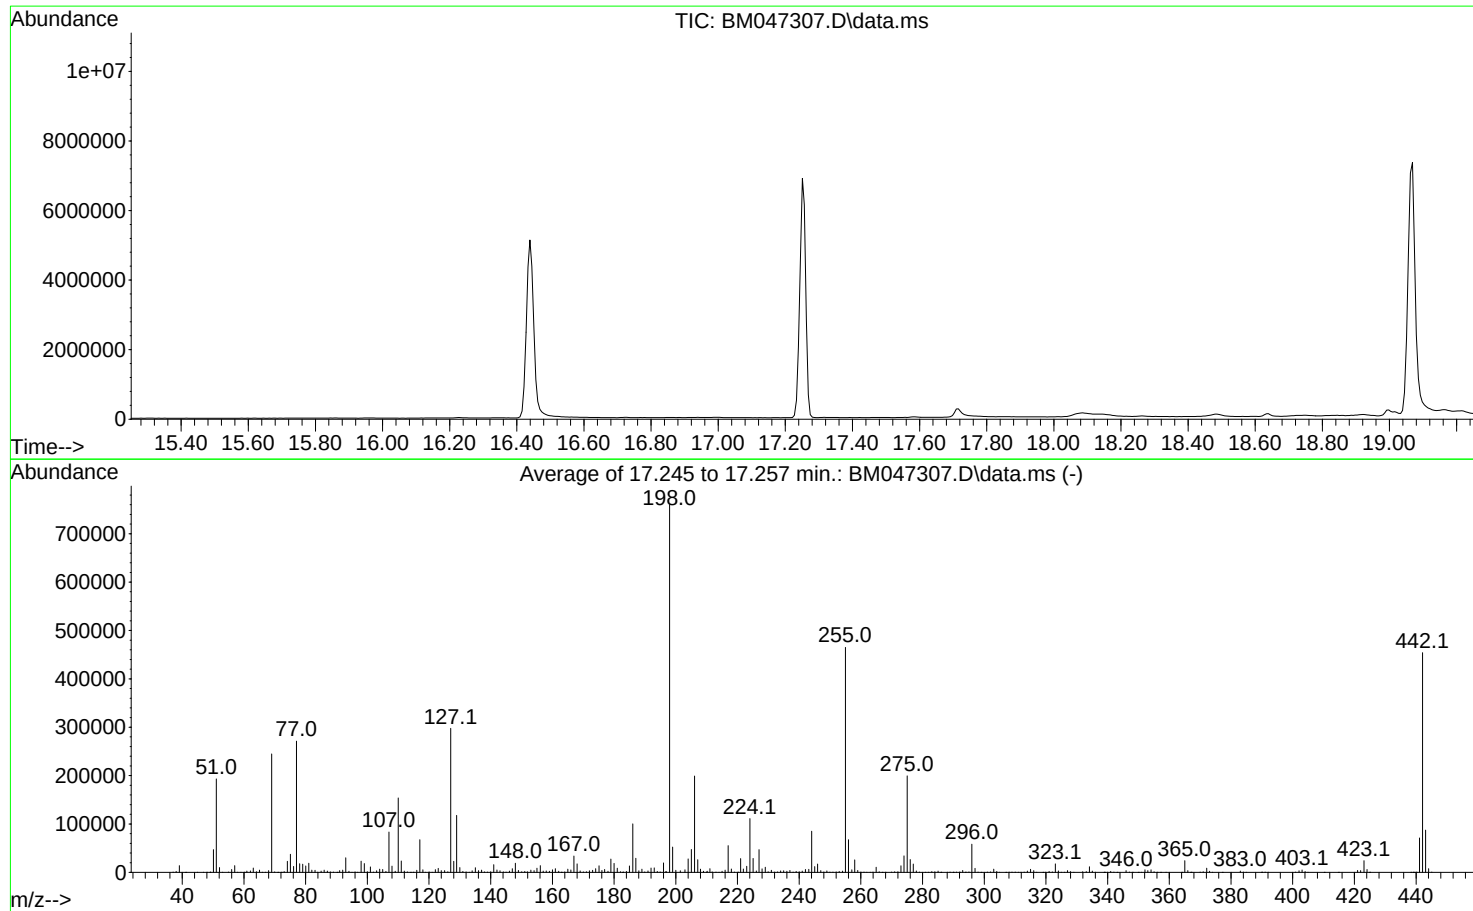

AutoFind: Scans 2441, 2442, 2443; Background Corrected with Scan 2434

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.4	193181	PASS
68	69	0.00	2	1.5	3779	PASS
69	198	0.00	100	32.2	244634	PASS
70	69	0.00	2	0.4	1038	PASS
127	198	10	80	39.1	297621	PASS
197	198	0.00	2	0.3	2079	PASS
198	198	100	100	100.0	760427	PASS
199	198	5	9	6.9	52152	PASS
275	198	10	60	26.2	199595	PASS
365	198	1	100	3.2	24227	PASS
441	198	0.01	100	9.3	70976	PASS
442	442	50	100	100.0	454208	PASS
443	442	15	24	19.2	87264	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/22/2024	BNA_M	<u>BM047307.D</u>
Compound Name	Response	Retention Time
DDT	2599731	20.309
DDD	150494	19.868
DDE	4792	19.351
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
155286	2755017	5.64

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082224\
Data File : BM047307.D
Acq On : 22 Aug 2024 08:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 22 10:58:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

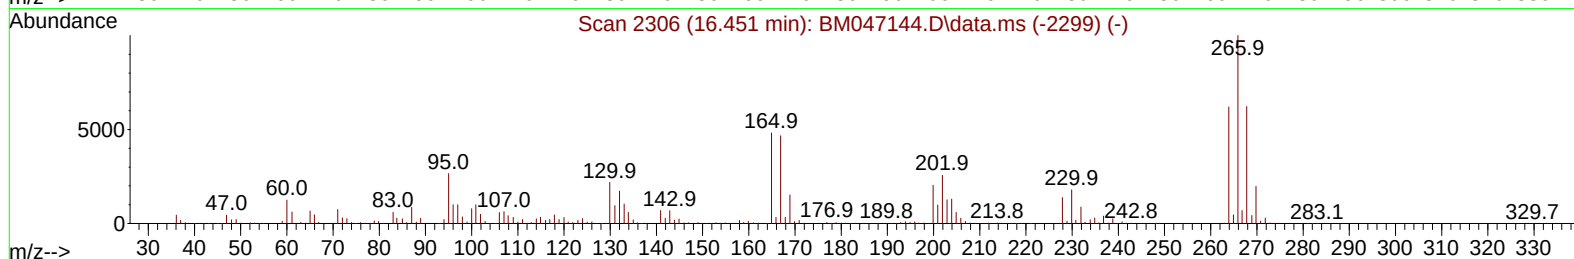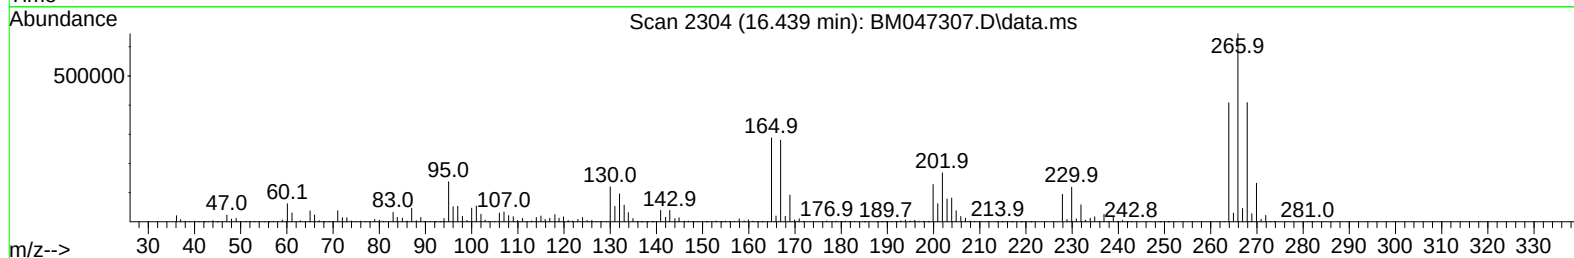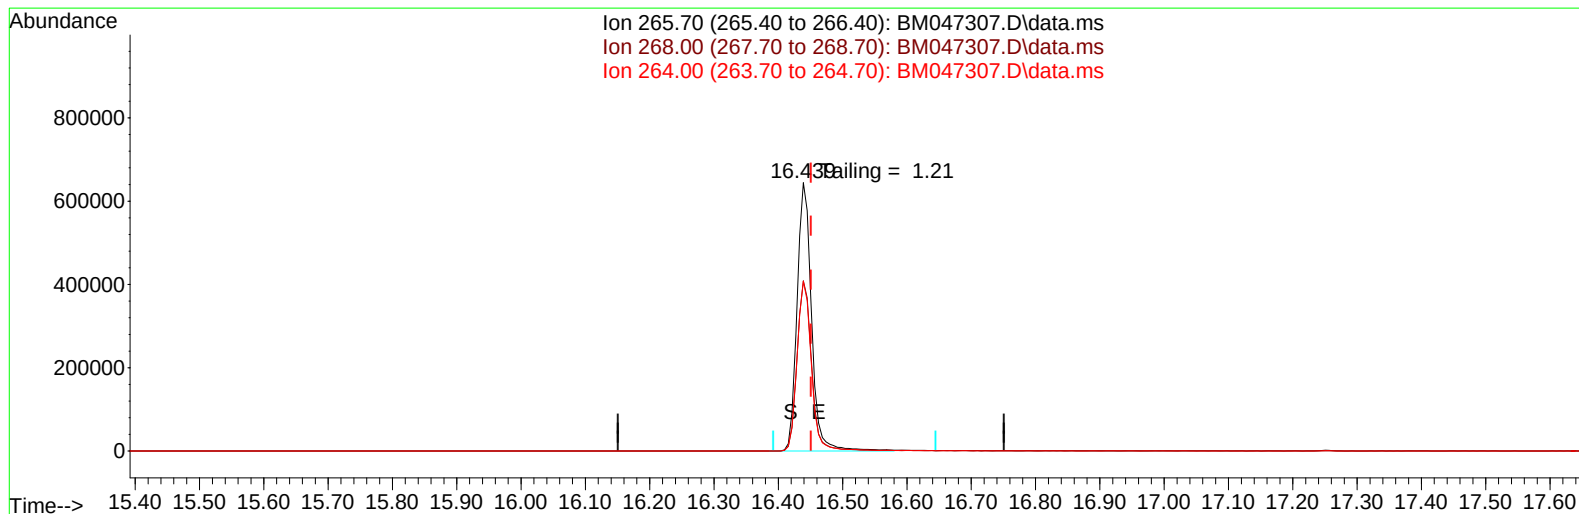

TIC: BM047307.D\data.ms

(70) Pentachlorophenol (C)

16.439min (-0.012) 305697.00 ng




response 1016426

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.44
264.00	62.00	63.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082224\
Data File : BM047307.D
Acq On : 22 Aug 2024 08:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 22 10:58:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

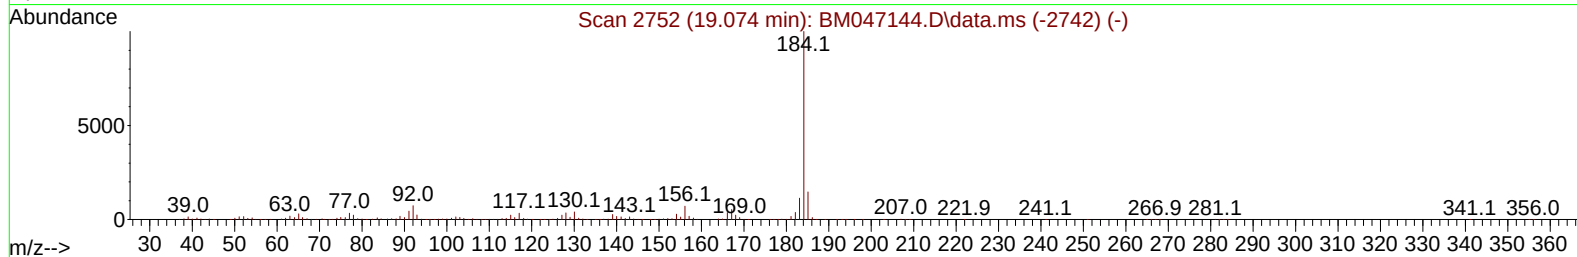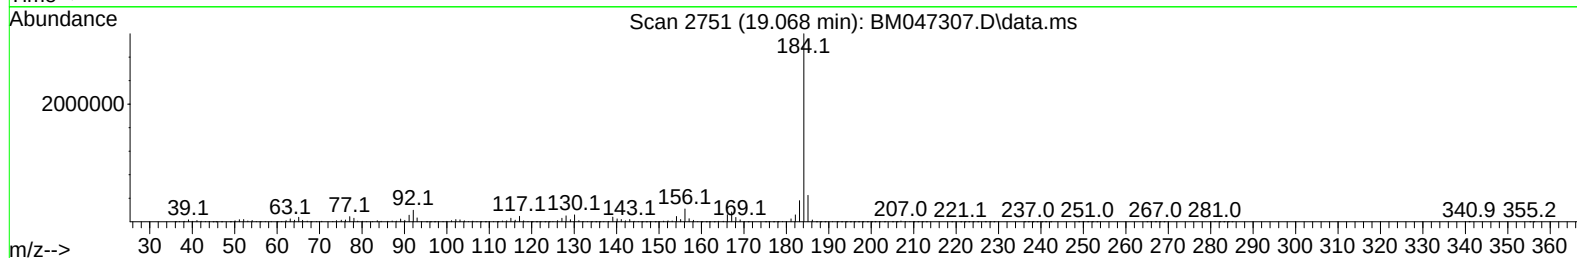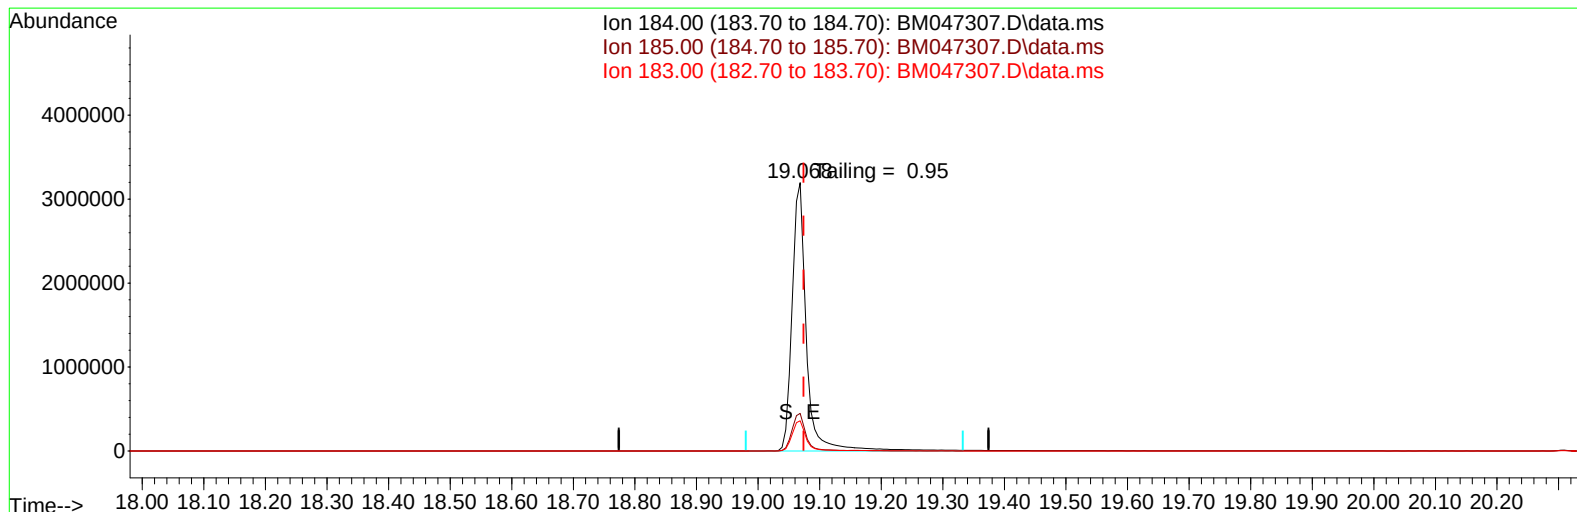

TIC: BM047307.D\data.ms

(77) Benzidine

19.068min (-0.006) 142115.28 ng

response 5191261

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.05
183.00	11.30	11.27
0.00	0.00	0.00