
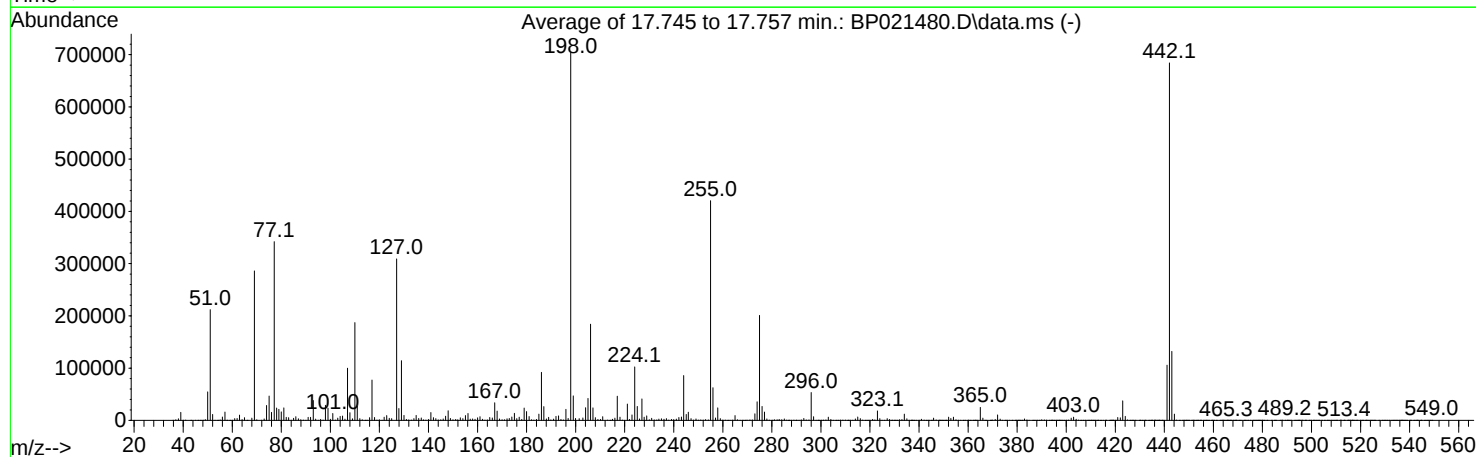


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081324\
Data File : BP021480.D
Acq On : 13 Aug 2024 11:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 14 00:00:30 2024

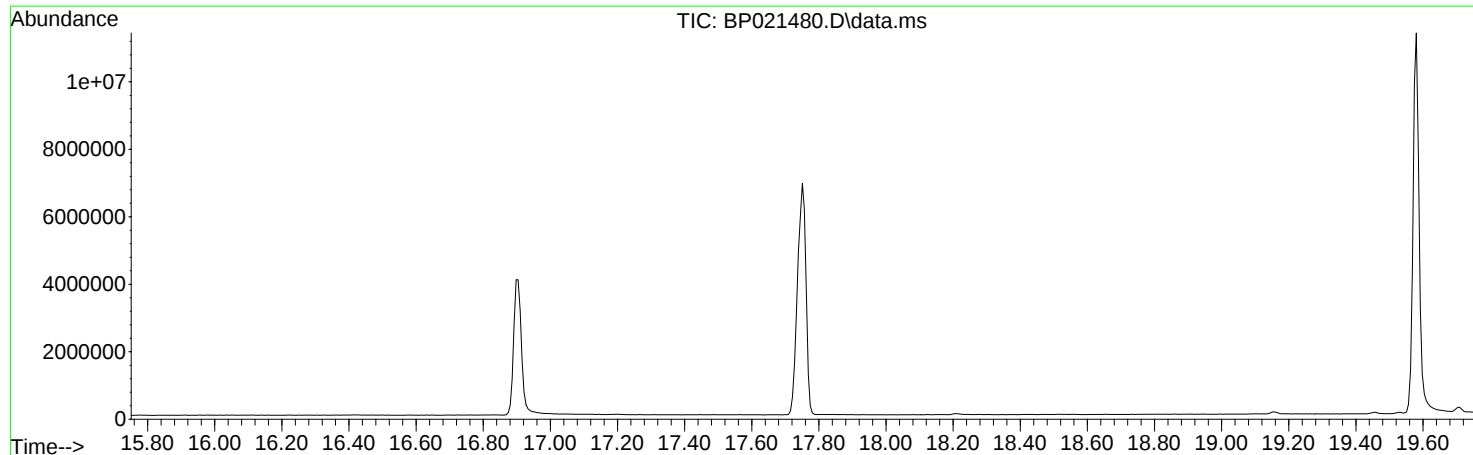




AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.1	212028	PASS
68	69	0.00	2	1.5	4256	PASS
69	198	0.00	100	40.6	286100	PASS
70	69	0.00	2	0.4	1197	PASS
127	198	10	80	43.9	309160	PASS
197	198	0.00	2	0.5	3666	PASS
198	198	100	100	100.0	704123	PASS
199	198	5	9	6.6	46731	PASS
275	198	10	60	28.5	200892	PASS
365	198	1	100	3.5	24968	PASS
441	198	0.01	100	15.0	105600	PASS
442	442	100	100	100.0	684335	PASS
443	442	15	24	19.3	131982	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081324\
Data File : BP021480.D
Acq On : 13 Aug 2024 11:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 14 00:14:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 00:00:30 2024
Response via : Initial Calibration

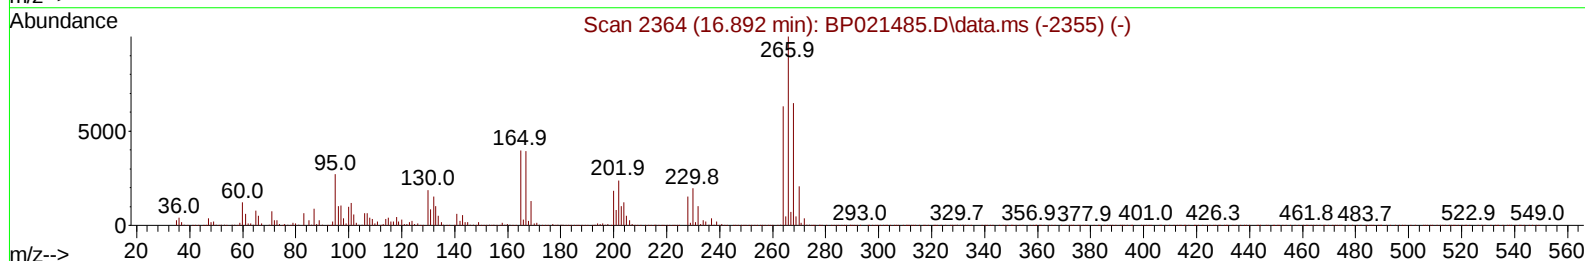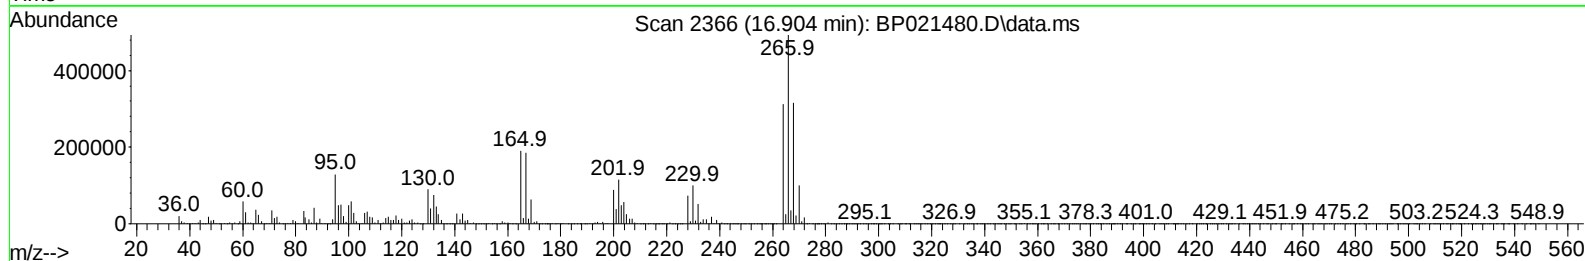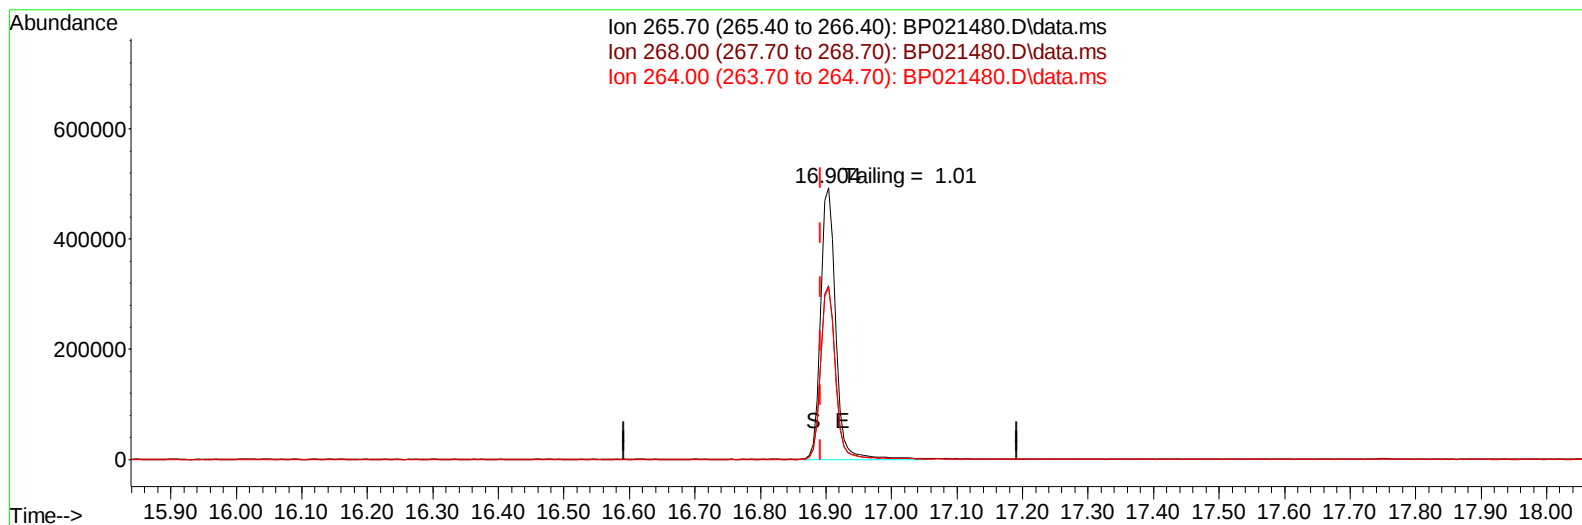

TIC: BP021480.D\data.ms

(70) Pentachlorophenol (C)

16.904min (+ 0.012) 6855729.98 ng




response 795611

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	64.10
264.00	63.10	63.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081324\
Data File : BP021480.D
Acq On : 13 Aug 2024 11:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 14 00:14:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 00:00:30 2024
Response via : Initial Calibration

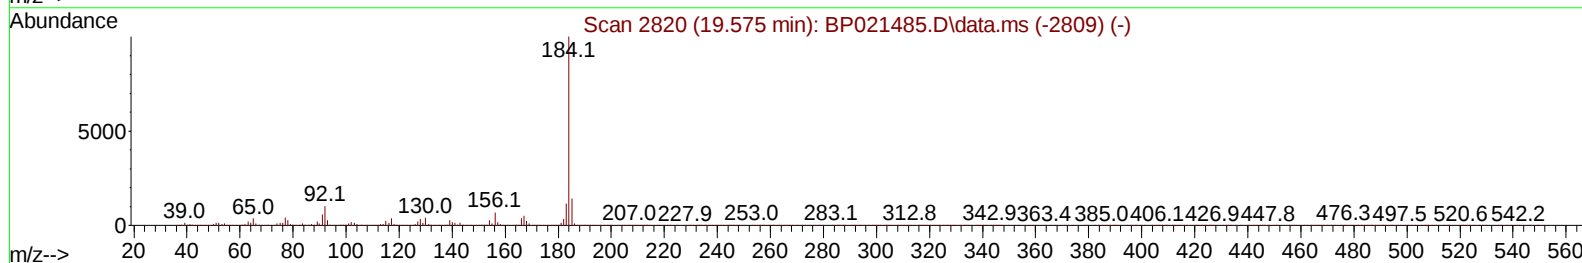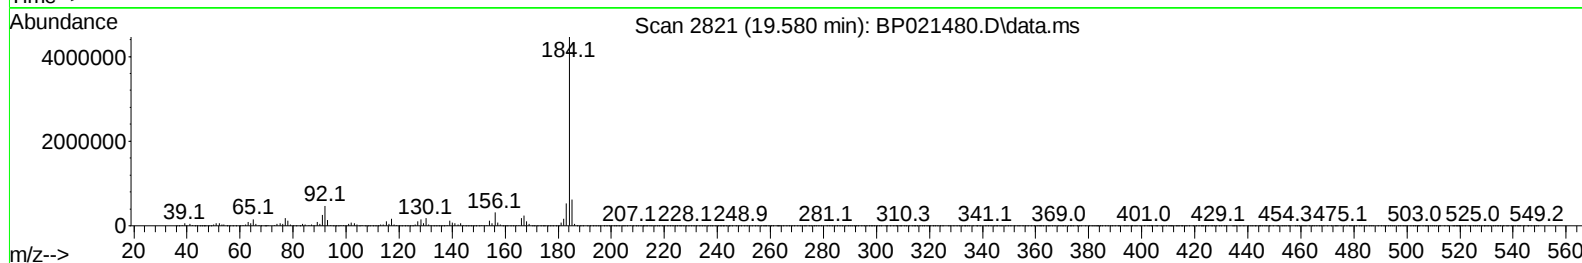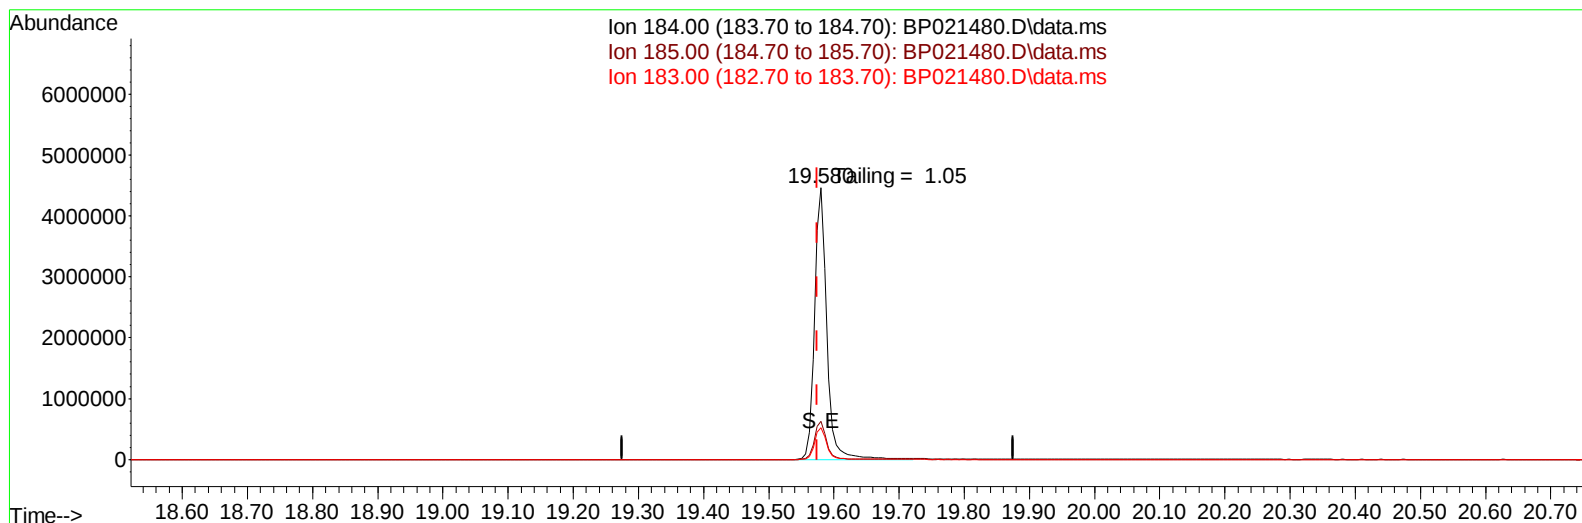

TIC: BP021480.D\data.ms

(77) Benzidine

19.580min (+ 0.005) -20.00 ng

response 5830874

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.05
183.00	11.60	11.75
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/13/2024	BNA_P	<u>BP021480.D</u>
Compound Name	Response	Retention Time
DDT	2081689	20.88
DDD	17224	20.486
DDE	158	19.962
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17382	2099071	0.83

Instrument :
BNA_P
ClientSampleId :
DFTPP