
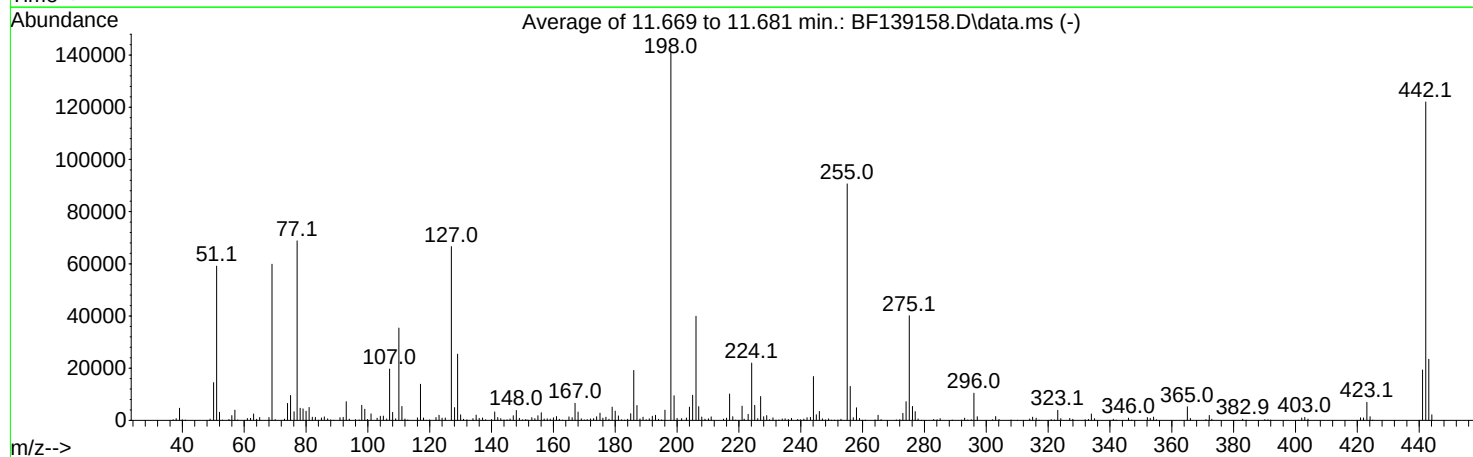


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF082624\  
Data File : BF139158.D  
Acq On : 26 Aug 2024 09:14  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF082024.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed Aug 21 01:25:05 2024

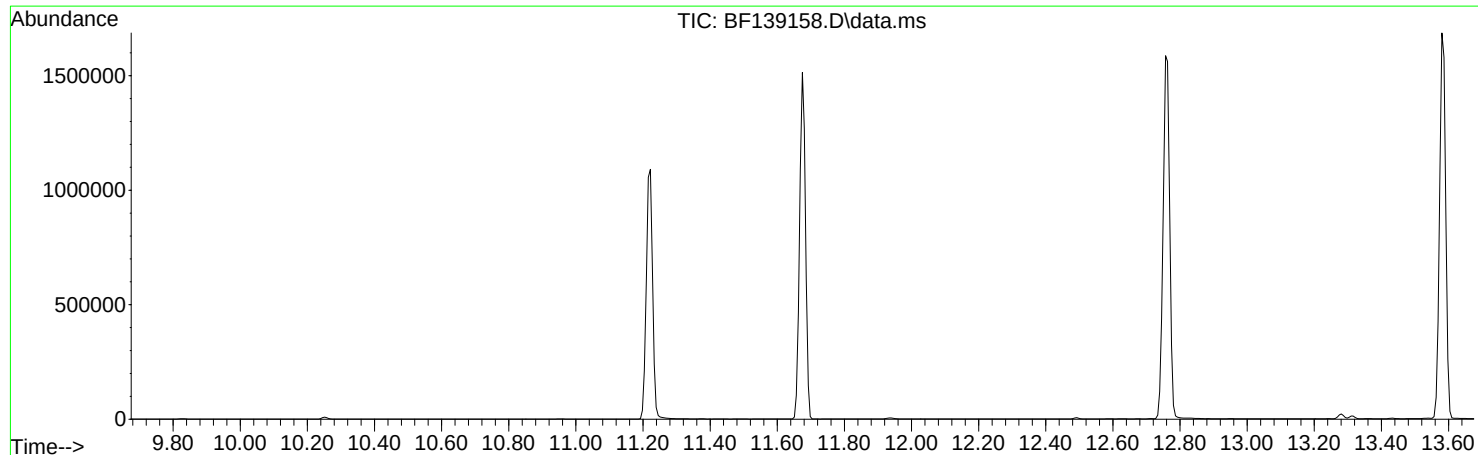

AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1622

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 41.9         | 59120      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.8          | 1099       | PASS                |
| 69             | 198             | 0.00            | 100             | 42.5         | 59883      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 302        | PASS                |
| 127            | 198             | 10              | 80              | 47.3         | 66616      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 140984     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 9430       | PASS                |
| 275            | 198             | 10              | 60              | 28.5         | 40117      | PASS                |
| 365            | 198             | 1               | 100             | 3.7          | 5187       | PASS                |
| 441            | 198             | 0.01            | 100             | 13.7         | 19312      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 122029     | PASS                |
| 443            | 442             | 15              | 24              | 19.2         | 23441      | PASS                |

### DDT Breakdown


| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 8/26/2024     | BNA_F            | <u>BF139158.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 410710           | 13.58              |
| DDD           | 9712             | 13.28              |
| DDE           | 439              | 12.945             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 10151         | 420861           | 2.41               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF082624\  
Data File : BF139158.D  
Acq On : 26 Aug 2024 09:14  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Aug 26 10:54:29 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF082024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 21 01:25:05 2024  
Response via : Initial Calibration

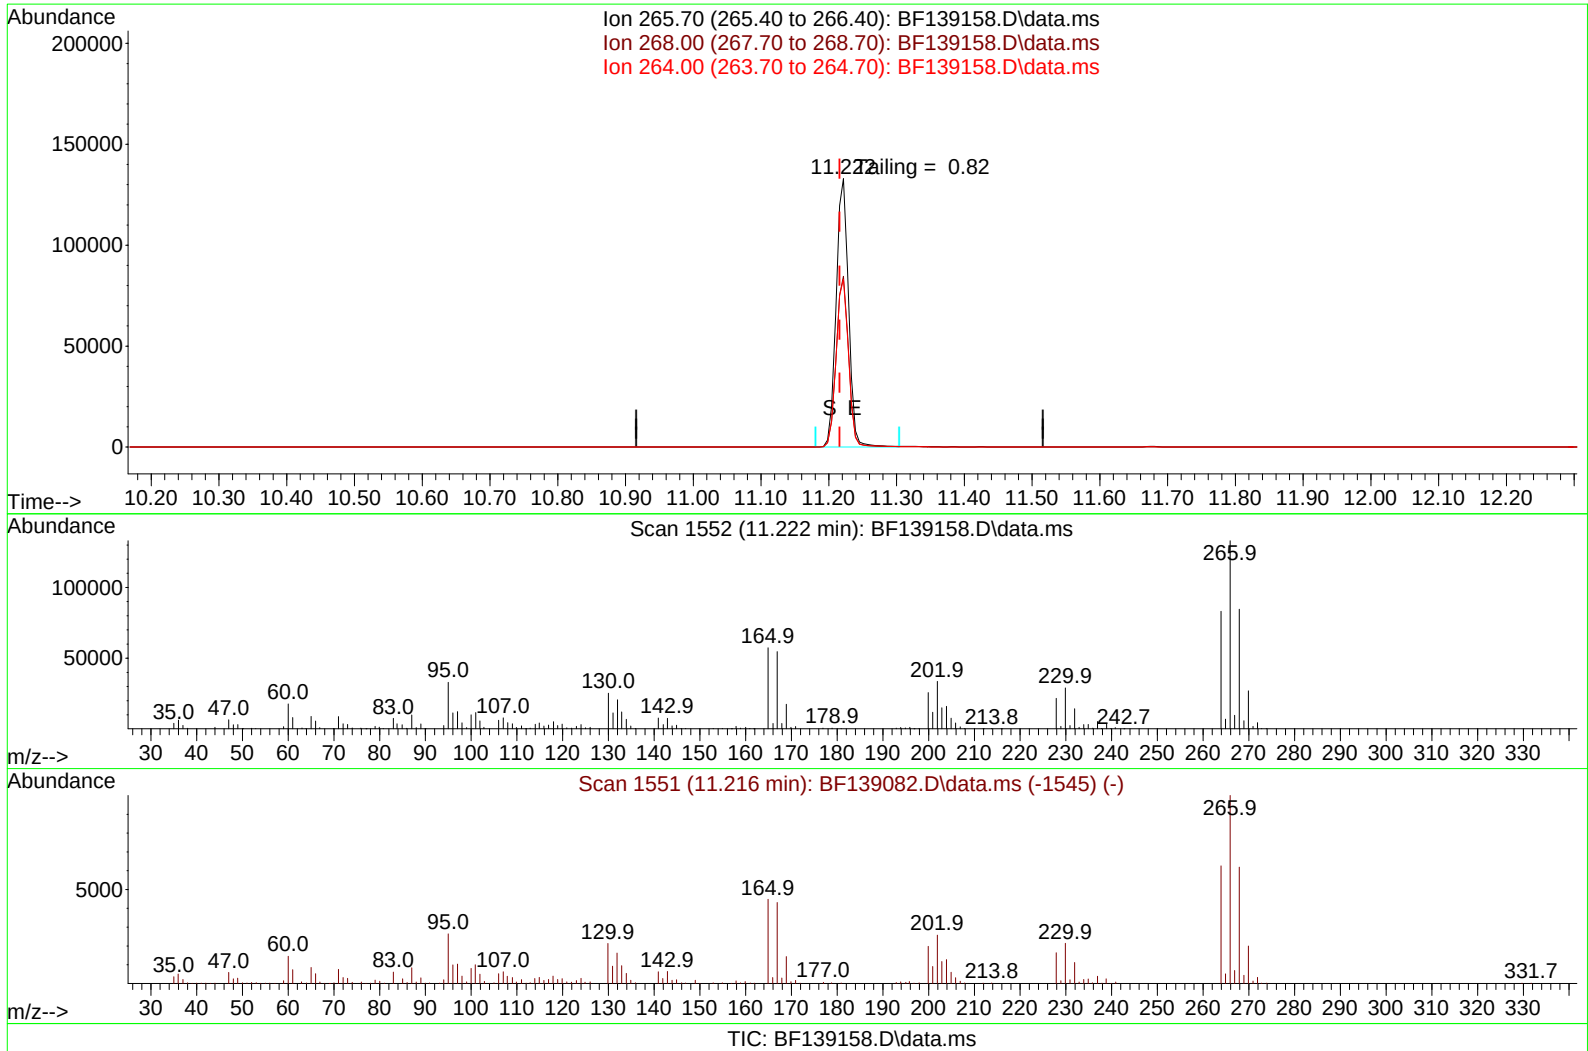

(70) Pentachlorophenol (C)

11.222min (+ 0.006) 29659.75 ng




response 170150

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.90  | 63.61  |
| 264.00 | 62.50  | 62.54  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF082624\  
Data File : BF139158.D  
Acq On : 26 Aug 2024 09:14  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Aug 26 10:54:29 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF082024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 21 01:25:05 2024  
Response via : Initial Calibration

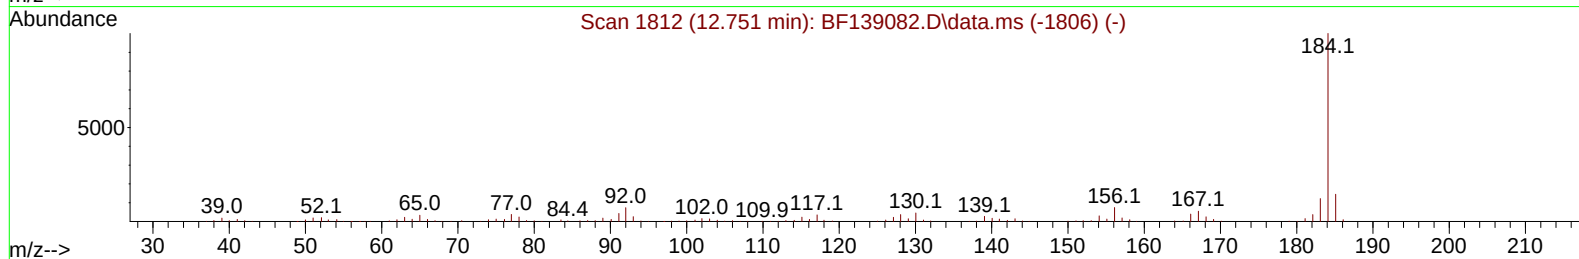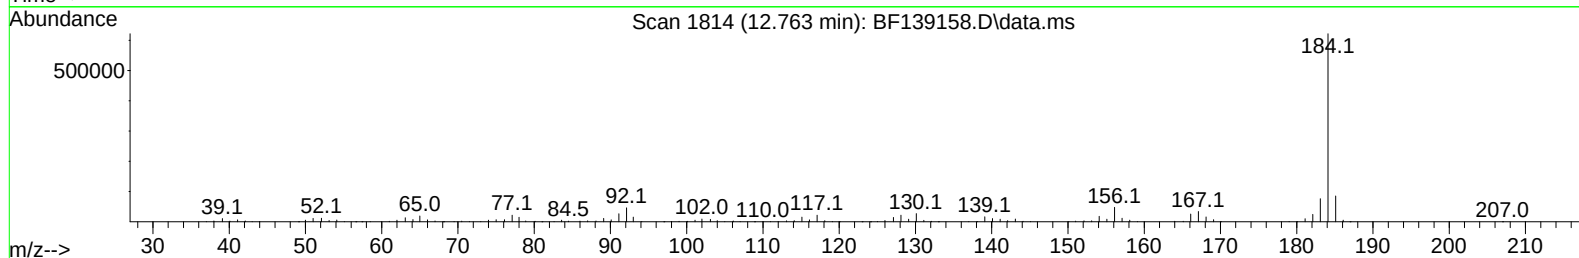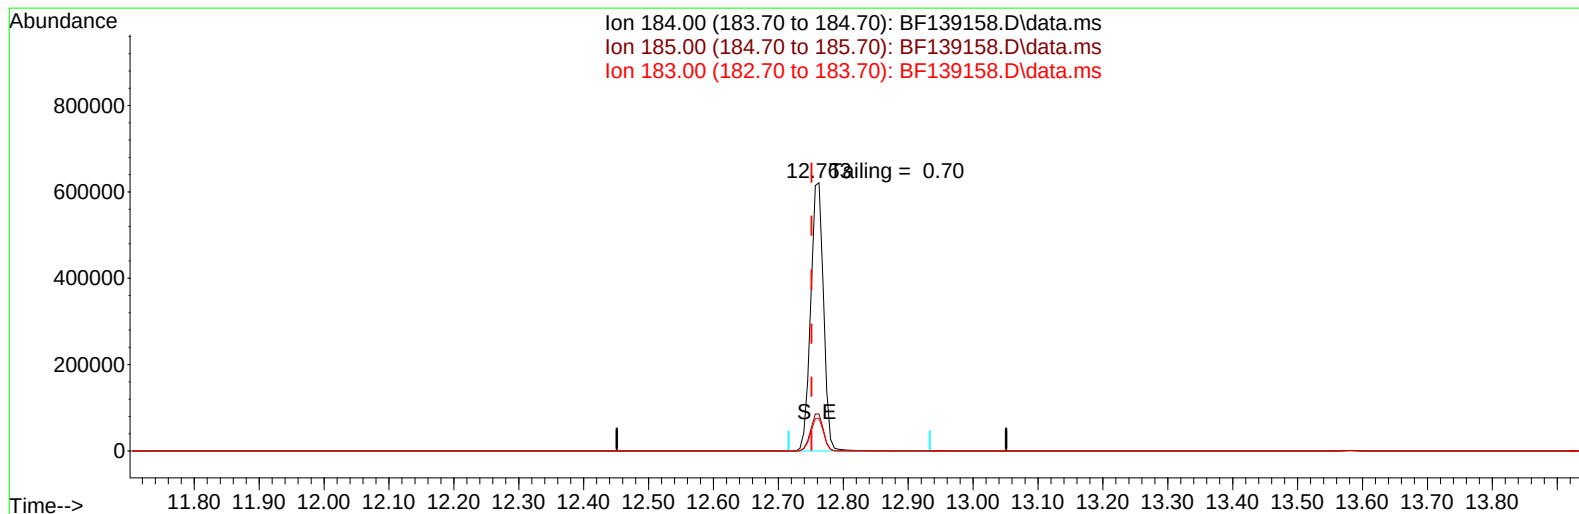

TIC: BF139158.D\data.ms

(77) Benzidine

12.763min (+ 0.012) 0.00 ng

response 856955

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.40  | 13.76  |
| 183.00 | 12.20  | 12.26  |
| 0.00   | 0.00   | 0.00   |