
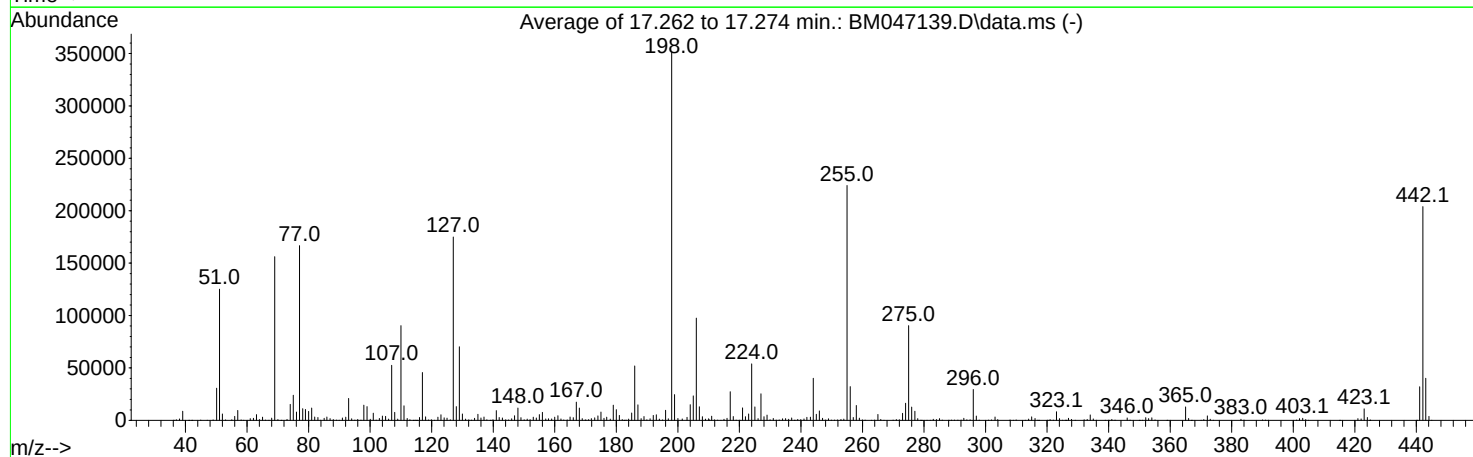


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081024\
Data File : BM047139.D
Acq On : 10 Aug 2024 12:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun Aug 11 23:47:58 2024

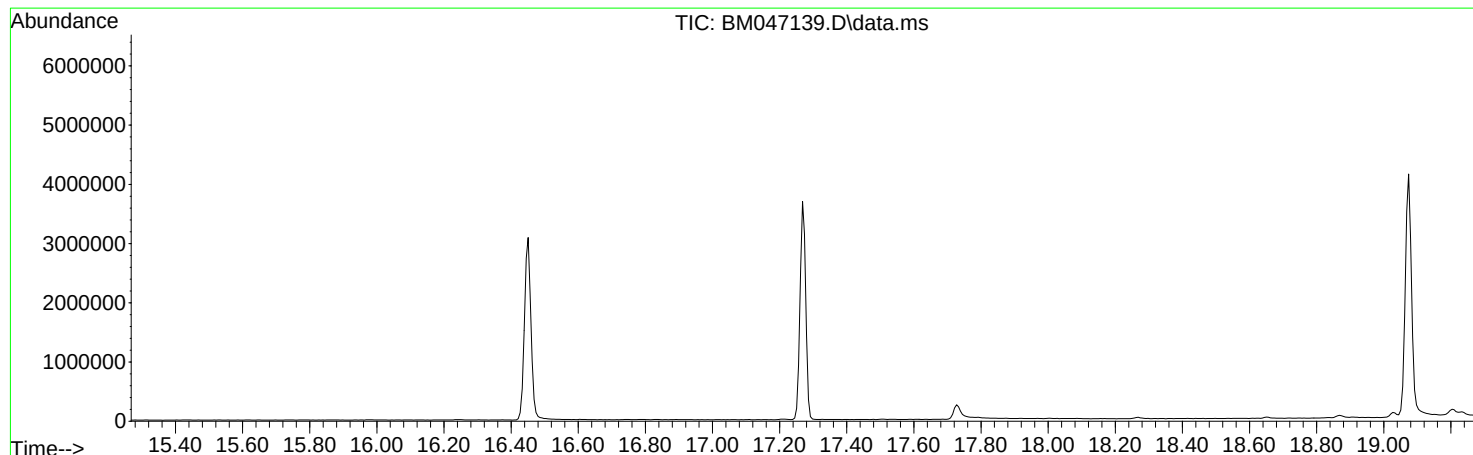

AutoFind: Scans 2444, 2445, 2446; Background Corrected with Scan 2437

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	125256	PASS
68	69	0.00	2	1.3	2089	PASS
69	198	0.00	100	44.5	156224	PASS
70	69	0.00	2	0.5	803	PASS
127	198	10	80	49.9	174976	PASS
197	198	0.00	2	0.4	1460	PASS
198	198	100	100	100.0	350933	PASS
199	198	5	9	7.0	24517	PASS
275	198	10	60	25.8	90373	PASS
365	198	1	100	3.6	12789	PASS
441	198	0.01	100	9.2	32133	PASS
442	442	50	100	100.0	203891	PASS
443	442	15	24	19.7	40160	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/10/2024	BNA_M	<u>BM047139.D</u>
Compound Name	Response	Retention Time
DDT	1324125	20.321
DDD	17903	19.927
DDE	740	19.362
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18643	1342768	1.39

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081024\
Data File : BM047139.D
Acq On : 10 Aug 2024 12:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 12 01:52:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

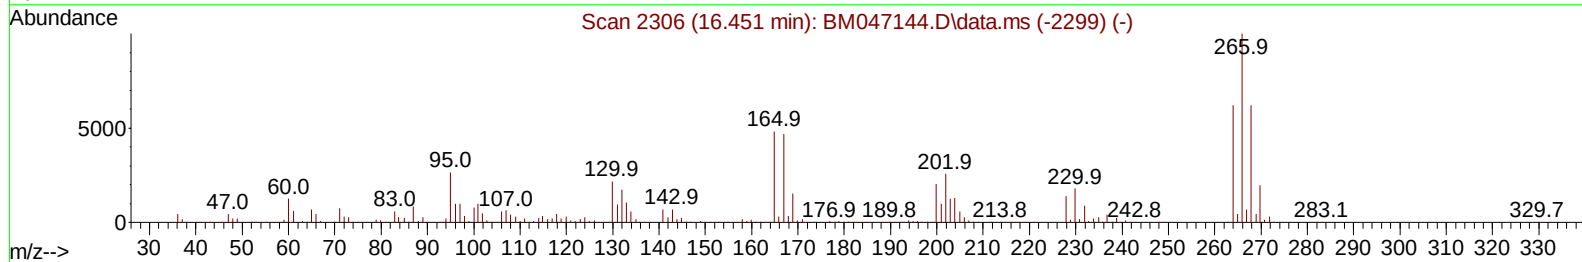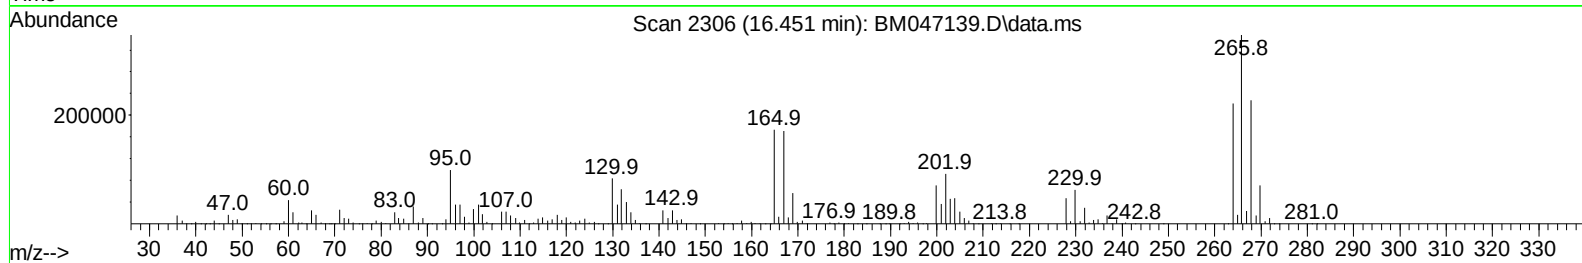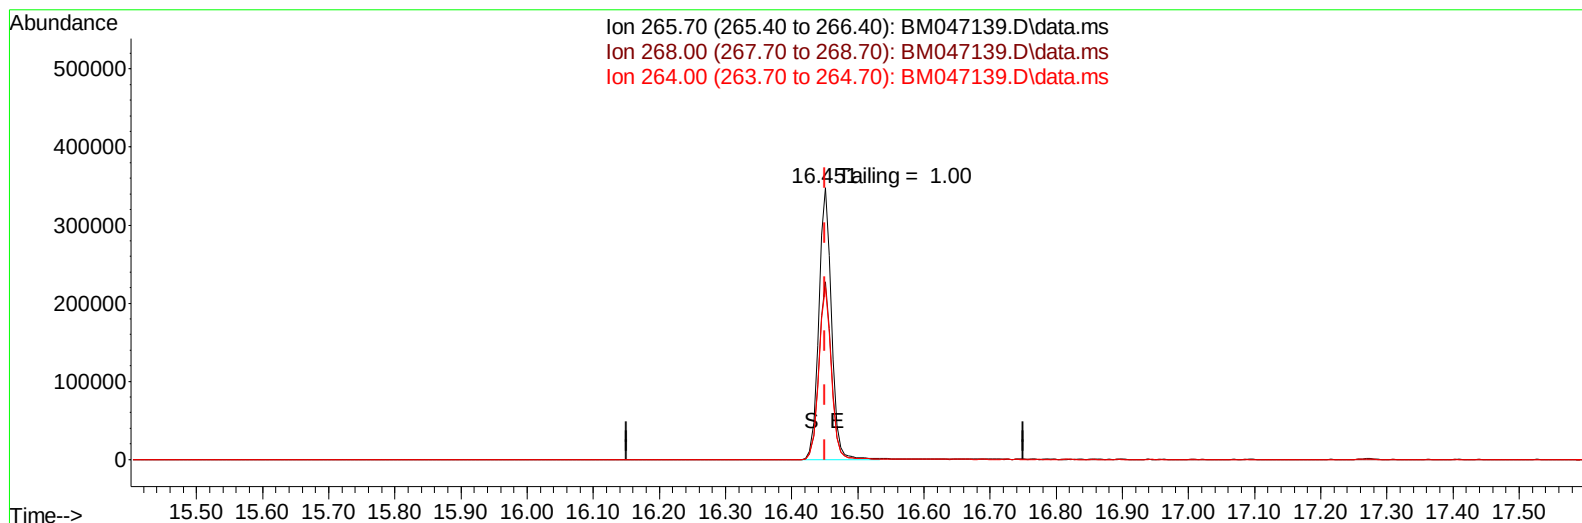

TIC: BM047139.D\data.ms

(70) Pentachlorophenol (C)

16.451min (-0.000) 14982.60 ng




response 465922

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.50
264.00	62.00	63.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081024\
Data File : BM047139.D
Acq On : 10 Aug 2024 12:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 12 01:52:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

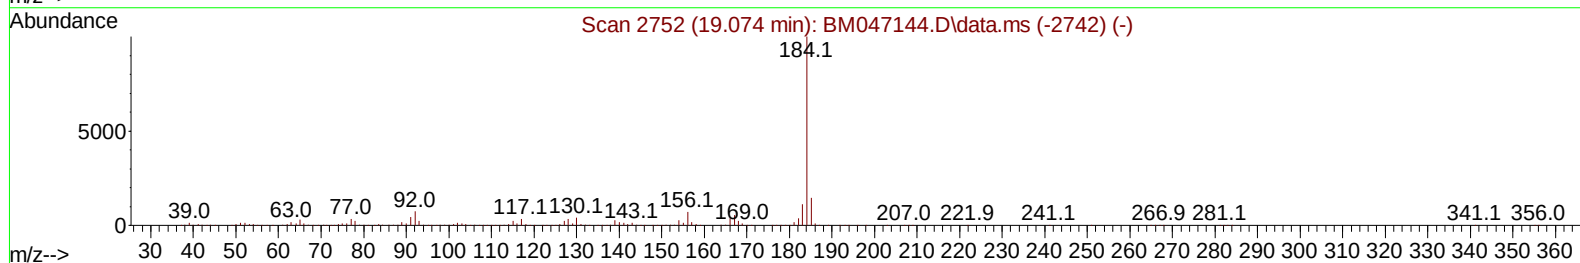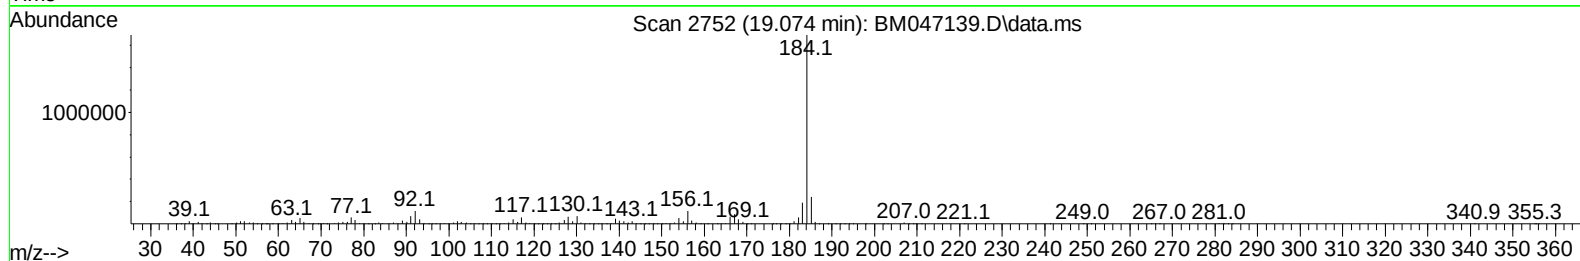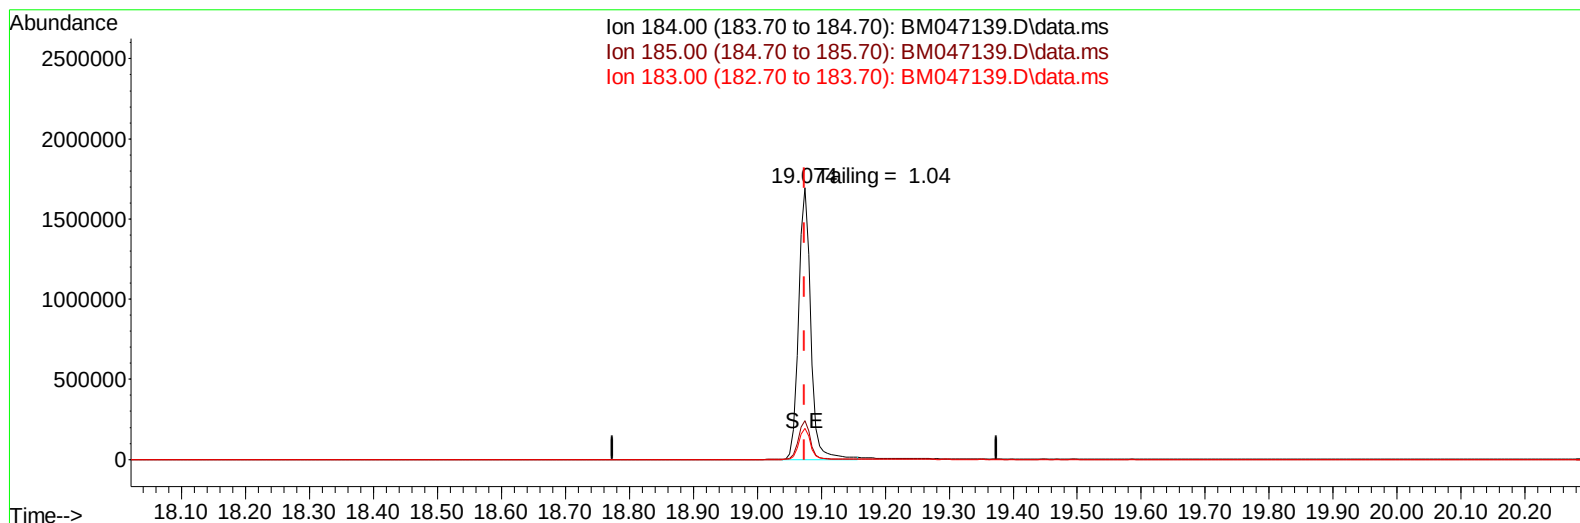

TIC: BM047139.D\data.ms

(77) Benzidine

19.074min (-0.000) 6495.62 ng

response 2296747

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.34
183.00	11.30	11.36
0.00	0.00	0.00