
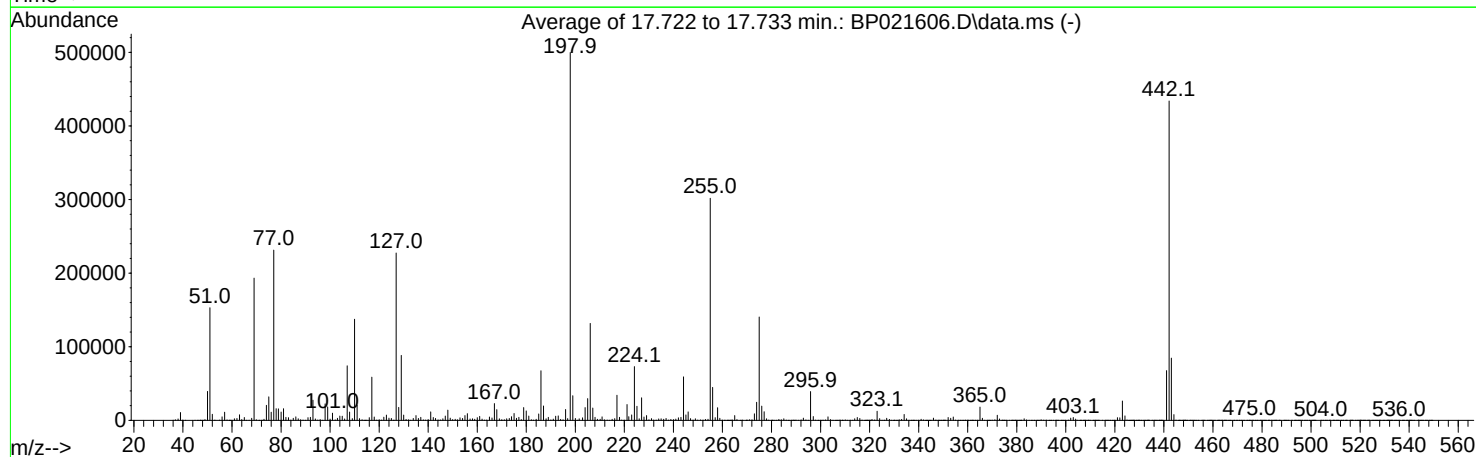


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082224\
Data File : BP021606.D
Acq On : 22 Aug 2024 08:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 22 11:12:31 2024

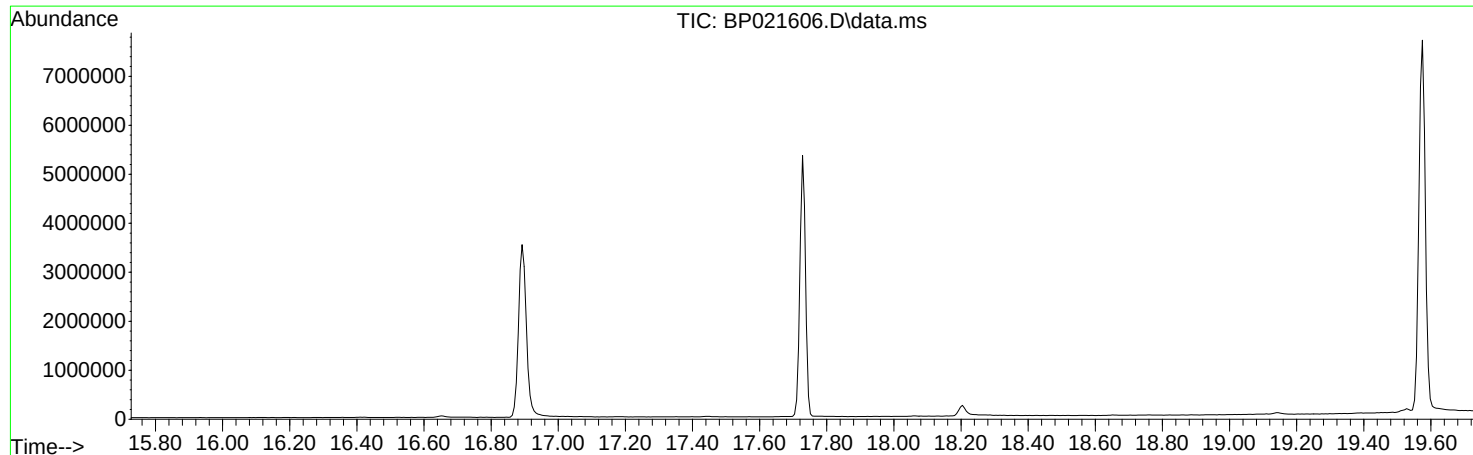

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2496

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	152975	PASS
68	69	0.00	2	1.4	2772	PASS
69	198	0.00	100	38.7	193286	PASS
70	69	0.00	2	0.5	912	PASS
127	198	10	80	45.5	227361	PASS
197	198	0.00	2	0.5	2487	PASS
198	198	100	100	100.0	499840	PASS
199	198	5	9	6.7	33470	PASS
275	198	10	60	28.1	140549	PASS
365	198	1	100	3.6	17954	PASS
441	198	0.01	100	13.5	67555	PASS
442	442	100	100	100.0	434035	PASS
443	442	15	24	19.5	84674	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/22/2024	BNA_P	<u>BP021606.D</u>
Compound Name	Response	Retention Time
DDT	1848167	20.88
DDD	72708	20.416
DDE	3986	19.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
76694	1924861	3.98

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082224\
Data File : BP021606.D
Acq On : 22 Aug 2024 08:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 23 01:29:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 11:12:31 2024
Response via : Initial Calibration

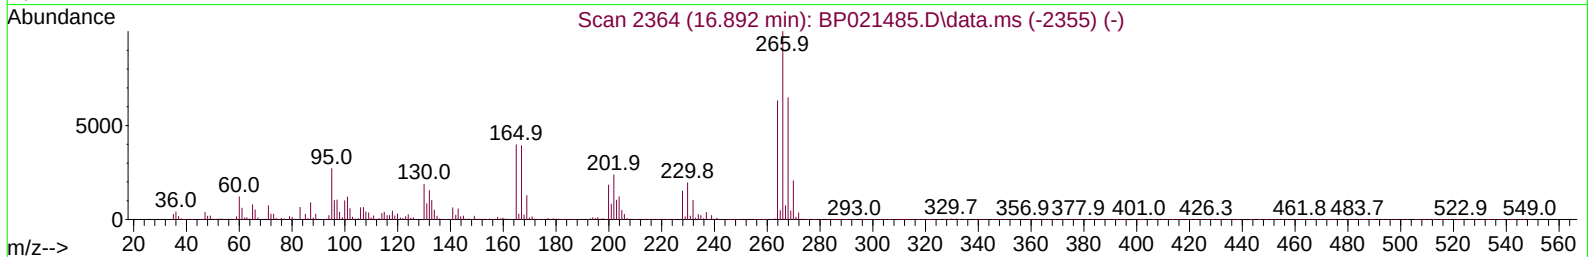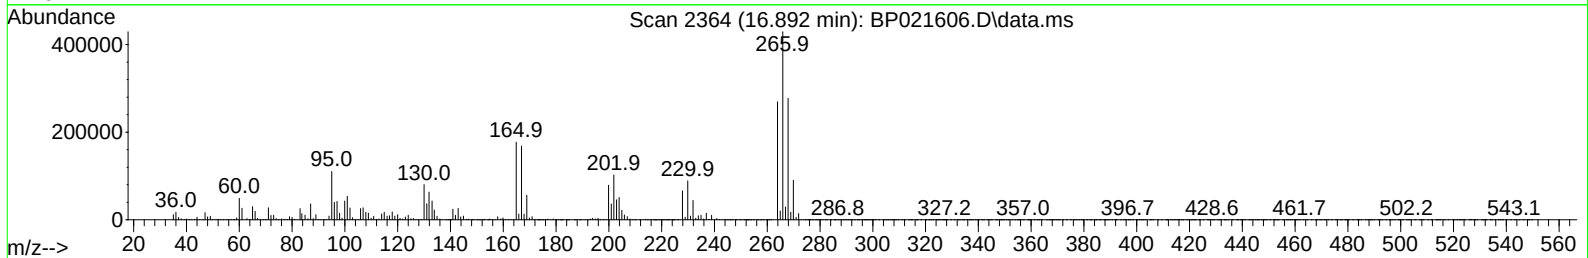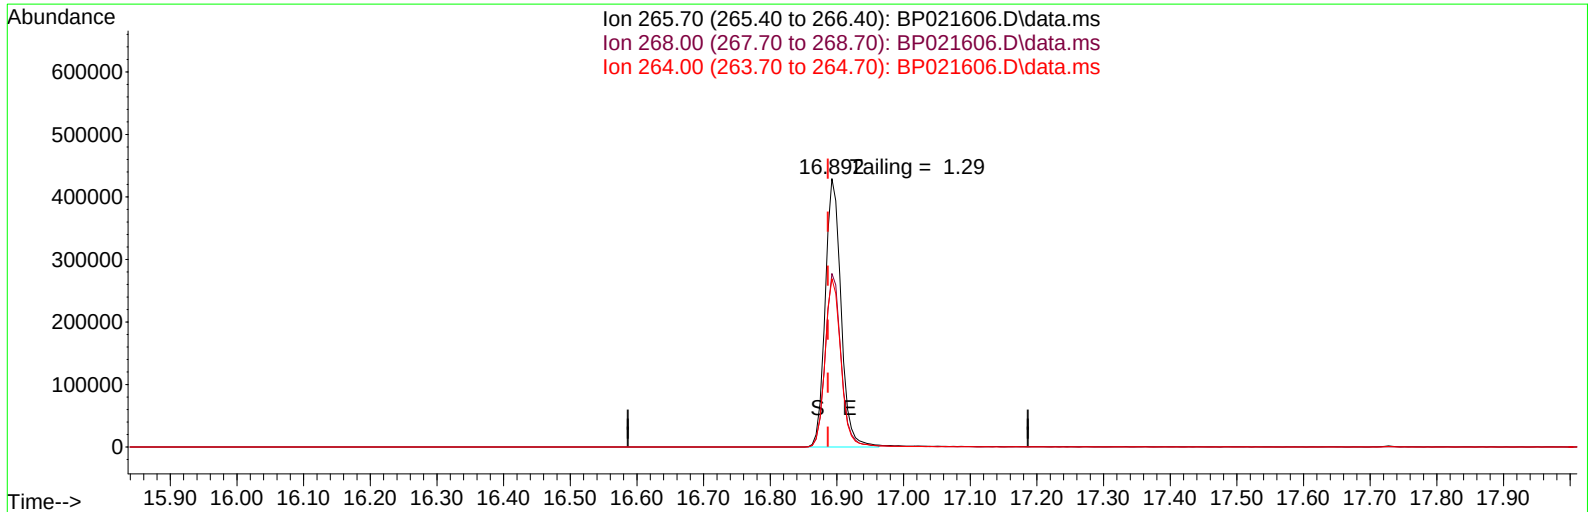

TIC: BP021606.D\data.ms

(70) Pentachlorophenol (C)

16.892min (+ 0.006) 219133.64 ng




response 712056

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	64.61
264.00	63.10	62.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082224\
Data File : BP021606.D
Acq On : 22 Aug 2024 08:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 23 01:29:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 11:12:31 2024
Response via : Initial Calibration

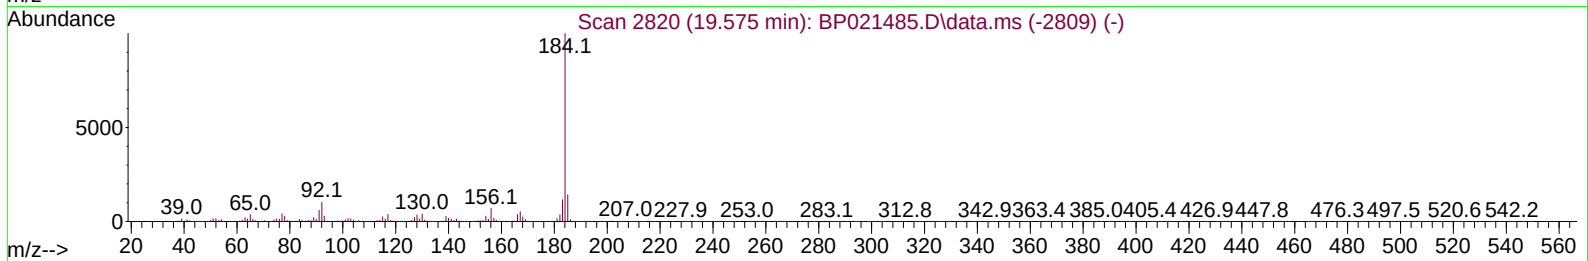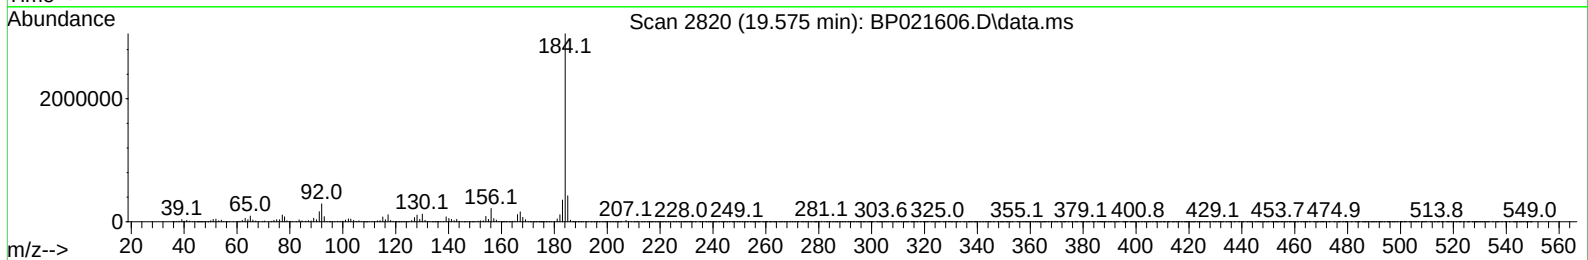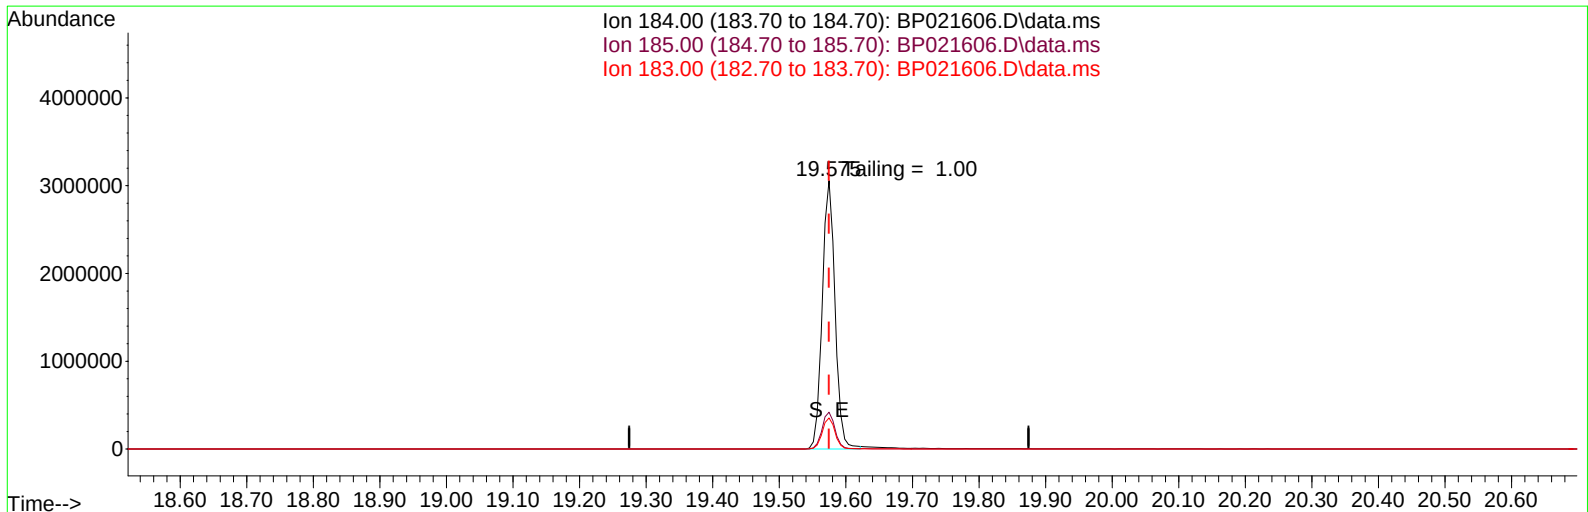

TIC: BP021606.D\data.ms

(77) Benzidine

19.575min (-0.000) -20.00 ng

response 4143250

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.76
183.00	11.60	11.60
0.00	0.00	0.00