
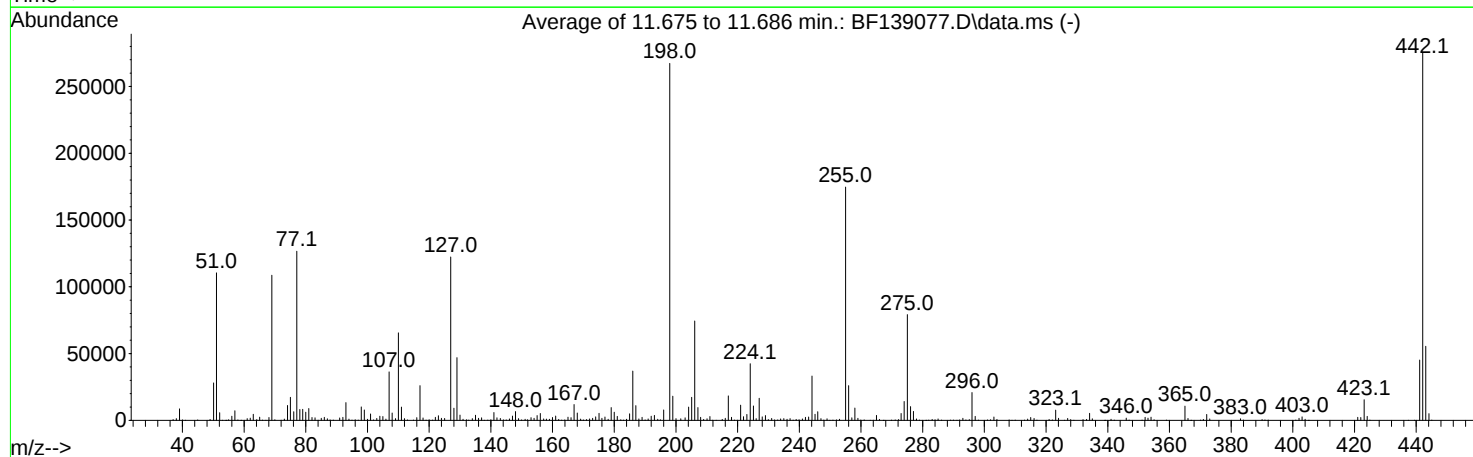


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082024\
Data File : BF139077.D
Acq On : 20 Aug 2024 16:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 21 01:25:05 2024

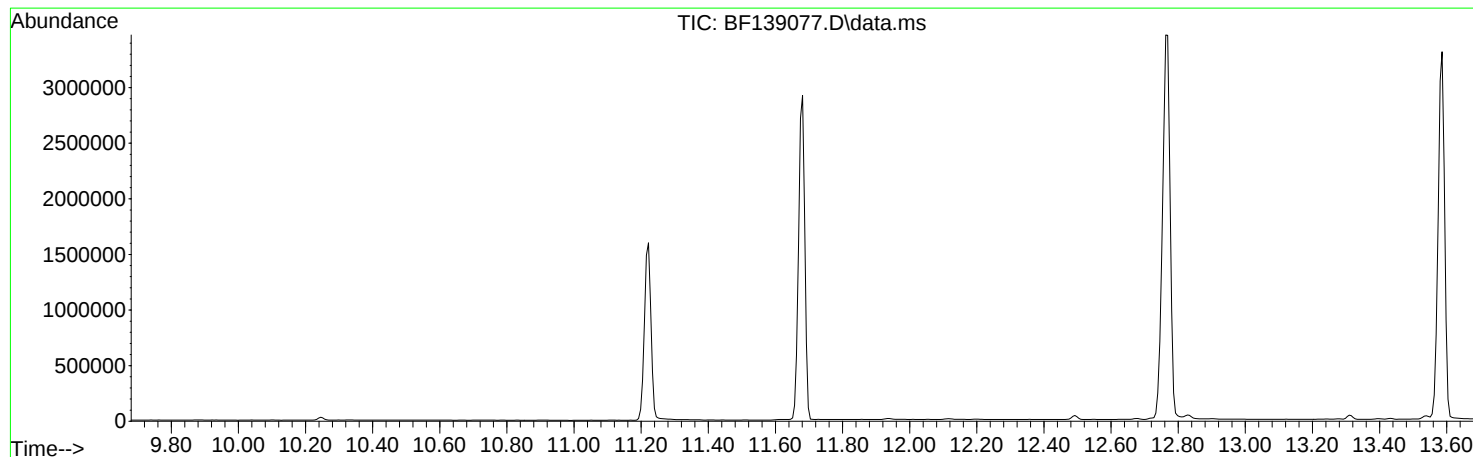




AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.3	110429	PASS
68	69	0.00	2	2.0	2125	PASS
69	198	0.00	100	40.7	108717	PASS
70	69	0.00	2	0.4	479	PASS
127	198	10	80	45.8	122331	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	267328	PASS
199	198	5	9	6.8	18110	PASS
275	198	10	60	29.6	79200	PASS
365	198	1	100	4.0	10643	PASS
441	198	0.01	100	16.9	45136	PASS
442	442	50	100	100.0	275456	PASS
443	442	15	24	20.2	55515	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082024\
Data File : BF139077.D
Acq On : 20 Aug 2024 16:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 21 01:32:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 01:25:05 2024
Response via : Initial Calibration

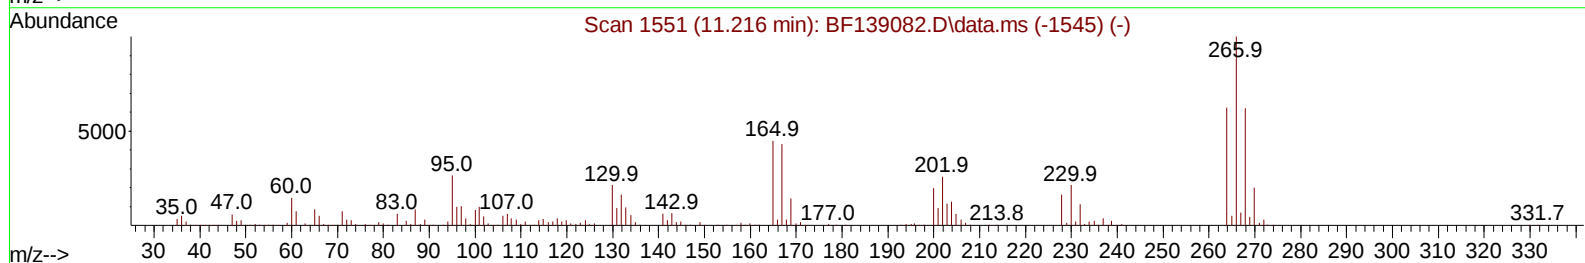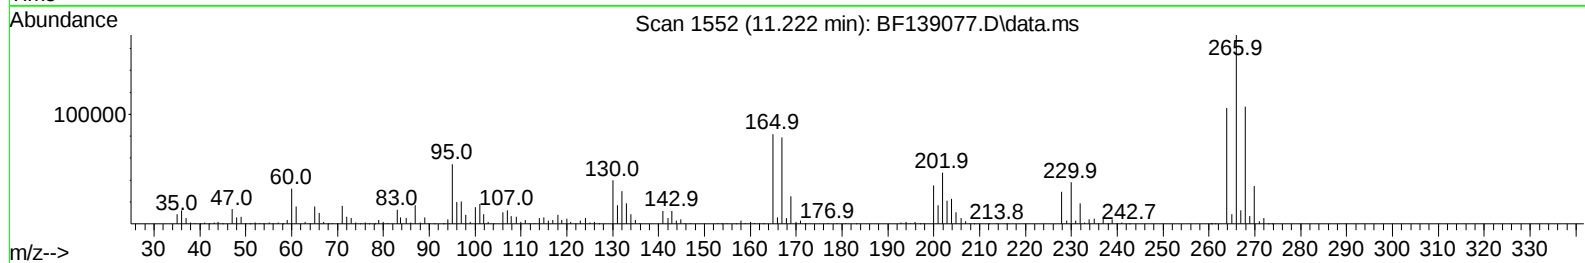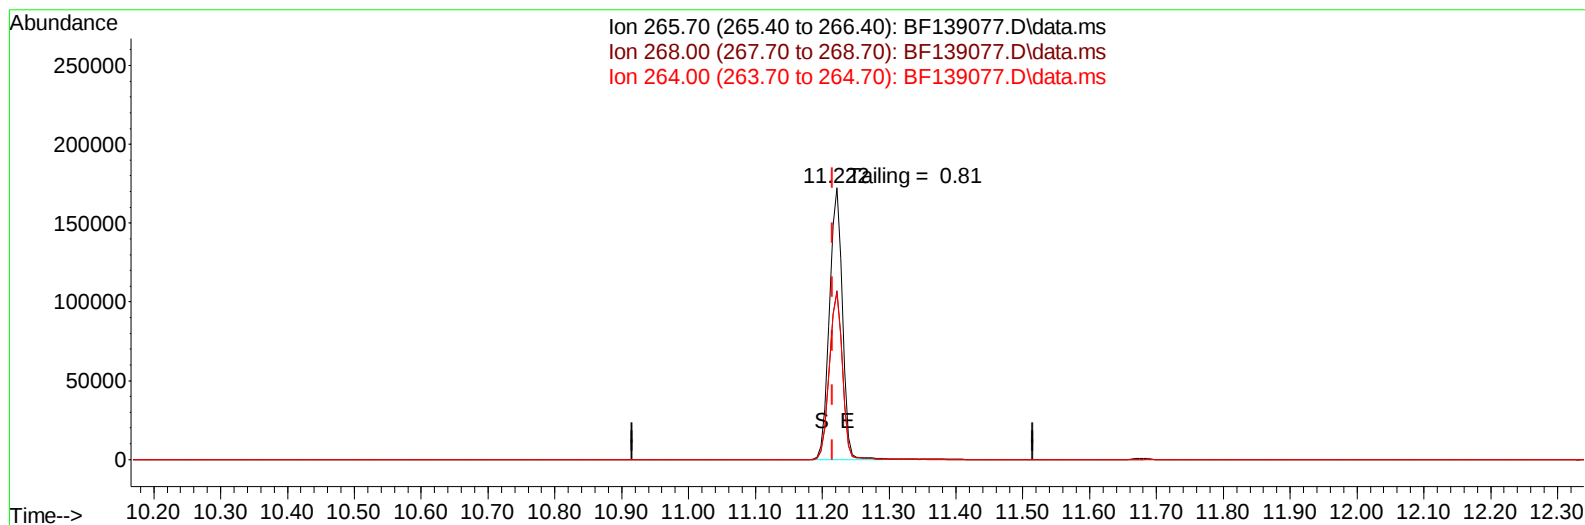

TIC: BF139077.D\data.ms

(70) Pentachlorophenol (C)

11.222min (+ 0.006) 19410.97 ng




response 232437

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	62.12
264.00	62.50	61.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082024\
Data File : BF139077.D
Acq On : 20 Aug 2024 16:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 21 01:32:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 01:25:05 2024
Response via : Initial Calibration

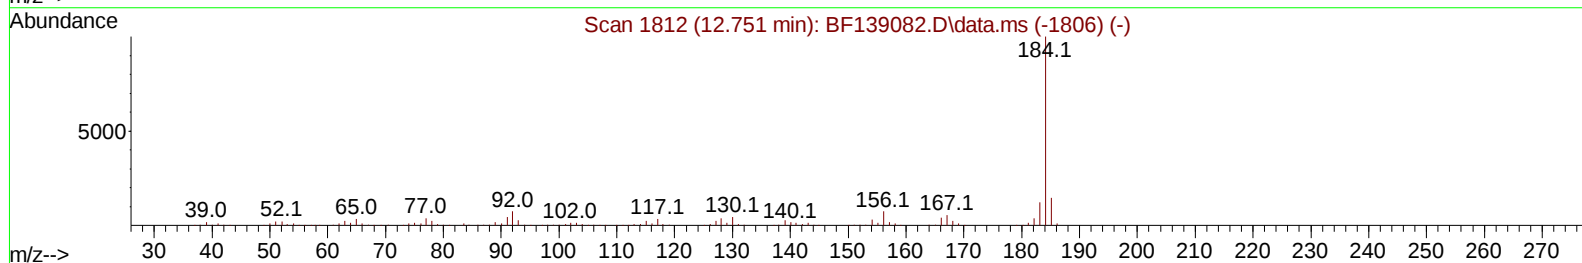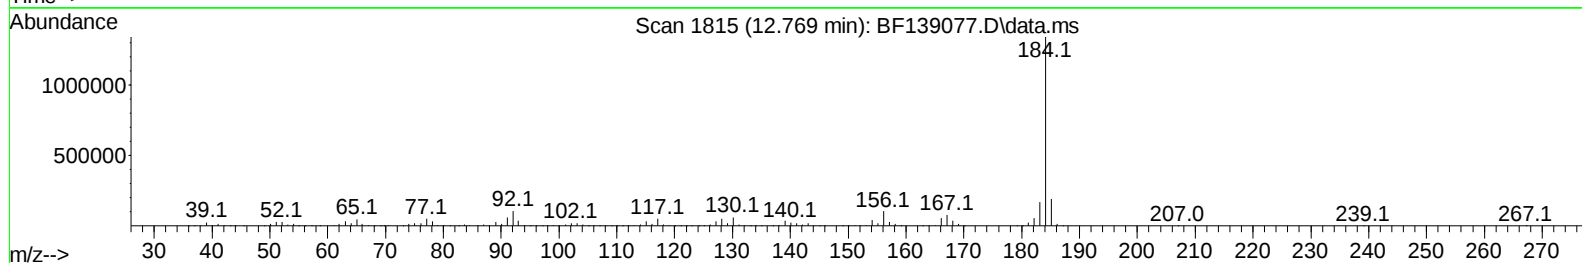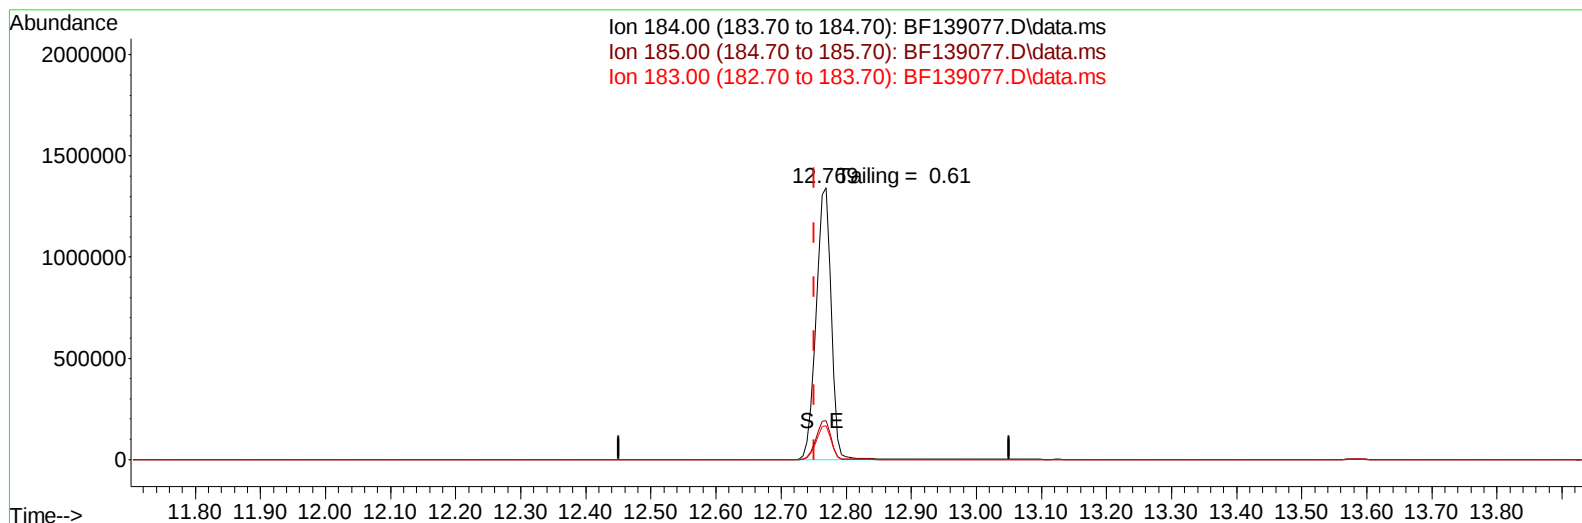

TIC: BF139077.D\data.ms

(77) Benzidine

12.769min (+ 0.018) 0.00 ng

response 2156347

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.24
183.00	12.20	12.45
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/20/2024	BNA_F	<u>BF139077.D</u>
Compound Name	Response	Retention Time
DDT	770140	13.586
DDD	8377	13.231
DDE	0	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8377	778517	1.08

Instrument :
BNA_F
ClientSampleId :
DFTPP