
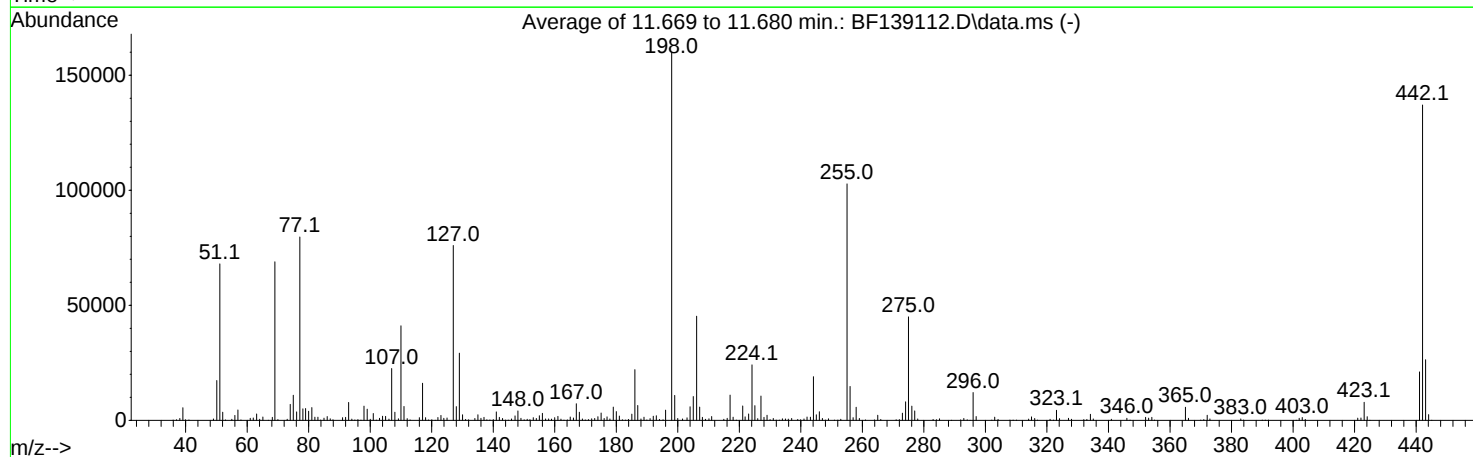


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082224\
Data File : BF139112.D
Acq On : 22 Aug 2024 09:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 21 01:25:05 2024

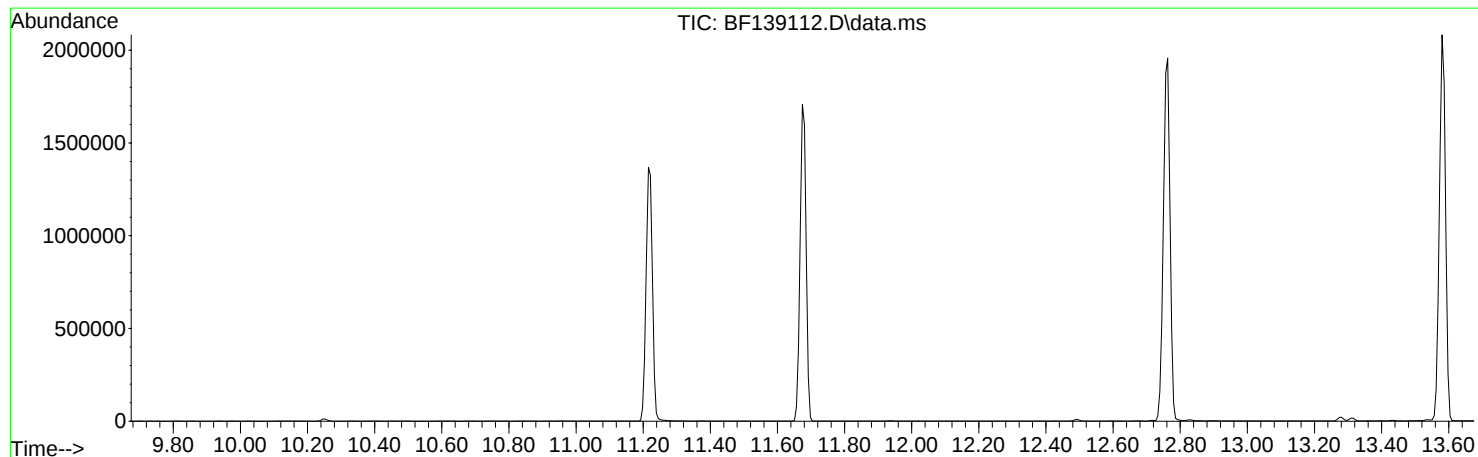

AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	68035	PASS
68	69	0.00	2	1.9	1326	PASS
69	198	0.00	100	43.1	68907	PASS
70	69	0.00	2	0.6	386	PASS
127	198	10	80	47.5	76008	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	159885	PASS
199	198	5	9	6.8	10861	PASS
275	198	10	60	28.1	44981	PASS
365	198	1	100	3.6	5740	PASS
441	198	0.01	100	13.2	21071	PASS
442	442	50	100	100.0	137080	PASS
443	442	15	24	19.3	26390	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/22/2024	BNA_F	<u>BF139112.D</u>
Compound Name	Response	Retention Time
DDT	502801	13.58
DDD	10401	13.28
DDE	229	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10630	513431	2.07

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082224\
Data File : BF139112.D
Acq On : 22 Aug 2024 09:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 22 10:59:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 01:25:05 2024
Response via : Initial Calibration

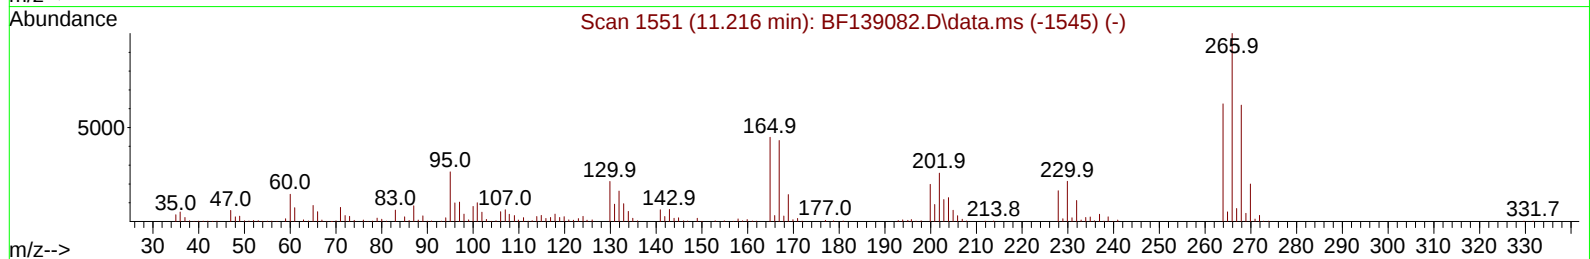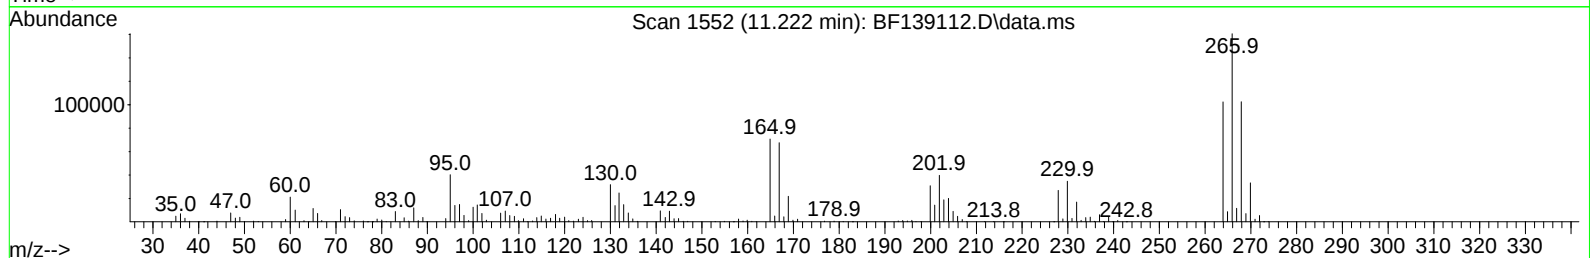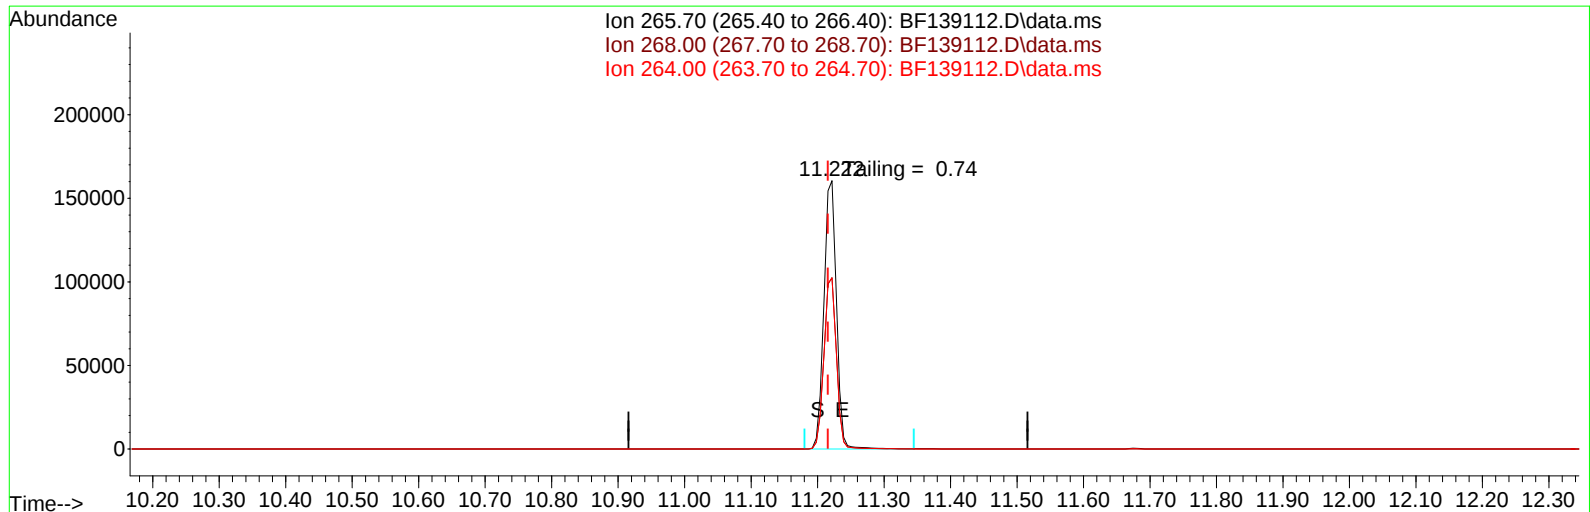

TIC: BF139112.D\data.ms

(70) Pentachlorophenol (C)

11.222min (+ 0.006) 34840.56 ng




response 211256

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	63.87
264.00	62.50	63.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082224\
Data File : BF139112.D
Acq On : 22 Aug 2024 09:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 22 10:59:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 01:25:05 2024
Response via : Initial Calibration

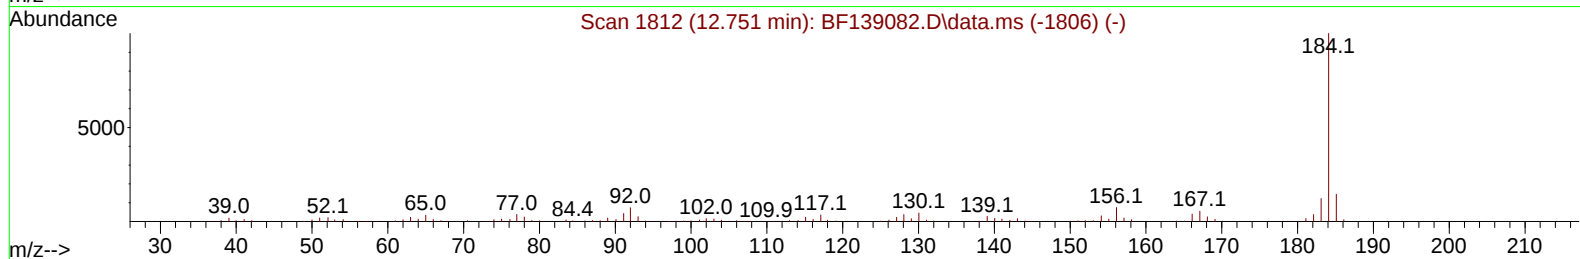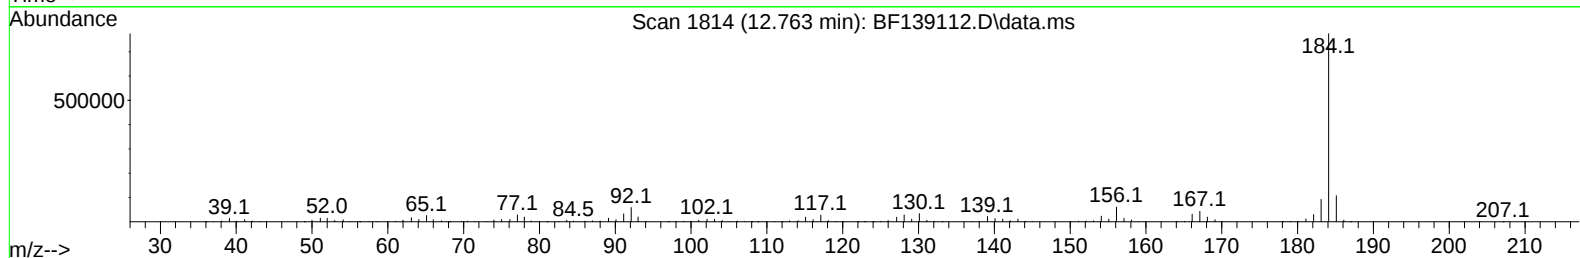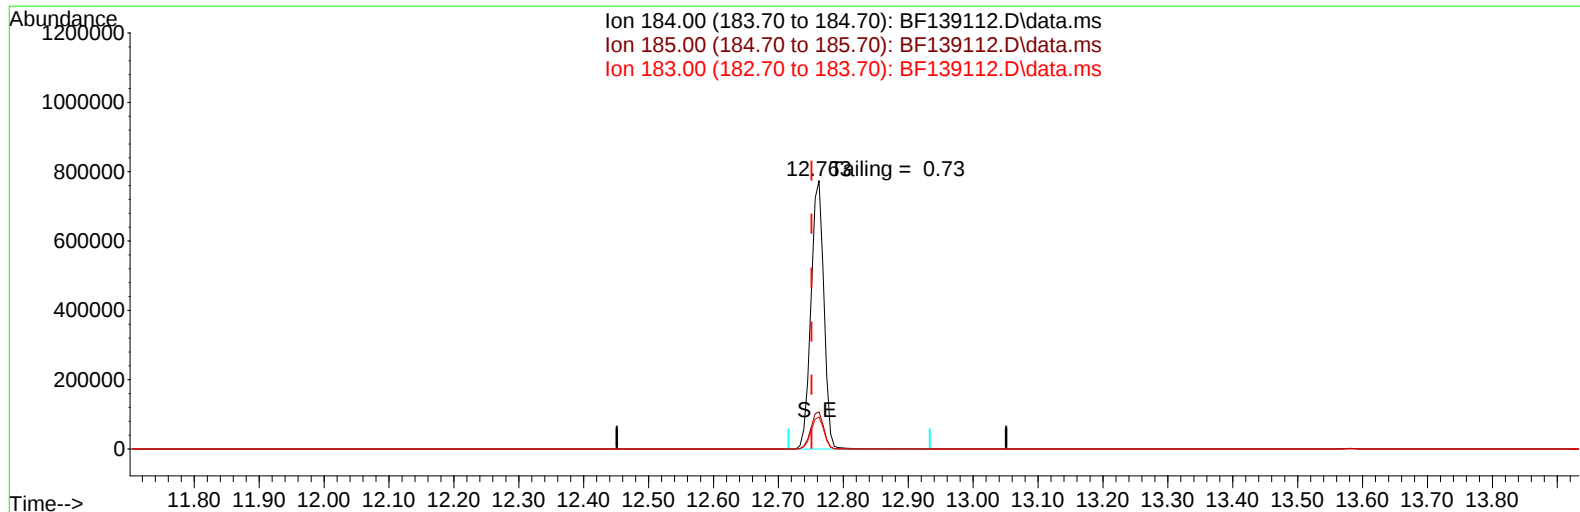

TIC: BF139112.D\data.ms

(77) Benzidine

12.763min (+ 0.012) 0.00 ng

response 1070049

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.87
183.00	12.20	11.96
0.00	0.00	0.00