
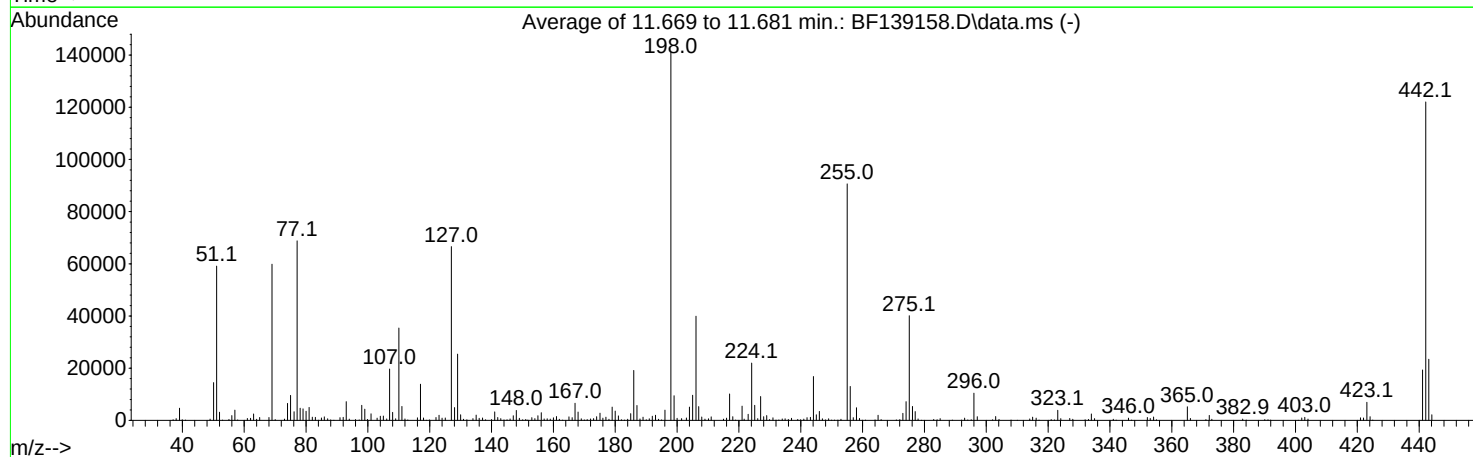


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082624\
Data File : BF139158.D
Acq On : 26 Aug 2024 09:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 21 01:25:05 2024

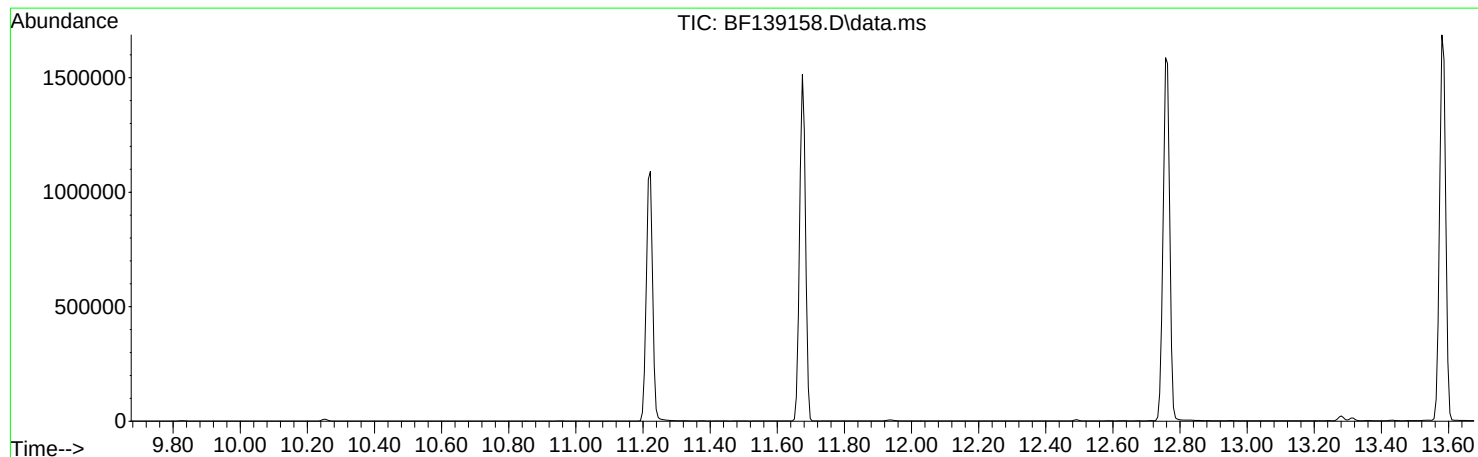

AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	59120	PASS
68	69	0.00	2	1.8	1099	PASS
69	198	0.00	100	42.5	59883	PASS
70	69	0.00	2	0.5	302	PASS
127	198	10	80	47.3	66616	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	140984	PASS
199	198	5	9	6.7	9430	PASS
275	198	10	60	28.5	40117	PASS
365	198	1	100	3.7	5187	PASS
441	198	0.01	100	13.7	19312	PASS
442	442	50	100	100.0	122029	PASS
443	442	15	24	19.2	23441	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
8/26/2024	BNA_F	<u>BF139158.D</u>
Compound Name	Response	Retention Time
DDT	410710	13.58
DDD	9712	13.28
DDE	439	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10151	420861	2.41

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082624\
Data File : BF139158.D
Acq On : 26 Aug 2024 09:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 26 10:54:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 01:25:05 2024
Response via : Initial Calibration

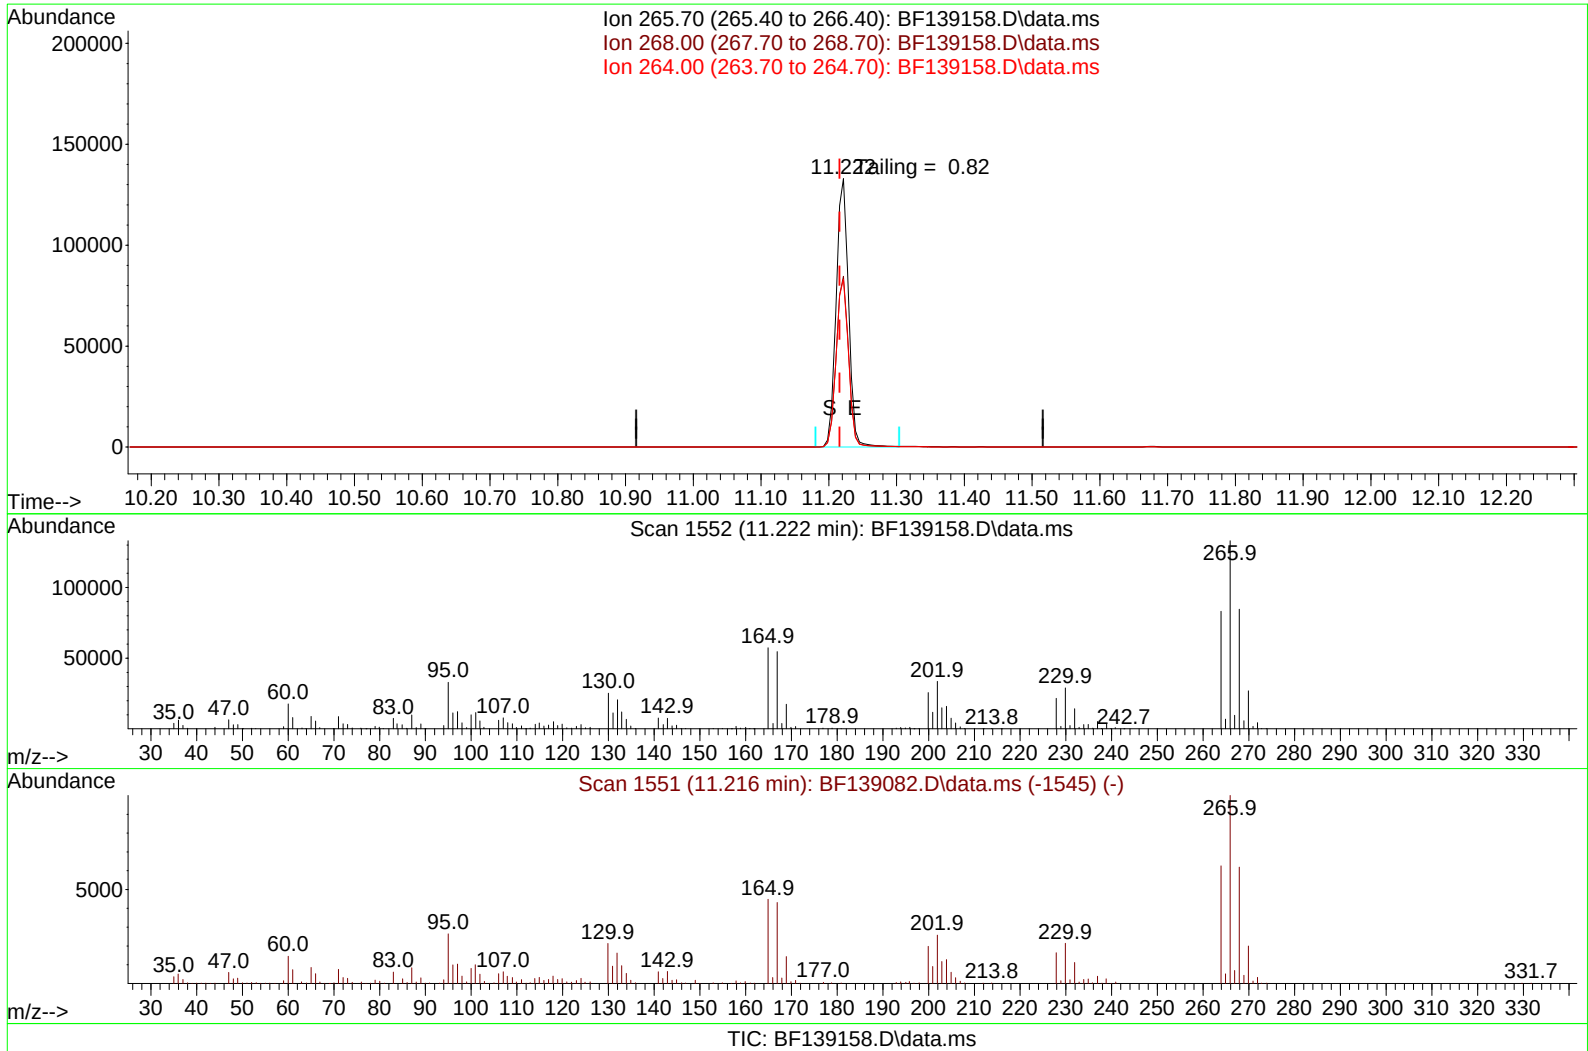

(70) Pentachlorophenol (C)

11.222min (+ 0.006) 29659.75 ng




response 170150

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	63.61
264.00	62.50	62.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082624\
Data File : BF139158.D
Acq On : 26 Aug 2024 09:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 26 10:54:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 01:25:05 2024
Response via : Initial Calibration

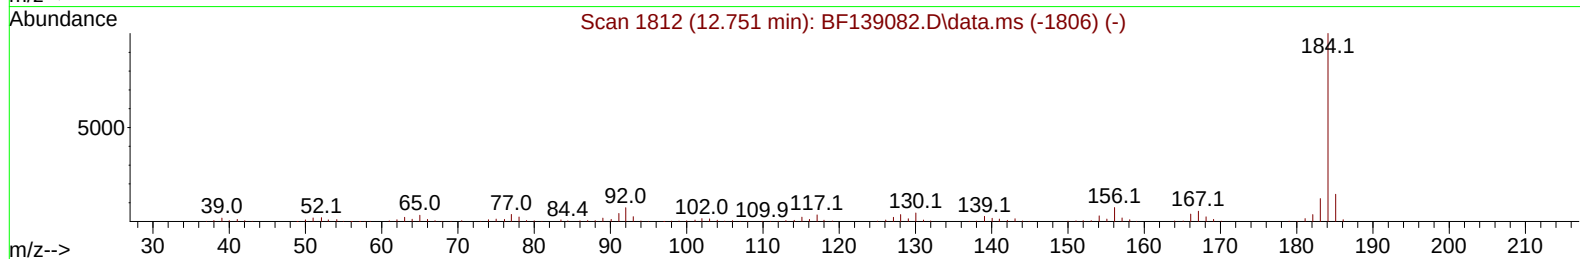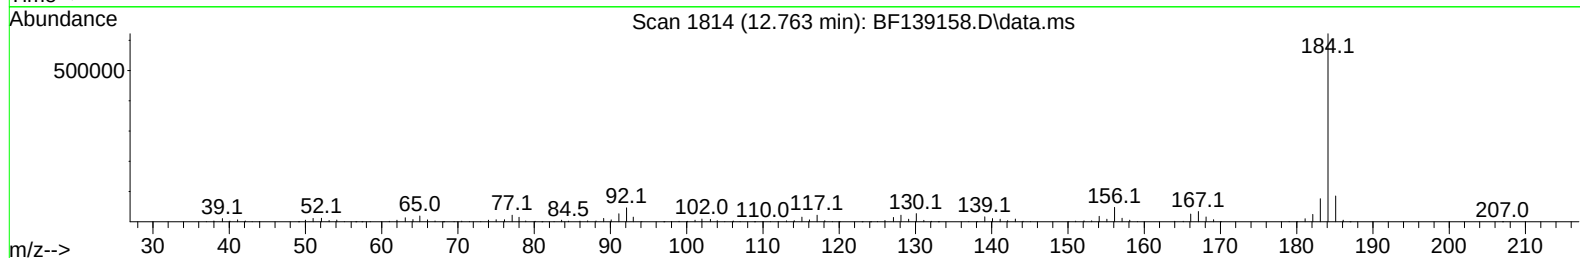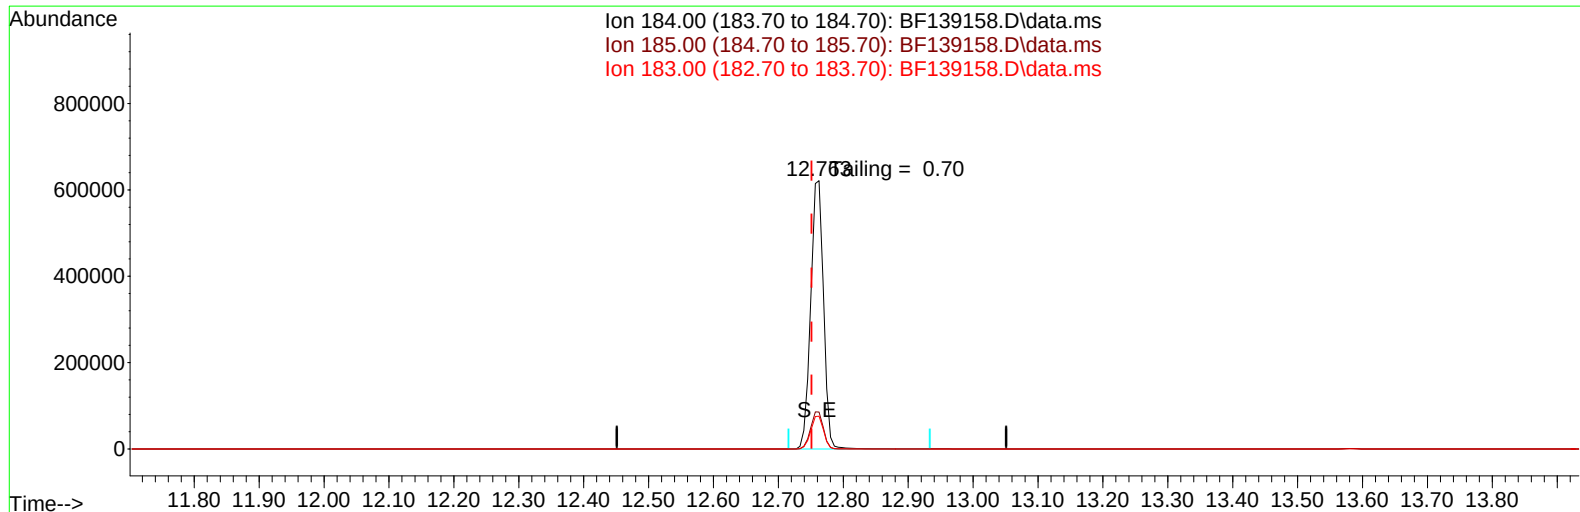

TIC: BF139158.D\data.ms

(77) Benzidine

12.763min (+ 0.012) 0.00 ng

response 856955

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.76
183.00	12.20	12.26
0.00	0.00	0.00