
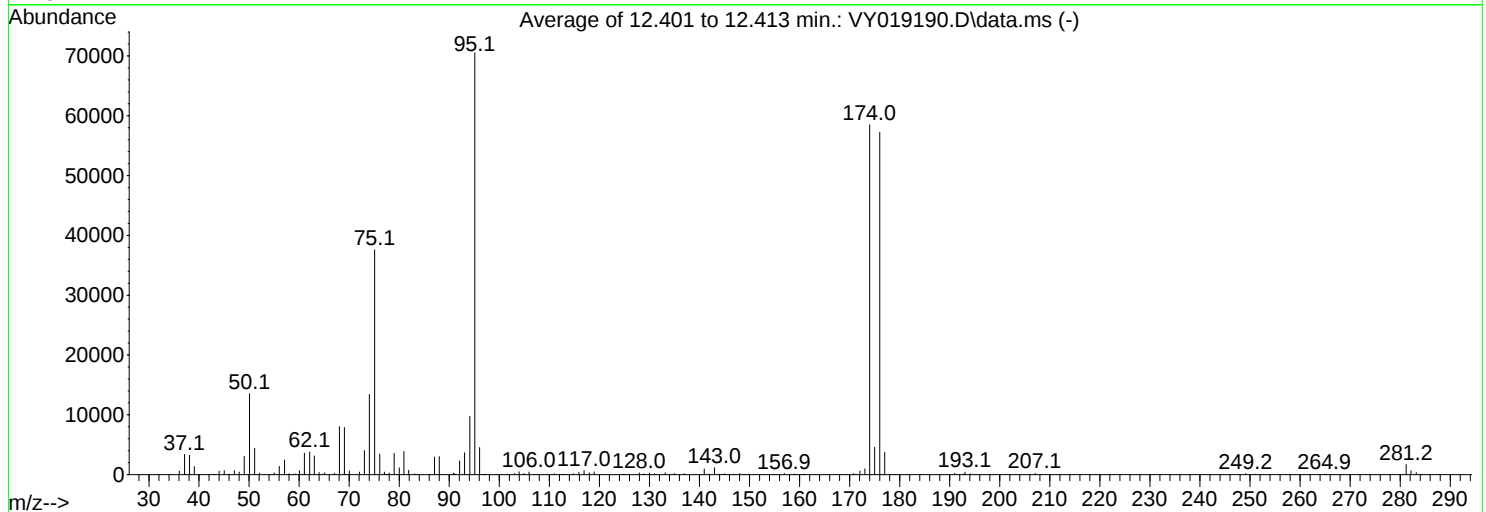


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082124\
Data File : VY019190.D
Acq On : 22 Aug 2024 00:38
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081524S.M
Title : SW846 8260
Last Update : Fri Aug 16 05:10:30 2024

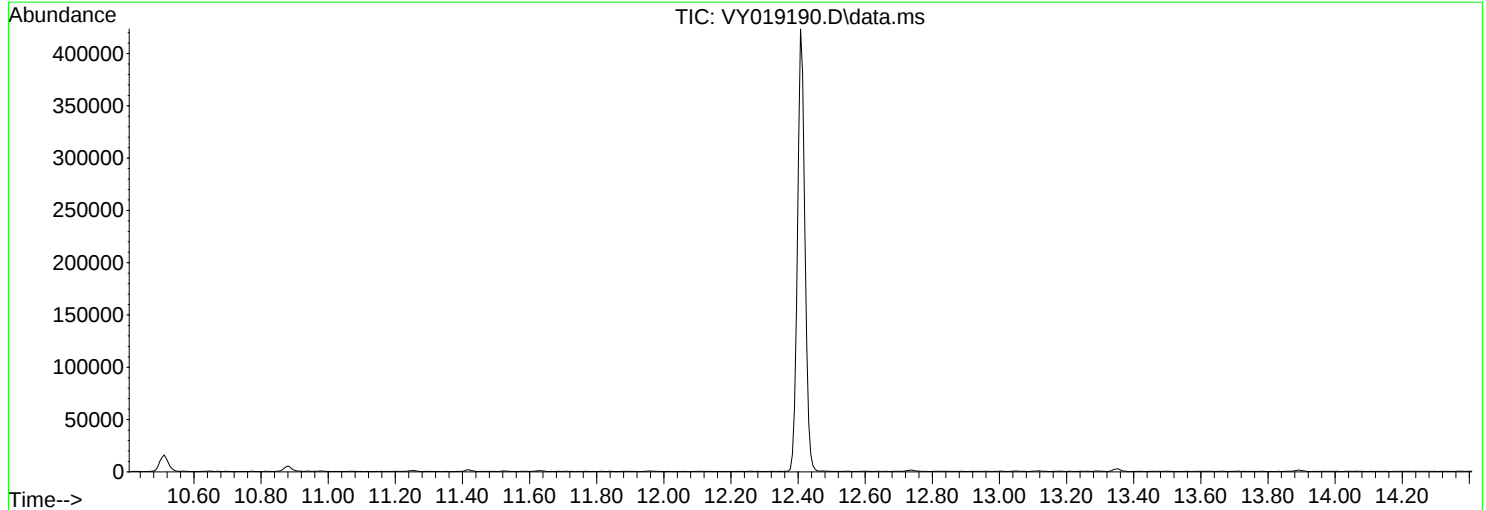

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	13537	PASS
75	95	30	60	53.3	37592	PASS
95	95	100	100	100.0	70525	PASS
96	95	5	9	6.4	4533	PASS
173	174	0.00	2	1.7	978	PASS
174	95	50	100	83.0	58507	PASS
175	174	5	9	7.8	4564	PASS
176	174	95	101	97.9	57256	PASS
177	176	5	9	6.5	3744	PASS