

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082124\
 Data File : VY019199.D
 Acq On : 22 Aug 2024 04:57
 Operator : SY/MD
 Sample : P3671-05
 Misc : 5.35g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 S-911-K1-SO-0-0.5-081924-FD

Quant Time: Aug 22 06:29:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081524S.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 16 05:10:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	81637	50.000	ug/l	0.01
34) 1,4-Difluorobenzene	8.609	114	146493	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.420	117	122862	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.352	152	38679	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.055	65	42446	51.868	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	103.740%
35) Dibromofluoromethane	7.634	113	48168	50.287	ug/l	0.01
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.580%
50) Toluene-d8	10.109	98	161402	46.824	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	93.640%
62) 4-Bromofluorobenzene	12.408	95	42871	36.484	ug/l	0.00
Spiked Amount	50.000	Range	29 - 146	Recovery	=	72.960%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082124\
Data File : VY019199.D
Acq On : 22 Aug 2024 04:57
Operator : SY/MD
Sample : P3671-05
Misc : 5.35g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
S-911-K1-SO-0-0.5-081924-FD

Quant Time: Aug 22 06:29:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081524S.M
Quant Title : SW846 8260
QLast Update : Fri Aug 16 05:10:30 2024
Response via : Initial Calibration




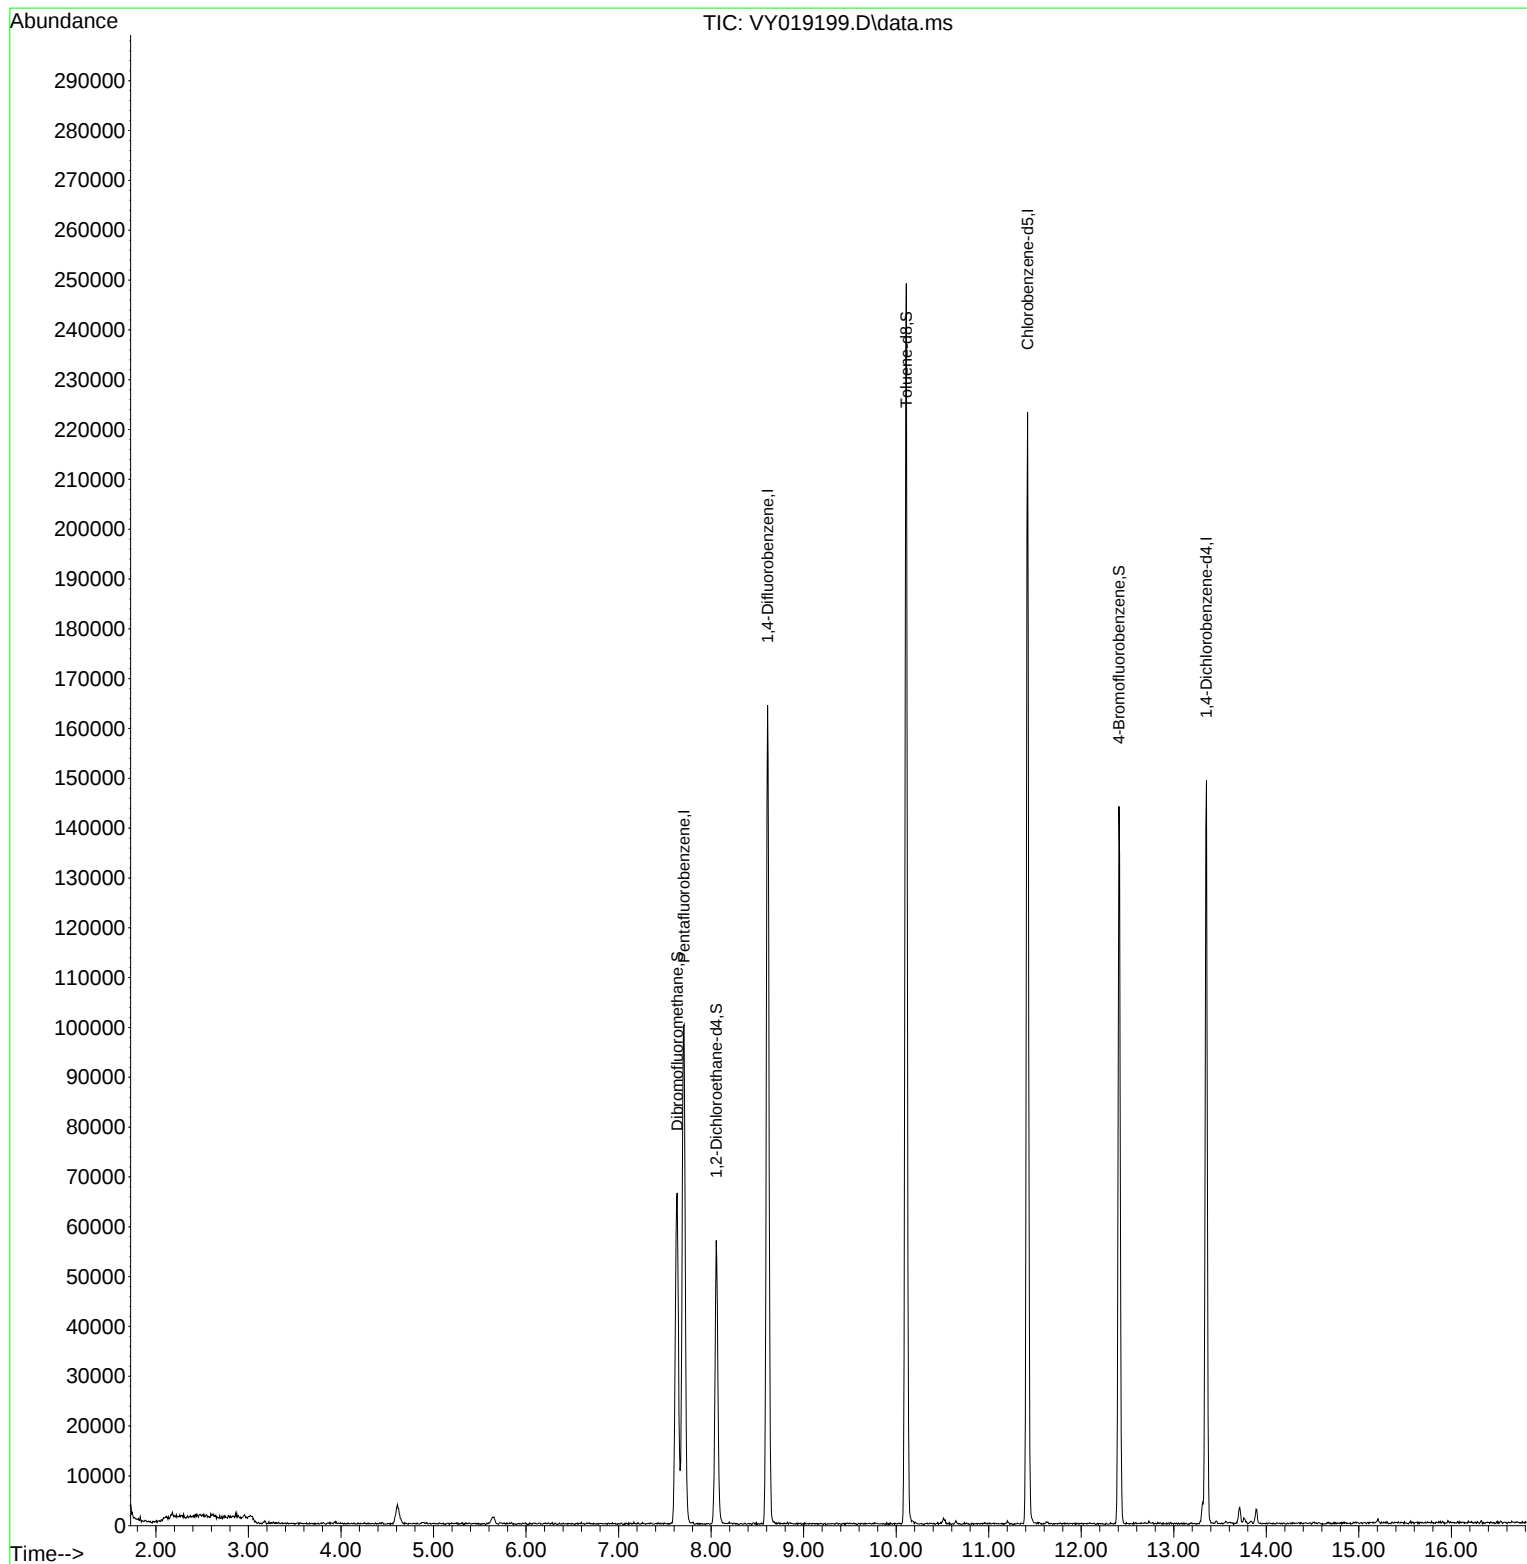


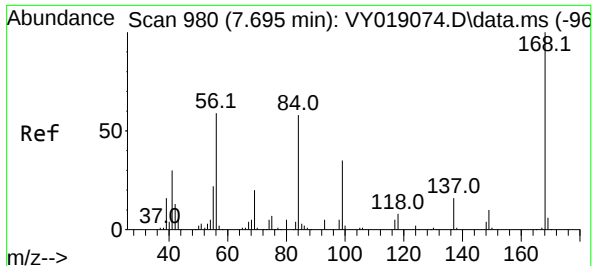

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. 0.012 min
Lab File: VY019199.D
Acq: 22 Aug 2024 04:57




Instrument :
MSVOA_Y
ClientSampleId :
S-911-K1-SO-0-0.5-081924-FD

Tgt Ion:168 Resp: 81637
Ion Ratio Lower Upper
168 100
99 50.7 39.1 58.7

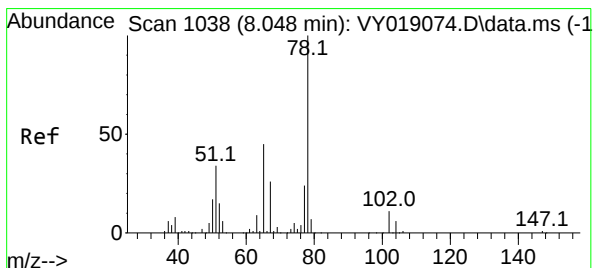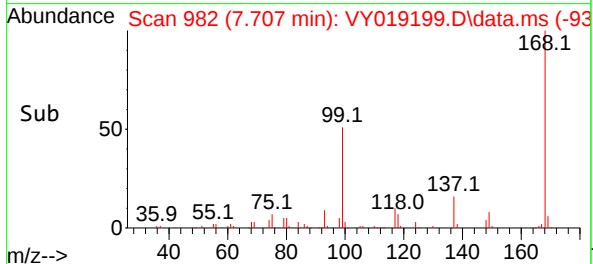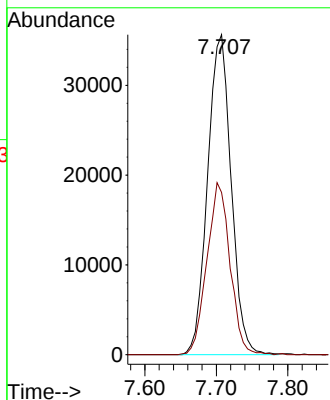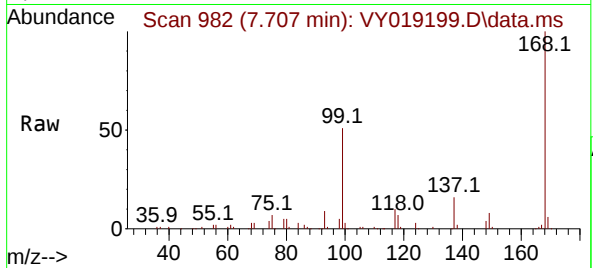

#33
1,2-Dichloroethane-d4
Concen: 51.868 ug/l
RT: 8.055 min Scan# 1039
Delta R.T. 0.006 min
Lab File: VY019199.D
Acq: 22 Aug 2024 04:57

Tgt Ion: 65 Resp: 42446
Ion Ratio Lower Upper
65 100
67 50.7 0.0 109.6

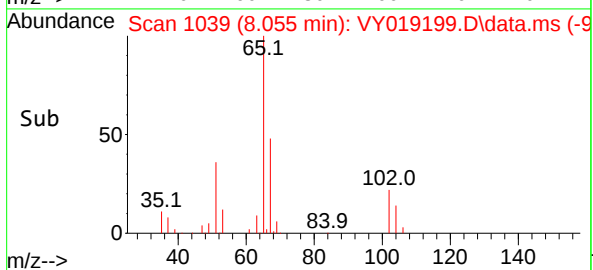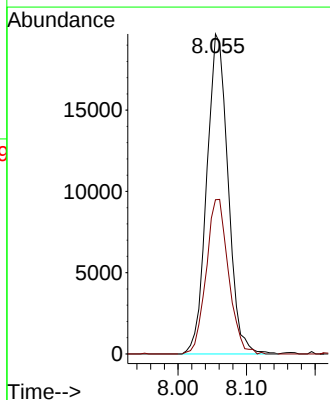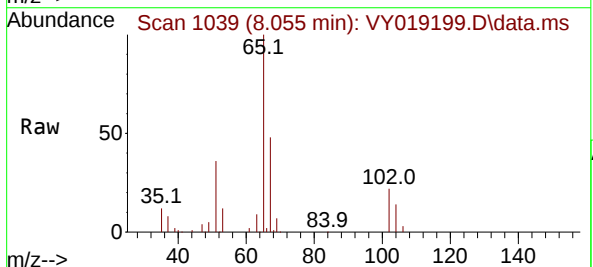



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.609 min Scan# 1129

Delta R.T. 0.006 min

Lab File: VY019199.D

Acq: 22 Aug 2024 04:57

Instrument :

MSVOA_Y

ClientSampleId :

S-911-K1-SO-0-0.5-081924-FD





Tgt Ion:114 Resp: 146493

Ion Ratio Lower Upper

114 100

63 17.8 0.0 35.0

88 15.0 0.0 27.2

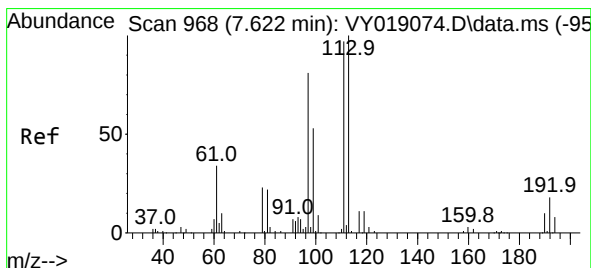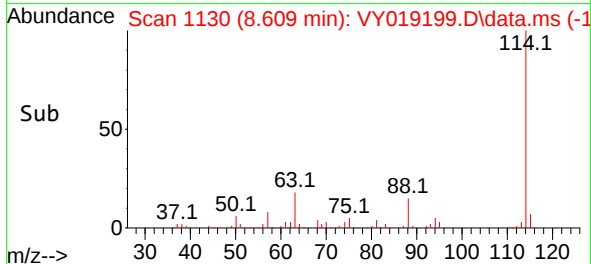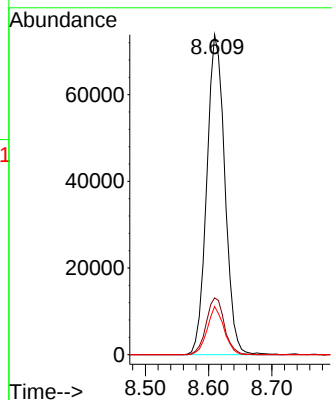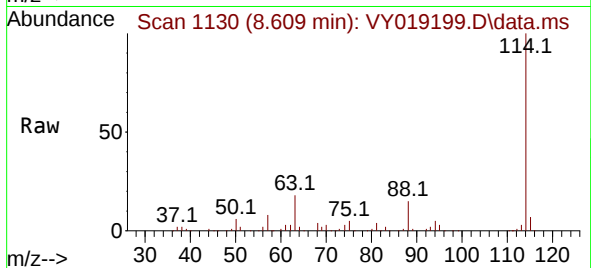

#35

Dibromofluoromethane

Concen: 50.287 ug/l

RT: 7.634 min Scan# 970

Delta R.T. 0.012 min

Lab File: VY019199.D

Acq: 22 Aug 2024 04:57




Tgt Ion:113 Resp: 48168


Ion Ratio Lower Upper

113 100

111 101.4 82.2 123.4

192 18.4 15.9 23.9

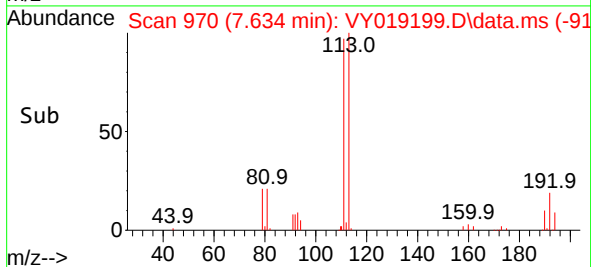
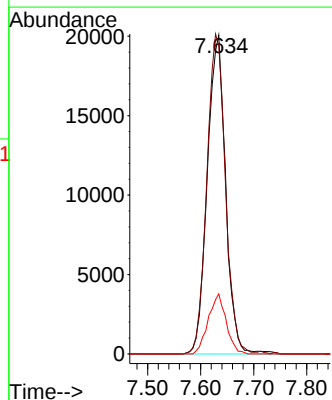
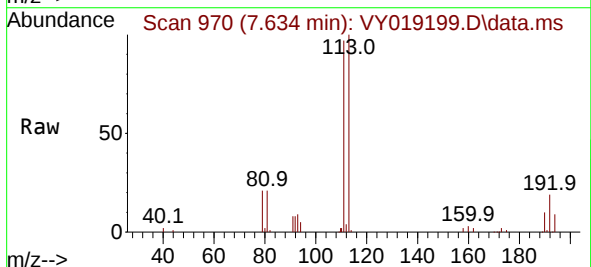


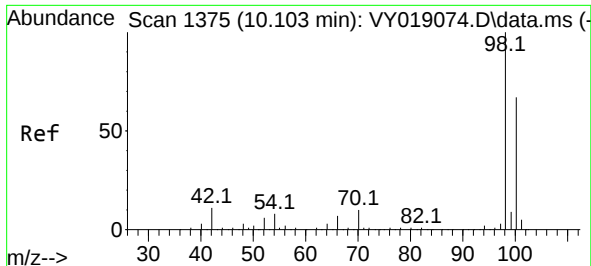

#50
Toluene-d8
Concen: 46.824 ug/l
RT: 10.109 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY019199.D
Acq: 22 Aug 2024 04:57




Instrument :
MSVOA_Y
ClientSampleId :
S-911-K1-SO-0-0.5-081924-FD


Tgt Ion: 98 Resp: 161402
Ion Ratio Lower Upper
98 100
100 67.0 52.0 78.0

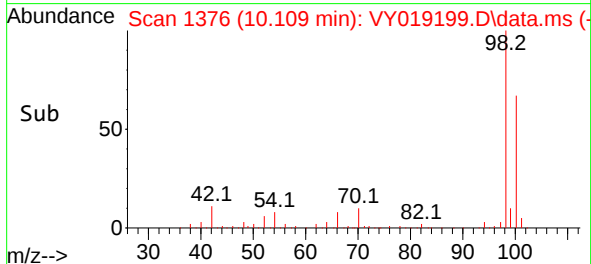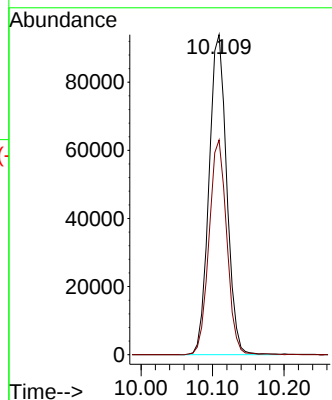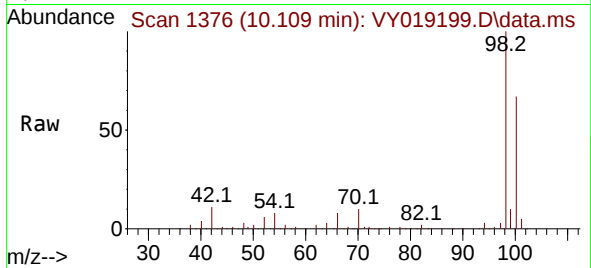

#62
4-Bromofluorobenzene
Concen: 36.484 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.006 min
Lab File: VY019199.D
Acq: 22 Aug 2024 04:57

Tgt Ion: 95 Resp: 42871
Ion Ratio Lower Upper
95 100
174 87.1 0.0 175.6
176 84.3 0.0 171.4

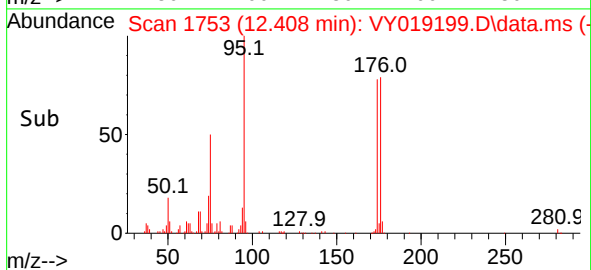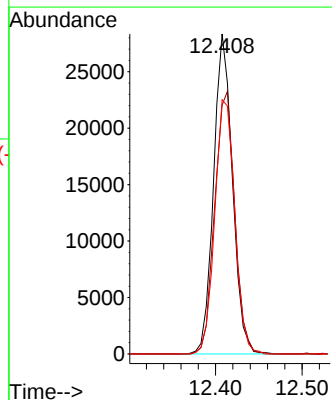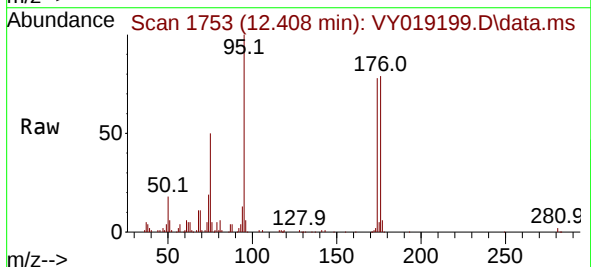

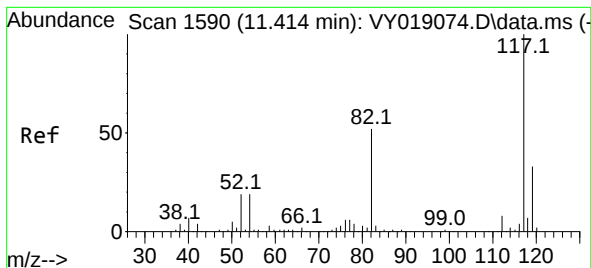

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.420 min Scan# 11

Delta R.T. 0.006 min

Lab File: VY019199.D

Acq: 22 Aug 2024 04:57

Instrument :

MSVOA_Y

ClientSampleId :

S-911-K1-SO-0-0.5-081924-FD





Tgt Ion:117 Resp: 122862

Ion Ratio Lower Upper

117 100

82 50.0 42.4 63.6

119 31.2 25.9 38.9

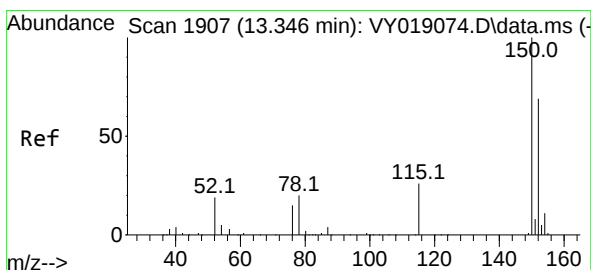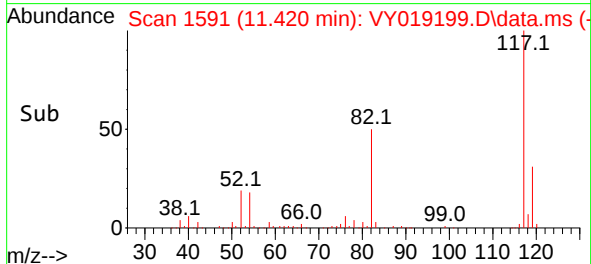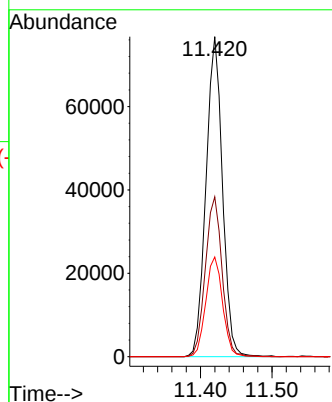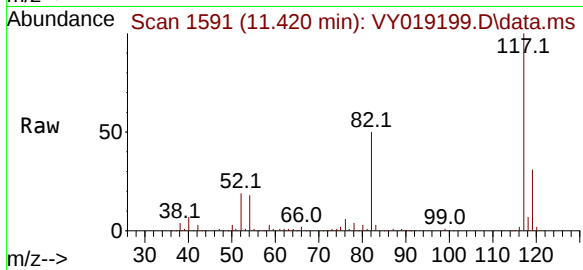

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.352 min Scan# 1908

Delta R.T. 0.006 min

Lab File: VY019199.D

Acq: 22 Aug 2024 04:57

Tgt Ion:152 Resp: 38679

Ion Ratio Lower Upper

152 100

115 56.6 28.2 84.7

150 156.9 0.0 345.6

