

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082224\
 Data File : VY019230.D
 Acq On : 22 Aug 2024 19:10
 Operator : SY/MD
 Sample : P3671-14
 Misc : 4.18g/5.0mL/MSVOA_Y/SOIL/B
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 S-912-J-SO-0.5-1-081924

Quant Time: Aug 23 01:56:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081524S.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 16 05:10:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.701	168	88575	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.609	114	159662	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	125272	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	42316	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.055	65	53101	59.805	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	119.620%
35) Dibromofluoromethane	7.622	113	48185	46.156	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	92.320%
50) Toluene-d8	10.103	98	182340	48.535	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	97.080%
62) 4-Bromofluorobenzene	12.408	95	47141	36.808	ug/l	0.00
Spiked Amount	50.000	Range	29 - 146	Recovery	=	73.620%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082224\
Data File : VY019230.D
Acq On : 22 Aug 2024 19:10
Operator : SY/MD
Sample : P3671-14
Misc : 4.18g/5.0mL/MSVOA_Y/SOIL/B
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
S-912-J-SO-0.5-1-081924

Quant Time: Aug 23 01:56:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081524S.M
Quant Title : SW846 8260
QLast Update : Fri Aug 16 05:10:30 2024
Response via : Initial Calibration




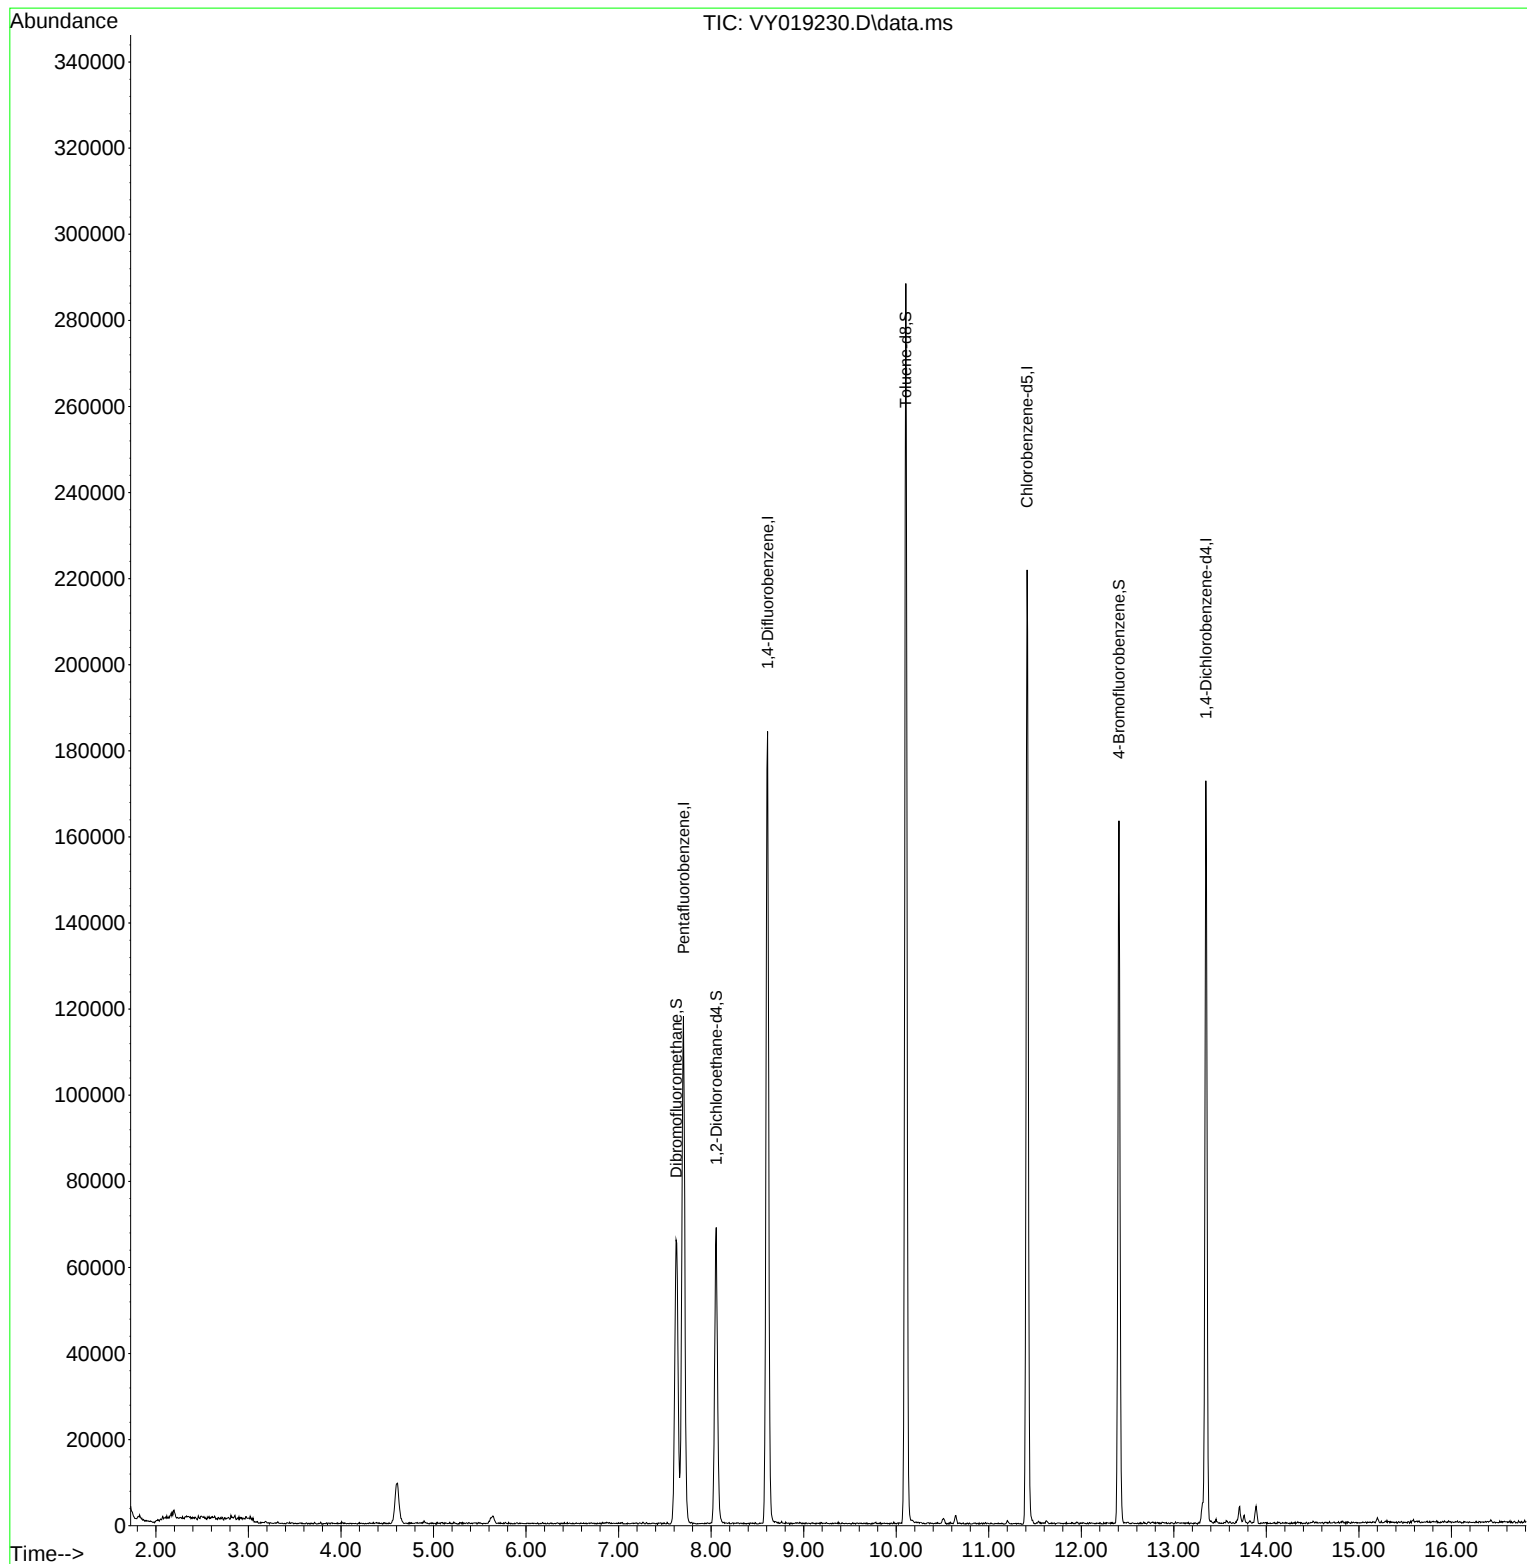


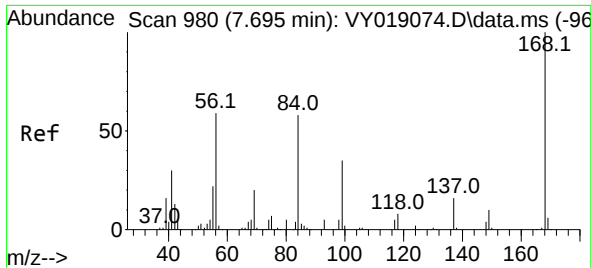

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.701 min Scan# 981
Delta R.T. 0.006 min
Lab File: VY019230.D
Acq: 22 Aug 2024 19:10




Instrument :
MSVOA_Y
ClientSampleId :
S-912-J-SO-0.5-1-081924

Tgt Ion:168 Resp: 88575
Ion Ratio Lower Upper
168 100
99 54.5 39.1 58.7

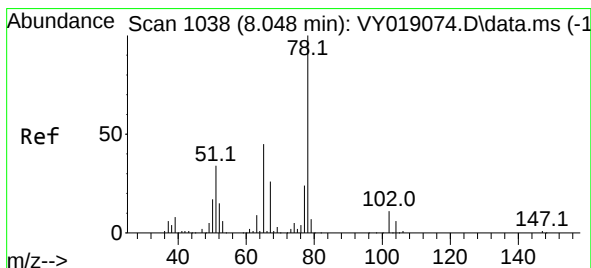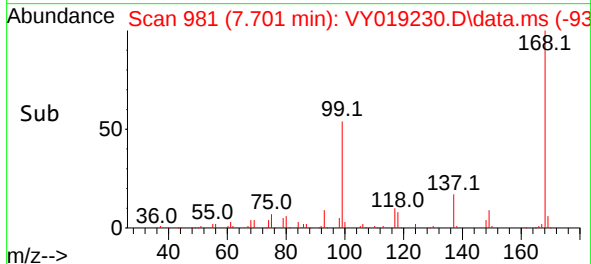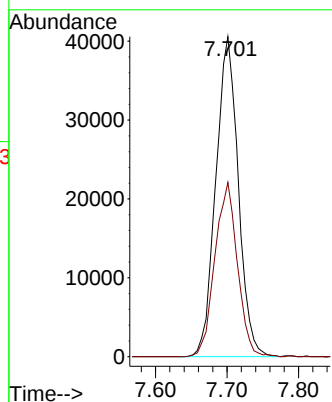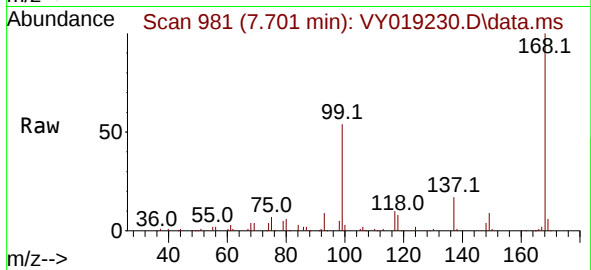

#33
1,2-Dichloroethane-d4
Concen: 59.805 ug/l
RT: 8.055 min Scan# 1039
Delta R.T. 0.006 min
Lab File: VY019230.D
Acq: 22 Aug 2024 19:10

Tgt Ion: 65 Resp: 53101
Ion Ratio Lower Upper
65 100
67 52.4 0.0 109.6


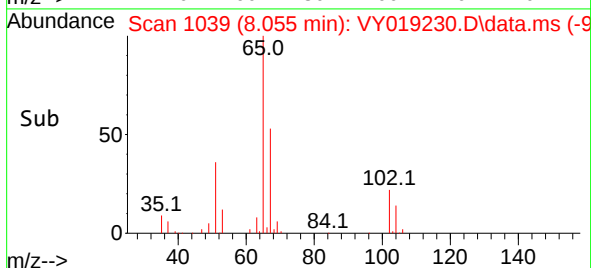
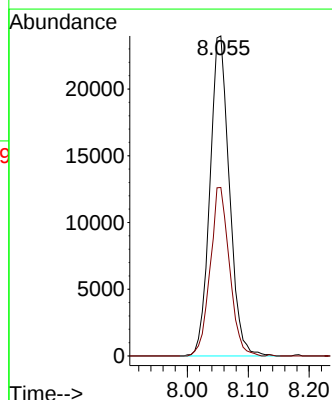
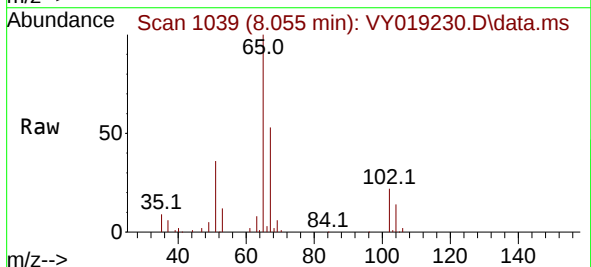




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.609 min Scan# 1129
Delta R.T. 0.006 min
Lab File: VY019230.D
Acq: 22 Aug 2024 19:10




Instrument :
MSVOA_Y
ClientSampleId :
S-912-J-SO-0.5-1-081924


Tgt Ion:114 Resp: 159662
Ion Ratio Lower Upper
114 100
63 18.8 0.0 35.0
88 14.3 0.0 27.2

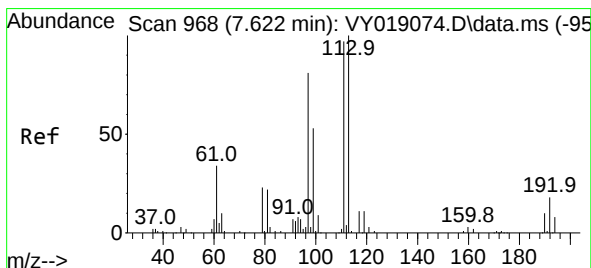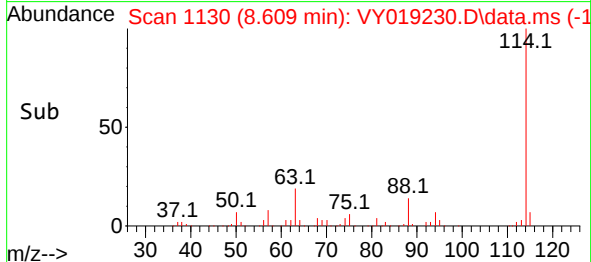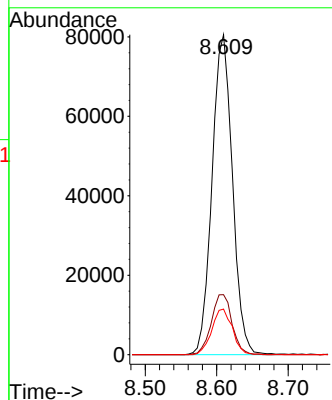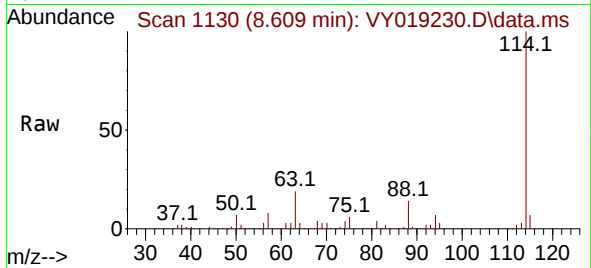

#35
Dibromofluoromethane
Concen: 46.156 ug/l
RT: 7.622 min Scan# 968
Delta R.T. 0.000 min
Lab File: VY019230.D
Acq: 22 Aug 2024 19:10

Tgt Ion:113 Resp: 48185
Ion Ratio Lower Upper
113 100
111 102.3 82.2 123.4
192 19.9 15.9 23.9

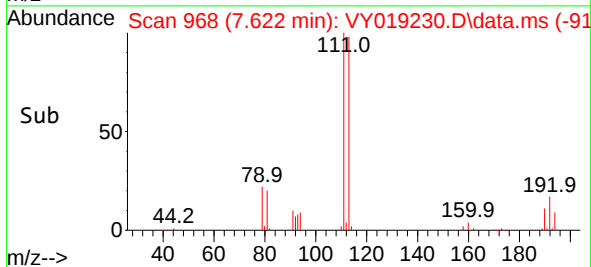
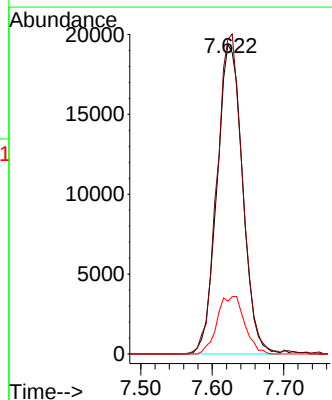
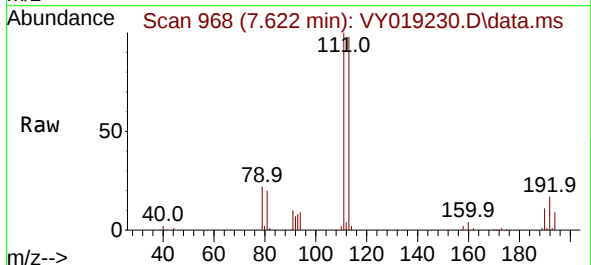


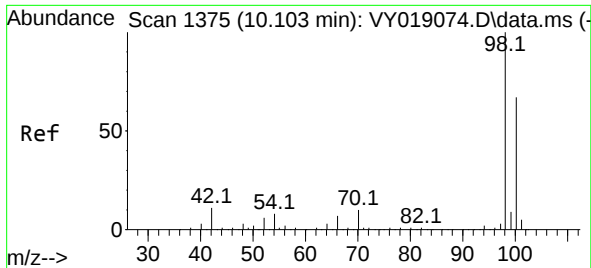

#50
Toluene-d8
Concen: 48.535 ug/l
RT: 10.103 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY019230.D
Acq: 22 Aug 2024 19:10




Instrument :
MSVOA_Y
ClientSampleId :
S-912-J-SO-0.5-1-081924


Tgt Ion: 98 Resp: 182340
Ion Ratio Lower Upper
98 100
100 66.7 52.0 78.0

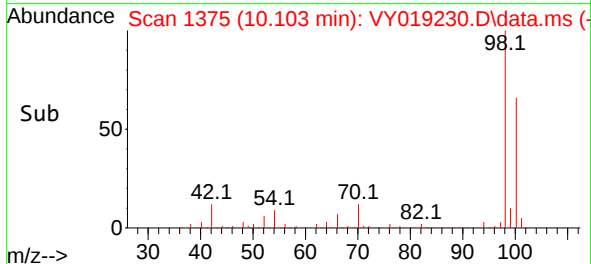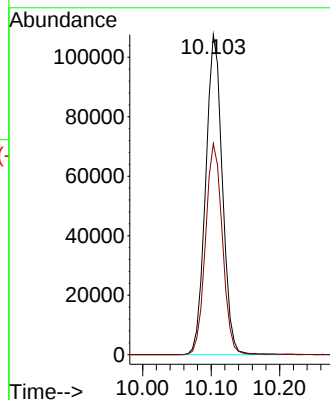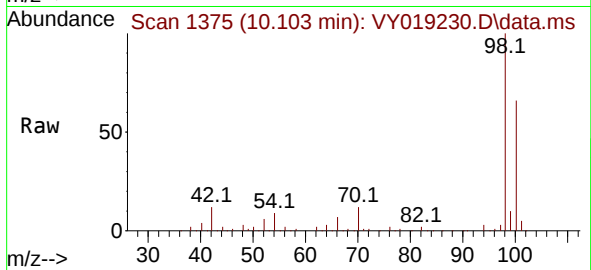

#62
4-Bromofluorobenzene
Concen: 36.808 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.006 min
Lab File: VY019230.D
Acq: 22 Aug 2024 19:10

Tgt Ion: 95 Resp: 47141
Ion Ratio Lower Upper
95 100
174 88.0 0.0 175.6
176 86.9 0.0 171.4

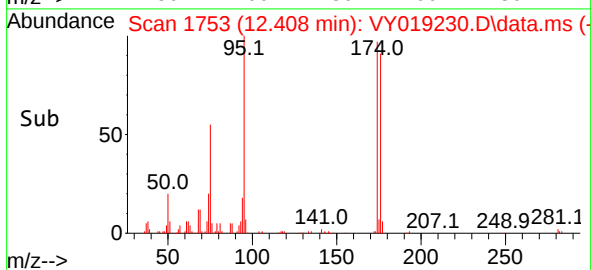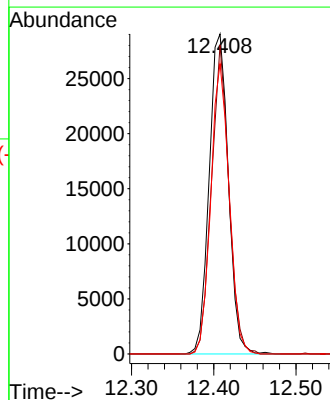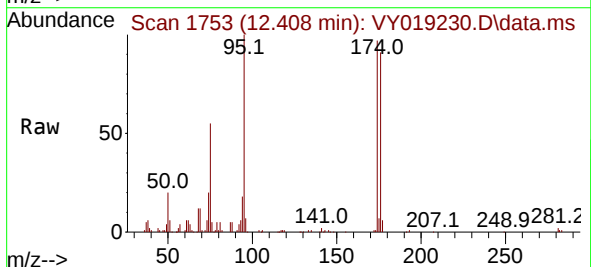

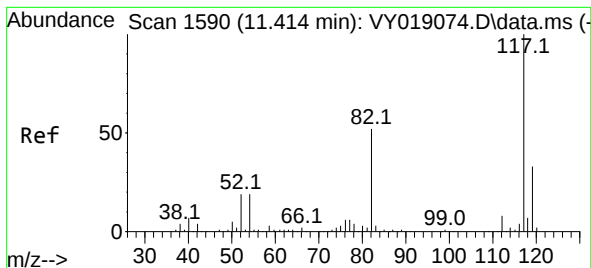

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY019230.D

Acq: 22 Aug 2024 19:10

Instrument :

MSVOA_Y

ClientSampleId :

S-912-J-SO-0.5-1-081924





Tgt Ion:117 Resp: 125272

Ion Ratio Lower Upper

117 100

82 53.0 42.4 63.6

119 31.6 25.9 38.9

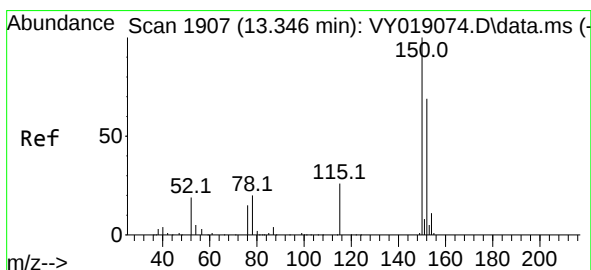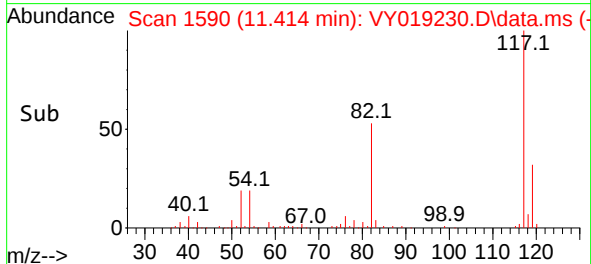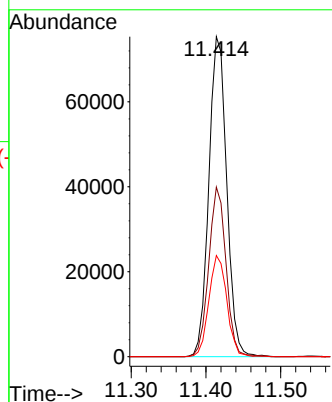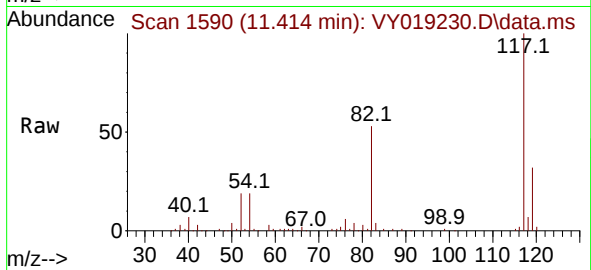

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. 0.000 min

Lab File: VY019230.D

Acq: 22 Aug 2024 19:10

Tgt Ion:152 Resp: 42316

Ion Ratio Lower Upper

152 100

115 57.1 28.2 84.7

150 159.7 0.0 345.6

