

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090924\
 Data File : PL091587.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2024 19:10
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL090924

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 19:24:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 09 19:23:02 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.542	2.781	82136840	123.4E6	54.067	55.643
28) SA Decachlor...	9.053	7.921	63278192	98168492	52.500	52.286
Target Compounds						
23) Chlordane-1	4.703	3.780	33873423	36368107	543.923	522.795
24) Chlordane-2	5.233	4.356	39026737	38911481	507.617	519.155
25) Chlordane-3	5.942	4.987	113.7E6	118.2E6	442.444	506.829
26) Chlordane-4	6.024	5.050	154.1E6	112.6E6	520.321	540.049
27) Chlordane-5	6.873	5.945	30416372	37732567	532.898	526.546



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090924\
Data File : PL091587.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2024 19:10
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL090924

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 19:24:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
Quant Title : GC Extractables
QLast Update : Mon Sep 09 19:23:02 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

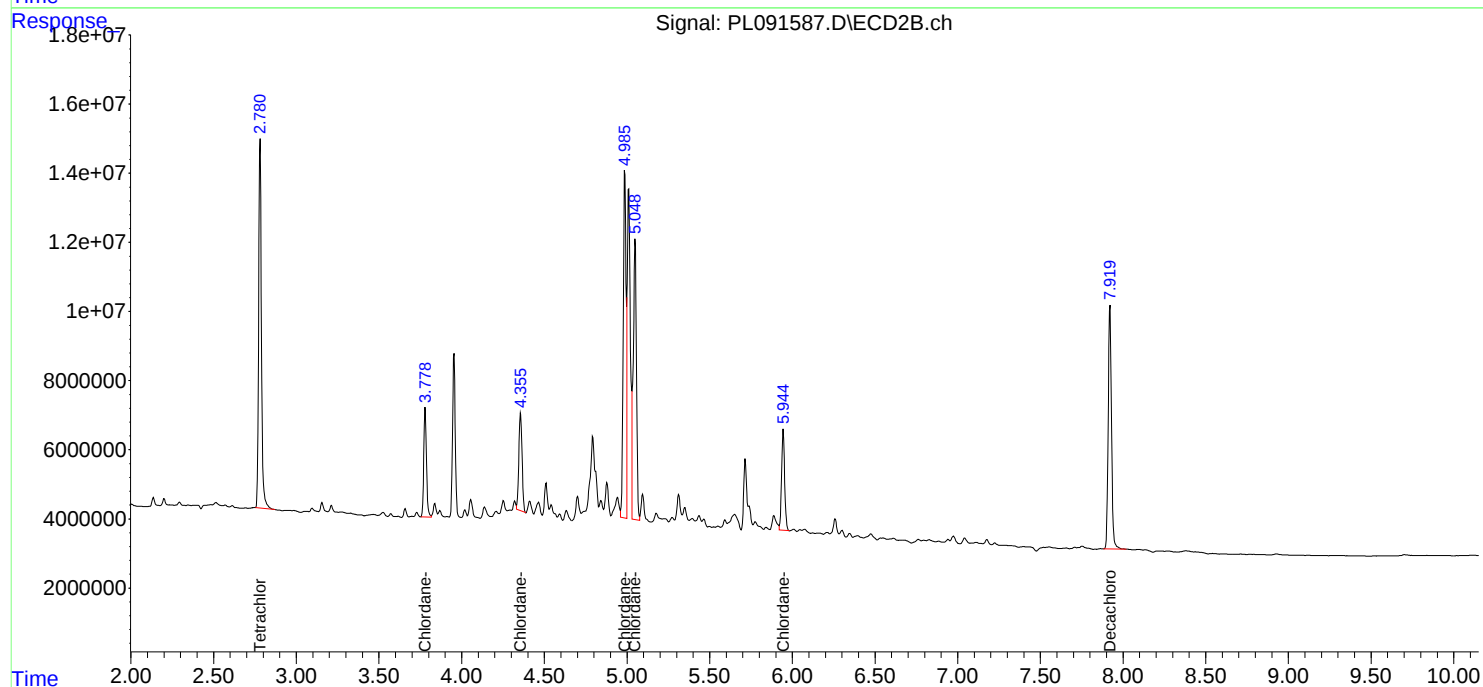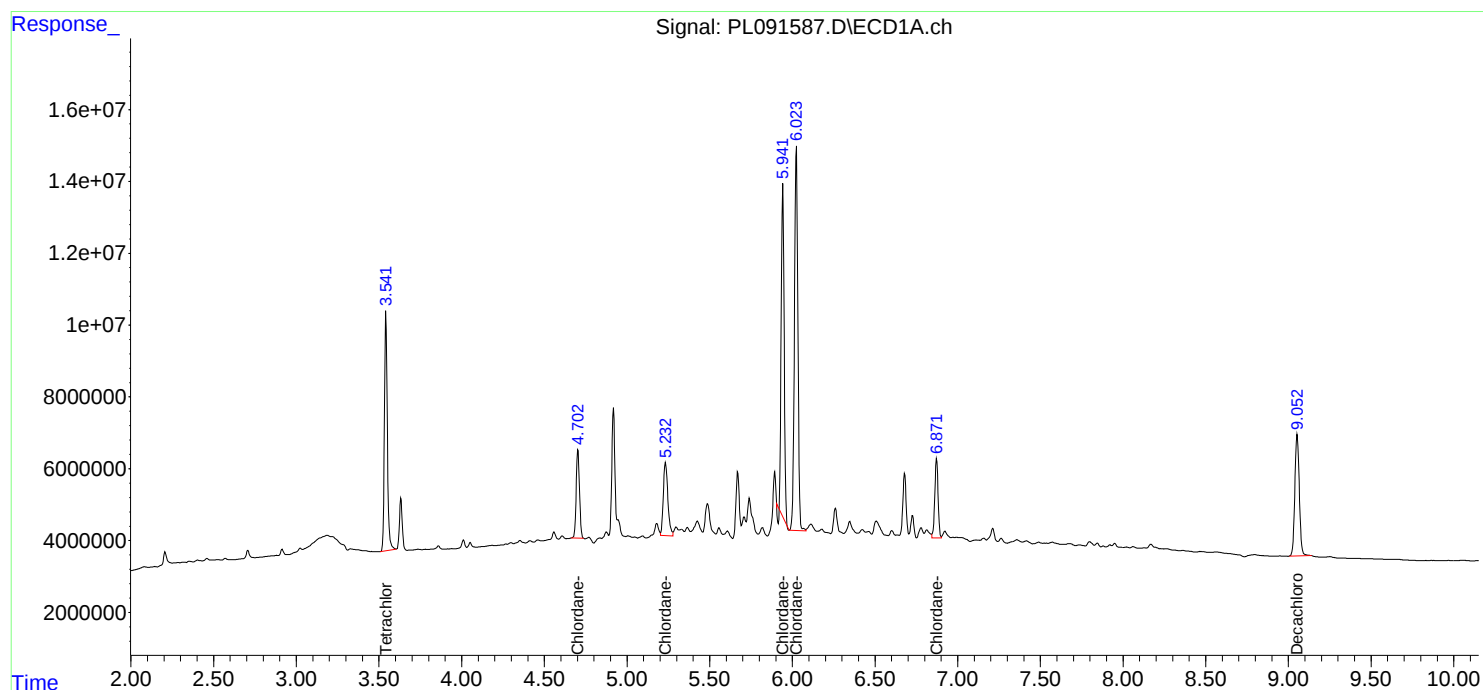


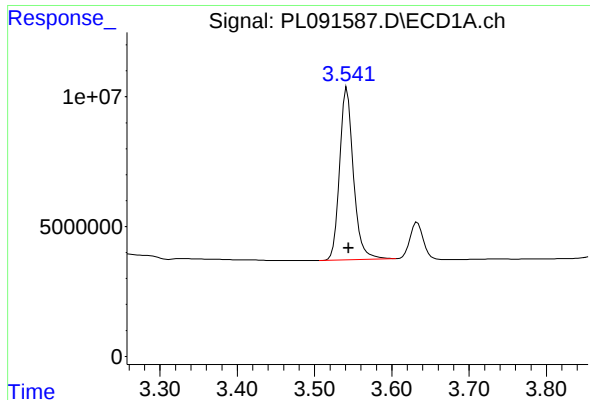

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 82136840
Conc: 54.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL090924

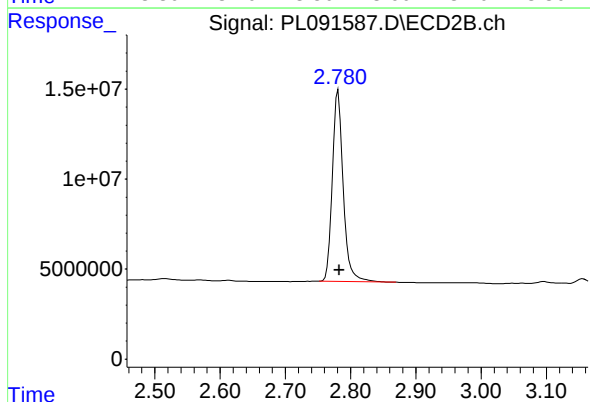


#1 Tetrachloro-m-xylene

R.T.: 2.781 min
Delta R.T.: -0.002 min
Response: 123412200
Conc: 55.64 ng/ml

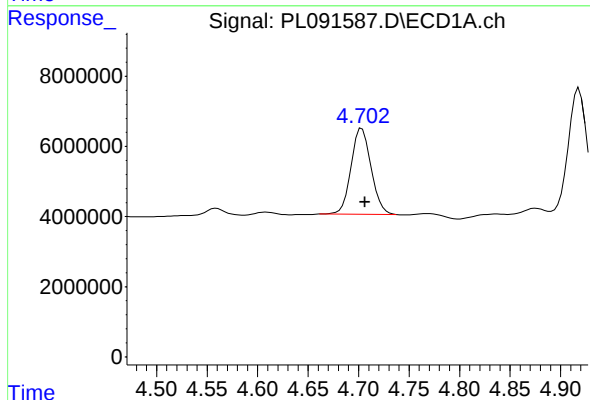


#23 Chlordane-1

R.T.: 4.703 min
Delta R.T.: -0.003 min
Response: 33873423
Conc: 543.92 ng/ml

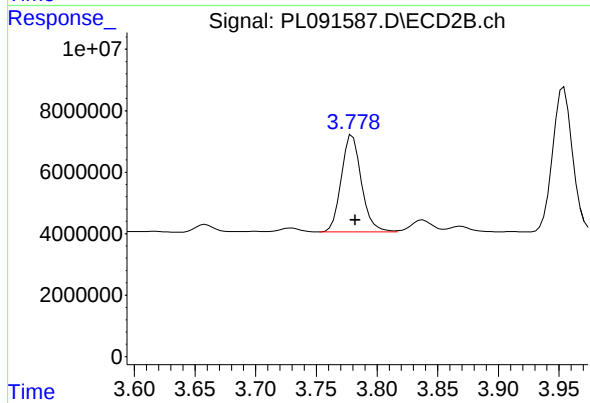

#23 Chlordane-1


R.T.: 3.780 min
Delta R.T.: -0.002 min
Response: 36368107
Conc: 522.79 ng/ml

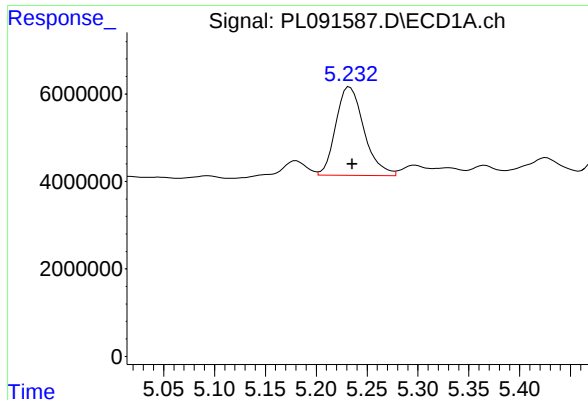

#24 Chlordane-2


R.T.: 5.233 min
Delta R.T.: -0.003 min
Response: 39026737
Conc: 507.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL090924

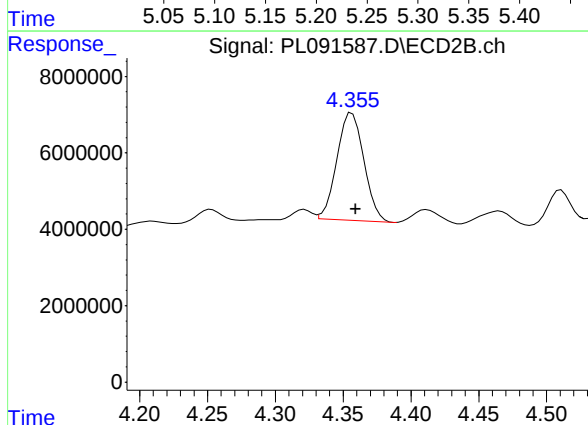


#24 Chlordane-2

R.T.: 4.356 min
Delta R.T.: -0.003 min
Response: 38911481
Conc: 519.15 ng/ml

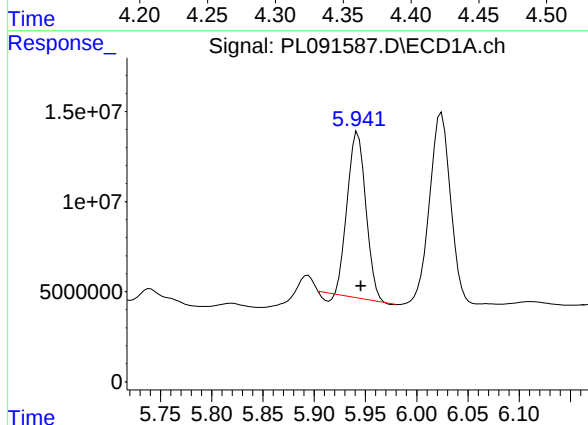


#25 Chlordane-3

R.T.: 5.942 min
Delta R.T.: -0.003 min
Response: 113663559
Conc: 442.44 ng/ml

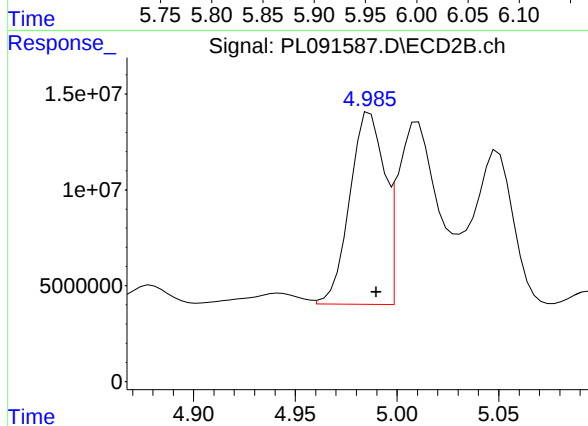

#25 Chlordane-3


R.T.: 4.987 min
Delta R.T.: -0.003 min
Response: 118162680
Conc: 506.83 ng/ml

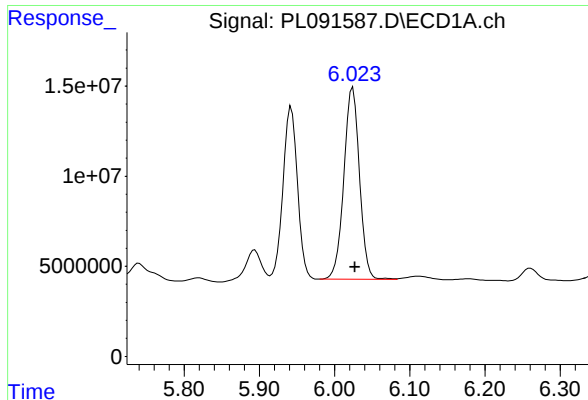

#26 Chlordane-4


R.T.: 6.024 min
Delta R.T.: -0.003 min
Response: 154096333
Conc: 520.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL090924

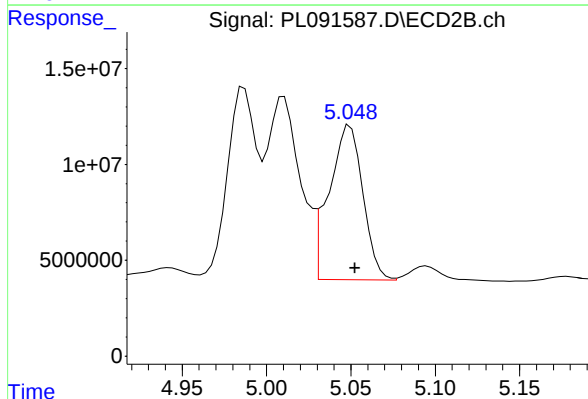


#26 Chlordane-4

R.T.: 5.050 min
Delta R.T.: -0.003 min
Response: 112618104
Conc: 540.05 ng/ml

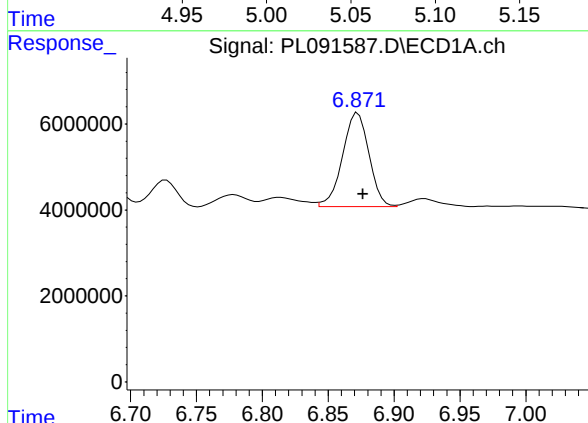


#27 Chlordane-5

R.T.: 6.873 min
Delta R.T.: -0.004 min
Response: 30416372
Conc: 532.90 ng/ml

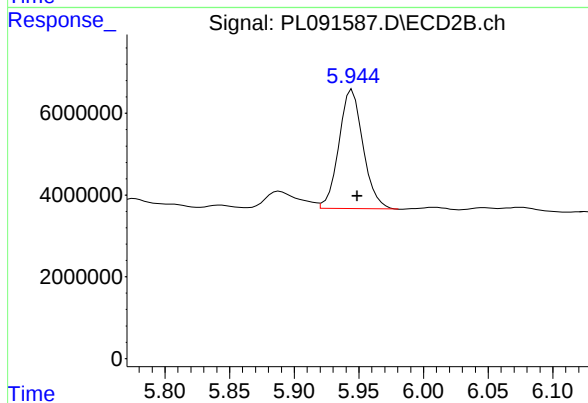

#27 Chlordane-5


R.T.: 5.945 min
Delta R.T.: -0.004 min
Response: 37732567
Conc: 526.55 ng/ml

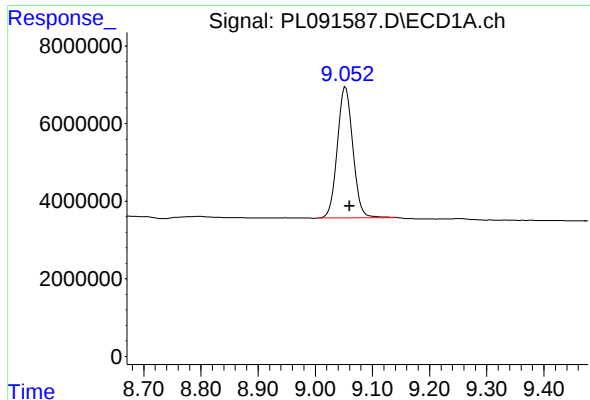

#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: -0.008 min
Response: 63278192
Conc: 52.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL090924

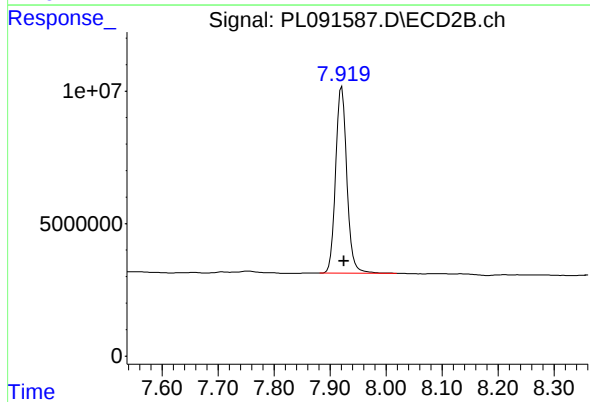

#28 Decachlorobiphenyl

R.T.: 7.921 min
Delta R.T.: -0.004 min
Response: 98168492
Conc: 52.29 ng/ml