

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090924\
 Data File : PL091576.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2024 16:39
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 17:21:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 09 17:19:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.545	2.783	145.4E6	226.2E6	99.807	100.844
28) SA Decachlor...	9.060	7.925	110.9E6	179.5E6	97.676	99.215
Target Compounds						
23) Chlordane-1	4.706	3.782	60104002	67613308	989.122	1003.881
24) Chlordane-2	5.237	4.359	67677534	72257952	957.523	995.703
25) Chlordane-3	5.946	4.990	243.1E6	230.3E6	995.905	1016.117
26) Chlordane-4	6.028	5.052	291.7E6	214.7E6	997.309	1014.664
27) Chlordane-5	6.877	5.949	54634339	73932244	984.766	1021.255



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090924\
Data File : PL091576.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2024 16:39
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 17:21:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
Quant Title : GC Extractables
QLast Update : Mon Sep 09 17:19:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

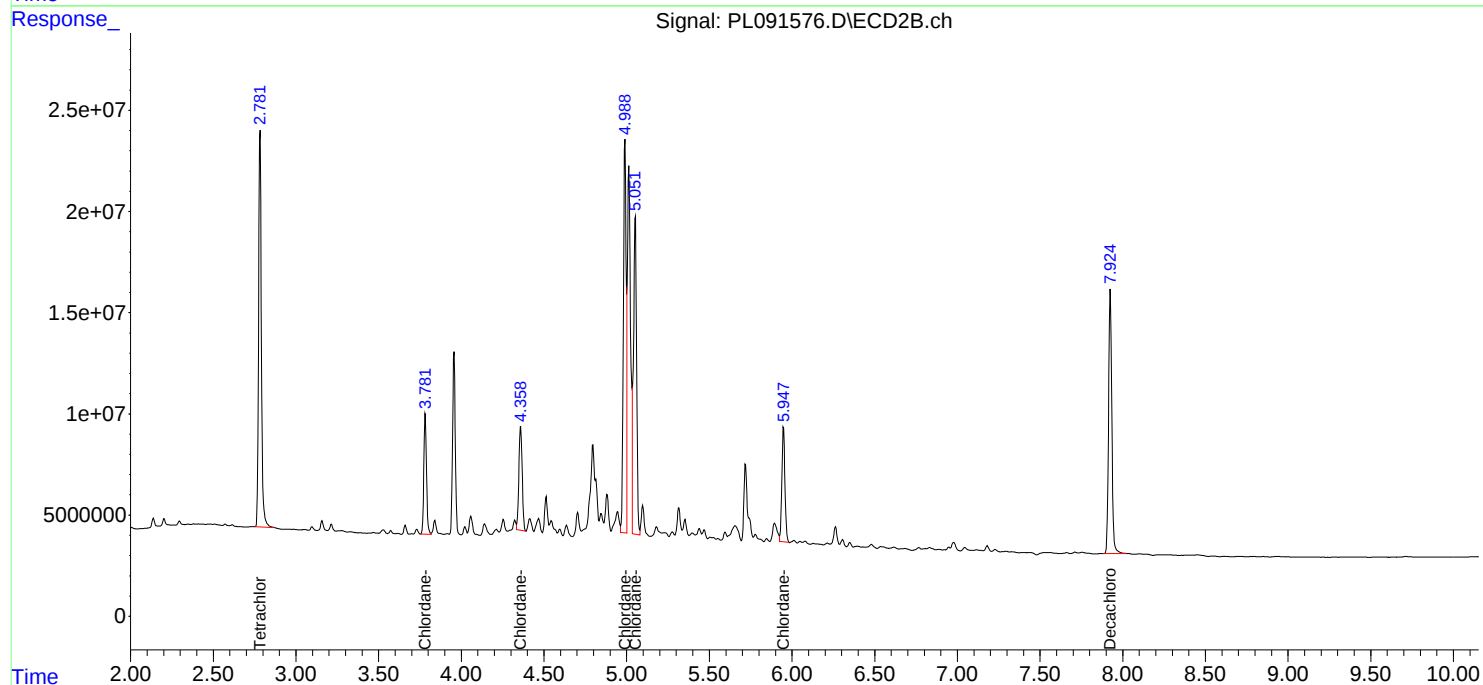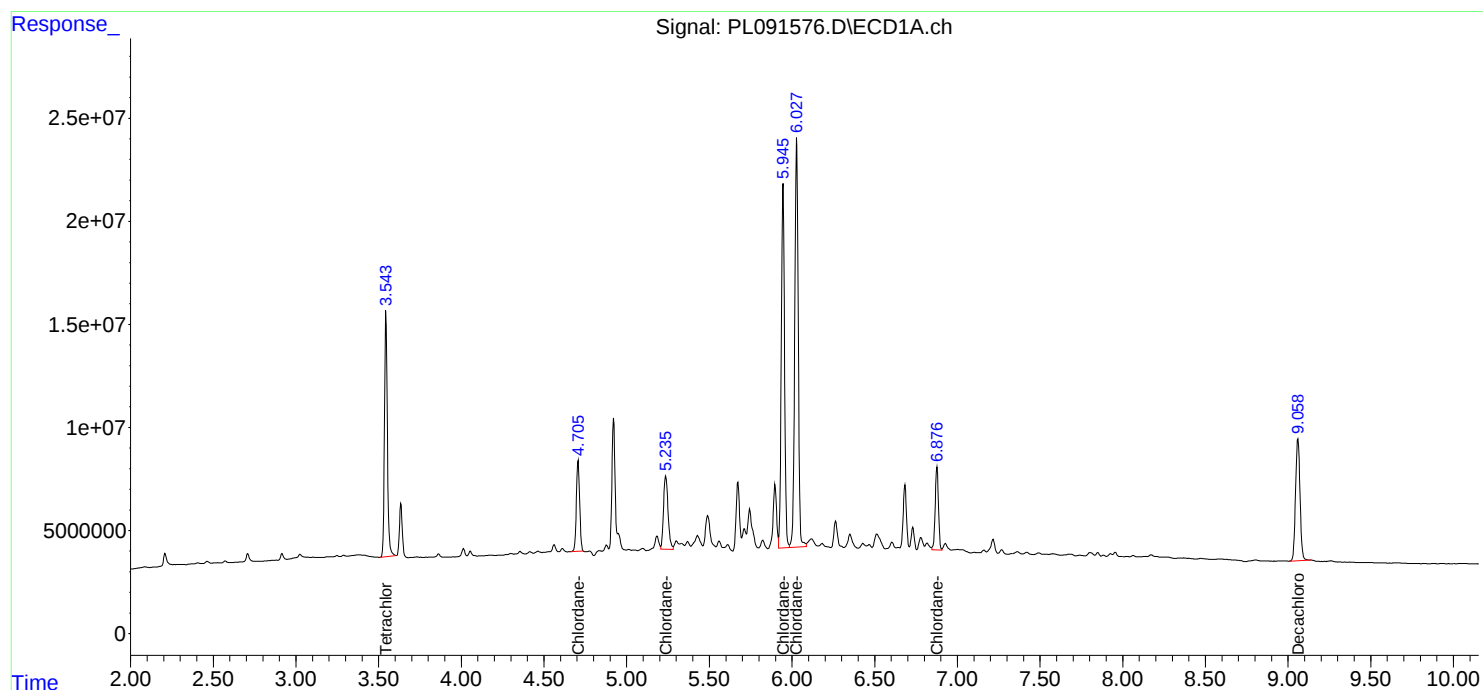


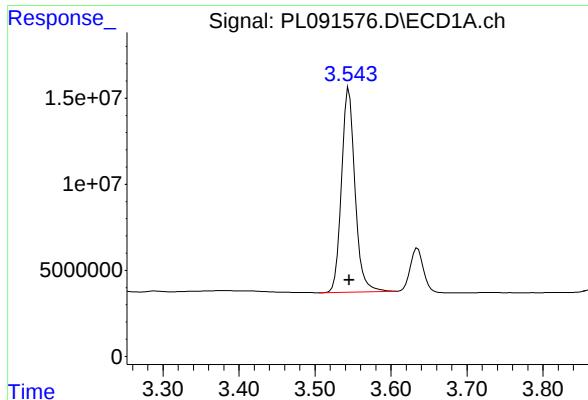

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 145375578
Conc: 99.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

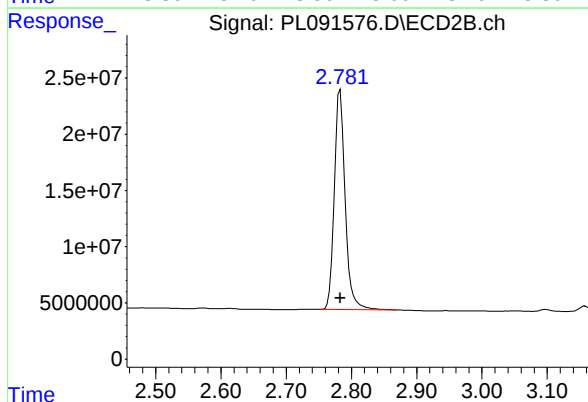


#1 Tetrachloro-m-xylene

R.T.: 2.783 min
Delta R.T.: 0.000 min
Response: 226151413
Conc: 100.84 ng/ml

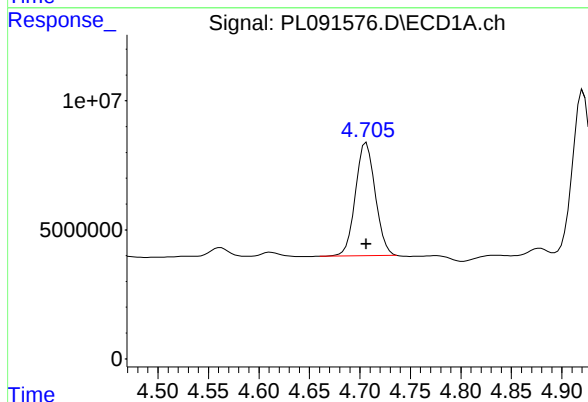


#23 Chlordane-1

R.T.: 4.706 min
Delta R.T.: 0.000 min
Response: 60104002
Conc: 989.12 ng/ml

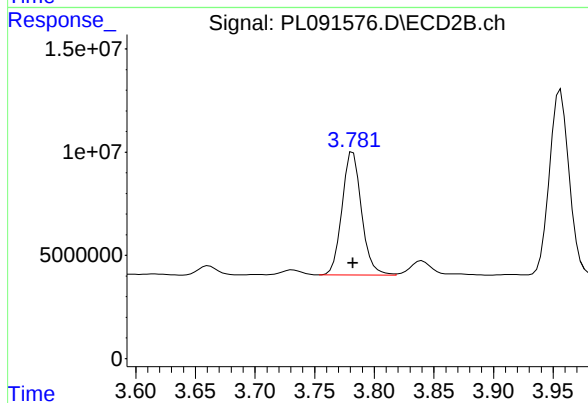

#23 Chlordane-1


R.T.: 3.782 min
Delta R.T.: 0.000 min
Response: 67613308
Conc: 1003.88 ng/ml

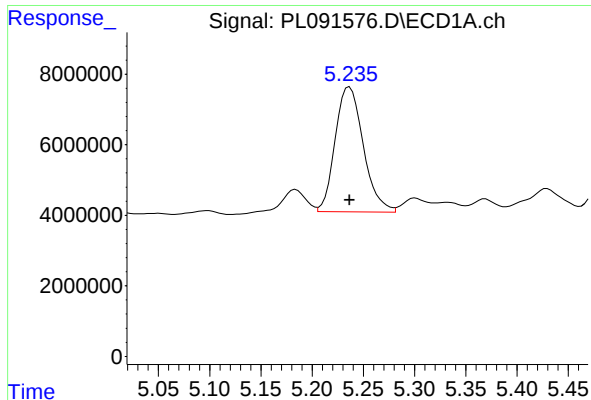

#24 Chlordane-2


R.T.: 5.237 min
Delta R.T.: 0.000 min
Response: 67677534
Conc: 957.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

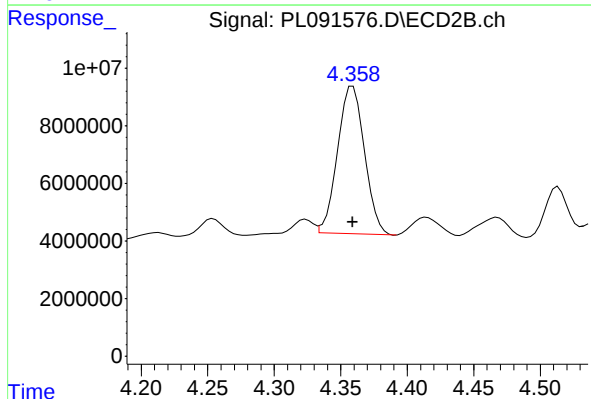


#24 Chlordane-2

R.T.: 4.359 min
Delta R.T.: 0.000 min
Response: 72257952
Conc: 995.70 ng/ml

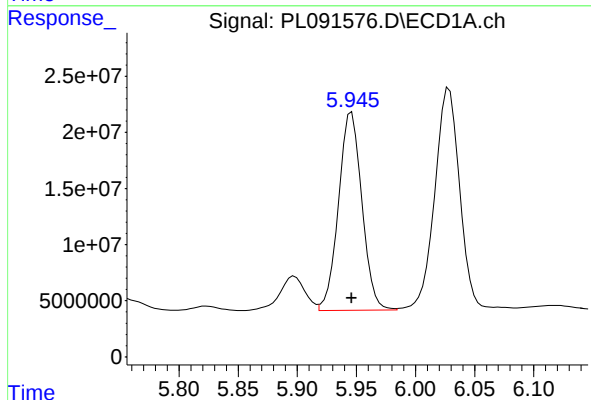


#25 Chlordane-3

R.T.: 5.946 min
Delta R.T.: 0.000 min
Response: 243077143
Conc: 995.90 ng/ml

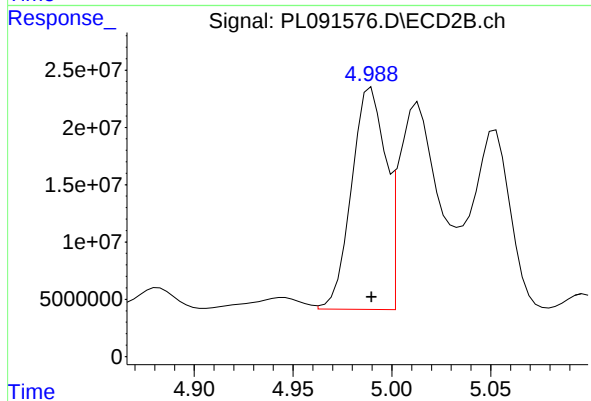

#25 Chlordane-3


R.T.: 4.990 min
Delta R.T.: 0.000 min
Response: 230321459
Conc: 1016.12 ng/ml

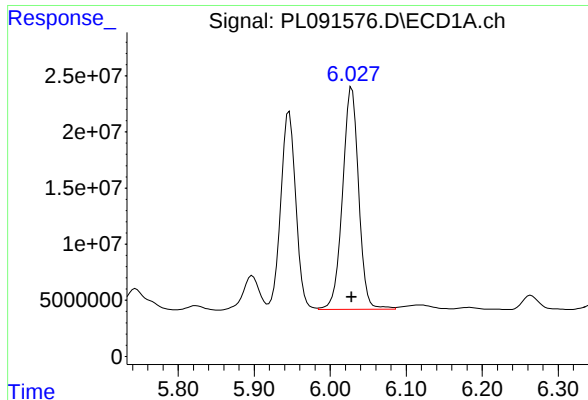

#26 Chlordane-4


R.T.: 6.028 min
Delta R.T.: 0.000 min
Response: 291650819
Conc: 997.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

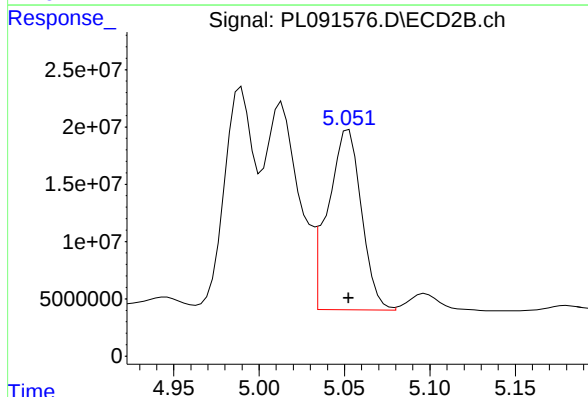


#26 Chlordane-4

R.T.: 5.052 min
Delta R.T.: 0.000 min
Response: 214746368
Conc: 1014.66 ng/ml

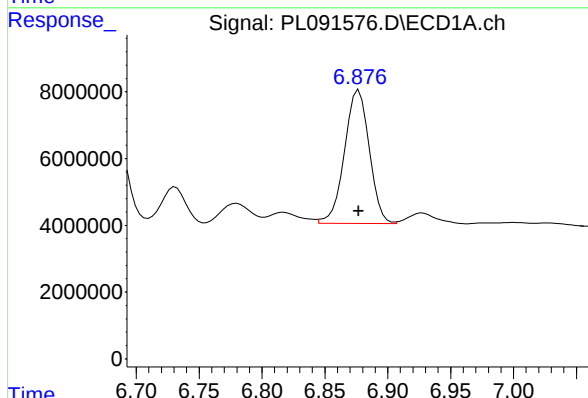


#27 Chlordane-5

R.T.: 6.877 min
Delta R.T.: 0.000 min
Response: 54634339
Conc: 984.77 ng/ml

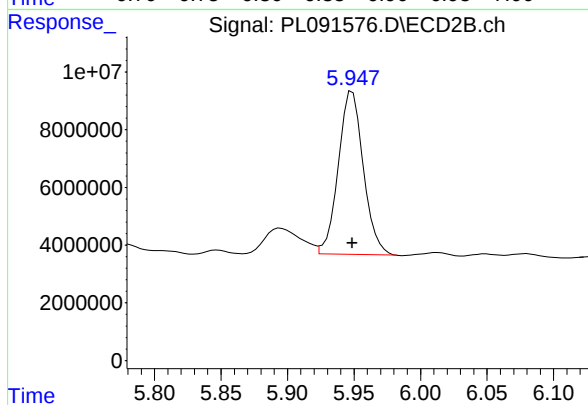

#27 Chlordane-5


R.T.: 5.949 min
Delta R.T.: 0.000 min
Response: 73932244
Conc: 1021.26 ng/ml

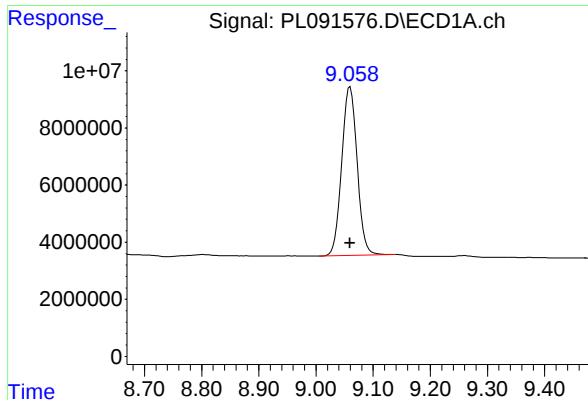

#28 Decachlorobiphenyl

R.T.: 9.060 min
Delta R.T.: 0.000 min
Response: 110886375
Conc: 97.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

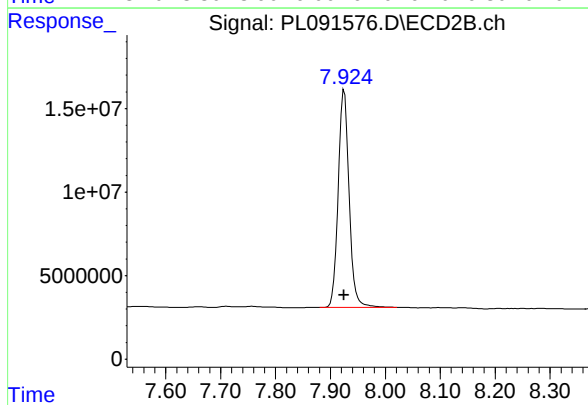

#28 Decachlorobiphenyl

R.T.: 7.925 min
Delta R.T.: 0.000 min
Response: 179513714
Conc: 99.22 ng/ml