


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091424\
Data File : BM047519.D
Acq On : 14 Sep 2024 11:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun Sep 15 08:56:37 2024

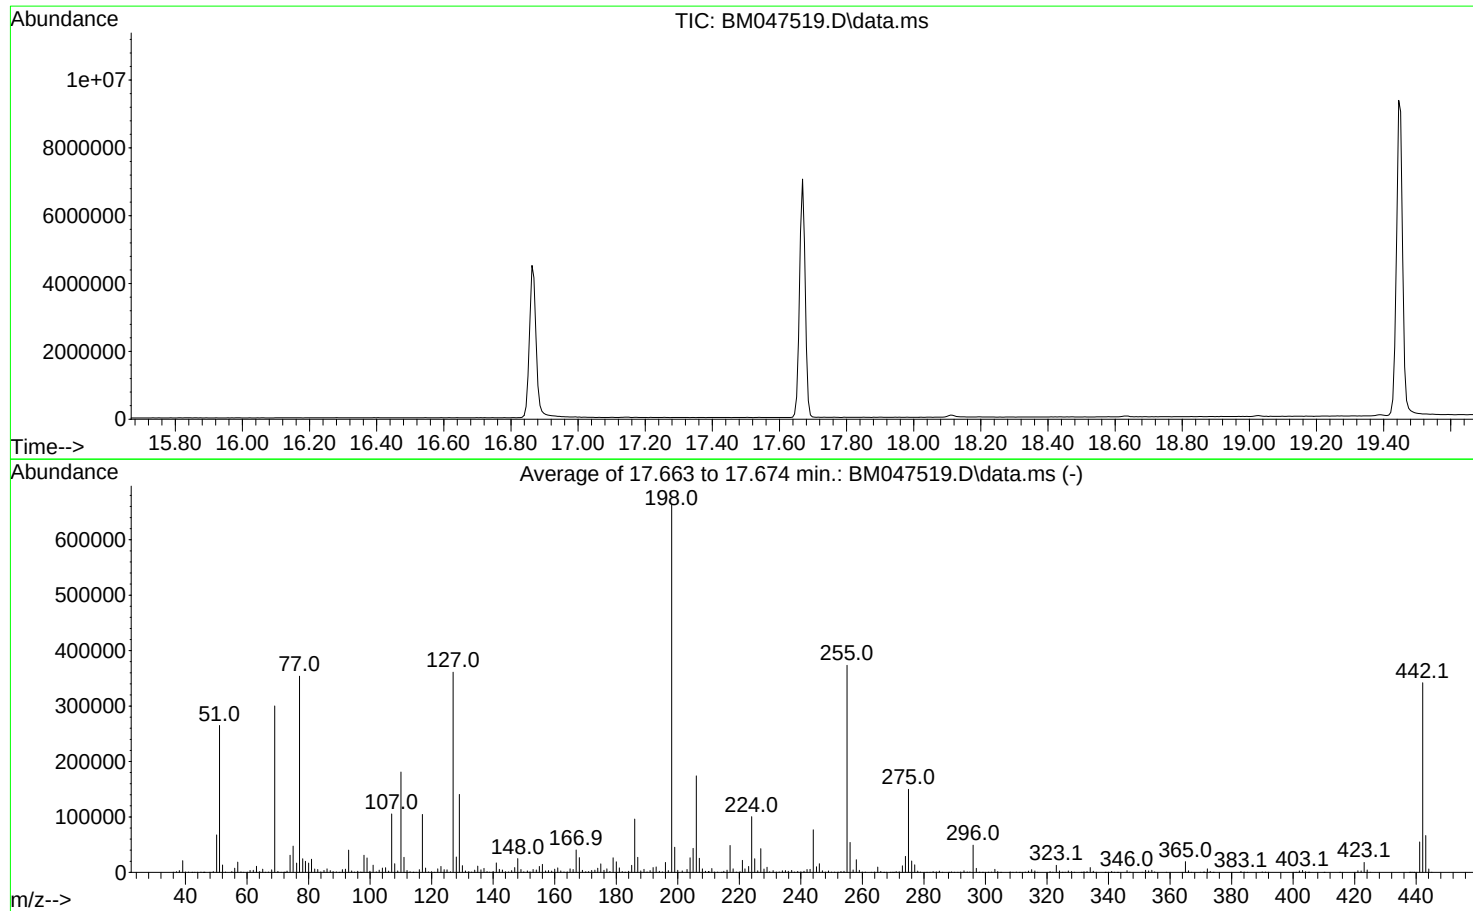




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	264866	PASS
68	69	0.00	2	1.5	4554	PASS
69	198	0.00	100	45.2	300217	PASS
70	69	0.00	2	0.6	1725	PASS
127	198	10	80	54.4	361109	PASS
197	198	0.00	2	0.5	3353	PASS
198	198	100	100	100.0	663616	PASS
199	198	5	9	6.8	45408	PASS
275	198	10	60	22.6	149971	PASS
365	198	1	100	2.9	19493	PASS
441	198	0.01	100	8.3	54813	PASS
442	442	50	100	100.0	341973	PASS
443	442	15	24	19.4	66293	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091424\
Data File : BM047519.D
Acq On : 14 Sep 2024 11:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 15 09:03:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 08:56:37 2024
Response via : Initial Calibration

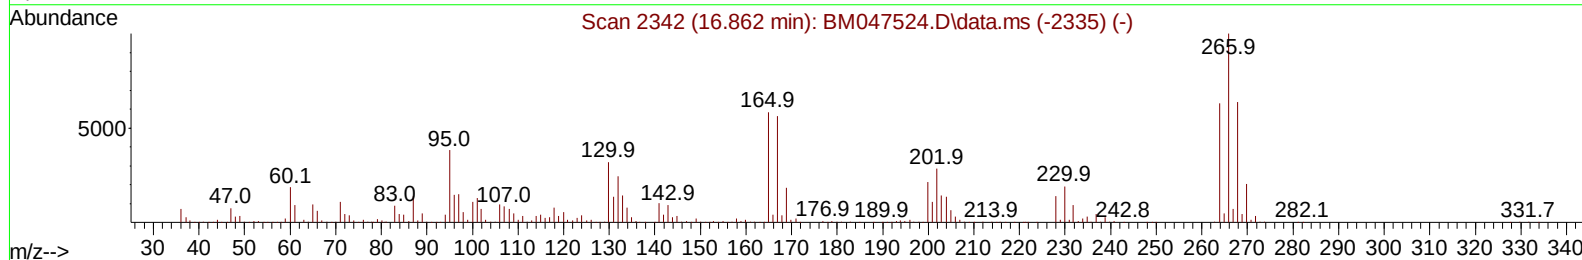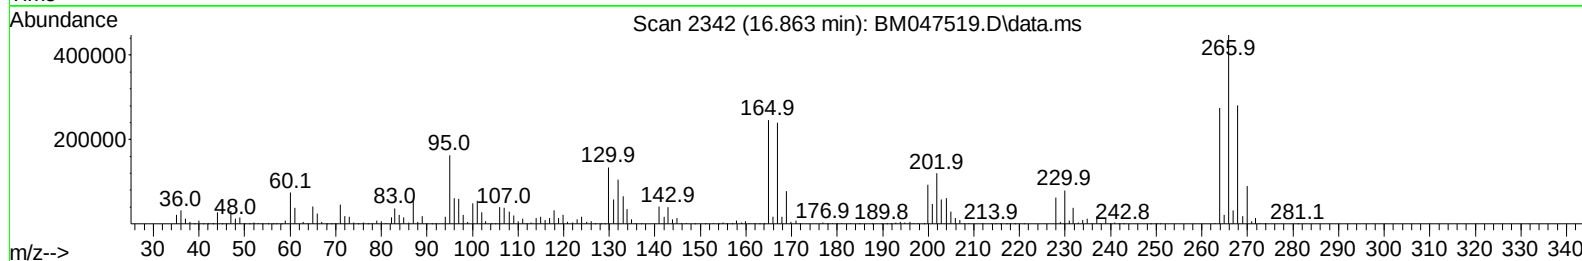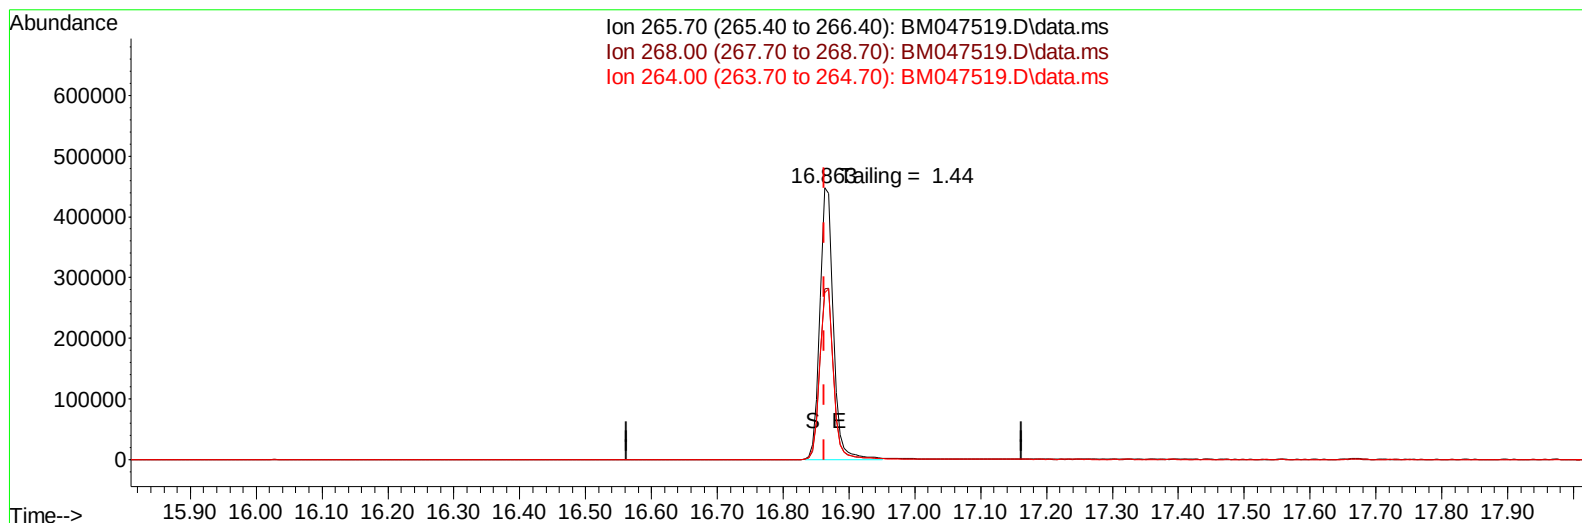

TIC: BM047519.D\data.ms

(70) Pentachlorophenol (C)

16.863min (+ 0.000) 149789.64 ng




response 629866

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.83
264.00	63.00	61.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091424\
 Data File : BM047519.D
 Acq On : 14 Sep 2024 11:17
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Sep 15 09:03:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 08:56:37 2024
 Response via : Initial Calibration

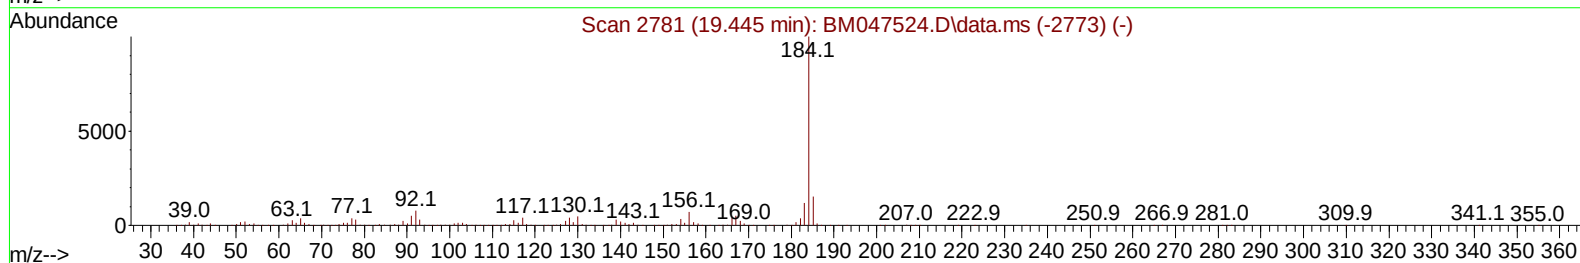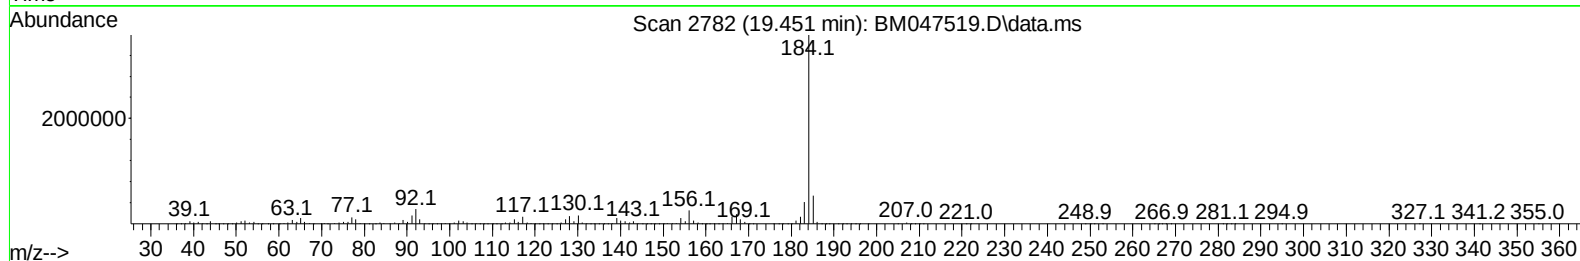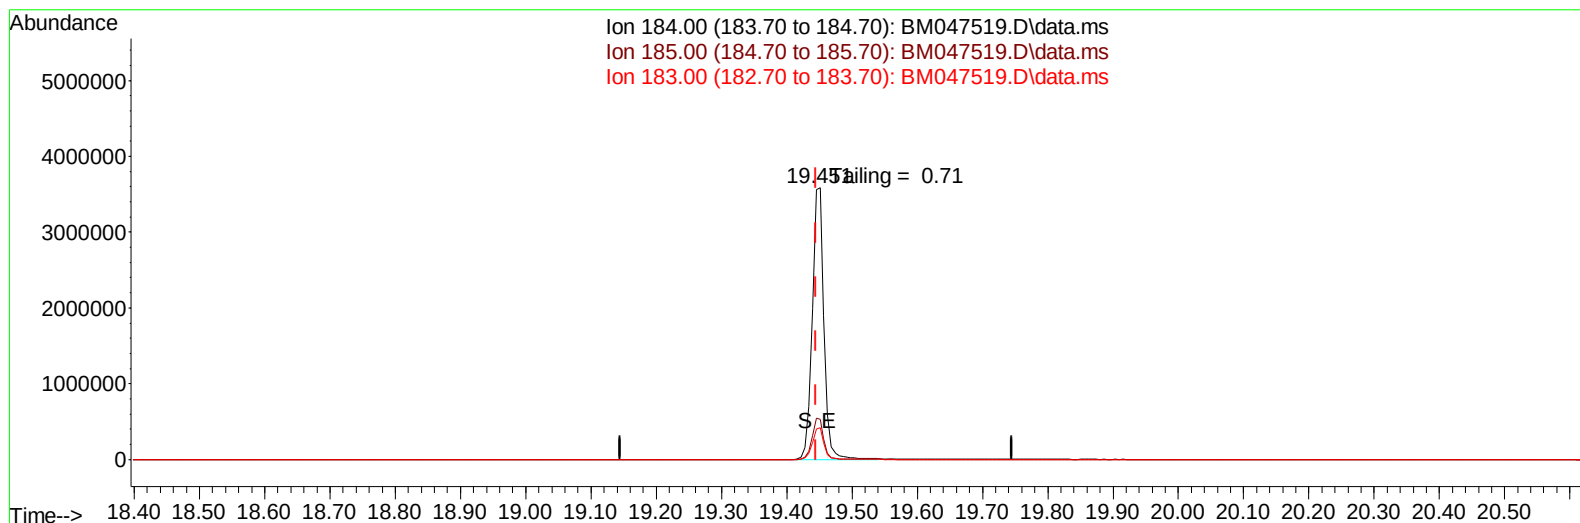

TIC: BM047519.D\data.ms

(77) Benzidine

19.451min (+ 0.006) 303907.69 ng

response 4609731

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.82
183.00	12.00	11.61
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/14/2024	BNA_M	<u>BM047519.D</u>
Compound Name	Response	Retention Time
DDT	2011863	20.686
DDD	13962	20.304
DDE	0	19.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13962	2025825	0.69

Instrument :
BNA_M
ClientSampleId :
DFTPP