


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091624\
Data File : BM047532.D
Acq On : 16 Sep 2024 09:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun Sep 15 08:56:37 2024

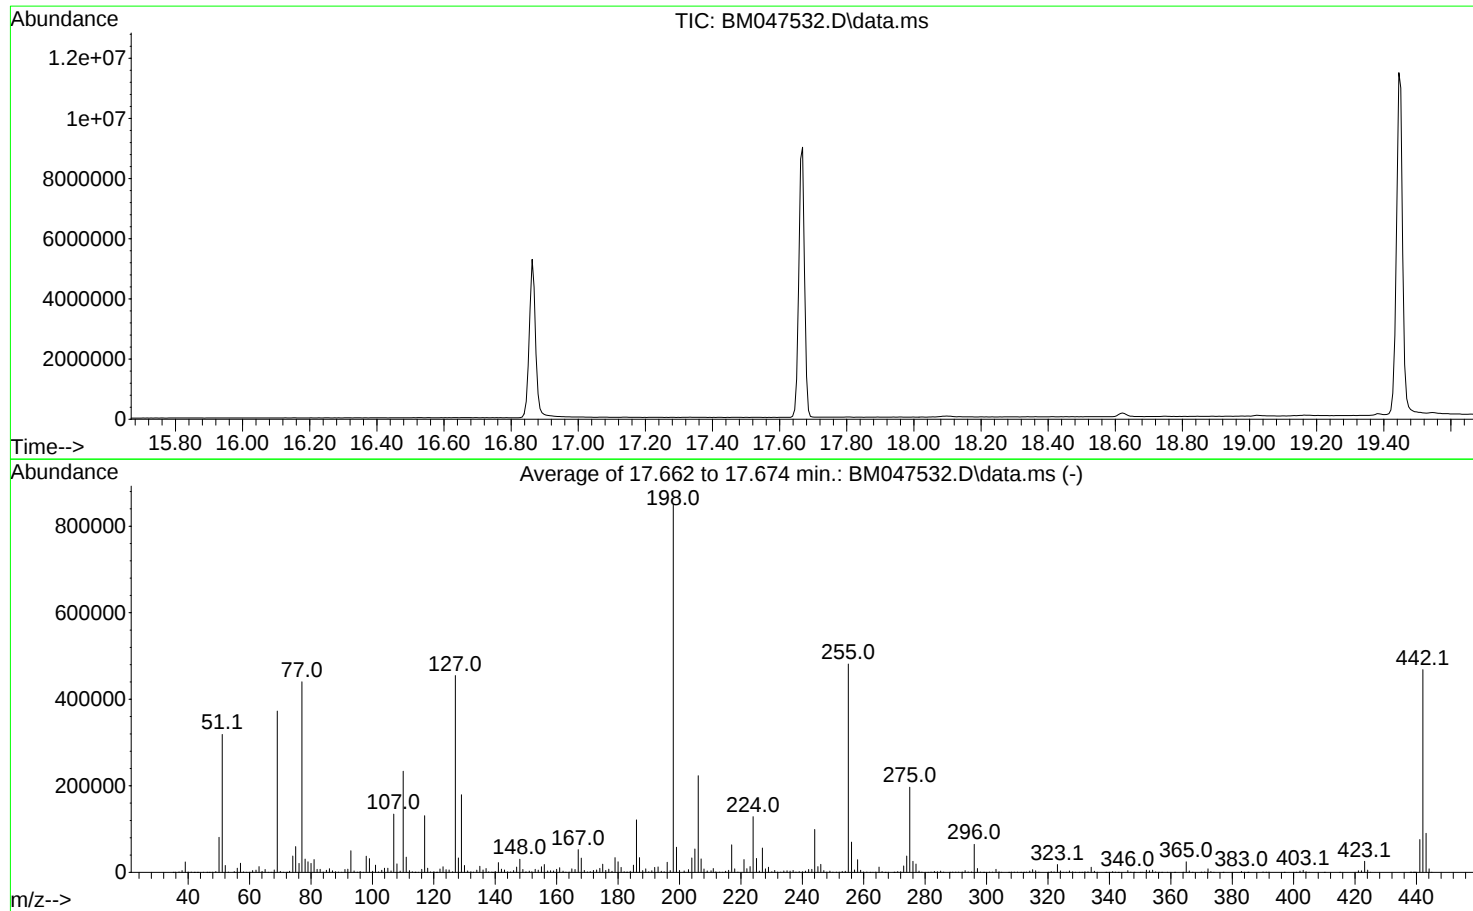




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	318753	PASS
68	69	0.00	2	1.5	5688	PASS
69	198	0.00	100	43.9	372949	PASS
70	69	0.00	2	0.5	2048	PASS
127	198	10	80	53.5	454912	PASS
197	198	0.00	2	0.5	3954	PASS
198	198	100	100	100.0	850133	PASS
199	198	5	9	6.8	58083	PASS
275	198	10	60	23.1	196757	PASS
365	198	1	100	2.9	24600	PASS
441	198	0.01	100	8.9	75757	PASS
442	442	50	100	100.0	468565	PASS
443	442	15	24	19.3	90395	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091624\
Data File : BM047532.D
Acq On : 16 Sep 2024 09:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 16 11:33:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 08:56:37 2024
Response via : Initial Calibration

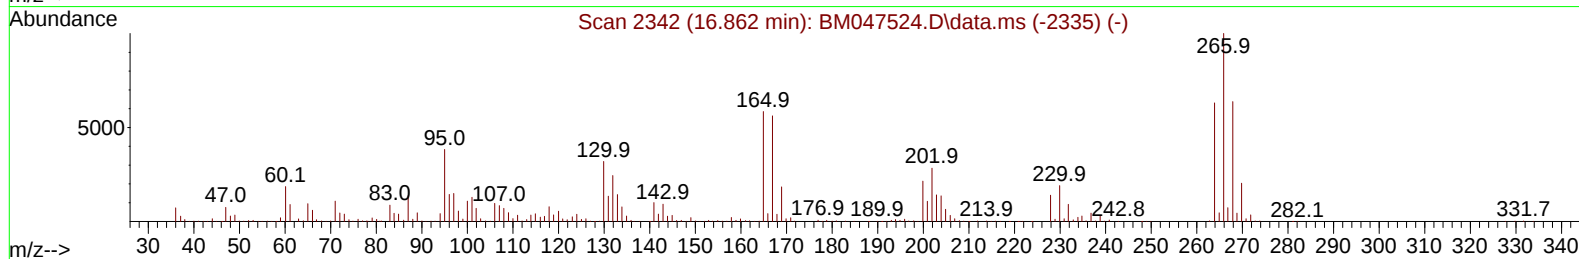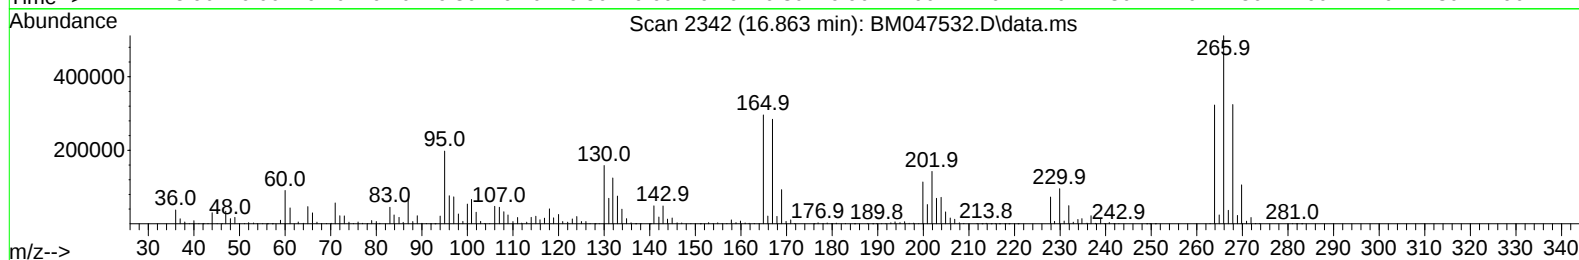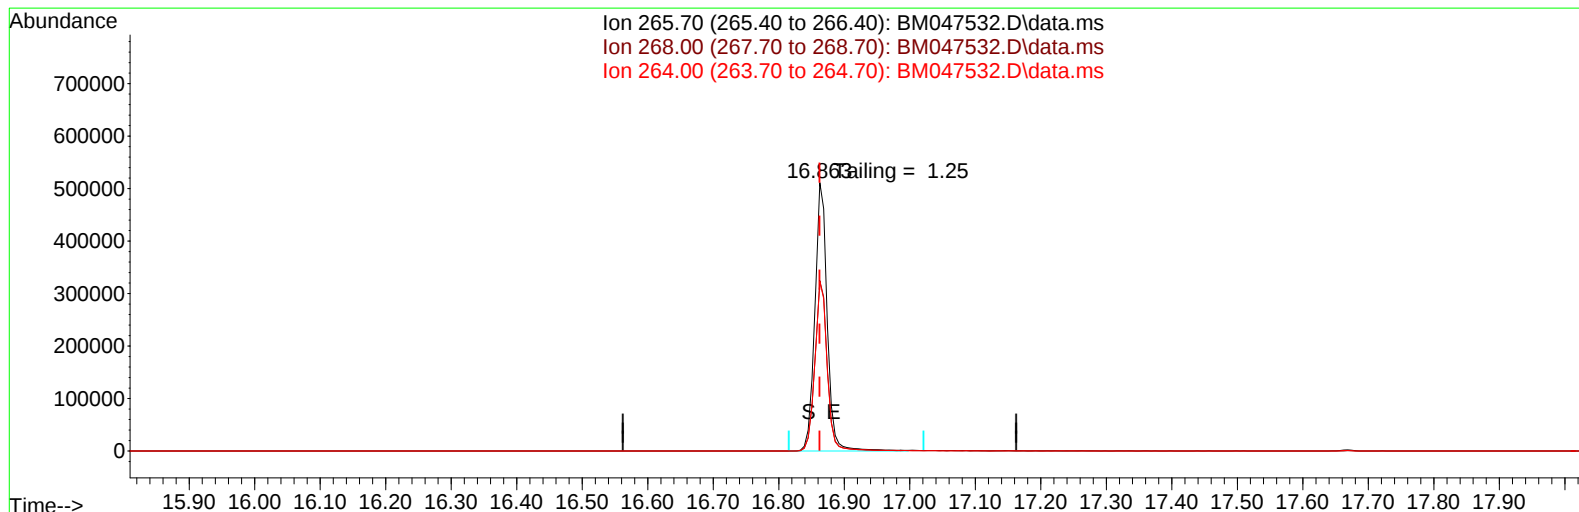

TIC: BM047532.D\data.ms

(70) Pentachlorophenol (C)

16.863min (+ 0.000) 1952988.49 ng




response 672937

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.45
264.00	63.00	63.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091624\
Data File : BM047532.D
Acq On : 16 Sep 2024 09:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 16 11:33:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 08:56:37 2024
Response via : Initial Calibration

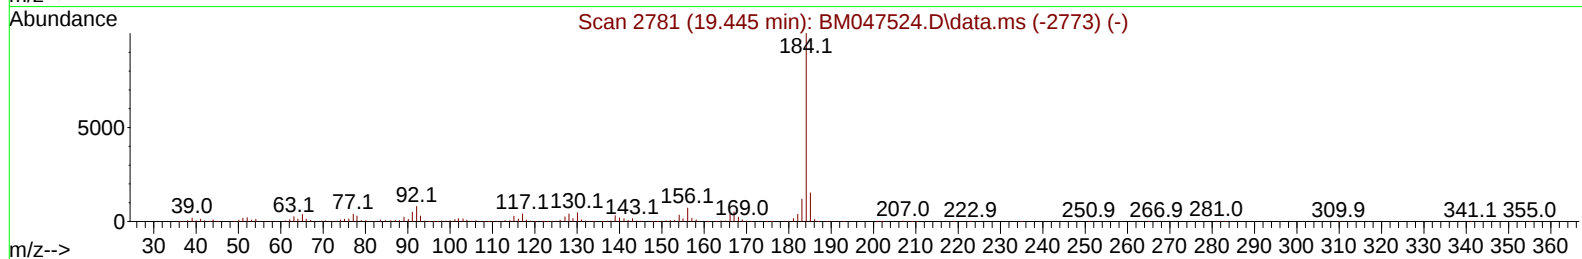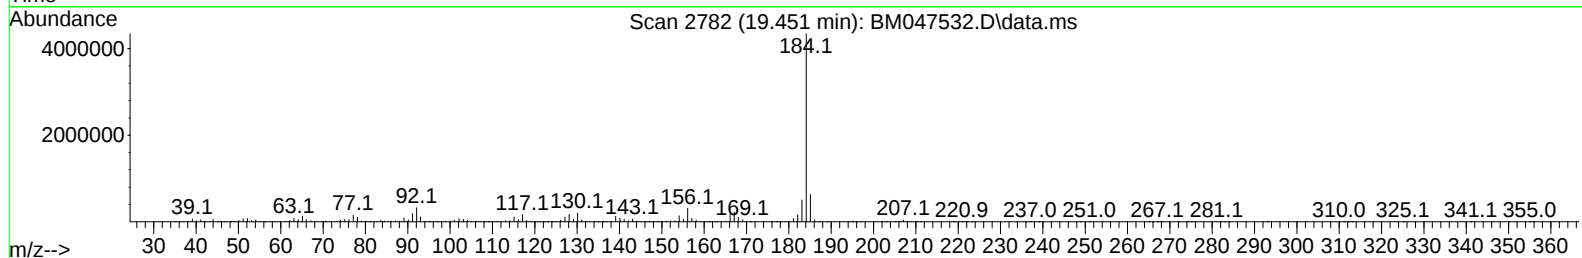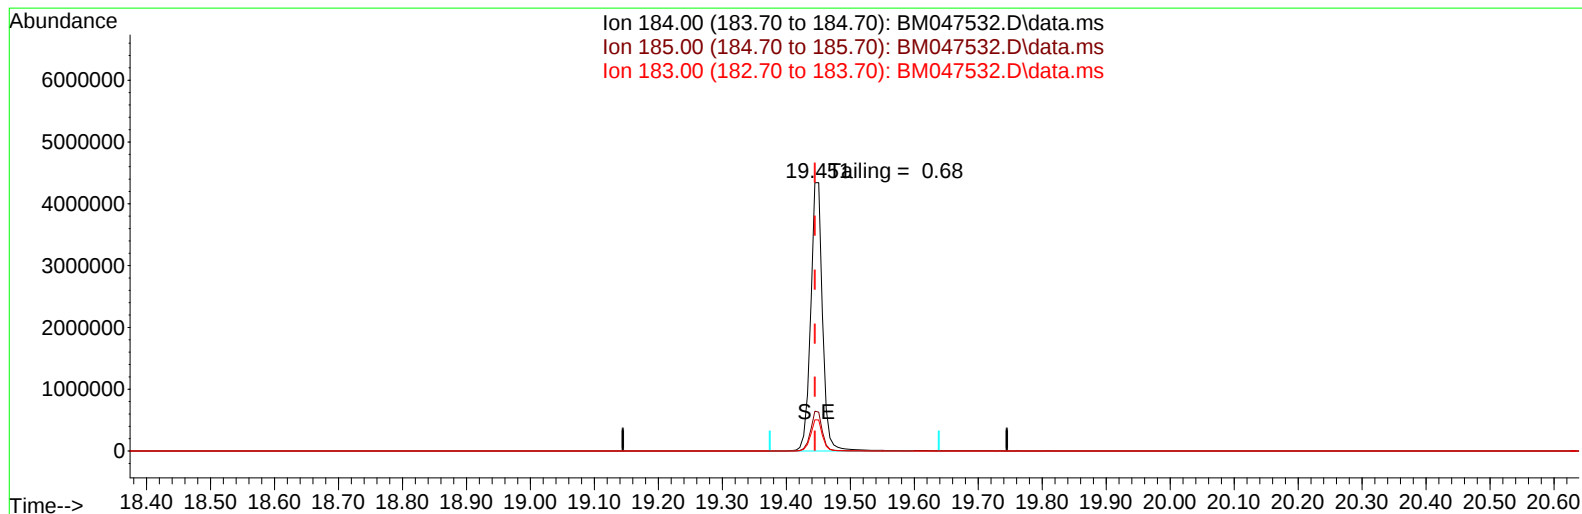

TIC: BM047532.D\data.ms

(77) Benzidine

19.451min (+ 0.006) 33612.78 ng

response 5649482

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.49
183.00	12.00	11.57
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/16/2024	BNA_M	<u>BM047532.D</u>
Compound Name	Response	Retention Time
DDT	2268067	20.686
DDD	25450	20.245
DDE	3522	19.739
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28972	2297039	1.26

Instrument :
BNA_M
ClientSampleId :
DFTPP