


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091924\
Data File : BM047565.D
Acq On : 19 Sep 2024 08:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun Sep 15 08:56:37 2024

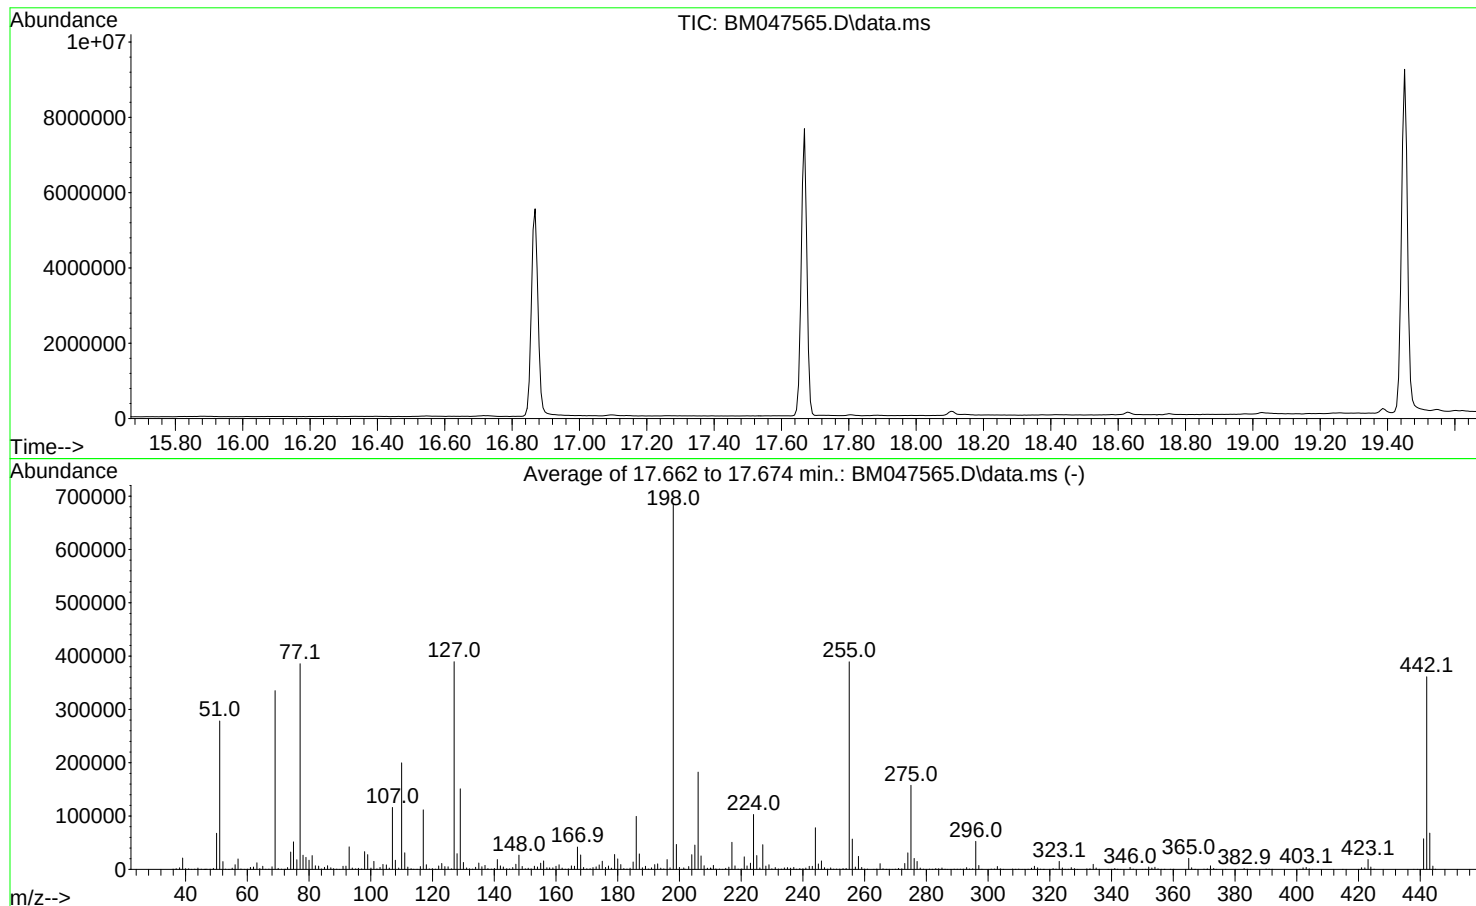




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	278274	PASS
68	69	0.00	2	1.5	4882	PASS
69	198	0.00	100	48.9	335179	PASS
70	69	0.00	2	0.6	1919	PASS
127	198	10	80	56.8	389461	PASS
197	198	0.00	2	0.4	2928	PASS
198	198	100	100	100.0	685845	PASS
199	198	5	9	6.8	46739	PASS
275	198	10	60	23.0	157611	PASS
365	198	1	100	3.0	20608	PASS
441	198	0.01	100	8.4	57341	PASS
442	442	50	100	100.0	361152	PASS
443	442	15	24	18.8	68013	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091924\
 Data File : BM047565.D
 Acq On : 19 Sep 2024 08:54
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Sep 19 12:50:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 08:56:37 2024
 Response via : Initial Calibration

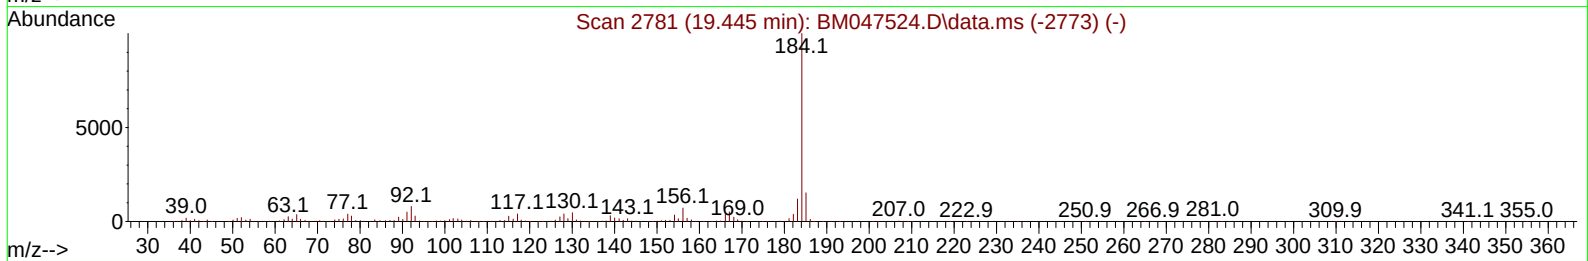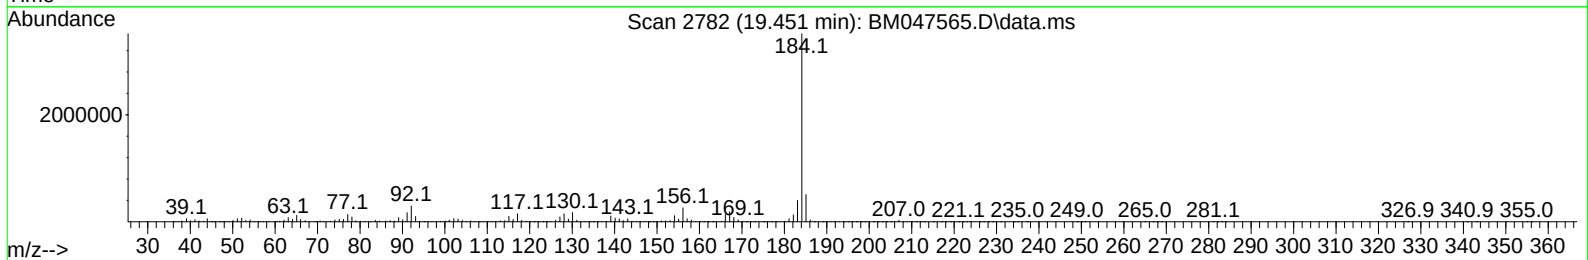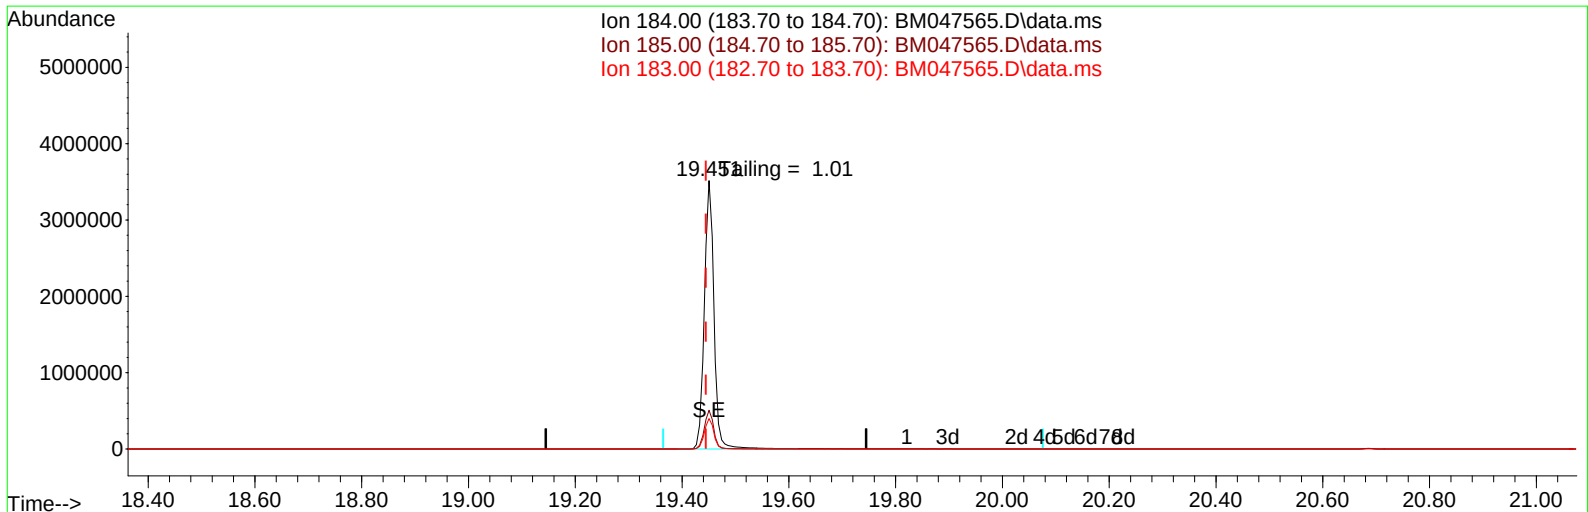

TIC: BM047565.D\data.ms

(77) Benzdine

19.451min (+ 0.006) 2160538.53 ng m

response 4472986

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.44
183.00	12.00	11.35
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/19/2024	BNA_M	<u>BM047565.D</u>
Compound Name	Response	Retention Time
DDT	1796898	20.686
DDD	111808	20.245
DDE	3650	19.745
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
115458	1912356	6.04

Instrument :
BNA_M
ClientSampleId :
DFTPP