
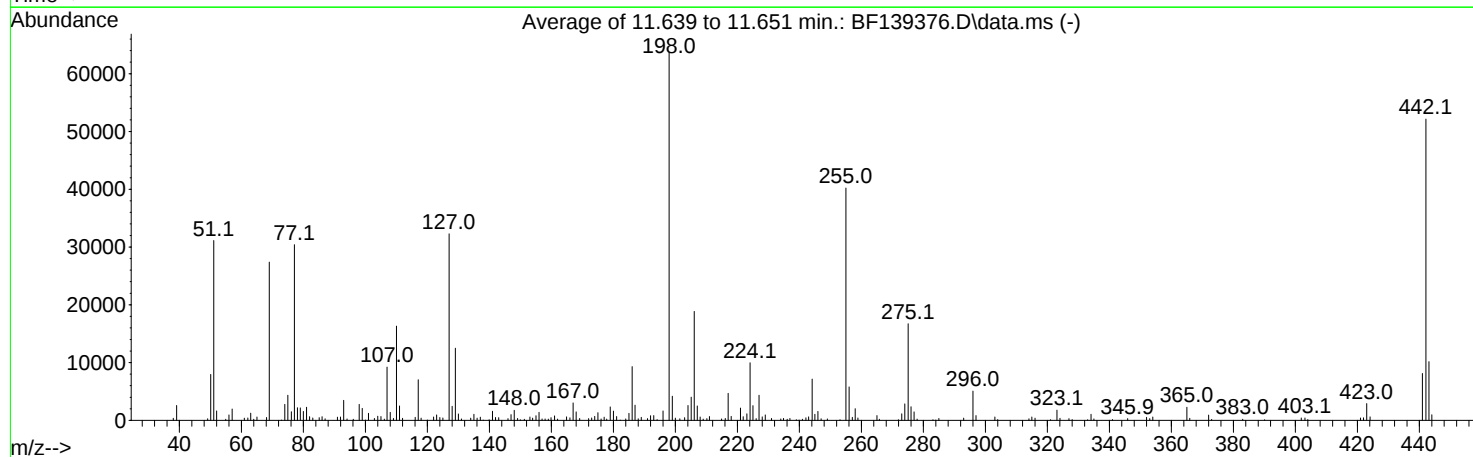


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091624\
Data File : BF139376.D
Acq On : 16 Sep 2024 10:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Sep 14 02:58:23 2024

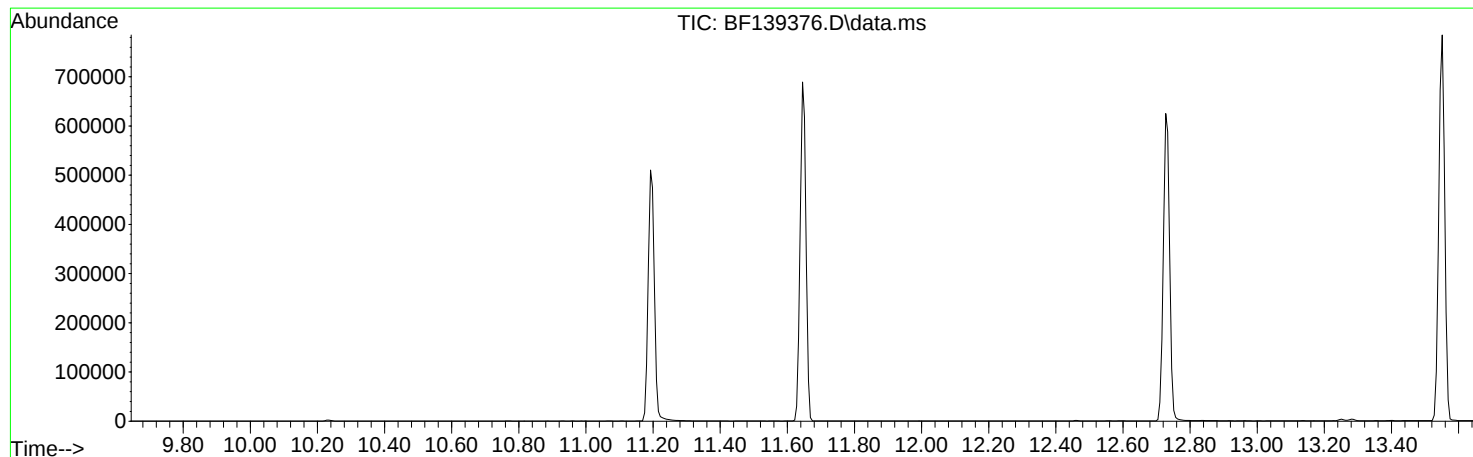




AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.9	31123	PASS
68	69	0.00	2	1.8	503	PASS
69	198	0.00	100	43.0	27395	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.7	32280	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	63672	PASS
199	198	5	9	6.6	4197	PASS
275	198	10	60	26.3	16737	PASS
365	198	1	100	3.6	2271	PASS
441	198	0.01	100	12.7	8118	PASS
442	442	50	100	100.0	52165	PASS
443	442	15	24	19.5	10168	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091624\  
Data File : BF139376.D  
Acq On    : 16 Sep 2024  10:09  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 16 11:15:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

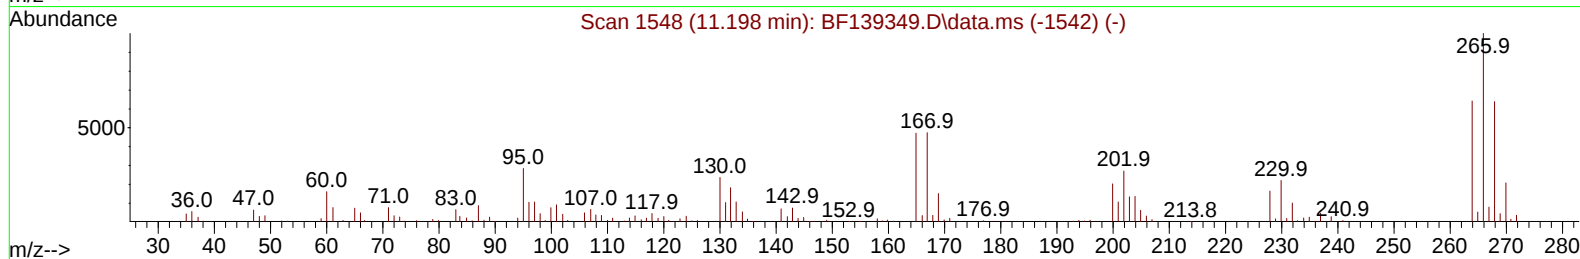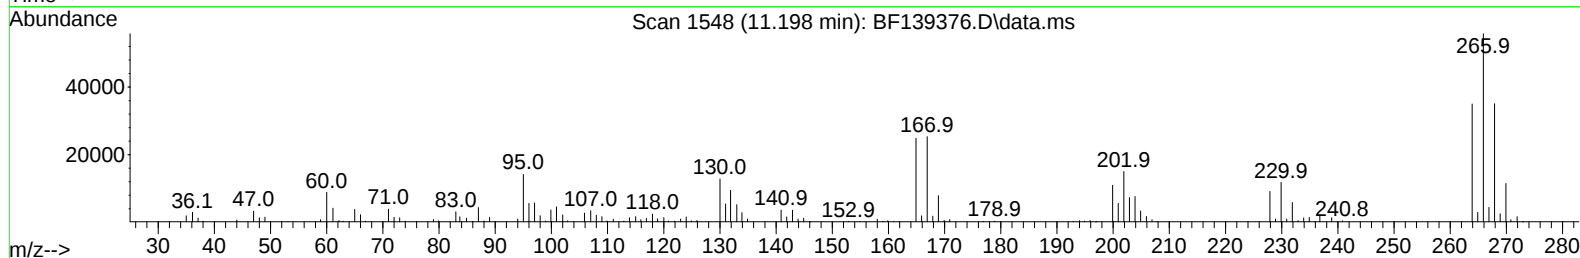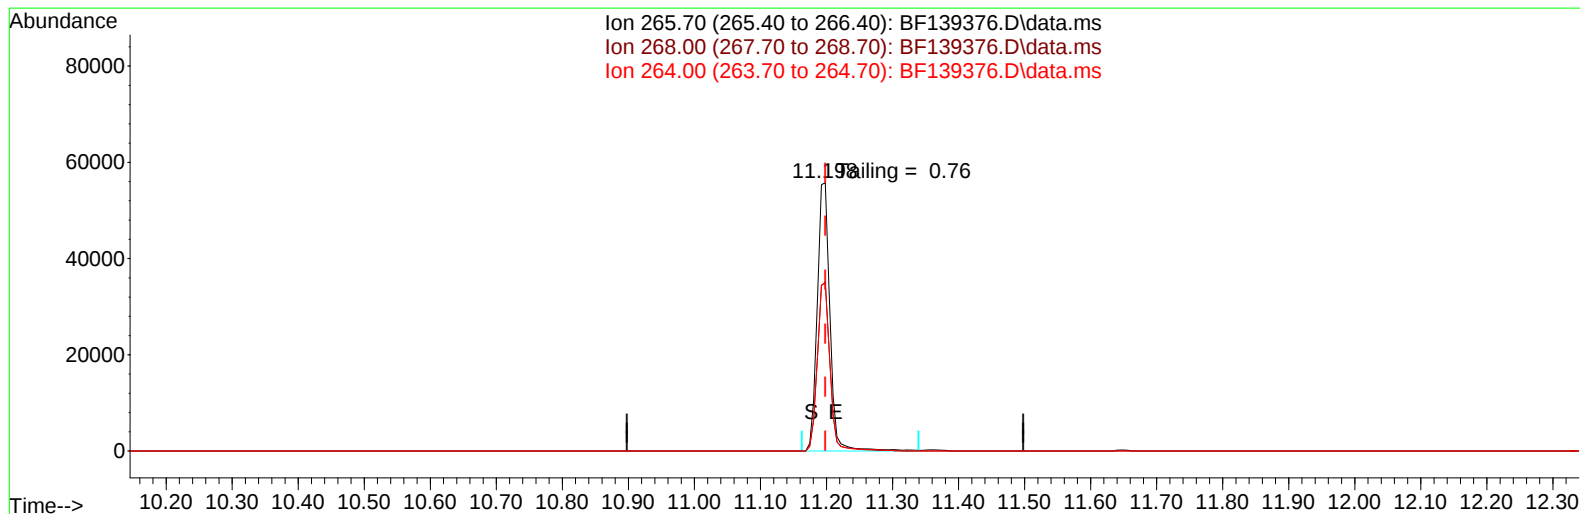

TIC: BF139376.D\data.ms

(70) Pentachlorophenol (C)

11.198min (0.000) 35373.17 ng




response **74798**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	62.89
264.00	64.20	62.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091624\
Data File : BF139376.D
Acq On : 16 Sep 2024 10:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 16 11:15:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

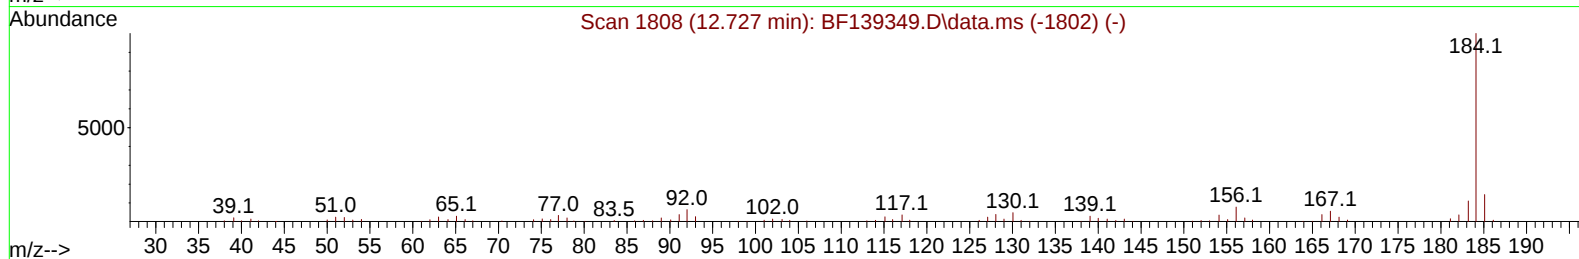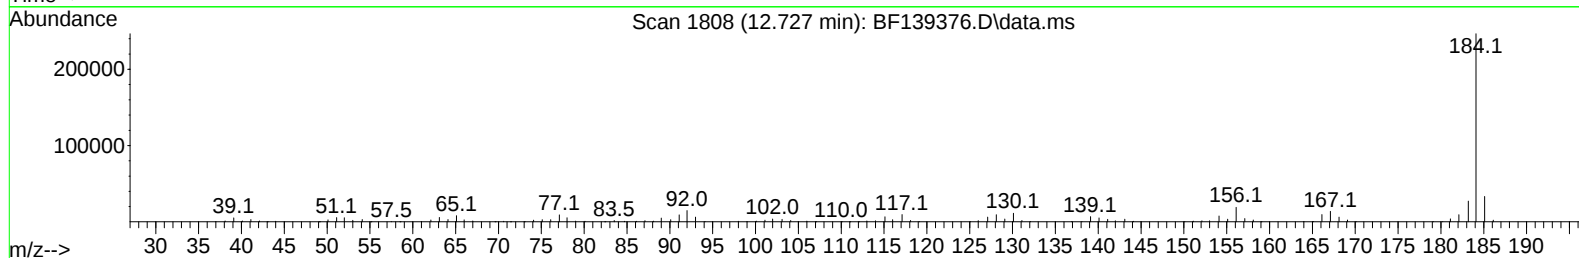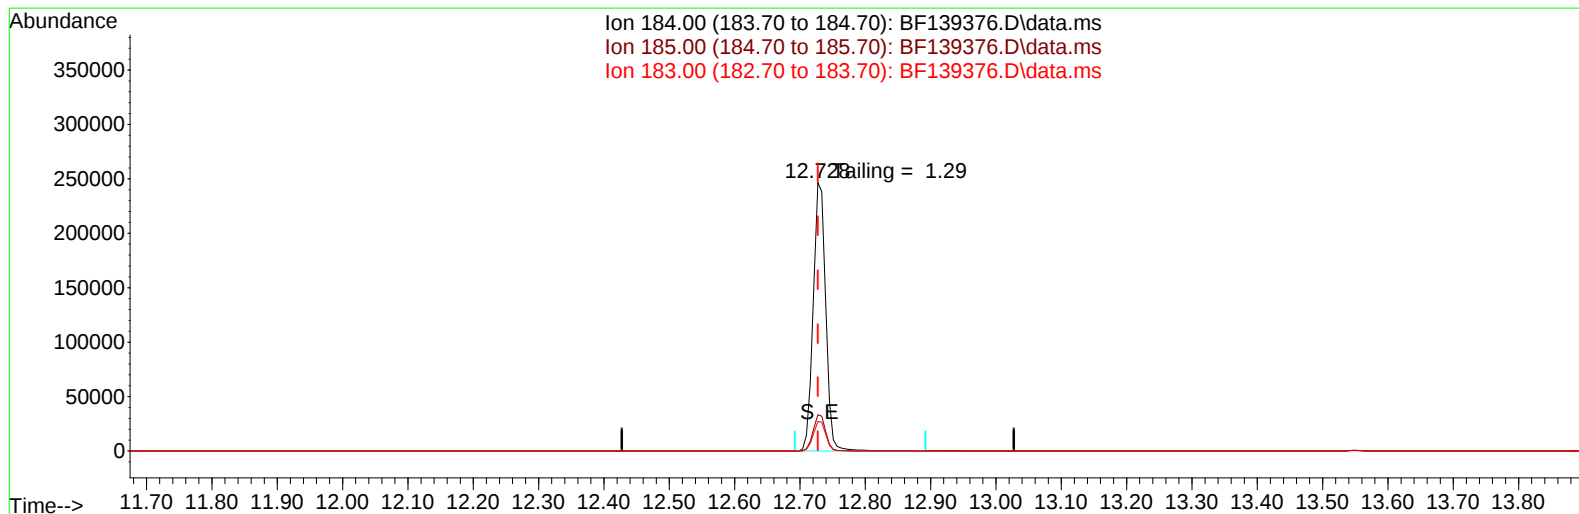

TIC: BF139376.D\data.ms

(77) Benzidine

12.727min (0.000) 0.00 ng

response 330188

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.54
183.00	11.10	11.05
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/16/2024	BNA_F	<u>BF139376.D</u>
Compound Name	Response	Retention Time
DDT	183313	13.551
DDD	2677	13.251
DDE	59	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2736	186049	1.47

Instrument :
BNA_F
ClientSampleId :
DFTPP