
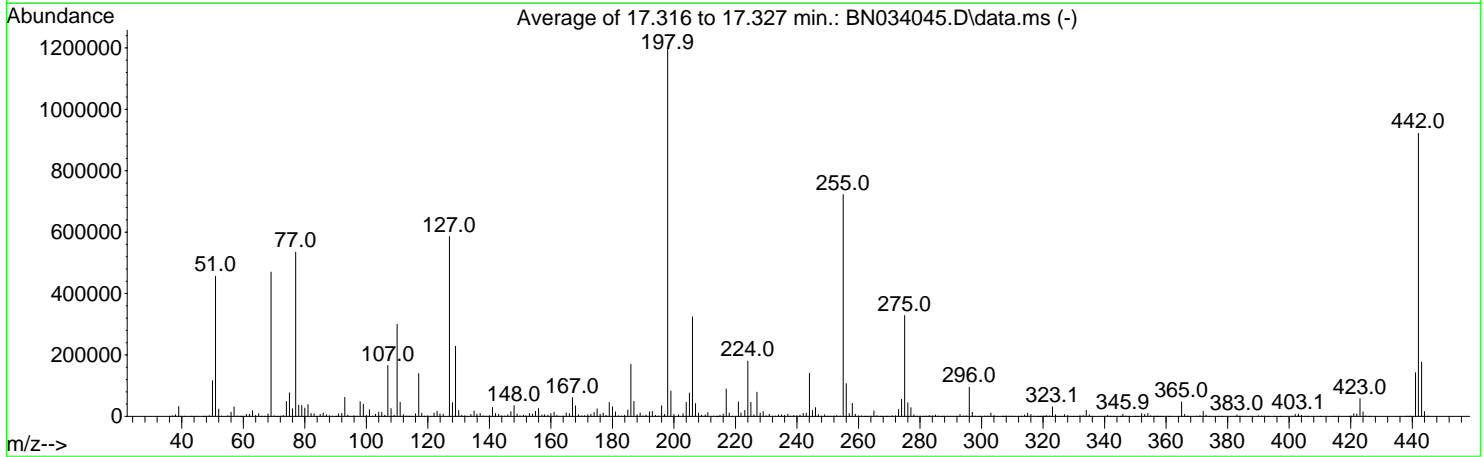


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091924\
 Data File : BN034045.D
 Acq On : 19 Sep 2024 08:54
 Operator : JU/RC
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 18 16:09:28 2024

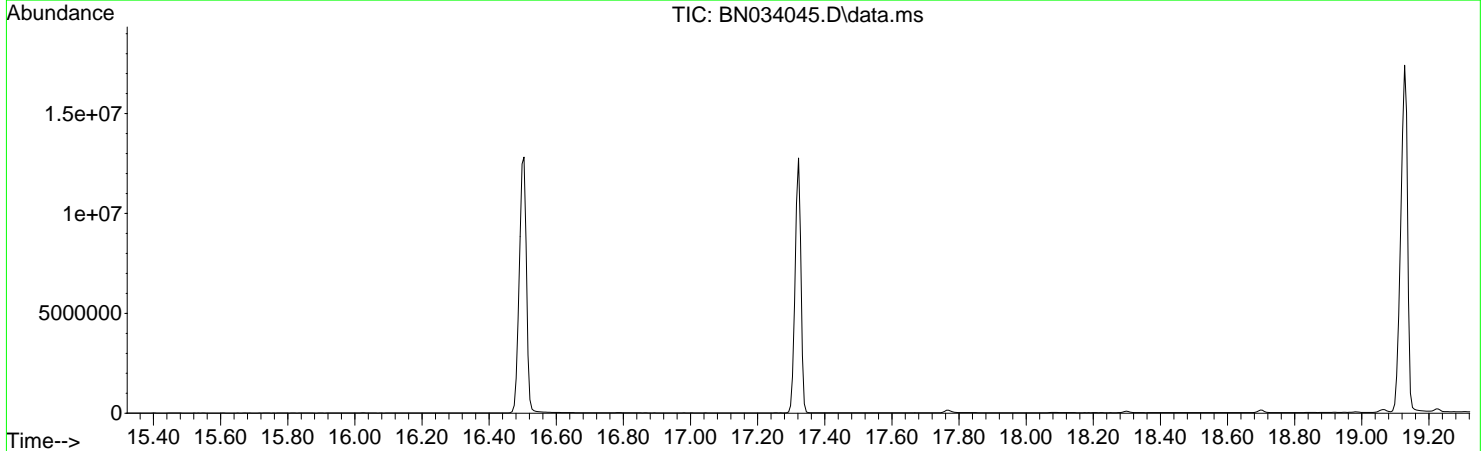




AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	456356	PASS
68	69	0.00	2	1.6	7706	PASS
69	198	0.00	100	39.2	470107	PASS
70	69	0.00	2	0.5	2262	PASS
127	198	10	80	48.9	585600	PASS
197	198	0.00	2	0.5	6379	PASS
198	198	100	100	100.0	1198187	PASS
199	198	5	9	6.9	82589	PASS
275	198	10	60	27.4	328149	PASS
365	198	1	100	3.9	46936	PASS
441	198	0.01	100	11.9	142091	PASS
442	442	50	100	100.0	921941	PASS
443	442	15	24	19.2	176675	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091924\
 Data File : BN034045.D
 Acq On : 19 Sep 2024 08:54
 Operator : JU/RC
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 20 04:53:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 20 04:53:44 2024
 Response via : Initial Calibration

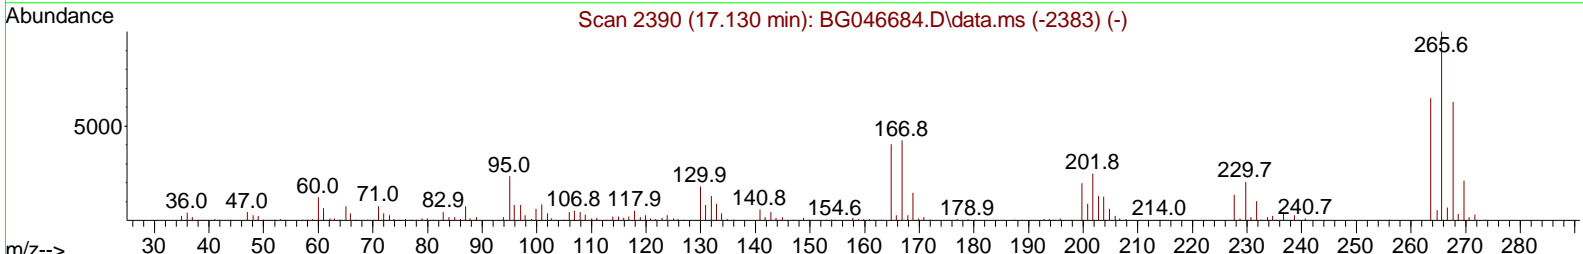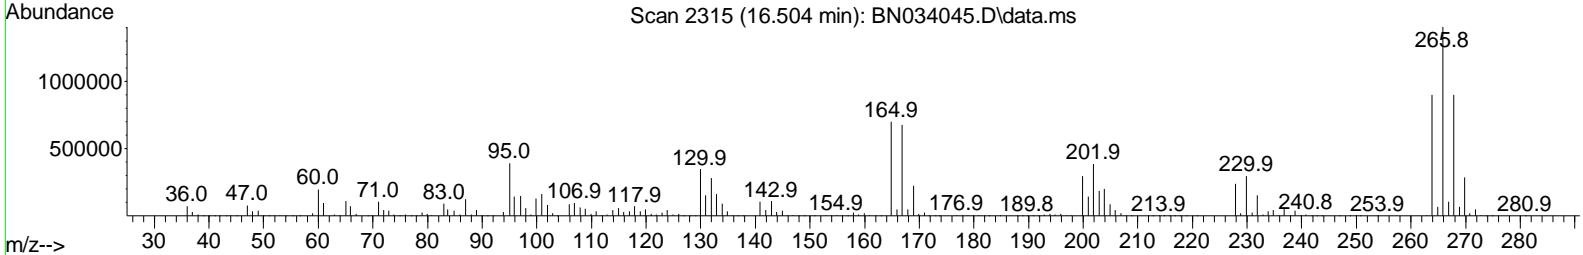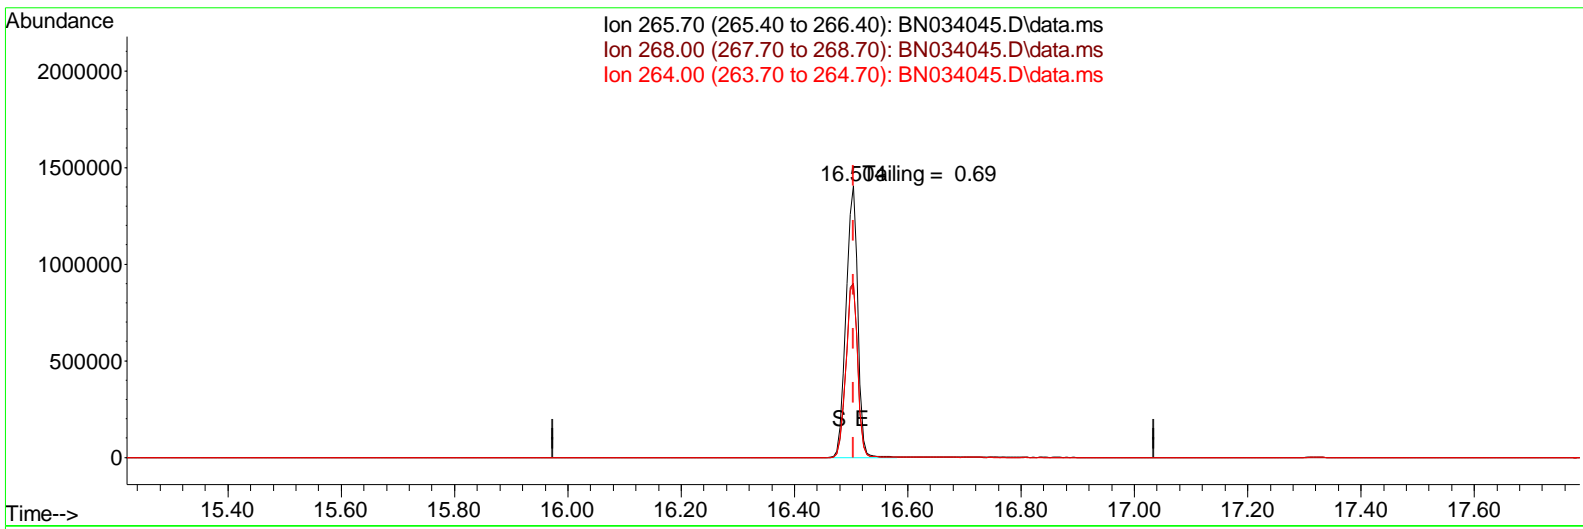

TIC: BN034045.D\data.ms

(70) Pentachlorophenol (C)

16.504min (0.000) 33339.48 ng




response 2034773

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.08
264.00	61.60	63.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091924\
 Data File : BN034045.D
 Acq On : 19 Sep 2024 08:54
 Operator : JU/RC
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 DFTPP

Quant Time: Sep 20 04:53:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 20 04:53:44 2024
 Response via : Initial Calibration

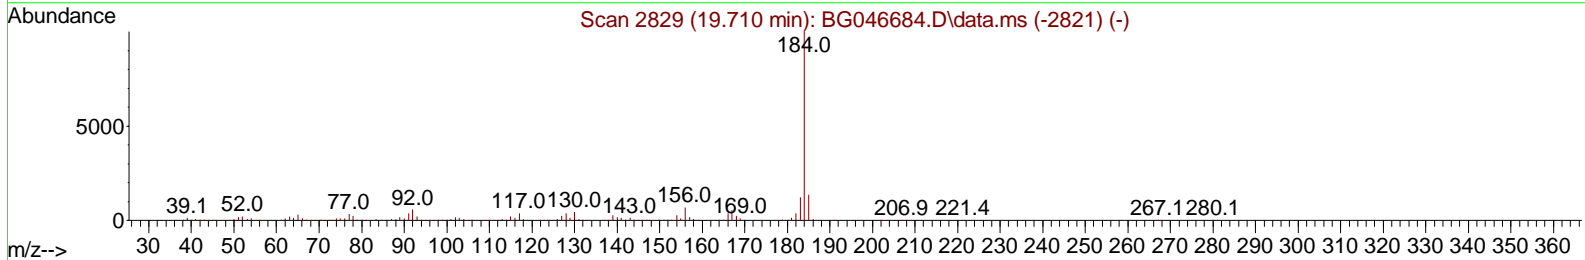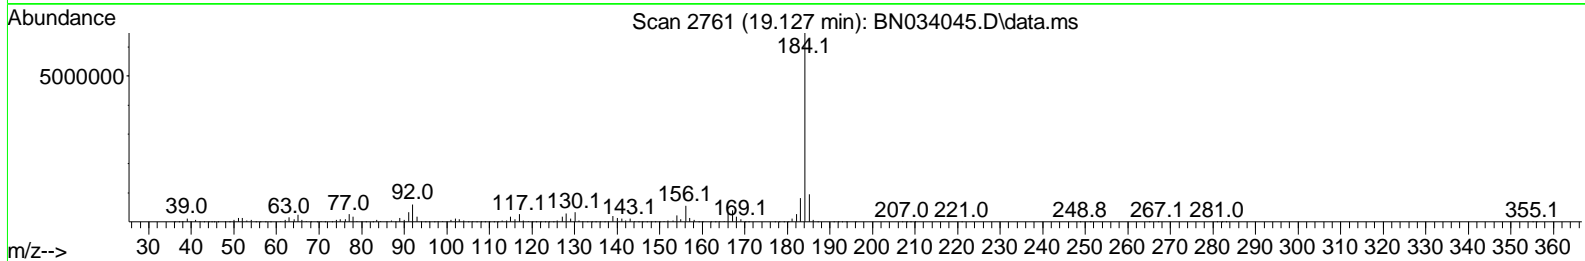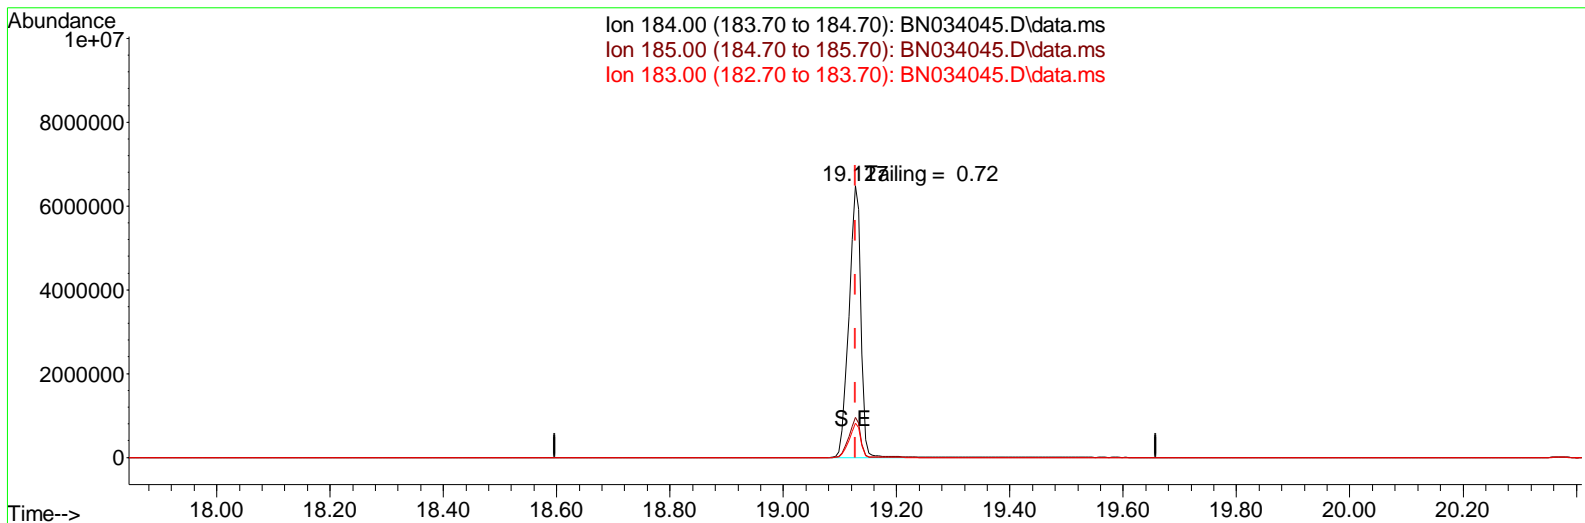

TIC: BN034045.D\data.ms

(77) Benzidine

19.127min (0.000) 0.00 ng

response 9558562

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.69
183.00	13.20	12.59
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/19/2024	BNA_N	<u>BN034045.D</u>
Compound Name	Response	Retention Time
DDT	4367080	20.374
DDD	37662	19.974
DDE	195	19.416
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
37857	4404937	0.86

Instrument :
 BNA_N
 ClientSampled :
 DFTPP