
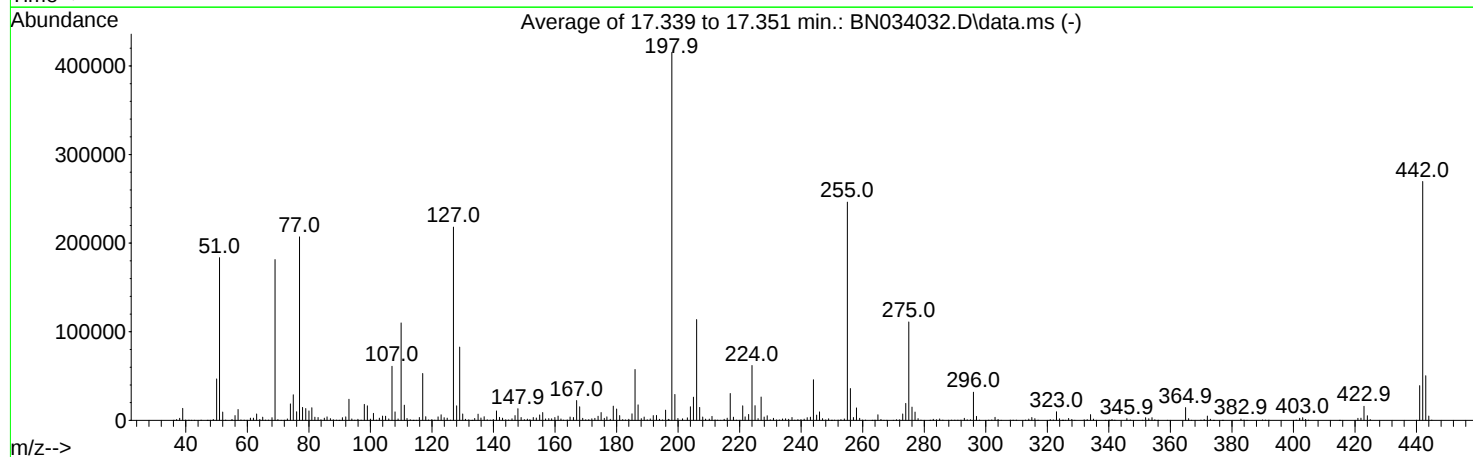


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091924\
Data File : BN034032.D
Acq On : 18 Sep 2024 08:34
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 18 16:09:28 2024

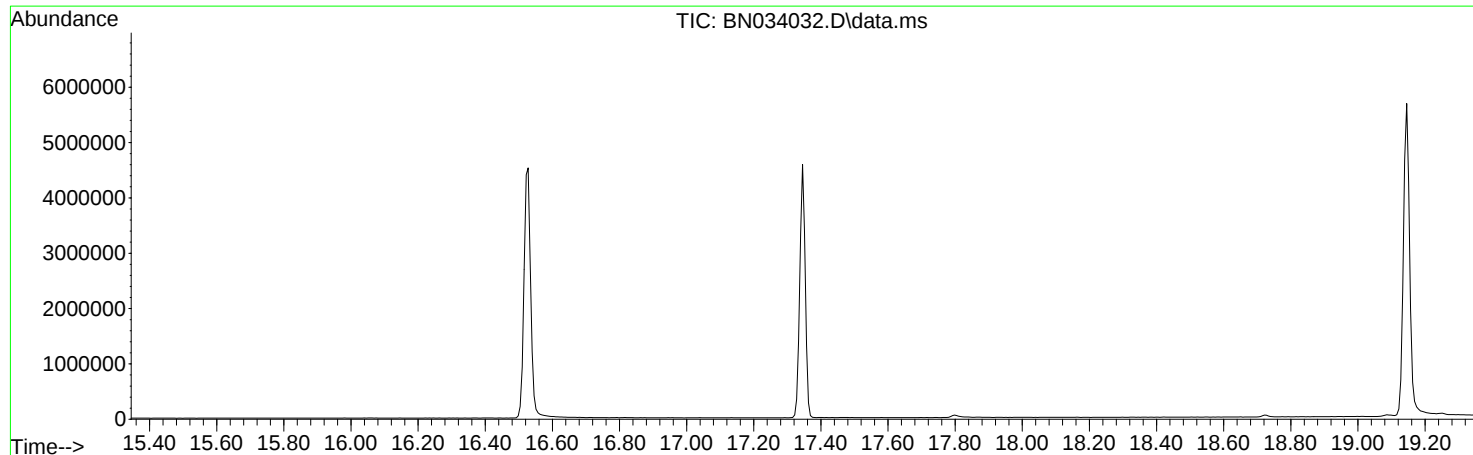




AutoFind: Scans 2440, 2441, 2442; Background Corrected with Scan 2433

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.2	183645	PASS
68	69	0.00	2	1.7	3129	PASS
69	198	0.00	100	43.7	181547	PASS
70	69	0.00	2	0.5	929	PASS
127	198	10	80	52.6	218219	PASS
197	198	0.00	2	0.3	1234	PASS
198	198	100	100	100.0	415168	PASS
199	198	5	9	7.0	29256	PASS
275	198	10	60	26.8	111072	PASS
365	198	1	100	3.5	14476	PASS
441	198	0.01	100	9.4	39211	PASS
442	442	50	100	100.0	269675	PASS
443	442	15	24	18.7	50309	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091924\
Data File : BN034032.D
Acq On : 18 Sep 2024 08:34
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 18 17:07:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 04:22:28 2024
Response via : Initial Calibration

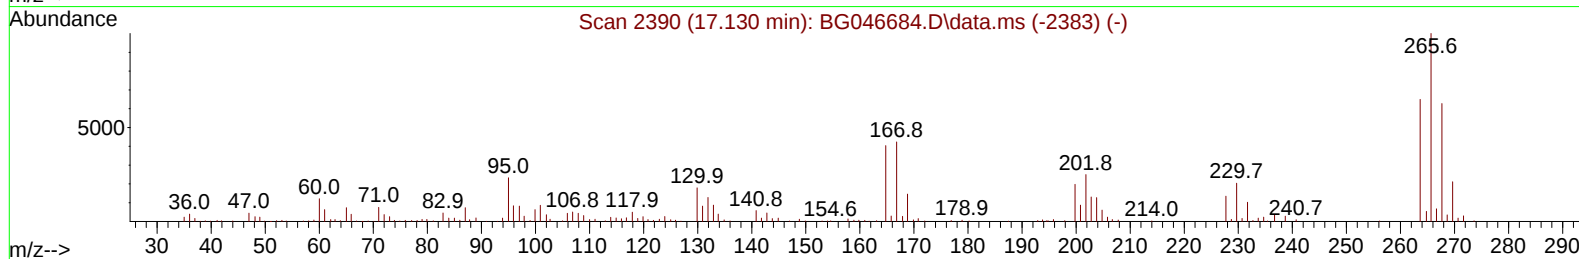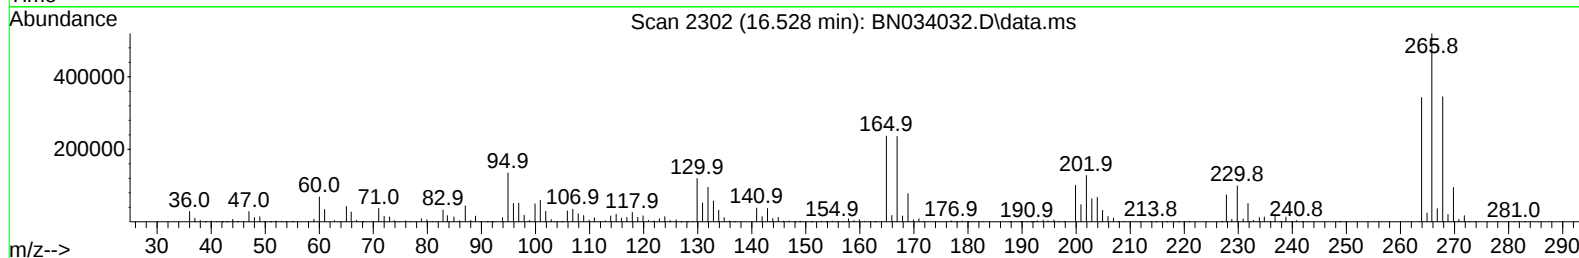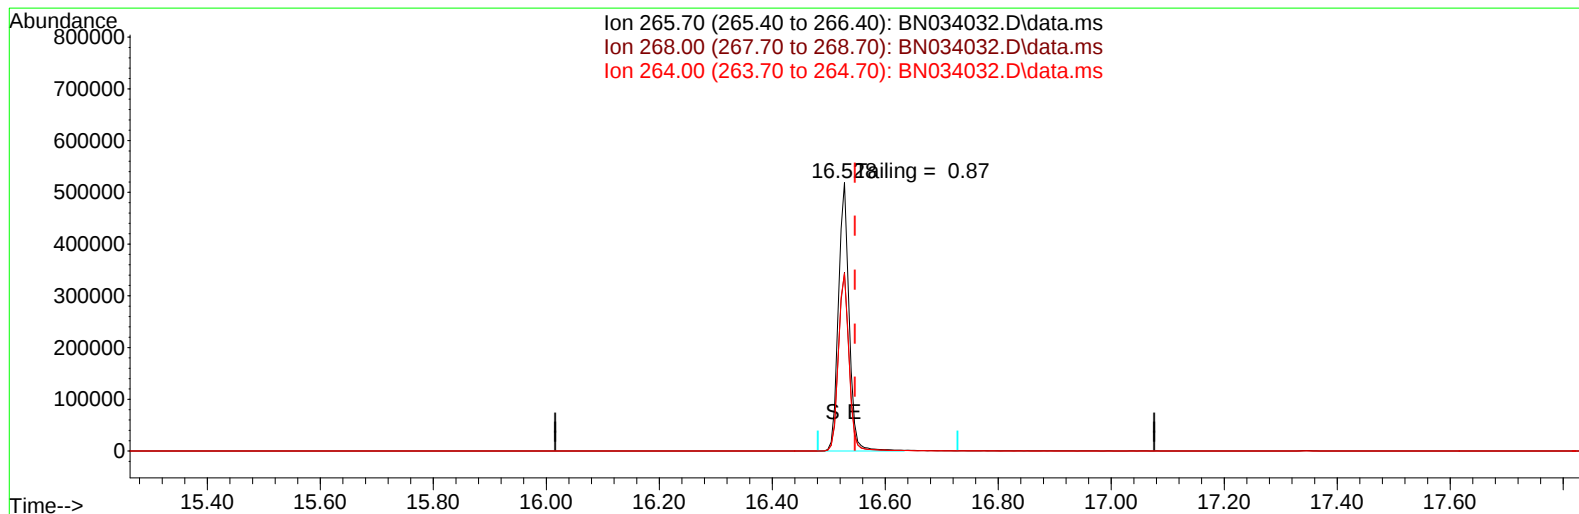

TIC: BN034032.D\data.ms

(70) Pentachlorophenol (C)

16.528min (-0.018) 32535.82 ng




response 682505

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.46
264.00	61.60	66.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091924\
Data File : BN034032.D
Acq On : 18 Sep 2024 08:34
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 18 17:07:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 04:22:28 2024
Response via : Initial Calibration

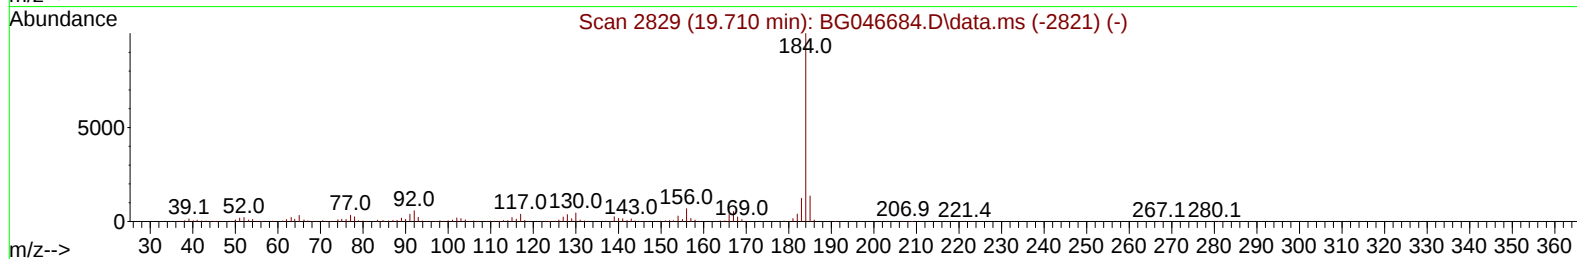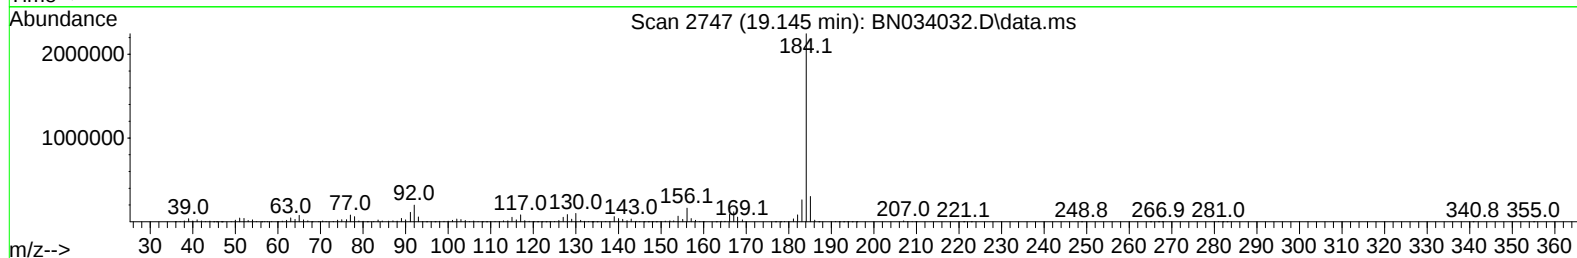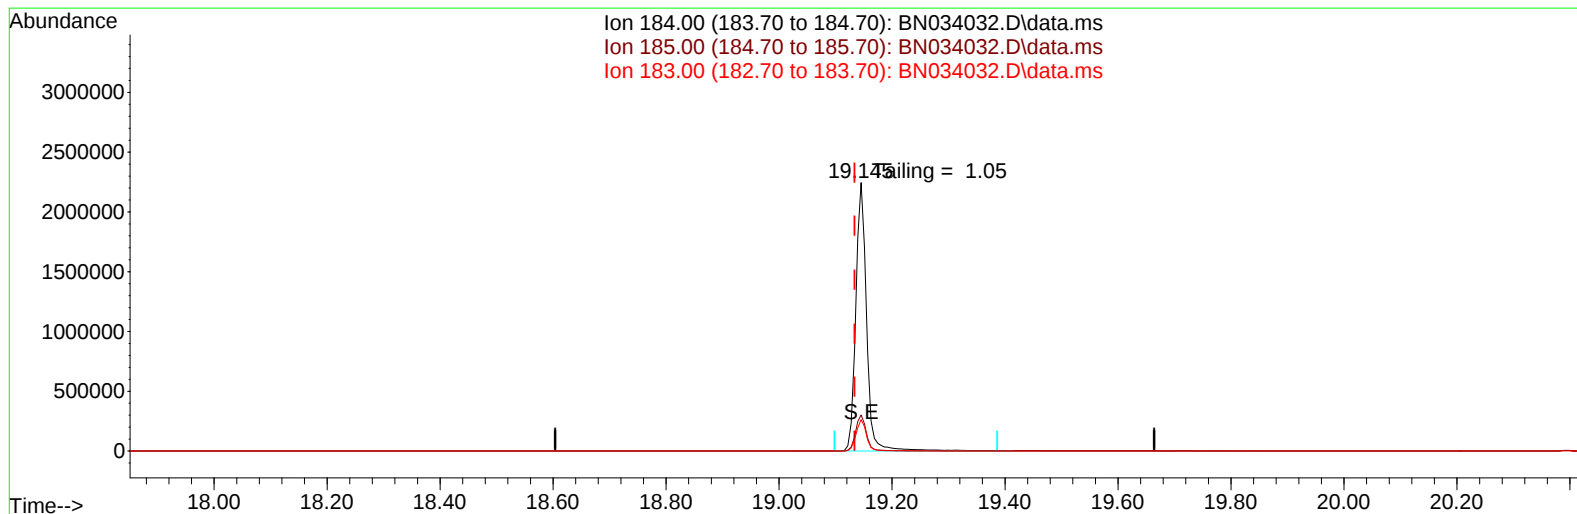

TIC: BN034032.D\data.ms

(77) Benzidine

19.145min (+ 0.011) 0.00 ng

response 3004968

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.44
183.00	13.20	11.67
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/19/2024	BNA_N	<u>BN034032.D</u>
Compound Name	Response	Retention Time
DDT	1434298	20.392
DDD	33424	19.951
DDE	2229	19.439
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
35653	1469951	2.43

Instrument :
BNA_N
ClientSampleId :
DFTPP