
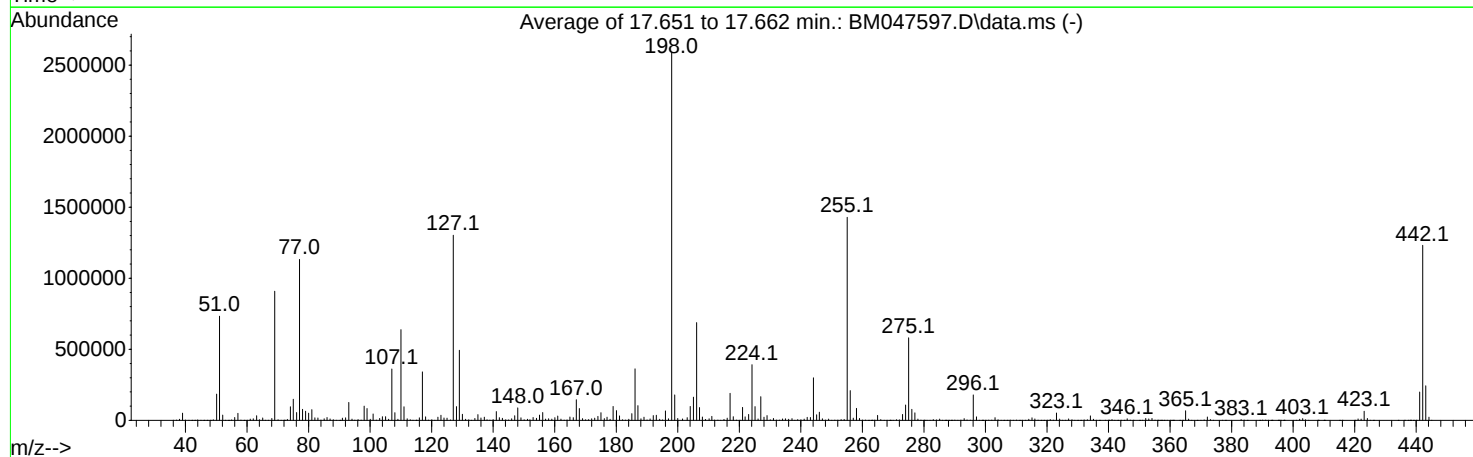


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092324\
Data File : BM047597.D
Acq On : 23 Sep 2024 08:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Sep 21 02:22:39 2024

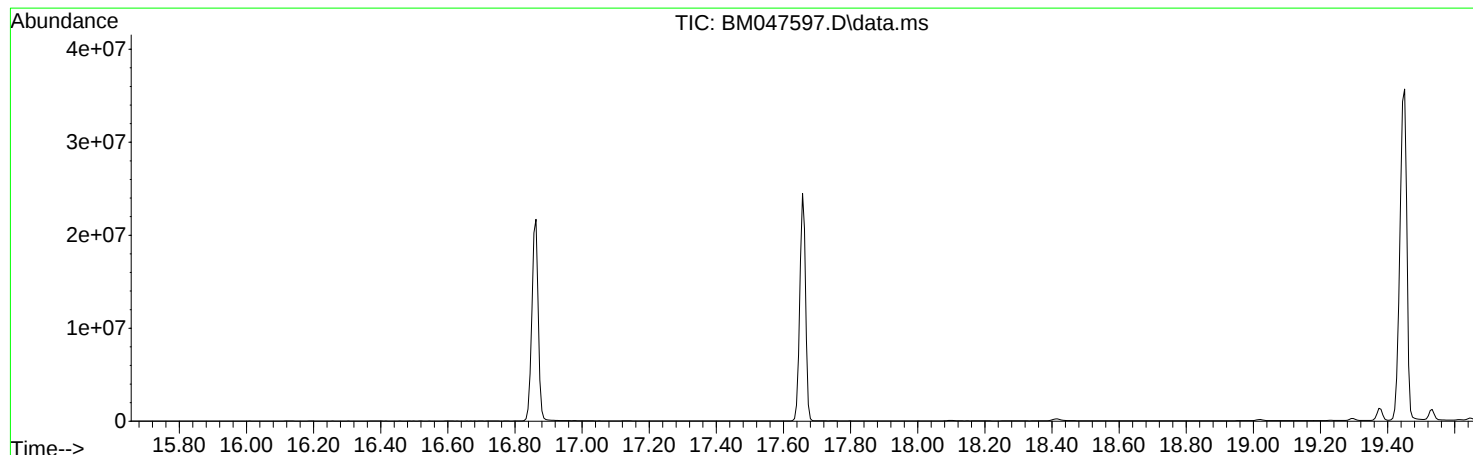




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.3	732675	PASS
68	69	0.00	2	1.5	13360	PASS
69	198	0.00	100	35.1	908480	PASS
70	69	0.00	2	0.5	4429	PASS
127	198	10	80	50.3	1303040	PASS
197	198	0.00	2	0.4	11218	PASS
198	198	100	100	100.0	2588501	PASS
199	198	5	9	6.9	178880	PASS
275	198	10	60	22.4	580843	PASS
365	198	1	100	2.6	67565	PASS
441	198	0.01	100	7.7	199245	PASS
442	442	50	100	100.0	1231595	PASS
443	442	15	24	19.7	242731	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092324\
Data File : BM047597.D
Acq On : 23 Sep 2024 08:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 23 11:22:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 21 02:22:39 2024
Response via : Initial Calibration

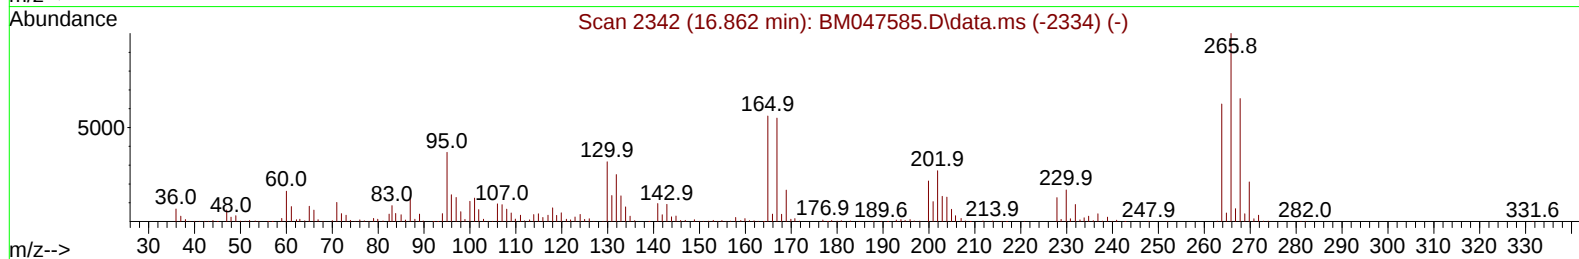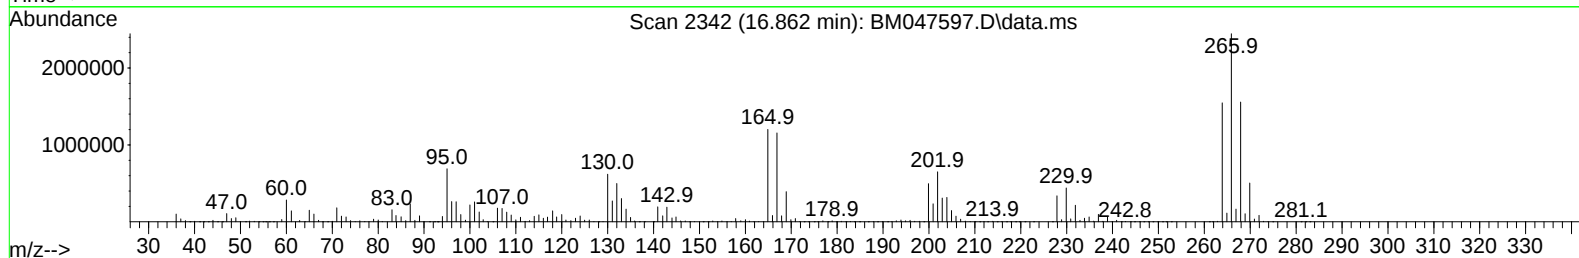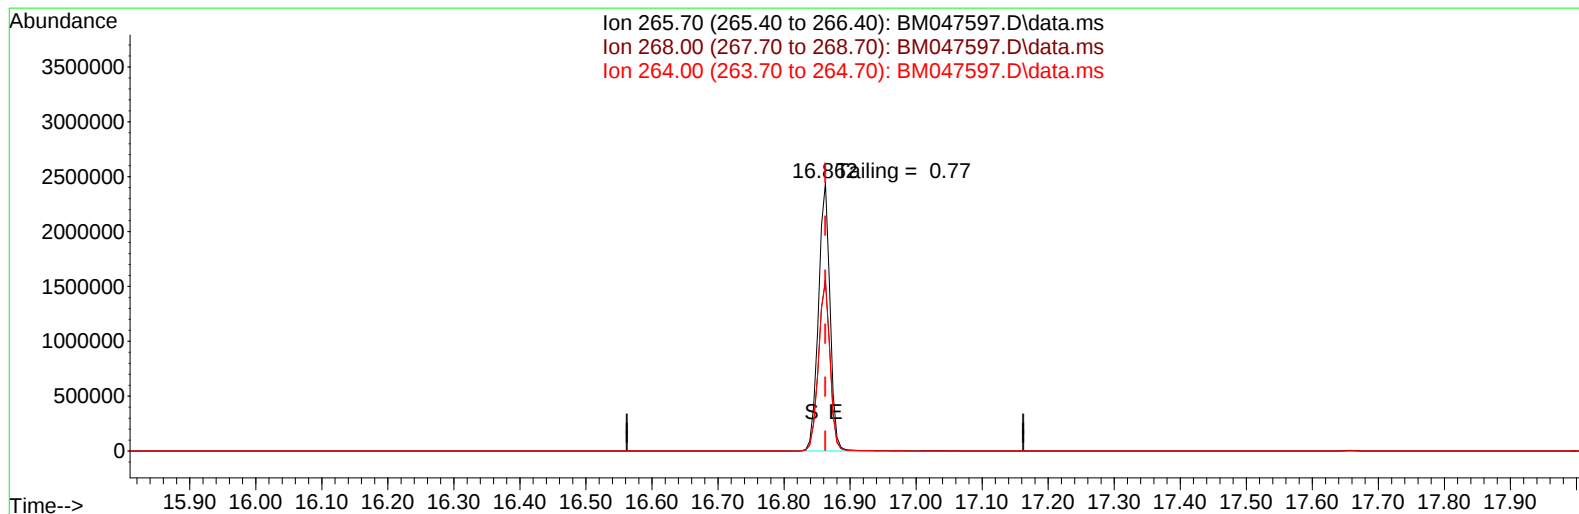

TIC: BM047597.D\data.ms

(70) Pentachlorophenol (C)

16.862min (+ 0.000) 0.00 ng




response 2968340

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	63.68
264.00	62.50	63.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092324\
 Data File : BM047597.D
 Acq On : 23 Sep 2024 08:47
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Sep 23 11:22:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 21 02:22:39 2024
 Response via : Initial Calibration

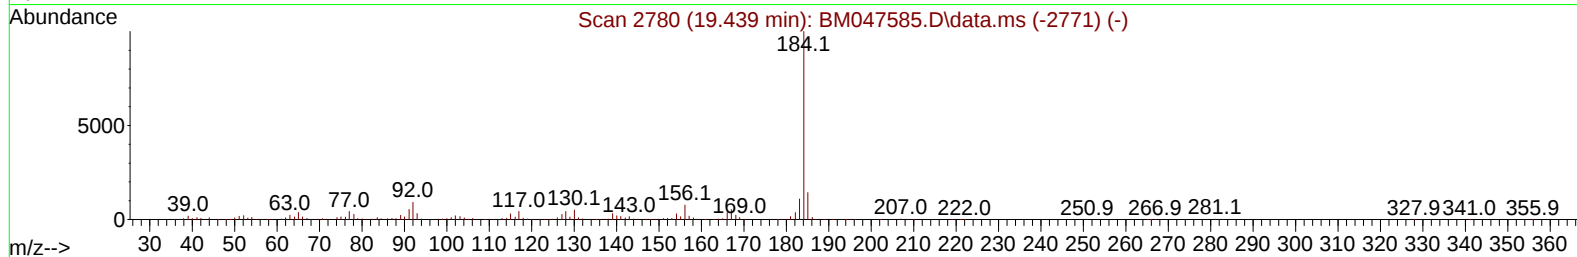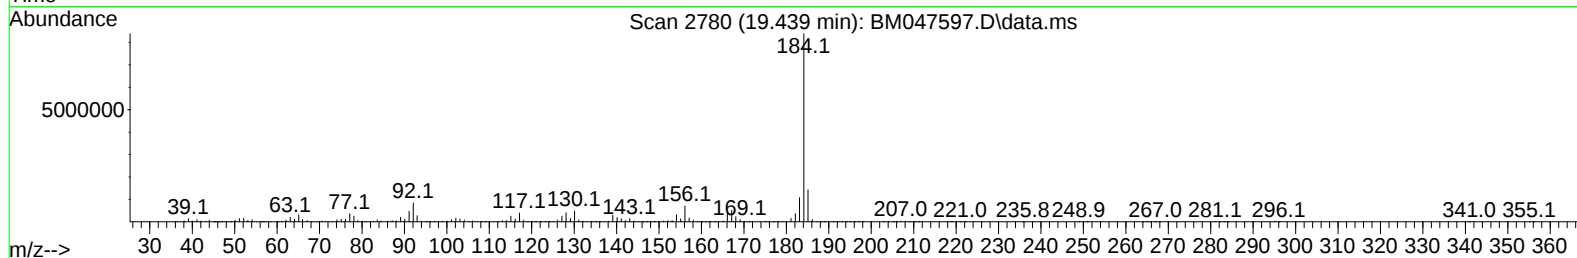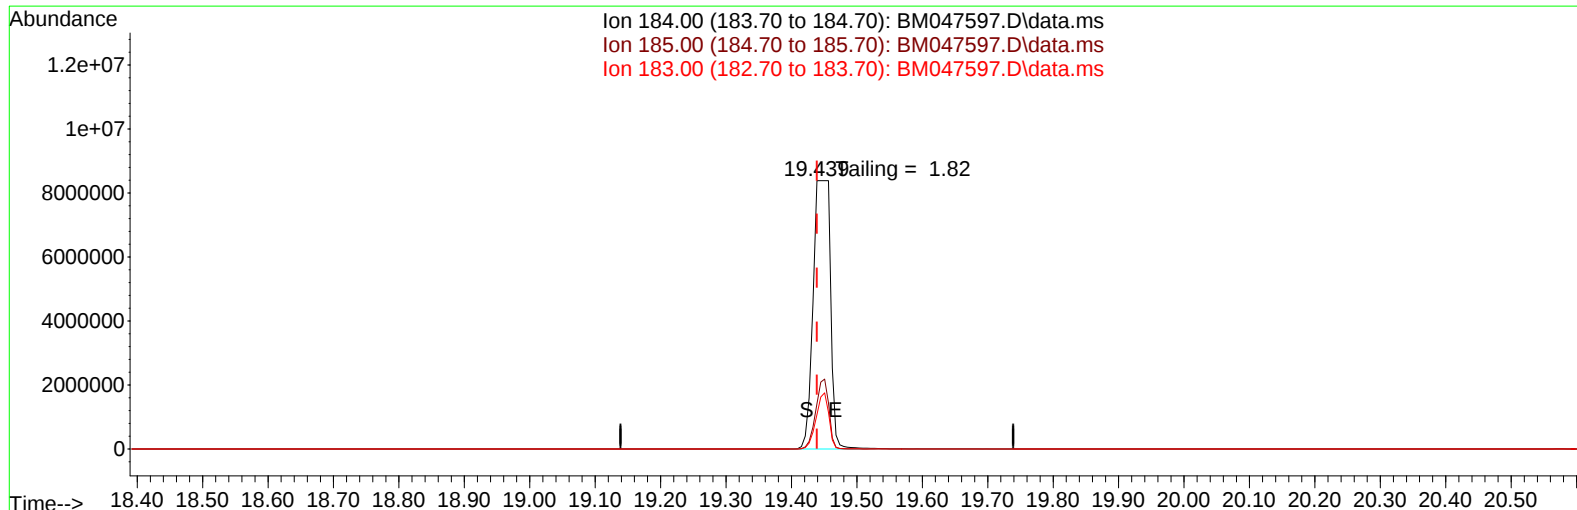

TIC: BM047597.D\data.ms

(77) Benzidine

19.439min (-0.000) 2994134.77 ng

response 15453930

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	16.91
183.00	10.90	12.85
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/23/2024	BNA_M	<u>BM047597.D</u>
Compound Name	Response	Retention Time
DDT	8671438	20.68
DDD	56131	20.292
DDE	1121	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
57252	8728690	0.66

Instrument :
BNA_M
ClientSampleId :
DFTPP