

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091924\
 Data File : P0106702.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2024 18:44
 Operator : YP/AJ
 Sample : P4103-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WC-14-7.5-10A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/20/2024
 Supervised By :Ankita Jodhani 09/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 05:21:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 10 09:57:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.450	3.713	80581924	29877879	10.742	11.185m
2) SA Decachlor...	10.195	8.737	92821578	37286041	18.779	18.641m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091924\
Data File : PO106702.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2024 18:44
Operator : YP/AJ
Sample : P4103-10
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WC-14-7.5-10A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/20/2024
Supervised By :Ankita Jodhani 09/20/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 05:21:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 10 09:57:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

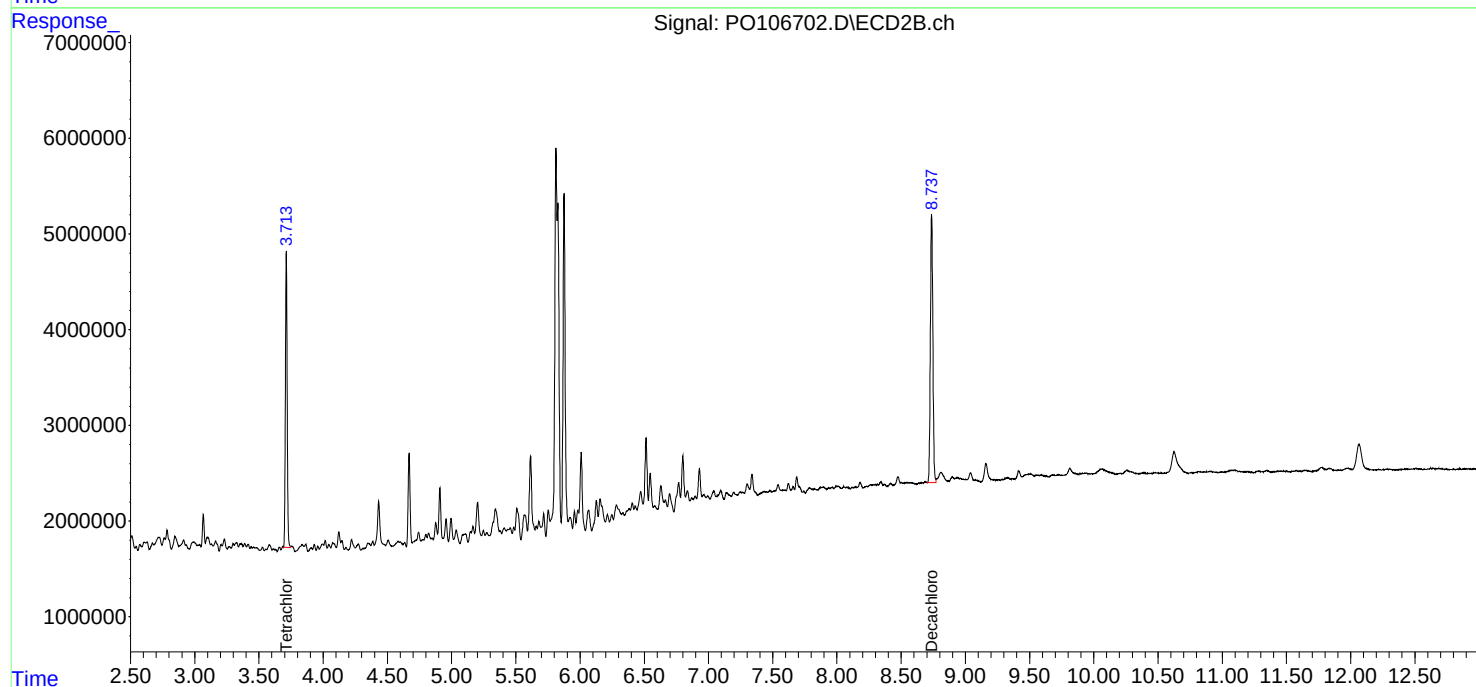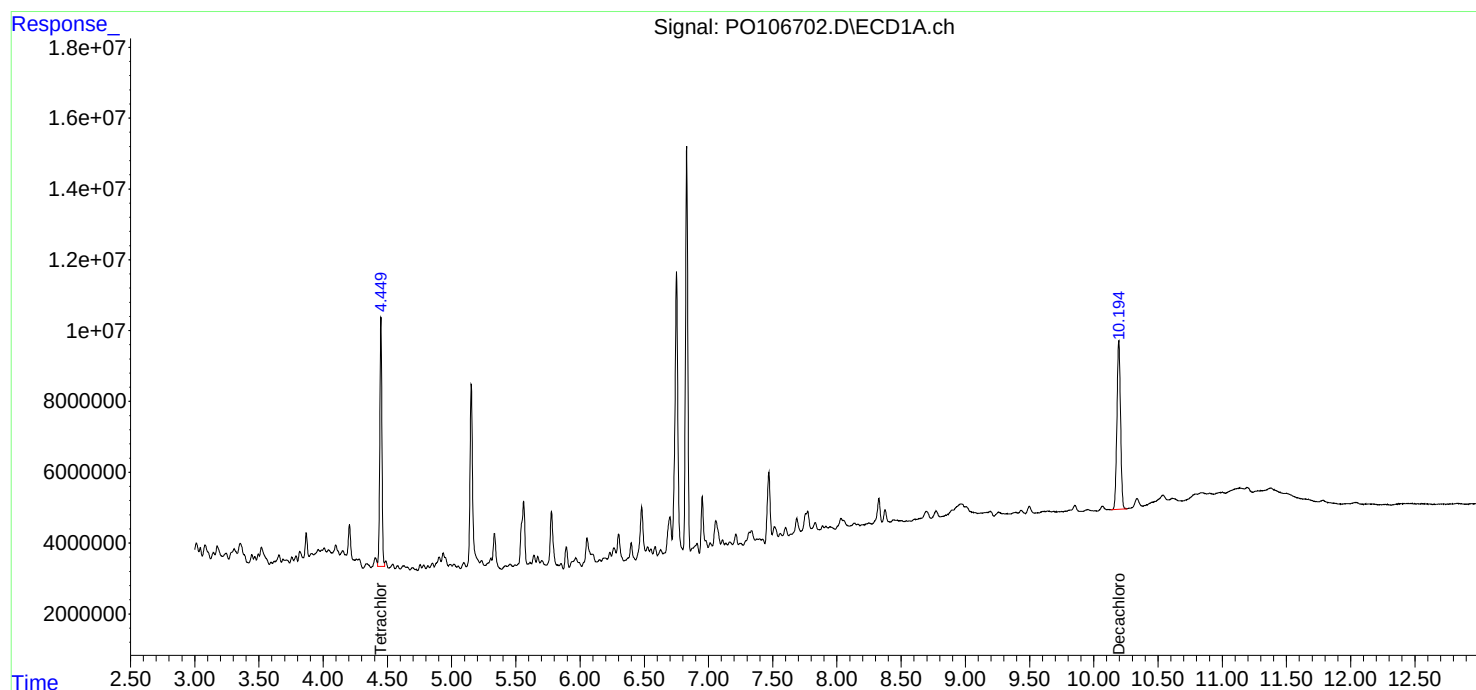

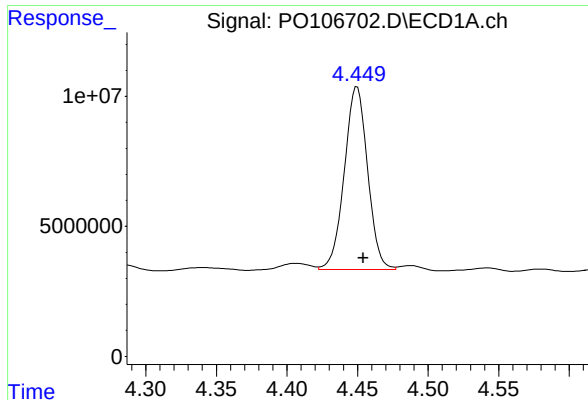


#1 Tetrachloro-m-xylene

R.T.: 4.450 min
Delta R.T.: -0.004 min
Response: 80581924
Conc: 10.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC-14-7.5-10A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/20/2024
Supervised By :Ankita Jodhani 09/20/2024

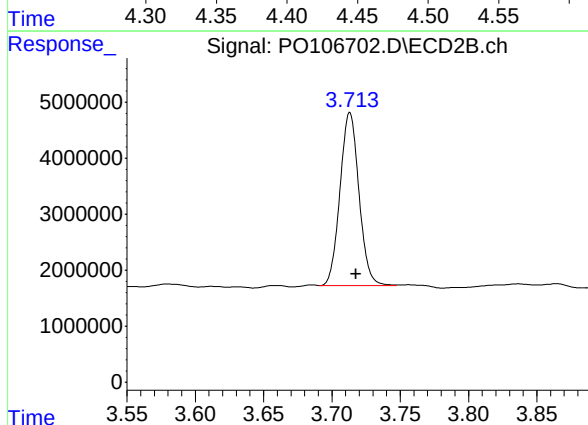


#1 Tetrachloro-m-xylene

R.T.: 3.713 min
Delta R.T.: -0.005 min
Response: 29877879
Conc: 11.19 ng/ml m

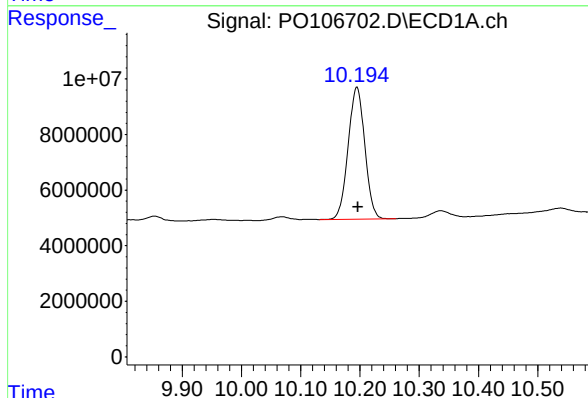

#2 Decachlorobiphenyl

R.T.: 10.195 min
Delta R.T.: -0.002 min
Response: 92821578
Conc: 18.78 ng/ml

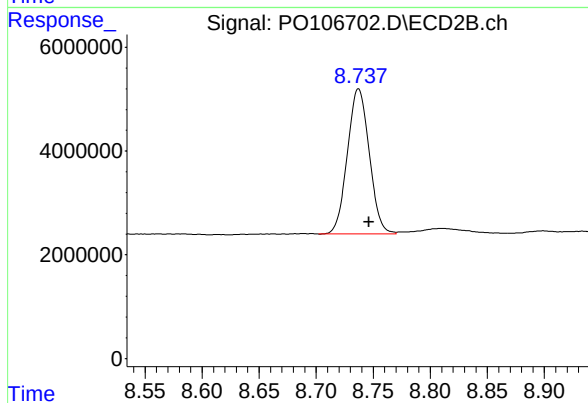

#2 Decachlorobiphenyl

R.T.: 8.737 min
Delta R.T.: -0.010 min
Response: 37286041
Conc: 18.64 ng/ml m