
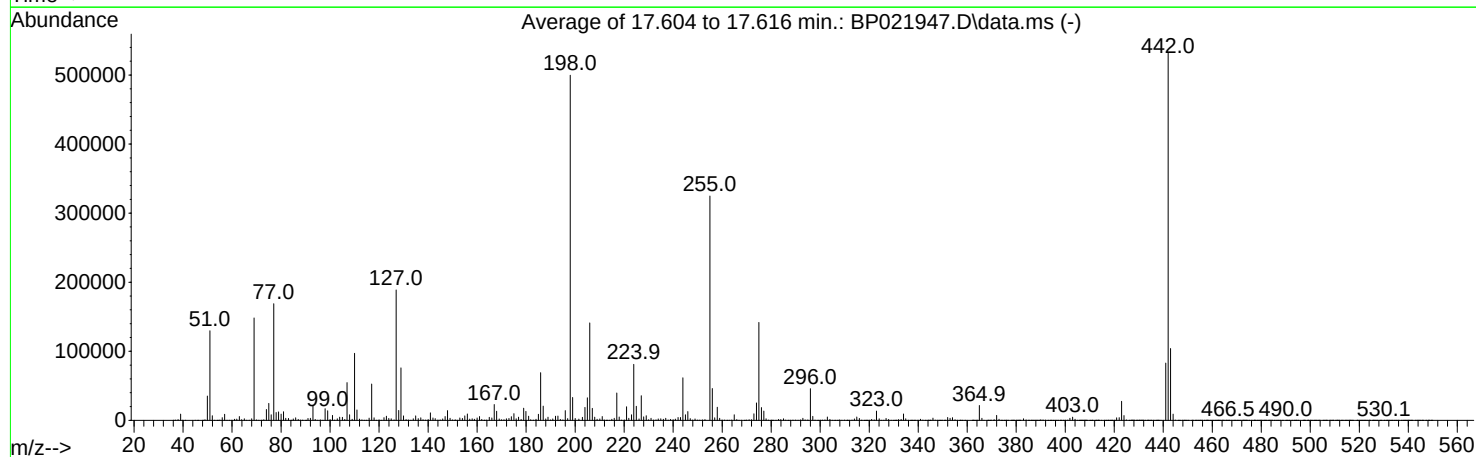


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091924\
Data File : BP021947.D
Acq On : 19 Sep 2024 12:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Sep 20 01:22:00 2024

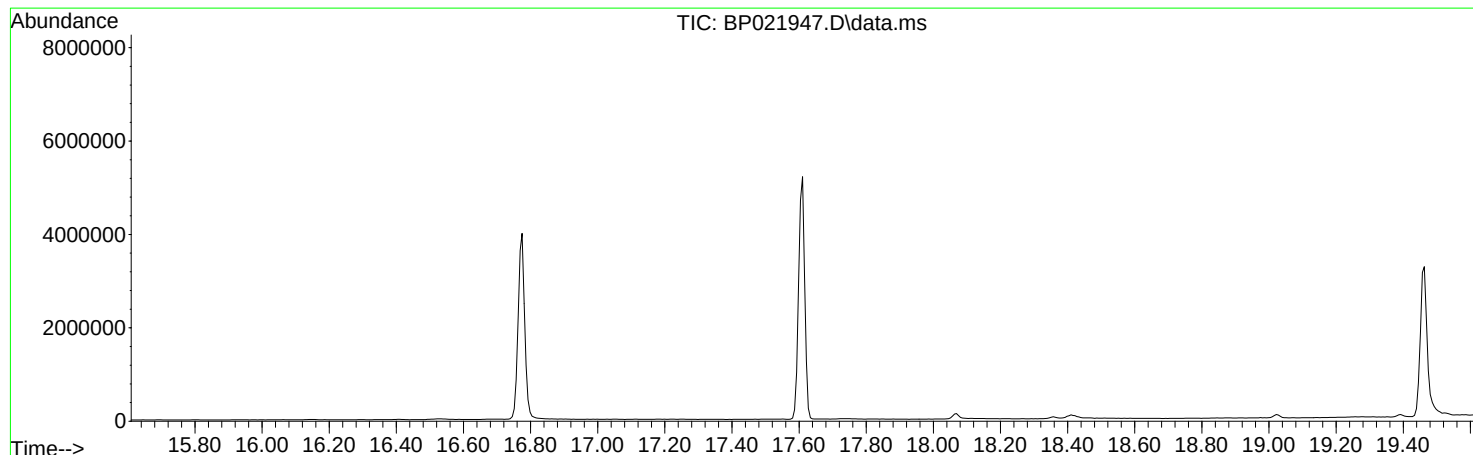




AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.0	129781	PASS
68	69	0.00	2	1.5	2241	PASS
69	198	0.00	100	29.7	148288	PASS
70	69	0.00	2	0.5	778	PASS
127	198	10	80	37.8	188904	PASS
197	198	0.00	2	0.5	2594	PASS
198	198	100	100	100.0	499781	PASS
199	198	5	9	6.6	33181	PASS
275	198	10	60	28.4	141738	PASS
365	198	1	100	4.3	21531	PASS
441	198	0.01	100	16.6	82873	PASS
442	442	100	100	100.0	532585	PASS
443	442	15	24	19.5	104076	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091924\
Data File : BP021947.D
Acq On : 19 Sep 2024 12:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 20 01:31:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 01:22:00 2024
Response via : Initial Calibration

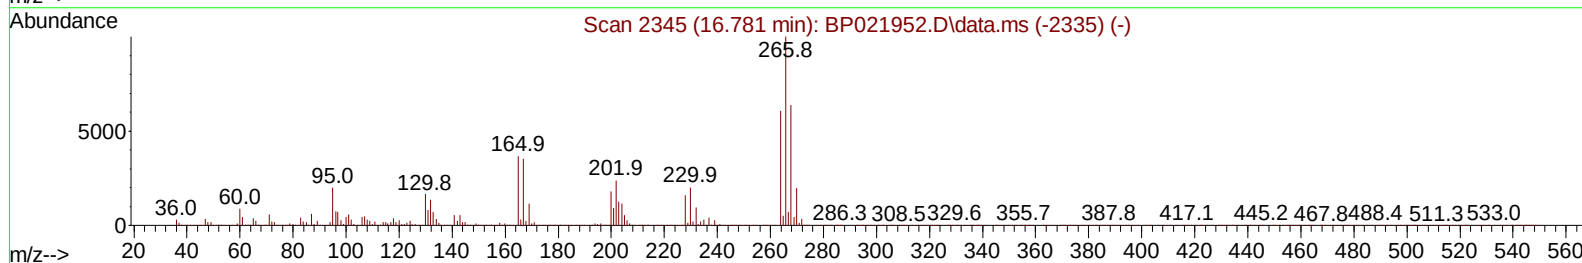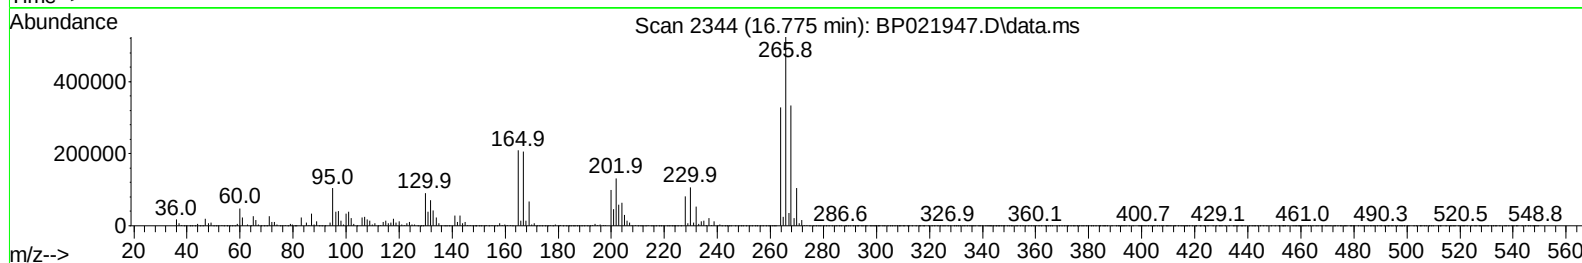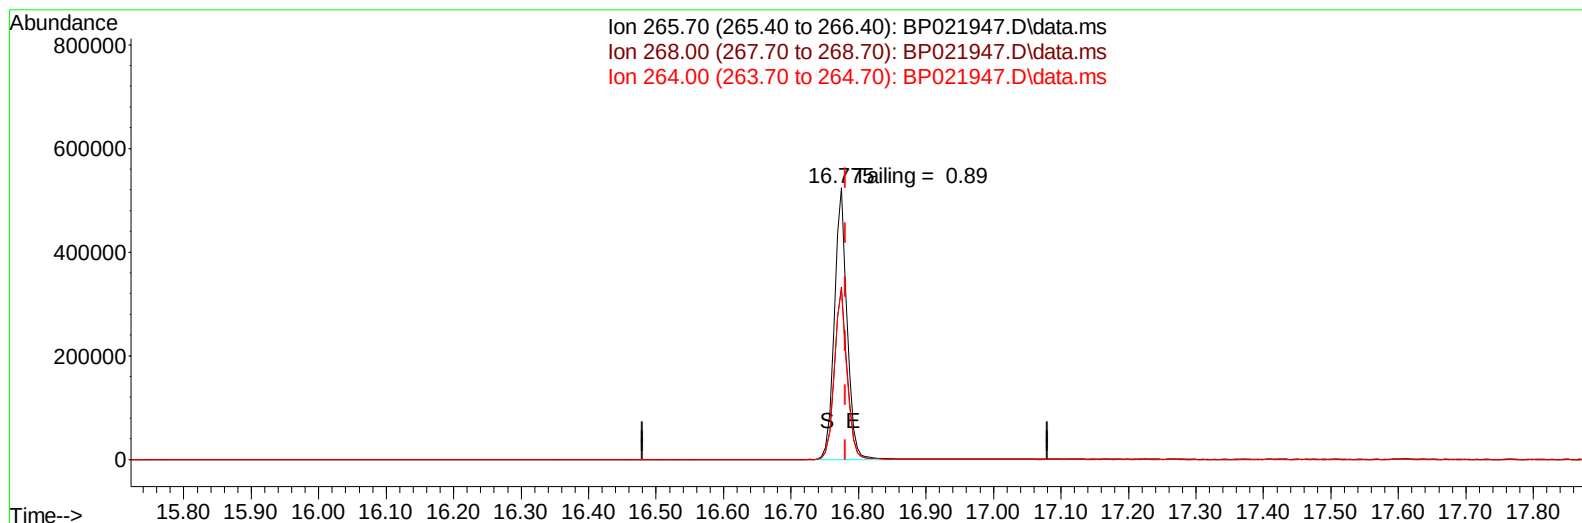

TIC: BP021947.D\data.ms

(70) Pentachlorophenol (C)

16.775min (-0.006) 135335.85 ng




response 685480

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	63.64
264.00	60.70	62.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091924\
Data File : BP021947.D
Acq On : 19 Sep 2024 12:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 20 01:31:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 01:22:00 2024
Response via : Initial Calibration

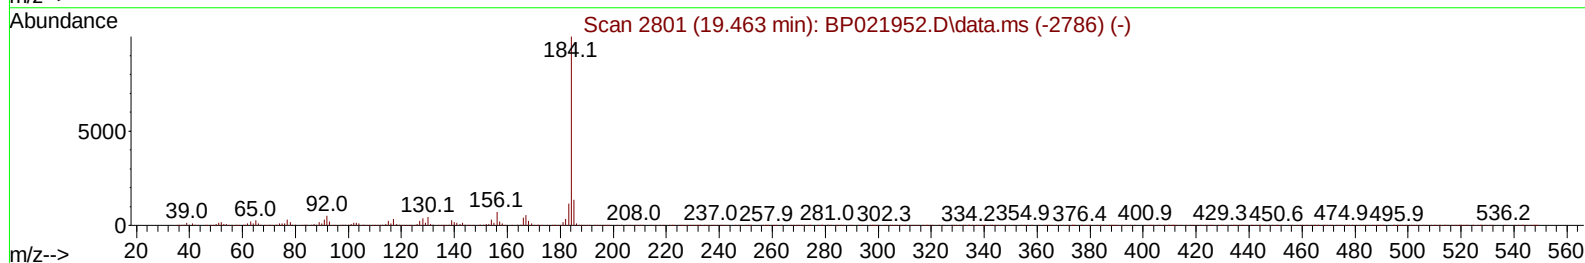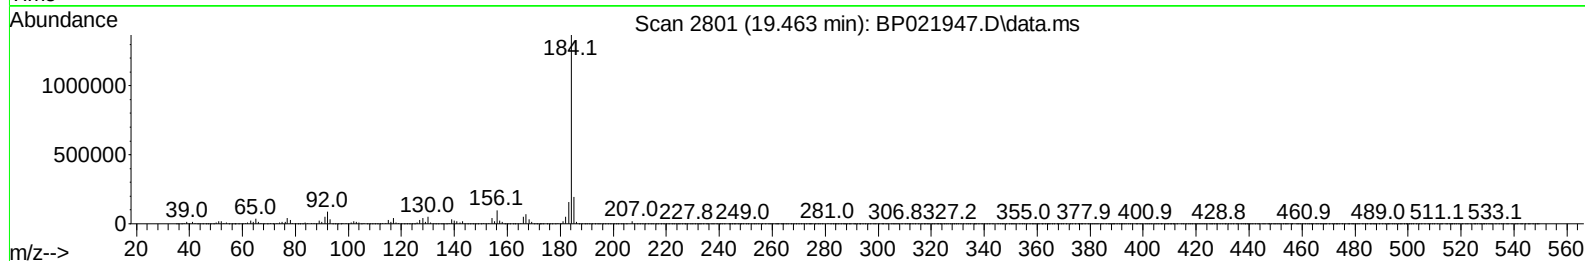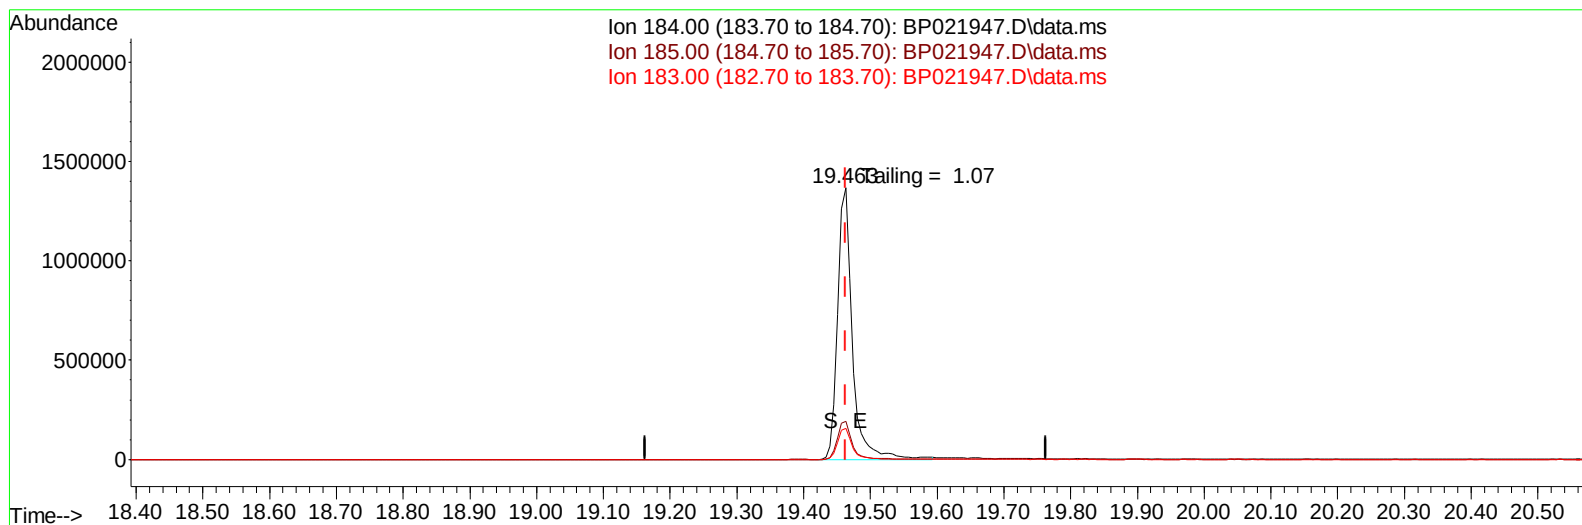

TIC: BP021947.D\data.ms

(77) Benzidine

19.463min (+ 0.000) 196747.95 ng

response 2060533

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.10
183.00	11.50	11.40
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/19/2024	BNA_P	<u>BP021947.D</u>
Compound Name	Response	Retention Time
DDT	1974757	20.757
DDD	25179	20.351
DDE	733	19.763
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25912	2000669	1.30

Instrument :
BNA_P
ClientSampleId :
DFTPP