
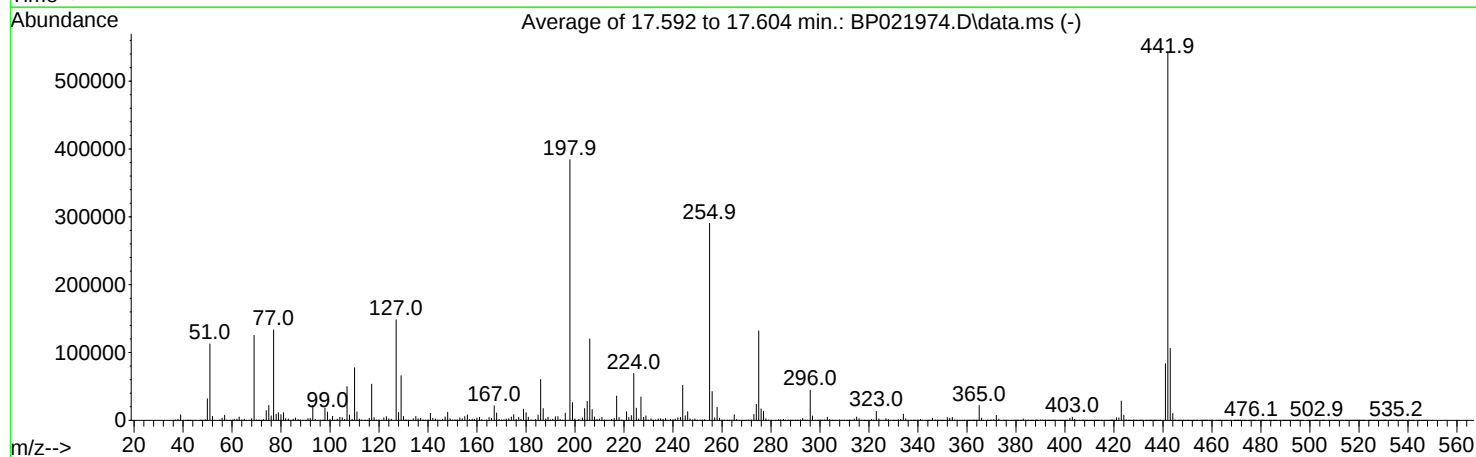


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092324\
Data File : BP021974.D
Acq On : 23 Sep 2024 08:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Sep 20 01:22:00 2024

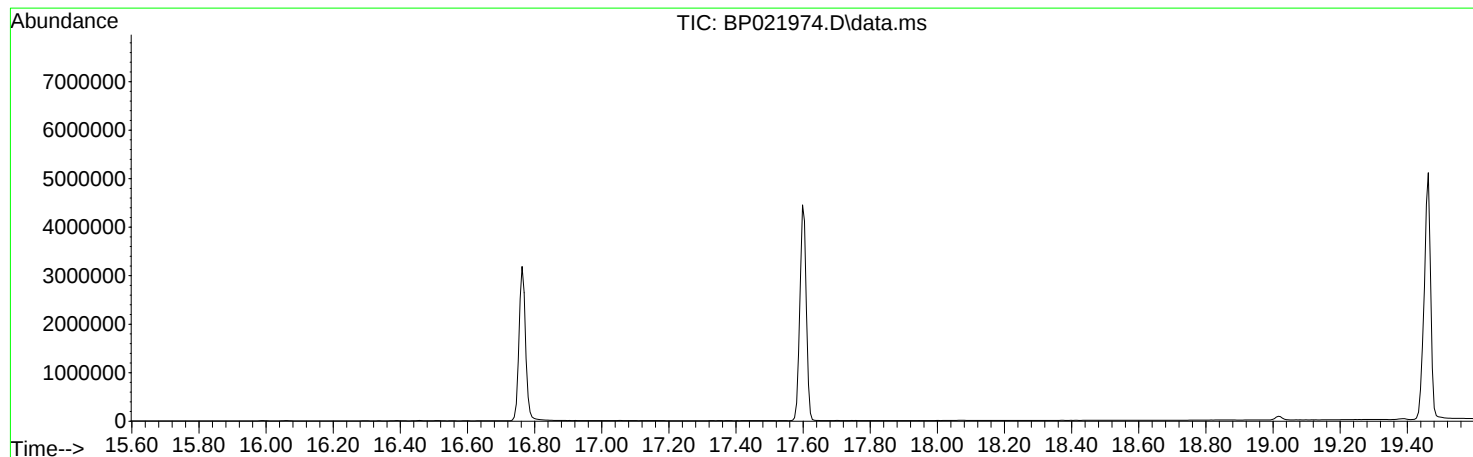




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.3	112614	PASS
68	69	0.00	2	2.0	2463	PASS
69	198	0.00	100	32.6	125219	PASS
70	69	0.00	2	0.5	627	PASS
127	198	10	80	38.6	148336	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	384233	PASS
199	198	5	9	6.8	26091	PASS
275	198	10	60	34.3	131914	PASS
365	198	1	100	5.7	21848	PASS
441	198	0.01	100	21.8	83574	PASS
442	442	100	100	100.0	542142	PASS
443	442	15	24	19.6	106256	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092324\
Data File : BP021974.D
Acq On : 23 Sep 2024 08:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 23 12:55:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 01:22:00 2024
Response via : Initial Calibration

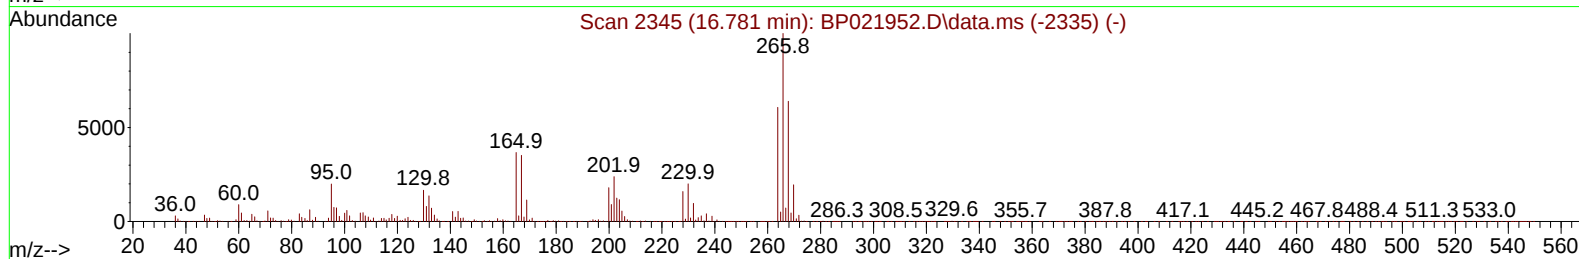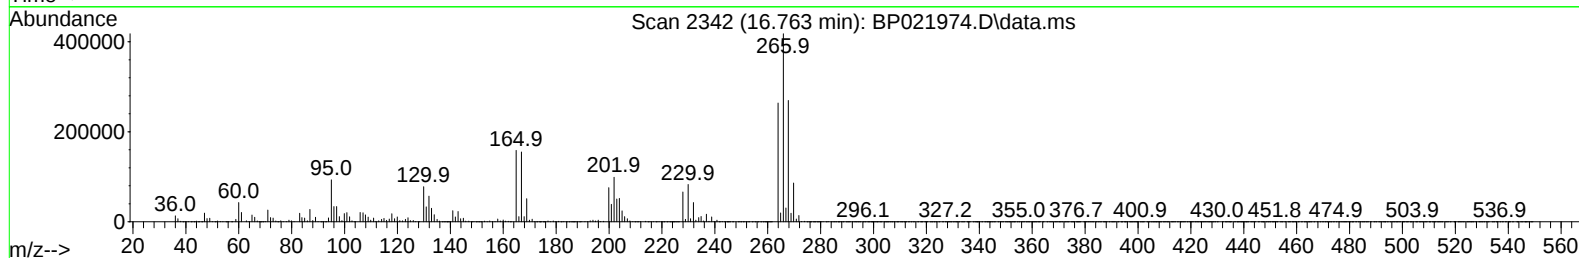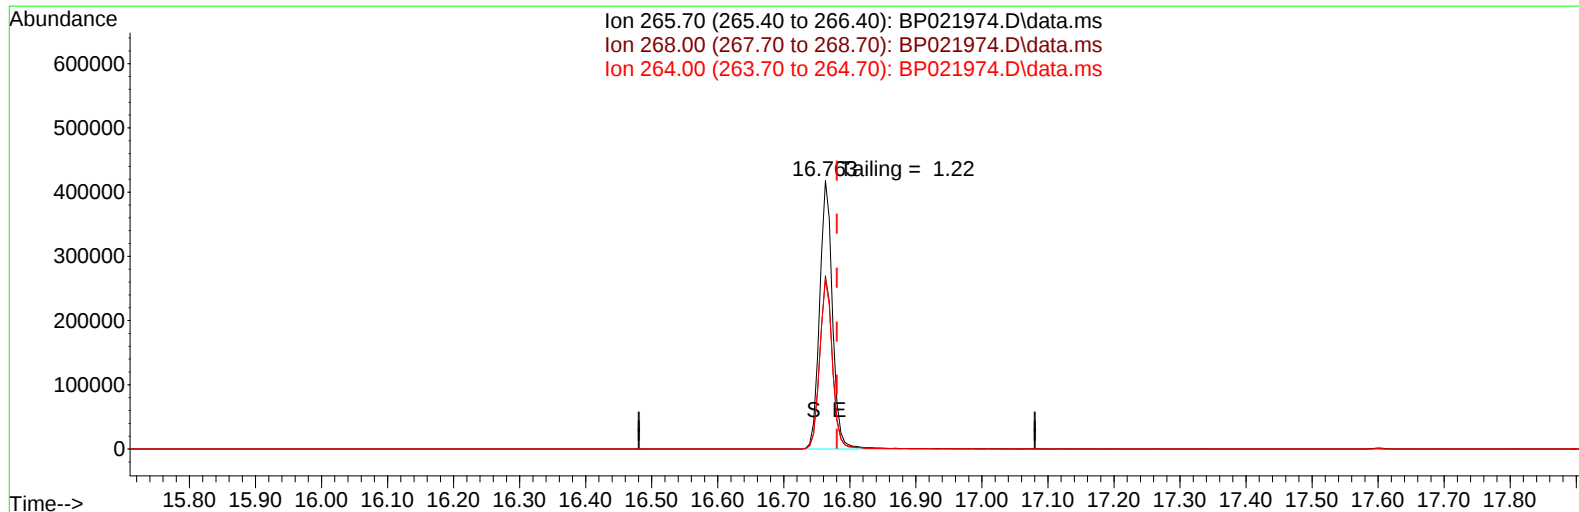

TIC: BP021974.D\data.ms

(70) Pentachlorophenol (C)

16.763min (-0.018) 5779292.50 ng




response 565102

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	64.50
264.00	60.70	63.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092324\
Data File : BP021974.D
Acq On : 23 Sep 2024 08:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 23 12:55:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 01:22:00 2024
Response via : Initial Calibration

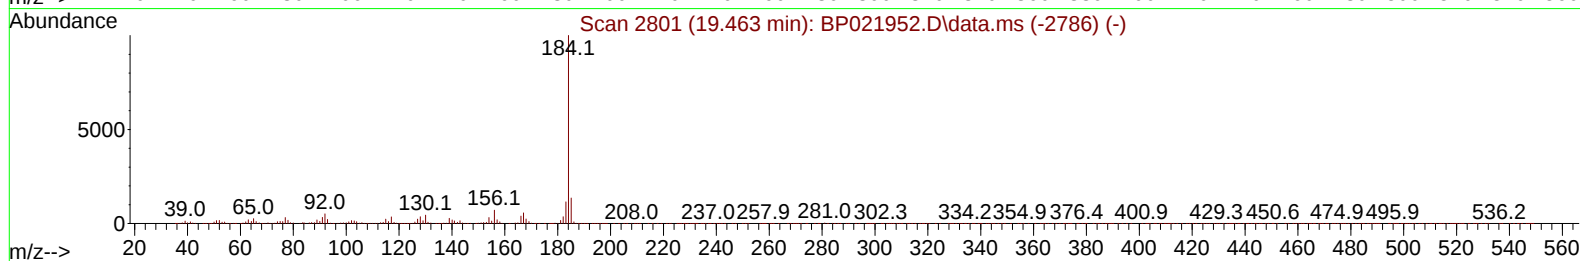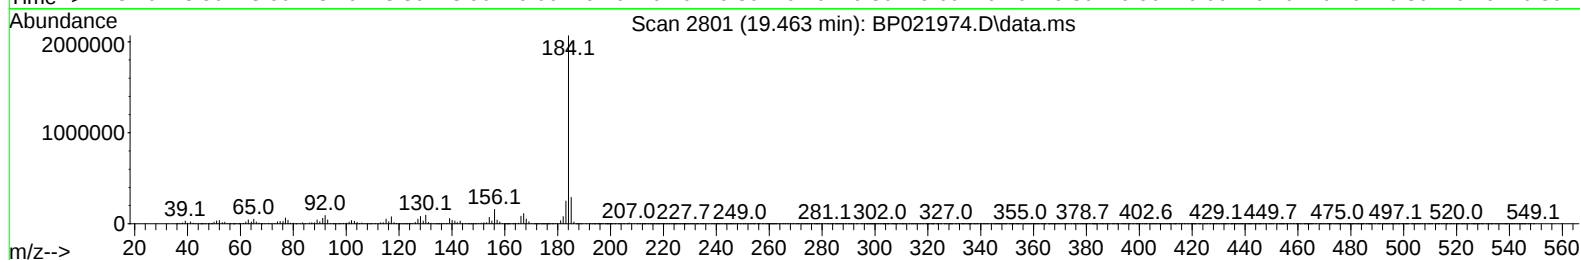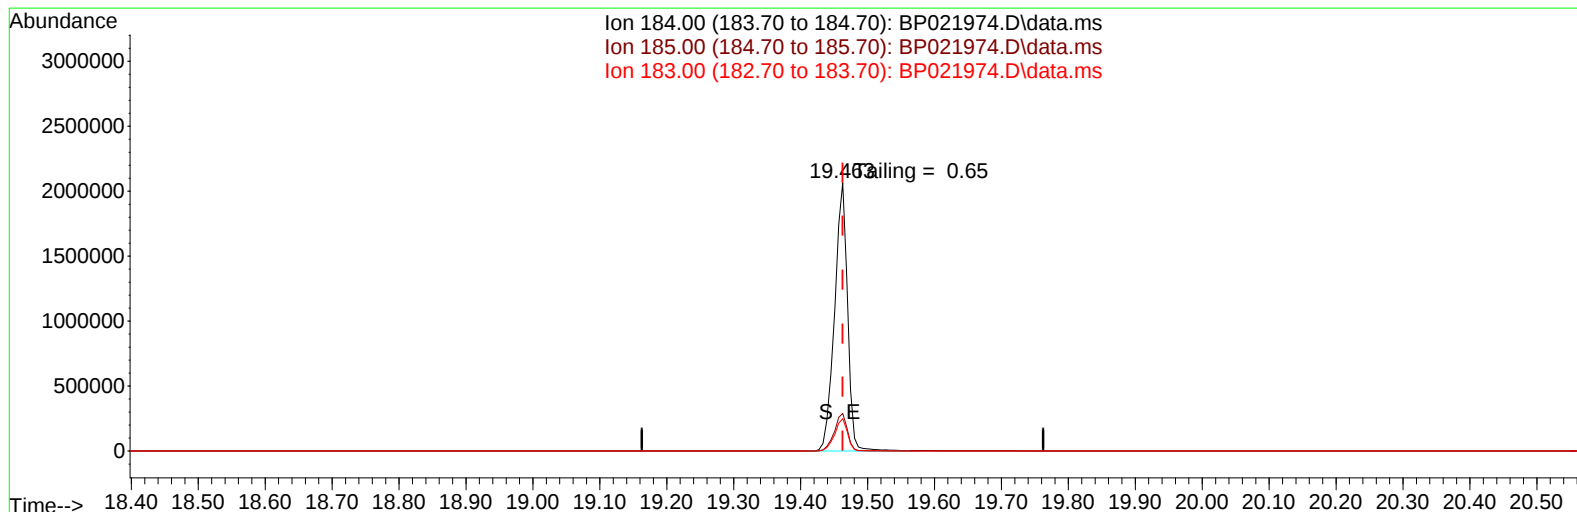

TIC: BP021974.D\data.ms

(77) Benzidine

19.463min (+ 0.000) 13419701.31 ng

response 2787920

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.05
183.00	11.50	12.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/23/2024	BNA_P	<u>BP021974.D</u>
Compound Name	Response	Retention Time
DDT	1790325	20.745
DDD	21049	20.339
DDE	1159	19.751
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22208	1812533	1.23

Instrument :
BNA_P
ClientSampleId :
DFTPP