

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092024\
 Data File : BF139509.D
 Acq On : 20 Sep 2024 18:49
 Operator : RC/JU
 Sample : P4103-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-14-5-7.5B

Quant Time: Sep 20 23:22:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 14 02:58:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.881	152	76931	20.000	ng	0.00
21) Naphthalene-d8	8.157	136	265343	20.000	ng	0.00
39) Acenaphthene-d10	9.910	164	123864	20.000	ng	0.00
64) Phenanthrene-d10	11.398	188	220987	20.000	ng	# 0.00
76) Chrysene-d12	14.033	240	131452	20.000	ng	# 0.00
86) Perylene-d12	15.509	264	98227	20.000	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.510	112	605769	128.455	ng	0.02
7) Phenol-d6	6.516	99	752732	121.608	ng	0.01
23) Nitrobenzene-d5	7.439	82	498841	88.381	ng	0.00
42) 2,4,6-Tribromophenol	10.704	330	159998	121.332	ng	0.00
45) 2-Fluorobiphenyl	9.233	172	791154	89.583	ng	0.00
79) Terphenyl-d14	12.986	244	817830	102.119	ng	0.00
Target Compounds						
						Qvalue
31) Naphthalene	8.181	128	49927	3.604	ng	99
37) 2-Methylnaphthalene	8.869	142	24604	2.798	ng	100
38) 1-Methylnaphthalene	8.969	142	36424	4.220	ng	100
70) Pentachlorophenol	11.204	266	3659	2.373	ng	# 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092024\
Data File : BF139509.D
Acq On : 20 Sep 2024 18:49
Operator : RC/JU
Sample : P4103-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-14-5-7.5B


Quant Time: Sep 20 23:22:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

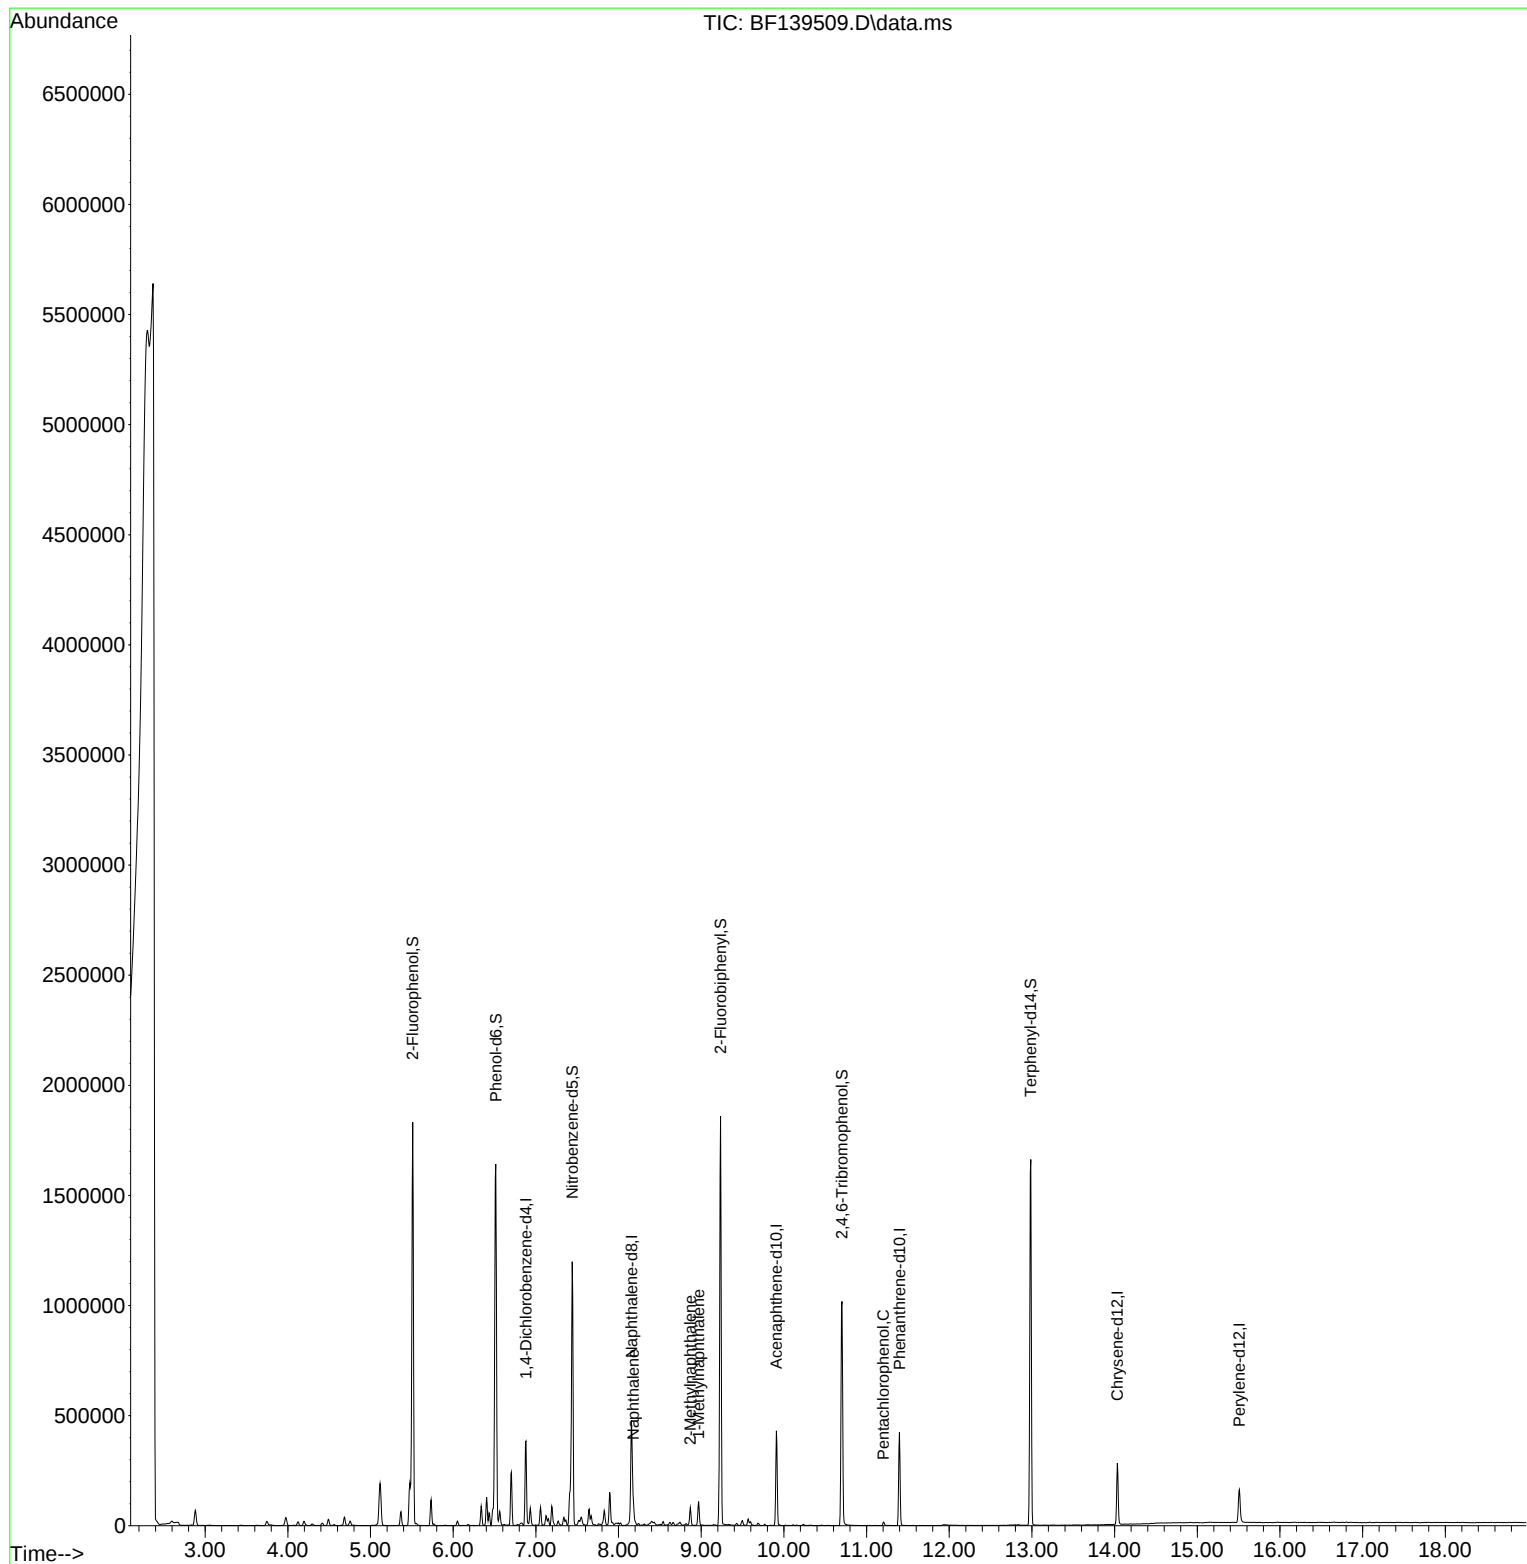






#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.881 min Scan# 814
Delta R.T. -0.000 min
Lab File: BF139509.D
Acq: 20 Sep 2024 18:49

Instrument :
BNA_F
ClientSampleId :
WC-14-5-7.5B



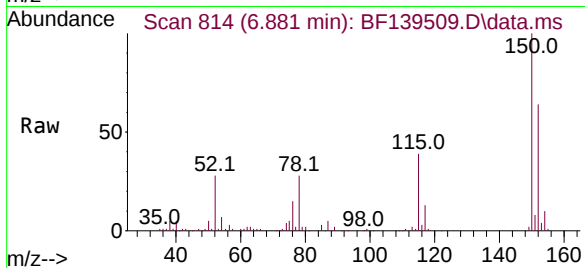



Tgt Ion:152 Resp: 76931
Ion Ratio Lower Upper
152 100
150 155.4 124.1 186.1
115 60.4 48.1 72.1

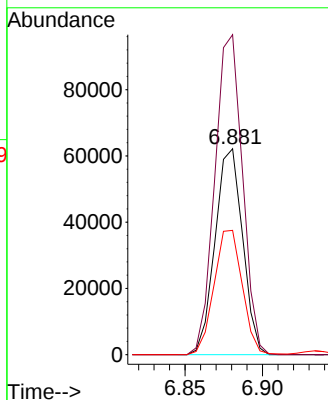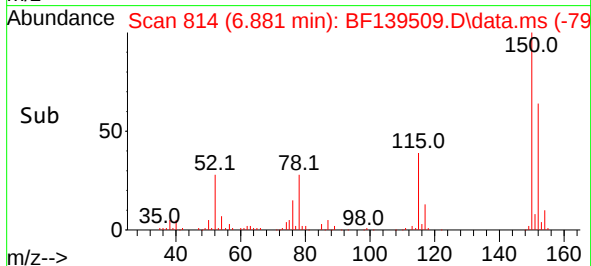

#5
2-Fluorophenol
Concen: 128.455 ng
RT: 5.510 min Scan# 581
Delta R.T. 0.017 min
Lab File: BF139509.D
Acq: 20 Sep 2024 18:49

Tgt Ion:112 Resp: 605769
Ion Ratio Lower Upper
112 100
64 69.8 54.8 82.2
63 38.8 33.0 49.4


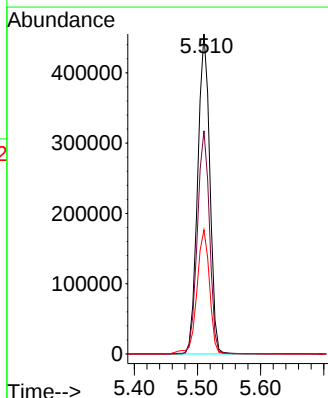

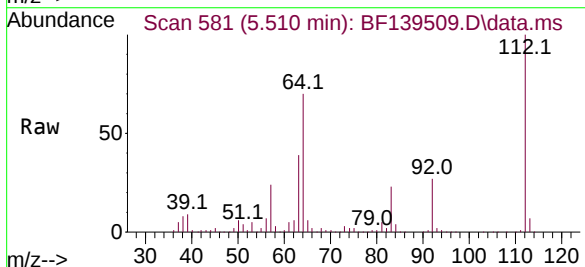


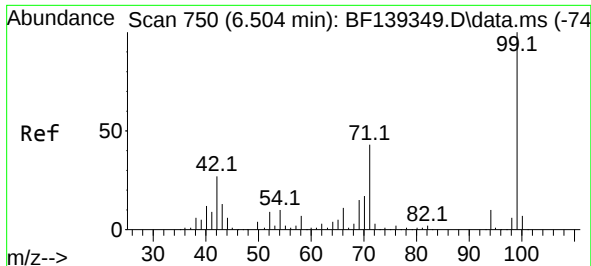

#7
Phenol-d6
Concen: 121.608 ng
RT: 6.516 min Scan# 71
Delta R.T. 0.012 min
Lab File: BF139509.D
Acq: 20 Sep 2024 18:49




Instrument :
BNA_F
ClientSampleId :
WC-14-5-7.5B


Tgt Ion: 99 Resp: 752732
Ion Ratio Lower Upper
99 100
42 24.6 21.9 32.9
71 38.9 34.6 52.0

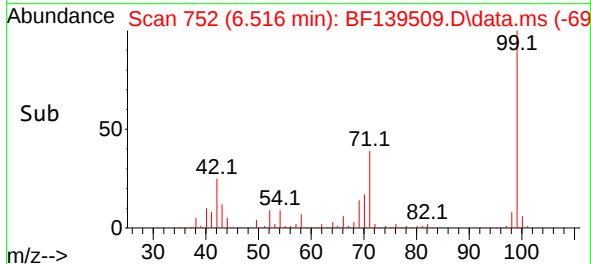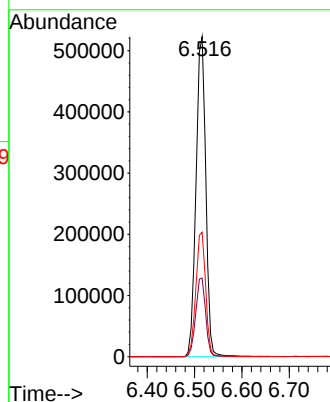

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.157 min Scan# 1031
Delta R.T. -0.006 min
Lab File: BF139509.D
Acq: 20 Sep 2024 18:49

Tgt Ion: 136 Resp: 265343
Ion Ratio Lower Upper
136 100
137 10.5 8.6 12.8
54 9.9 7.8 11.8
68 5.1 3.6 5.4

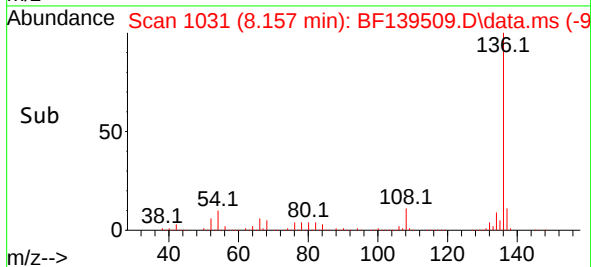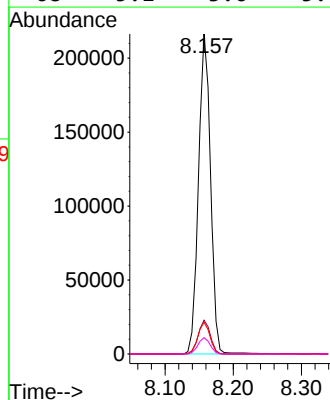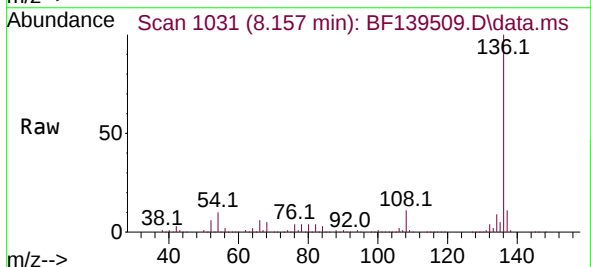

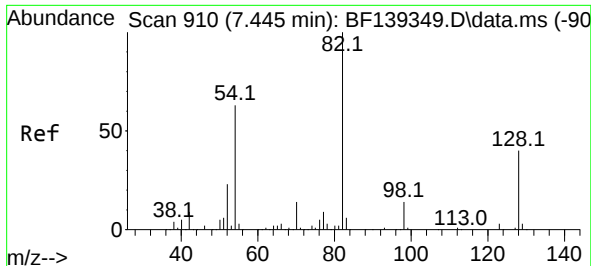

#23

Nitrobenzene-d5

Concen: 88.381 ng

RT: 7.439 min Scan# 909

Delta R.T. -0.006 min

Lab File: BF139509.D

Acq: 20 Sep 2024 18:49

Instrument :

BNA_F

ClientSampleId :

WC-14-5-7.5B





Tgt Ion: 82 Resp: 498841

Ion Ratio Lower Upper

82 100

128 40.0 31.8 47.6

54 61.8 50.6 75.8

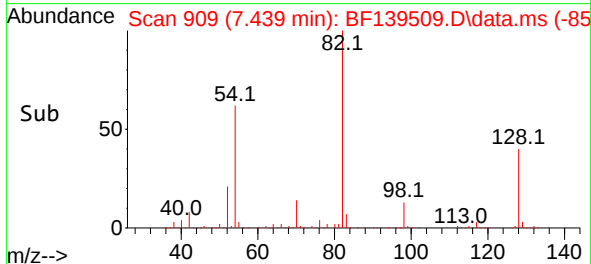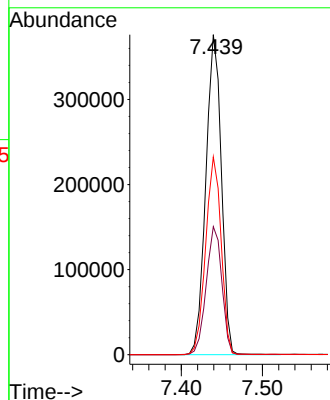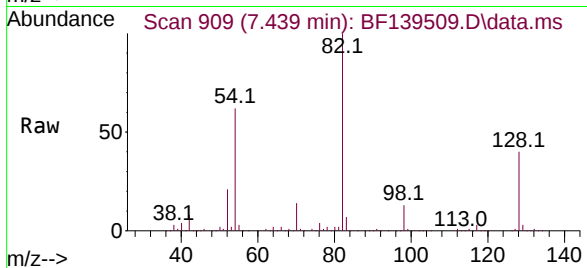

#31

Naphthalene

Concen: 3.604 ng

RT: 8.181 min Scan# 1035

Delta R.T. -0.000 min

Lab File: BF139509.D

Acq: 20 Sep 2024 18:49




Tgt Ion: 128 Resp: 49927


Ion Ratio Lower Upper

128 100

129 11.3 8.6 13.0

127 13.2 10.6 16.0



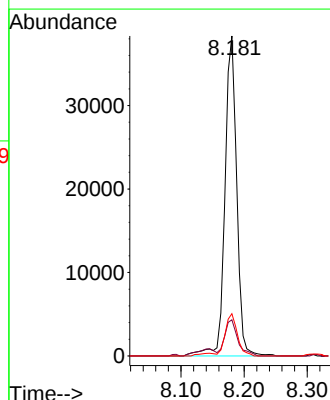
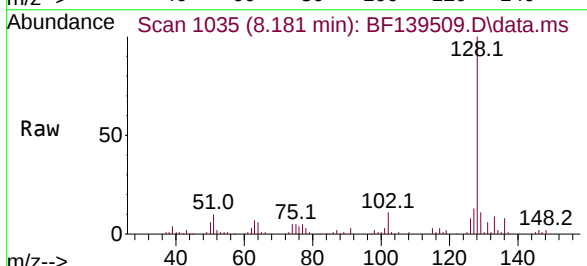




#37
2-Methylnaphthalene
Concen: 2.798 ng
RT: 8.869 min Scan# 1152
Delta R.T. -0.006 min
Lab File: BF139509.D
Acq: 20 Sep 2024 18:49




Instrument :
BNA_F
ClientSampleId :
WC-14-5-7.5B


Tgt Ion:142 Resp: 24604
Ion Ratio Lower Upper
142 100
141 90.0 71.6 107.4

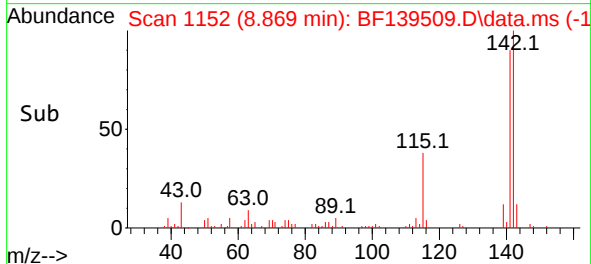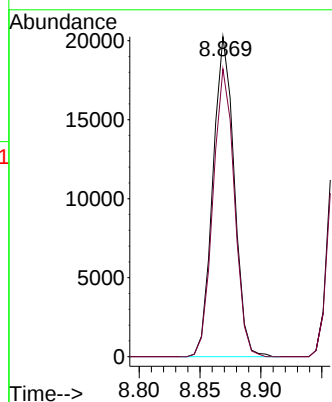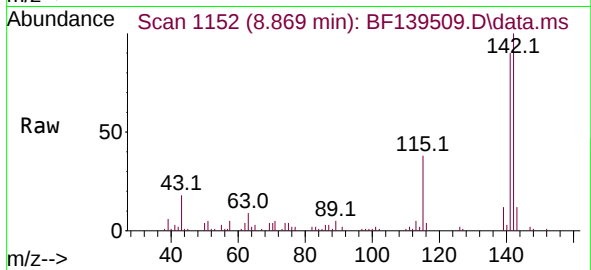

#38
1-Methylnaphthalene
Concen: 4.220 ng
RT: 8.969 min Scan# 1169
Delta R.T. -0.006 min
Lab File: BF139509.D
Acq: 20 Sep 2024 18:49

Tgt Ion:142 Resp: 36424
Ion Ratio Lower Upper
142 100
141 91.3 73.2 109.8

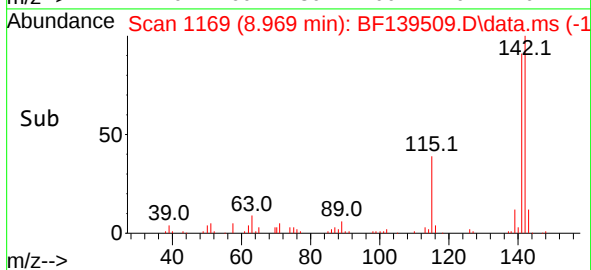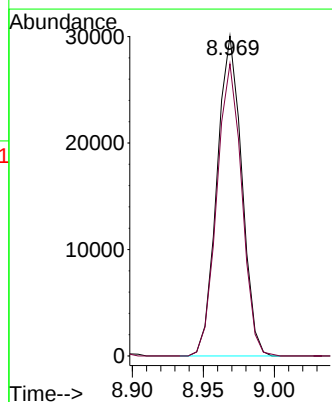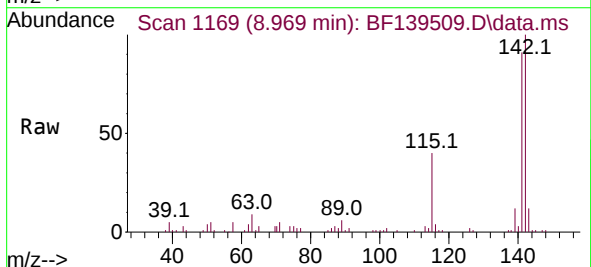

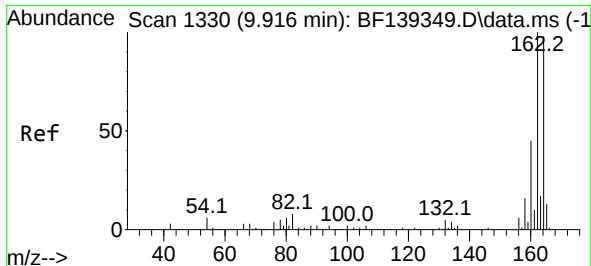

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.910 min Scan# 1

Delta R.T. -0.006 min

Lab File: BF139509.D

Acq: 20 Sep 2024 18:49

Instrument :

BNA_F

ClientSampleId :

WC-14-5-7.5B





Tgt Ion:164 Resp: 123864

Ion Ratio Lower Upper

164 100

162 98.8 81.3 121.9

160 44.7 36.4 54.6

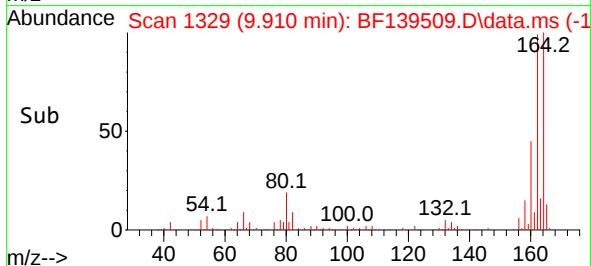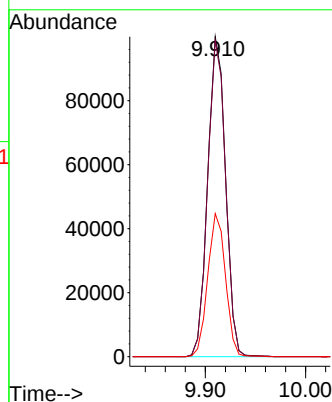

#42

2,4,6-Tribromophenol

Concen: 121.332 ng

RT: 10.704 min Scan# 1464

Delta R.T. 0.006 min

Lab File: BF139509.D

Acq: 20 Sep 2024 18:49




Tgt Ion:330 Resp: 159998


Ion Ratio Lower Upper

330 100

332 96.3 75.2 112.8

141 36.4 31.2 46.8

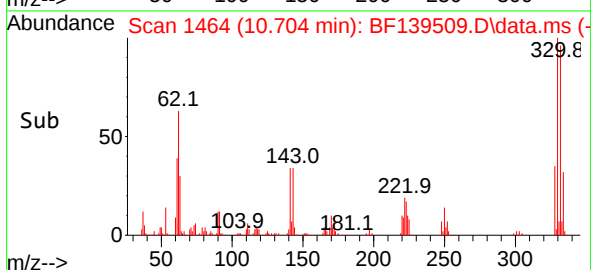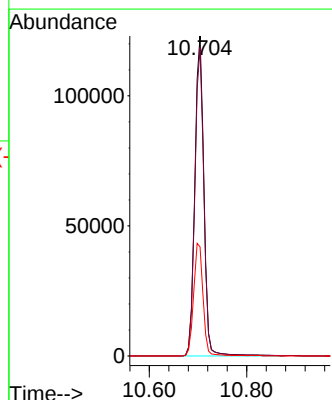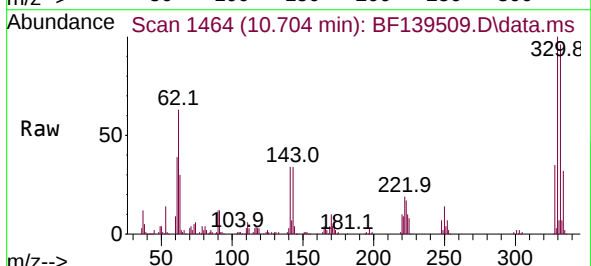

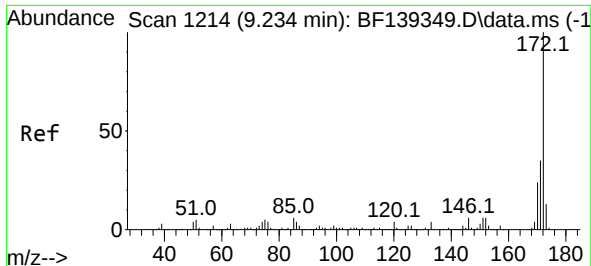

#45

2-Fluorobiphenyl

Concen: 89.583 ng

RT: 9.233 min Scan# 1

Delta R.T. -0.000 min

Lab File: BF139509.D

Acq: 20 Sep 2024 18:49

Instrument :

BNA_F

ClientSampleId :

WC-14-5-7.5B





Tgt Ion:172 Resp: 791154

Ion Ratio Lower Upper

172 100

171 35.3 28.3 42.5

170 23.3 19.0 28.6

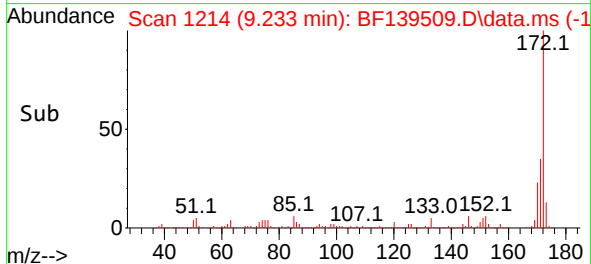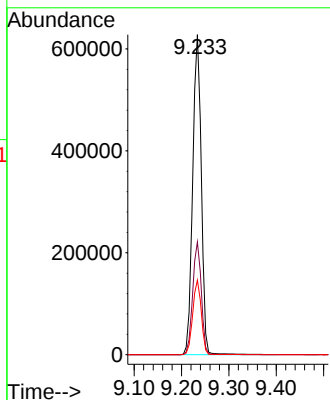

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.398 min Scan# 1582

Delta R.T. -0.000 min

Lab File: BF139509.D

Acq: 20 Sep 2024 18:49




Tgt Ion:188 Resp: 220987


Ion Ratio Lower Upper

188 100

94 8.7 5.5 8.3#

80 8.8 6.6 9.8


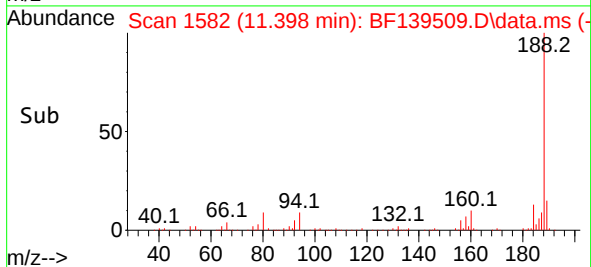
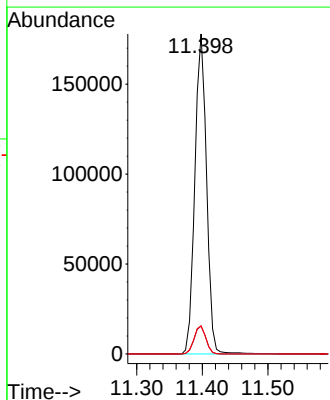
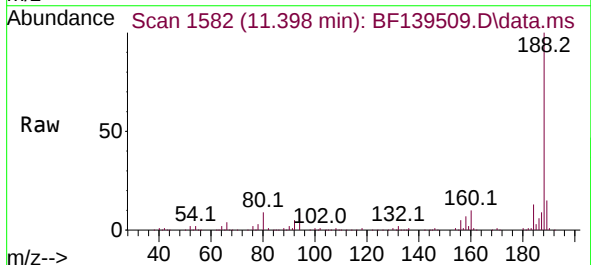


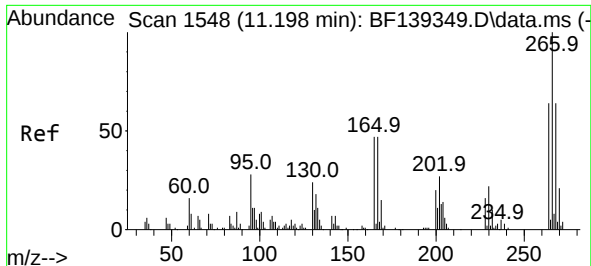

#70
 Pentachlorophenol
 Concen: 2.373 ng
 RT: 11.204 min Scan# 1549
 Delta R.T. 0.006 min
 Lab File: BF139509.D
 Acq: 20 Sep 2024 18:49




Instrument :
 BNA_F
 ClientSampleId :
 WC-14-5-7.5B


Tgt Ion:266 Resp: 3659
 Ion Ratio Lower Upper
 266 100
 268 79.7 51.1 76.7#
 264 67.6 51.4 77.0

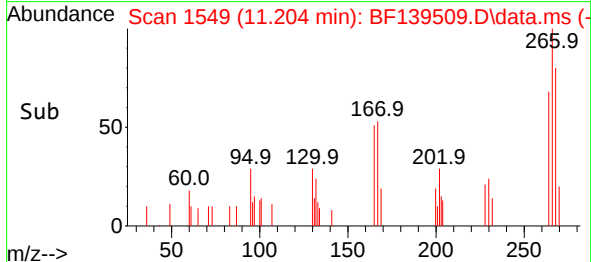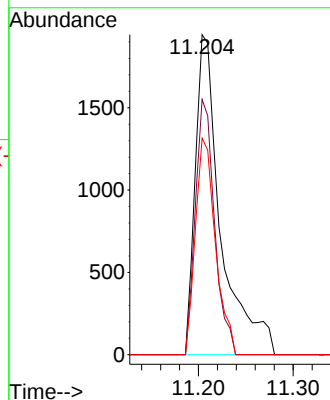

#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 14.033 min Scan# 2030
 Delta R.T. -0.000 min
 Lab File: BF139509.D
 Acq: 20 Sep 2024 18:49


Tgt Ion:240 Resp: 131452
 Ion Ratio Lower Upper
 240 100
 120 9.7 6.2 9.2#
 236 25.8 20.9 31.3

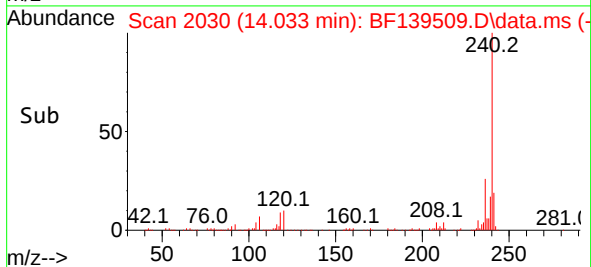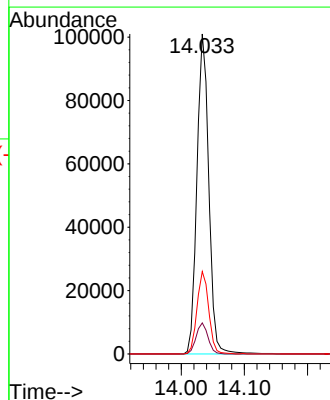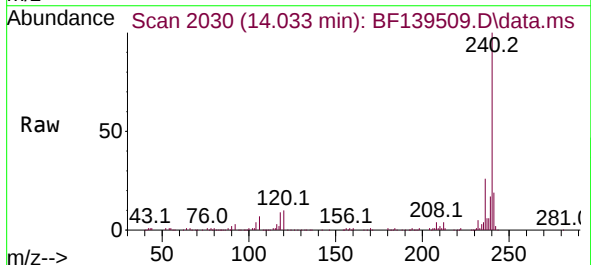






#79
 Terphenyl-d14
 Concen: 102.119 ng
 RT: 12.986 min Scan# 11
 Delta R.T. 0.006 min
 Lab File: BF139509.D
 Acq: 20 Sep 2024 18:49

Instrument :
 BNA_F
 ClientSampleId :
 WC-14-5-7.5B

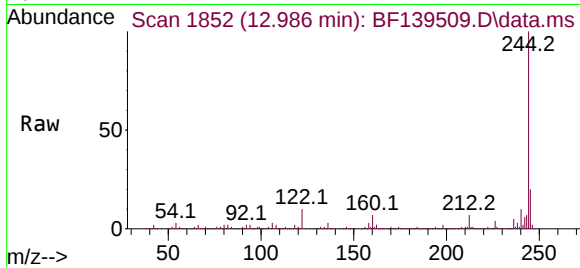

Tgt Ion:244 Resp: 817830
 Ion Ratio Lower Upper
 244 100
 212 7.3 6.0 9.0
 122 9.6 7.6 11.4

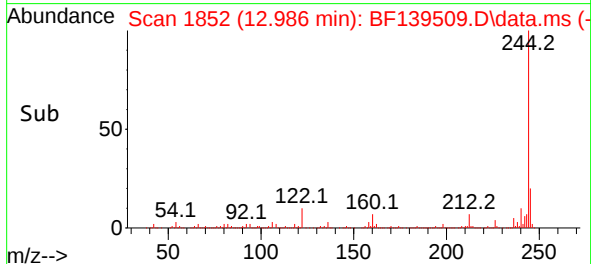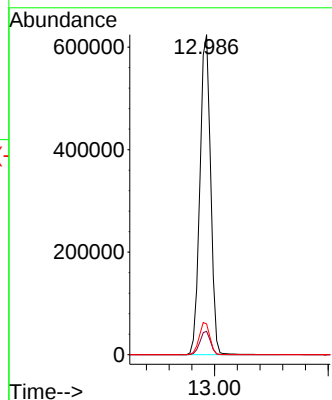

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.509 min Scan# 2281
 Delta R.T. 0.012 min
 Lab File: BF139509.D
 Acq: 20 Sep 2024 18:49

Tgt Ion:264 Resp: 98227
 Ion Ratio Lower Upper
 264 100
 260 22.7 19.5 29.3
 265 20.7 16.6 25.0

