
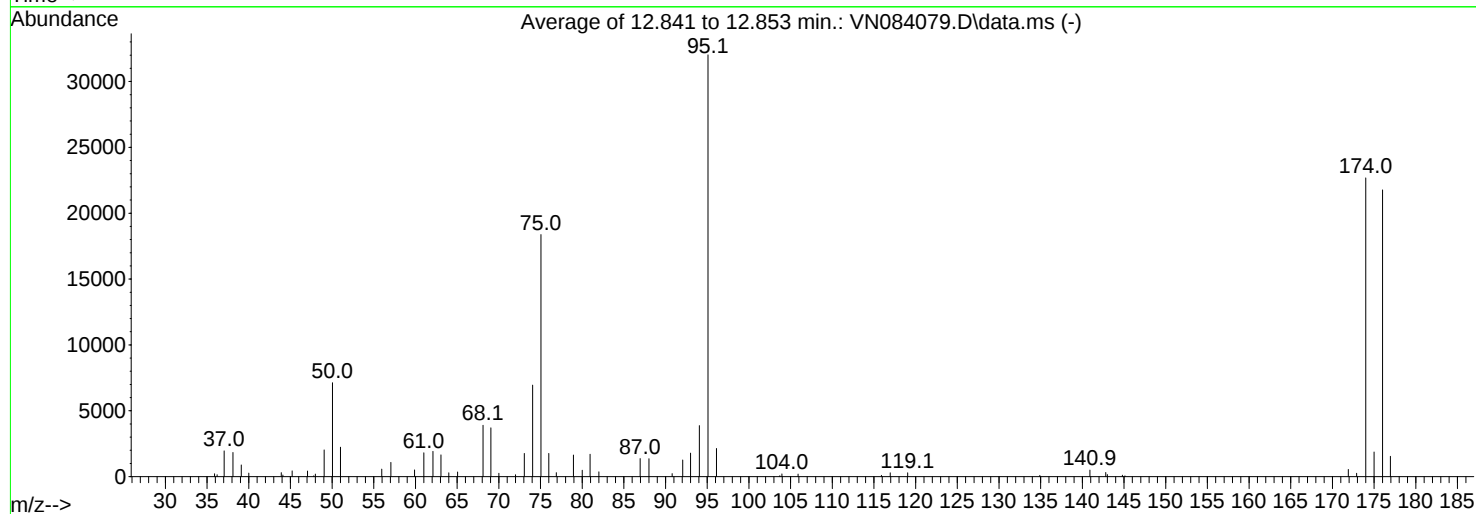


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092024\
Data File : VN084079.D
Acq On : 20 Sep 2024 23:44
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091024W.M
Title : SW846 8260
Last Update : Wed Sep 11 15:18:56 2024

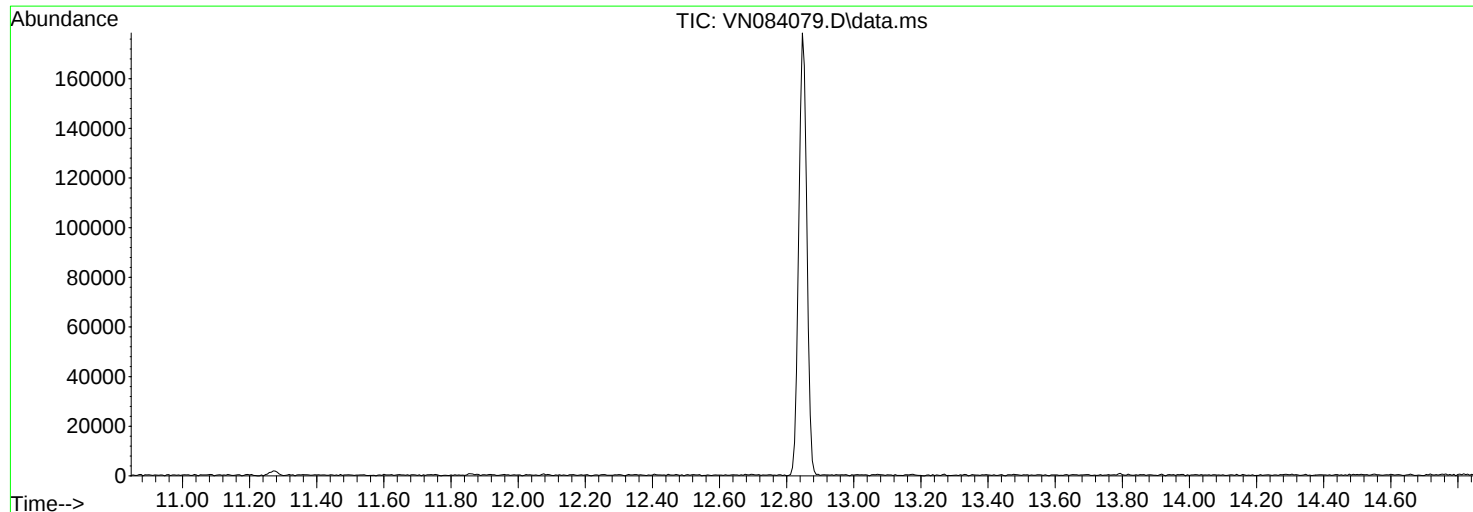

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.3	7133	PASS
75	95	30	60	57.4	18384	PASS
95	95	100	100	100.0	32024	PASS
96	95	5	9	6.7	2137	PASS
173	174	0.00	2	1.1	260	PASS
174	95	50	100	70.8	22675	PASS
175	174	5	9	8.2	1868	PASS
176	174	95	101	96.0	21768	PASS
177	176	5	9	7.1	1549	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	214	48.00	190	65.05	353	80.00	484
36.20	145	49.05	2034	68.10	3902	80.95	1704
37.05	1955	50.05	7133	69.05	3710	82.00	361
38.10	1834	51.00	2238	70.00	261	86.95	1361
39.10	892	55.95	569	72.00	153	88.00	1361
40.00	269	57.05	1085	73.05	1761	90.80	236
43.90	311	59.90	506	74.05	6951	92.05	1259
44.10	124	61.00	1811	75.05	18384	93.00	1790
45.20	442	62.10	1924	76.00	1756	94.05	3881
47.05	427	63.05	1659	76.90	307	95.10	32024
47.80	67	64.00	286	78.95	1641	96.10	2137

Average of 12.841 to 12.853 min.: VN084079.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
103.70	69	145.10	56				
103.95	207	171.90	552				
105.90	196	172.90	260				
115.90	93	174.00	22675				
116.95	290	175.00	1868				
119.05	292	176.00	21768				
134.90	92	176.95	1549				
140.90	500						
142.80	312						
143.00	161						
144.80	111						

Instrument :

MSVOA_N

ClientSampleId :

BFB