

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100524\
 Data File : PL092222.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2024 17:09
 Operator : AR\AJ
 Sample : PB163891BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB163891BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/04/2024
 Supervised By : Ankita Jodhani 10/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 02:51:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 23 16:44:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.551	2.782	39811259	42972537	17.895	17.134
28) SA Decachlor...	9.067	7.924	31190593	44979543	19.039m	17.978

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100524\
Data File : PL092222.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2024 17:09
Operator : AR\AJ
Sample : PB163891BL
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB163891BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/04/2024
Supervised By : Ankita Jodhani 10/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 02:51:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
Quant Title : GC Extractables
QLast Update : Mon Sep 23 16:44:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

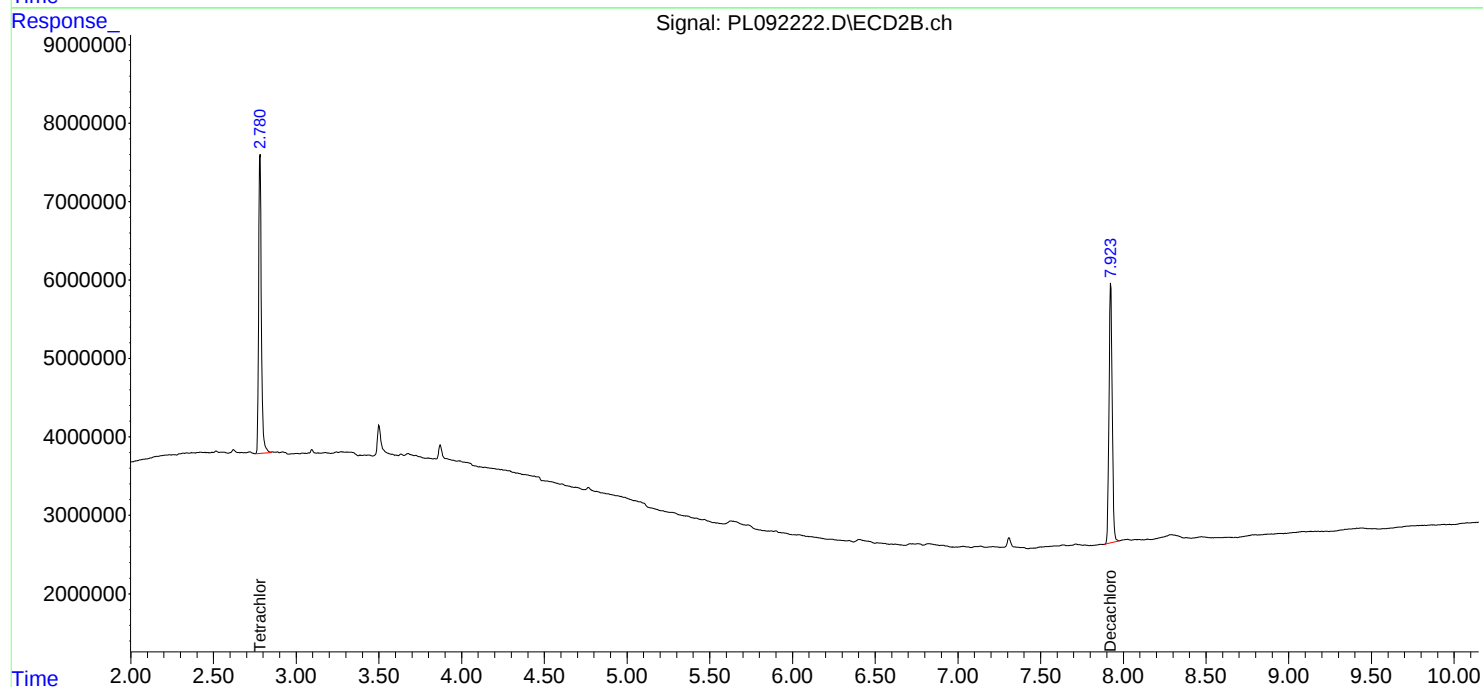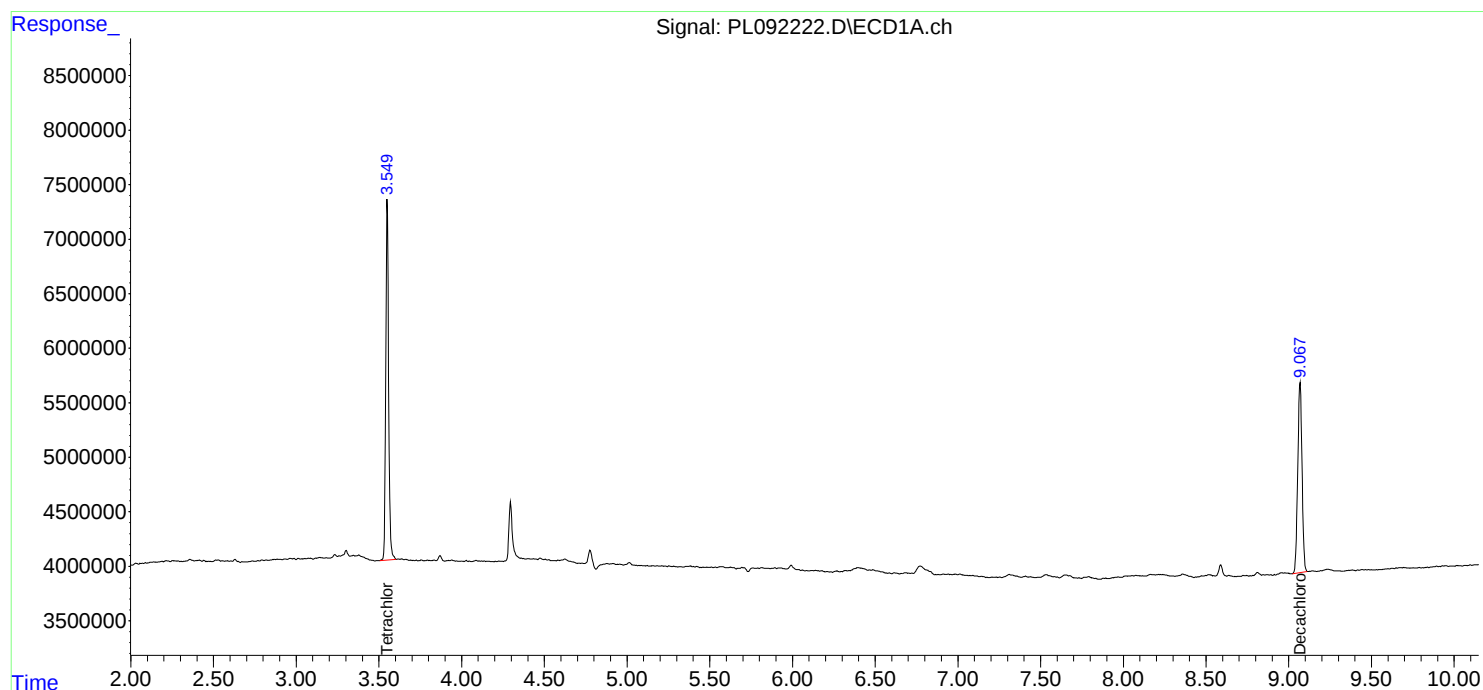

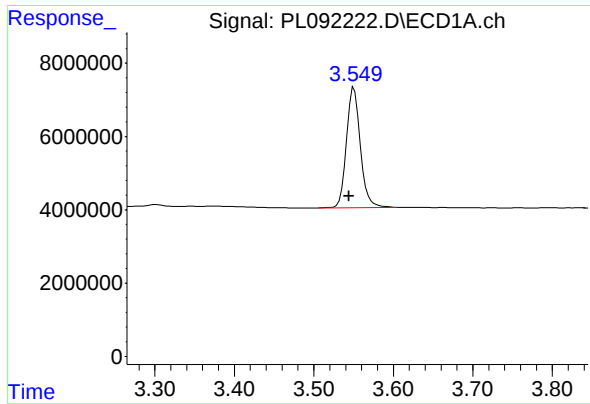


#1 Tetrachloro-m-xylene

R.T.: 3.551 min
Delta R.T.: 0.007 min
Response: 39811259
Conc: 17.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB163891BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

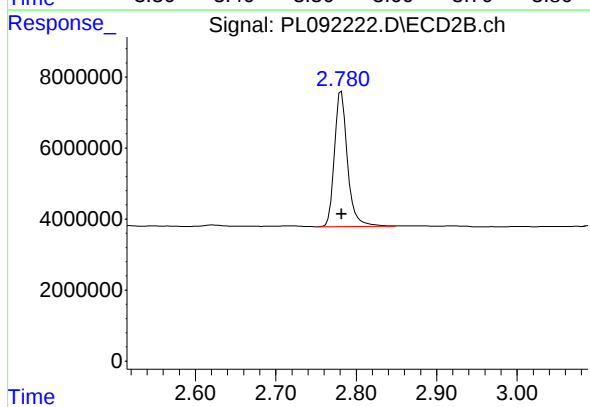


#1 Tetrachloro-m-xylene

R.T.: 2.782 min
Delta R.T.: 0.000 min
Response: 42972537
Conc: 17.13 ng/ml

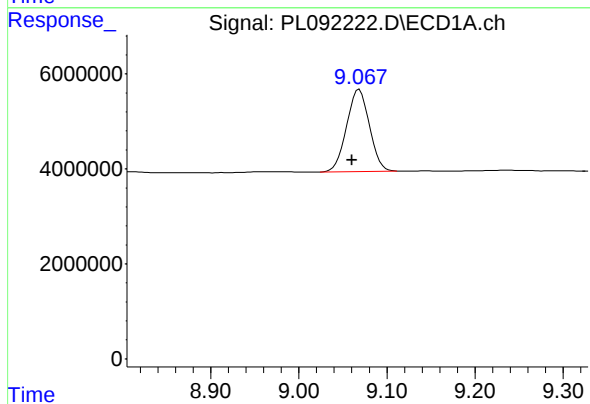

#28 Decachlorobiphenyl

R.T.: 9.067 min
Delta R.T.: 0.007 min
Response: 31190593
Conc: 19.04 ng/ml m

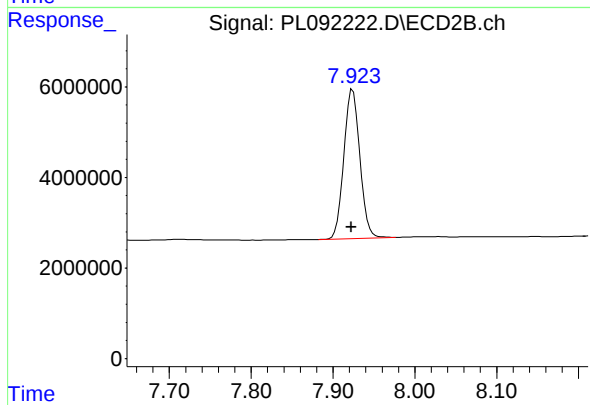

#28 Decachlorobiphenyl

R.T.: 7.924 min
Delta R.T.: 0.002 min
Response: 44979543
Conc: 17.98 ng/ml